


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051525\
Data File : BN037024.D
Acq On : 15 May 2025 09:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 14 11:26:32 2025

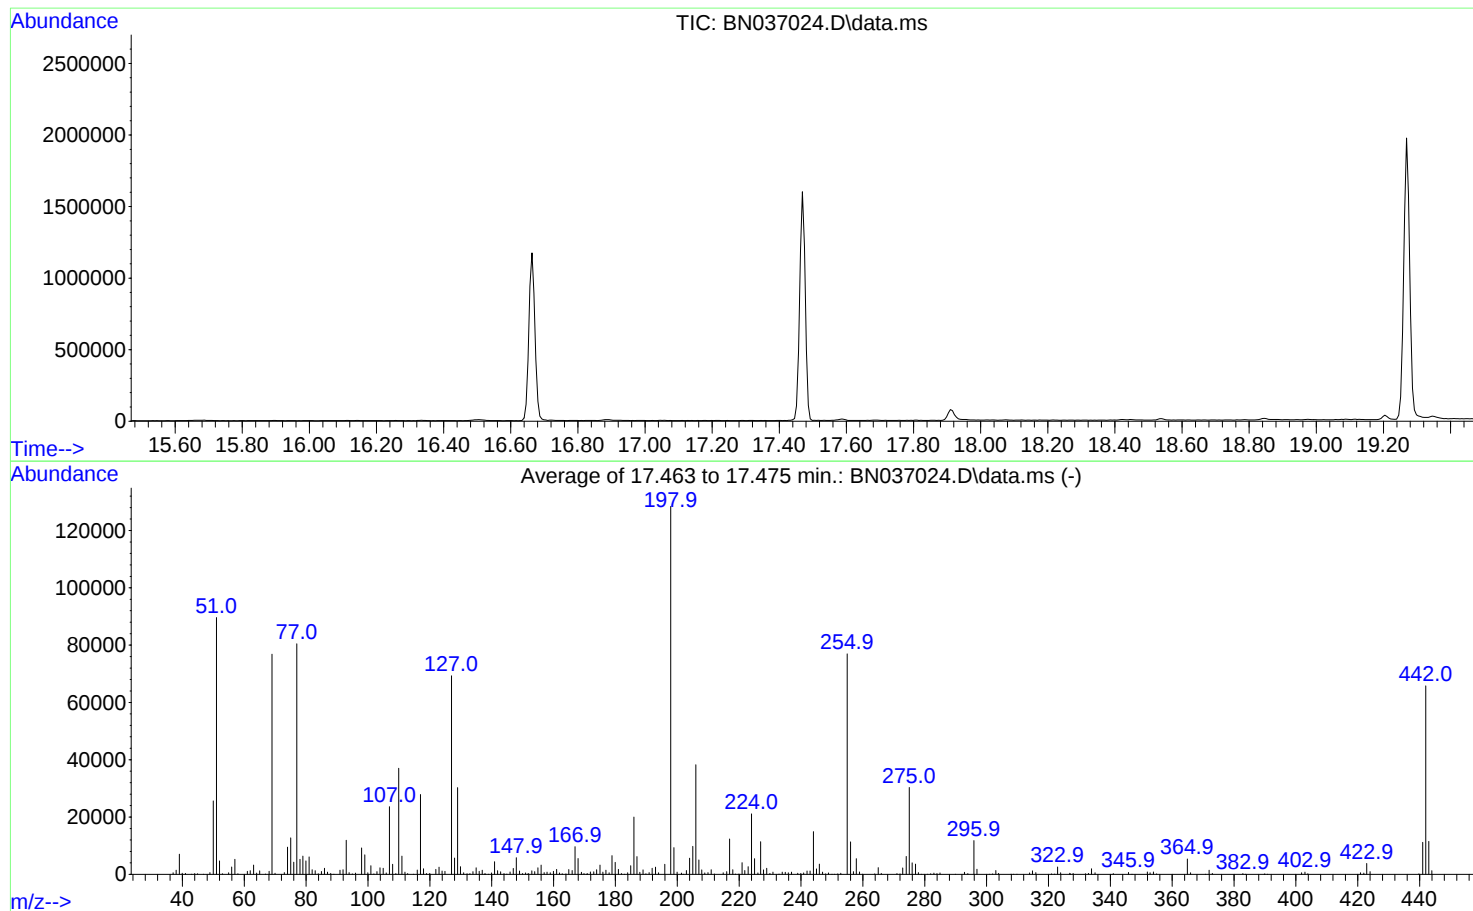




Spectrum Information: Average of 17.463 to 17.475 min.

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	69.8	89624	PASS
68	69	0.00	2	1.4	1072	PASS
69	198	0.00	100	59.8	76829	PASS
70	69	0.00	2	0.5	418	PASS
127	198	10	80	54.0	69320	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	128384	PASS
199	198	5	9	7.3	9316	PASS
275	198	10	60	23.6	30328	PASS
365	198	1	100	4.2	5382	PASS
441	198	0.01	100	8.7	11167	PASS
442	442	50	100	100.0	65773	PASS
443	442	15	24	17.5	11496	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051525\
Data File : BN037024.D
Acq On : 15 May 2025 09:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 16 02:43:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 16 02:43:29 2025
Response via : Initial Calibration

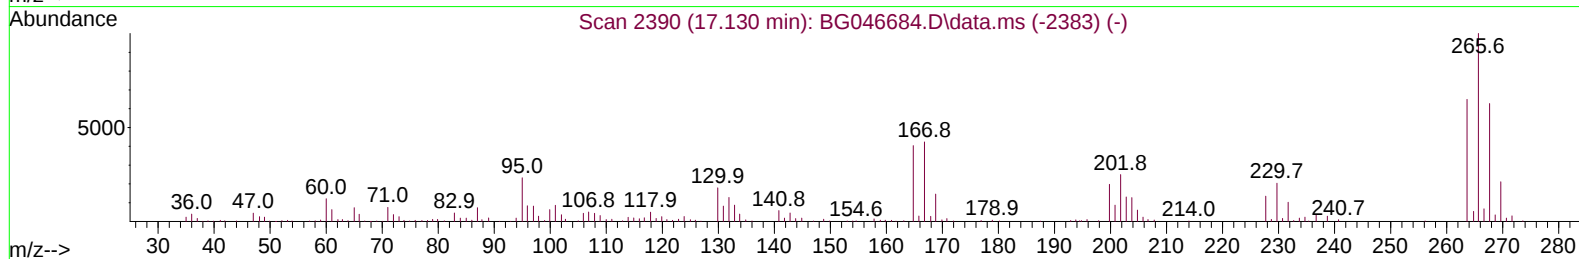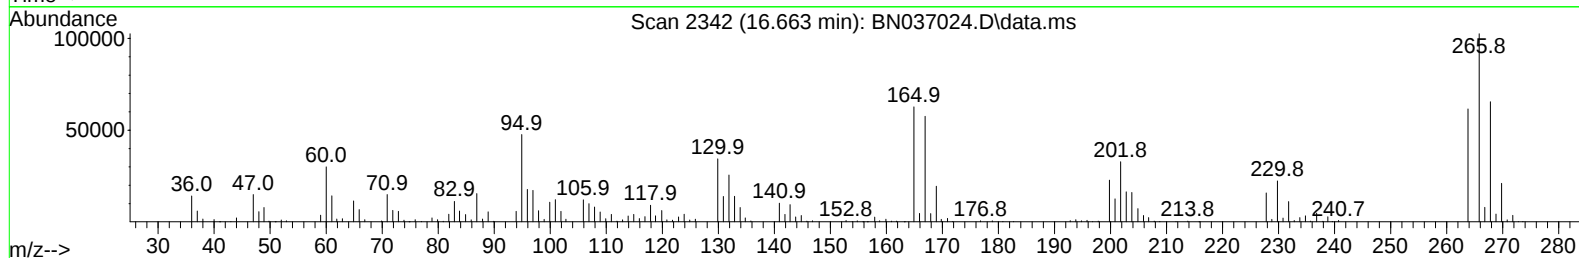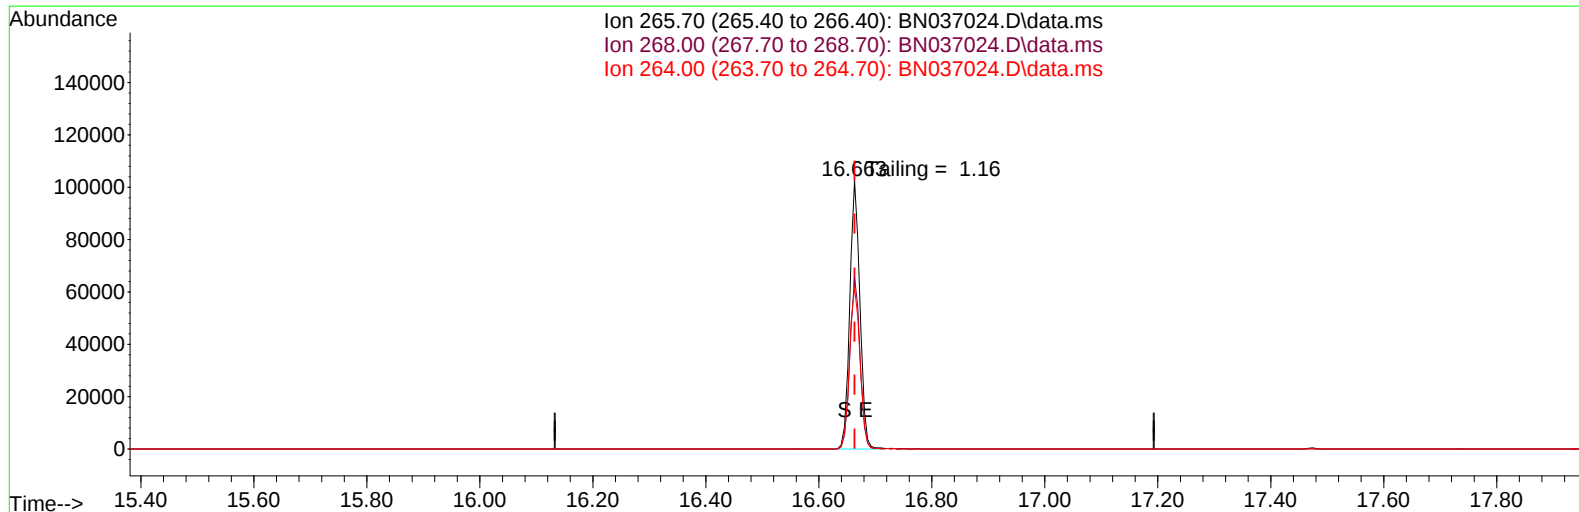

TIC: BN037024.D\data.ms

(70) Pentachlorophenol (C)

16.663min (0.000) 17096.69 ng




response 128267

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.93
264.00	61.60	60.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051525\
Data File : BN037024.D
Acq On : 15 May 2025 09:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 16 02:43:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 16 02:43:29 2025
Response via : Initial Calibration

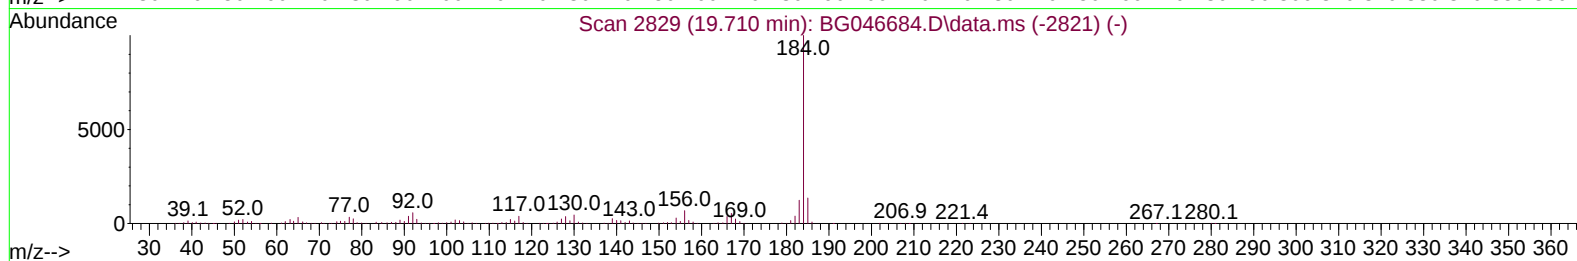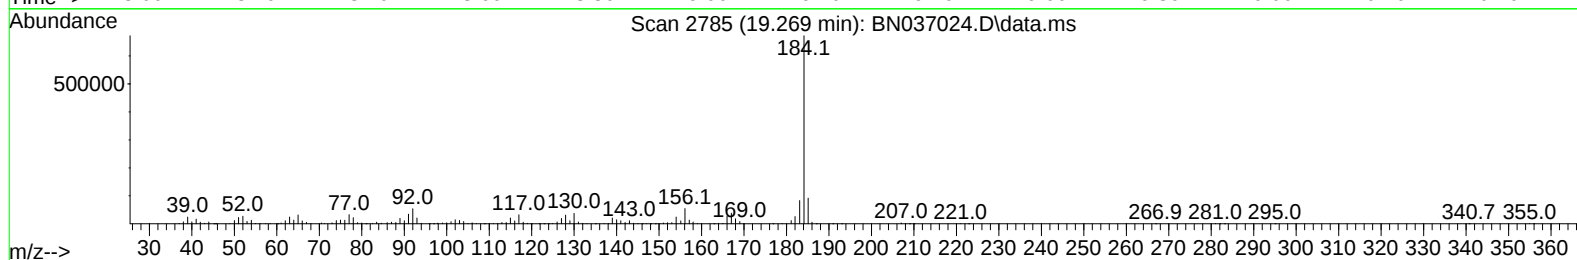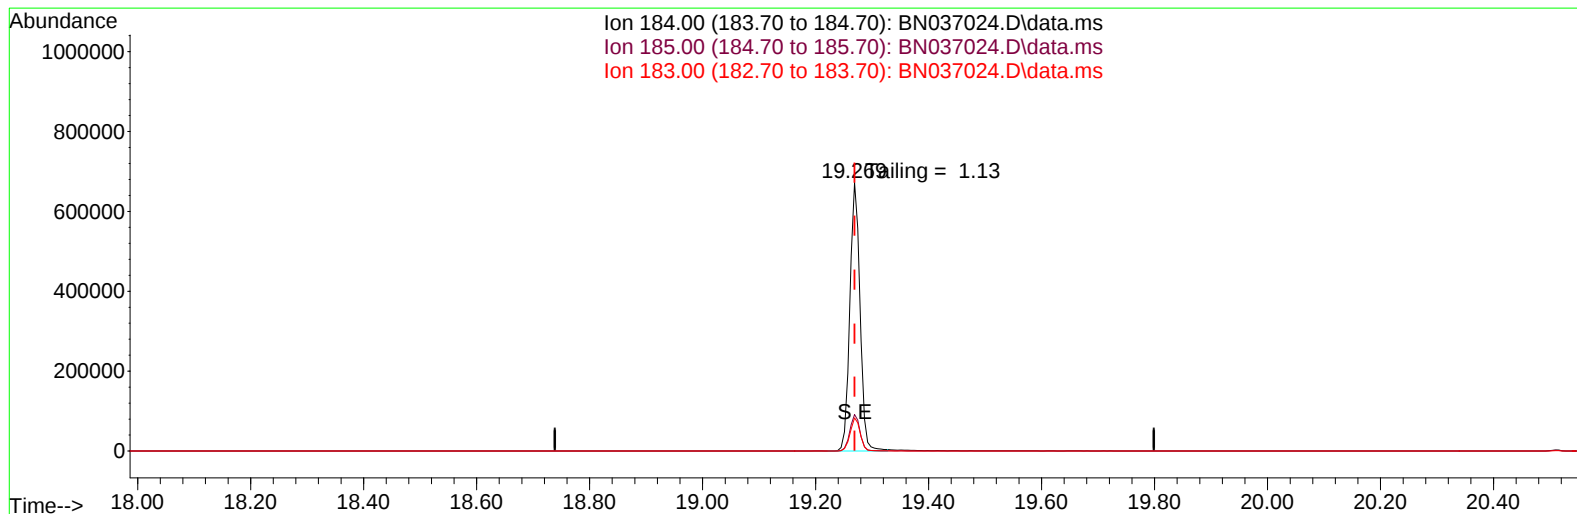

TIC: BN037024.D\data.ms

(77) Benzidine

19.269min (0.000) 0.00 ng

response 850270

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.64
183.00	13.20	12.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/15/2025	BNA_N	<u>BN037024.D</u>
Compound Name	Response	Retention Time
DDT	427034	20.51
DDD	16143	20.069
DDE	276	19.557
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16419	443453	3.70

Instrument :
BNA_N
ClientSampleId :
DFTPP