

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051325\
 Data File : VX046162.D
 Acq On : 13 May 2025 13:38
 Operator : JC/MD
 Sample : Q2013-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TB-20250508

Quant Time: May 14 01:39:00 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 06 07:12:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	61629	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	121469	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	115380	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	45238	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	62290	54.214	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	108.420%
35) Dibromofluoromethane	5.385	113	44573	50.958	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.920%
50) Toluene-d8	8.647	98	153178	50.596	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.200%
62) 4-Bromofluorobenzene	11.079	95	57615	49.613	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	99.220%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051325\
Data File : VX046162.D
Acq On : 13 May 2025 13:38
Operator : JC/MD
Sample : Q2013-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20250508

Quant Time: May 14 01:39:00 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260
QLast Update : Tue May 06 07:12:22 2025
Response via : Initial Calibration




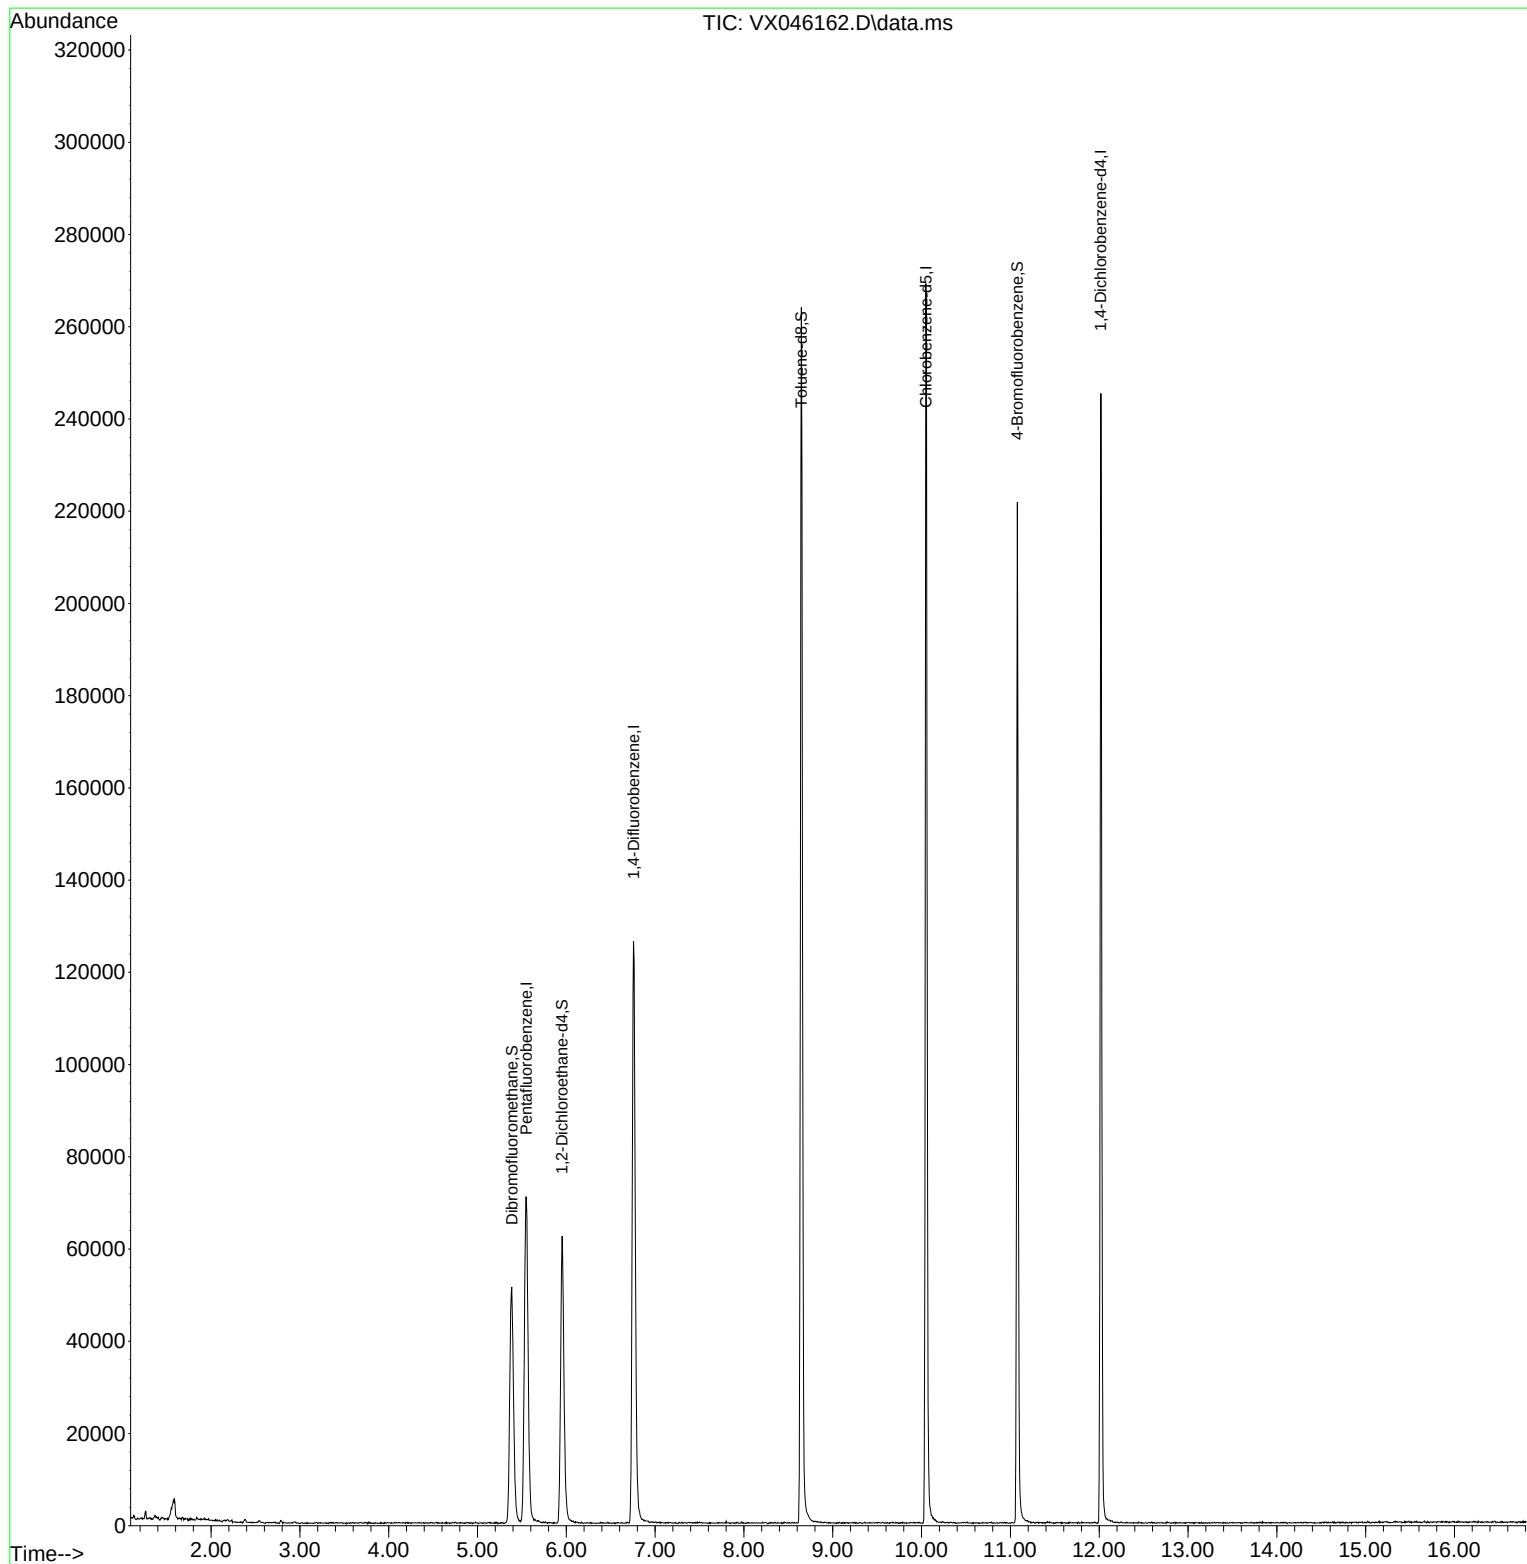


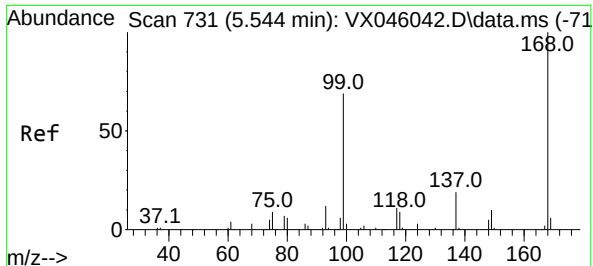

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 711
Delta R.T. 0.006 min
Lab File: VX046162.D
Acq: 13 May 2025 13:38




Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20250508


Tgt Ion:168 Resp: 61629
Ion Ratio Lower Upper
168 100
99 69.8 54.9 82.3

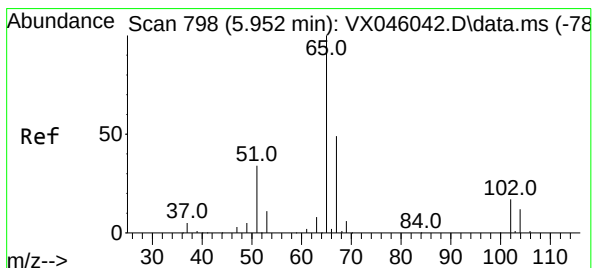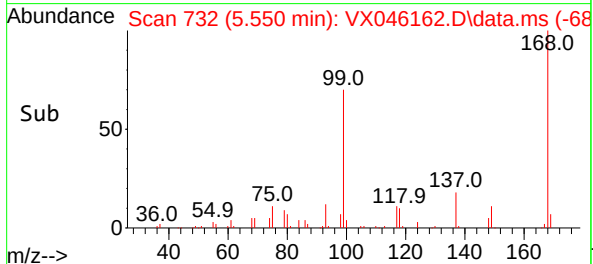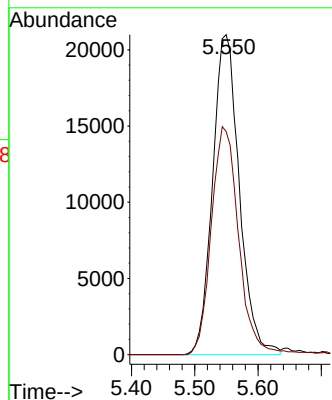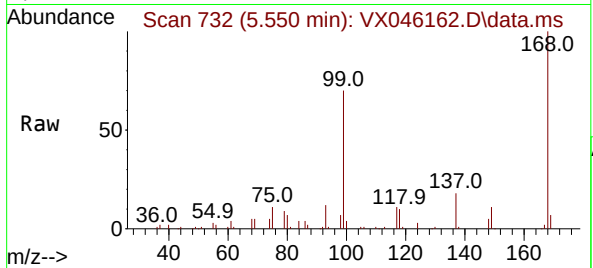

#33
1,2-Dichloroethane-d4
Concen: 54.214 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX046162.D
Acq: 13 May 2025 13:38

Tgt Ion: 65 Resp: 62290
Ion Ratio Lower Upper
65 100
67 49.9 0.0 99.0


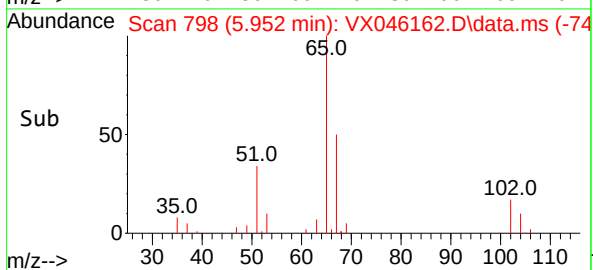
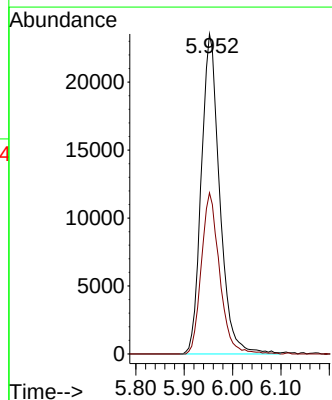
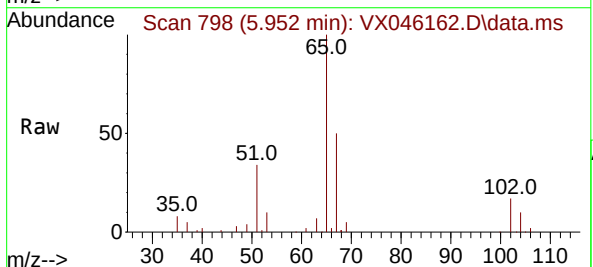


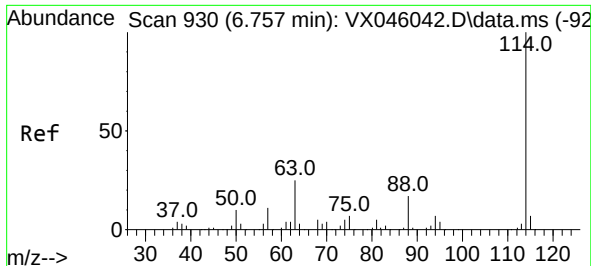

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX046162.D
Acq: 13 May 2025 13:38




Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20250508


Tgt Ion:114 Resp: 121469
Ion Ratio Lower Upper
114 100
63 23.3 0.0 49.2
88 17.4 0.0 33.6

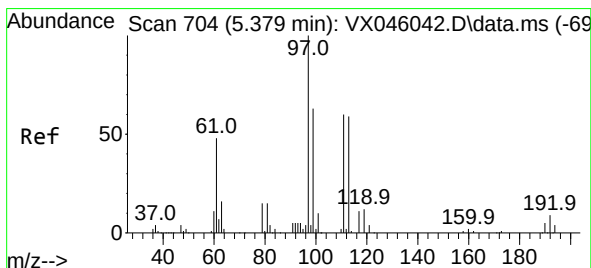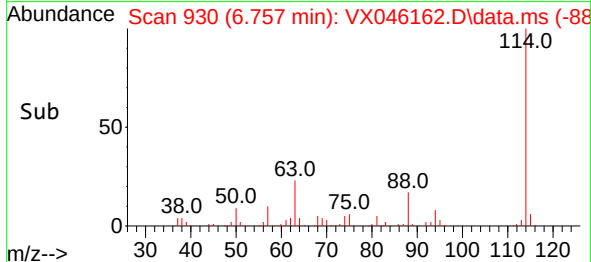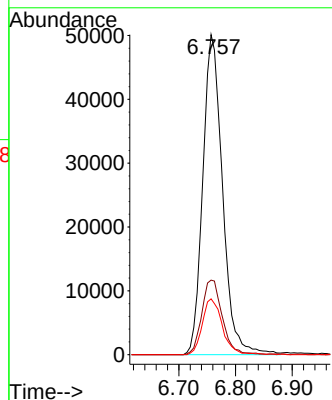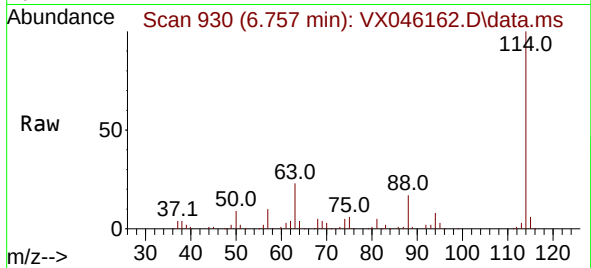

#35
Dibromofluoromethane
Concen: 50.958 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX046162.D
Acq: 13 May 2025 13:38

Tgt Ion:113 Resp: 44573
Ion Ratio Lower Upper
113 100
111 104.1 83.1 124.7
192 17.2 13.3 19.9


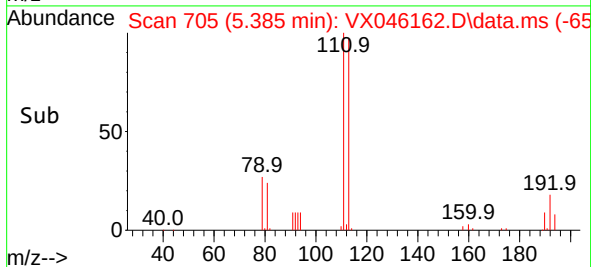
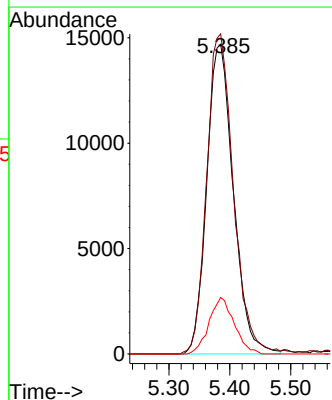
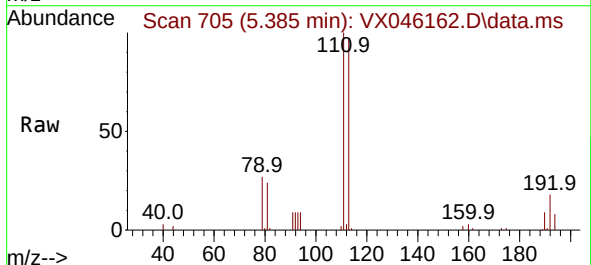


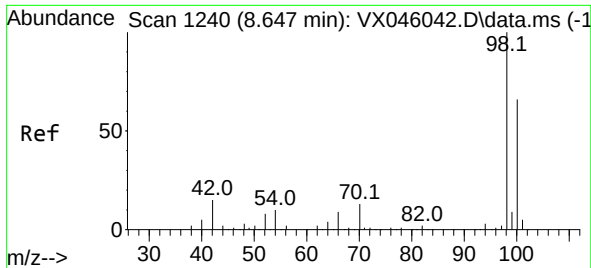

#50
Toluene-d8
Concen: 50.596 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046162.D
Acq: 13 May 2025 13:38




Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20250508


Tgt Ion: 98 Resp: 153178
Ion Ratio Lower Upper
98 100
100 65.1 53.5 80.3

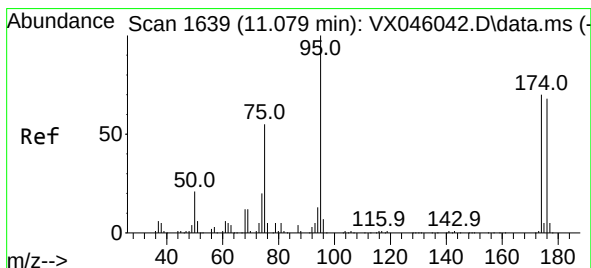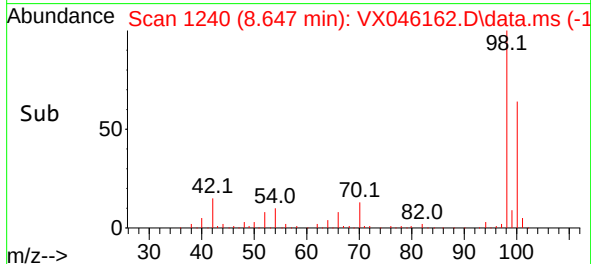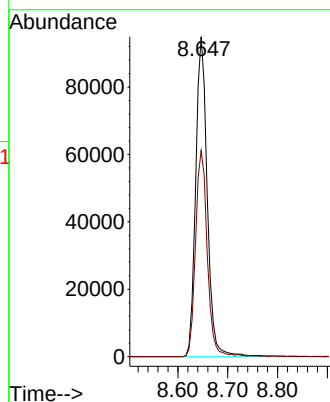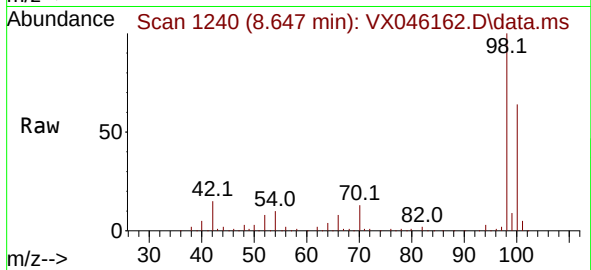

#62
4-Bromofluorobenzene
Concen: 49.613 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX046162.D
Acq: 13 May 2025 13:38

Tgt Ion: 95 Resp: 57615
Ion Ratio Lower Upper
95 100
174 66.9 0.0 135.8
176 63.9 0.0 131.4


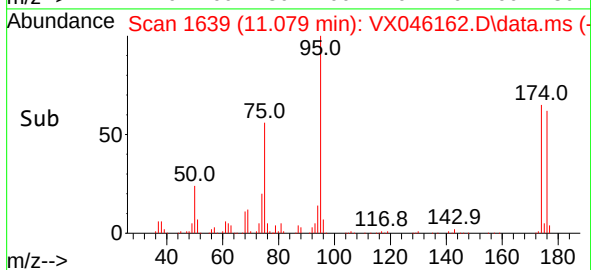
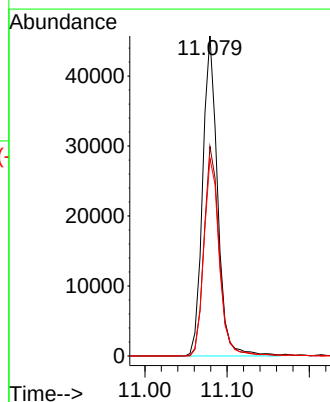
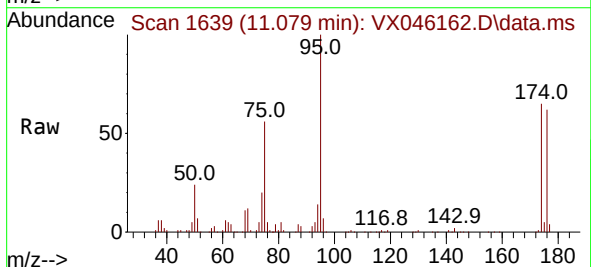


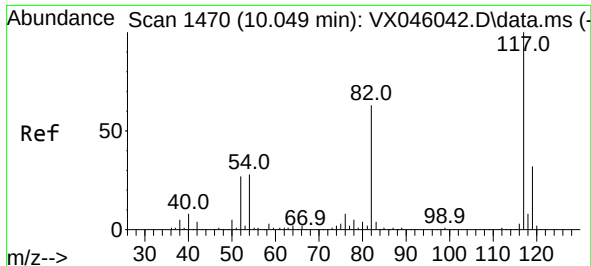

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX046162.D
Acq: 13 May 2025 13:38

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20250508

Tgt Ion:117 Resp: 115380
Ion Ratio Lower Upper
117 100
82 63.2 50.6 76.0
119 31.4 25.8 38.6

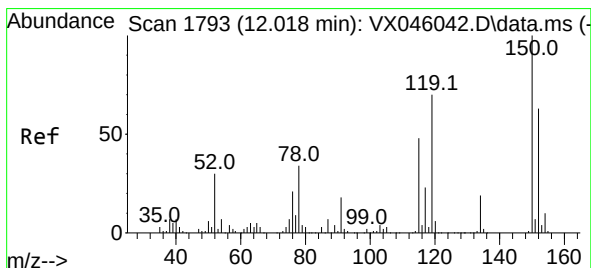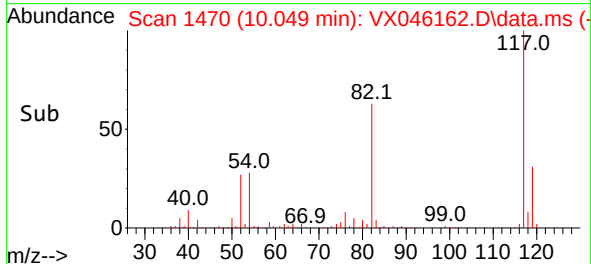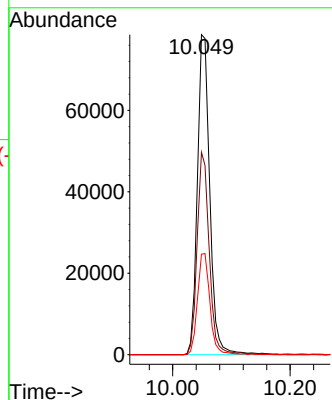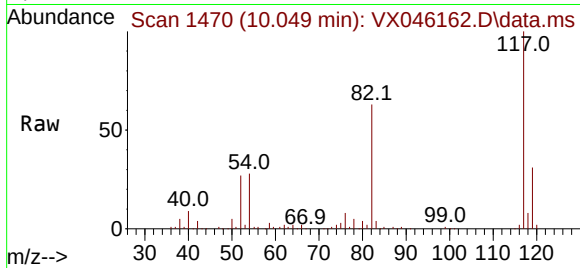

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX046162.D
Acq: 13 May 2025 13:38

Tgt Ion:152 Resp: 45238
Ion Ratio Lower Upper
152 100
115 65.3 46.9 140.7
150 159.1 0.0 351.0

