


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052125\
Data File : BP024736.D
Acq On : 21 May 2025 12:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 13 16:21:39 2025

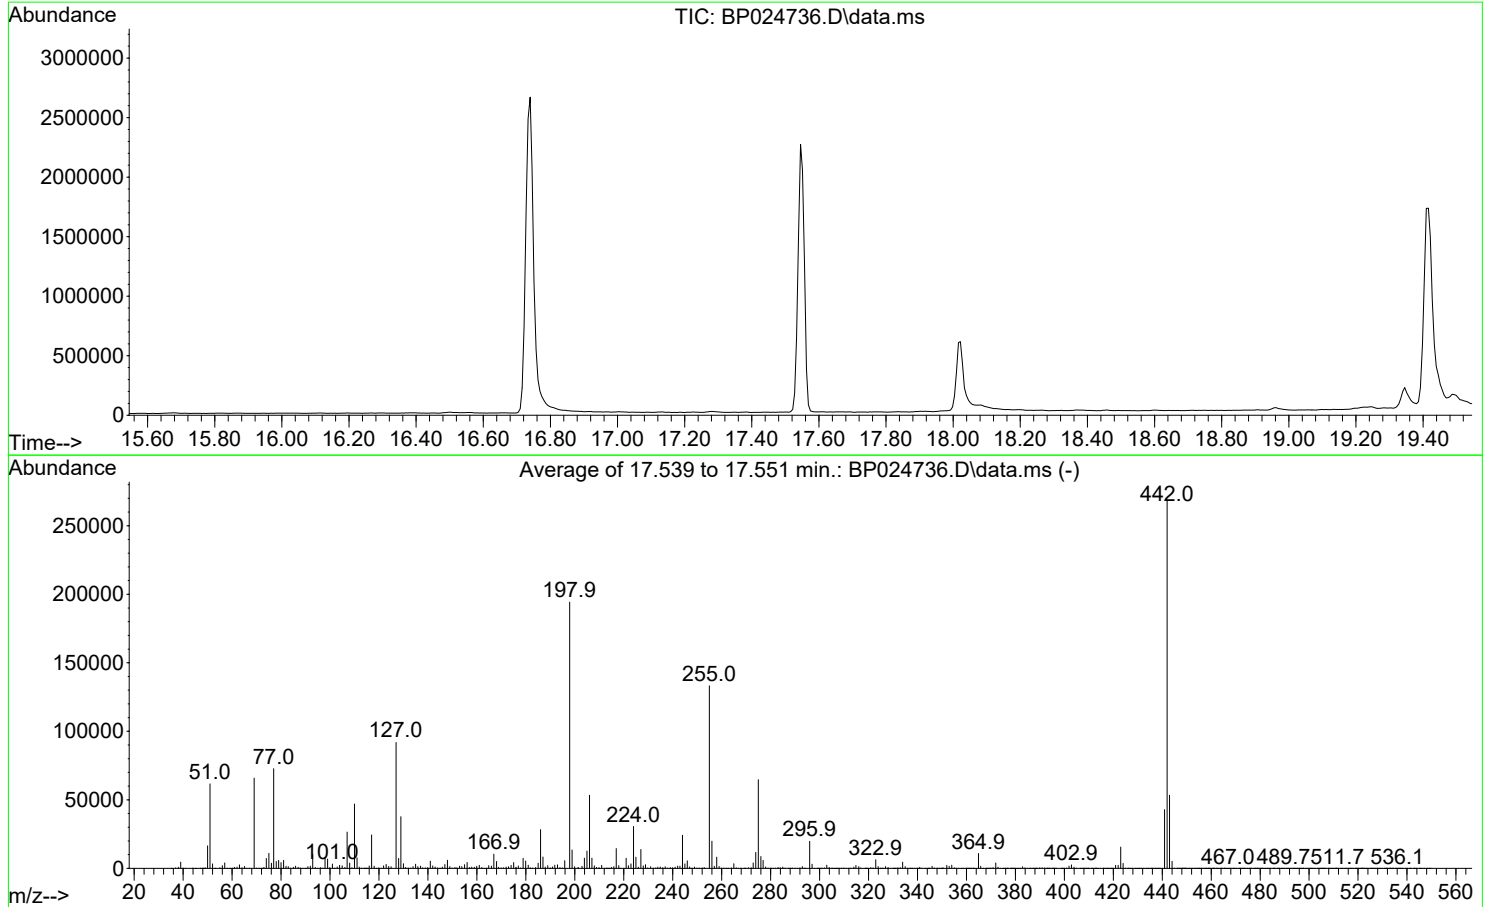

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	61657	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.9	65818	PASS
70	69	0.00	2	0.4	274	PASS
127	198	10	80	47.3	91936	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	194292	PASS
199	198	5	9	6.9	13462	PASS
275	198	10	60	33.3	64736	PASS
365	198	1	100	5.6	10847	PASS
441	198	0.01	100	22.0	42816	PASS
442	442	100	100	100.0	268409	PASS
443	442	15	24	19.9	53388	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/21/2025	BNA_P	<u>BP024736.D</u>
Compound Name	Response	Retention Time
DDT	699525	20.692
DDD	23692	20.239
DDE	2282	19.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25974	725499	3.58

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052125\
Data File : BP024736.D
Acq On : 21 May 2025 12:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 21 13:50:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

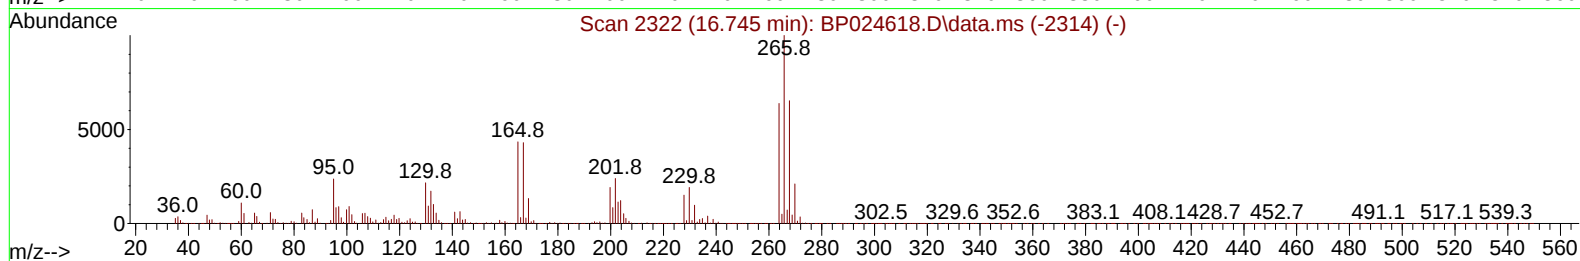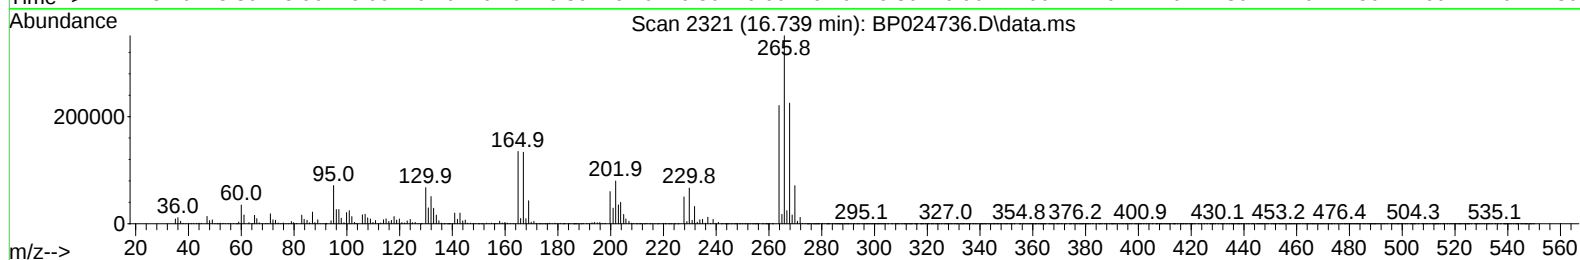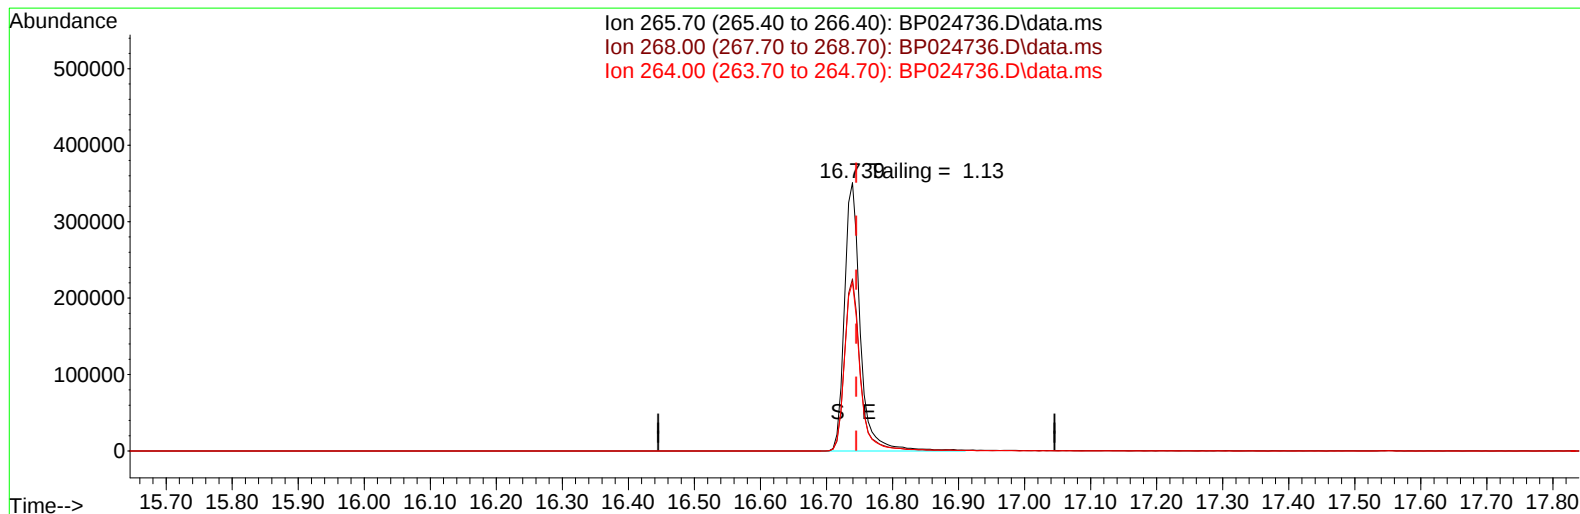

TIC: BP024736.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.006) 2229164.54 ng




response 580825

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.16
264.00	63.90	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052125\
Data File : BP024736.D
Acq On : 21 May 2025 12:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 21 13:50:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

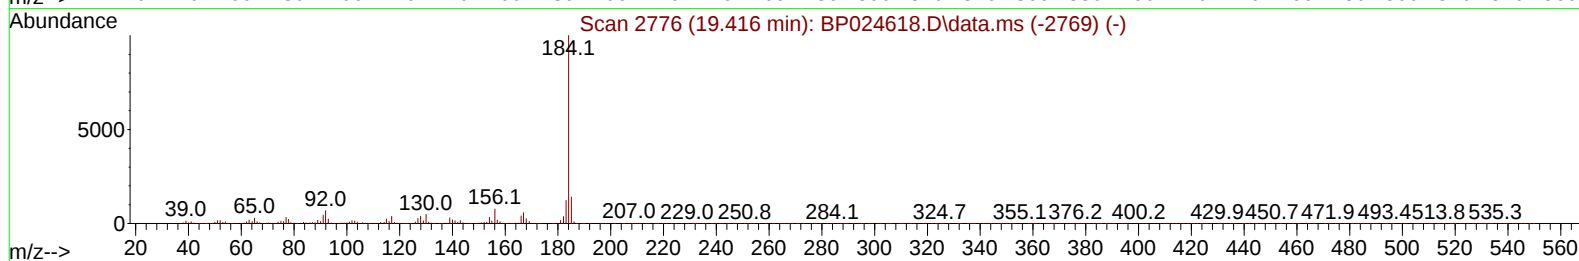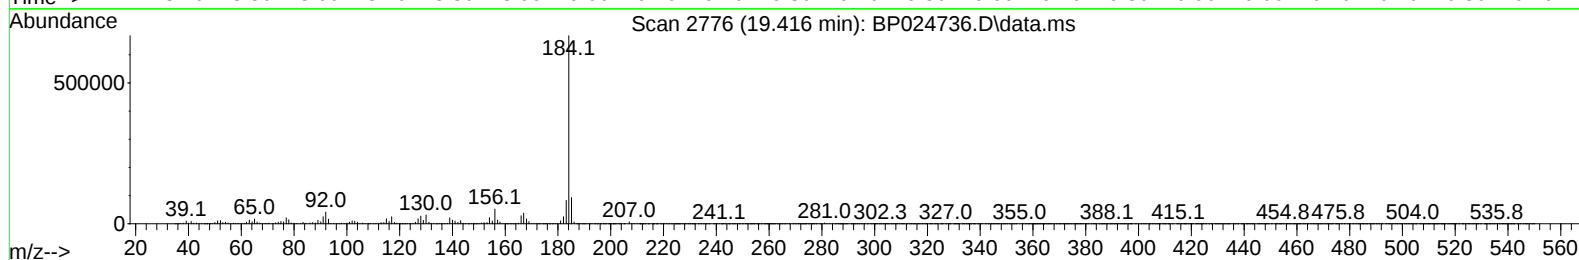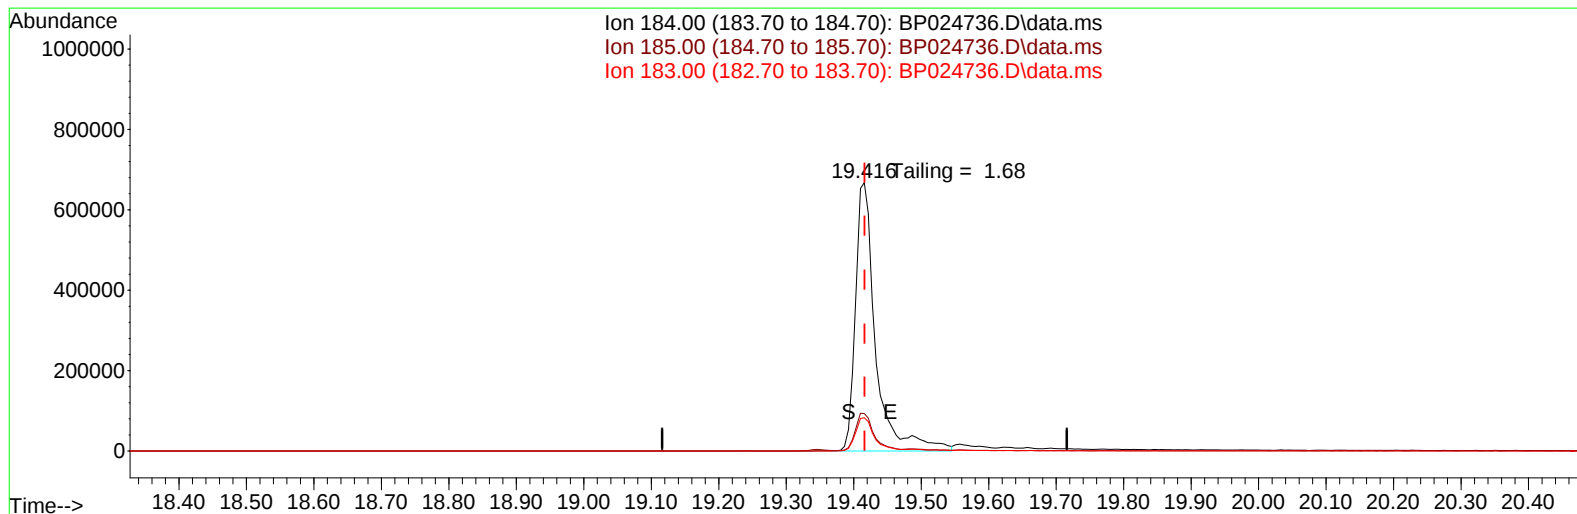

TIC: BP024736.D\data.ms

(77) Benzidine

19.416min (-0.000) 1103021.58 ng

response 1291799

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.97
183.00	12.30	12.45
0.00	0.00	0.00