

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051425\
 Data File : PL095682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 20:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 02:17:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
 Quant Title : GC Extractables
 QLast Update : Tue May 13 14:38:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.611f	2.907	81003178	88171842	19.825	18.824
28)	SA Decachlor...	9.134f	8.082	70195727	80279677	20.692	19.463
Target Compounds							
7)	B delta-BHC	4.835f	0.000	3330835	0	0.613	N.D. #
8)	B Heptachlo...	5.743	0.000	96062226	0	18.538	N.D. #
14)	MA Endrin	0.000	5.808	0	21655940	N.D.	4.065 #
15)	B Endosulfa...	6.829	6.091	24022462	6700948	5.763	1.224 #
16)	A 4,4'-DDD	6.759	0.000	71750700	0	18.466	N.D. #
19)	B Endosulfa...	7.210f	0.000	16047208	0	4.372	N.D. #
24)	Chlordane-2	0.000	4.498	0	2986387	N.D.	11.221 #
27)	Chlordane-5	0.000	6.091	0	6700948	N.D.	23.330 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051425\
Data File : PL095682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 20:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 02:17:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
Quant Title : GC Extractables
QLast Update : Tue May 13 14:38:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

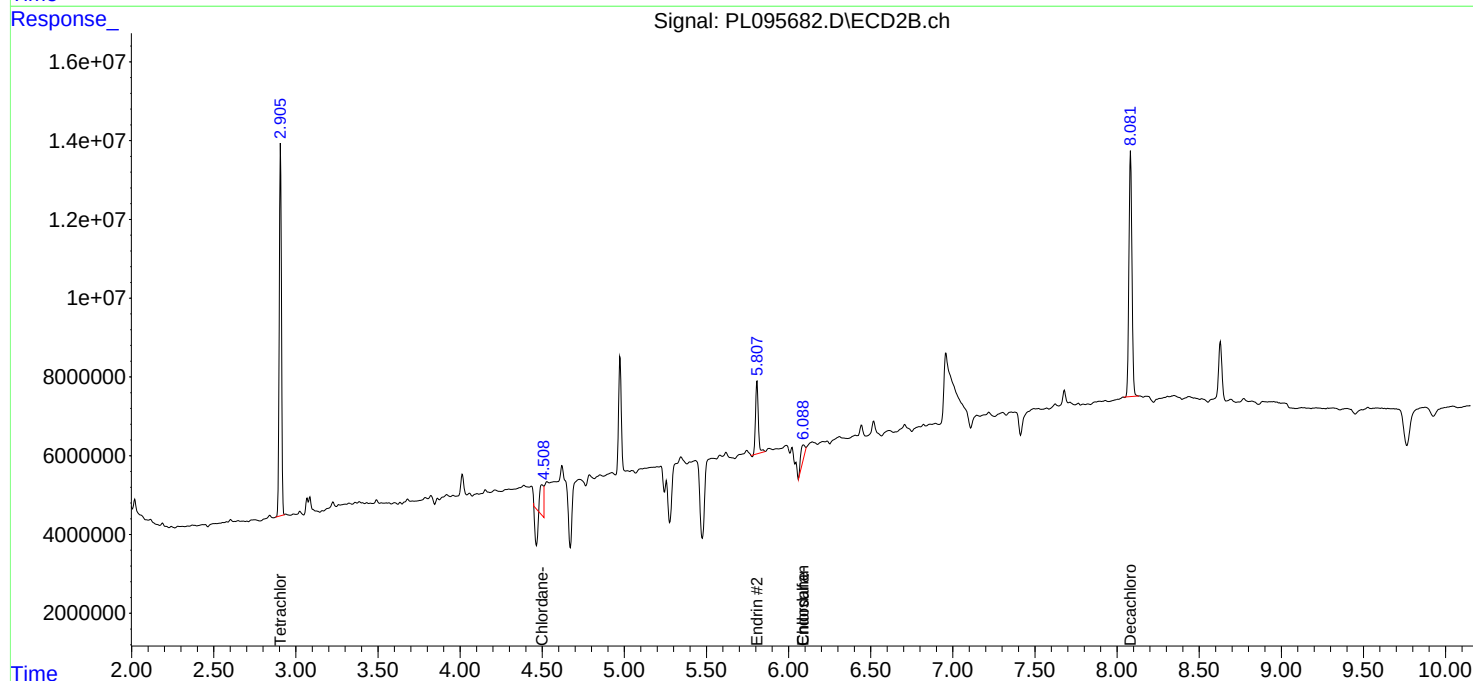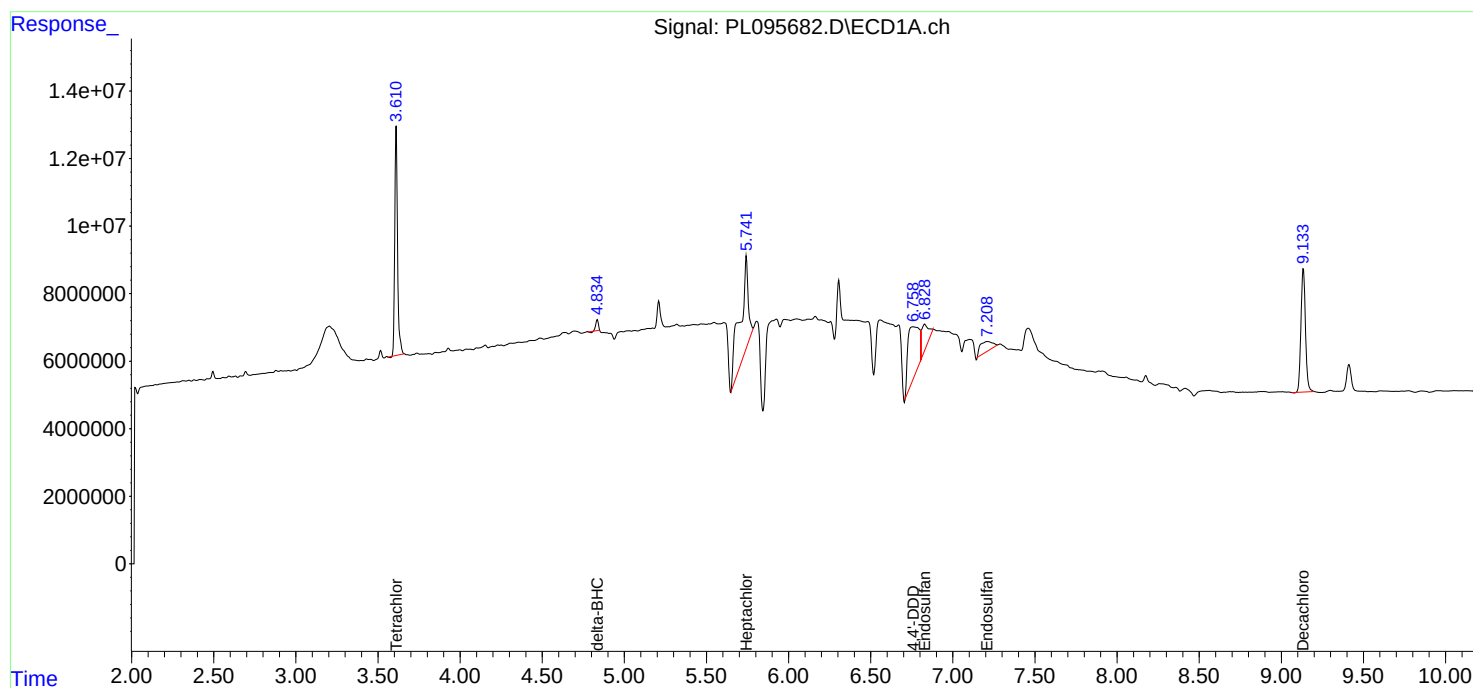


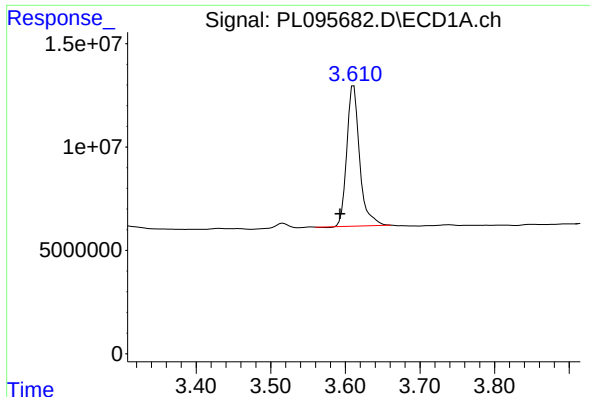

#1 Tetrachloro-m-xylene


R.T.: 3.611 min
Delta R.T.: 0.018 min
Response: 81003178
Conc: 19.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

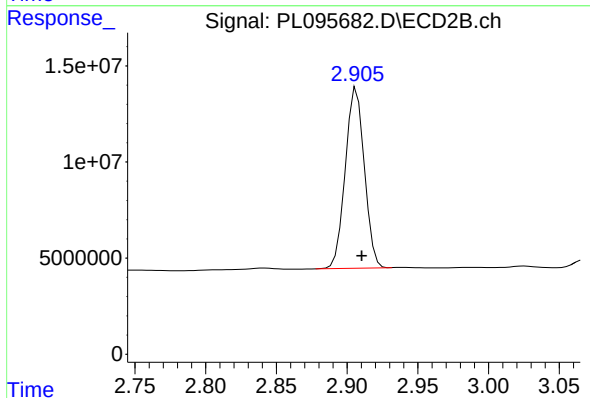


#1 Tetrachloro-m-xylene

R.T.: 2.907 min
Delta R.T.: -0.004 min
Response: 88171842
Conc: 18.82 ng/ml

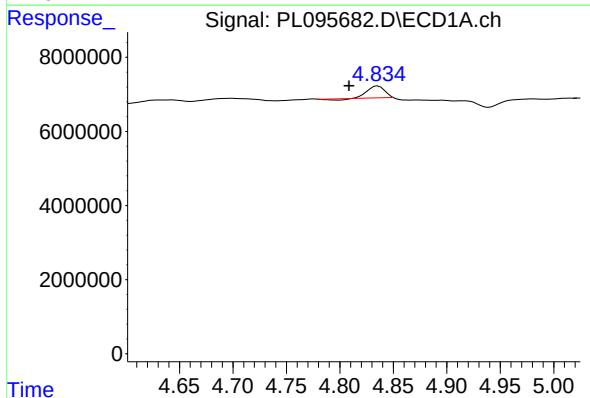


#7 delta-BHC

R.T.: 4.835 min
Delta R.T.: 0.027 min
Response: 3330835
Conc: 0.61 ng/ml

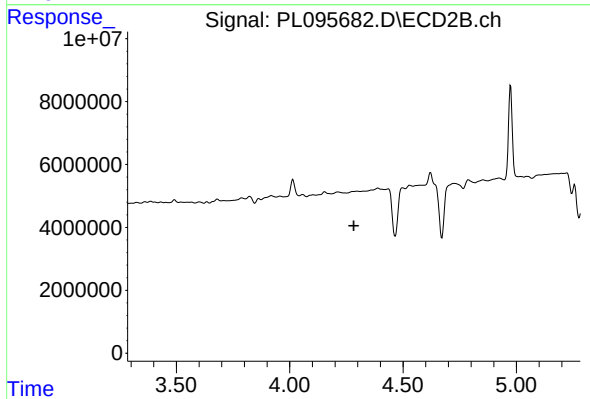

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

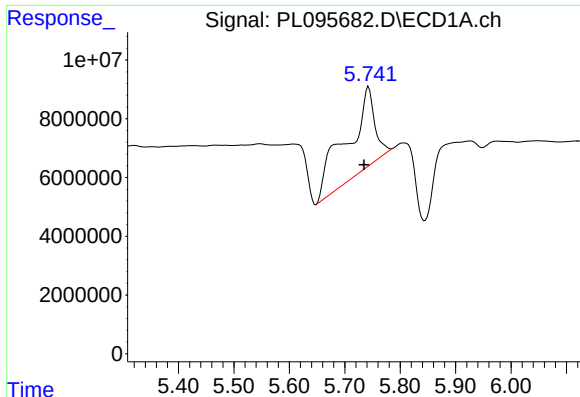

#8 Heptachlor epoxide


R.T.: 5.743 min
Delta R.T.: 0.008 min
Response: 96062226
Conc: 18.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

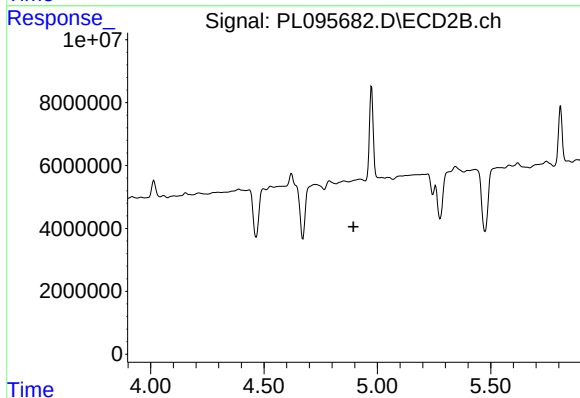


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.895 min
Response: 0
Conc: N.D.

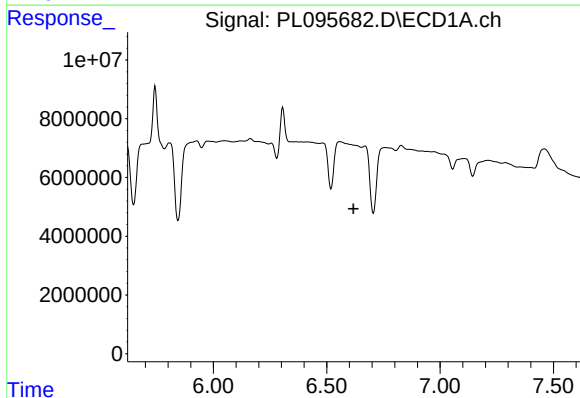


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.619 min
Response: 0
Conc: N.D.

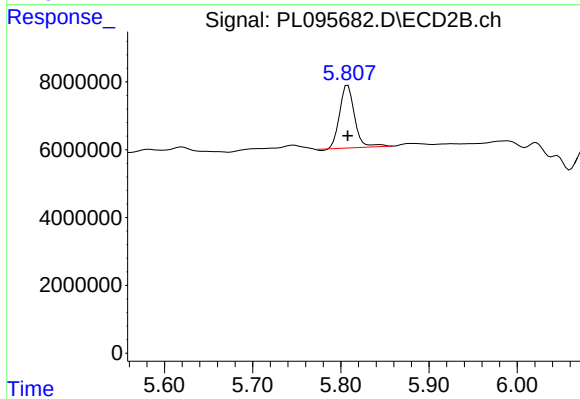

#14 Endrin


R.T.: 5.808 min
Delta R.T.: 0.000 min
Response: 21655940
Conc: 4.06 ng/ml

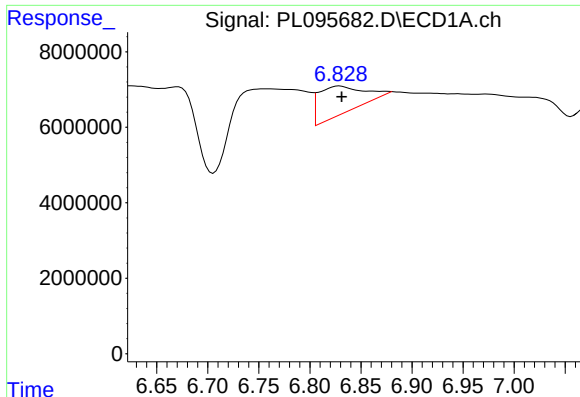

#15 Endosulfan II


R.T.: 6.829 min
Delta R.T.: -0.002 min
Response: 24022462
Conc: 5.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

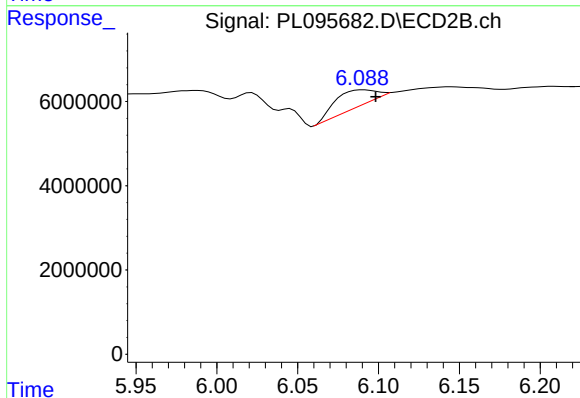


#15 Endosulfan II

R.T.: 6.091 min
Delta R.T.: -0.007 min
Response: 6700948
Conc: 1.22 ng/ml

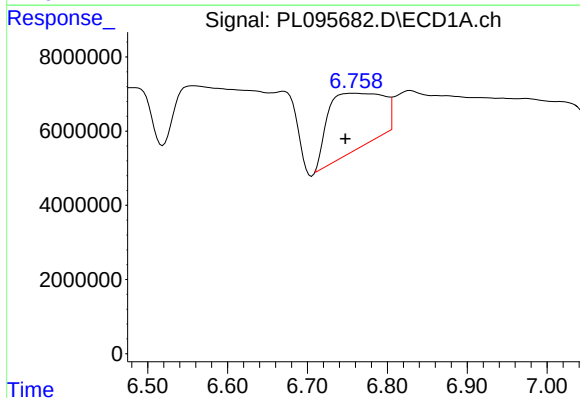


#16 4,4'-DDD

R.T.: 6.759 min
Delta R.T.: 0.011 min
Response: 71750700
Conc: 18.47 ng/ml

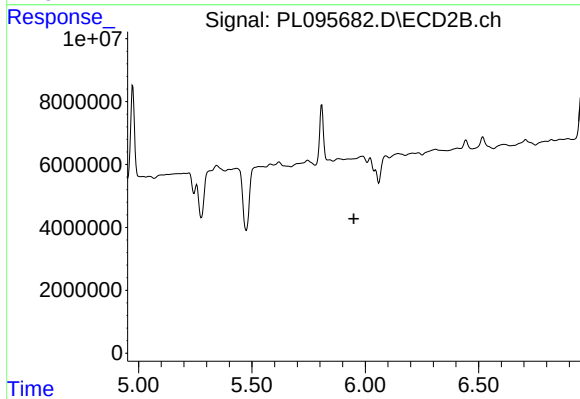

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

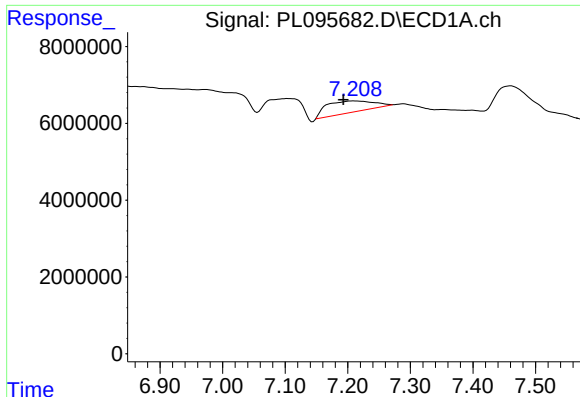

#19 Endosulfan Sulfate


R.T.: 7.210 min
Delta R.T.: 0.017 min
Response: 16047208
Conc: 4.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

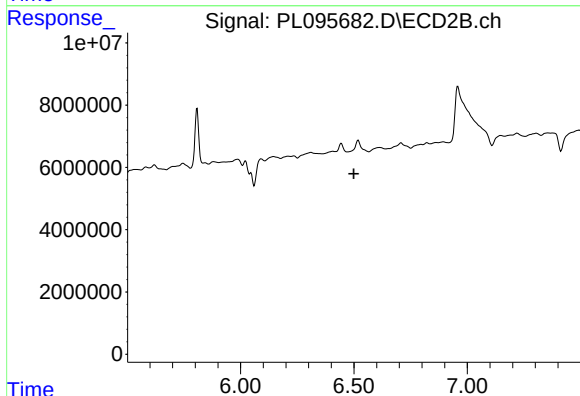


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.499 min
Response: 0
Conc: N.D.

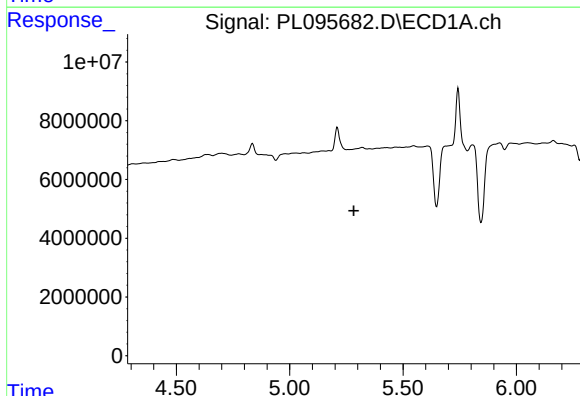


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.282 min
Response: 0
Conc: N.D.

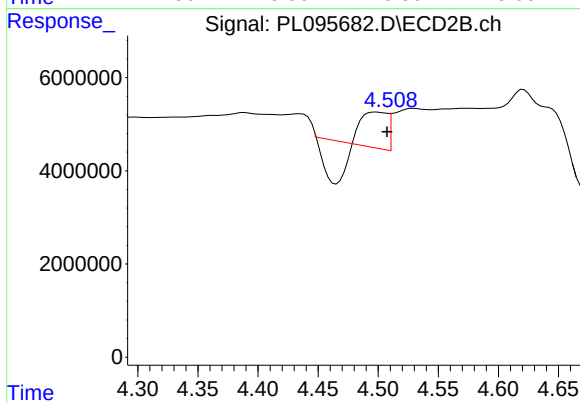

#24 Chlordane-2


R.T.: 4.498 min
Delta R.T.: -0.009 min
Response: 2986387
Conc: 11.22 ng/ml

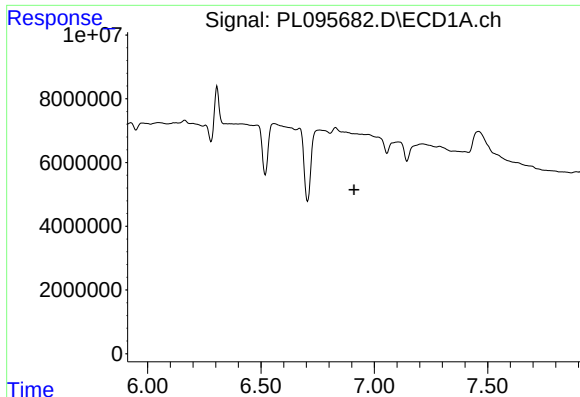

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

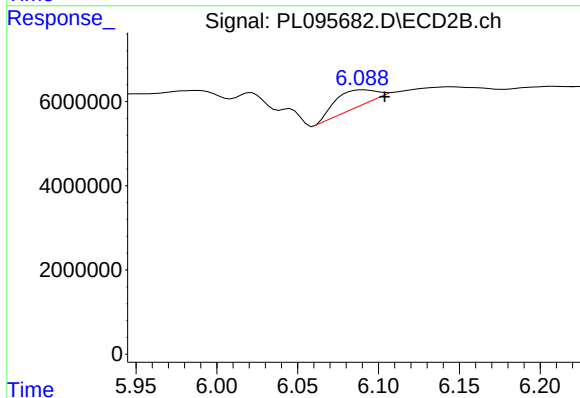


#27 Chlordane-5

R.T.: 6.091 min
Delta R.T.: -0.013 min
Response: 6700948
Conc: 23.33 ng/ml

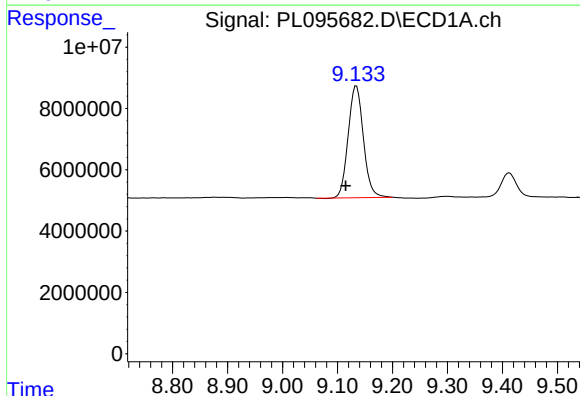

#28 Decachlorobiphenyl

R.T.: 9.134 min
Delta R.T.: 0.019 min
Response: 70195727
Conc: 20.69 ng/ml

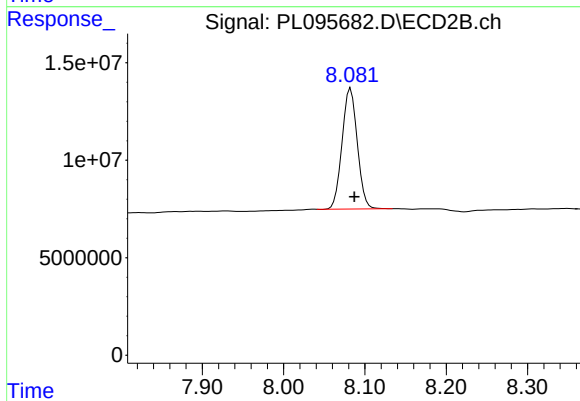

#28 Decachlorobiphenyl

R.T.: 8.082 min
Delta R.T.: -0.005 min
Response: 80279677
Conc: 19.46 ng/ml