

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051625\
 Data File : PL095728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2025 15:27
 Operator : AR\AJ
 Sample : Q2032-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-32

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:57:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
 Quant Title : GC Extractables
 QLast Update : Tue May 13 14:38:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.591	2.907	92769278	80201527	22.704	17.122
28)	SA Decachlor...	9.113	8.084	46283029	58626370	13.643	14.213
Target Compounds							
9)	A Endosulfan I	0.000	5.284f	0	14065075	N.D.	2.719 #
13)	MA Dieldrin	6.393	0.000	7676448	0	1.558	N.D. #
15)	B Endosulfa...	0.000	6.093	0	4812291	N.D.	0.879 #
16)	A 4,4'-DDD	6.740	0.000	15110724	0	3.889	N.D. #
23)	Chlordane-1	0.000	3.922	0	9931512	N.D.	41.267 #
27)	Chlordane-5	0.000	6.093	0	4812291	N.D.	16.754 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051625\
Data File : PL095728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2025 15:27
Operator : AR\AJ
Sample : Q2032-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-32

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:57:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051325.M
Quant Title : GC Extractables
QLast Update : Tue May 13 14:38:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

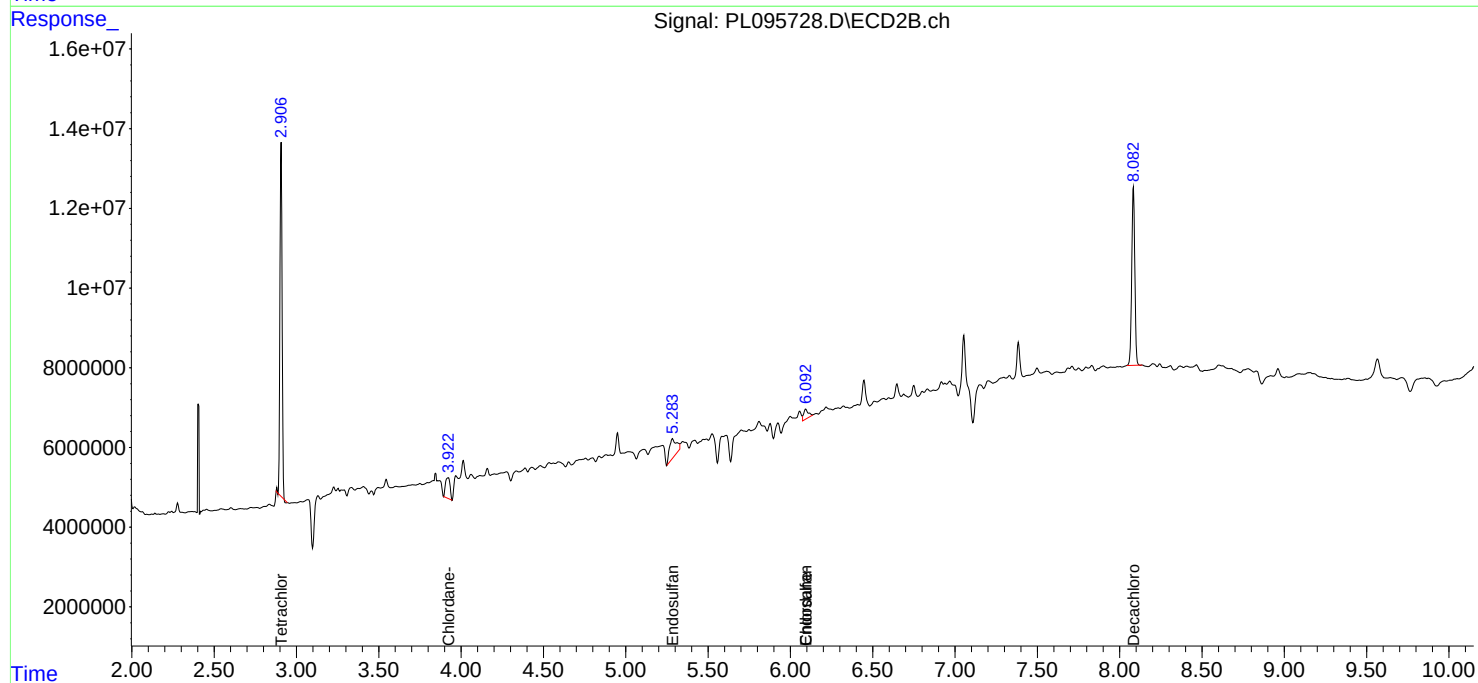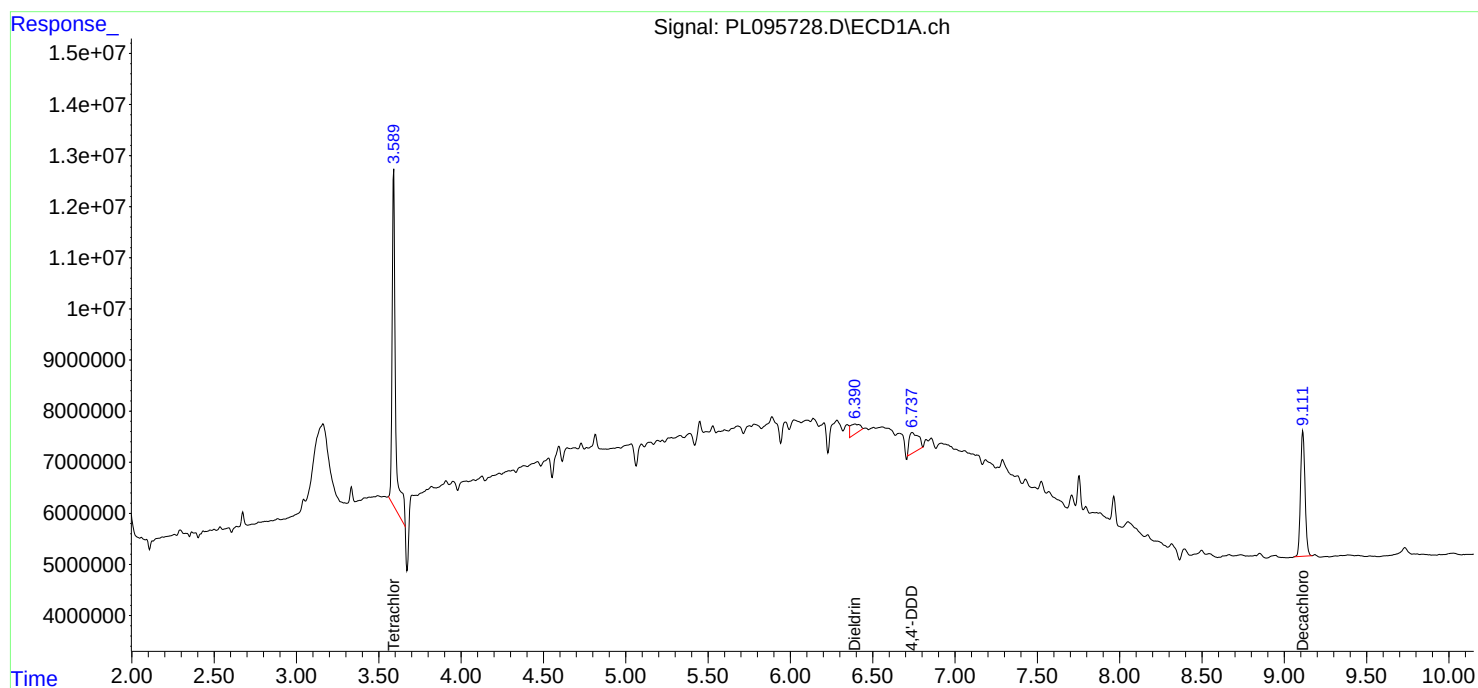


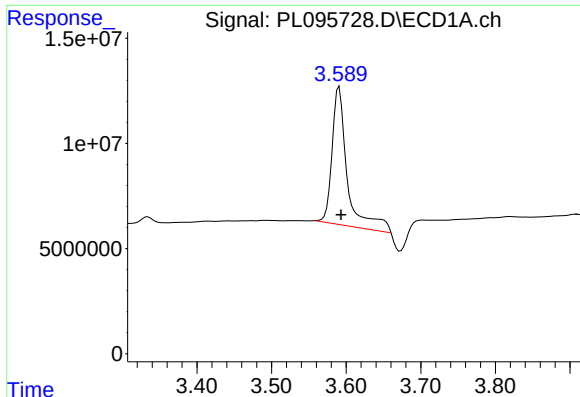

#1 Tetrachloro-m-xylene


R.T.: 3.591 min
Delta R.T.: -0.002 min
Response: 92769278
Conc: 22.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-32

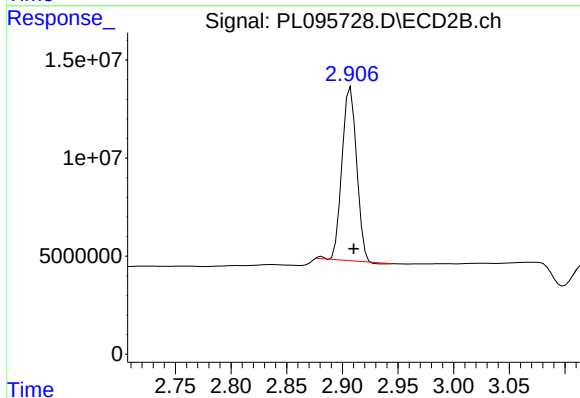


#1 Tetrachloro-m-xylene

R.T.: 2.907 min
Delta R.T.: -0.003 min
Response: 80201527
Conc: 17.12 ng/ml

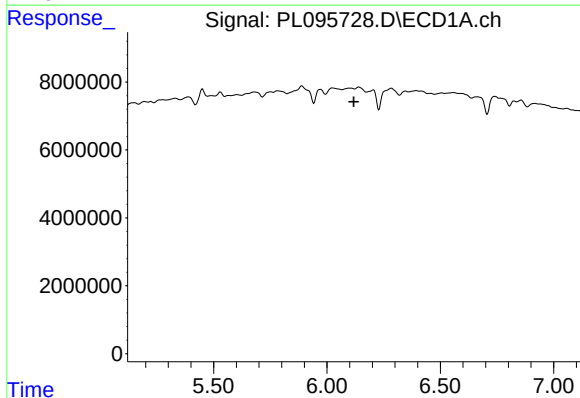


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.119 min
Response: 0
Conc: N.D.

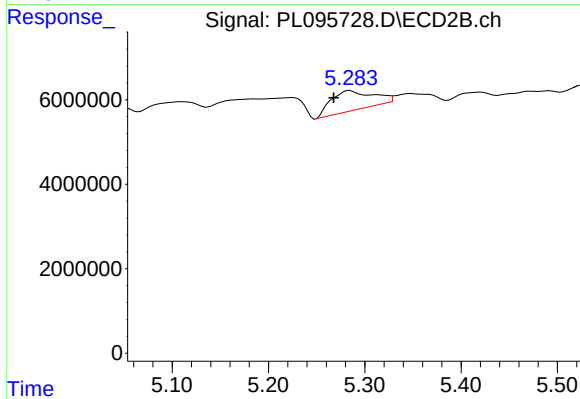

#9 Endosulfan I


R.T.: 5.284 min
Delta R.T.: 0.017 min
Response: 14065075
Conc: 2.72 ng/ml

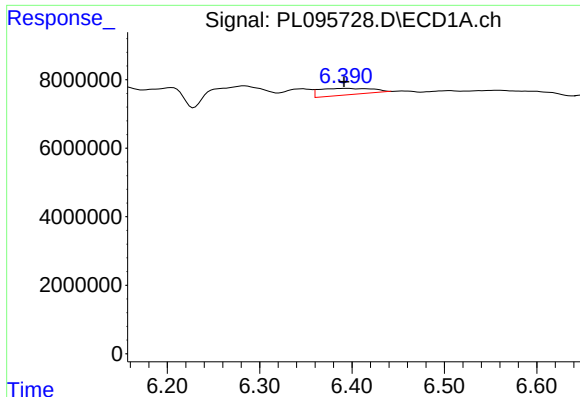

#13 Dieldrin


R.T.: 6.393 min
Delta R.T.: 0.002 min
Response: 7676448
Conc: 1.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-32

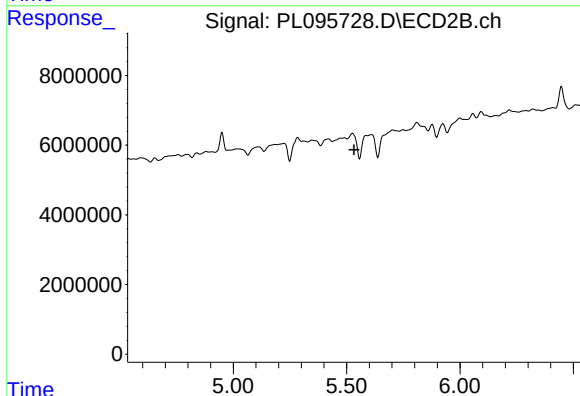


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.533 min
Response: 0
Conc: N.D.

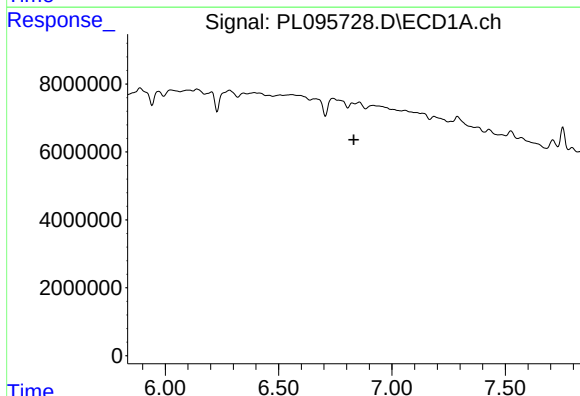


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.831 min
Response: 0
Conc: N.D.

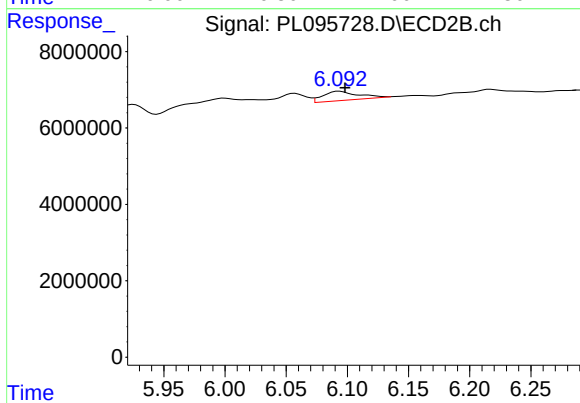

#15 Endosulfan II


R.T.: 6.093 min
Delta R.T.: -0.005 min
Response: 4812291
Conc: 0.88 ng/ml

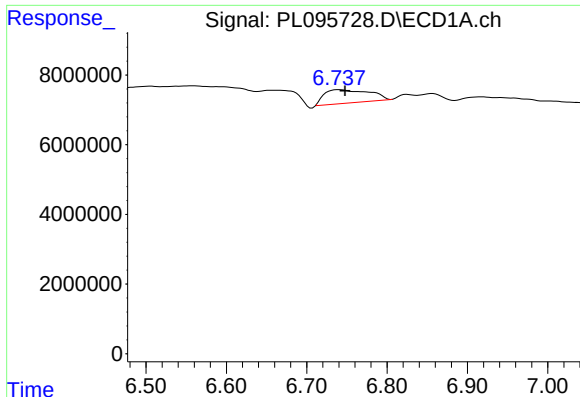

#16 4,4'-DDD


R.T.: 6.740 min
Delta R.T.: -0.008 min
Response: 15110724
Conc: 3.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-32

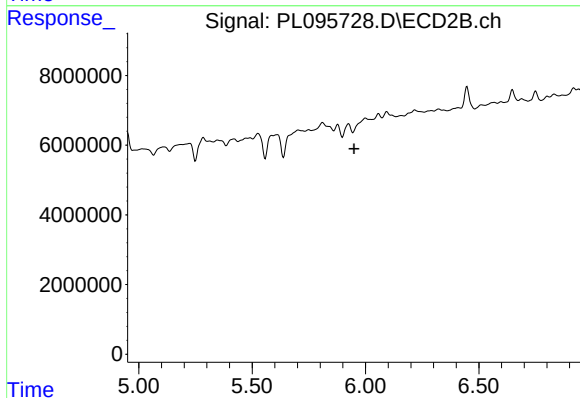


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

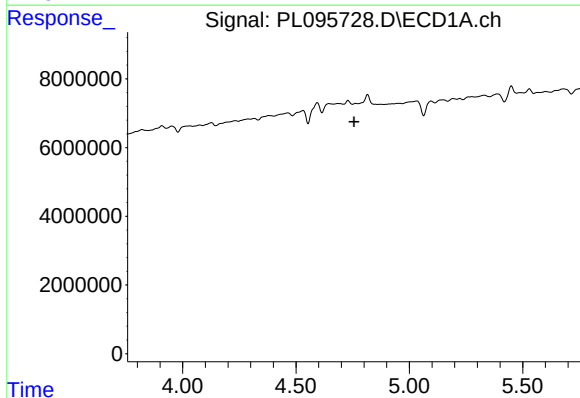


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.756 min
Response: 0
Conc: N.D.

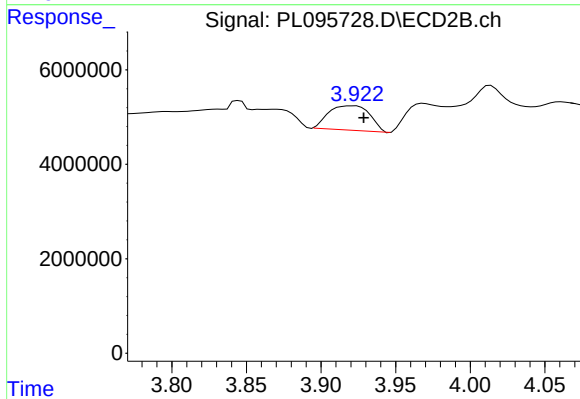

#23 Chlordane-1


R.T.: 3.922 min
Delta R.T.: -0.007 min
Response: 9931512
Conc: 41.27 ng/ml

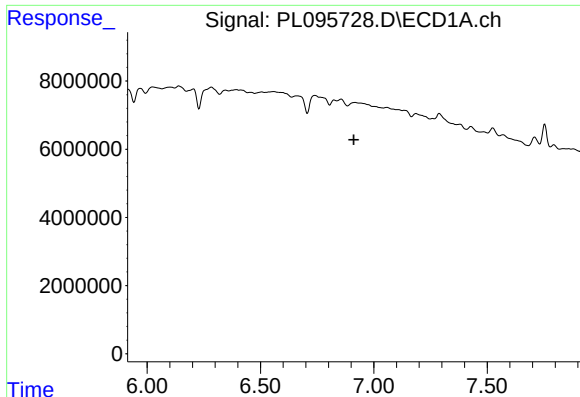

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-32

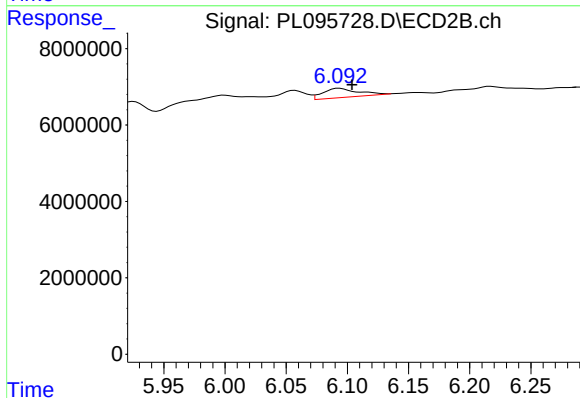


#27 Chlordane-5

R.T.: 6.093 min
Delta R.T.: -0.010 min
Response: 4812291
Conc: 16.75 ng/ml

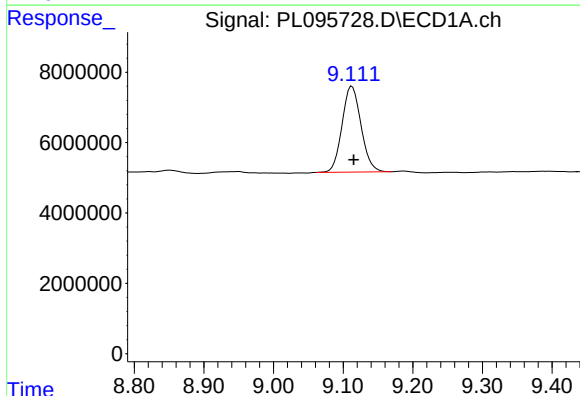

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: -0.003 min
Response: 46283029
Conc: 13.64 ng/ml

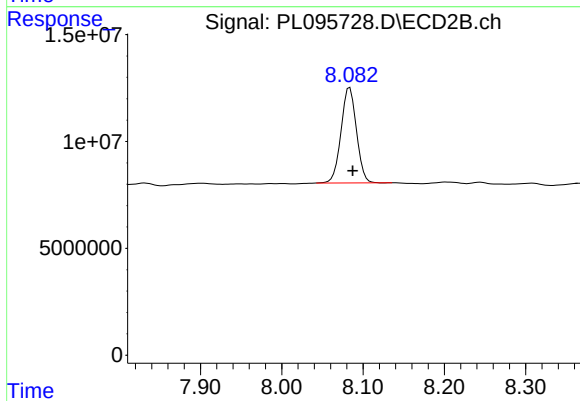

#28 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: -0.004 min
Response: 58626370
Conc: 14.21 ng/ml