
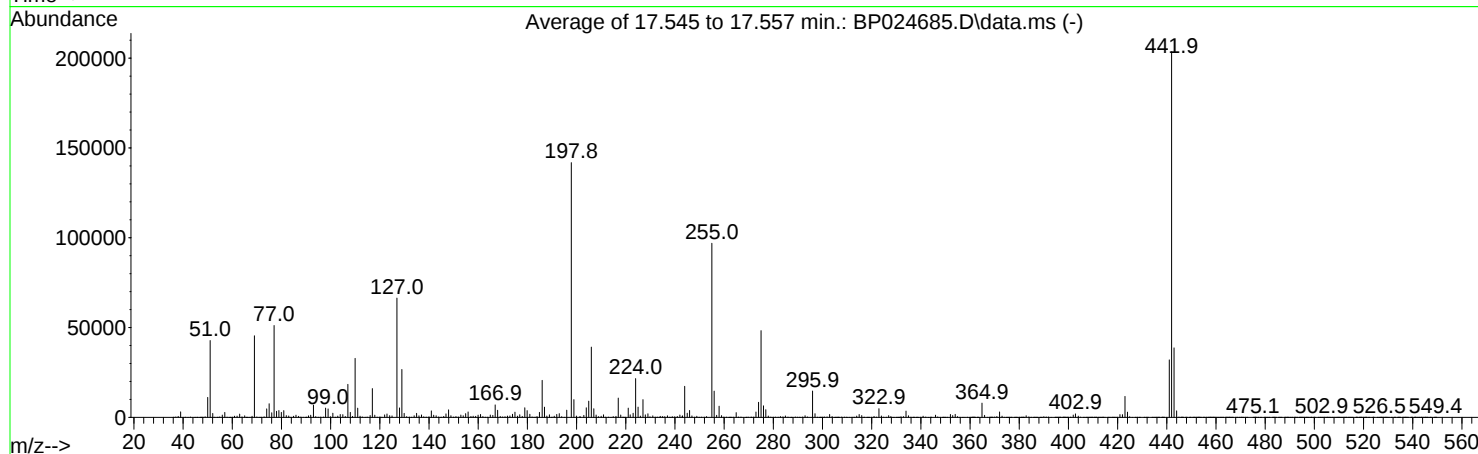


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051925\
Data File : BP024685.D
Acq On : 19 May 2025 11:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 13 16:21:39 2025

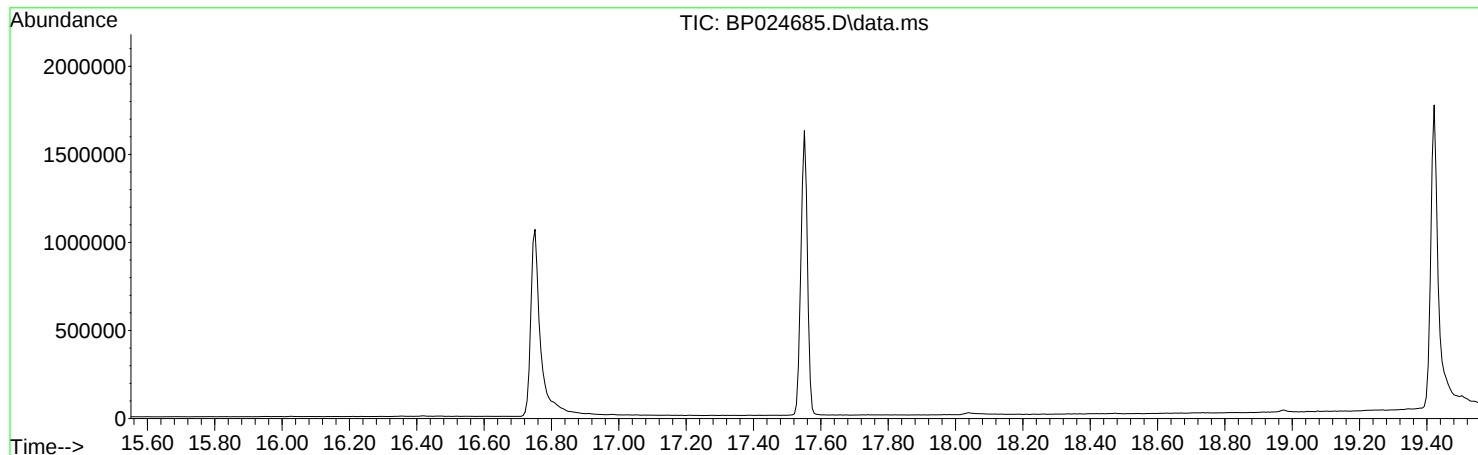

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	42781	PASS
68	69	0.00	2	1.3	608	PASS
69	198	0.00	100	32.0	45436	PASS
70	69	0.00	2	0.5	248	PASS
127	198	10	80	46.8	66420	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	141834	PASS
199	198	5	9	7.0	9883	PASS
275	198	10	60	34.1	48297	PASS
365	198	1	100	5.6	7951	PASS
441	198	0.01	100	22.6	32009	PASS
442	442	100	100	100.0	203603	PASS
443	442	15	24	19.0	38702	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/19/2025	BNA_P	<u>BP024685.D</u>
Compound Name	Response	Retention Time
DDT	528818	20.71
DDD	19377	20.251
DDE	3479	19.721
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22856	551674	4.14

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051925\
Data File : BP024685.D
Acq On : 19 May 2025 11:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 19 14:36:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

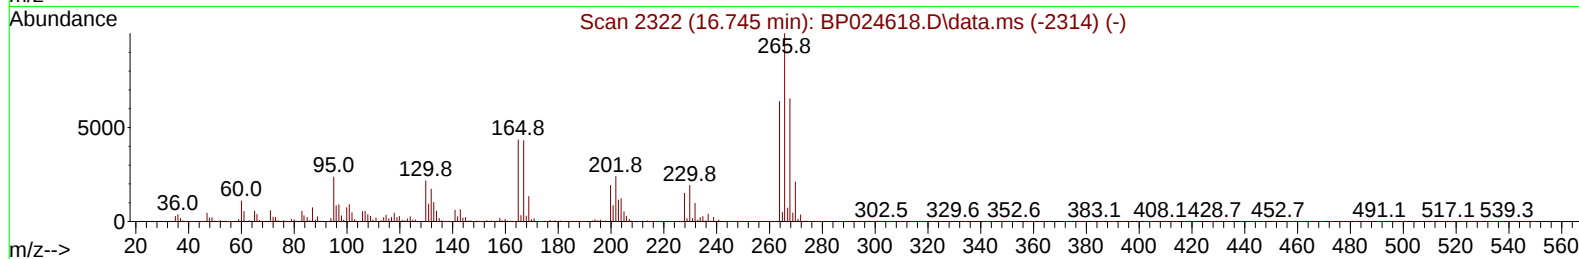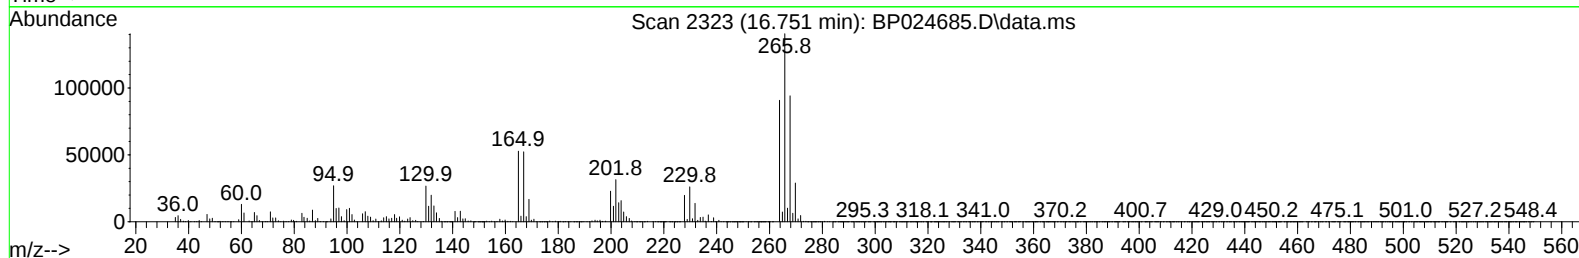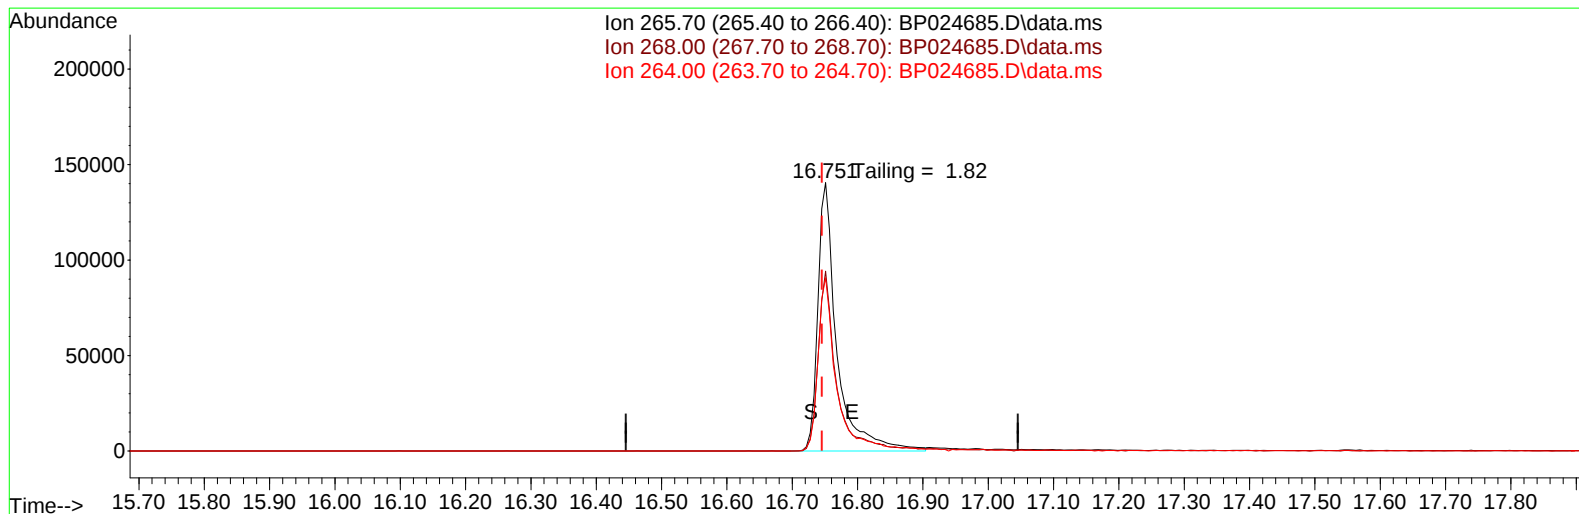

TIC: BP024685.D\data.ms

(70) Pentachlorophenol (C)

16.751min (+ 0.006) 677862.06 ng




response 284874

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	67.02
264.00	63.90	64.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051925\
Data File : BP024685.D
Acq On : 19 May 2025 11:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 19 14:36:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

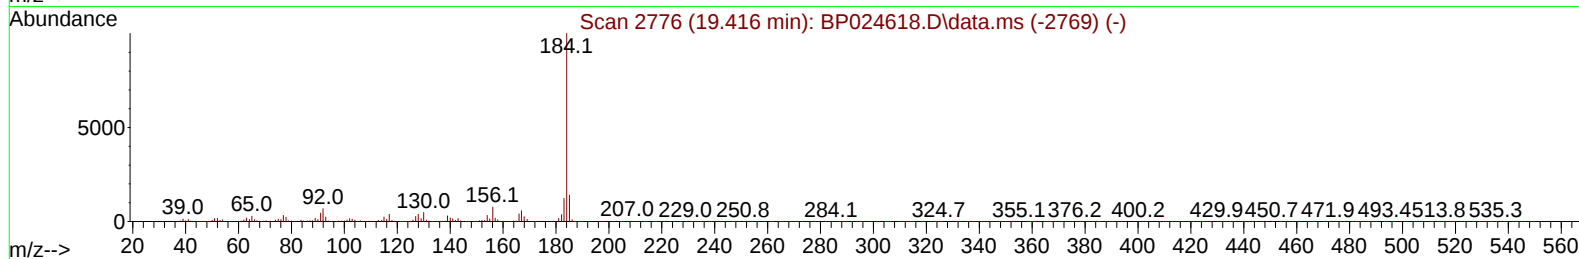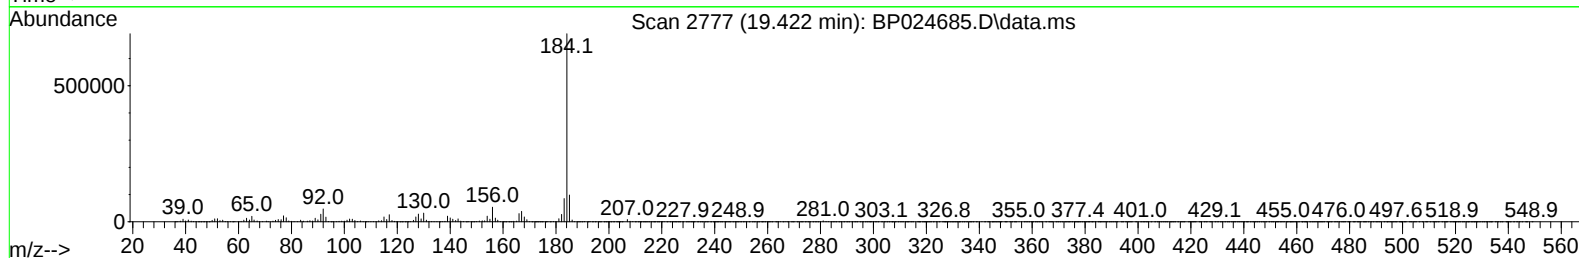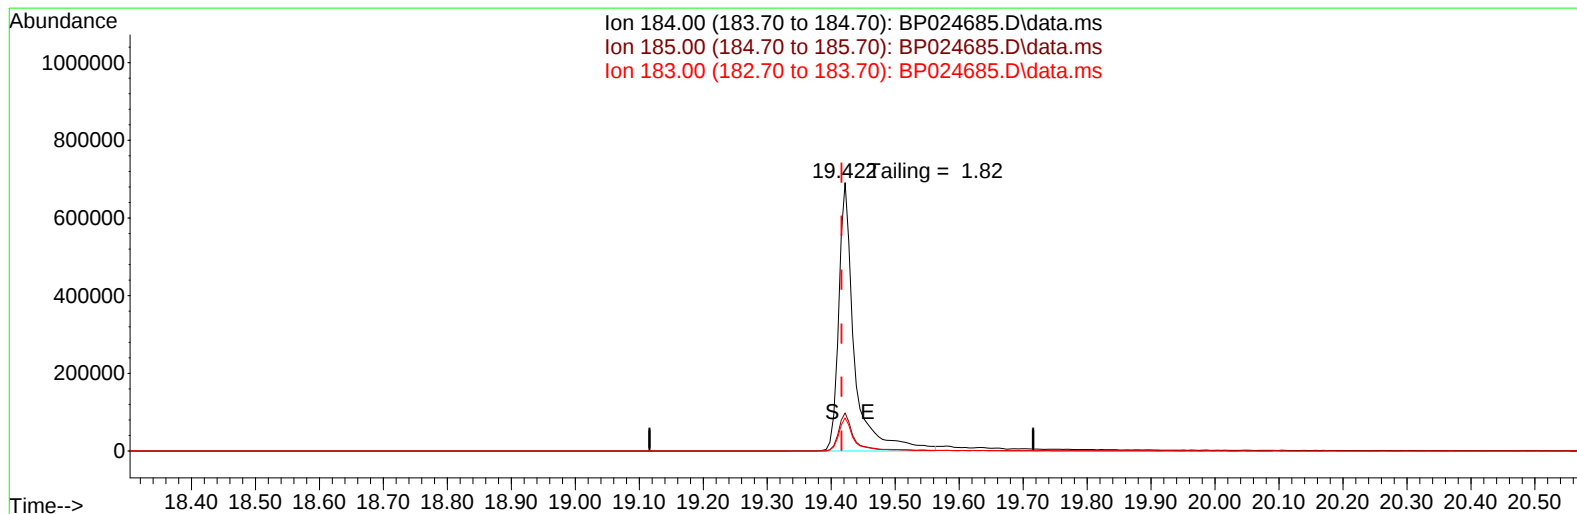

TIC: BP024685.D\data.ms

(77) Benzidine

19.422min (+ 0.006) 78779.38 ng

response 1186534

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.18
183.00	12.30	12.34
0.00	0.00	0.00