

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052125\
 Data File : VN086723.D
 Acq On : 21 May 2025 11:44
 Operator : JC\MD
 Sample : VN0521MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0521MBL01

Quant Time: May 22 01:19:34 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
 Quant Title : SW846 8260
 QLast Update : Sat May 17 00:46:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	158233	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	315437	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	297842	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	126400	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	114876	52.539	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	105.080%
35) Dibromofluoromethane	8.165	113	99727	53.087	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	106.180%
50) Toluene-d8	10.565	98	404936	52.016	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	104.040%
62) 4-Bromofluorobenzene	12.847	95	141014	51.300	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	102.600%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052125\
Data File : VN086723.D
Acq On : 21 May 2025 11:44
Operator : JC\MD
Sample : VN0521MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0521MBL01

Quant Time: May 22 01:19:34 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
Quant Title : SW846 8260
QLast Update : Sat May 17 00:46:13 2025
Response via : Initial Calibration




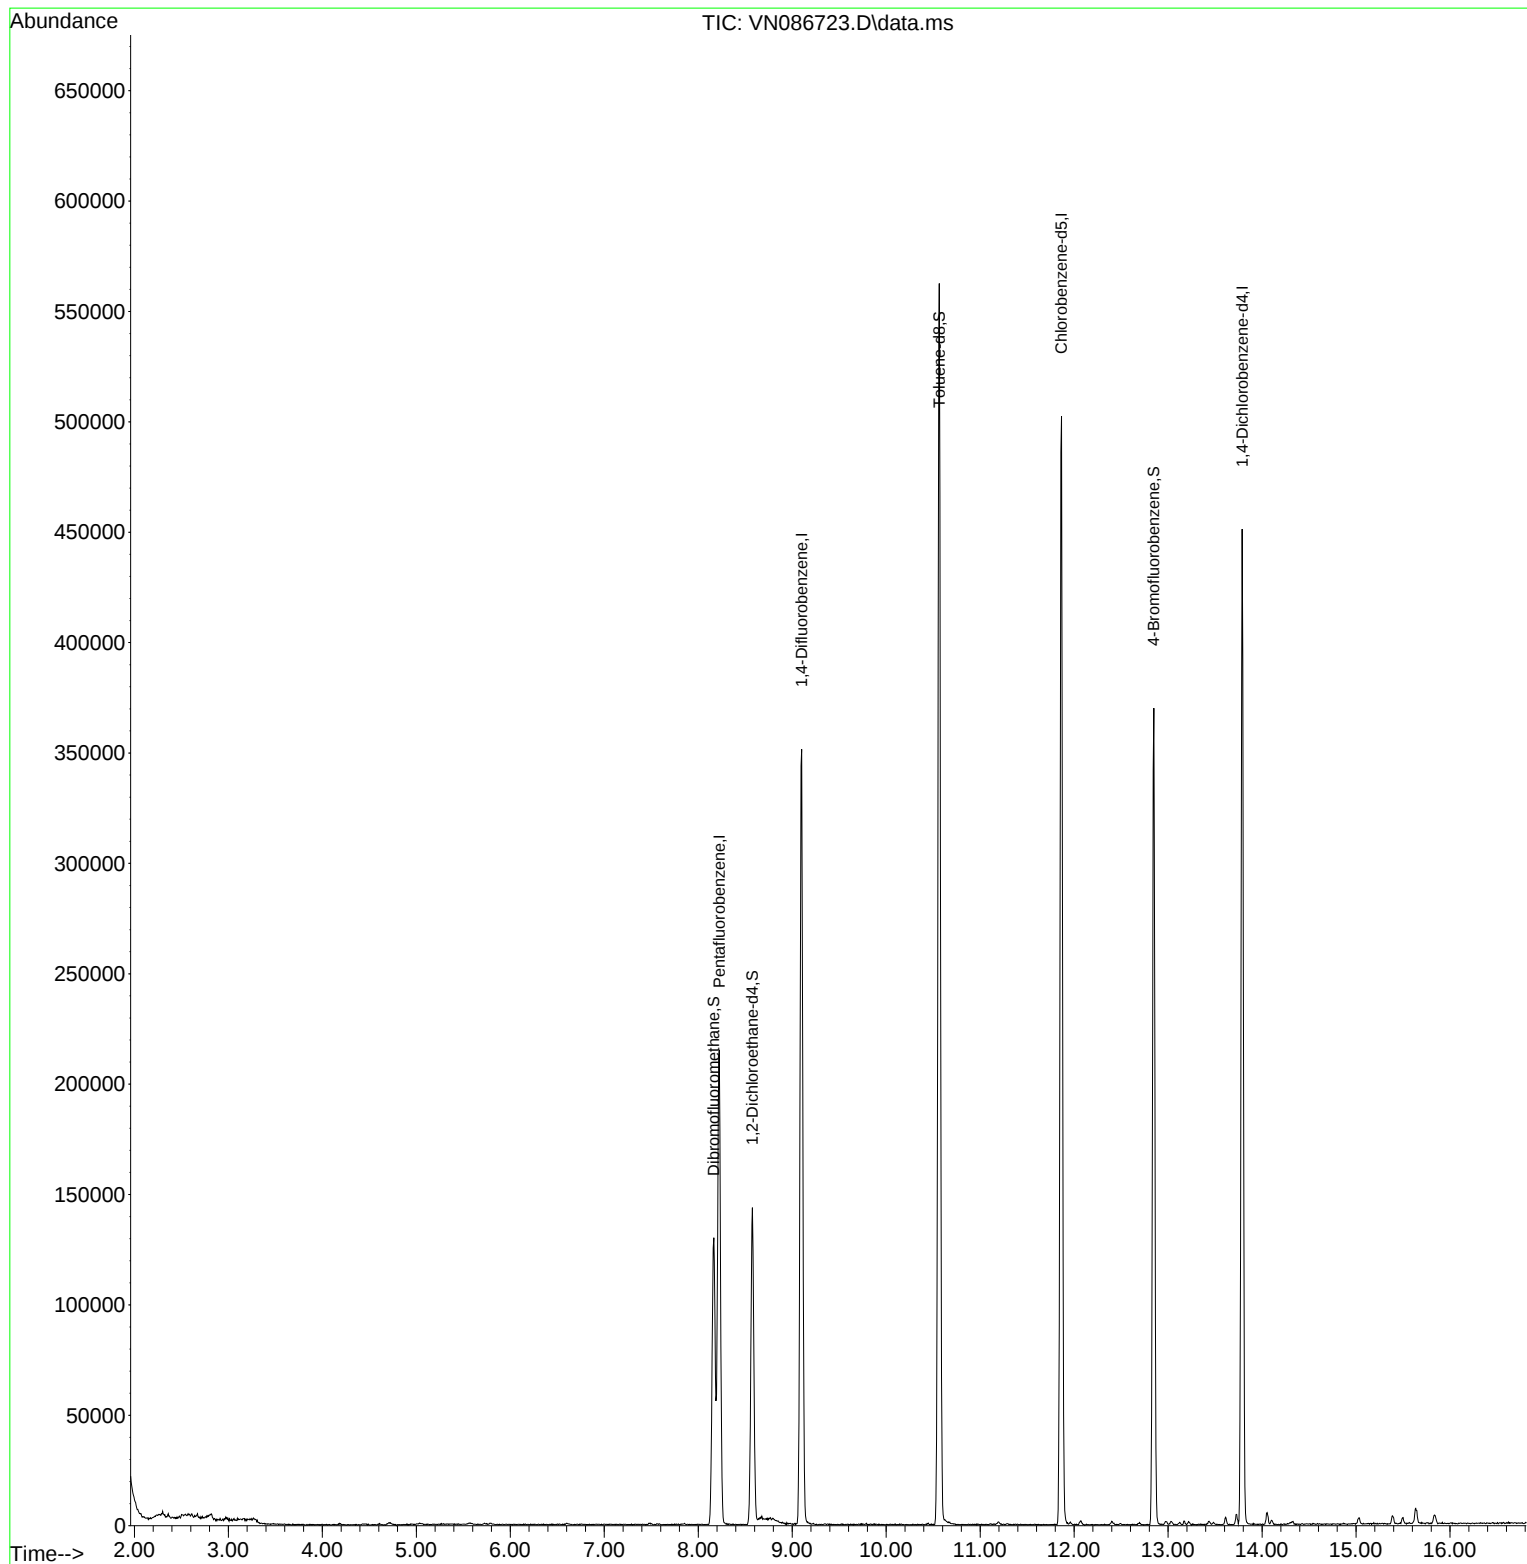


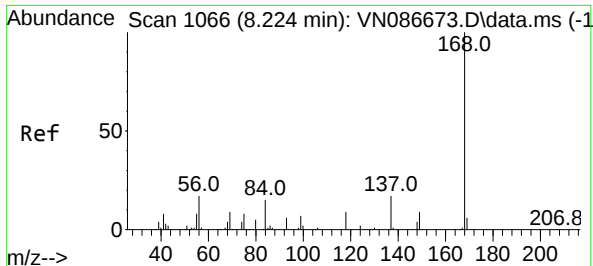

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN086723.D
Acq: 21 May 2025 11:44




Instrument :
MSVOA_N
ClientSampleId :
VN0521MBL01


Tgt Ion:168 Resp: 158233
Ion Ratio Lower Upper
168 100
99 60.4 47.0 70.4

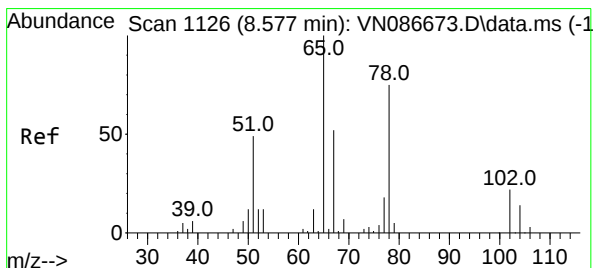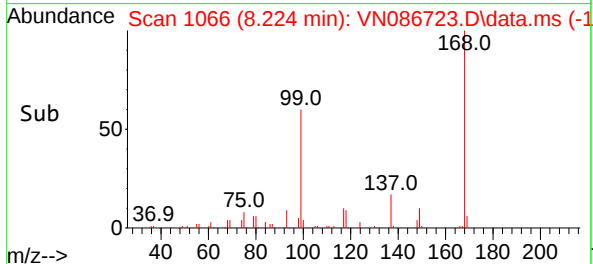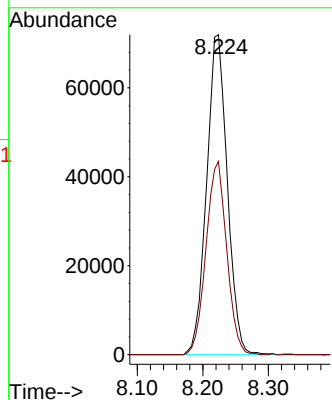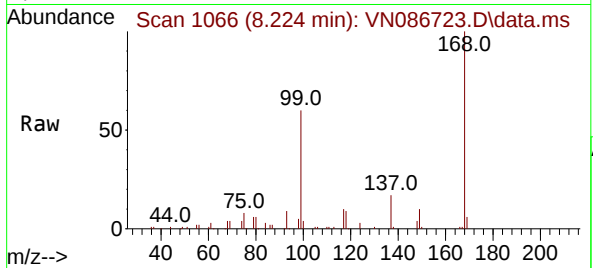

#33
1,2-Dichloroethane-d4
Concen: 52.539 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN086723.D
Acq: 21 May 2025 11:44

Tgt Ion: 65 Resp: 114876
Ion Ratio Lower Upper
65 100
67 55.1 0.0 106.4

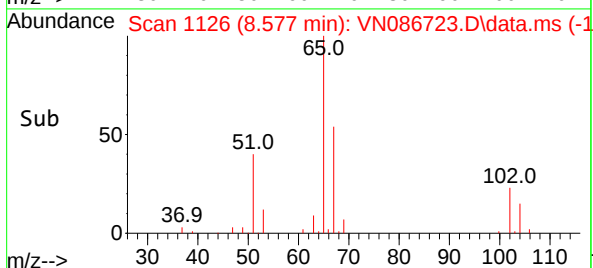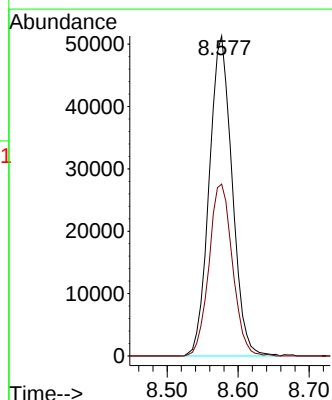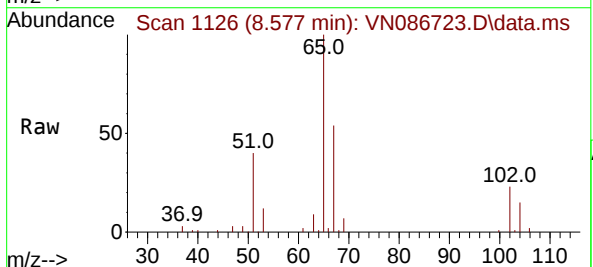

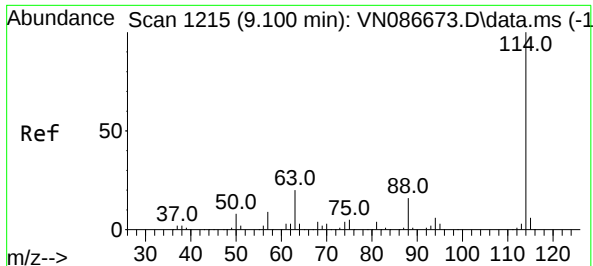

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN086723.D

Acq: 21 May 2025 11:44

Instrument :

MSVOA_N

ClientSampleId :

VN0521MBL01





Tgt Ion:114 Resp: 315437

Ion Ratio Lower Upper

114 100

63 20.4 0.0 40.2

88 15.5 0.0 31.2

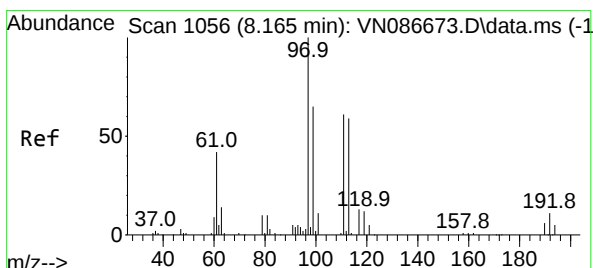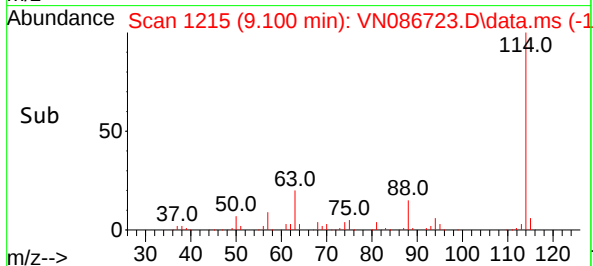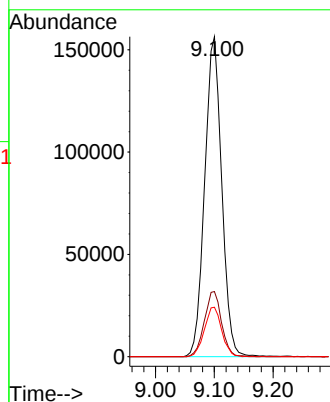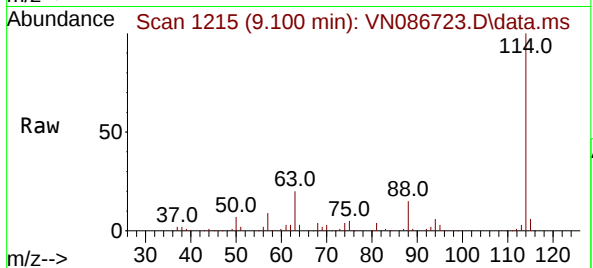

#35

Dibromofluoromethane

Concen: 53.087 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN086723.D

Acq: 21 May 2025 11:44




Tgt Ion:113 Resp: 99727


Ion Ratio Lower Upper

113 100

111 102.0 82.2 123.2

192 16.2 13.8 20.8


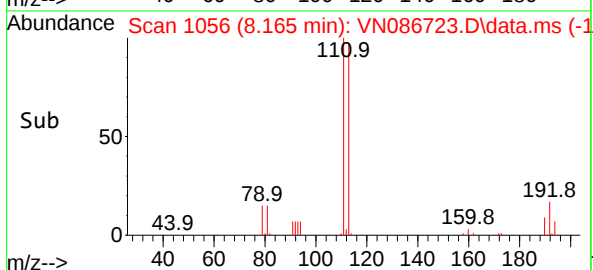
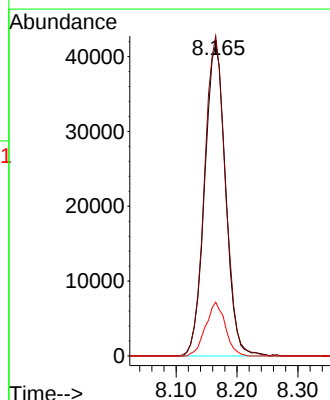
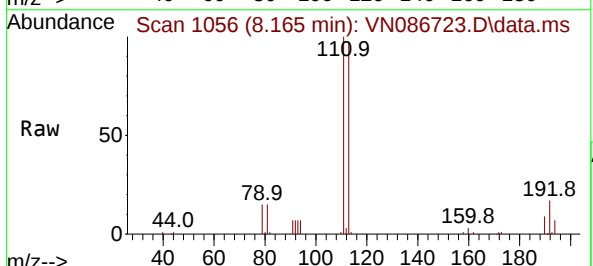


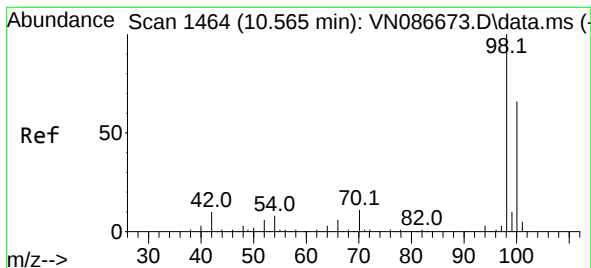

#50
Toluene-d8
Concen: 52.016 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN086723.D
Acq: 21 May 2025 11:44




Instrument :
MSVOA_N
ClientSampleId :
VN0521MBL01


Tgt Ion: 98 Resp: 404936
Ion Ratio Lower Upper
98 100
100 65.3 52.9 79.3

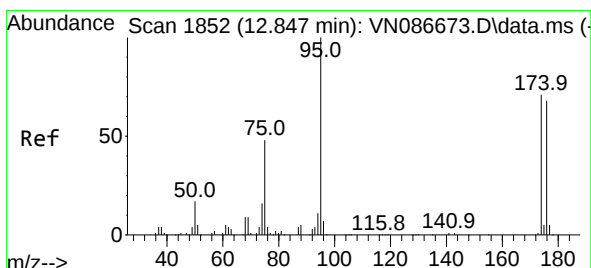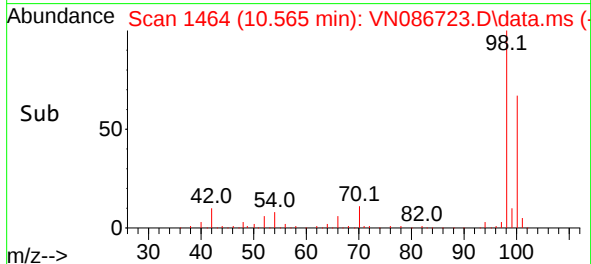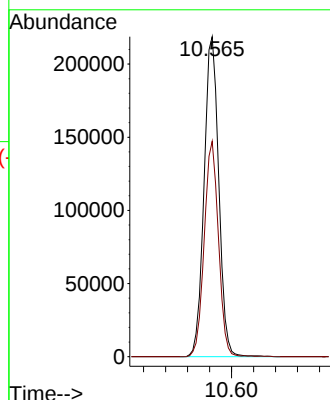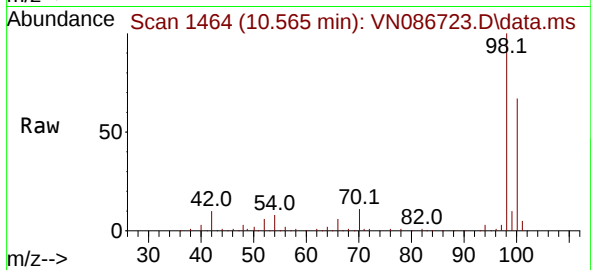

#62
4-Bromofluorobenzene
Concen: 51.300 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN086723.D
Acq: 21 May 2025 11:44

Tgt Ion: 95 Resp: 141014
Ion Ratio Lower Upper
95 100
174 70.4 0.0 145.4
176 68.0 0.0 137.8


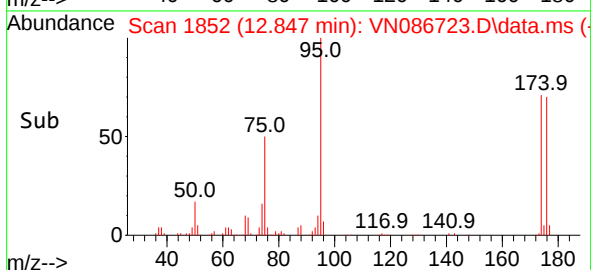
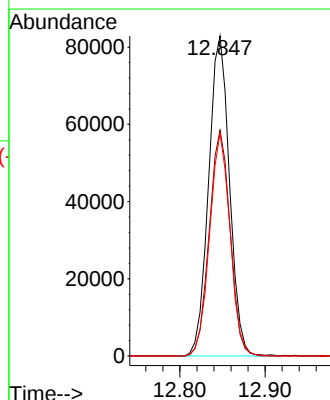
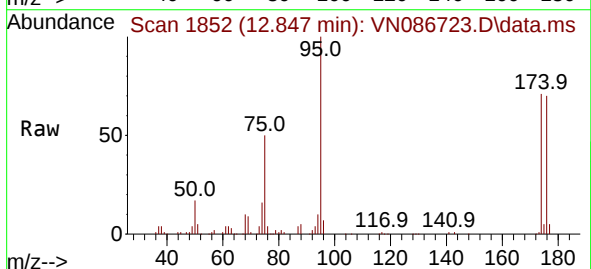


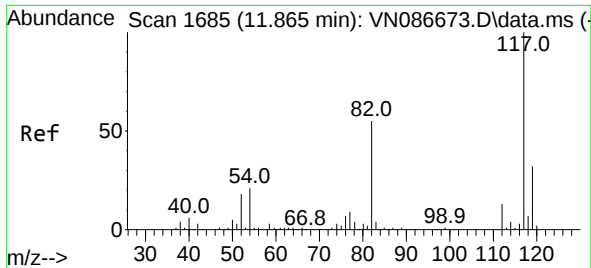

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN086723.D
Acq: 21 May 2025 11:44

Instrument :
MSVOA_N
ClientSampleId :
VN0521MBL01

Tgt Ion:117 Resp: 297842
Ion Ratio Lower Upper
117 100
82 57.5 44.2 66.2
119 32.9 25.4 38.2

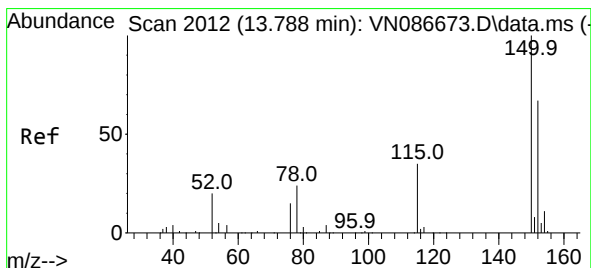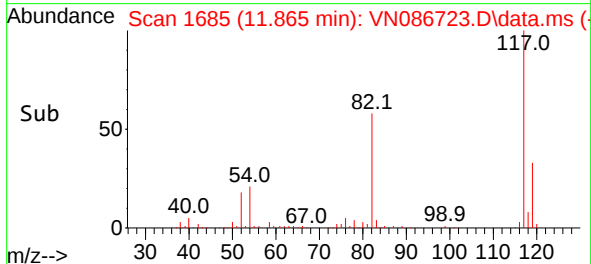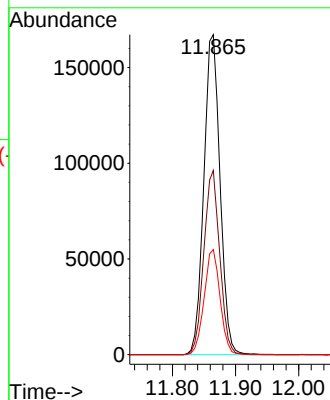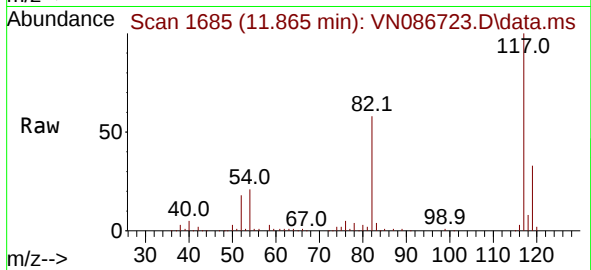

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. 0.000 min
Lab File: VN086723.D
Acq: 21 May 2025 11:44

Tgt Ion:152 Resp: 126400
Ion Ratio Lower Upper
152 100
115 61.0 30.0 90.1
150 157.3 0.0 347.8

