

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL041725

Review By	MMDadoda	Review On	4/18/2025 10:46:12 PM
Supervise By		Supervise On	
SubDirectory	VL041725	HP Acquire Method	TO15AIR.M
		HP Processing Method	VL041725AIR.M
STD. NAME	STD REF.#		
Tune/Reschk	AP2590		
Initial Calibration Stds	AP2598,AP2599,AP2600		
CCC	AP2598		
Internal Standard/PEM	AP2590		
ICV/I.BLK	AP2601		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VL042348.D	17 Apr 2025 07:50	SY/MD	Ok
2	VSTDICCC010	VL042349.D	17 Apr 2025 09:44	SY/MD	Ok,M
3	VSTDICCC002	VL042350.D	17 Apr 2025 10:17	SY/MD	Ok,M
4	VSTDICCC001	VL042351.D	17 Apr 2025 10:48	SY/MD	Ok,M
5	VSTDICCC0.5	VL042352.D	17 Apr 2025 11:19	SY/MD	Ok,M
6	VSTDICCC0.1	VL042353.D	17 Apr 2025 11:50	SY/MD	Ok,M
7	VSTDICCC0.03	VL042354.D	17 Apr 2025 12:22	SY/MD	Ok,M
8	VSTDICCC015	VL042355.D	17 Apr 2025 12:54	SY/MD	Ok,M
9	VSTDICV010	VL042356.D	17 Apr 2025 13:43	SY/MD	Ok,M
10	VL0417ABL01	VL042357.D	17 Apr 2025 14:23	SY/MD	Ok
11	VL0417ABS01	VL042358.D	17 Apr 2025 15:39	SY/MD	Ok,M
12	Q1665-15	VL042359.D	17 Apr 2025 16:12	SY/MD	Dilution
13	Q1665-15DL	VL042360.D	17 Apr 2025 16:44	SY/MD	Ok,M
14	Q1668-01	VL042361.D	17 Apr 2025 17:17	SY/MD	Dilution
15	Q1668-01DUP	VL042362.D	17 Apr 2025 17:51	SY/MD	Ok,M
16	Q1668-03	VL042363.D	17 Apr 2025 18:24	SY/MD	Dilution
17	Q1668-04	VL042364.D	17 Apr 2025 18:58	SY/MD	Ok,M
18	Q1668-02	VL042365.D	17 Apr 2025 19:31	SY/MD	Ok,M
19	Q1726-01	VL042366.D	17 Apr 2025 20:05	SY/MD	Dilution
20	Q1726-02	VL042367.D	17 Apr 2025 20:38	SY/MD	Dilution
21	Q1726-03	VL042368.D	17 Apr 2025 21:12	SY/MD	Dilution

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL041725

Review By	MMDadoda	Review On	4/18/2025 10:46:12 PM
Supervise By		Supervise On	
SubDirectory	VL041725	HP Acquire Method	TO15AIR.M
		HP Processing Method	VL041725AIR.M
STD. NAME	STD REF.#		
Tune/Reschk	AP2590		
Initial Calibration Stds	AP2598,AP2599,AP2600		
CCC	AP2598		
Internal Standard/PEM	AP2590		
ICV/I.BLK	AP2601		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	Q1726-04	VL042369.D	17 Apr 2025 21:45	SY/MD	Dilution
23	Q1726-05	VL042370.D	17 Apr 2025 22:19	SY/MD	Dilution
24	Q1726-06	VL042371.D	17 Apr 2025 22:52	SY/MD	Dilution
25	Q1726-07	VL042372.D	17 Apr 2025 23:26	SY/MD	Dilution
26	Q1726-07DL	VL042373.D	17 Apr 2025 23:57	SY/MD	Dilution
27	Q1668-01DL	VL042374.D	18 Apr 2025 00:28	SY/MD	Ok,M
28	Q1668-03DL	VL042375.D	18 Apr 2025 00:59	SY/MD	Ok,M
29	Q1726-01DL	VL042376.D	18 Apr 2025 01:30	SY/MD	Dilution
30	Q1726-02DL	VL042377.D	18 Apr 2025 02:01	SY/MD	Dilution
31	Q1726-03DL	VL042378.D	18 Apr 2025 02:32	SY/MD	Dilution
32	Q1726-04DL	VL042379.D	18 Apr 2025 03:03	SY/MD	Dilution
33	Q1726-05DL	VL042380.D	18 Apr 2025 03:34	SY/MD	Dilution
34	Q1726-06DL	VL042381.D	18 Apr 2025 04:05	SY/MD	Dilution

M : Manual Integration

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL042125

Review By	MMDadoda	Review On	4/22/2025 2:00:33 PM
Supervise By		Supervise On	
SubDirectory	VL042125	HP Acquire Method	TO15AIR.M
		HP Processing Method	VL041725AIR.M
STD. NAME	STD REF.#		
Tune/Reschk	AP2602		
Initial Calibration Stds	AP2598,AP2599,AP2600		
CCC	AP2598		
Internal Standard/PEM	AP2602		
ICV/I.BLK	AP2601		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VL042394.D	21 Apr 2025 07:58	SY/MD	Ok
2	VSTDCCC010	VL042395.D	21 Apr 2025 08:41	SY/MD	Ok,M
3	VL0421ABL01	VL042396.D	21 Apr 2025 09:28	SY/MD	Ok
4	VL0421ABS01	VL042397.D	21 Apr 2025 10:14	SY/MD	Ok,M
5	QC041625 CAN 10329	VL042398.D	21 Apr 2025 11:04	SY/MD	Not Ok
6	QC041625 CAN 10329	VL042399.D	21 Apr 2025 11:36	SY/MD	Ok
7	Q1801-01	VL042400.D	21 Apr 2025 12:07	SY/MD	Ok,M
8	Q1801-02	VL042401.D	21 Apr 2025 12:51	SY/MD	Ok,M
9	Q1844-02	VL042402.D	21 Apr 2025 13:38	SY/MD	Dilution
10	Q1844-02DUP	VL042403.D	21 Apr 2025 14:13	SY/MD	Ok,M
11	Q1844-02DL	VL042404.D	21 Apr 2025 14:44	SY/MD	Ok,M
12	Q1843-02	VL042405.D	21 Apr 2025 15:18	SY/MD	Ok,M
13	Q1843-02DL	VL042406.D	21 Apr 2025 15:49	SY/MD	Not Ok
14	Q1844-01	VL042407.D	21 Apr 2025 16:20	SY/MD	Dilution
15	Q1844-01DL	VL042408.D	21 Apr 2025 16:51	SY/MD	Dilution
16	Q1843-01	VL042409.D	21 Apr 2025 17:23	SY/MD	Ok,M
17	Q1843-01DL	VL042410.D	21 Apr 2025 17:54	SY/MD	Not Ok
18	Q1843-01DUP	VL042411.D	21 Apr 2025 19:16	SY/MD	Ok,M
19	QC041725 CA 27806	VL042412.D	21 Apr 2025 19:47	SY/MD	Not Ok
20	QC041725 CA 27806	VL042413.D	21 Apr 2025 20:18	SY/MD	Ok
21	Q1844-01DL2	VL042414.D	22 Apr 2025 07:47	SY/MD	Ok,M

M : Manual Integration

Process Report

Order ID : q2037



Date	Bottle ID	Lab Sample Number	InComing Vacuum	Canister ID	Can Size	Reg ID	Reg Size	Batch Code	Certification ID
05/14/2025	B2505020	Q2037-01	-5.5	10609	6 L	10550		C2504008	VL042399.D Seq :VL042125 TUNE : VL042394.D ICAL : VL042354.D CCAL : VL042395.D MB : VL042396.D
05/14/2025	B2505020	Q2037-02	-5.5	10285	6 L	10503		C2504008	VL042399.D Seq :VL042125 TUNE : VL042394.D ICAL : VL042354.D CCAL : VL042395.D MB : VL042396.D

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
Data File : VL042348.D
Acq On : 17 Apr 2025 07:50
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Apr 18 02:14:00 2025

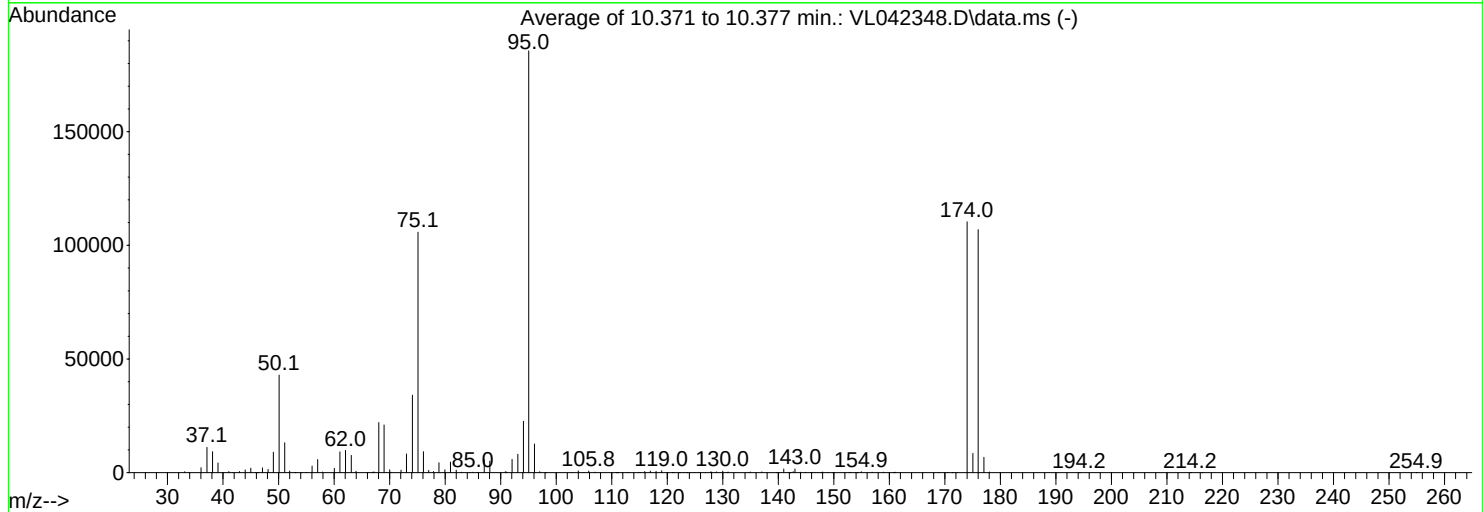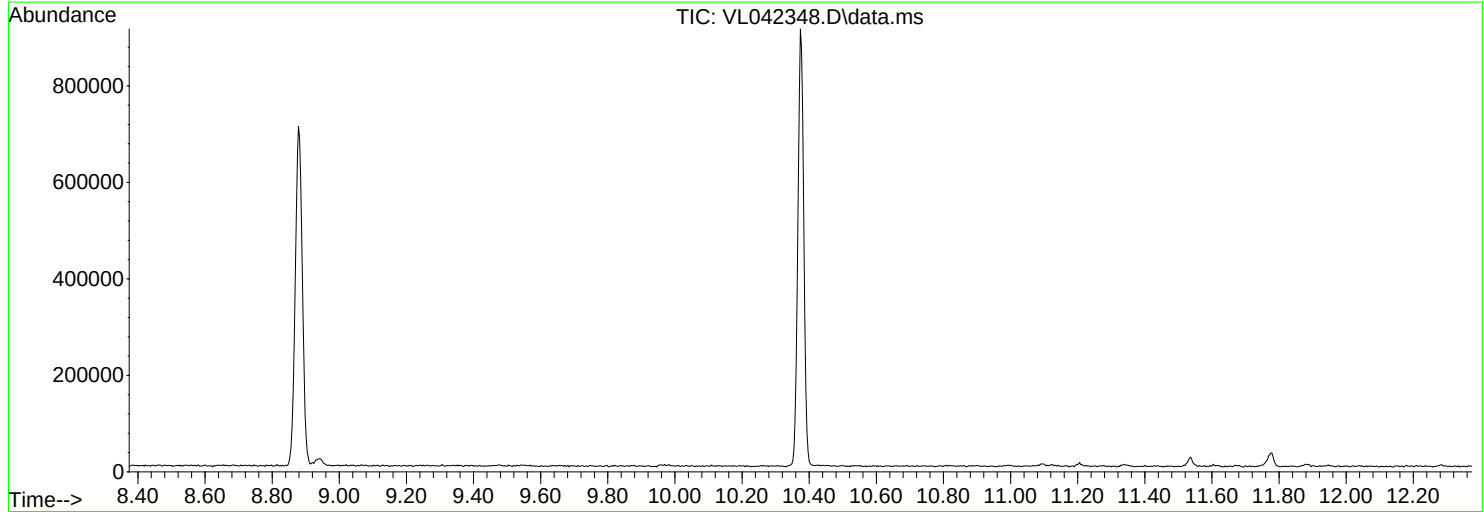

AutoFind: Scans 3177, 3178, 3179; Background Corrected with Scan 3162

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	23.1	42933	PASS
75	95	30	66	57.0	105781	PASS
95	95	100	100	100.0	185564	PASS
96	95	5	9	6.8	12627	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	59.5	110360	PASS
175	174	4	9	7.6	8420	PASS
176	174	93	101	96.9	106933	PASS
177	176	5	9	6.3	6744	PASS

Average of 10.371 to 10.377 min.: VL042348.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	400	45.00	1996	55.00	78	67.20	32
34.00	54	45.90	94	56.05	2900	68.05	2203
36.05	2214	46.20	34	57.05	5754	69.00	2101
37.10	11145	47.10	2100	57.95	265	70.00	130
38.10	9197	48.10	1438	60.05	1919	70.20	209
39.10	4289	49.05	9045	61.05	9155	72.05	1141
39.95	158	50.10	42933	62.05	9788	73.05	8240
41.05	513	51.10	13188	63.10	7593	74.10	34064
41.80	79	52.00	718	63.95	632	75.10	105781
42.95	504	52.95	9	66.10	115	76.10	9240
44.00	1207	54.15	112	66.90	196	77.05	979

Average of 10.371 to 10.377 min.: VL042348.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.90	494	90.85	447	105.00	95	115.95	528
78.90	4344	91.10	262	105.85	680	116.95	712
79.95	1296	92.05	5876	107.00	225	118.00	575
80.95	4648	93.10	8069	110.10	136	119.00	881
82.00	1107	94.10	22619	110.80	37	120.10	70
83.00	249	95.05	185564	111.10	8	120.90	30
84.40	55	96.10	12627	111.95	156	121.30	47
85.00	227	97.05	457	112.75	77	122.20	21
85.85	131	98.05	5	113.10	144	122.95	44
87.05	5767	102.90	78	114.80	135	123.50	25
88.05	5057	104.00	767	115.10	50	124.10	89

Average of 10.371 to 10.377 min.: VL042348.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.90	71	137.05	364	146.15	158	153.90	93
125.75	72	139.65	74	146.65	58	154.20	27
126.90	80	140.00	38	147.10	68	154.95	399
127.80	297	141.00	1612	147.70	38	156.90	228
128.00	275	141.80	139	148.00	288	158.95	203
128.85	366	142.10	34	148.95	115	160.80	26
130.00	693	142.70	434	149.80	37	161.05	186
130.80	55	143.00	1656	149.95	79	168.90	83
130.95	285	143.95	200	151.90	60	170.50	119
134.70	94	144.95	161	152.75	91	171.30	19
135.00	292	145.80	67	153.05	144	171.90	90

Average of 10.371 to 10.377 min.: VL042348.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.30	132						
174.00	110360						
175.05	8420						
176.00	106933						
177.05	6744						
178.05	298						
194.20	17						
214.20	17						
216.30	17						
254.90	17						

Instrument :

MSVOA.L

ClientSampleId :

BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
 Data File : VL042349.D
 Acq On : 17 Apr 2025 09:44
 Operator : SY/MD
 Sample : VSTDICCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/18/2025
 Supervised By : Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 01:25:08 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2025

QLast Update : Fri Apr 18 01:24:29 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	125455	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.959	114	366544	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.882	117	338126	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.377 95 281013 10.114 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 101.100%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.499	85	207962	9.382	ppbv	100
3) Chlorodifluoromethane	1.476	51	197334	9.350	ppbv	100
4) Chloromethane	1.531	50	81843	9.330	ppbv	100
5) Vinyl Chloride	1.580	62	80068	8.385	ppbv	100
6) Bromomethane	1.667	94	38128	9.219	ppbv	100
7) Chloroethane	1.703	64	31705	9.182	ppbv	100
8) Dichlorotetrafluoroethane	1.554	85	179696	9.442	ppbv	100
9) Propene	1.483	41	86530	9.002	ppbv	100
10) Heptane	4.978	43	236341	9.138	ppbv	100
11) Trichlorofluoromethane	1.877	101	196596	9.327	ppbv	100
12) 1,1,2-Trichlorotrifluo...	2.136	101	160682	9.323	ppbv	100
13) Ethanol	1.719	45	4439	5.651	ppbv	100
14) Bromoethene	1.780	108	61493	9.466	ppbv	100
15) Acetone	1.835	43	158490	7.717	ppbv	100
16) 1,3-Butadiene	1.609	39	81688	8.470	ppbv	100
17) tert-Butyl alcohol	2.039	59	226280	8.891	ppbv	100
18) 1,1-Dichloroethene	2.033	96	73186	8.833	ppbv	100
19) Isopropyl Alcohol	1.884	45	103029	9.031	ppbv	100
20) Methylene Chloride	2.062	84	62414	7.760	ppbv	100
21) Allyl Chloride	2.094	41	122115	8.611	ppbv	100
22) trans-1,2-Dichloroethene	2.340	96	83278	9.084	ppbv	100
23) Vinyl Acetate	2.460	43	69649	8.378	ppbv	100
24) 1,1-Dichloroethane	2.408	63	161102	9.251	ppbv	100
25) Ethyl Acetate	2.836	43	461315	9.110	ppbv	100
26) Hexane	2.826	57	178691	8.720	ppbv	100
27) Carbon Disulfide	2.149	76	209297	9.539	ppbv	100
28) Methyl tert-Butyl Ether	2.441	73	117924	8.783	ppbv	100
29) Chloroform	2.848	83	269088	9.290	ppbv	100
30) Cyclohexane	3.855	84	157035	9.517	ppbv	100
31) cis-1,2-Dichloroethene	2.719	61	183082	9.397	ppbv	100
32) 1,1,1-Trichloroethane	3.366	97	285336	9.187	ppbv	100
34) 2-Butanone	2.557	43	251704	8.683	ppbv	100
35) Carbon Tetrachloride	3.761	117	282402	8.513	ppbv	100
36) Benzene	3.654	78	367355	9.292	ppbv	100
37) 1,2-Dichloroethane	3.217	62	216999	9.145	ppbv	100
38) Trichloroethene	4.548	130	144767	8.352	ppbv	100
39) 1,2-Dichloropropane	4.311	63	135605	9.197	ppbv	100
40) 1,4-Dioxane	4.580	88	66662	8.348	ppbv #	100
41) Tetrahydrofuran	3.052	42	149905	8.950	ppbv	100
42) Bromodichloromethane	4.489	83	312268	9.456	ppbv	100
43) Methyl Methacrylate	4.881	69	157501	8.876	ppbv	100
44) 2,2,4-Trimethylpentane	4.642	57	626085	9.157	ppbv	100
45) t-1,3-Dichloropropene	6.415	75	168223	9.233	ppbv	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
 Data File : VL042349.D
 Acq On : 17 Apr 2025 09:44
 Operator : SY/MD
 Sample : VSTDICCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICCC010

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/18/2025
 Supervised By :Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 01:25:08 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Apr 18 01:24:29 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.600	75	208811	9.377	ppbv	100
47) 1,1,2-Trichloroethane	6.580	97	137898	9.181	ppbv	100
48) Dibromochloromethane	7.386	129	248954	9.388	ppbv	100
49) Bromoform	9.480	173	225706	9.734	ppbv	100
50) 4-Methyl-2-Pentanone	5.752	43	396548	8.215	ppbv	100
51) 2-Hexanone	7.435	43	327165	7.511	ppbv	100
52) Tetrachloroethene	8.225	164	130720	8.553	ppbv	100
53) Toluene	6.933	91	437258	9.216	ppbv	100
54) 1,2-Dibromoethane	7.652	107	197665	9.235	ppbv	100
56) 1,1,1,2-Tetrachloroethane	8.927	131	186041	9.091	ppbv	100
57) Chlorobenzene	8.920	112	323084	9.187	ppbv	100
58) Ethyl Benzene	9.354	91	619581	9.248	ppbv	100
59) m/p-Xylene	9.552	91	984458m	18.187	ppbv	
60) o-Xylene	9.963	91	487616	8.972	ppbv	100
61) Styrene	9.869	104	245487	9.464	ppbv	100
62) Isopropylbenzene	10.539	105	733788	9.197	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.963	83	295041	8.355	ppbv	100
64) n-propylbenzene	10.989	120	183390	9.144	ppbv	100
65) tert-Butylbenzene	11.532	119	644953	8.795	ppbv	100
66) Benzyl Chloride	11.617	91	83269	10.333	ppbv	100
67) sec-Butylbenzene	11.769	105	900074	8.824	ppbv	100
69) p-Isopropyltoluene	11.927	119	778987	8.790	ppbv	100
70) n-Butylbenzene	12.283	91	801364	8.682	ppbv	100
71) 2-Chlorotoluene	10.901	91	573039	9.157	ppbv	100
72) 4-Ethyltoluene	11.125	105	596757	8.982	ppbv	100
73) 1,3,5-Trimethylbenzene	11.205	105	512855	8.743	ppbv	100
74) 1,2,4-Trimethylbenzene	11.539	105	565064	8.248	ppbv	100
75) 1,3-Dichlorobenzene	11.607	146	320380	8.997	ppbv	100
76) 1,4-Dichlorobenzene	11.672	146	319089	8.915	ppbv	100
77) 1,2-Dichlorobenzene	11.947	146	305822	8.832	ppbv	100
78) Hexachloro-1,3-Butadiene	13.882	225	291833	8.346	ppbv	100
79) Naphthalene	13.513	128	677578	8.271	ppbv	100
80) Naphthalene,2-methyl-	14.458	142	376995	8.074	ppbv	100
81) 1,2,4-Trichlorobenzene	13.442	180	306119	8.702	ppbv	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
 Data File : VL042350.D
 Acq On : 17 Apr 2025 10:17
 Operator : SY/MD
 Sample : VSTDICC002
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC002

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/18/2025
 Supervised By : Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 01:26:23 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2025

QLast Update : Fri Apr 18 01:24:29 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	123206	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.959	114	355918	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.881	117	335603	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.377 95 275715 9.998 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 100.000%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.499	85	45008	2.068	ppbv	95
3) Chlorodifluoromethane	1.476	51	41853	2.019	ppbv	97
4) Chloromethane	1.534	50	17272	2.005	ppbv	93
5) Vinyl Chloride	1.580	62	16979	1.811	ppbv	92
6) Bromomethane	1.667	94	7398	1.821	ppbv #	80
7) Chloroethane	1.706	64	6889	2.031	ppbv	98
8) Dichlorotetrafluoroethane	1.554	85	38955	2.084	ppbv	98
9) Propene	1.483	41	18671	1.978	ppbv	97
10) Heptane	4.978	43	54438m	2.143	ppbv	
11) Trichlorofluoromethane	1.877	101	43035	2.079	ppbv	99
12) 1,1,2-Trichlorotrifluo...	2.140	101	35415	2.092	ppbv	100
13) Ethanol	1.722	45	3034m	3.933	ppbv	
14) Bromoethene	1.780	108	13049	2.045	ppbv #	92
15) Acetone	1.835	43	42949	2.129	ppbv	93
16) 1,3-Butadiene	1.609	39	18110	1.912	ppbv	96
17) tert-Butyl alcohol	2.042	59	51829	2.074	ppbv #	94
18) 1,1-Dichloroethene	2.036	96	15690	1.928	ppbv	87
19) Isopropyl Alcohol	1.887	45	22106	1.973	ppbv #	38
20) Methylene Chloride	2.062	84	14329	1.814	ppbv #	82
21) Allyl Chloride	2.098	41	27340	1.963	ppbv	95
22) trans-1,2-Dichloroethene	2.340	96	18142	2.015	ppbv	97
23) Vinyl Acetate	2.463	43	18454	2.260	ppbv #	91
24) 1,1-Dichloroethane	2.411	63	34077	1.993	ppbv	96
25) Ethyl Acetate	2.835	43	101467	2.040	ppbv	99
26) Hexane	2.826	57	40046	1.990	ppbv	99
27) Carbon Disulfide	2.149	76	43975	2.041	ppbv #	64
28) Methyl tert-Butyl Ether	2.441	73	27905	2.116	ppbv	97
29) Chloroform	2.848	83	58946	2.072	ppbv	100
30) Cyclohexane	3.858	84	33195	2.048	ppbv	94
31) cis-1,2-Dichloroethene	2.722	61	39249	2.051	ppbv	98
32) 1,1,1-Trichloroethane	3.366	97	61442	2.014	ppbv	99
34) 2-Butanone	2.560	43	58249	2.069	ppbv	100
35) Carbon Tetrachloride	3.761	117	60291	1.872	ppbv	88
36) Benzene	3.658	78	79814	2.079	ppbv	98
37) 1,2-Dichloroethane	3.217	62	47398	2.057	ppbv	100
38) Trichloroethene	4.544	130	31826m	1.891	ppbv	
39) 1,2-Dichloropropane	4.315	63	28806	2.012	ppbv	96
40) 1,4-Dioxane	4.593	88	16536m	2.133	ppbv	
41) Tetrahydrofuran	3.059	42	33298	2.047	ppbv	98
42) Bromodichloromethane	4.489	83	64941	2.025	ppbv	97
43) Methyl Methacrylate	4.881	69	35256	2.046	ppbv	97
44) 2,2,4-Trimethylpentane	4.645	57	139641	2.103	ppbv	99
45) t-1,3-Dichloropropene	6.415	75	36265	2.050	ppbv	94

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
 Data File : VL042350.D
 Acq On : 17 Apr 2025 10:17
 Operator : SY/MD
 Sample : VSTDICC002
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC002

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/18/2025
 Supervised By :Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 01:26:23 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Apr 18 01:24:29 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.600	75	45327m	2.096	ppbv	
47) 1,1,2-Trichloroethane	6.590	97	29879	2.049	ppbv	88
48) Dibromochloromethane	7.389	129	53069	2.061	ppbv	100
49) Bromoform	9.483	173	48069	2.135	ppbv	97
50) 4-Methyl-2-Pentanone	5.758	43	102182	2.180	ppbv	99
51) 2-Hexanone	7.441	43	100443	2.375	ppbv	98
52) Tetrachloroethene	8.228	164	27854	1.877	ppbv	96
53) Toluene	6.933	91	97493	2.116	ppbv	98
54) 1,2-Dibromoethane	7.655	107	43153	2.076	ppbv	87
56) 1,1,1,2-Tetrachloroethane	8.924	131	42601	2.097	ppbv	95
57) Chlorobenzene	8.924	112	71685	2.054	ppbv	98
58) Ethyl Benzene	9.357	91	138810	2.088	ppbv	98
59) m/p-Xylene	9.532	91	222542m	4.142	ppbv	
60) o-Xylene	9.963	91	111972	2.076	ppbv	98
61) Styrene	9.872	104	54229	2.106	ppbv	98
62) Isopropylbenzene	10.539	105	163716	2.067	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.963	83	64952	1.853	ppbv	99
64) n-propylbenzene	10.989	120	40956	2.058	ppbv	96
65) tert-Butylbenzene	11.532	119	155401	2.135	ppbv	92
66) Benzyl Chloride	11.616	91	17300	2.163	ppbv	98
67) sec-Butylbenzene	11.769	105	218327	2.156	ppbv	100
69) p-Isopropyltoluene	11.927	119	188657	2.145	ppbv	99
70) n-Butylbenzene	12.283	91	198221	2.164	ppbv	99
71) 2-Chlorotoluene	10.901	91	128858	2.075	ppbv	98
72) 4-Ethyltoluene	11.124	105	137872	2.091	ppbv	97
73) 1,3,5-Trimethylbenzene	11.205	105	123580	2.123	ppbv	98
74) 1,2,4-Trimethylbenzene	11.539	105	145510	2.140	ppbv	92
75) 1,3-Dichlorobenzene	11.607	146	75082	2.124	ppbv	98
76) 1,4-Dichlorobenzene	11.671	146	75323	2.120	ppbv	99
77) 1,2-Dichlorobenzene	11.947	146	74786	2.176	ppbv	98
78) Hexachloro-1,3-Butadiene	13.882	225	76158	2.194	ppbv	100
79) Naphthalene	13.513	128	195233	2.401	ppbv	99
80) Naphthalene,2-methyl-	14.458	142	119262	2.574	ppbv	99
81) 1,2,4-Trichlorobenzene	13.442	180	82156	2.353	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
 Data File : VL042351.D
 Acq On : 17 Apr 2025 10:48
 Operator : SY/MD
 Sample : VSTDICC001
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC001

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/18/2025
 Supervised By :Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 01:27:33 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2025

QLast Update : Fri Apr 18 01:24:29 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.791	49	124177	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.962	114	359907	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.885	117	329090	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.377 95 269087 9.950 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 99.500%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.499	85	22816	1.040	ppbv	93
3) Chlorodifluoromethane	1.476	51	20573	0.985	ppbv	97
4) Chloromethane	1.535	50	9008	1.038	ppbv	99
5) Vinyl Chloride	1.580	62	8807	0.932	ppbv	98
6) Bromomethane	1.671	94	4099	1.001	ppbv	91
7) Chloroethane	1.706	64	3559	1.041	ppbv	90
8) Dichlorotetrafluoroethane	1.554	85	19251	1.022	ppbv	100
9) Propene	1.486	41	9892	1.040	ppbv	92
10) Heptane	4.982	43	28507m	1.114	ppbv	
11) Trichlorofluoromethane	1.878	101	22428	1.075	ppbv	99
12) 1,1,2-Trichlorotrifluo...	2.140	101	17865	1.047	ppbv	98
13) Ethanol	1.722	45	1730m	2.225	ppbv	
14) Bromoethene	1.784	108	6766	1.052	ppbv #	89
15) Acetone	1.839	43	23537	1.158	ppbv	97
16) 1,3-Butadiene	1.609	39	10377m	1.087	ppbv	
17) tert-Butyl alcohol	2.043	59	26477	1.051	ppbv #	90
18) 1,1-Dichloroethene	2.036	96	7890	0.962	ppbv	94
19) Isopropyl Alcohol	1.888	45	12175	1.078	ppbv #	39
20) Methylene Chloride	2.062	84	9046	1.136	ppbv	87
21) Allyl Chloride	2.098	41	15057	1.073	ppbv	91
22) trans-1,2-Dichloroethene	2.344	96	9421	1.038	ppbv	96
23) Vinyl Acetate	2.467	43	9234	1.122	ppbv #	90
24) 1,1-Dichloroethane	2.409	63	18236	1.058	ppbv	99
25) Ethyl Acetate	2.842	43	51494	1.027	ppbv #	97
26) Hexane	2.826	57	21350	1.053	ppbv	95
27) Carbon Disulfide	2.153	76	20739	0.955	ppbv #	1
28) Methyl tert-Butyl Ether	2.444	73	14164	1.066	ppbv #	85
29) Chloroform	2.852	83	28973	1.011	ppbv	100
30) Cyclohexane	3.862	84	16547m	1.013	ppbv	
31) cis-1,2-Dichloroethene	2.723	61	19904	1.032	ppbv	97
32) 1,1,1-Trichloroethane	3.376	97	31653	1.030	ppbv	98
34) 2-Butanone	2.564	43	29735	1.045	ppbv	99
35) Carbon Tetrachloride	3.768	117	29875	0.917	ppbv	94
36) Benzene	3.661	78	38707	0.997	ppbv	95
37) 1,2-Dichloroethane	3.224	62	23284	0.999	ppbv	97
38) Trichloroethene	4.551	130	16119	0.947	ppbv	96
39) 1,2-Dichloropropane	4.318	63	14866	1.027	ppbv	96
40) 1,4-Dioxane	4.597	88	8737m	1.114	ppbv	
41) Tetrahydrofuran	3.062	42	17259	1.049	ppbv	96
42) Bromodichloromethane	4.490	83	32721	1.009	ppbv #	98
43) Methyl Methacrylate	4.885	69	18699m	1.073	ppbv	
44) 2,2,4-Trimethylpentane	4.642	57	68946m	1.027	ppbv	
45) t-1,3-Dichloropropene	6.416	75	18347m	1.026	ppbv	

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
 Data File : VL042351.D
 Acq On : 17 Apr 2025 10:48
 Operator : SY/MD
 Sample : VSTDICC001
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC001

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/18/2025
 Supervised By :Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 01:27:33 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Apr 18 01:24:29 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.603	75	22189m	1.015	ppbv	
47) 1,1,2-Trichloroethane	6.587	97	15457m	1.048	ppbv	
48) Dibromochloromethane	7.390	129	25948	0.997	ppbv	100
49) Bromoform	9.484	173	22413	0.984	ppbv	98
50) 4-Methyl-2-Pentanone	5.765	43	49725	1.049	ppbv	97
51) 2-Hexanone	7.445	43	47178	1.103	ppbv	99
52) Tetrachloroethene	8.228	164	14154	0.943	ppbv	93
53) Toluene	6.940	91	46611	1.001	ppbv	100
54) 1,2-Dibromoethane	7.658	107	21780	1.036	ppbv	93
56) 1,1,1,2-Tetrachloroethane	8.927	131	21052	1.057	ppbv	95
57) Chlorobenzene	8.921	112	35113	1.026	ppbv #	95
58) Ethyl Benzene	9.354	91	68703	1.054	ppbv	96
59) m/p-Xylene	9.552	91	110702m	2.101	ppbv	
60) o-Xylene	9.966	91	55831	1.056	ppbv	99
61) Styrene	9.872	104	25544	1.012	ppbv	100
62) Isopropylbenzene	10.542	105	81286	1.047	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.966	83	32410	0.943	ppbv	99
64) n-propylbenzene	10.989	120	19898	1.019	ppbv	90
65) tert-Butylbenzene	11.533	119	77598	1.087	ppbv	92
66) Benzyl Chloride	11.617	91	7864	1.003	ppbv #	91
67) sec-Butylbenzene	11.769	105	105919	1.067	ppbv	97
69) p-Isopropyltoluene	11.928	119	92733	1.075	ppbv	97
70) n-Butylbenzene	12.284	91	96306	1.072	ppbv	99
71) 2-Chlorotoluene	10.905	91	63321	1.040	ppbv	99
72) 4-Ethyltoluene	11.128	105	69698	1.078	ppbv	99
73) 1,3,5-Trimethylbenzene	11.206	105	60927	1.067	ppbv	99
74) 1,2,4-Trimethylbenzene	11.539	105	73888	1.108	ppbv	95
75) 1,3-Dichlorobenzene	11.610	146	36877	1.064	ppbv	98
76) 1,4-Dichlorobenzene	11.675	146	36692	1.053	ppbv	98
77) 1,2-Dichlorobenzene	11.950	146	35977	1.068	ppbv	97
78) Hexachloro-1,3-Butadiene	13.886	225	37377	1.098	ppbv	99
79) Naphthalene	13.517	128	90710	1.138	ppbv	99
80) Naphthalene,2-methyl-	14.462	142	50487	1.111	ppbv	98
81) 1,2,4-Trichlorobenzene	13.442	180	36764	1.074	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
Data File : VL042351.D
Acq On : 17 Apr 2025 10:48
Operator : SY/MD
Sample : VSTDIC001
Misc : 400mL/MSVOA_L
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDIC001

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/18/2025
Supervised By :Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 01:27:33 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Fri Apr 18 01:24:29 2025
Response via : Initial Calibration

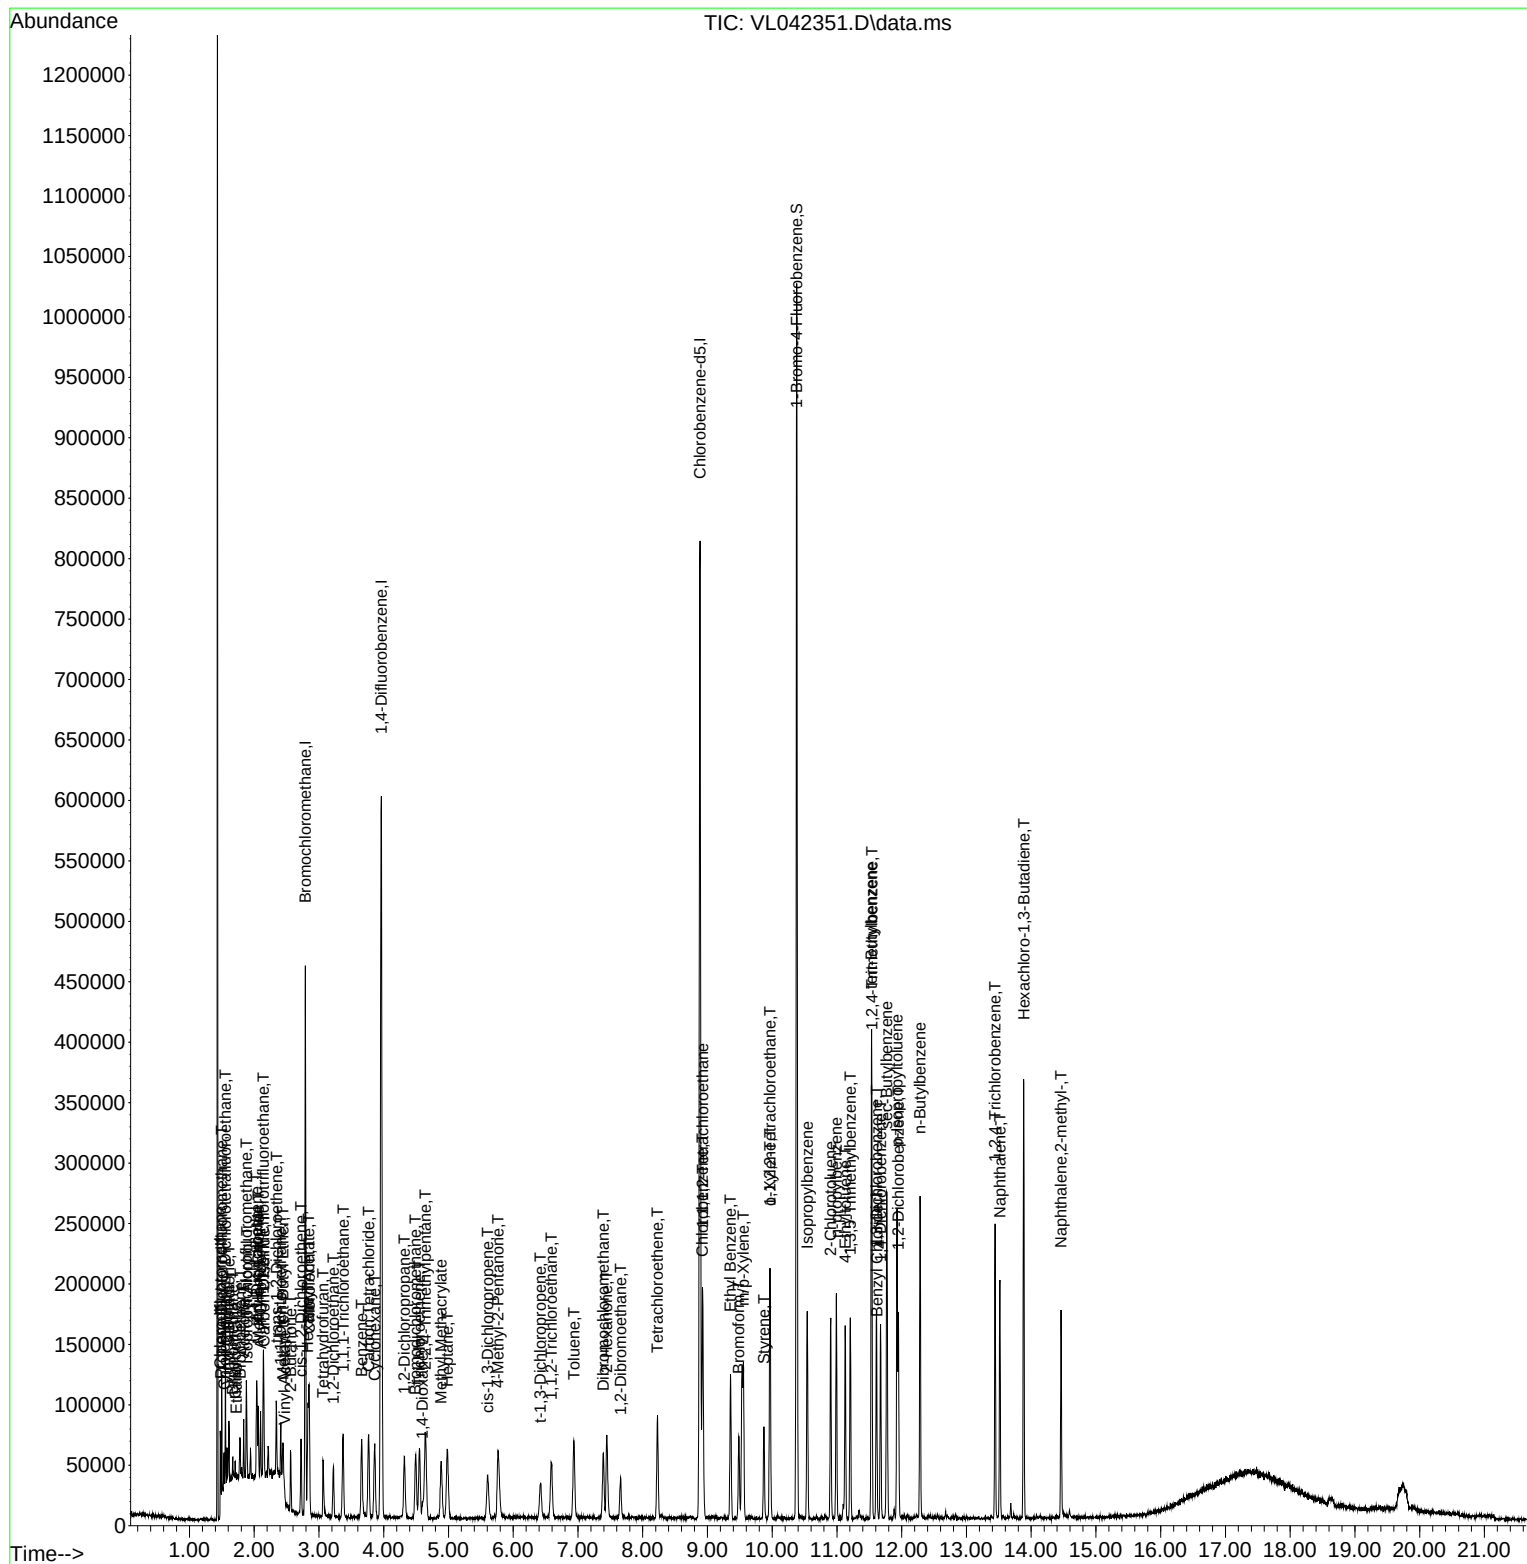

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
 Data File : VL042352.D
 Acq On : 17 Apr 2025 11:19
 Operator : SY/MD
 Sample : VSTDICC0.5
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.5

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/18/2025
 Supervised By : Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 01:28:45 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2025

QLast Update : Fri Apr 18 01:24:29 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	120542	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.952	114	353137	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.878	117	321644	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.374 95 265161 10.032 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 100.300%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.499	85	11036	0.518	ppbv	92
3) Chlorodifluoromethane	1.476	51	11304	0.557	ppbv #	84
4) Chloromethane	1.531	50	4534	0.538	ppbv	97
5) Vinyl Chloride	1.580	62	4406	0.480	ppbv	97
6) Bromomethane	1.667	94	2394	0.602	ppbv	95
7) Chloroethane	1.703	64	1824	0.550	ppbv #	87
8) Dichlorotetrafluoroethane	1.554	85	9381	0.513	ppbv	99
9) Propene	1.483	41	5303	0.574	ppbv	93
10) Heptane	4.978	43	14728m	0.593	ppbv	
11) Trichlorofluoromethane	1.877	101	10150	0.501	ppbv	97
12) 1,1,2-Trichlorotrifluo...	2.136	101	8371	0.506	ppbv	93
13) Ethanol	1.719	45	1656m	2.194	ppbv	
14) Bromoethene	1.780	108	3238	0.519	ppbv #	93
15) Acetone	1.835	43	11859	0.601	ppbv #	74
16) 1,3-Butadiene	1.609	39	6120	0.660	ppbv #	82
17) tert-Butyl alcohol	2.043	59	13640	0.558	ppbv #	85
18) 1,1-Dichloroethene	2.033	96	4430	0.556	ppbv #	87
19) Isopropyl Alcohol	1.884	45	6327	0.577	ppbv #	39
20) Methylene Chloride	2.059	84	5273	0.682	ppbv	93
21) Allyl Chloride	2.094	41	7692	0.565	ppbv #	81
22) trans-1,2-Dichloroethene	2.340	96	4908	0.557	ppbv	92
23) Vinyl Acetate	2.460	43	3953	0.495	ppbv #	57
24) 1,1-Dichloroethane	2.408	63	8753	0.523	ppbv #	94
25) Ethyl Acetate	2.835	43	26686	0.548	ppbv #	93
26) Hexane	2.823	57	11448	0.581	ppbv	91
27) Carbon Disulfide	2.149	76	11472	0.544	ppbv #	1
28) Methyl tert-Butyl Ether	2.441	73	6833	0.530	ppbv #	32
29) Chloroform	2.848	83	14815	0.532	ppbv	93
30) Cyclohexane	3.852	84	8572	0.541	ppbv	94
31) cis-1,2-Dichloroethene	2.722	61	9571	0.511	ppbv	96
32) 1,1,1-Trichloroethane	3.370	97	15413	0.516	ppbv	97
34) 2-Butanone	2.560	43	15640	0.560	ppbv	97
35) Carbon Tetrachloride	3.761	117	14683	0.459	ppbv	87
36) Benzene	3.651	78	20233	0.531	ppbv	97
37) 1,2-Dichloroethane	3.217	62	12194	0.533	ppbv #	95
38) Trichloroethene	4.551	130	7819	0.468	ppbv #	78
39) 1,2-Dichloropropane	4.308	63	7790m	0.548	ppbv	
40) 1,4-Dioxane	4.599	88	4637m	0.603	ppbv	
41) Tetrahydrofuran	3.062	42	9144m	0.567	ppbv	
42) Bromodichloromethane	4.489	83	16642	0.523	ppbv #	91
43) Methyl Methacrylate	4.881	69	9620m	0.563	ppbv	
44) 2,2,4-Trimethylpentane	4.635	57	34170	0.519	ppbv	91
45) t-1,3-Dichloropropene	6.415	75	9073m	0.517	ppbv	

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
 Data File : VL042352.D
 Acq On : 17 Apr 2025 11:19
 Operator : SY/MD
 Sample : VSTDICC0.5
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.5

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/18/2025
 Supervised By :Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 01:28:45 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Apr 18 01:24:29 2025


Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.596	75	10827m	0.505	ppbv	
47) 1,1,2-Trichloroethane	6.577	97	7466m	0.516	ppbv	
48) Dibromochloromethane	7.386	129	13122	0.514	ppbv	97
49) Bromoform	9.477	173	10988	0.492	ppbv	99
50) 4-Methyl-2-Pentanone	5.761	43	27206m	0.585	ppbv	
51) 2-Hexanone	7.441	43	23684	0.564	ppbv	98
52) Tetrachloroethene	8.221	164	7412	0.503	ppbv #	88
53) Toluene	6.927	91	24200	0.529	ppbv	97
54) 1,2-Dibromoethane	7.645	107	10282	0.499	ppbv	84
56) 1,1,1,2-Tetrachloroethane	8.930	131	9987	0.513	ppbv #	1
57) Chlorobenzene	8.917	112	18149m	0.543	ppbv	
58) Ethyl Benzene	9.351	91	32624	0.512	ppbv	97
59) m/p-Xylene	9.532	91	54197m	1.053	ppbv	
60) o-Xylene	9.963	91	27983	0.541	ppbv	99
61) Styrene	9.869	104	12736	0.516	ppbv	96
62) Isopropylbenzene	10.539	105	40481	0.533	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.959	83	15920	0.474	ppbv	99
64) n-propylbenzene	10.985	120	10369	0.544	ppbv	97
65) tert-Butylbenzene	11.529	119	37294	0.535	ppbv	93
66) Benzyl Chloride	11.613	91	3878	0.506	ppbv #	91
67) sec-Butylbenzene	11.765	105	52139	0.537	ppbv	97
69) p-Isopropyltoluene	11.924	119	45574	0.541	ppbv	98
70) n-Butylbenzene	12.280	91	48004	0.547	ppbv	99
71) 2-Chlorotoluene	10.898	91	31709	0.533	ppbv	100
72) 4-Ethyltoluene	11.125	105	33048	0.523	ppbv #	95
73) 1,3,5-Trimethylbenzene	11.202	105	30464	0.546	ppbv	99
74) 1,2,4-Trimethylbenzene	11.536	105	37765	0.579	ppbv #	90
75) 1,3-Dichlorobenzene	11.607	146	18003	0.531	ppbv	99
76) 1,4-Dichlorobenzene	11.668	146	18300	0.537	ppbv	96
77) 1,2-Dichlorobenzene	11.947	146	17446	0.530	ppbv	95
78) Hexachloro-1,3-Butadiene	13.879	225	18705	0.562	ppbv	98
79) Naphthalene	13.513	128	38521	0.494	ppbv #	92
80) Naphthalene,2-methyl-	14.458	142	21076	0.475	ppbv	96
81) 1,2,4-Trichlorobenzene	13.442	180	16504	0.493	ppbv	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual Integrations APPROVED

Quant Time: Apr 18 01:28:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug
QLast Update : Fri Apr 18 01:24:29 2025
Response via : Initial Calibration

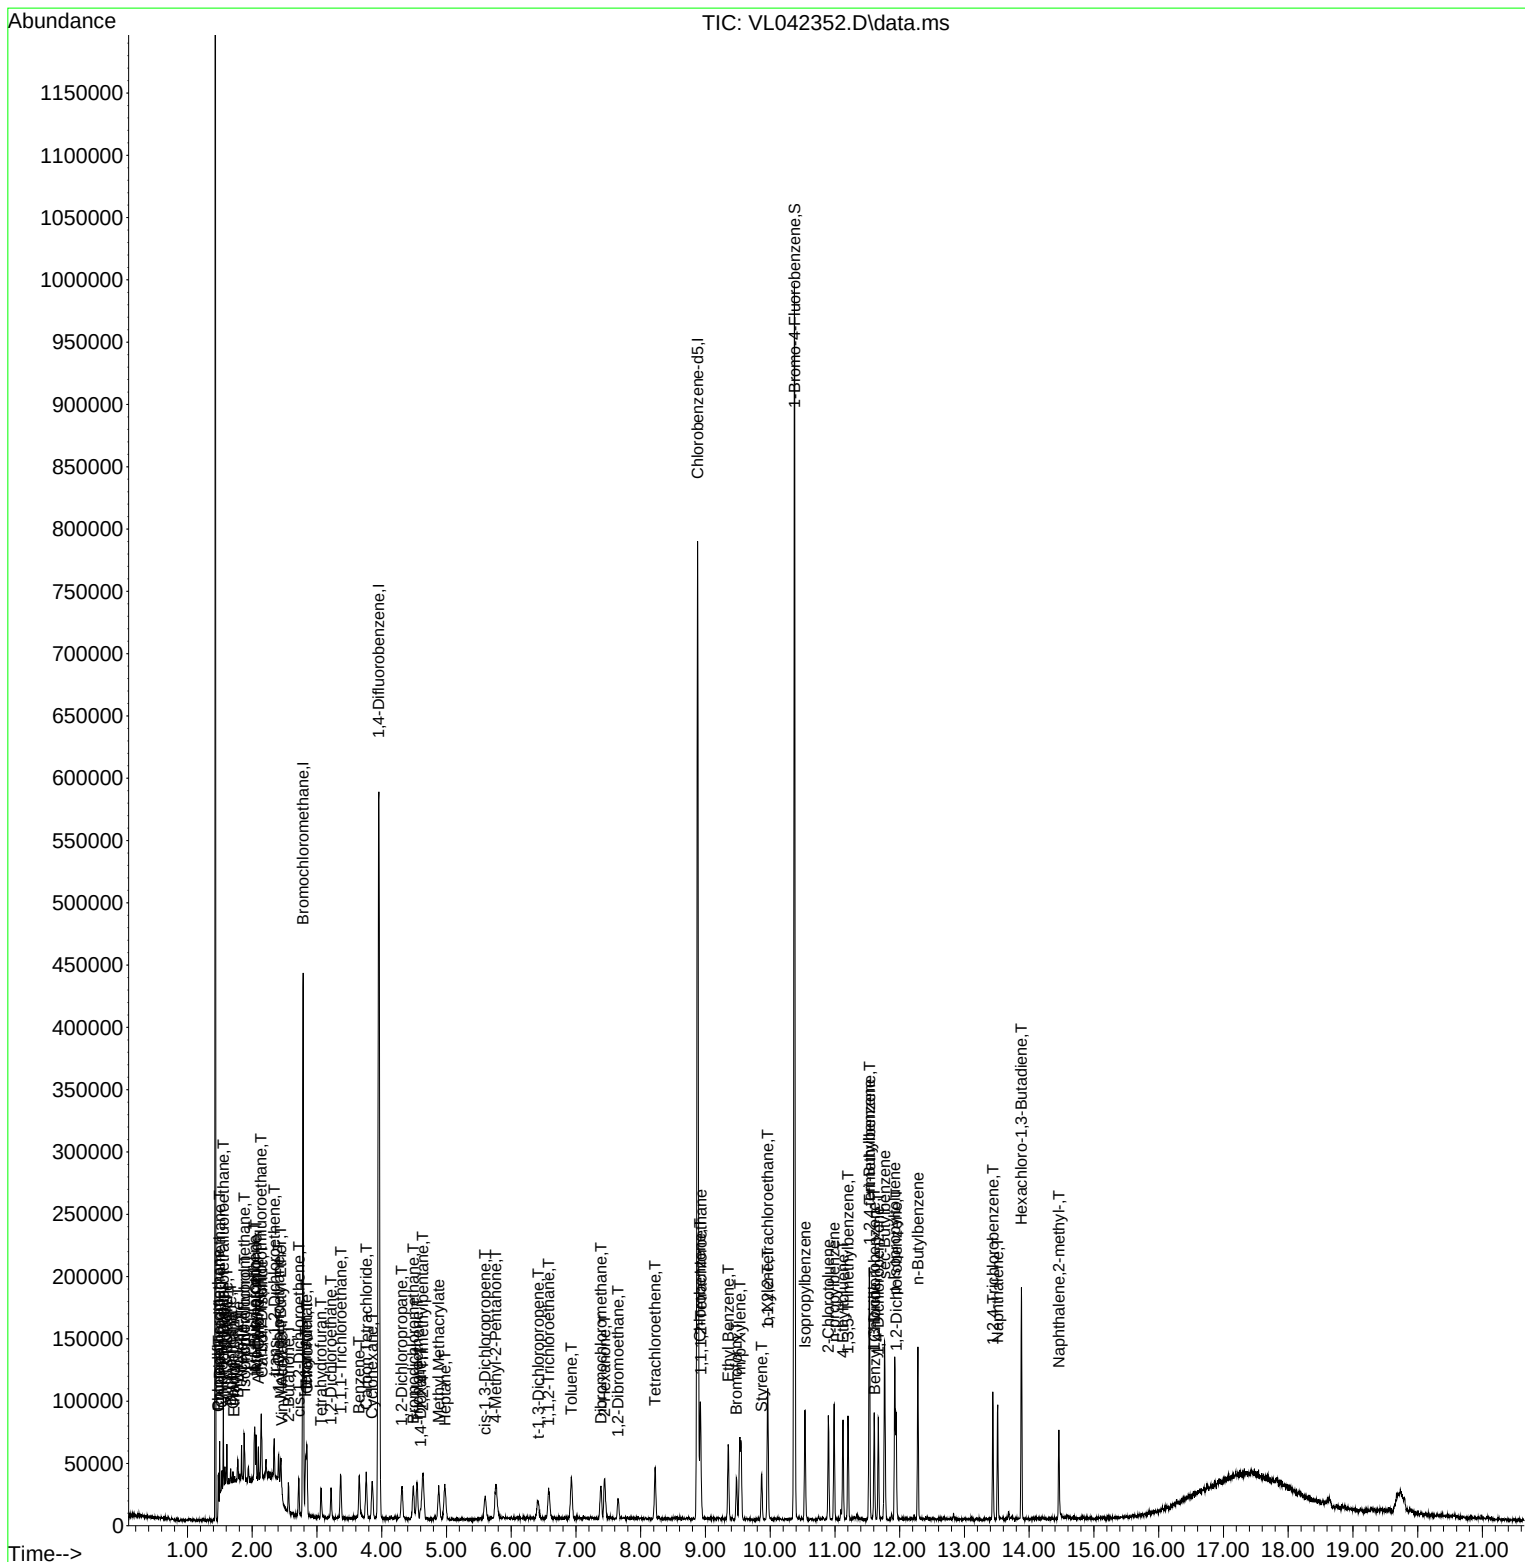

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
 Data File : VL042353.D
 Acq On : 17 Apr 2025 11:50
 Operator : SY/MD
 Sample : VSTDICC0.1
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/18/2025
 Supervised By :Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 01:29:39 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Fri Apr 18 01:24:29 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.791	49	119461	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.962	114	350484	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.885	117	315004	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.381	95	256417	9.906	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.100%
Target Compounds						
5) Vinyl Chloride	1.580	62	1088	0.120	ppbv #	74
32) 1,1,1-Trichloroethane	3.367	97	3393m	0.115	ppbv	
35) Carbon Tetrachloride	3.771	117	3204	0.101	ppbv #	94
38) Trichloroethene	4.551	130	1771m	0.107	ppbv	
52) Tetrachloroethene	8.222	164	1583m	0.108	ppbv	
54) 1,2-Dibromoethane	7.662	107	2177m	0.106	ppbv	
63) 1,1,2,2-Tetrachloroethane	9.966	83	3706m	0.113	ppbv	
79) Naphthalene	13.517	128	7664	0.100	ppbv #	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
Data File : VL042353.D
Acq On : 17 Apr 2025 11:50
Operator : SY/MD
Sample : VSTDICC0.1
Misc : 400mL/MSVOA_L
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC0.1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/18/2025
Supervised By :Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 01:29:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Fri Apr 18 01:24:29 2025
Response via : Initial Calibration

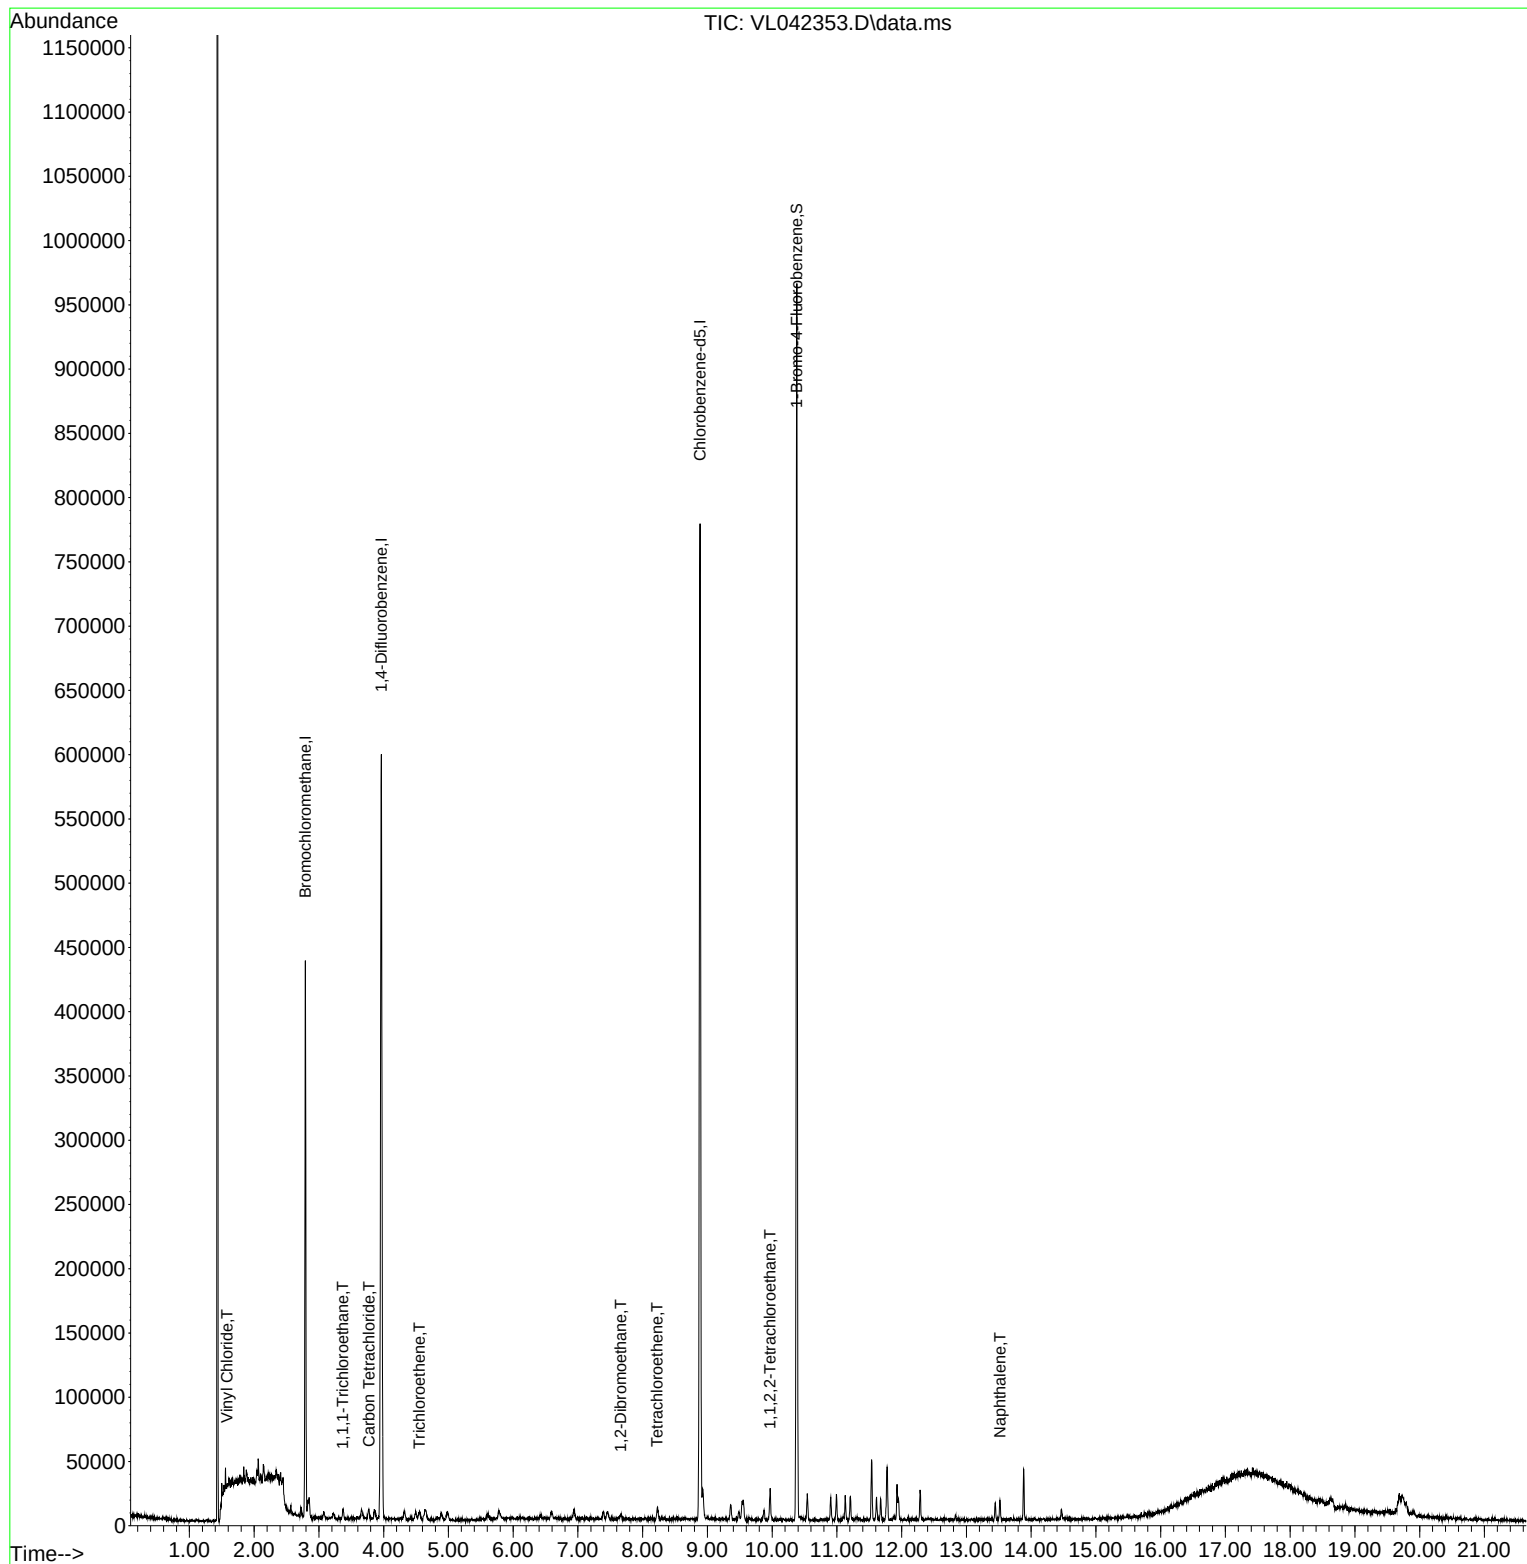

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
 Data File : VL042354.D
 Acq On : 17 Apr 2025 12:22
 Operator : SY/MD
 Sample : VSTDICC0.03
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.03

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/18/2025
 Supervised By :Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 02:07:48 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2025

QLast Update : Fri Apr 18 01:24:29 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.790	49	120042	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.965	114	349264	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.885	117	312999	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.380	95	256230	9.962	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.600%
Target Compounds						
5) Vinyl Chloride	1.583	62	361	0.040	ppbv	Qvalue # 76
32) 1,1,1-Trichloroethane	3.373	97	1120m	0.038	ppbv	
35) Carbon Tetrachloride	3.768	117	1382m	0.044	ppbv	
38) Trichloroethene	4.538	130	674m	0.041	ppbv	
52) Tetrachloroethene	8.228	164	569m	0.039	ppbv	
63) 1,1,2,2-Tetrachloroethane	9.972	83	1321m	0.040	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
Data File : VL042354.D
Acq On : 17 Apr 2025 12:22
Operator : SY/MD
Sample : VSTDICC0.03
Misc : 400mL/MSVOA_L
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC0.03

Quant Time: Apr 18 02:07:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Fri Apr 18 01:24:29 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 04/18/2025
Supervised By : Mahesh Dadoda 04/18/2025

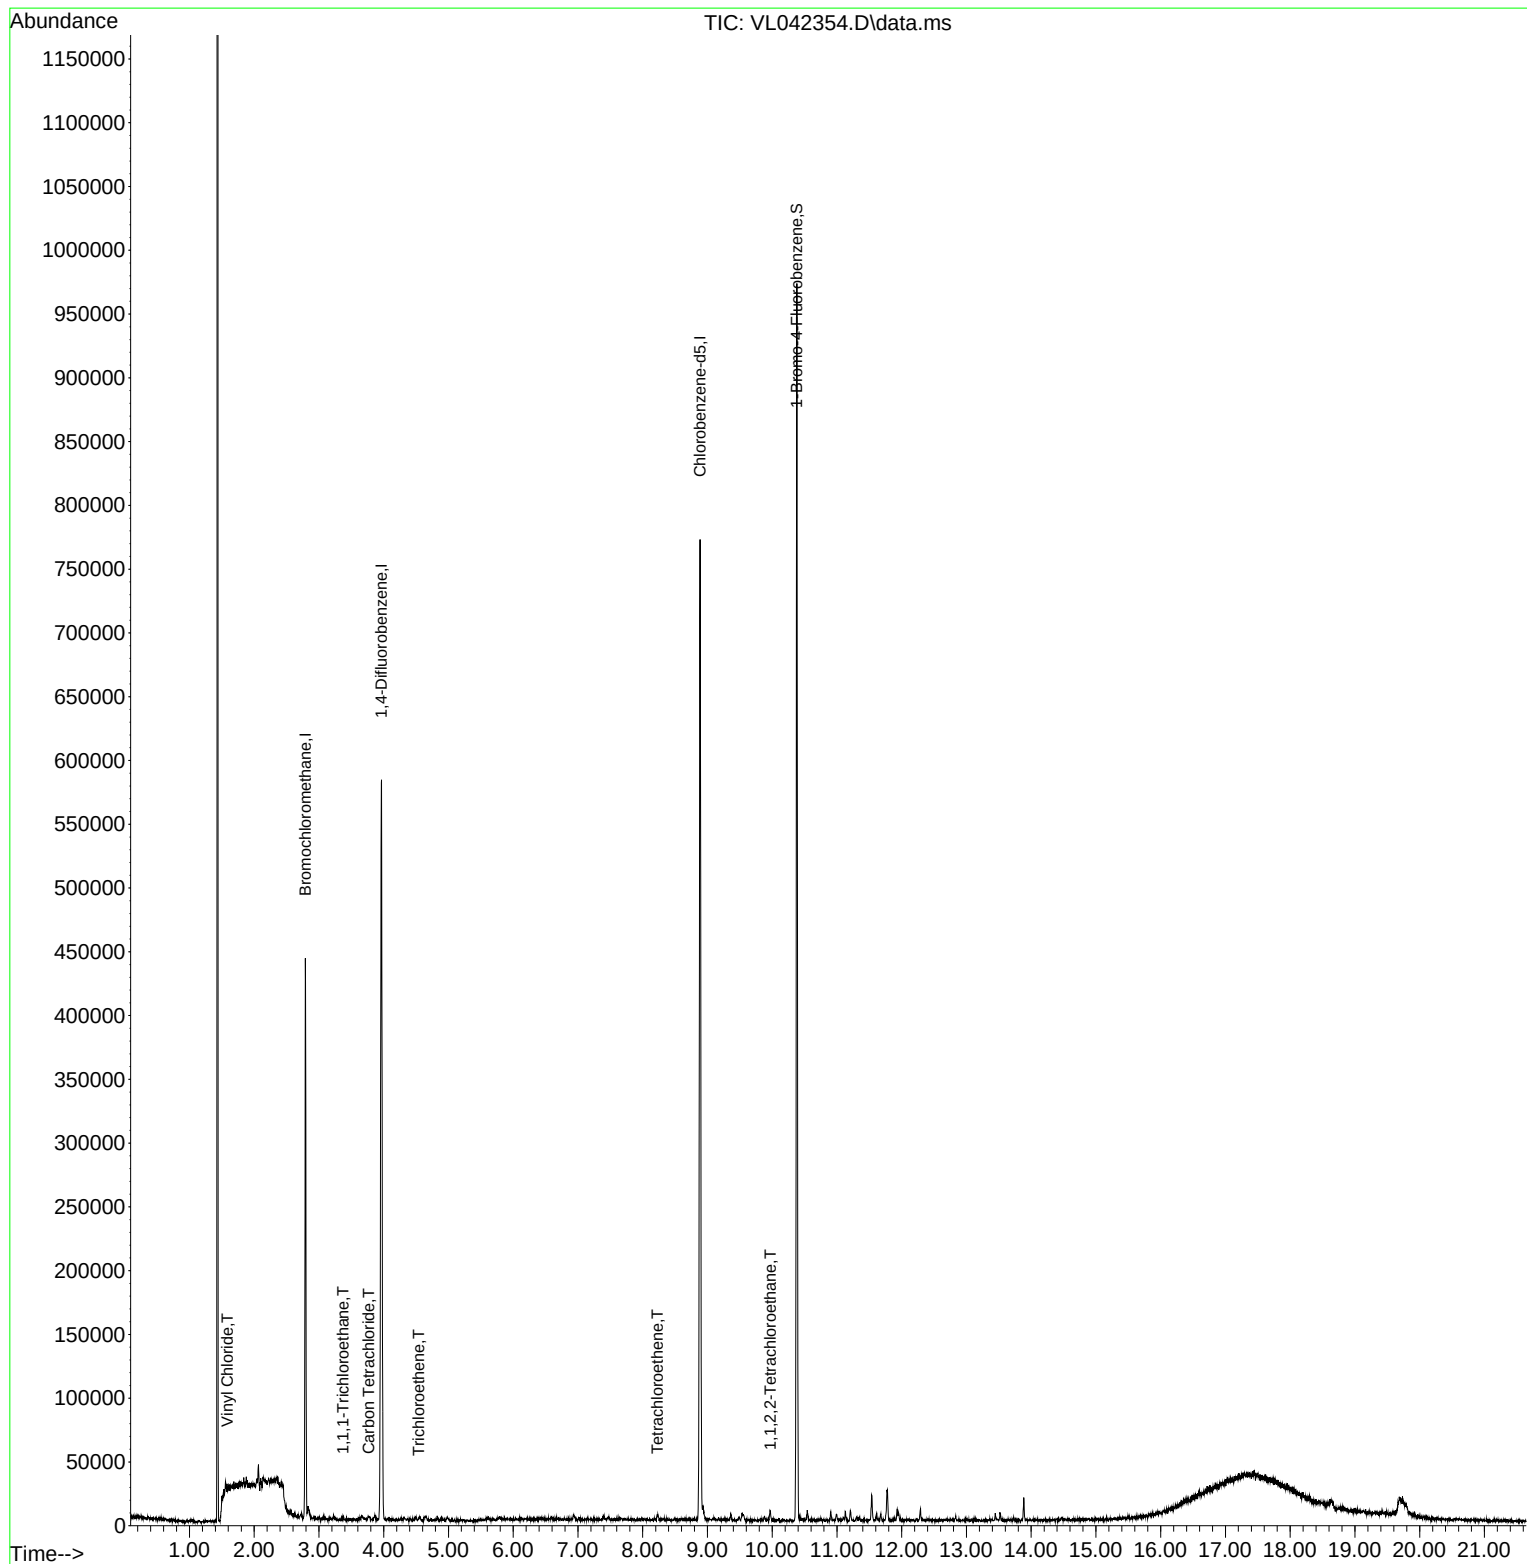

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
 Data File : VL042355.D
 Acq On : 17 Apr 2025 12:54
 Operator : SY/MD
 Sample : VSTDICC015
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC015

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/18/2025
 Supervised By :Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 01:31:10 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2025

QLast Update : Fri Apr 18 01:24:29 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.787	49	116071	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.959	114	332080	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.882	117	308463	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.374 95 254437 10.038 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 100.400%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.499	85	292784	14.277	ppbv	99
3) Chlorodifluoromethane	1.477	51	280042	14.341	ppbv	98
4) Chloromethane	1.532	50	115775	14.266	ppbv	99
5) Vinyl Chloride	1.580	62	112650	12.752	ppbv	100
6) Bromomethane	1.667	94	52805	13.800	ppbv	88
7) Chloroethane	1.703	64	44347	13.881	ppbv	98
8) Dichlorotetrafluoroethane	1.554	85	255029	14.484	ppbv	98
9) Propene	1.483	41	123102	13.842	ppbv	95
10) Heptane	4.979	43	336134	14.047	ppbv	100
11) Trichlorofluoromethane	1.875	101	278059	14.258	ppbv	99
12) 1,1,2-Trichlorotrifluo...	2.137	101	230366	14.447	ppbv	99
13) Ethanol	1.719	45	6324	8.702	ppbv	76
14) Bromoethene	1.781	108	84851	14.117	ppbv	99
15) Acetone	1.833	43	229086	12.056	ppbv	99
16) 1,3-Butadiene	1.609	39	117997	13.224	ppbv	96
17) tert-Butyl alcohol	2.040	59	320605	13.615	ppbv	99
18) 1,1-Dichloroethene	2.033	96	107666	14.045	ppbv	99
19) Isopropyl Alcohol	1.884	45	139004	13.169	ppbv	94
20) Methylene Chloride	2.059	84	91093	12.241	ppbv	90
21) Allyl Chloride	2.095	41	187995	14.329	ppbv	99
22) trans-1,2-Dichloroethene	2.341	96	118492	13.970	ppbv	94
23) Vinyl Acetate	2.460	43	106135	13.799	ppbv #	98
24) 1,1-Dichloroethane	2.409	63	235466	14.615	ppbv	99
25) Ethyl Acetate	2.836	43	663644	14.166	ppbv	100
26) Hexane	2.826	57	260975	13.765	ppbv	97
27) Carbon Disulfide	2.150	76	299098	14.734	ppbv	97
28) Methyl tert-Butyl Ether	2.438	73	174855	14.076	ppbv	95
29) Chloroform	2.849	83	385686	14.393	ppbv	99
30) Cyclohexane	3.855	84	217375	14.238	ppbv	98
31) cis-1,2-Dichloroethene	2.719	61	264972	14.700	ppbv	98
32) 1,1,1-Trichloroethane	3.367	97	412537	14.357	ppbv	99
34) 2-Butanone	2.558	43	367315	13.986	ppbv	100
35) Carbon Tetrachloride	3.762	117	409916	13.639	ppbv	94
36) Benzene	3.655	78	522156	14.578	ppbv	97
37) 1,2-Dichloroethane	3.218	62	319517	14.863	ppbv	100
38) Trichloroethene	4.548	130	208508	13.278	ppbv	98
39) 1,2-Dichloropropane	4.312	63	189697	14.201	ppbv	97
40) 1,4-Dioxane	4.580	88	92114	12.733	ppbv #	95
41) Tetrahydrofuran	3.053	42	214949	14.166	ppbv	98
42) Bromodichloromethane	4.490	83	442735	14.798	ppbv	95
43) Methyl Methacrylate	4.878	69	219757	13.670	ppbv	95
44) 2,2,4-Trimethylpentane	4.642	57	893529	14.425	ppbv	99
45) t-1,3-Dichloropropene	6.412	75	244470	14.810	ppbv	94

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041725\
 Data File : VL042355.D
 Acq On : 17 Apr 2025 12:54
 Operator : SY/MD
 Sample : VSTDIC015
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDIC015

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/18/2025
 Supervised By : Mahesh Dadoda 04/18/2025

Quant Time: Apr 18 01:31:10 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Apr 18 01:24:29 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.600	75	300145	14.878	ppbv	90
47) 1,1,2-Trichloroethane	6.581	97	198874	14.615	ppbv	98
48) Dibromochloromethane	7.390	129	362887	15.105	ppbv	98
49) Bromoform	9.484	173	312282	14.865	ppbv	99
50) 4-Methyl-2-Pentanone	5.749	43	563658	12.889	ppbv	99
51) 2-Hexanone	7.435	43	467001	11.834	ppbv #	98
52) Tetrachloroethene	8.225	164	180631	13.046	ppbv	97
53) Toluene	6.933	91	619420	14.411	ppbv	99
54) 1,2-Dibromoethane	7.652	107	280071	14.442	ppbv	92
56) 1,1,1,2-Tetrachloroethane	8.927	131	268626	14.389	ppbv	97
57) Chlorobenzene	8.921	112	454017	14.151	ppbv	97
58) Ethyl Benzene	9.354	91	874424	14.308	ppbv	100
59) m/p-Xylene	9.552	91	1388086m	28.109	ppbv	
60) o-Xylene	9.963	91	689246	13.902	ppbv	99
61) Styrene	9.872	104	339508	14.347	ppbv	99
62) Isopropylbenzene	10.539	105	1018968	13.999	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.963	83	412898	12.816	ppbv	100
64) n-propylbenzene	10.989	120	260812	14.255	ppbv	94
65) tert-Butylbenzene	11.533	119	899720	13.449	ppbv	93
66) Benzyl Chloride	11.617	91	96016	13.061	ppbv	96
67) sec-Butylbenzene	11.769	105	1253263	13.468	ppbv	100
69) p-Isopropyltoluene	11.928	119	1081850	13.382	ppbv	99
70) n-Butylbenzene	12.284	91	1117042	13.266	ppbv	100
71) 2-Chlorotoluene	10.902	91	806728	14.131	ppbv	100
72) 4-Ethyltoluene	11.125	105	848077	13.992	ppbv	99
73) 1,3,5-Trimethylbenzene	11.206	105	726558	13.578	ppbv	99
74) 1,2,4-Trimethylbenzene	11.539	105	785772	12.572	ppbv	97
75) 1,3-Dichlorobenzene	11.610	146	444086	13.670	ppbv	99
76) 1,4-Dichlorobenzene	11.672	146	450662	13.802	ppbv	98
77) 1,2-Dichlorobenzene	11.947	146	427372	13.529	ppbv	99
78) Hexachloro-1,3-Butadiene	13.883	225	404441	12.679	ppbv	100
79) Naphthalene	13.514	128	944085	12.632	ppbv	98
80) Naphthalene,2-methyl-	14.459	142	540339	12.686	ppbv	99
81) 1,2,4-Trichlorobenzene	13.442	180	429982	13.398	ppbv	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual Integrations APPROVED

Quant Time: Apr 18 01:31:10 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug
QLast Update : Fri Apr 18 01:24:29 2025
Response via : Initial Calibration





Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042125\
Data File : VL042394.D
Acq On : 21 Apr 2025 07:58
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Apr 18 02:14:00 2025

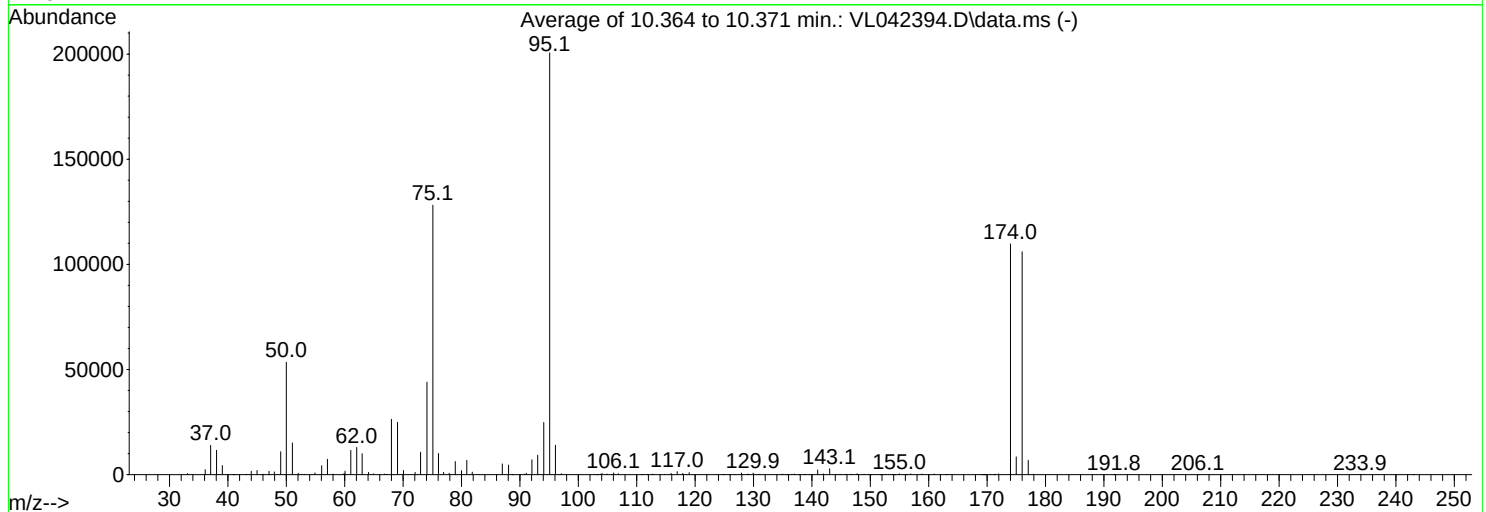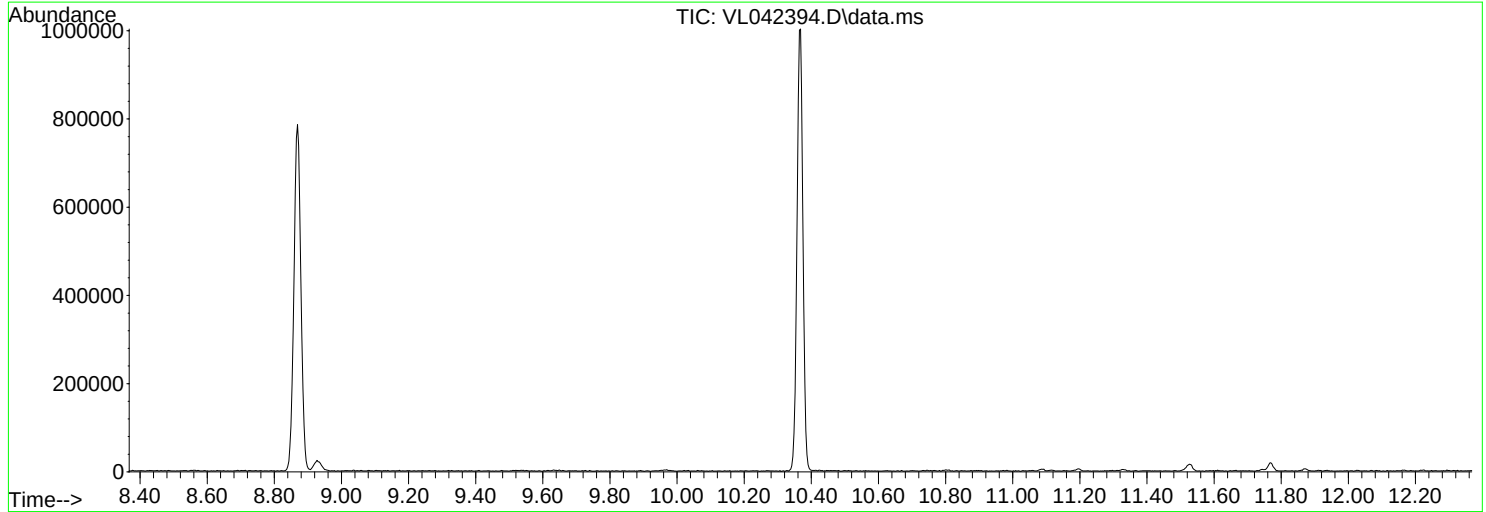

AutoFind: Scans 3175, 3176, 3177; Background Corrected with Scan 3159

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	26.7	53502	PASS
75	95	30	66	63.9	128181	PASS
95	95	100	100	100.0	200597	PASS
96	95	5	9	7.0	13990	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	54.7	109757	PASS
175	174	4	9	7.7	8464	PASS
176	174	93	101	96.6	106032	PASS
177	176	5	9	6.4	6826	PASS

Average of 10.364 to 10.371 min.: VL042394.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	518	45.00	2010	54.90	832	66.85	304
36.10	2394	45.85	194	56.05	4237	67.20	161
37.05	13953	46.10	197	57.05	7329	68.00	2631
38.05	11556	47.05	1570	58.00	328	69.05	2485
39.05	4320	47.95	1283	59.90	593	70.05	2000
39.90	57	49.05	10899	60.05	1702	72.05	1049
40.90	31	50.00	53502	61.05	11547	73.00	10643
41.30	48	51.05	15046	62.05	12934	74.10	44016
43.00	64	52.05	608	63.00	9941	75.10	128181
43.20	184	52.70	76	64.10	1108	76.05	10068
44.00	1632	53.15	138	64.90	355	76.95	1033

Average of 10.364 to 10.371 min.: VL042394.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.90	700	91.10	697	104.05	598	114.80	178
78.95	6226	92.05	7067	104.95	278	115.90	632
80.00	1878	93.05	9194	105.70	188	116.95	1450
80.90	6765	94.10	24813	106.05	831	117.90	579
81.85	1186	95.10	200597	106.85	467	119.00	1019
83.00	184	96.10	13990	109.95	82	121.90	17
86.05	106	96.90	128	110.85	113	124.00	56
87.00	5101	97.15	433	111.10	91	124.80	25
88.05	4600	102.75	176	111.85	167	125.90	42
88.70	40	103.20	26	112.75	225	126.85	64
90.80	235	103.80	263	113.00	54	127.95	770

Average of 10.364 to 10.371 min.: VL042394.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
128.80	183	137.80	21	145.00	70	152.60	135
129.10	275	138.70	105	145.70	127	153.10	56
129.95	780	138.90	54	145.85	120	153.80	154
130.85	125	139.55	52	146.75	211	154.20	31
131.00	55	140.05	163	147.75	498	154.80	81
131.20	65	141.00	2199	148.80	55	155.00	397
134.80	172	141.95	402	149.05	129	155.70	99
135.05	261	143.05	2809	149.65	112	156.20	25
135.70	20	144.00	151	150.10	20	156.95	371
136.60	73	144.20	61	151.70	27	158.85	322
137.00	333	144.80	162	152.00	33	160.90	347

Average of 10.364 to 10.371 min.: VL042394.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
163.00	37	176.00	106032				
169.00	59	177.05	6826				
169.20	38	177.90	242				
169.50	29	191.75	41				
169.70	25	206.10	24				
170.65	116	233.90	67				
171.20	28	243.00	24				
171.45	164						
171.95	381						
174.00	109757						
175.00	8464						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042125\
 Data File : VL042395.D
 Acq On : 21 Apr 2025 08:41
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/22/2025
 Supervised By : Mahesh Dadoda 04/22/2025

Quant Time: Apr 22 02:50:13 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Apr 18 02:14:00 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.784	49	118349	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.952	114	334726	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.875	117	297161	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.370 95 262155 10.736 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 107.400%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.496	85	214405	10.253	ppbv	95
3) Chlorodifluoromethane	1.473	51	172276	8.652	ppbv	96
4) Chloromethane	1.531	50	78242	9.455	ppbv	99
5) Vinyl Chloride	1.576	62	78692	8.736	ppbv	98
6) Bromomethane	1.664	94	36698	9.484	ppbv	92
7) Chloroethane	1.703	64	31945	9.806	ppbv	98
8) Dichlorotetrafluoroethane	1.551	85	182317	10.155	ppbv	94
9) Propene	1.483	41	67297	7.422	ppbv	98
10) Heptane	4.972	43	178981	7.026	ppbv	98
11) Trichlorofluoromethane	1.874	101	205368	10.328	ppbv	98
12) 1,1,2-Trichlorotrifluo...	2.136	101	154701	9.515	ppbv	99
13) Ethanol	1.719	45	4511	3.130	ppbv	88
14) Bromoethene	1.780	108	59325	9.680	ppbv	98
15) Acetone	1.832	43	168061	8.675	ppbv	99
16) 1,3-Butadiene	1.606	39	81189	8.762	ppbv	96
17) tert-Butyl alcohol	2.036	59	221320	9.218	ppbv	100
18) 1,1-Dichloroethene	2.030	96	70214	9.244	ppbv	97
19) Isopropyl Alcohol	1.884	45	98218	9.126	ppbv	94
20) Methylene Chloride	2.059	84	60052	7.915	ppbv	92
21) Allyl Chloride	2.091	41	121139	9.056	ppbv	97
22) trans-1,2-Dichloroethene	2.337	96	79496	9.192	ppbv	92
23) Vinyl Acetate	2.457	43	57298	7.306	ppbv	97
24) 1,1-Dichloroethane	2.405	63	154500	9.405	ppbv	100
25) Ethyl Acetate	2.832	43	392210	8.211	ppbv	99
26) Hexane	2.823	57	150573	7.789	ppbv	98
27) Carbon Disulfide	2.146	76	199908	9.658	ppbv	98
28) Methyl tert-Butyl Ether	2.437	73	106569	8.414	ppbv	95
29) Chloroform	2.845	83	259635	9.502	ppbv	98
30) Cyclohexane	3.852	84	126496	8.095	ppbv	97
31) cis-1,2-Dichloroethene	2.716	61	166357	9.051	ppbv	98
32) 1,1,1-Trichloroethane	3.363	97	285590	9.284	ppbv	99
34) 2-Butanone	2.554	43	220144	8.316	ppbv	99
35) Carbon Tetrachloride	3.755	117	291229	9.614	ppbv	91
36) Benzene	3.651	78	303987	8.420	ppbv	97
37) 1,2-Dichloroethane	3.214	62	221151	10.206	ppbv	97
38) Trichloroethene	4.541	130	123150	7.804	ppbv	94
39) 1,2-Dichloropropane	4.305	63	107877	8.018	ppbv #	88
40) 1,4-Dioxane	4.574	88	53874	7.286	ppbv #	94
41) Tetrahydrofuran	3.049	42	118863	7.701	ppbv	99
42) Bromodichloromethane	4.483	83	295552	9.800	ppbv	98
43) Methyl Methacrylate	4.875	69	124747	7.667	ppbv	95
44) 2,2,4-Trimethylpentane	4.629	57	507437	8.138	ppbv	95
45) t-1,3-Dichloropropene	6.406	75	142879	8.596	ppbv	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042125\
 Data File : VL042395.D
 Acq On : 21 Apr 2025 08:41
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/22/2025
 Supervised By :Mahesh Dadoda 04/22/2025

Quant Time: Apr 22 02:50:13 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Apr 18 02:14:00 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.590	75	174844	8.595	ppbv	88
47) 1,1,2-Trichloroethane	6.571	97	119399	8.711	ppbv	92
48) Dibromochloromethane	7.380	129	229466	9.476	ppbv	99
49) Bromoform	9.480	173	187094	8.836	ppbv	99
50) 4-Methyl-2-Pentanone	5.742	43	321752	7.314	ppbv	99
51) 2-Hexanone	7.425	43	260009	6.590	ppbv #	95
52) Tetrachloroethene	8.218	164	104294	7.474	ppbv	90
53) Toluene	6.923	91	355540	8.206	ppbv	99
54) 1,2-Dibromoethane	7.642	107	169774	8.654	ppbv	91
56) 1,1,1,2-Tetrachloroethane	8.917	131	170285	9.468	ppbv	96
57) Chlorobenzene	8.917	112	276428	8.944	ppbv	98
58) Ethyl Benzene	9.348	91	517937	8.797	ppbv	100
59) m/p-Xylene	9.545	91	847455m	17.868	ppbv	
60) o-Xylene	9.959	91	433569	9.078	ppbv	96
61) Styrene	9.866	104	192729	8.454	ppbv	96
62) Isopropylbenzene	10.535	105	625514	8.920	ppbv	98
63) 1,1,2,2-Tetrachloroethane	9.956	83	250238	8.085	ppbv	100
64) n-propylbenzene	10.985	120	154114	8.744	ppbv	97
65) tert-Butylbenzene	11.526	119	570548	8.853	ppbv	96
66) Benzyl Chloride	11.610	91	57090	8.061	ppbv	99
67) sec-Butylbenzene	11.765	105	797738	8.899	ppbv	99
69) p-Isopropyltoluene	11.921	119	684482	8.789	ppbv	97
70) n-Butylbenzene	12.277	91	720062	8.877	ppbv	97
71) 2-Chlorotoluene	10.898	91	493192	8.967	ppbv	97
72) 4-Ethyltoluene	11.121	105	521390	8.929	ppbv	97
73) 1,3,5-Trimethylbenzene	11.199	105	451158	8.752	ppbv	96
74) 1,2,4-Trimethylbenzene	11.532	105	502117	8.340	ppbv #	87
75) 1,3-Dichlorobenzene	11.604	146	264024	8.436	ppbv	97
76) 1,4-Dichlorobenzene	11.668	146	265655	8.445	ppbv	98
77) 1,2-Dichlorobenzene	11.943	146	260133	8.548	ppbv	97
78) Hexachloro-1,3-Butadiene	13.879	225	245910	8.002	ppbv	99
79) Naphthalene	13.510	128	570593	7.925	ppbv	100
80) Naphthalene,2-methyl-	14.455	142	304139	7.412	ppbv	96
81) 1,2,4-Trichlorobenzene	13.439	180	250801	8.112	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual Integrations

Quant Time: Apr 22 02:50:13 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug
QLast Update : Fri Apr 18 02:14:00 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042125\
 Data File : VL042397.D
 Acq On : 21 Apr 2025 10:14
 Operator : SY/MD
 Sample : VL0421ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0421ABS01

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/22/2025
 Supervised By : Mahesh Dadoda 04/22/2025

Quant Time: Apr 22 02:51:20 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Apr 18 02:14:00 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.781	49	118401	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.949	114	337921	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.875	117	293537	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.371 95 260048 10.781 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 107.800%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.496	85	212503	10.158	ppbv	98
3) Chlorodifluoromethane	1.473	51	175535	8.812	ppbv	95
4) Chloromethane	1.531	50	79791	9.638	ppbv	94
5) Vinyl Chloride	1.577	62	77905	8.645	ppbv	97
6) Bromomethane	1.664	94	35087	9.064	ppbv	87
7) Chloroethane	1.700	64	30814	9.455	ppbv	96
8) Dichlorotetrafluoroethane	1.551	85	182258	10.147	ppbv	94
9) Propene	1.480	41	69080	7.615	ppbv	97
10) Heptane	4.969	43	187072	7.340	ppbv	99
11) Trichlorofluoromethane	1.875	101	205641	10.337	ppbv	100
12) 1,1,2-Trichlorotrifluo...	2.133	101	156363	9.613	ppbv	98
13) Ethanol	1.716	45	4602	3.192	ppbv	92
14) Bromoethene	1.777	108	58938	9.613	ppbv	98
15) Acetone	1.832	43	168065	8.671	ppbv	98
16) 1,3-Butadiene	1.606	39	83577	9.015	ppbv	92
17) tert-Butyl alcohol	2.036	59	216440	9.011	ppbv	100
18) 1,1-Dichloroethene	2.030	96	71097	9.356	ppbv	95
19) Isopropyl Alcohol	1.881	45	96437	8.956	ppbv	93
20) Methylene Chloride	2.056	84	60417	7.959	ppbv	89
21) Allyl Chloride	2.091	41	122313	9.140	ppbv	97
22) trans-1,2-Dichloroethene	2.334	96	78976	9.128	ppbv	98
23) Vinyl Acetate	2.457	43	54610	6.961	ppbv #	96
24) 1,1-Dichloroethane	2.402	63	157093	9.559	ppbv	99
25) Ethyl Acetate	2.829	43	393203	8.228	ppbv	99
26) Hexane	2.820	57	151103	7.813	ppbv	99
27) Carbon Disulfide	2.146	76	194719	9.404	ppbv	98
28) Methyl tert-Butyl Ether	2.434	73	108007	8.524	ppbv	93
29) Chloroform	2.842	83	262639	9.608	ppbv	98
30) Cyclohexane	3.846	84	133153	8.517	ppbv	98
31) cis-1,2-Dichloroethene	2.713	61	166447	9.052	ppbv	95
32) 1,1,1-Trichloroethane	3.360	97	285156	9.266	ppbv	98
34) 2-Butanone	2.554	43	220966	8.268	ppbv	98
35) Carbon Tetrachloride	3.755	117	291941	9.546	ppbv	95
36) Benzene	3.648	78	312290	8.568	ppbv	97
37) 1,2-Dichloroethane	3.211	62	225346	10.301	ppbv #	96
38) Trichloroethene	4.542	130	123977	7.783	ppbv	98
39) 1,2-Dichloropropane	4.305	63	112058	8.250	ppbv #	90
40) 1,4-Dioxane	4.571	88	55511	7.437	ppbv #	93
41) Tetrahydrofuran	3.046	42	121497	7.797	ppbv	99
42) Bromodichloromethane	4.480	83	294127	9.661	ppbv	98
43) Methyl Methacrylate	4.872	69	125779	7.657	ppbv	93
44) 2,2,4-Trimethylpentane	4.629	57	508984	8.085	ppbv	95
45) t-1,3-Dichloropropene	6.399	75	142114	8.469	ppbv	93

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042125\
 Data File : VL042397.D
 Acq On : 21 Apr 2025 10:14
 Operator : SY/MD
 Sample : VL0421ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0421ABS01

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/22/2025
 Supervised By :Mahesh Dadoda 04/22/2025

Quant Time: Apr 22 02:51:20 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Fri Apr 18 02:14:00 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.590	75	171445	8.348	ppbv #	84
47) 1,1,2-Trichloroethane	6.574	97	124092	8.967	ppbv	95
48) Dibromochloromethane	7.377	129	225553	9.226	ppbv	99
49) Bromoform	9.474	173	188764	8.830	ppbv	100
50) 4-Methyl-2-Pentanone	5.739	43	318982	7.182	ppbv	99
51) 2-Hexanone	7.429	43	266951	6.702	ppbv #	95
52) Tetrachloroethene	8.222	164	104899	7.446	ppbv	97
53) Toluene	6.920	91	361443	8.264	ppbv	99
54) 1,2-Dibromoethane	7.645	107	175799	8.877	ppbv	94
56) 1,1,1,2-Tetrachloroethane	8.917	131	169656	9.550	ppbv	97
57) Chlorobenzene	8.914	112	270733	8.868	ppbv	98
58) Ethyl Benzene	9.348	91	524070	9.011	ppbv	100
59) m/p-Xylene	9.545	91	852193m	18.189	ppbv	
60) o-Xylene	9.956	91	433062	9.179	ppbv	97
61) Styrene	9.866	104	194756	8.648	ppbv	98
62) Isopropylbenzene	10.533	105	641535	9.262	ppbv	97
63) 1,1,2,2-Tetrachloroethane	9.956	83	257428	8.420	ppbv	99
64) n-propylbenzene	10.982	120	155343	8.922	ppbv	96
65) tert-Butylbenzene	11.526	119	573929	9.015	ppbv	96
66) Benzyl Chloride	11.610	91	51025	7.294	ppbv	97
67) sec-Butylbenzene	11.762	105	802355	9.061	ppbv	99
69) p-Isopropyltoluene	11.921	119	685449	8.910	ppbv	97
70) n-Butylbenzene	12.277	91	723138	9.025	ppbv	98
71) 2-Chlorotoluene	10.895	91	500409	9.211	ppbv	97
72) 4-Ethyltoluene	11.122	105	519236	9.002	ppbv	98
73) 1,3,5-Trimethylbenzene	11.199	105	456404	8.963	ppbv	96
74) 1,2,4-Trimethylbenzene	11.533	105	509154	8.561	ppbv	91
75) 1,3-Dichlorobenzene	11.604	146	267483	8.652	ppbv	98
76) 1,4-Dichlorobenzene	11.669	146	267283	8.602	ppbv	98
77) 1,2-Dichlorobenzene	11.944	146	261316	8.693	ppbv	97
78) Hexachloro-1,3-Butadiene	13.879	225	259140	8.537	ppbv	99
79) Naphthalene	13.510	128	584987	8.225	ppbv	99
80) Naphthalene,2-methyl-	14.455	142	300148	7.405	ppbv	96
81) 1,2,4-Trichlorobenzene	13.436	180	258107	8.452	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042125\
 Data File : VL042399.D
 Acq On : 21 Apr 2025 11:36
 Operator : SY/MD
 Sample : QC041625 CAN 10329
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC041625 CAN 10329

Quant Time: Apr 22 02:52:23 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Fri Apr 18 02:14:00 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.781	49	116817	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.949	114	332871	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.875	117	284301	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	10.371	95	248070	10.618	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	106.200%

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042125\
Data File : VL042399.D
Acq On : 21 Apr 2025 11:36
Operator : SY/MD
Sample : QC041625 CAN 10329
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC041625 CAN 10329

Quant Time: Apr 22 02:52:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Fri Apr 18 02:14:00 2025
Response via : Initial Calibration

