

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051525\
 Data File : VX046213.D
 Acq On : 15 May 2025 14:58
 Operator : JC/MD
 Sample : Q2050-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-182-GW-205-207

Quant Time: May 16 01:06:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 06 07:12:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	60533	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	121144	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	113426	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	47407	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	62575	55.448	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	110.900%
35) Dibromofluoromethane	5.379	113	45370	52.008	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.020%
50) Toluene-d8	8.647	98	155555	51.519	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	103.040%
62) 4-Bromofluorobenzene	11.079	95	57300	49.474	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	98.940%
Target Compounds						
16) Acetone	2.380	43	2332	5.154	ug/l	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX051525\
Data File : VX046213.D
Acq On : 15 May 2025 14:58
Operator : JC/MD
Sample : Q2050-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-182-GW-205-207

Quant Time: May 16 01:06:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260
QLast Update : Tue May 06 07:12:22 2025
Response via : Initial Calibration




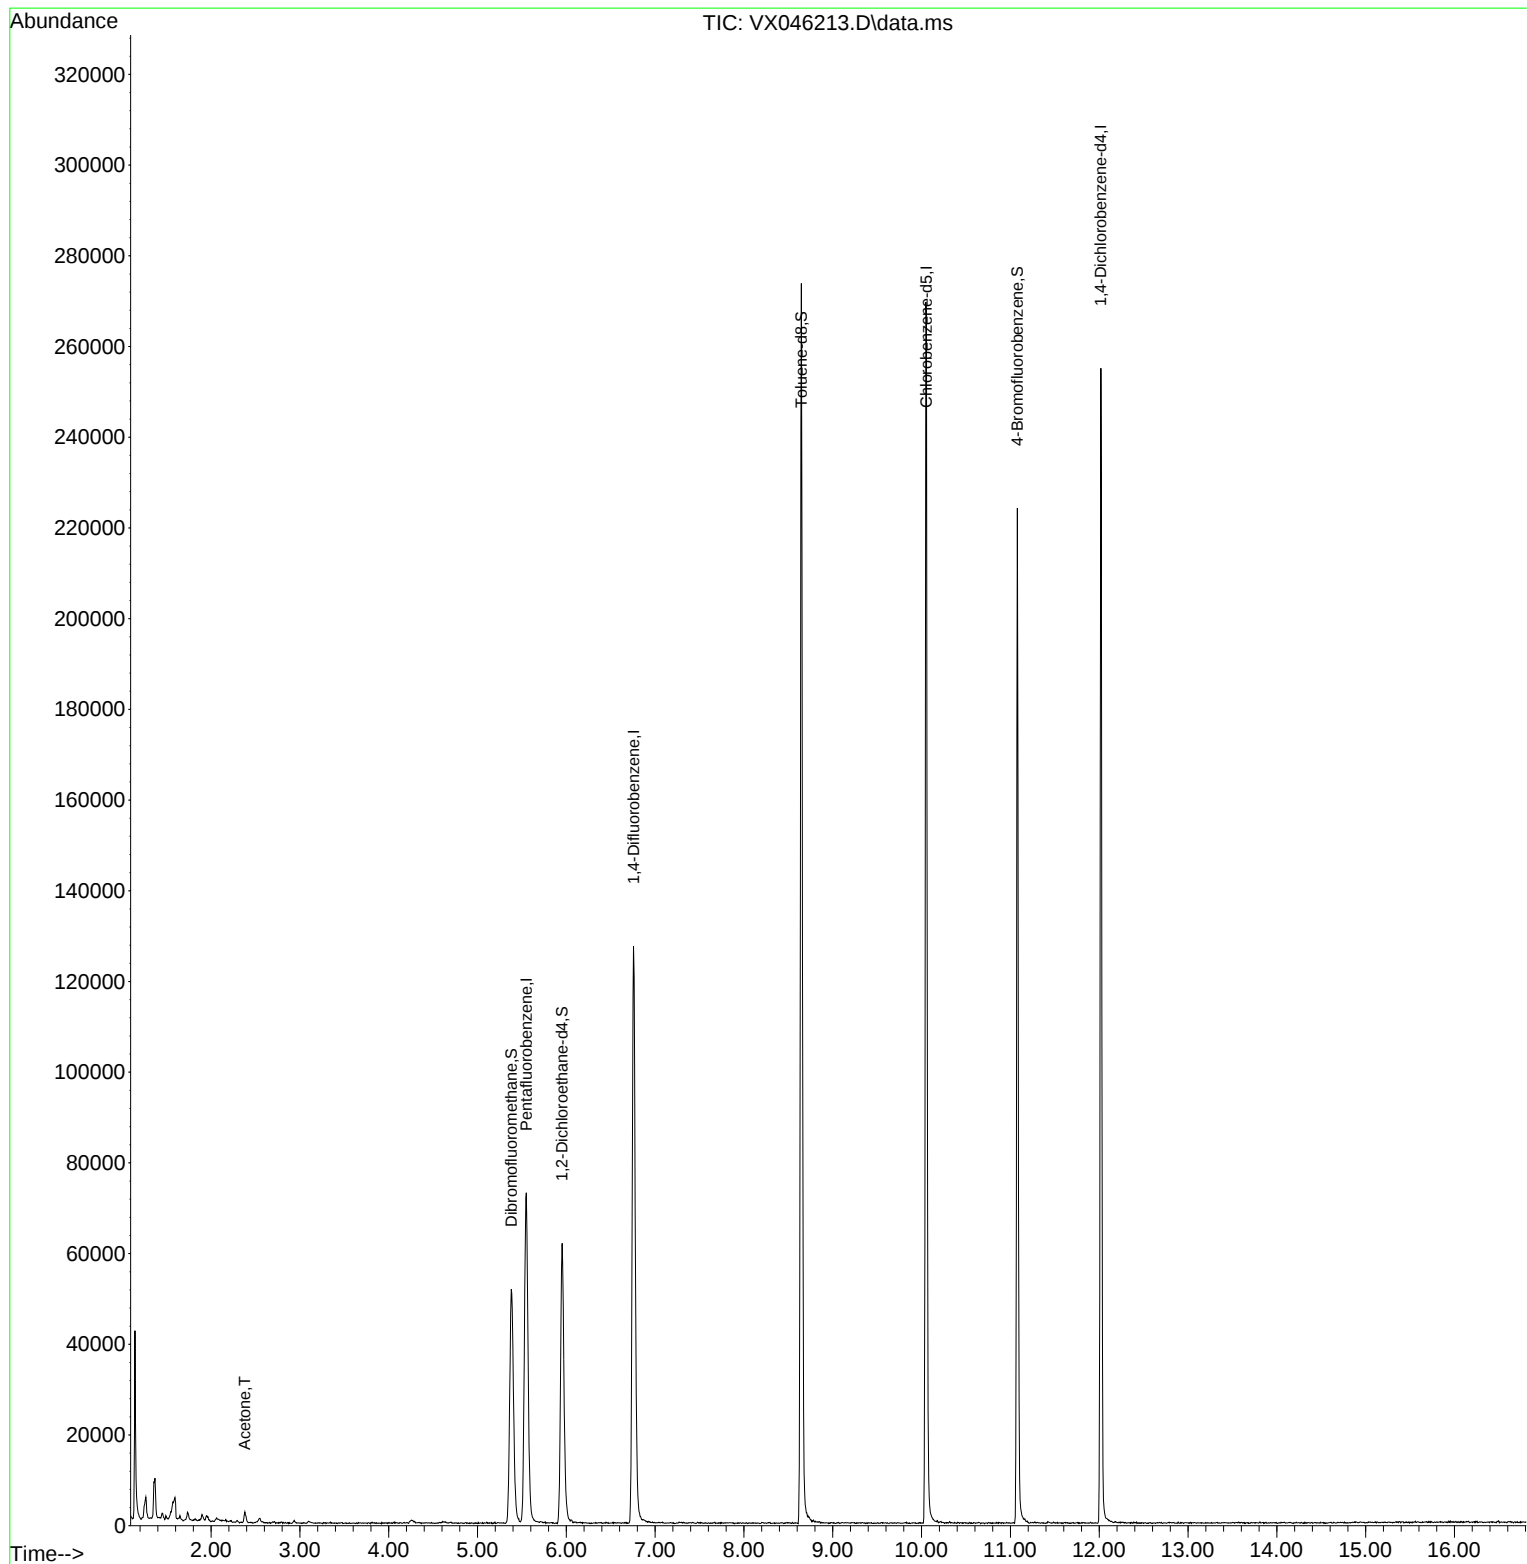




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX046213.D
Acq: 15 May 2025 14:58




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-182-GW-205-207


Tgt Ion:168 Resp: 60533
Ion Ratio Lower Upper
168 100
99 70.9 54.9 82.3

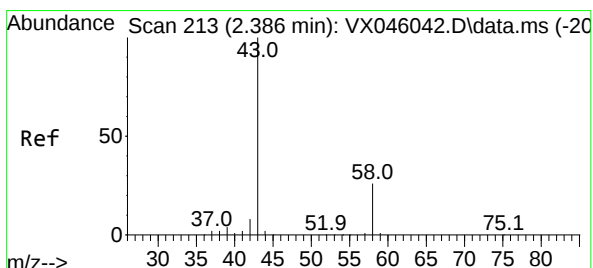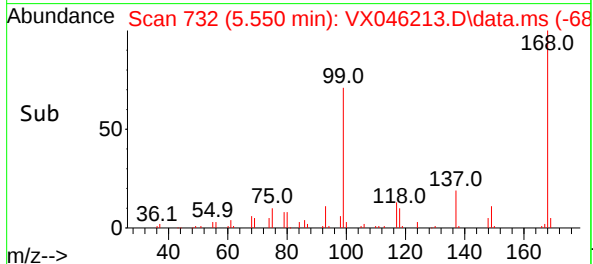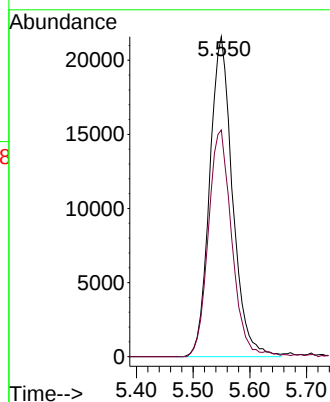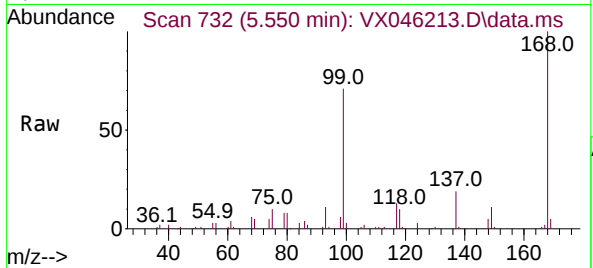

#16
Acetone
Concen: 5.154 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.006 min
Lab File: VX046213.D
Acq: 15 May 2025 14:58

Tgt Ion: 43 Resp: 2332
Ion Ratio Lower Upper
43 100
58 27.2 21.2 31.8

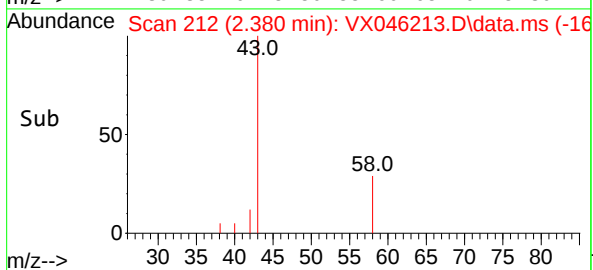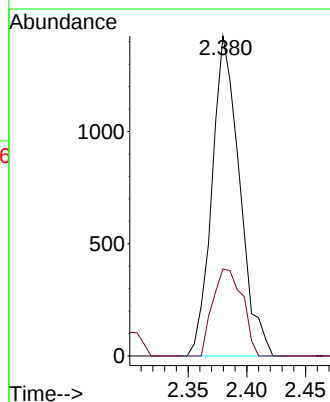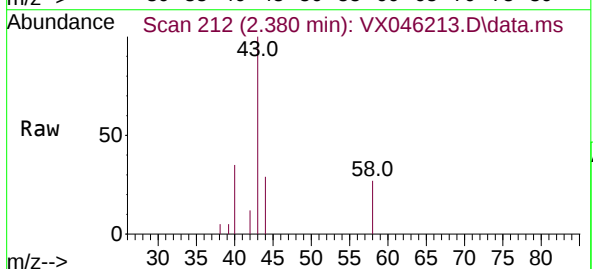

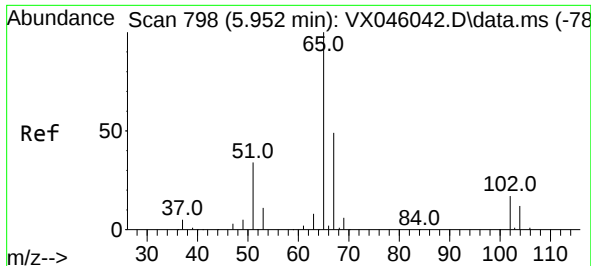

#33

1,2-Dichloroethane-d4

Concen: 55.448 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX046213.D

Acq: 15 May 2025 14:58

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB-182-GW-205-207

Tgt Ion: 65 Resp: 62575

Ion Ratio Lower Upper

65 100

67 50.3 0.0 99.0

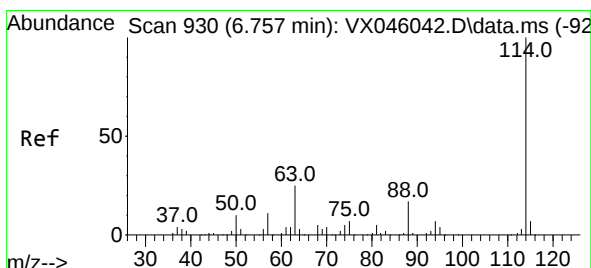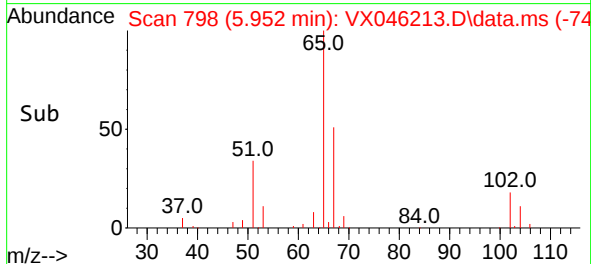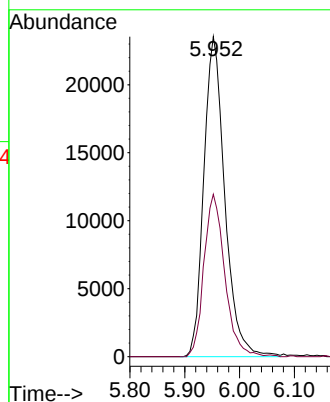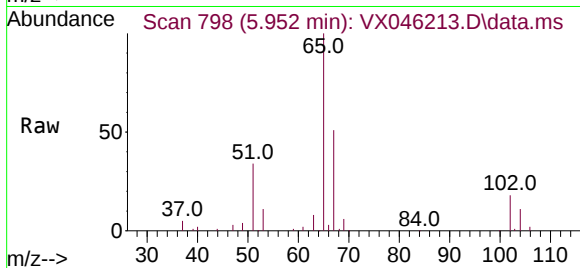

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX046213.D

Acq: 15 May 2025 14:58




Tgt Ion: 114 Resp: 121144

Ion Ratio Lower Upper

114 100

63 25.7 0.0 49.2

88 16.9 0.0 33.6


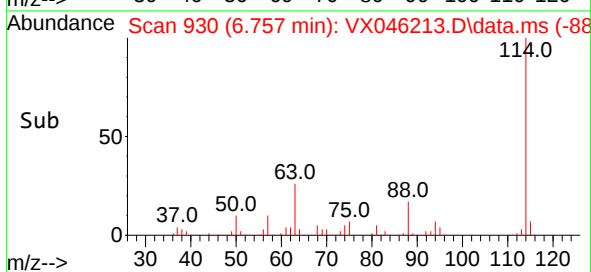
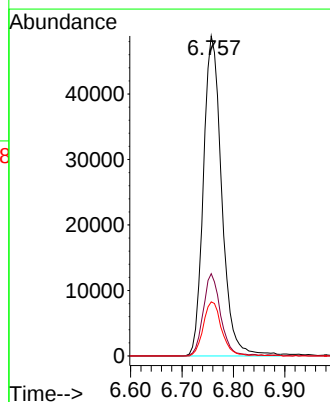
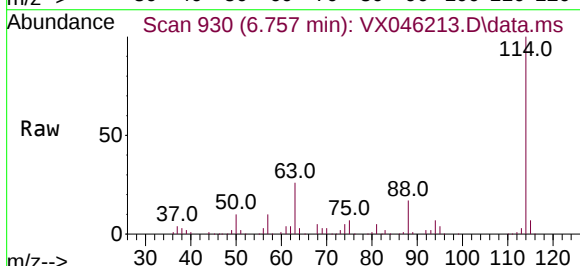




#35
Dibromofluoromethane
Concen: 52.008 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX046213.D
Acq: 15 May 2025 14:58




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-182-GW-205-207

Tgt Ion:113 Resp: 45370
Ion Ratio Lower Upper
113 100
111 104.4 83.1 124.7
192 16.6 13.3 19.9

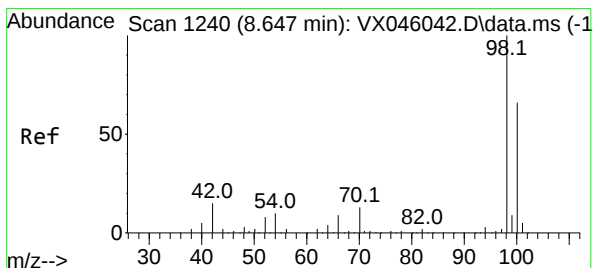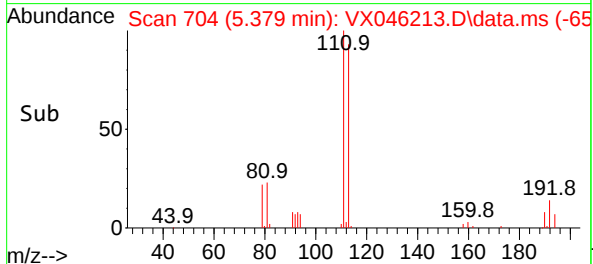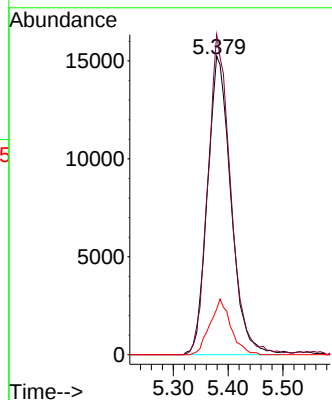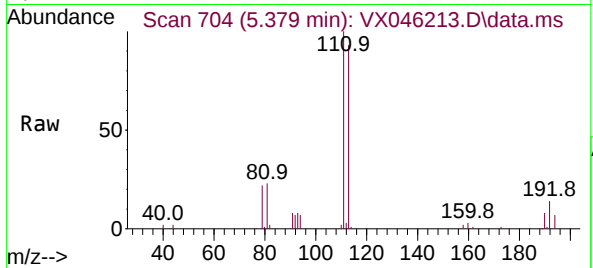

#50
Toluene-d8
Concen: 51.519 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX046213.D
Acq: 15 May 2025 14:58

Tgt Ion: 98 Resp: 155555
Ion Ratio Lower Upper
98 100
100 63.3 53.5 80.3


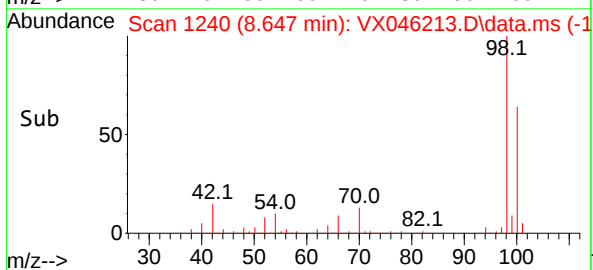
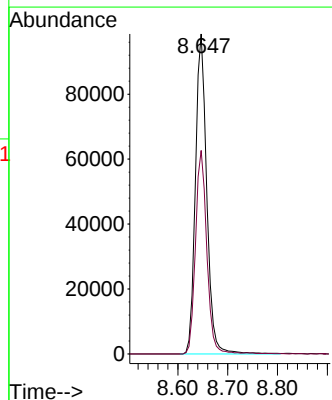
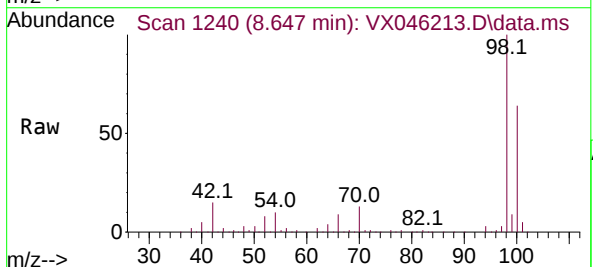




#62
4-Bromofluorobenzene
Concen: 49.474 ug/l
RT: 11.079 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046213.D
Acq: 15 May 2025 14:58




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-182-GW-205-207


Tgt Ion: 95 Resp: 57300
Ion Ratio Lower Upper
95 100
174 68.4 0.0 135.8
176 64.6 0.0 131.4

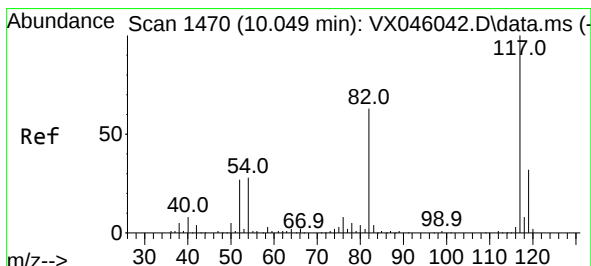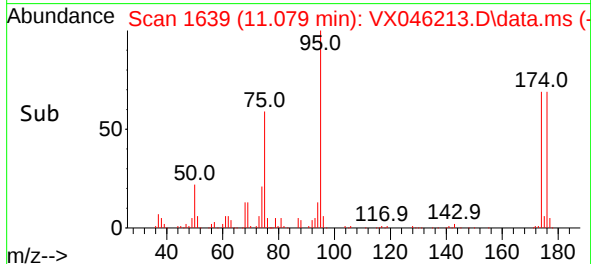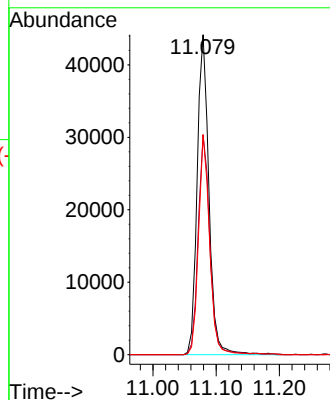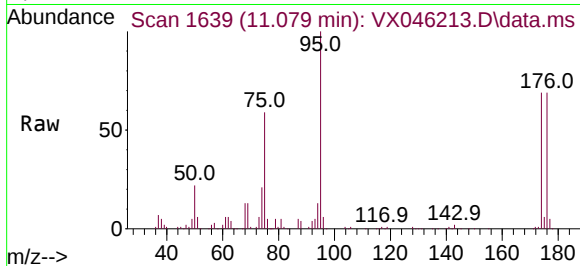

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VX046213.D
Acq: 15 May 2025 14:58


Tgt Ion: 117 Resp: 113426
Ion Ratio Lower Upper
117 100
82 60.4 50.6 76.0
119 32.9 25.8 38.6

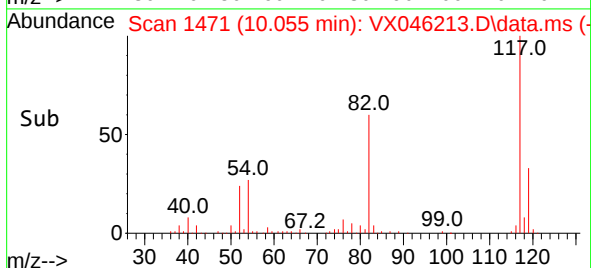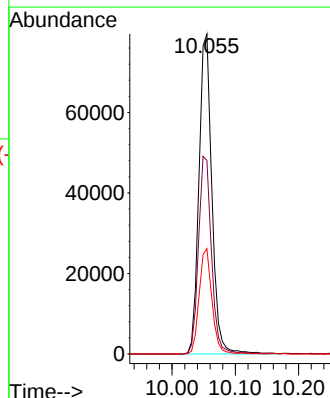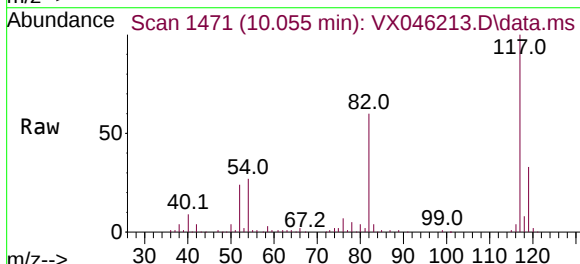

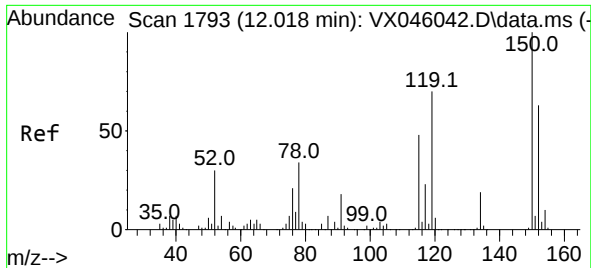

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.018 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX046213.D
 Acq: 15 May 2025 14:58

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-182-GW-205-207

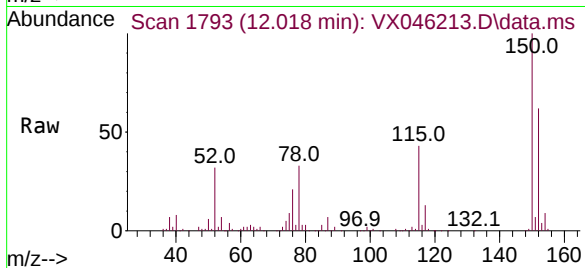

Tgt Ion:152 Resp: 47407
 Ion Ratio Lower Upper
 152 100
 115 66.7 46.9 140.7
 150 158.2 0.0 351.0

