

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051425\
 Data File : BN037000.D
 Acq On : 13 May 2025 18:17
 Operator : RC/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Manual Integrations
 APPROVED

Reviewed By :Rahul
 Chavli

05/15/2025
 Supervised By :Jagrut
 Upadhyay

Quant Time: May 14 11:00:10 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 14 10:57:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.618	152	2140	0.400	ng	0.00
7) Naphthalene-d8	10.404	136	5637	0.400	ng	0.00
13) Acenaphthene-d10	14.266	164	3174	0.400	ng	0.00
19) Phenanthrene-d10	17.009	188	6255	0.400	ng	0.00
29) Chrysene-d12	21.206	240	5420	0.400	ng	0.00
35) Perylene-d12	23.415	264	5487	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.213	112	1178	0.210	ng	0.00
5) Phenol-d6	6.795	99	1395	0.199	ng	0.00
8) Nitrobenzene-d5	8.771	82	1080	0.176	ng	0.00
11) 2-Methylnaphthalene-d10	11.996	152	1543	0.194	ng	0.00
14) 2,4,6-Tribromophenol	15.767	330	267	0.192	ng	0.00
15) 2-Fluorobiphenyl	12.888	172	2858	0.197	ng	0.00
27) Fluoranthene-d10	19.049	212	3232	0.188	ng	0.00
31) Terphenyl-d14	19.658	244	2287	0.197	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.140	88	546	0.208	ng	97
3) n-Nitrosodimethylamine	3.458	42	1042	0.185	ng	# 95
6) bis(2-Chloroethyl)ether	7.048	93	1244	0.193	ng	99
9) Naphthalene	10.447	128	3213	0.193	ng	99
10) Hexachlorobutadiene	10.746	225	698	0.200	ng	# 99
12) 2-Methylnaphthalene	12.072	142	2041	0.191	ng	99
16) Acenaphthylene	13.978	152	2917	0.189	ng	99
17) Acenaphthene	14.331	154	1950	0.193	ng	99
18) Fluorene	15.325	166	2509	0.189	ng	99
20) 4,6-Dinitro-2-methylph...	15.410	198	187	0.167	ng	# 48
21) 4-Bromophenyl-phenylether	16.214	248	770	0.195	ng	99
22) Hexachlorobenzene	16.326	284	840	0.199	ng	98
23) Atrazine	16.487	200	647	0.188	ng	98
24) Pentachlorophenol	16.673	266	419	0.178	ng	98
25) Phenanthrene	17.058	178	3977	0.195	ng	100
26) Anthracene	17.145	178	3452	0.186	ng	99
28) Fluoranthene	19.082	202	4499	0.184	ng	99
30) Pyrene	19.444	202	4629	0.200	ng	100
32) Benzo(a)anthracene	21.197	228	3882	0.190	ng	98
33) Chrysene	21.251	228	4226	0.196	ng	98
34) Bis(2-ethylhexyl)phtha...	21.135	149	2490	0.198	ng	99
36) Indeno(1,2,3-cd)pyrene	25.628	276	4426	0.198	ng	99
37) Benzo(b)fluoranthene	22.757	252	4306m	0.189	ng	
38) Benzo(k)fluoranthene	22.798	252	4219	0.188	ng	# 91
39) Benzo(a)pyrene	23.322	252	3685	0.191	ng	# 88
40) Dibenzo(a,h)anthracene	25.646	278	3380	0.194	ng	94
41) Benzo(g,h,i)perylene	26.301	276	3861	0.204	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051425\
Data File : BN037000.D
Acq On : 13 May 2025 18:17
Operator : RC/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Quant Time: May 14 11:00:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 14 10:57:36 2025
Response via : Initial Calibration


Manual Integrations
APPROVED

Reviewed By :Rahul
Chavli

05/15/2025
Supervised By :Jagrut
Upadhyay

05/15/2025

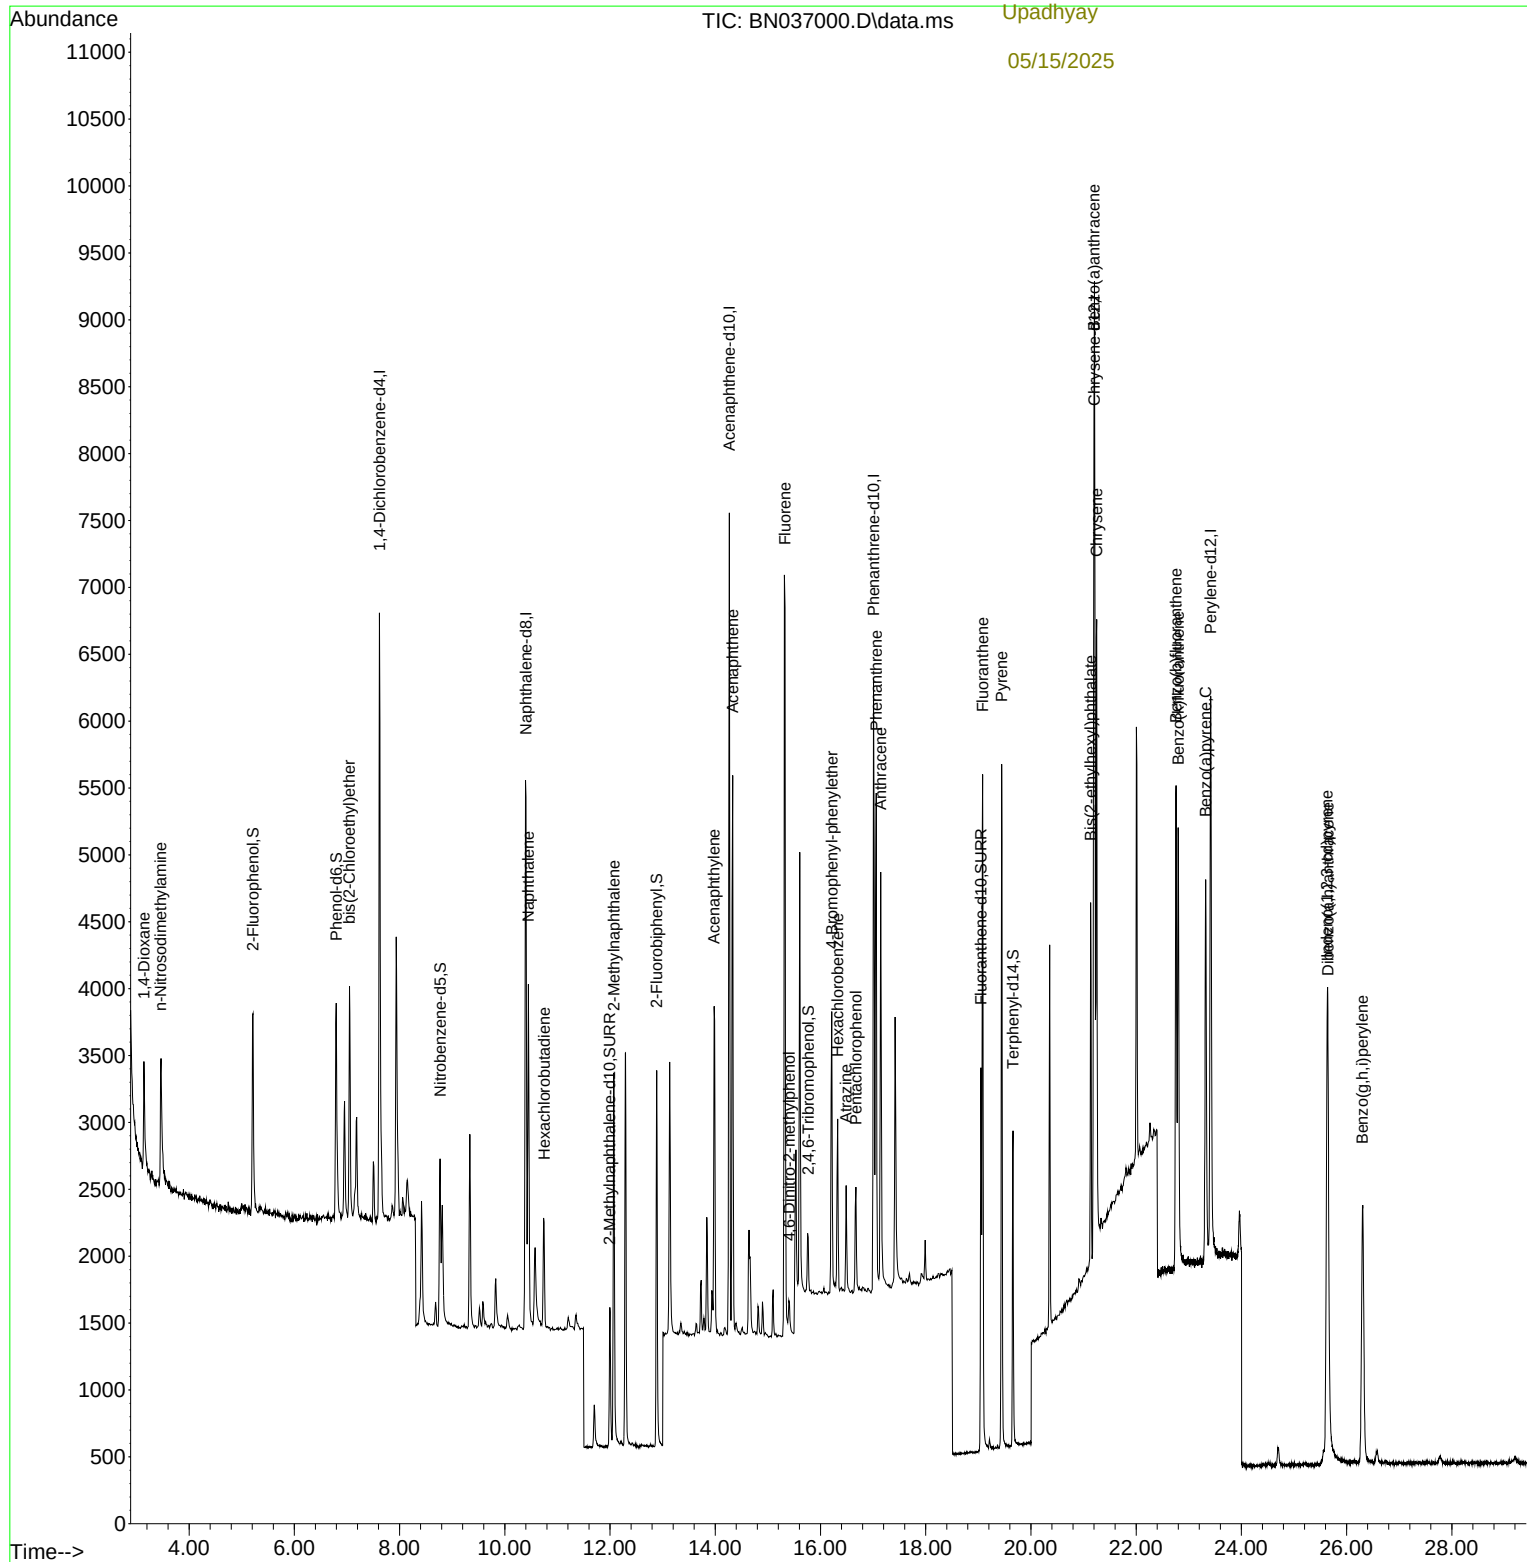




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.618 min Scan# 656
 Delta R.T. 0.000 min
 Lab File: BN037000.D
 Acq: 13 May 2025 18:17

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2



Tgt Ion: 152 Resp: 2140
 Ion Ratio Lower Upper
 152 100
 150 153.5 123.9 185.9
 115 68.7 55.8 83.8



Manual Integrations
 APPROVED

Reviewed By :Rahul
 Chavli


05/15/2025

Supervised By :Jagrut
 Upadhyay



05/15/2025

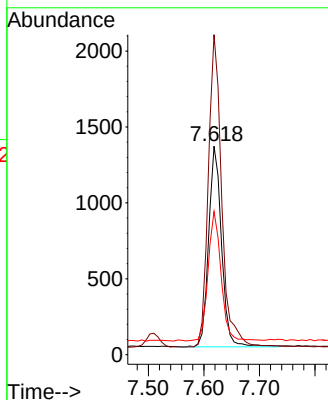


#2
 1,4-Dioxane
 Concen: 0.208 ng
 RT: 3.140 min Scan# 36
 Delta R.T. 0.000 min
 Lab File: BN037000.D
 Acq: 13 May 2025 18:17

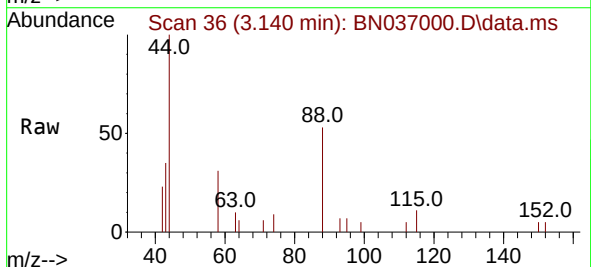


Tgt Ion: 88 Resp: 546
 Ion Ratio Lower Upper
 88 100
 43 52.4 37.4 56.0
 58 85.7 68.8 103.2

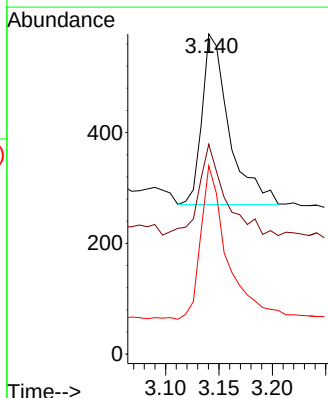



#3
n-Nitrosodimethylamine
Concen: 0.185 ng
RT: 3.458 min Scan# 80
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

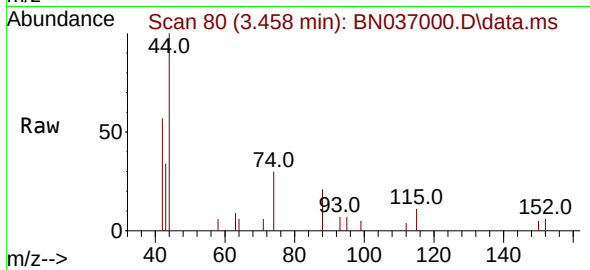

Tgt Ion: 42 Resp: 104
Ion Ratio Lower Upper
42 100
74 72.6 59.8 89.6
44 7.5 11.9 17.9




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 05/15/2025
Supervised By :Jagrut Upadhyay 05/15/2025



#4
2-Fluorophenol
Concen: 0.210 ng
RT: 5.213 min Scan# 323
Delta R.T. 0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17

Tgt Ion:112 Resp: 1178
Ion Ratio Lower Upper
112 100
64 68.7 55.7 83.5
63 47.2 34.6 51.8

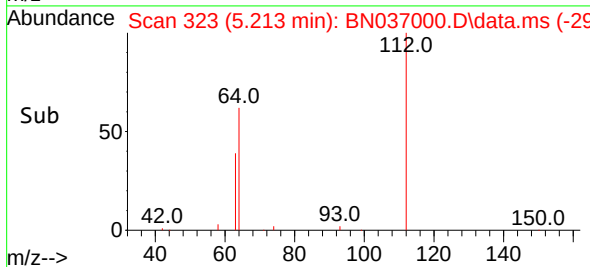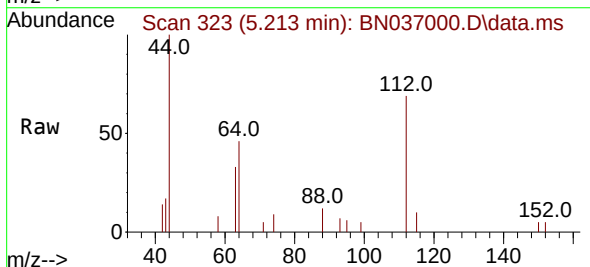



#5

Phenol-d6

Concen: 0.199 ng

RT: 6.795 min Scan# 542

Delta R.T. -0.000 min

Lab File: BN037000.D


Acq: 13 May 2025 18:17

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2

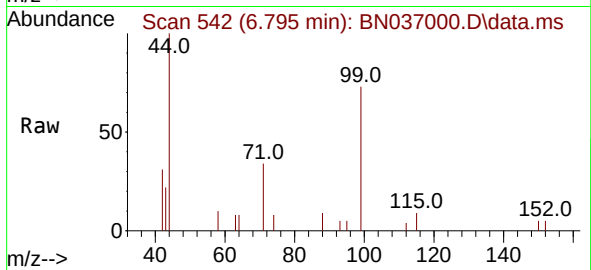




Tgt Ion:	99	Resp:	139
Ion	Ratio	Lower	Upper
99	100		
42	34.2	29.3	43.9
71	42.7	35.7	53.5

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 05/15/2025

Supervised By :Jagrut Upadhyay 05/15/2025

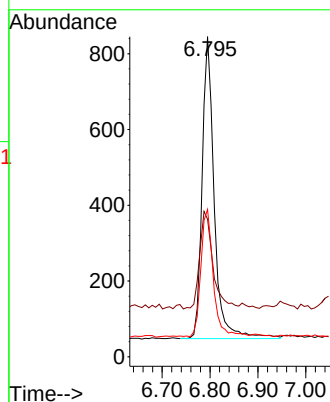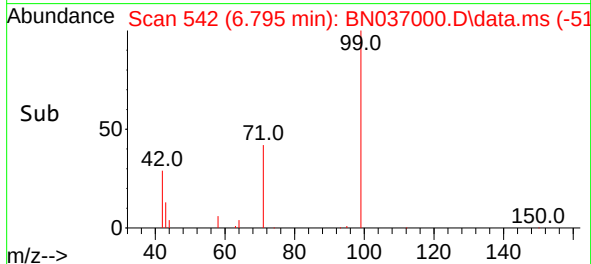

#6

bis(2-Chloroethyl)ether

Concen: 0.193 ng




RT: 7.048 min Scan# 577


Delta R.T. -0.000 min

Lab File: BN037000.D

Acq: 13 May 2025 18:17

Tgt Ion:	93	Resp:	1244
Ion	Ratio	Lower	Upper
93	100		
63	86.9	70.1	105.1
95	31.8	26.2	39.2

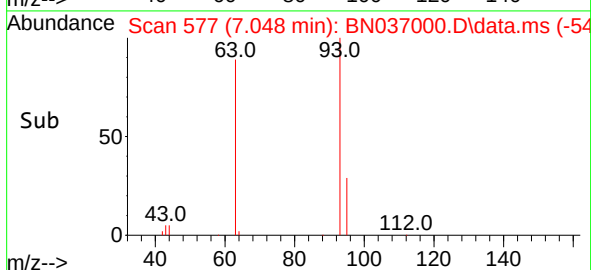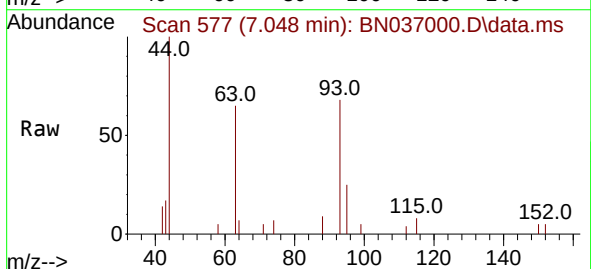

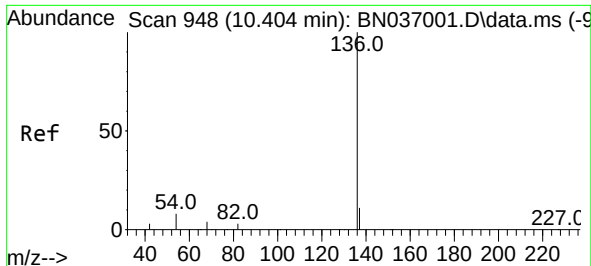





#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.404 min Scan# 948
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion:136	Resp:	563
Ion Ratio	Lower	Upper
136	100	
137	12.3	10.4 15.6
54	10.0	8.5 12.7
68	6.5	5.1 7.7




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 05/15/2025
Supervised By :Jagrut Upadhyay 05/15/2025

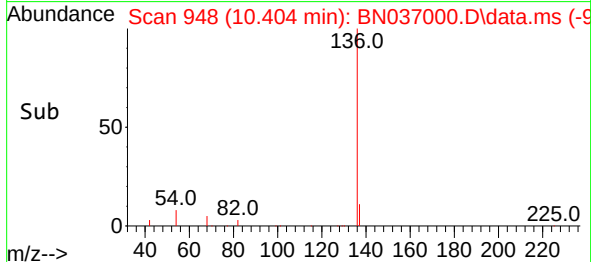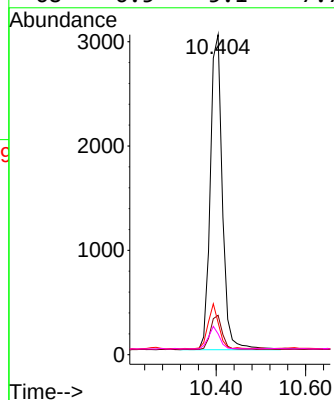

#8
Nitrobenzene-d5
Concen: 0.176 ng
RT: 8.771 min Scan# 795
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17

Tgt Ion: 82	Resp:	1080
Ion Ratio	Lower	Upper
82	100	
128	42.5	34.0 51.0
54	68.2	55.0 82.4

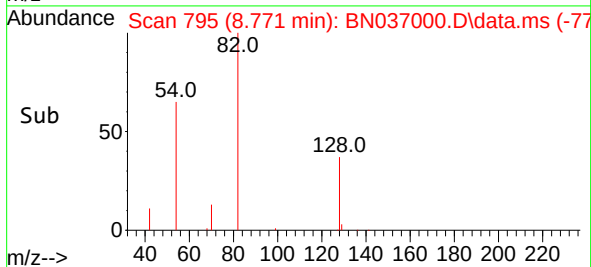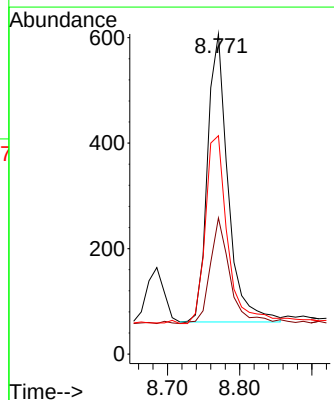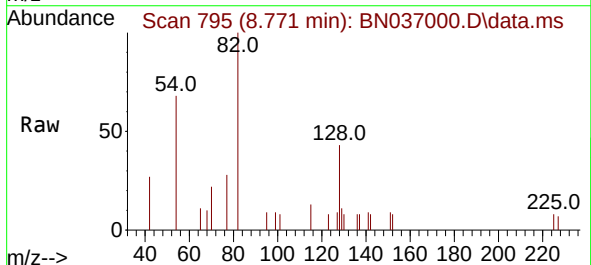

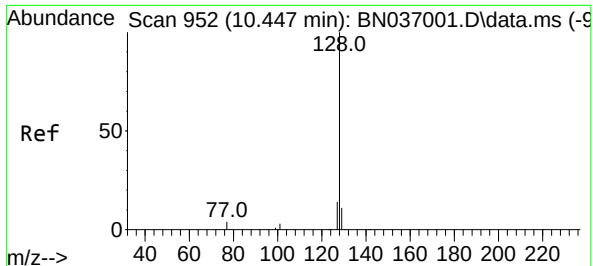





#9
Naphthalene
Concen: 0.193 ng
RT: 10.447 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Tgt Ion:128 Resp: 321
Ion Ratio Lower Upper
128 100
129 13.0 9.7 14.5
127 15.6 12.4 18.6




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 05/15/2025
Supervised By :Jagrut Upadhyay 05/15/2025

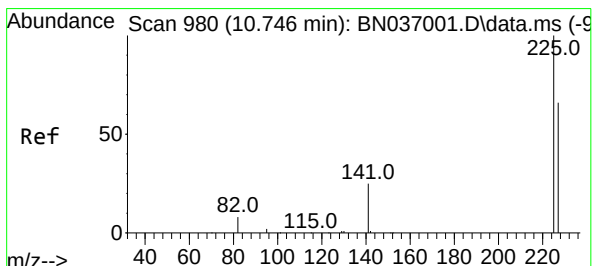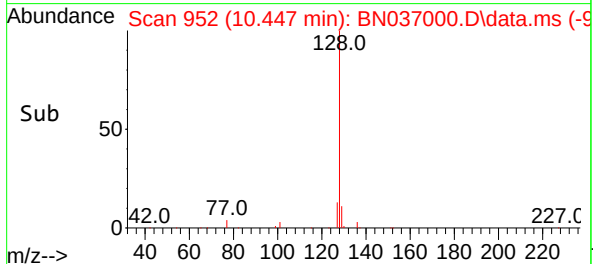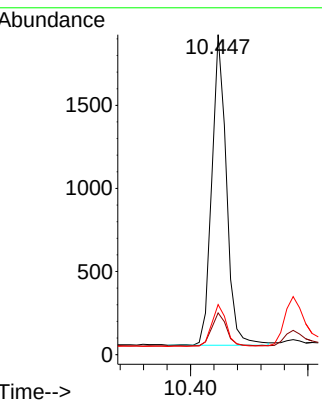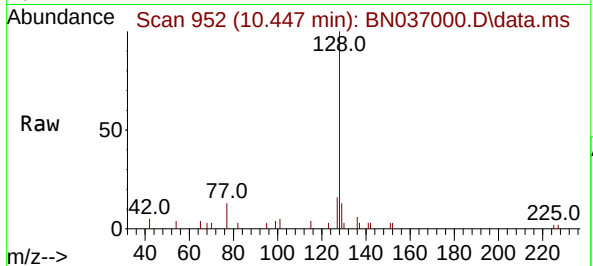

#10
Hexachlorobutadiene
Concen: 0.200 ng
RT: 10.746 min Scan# 980
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17


Tgt Ion:225 Resp: 698
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.6 50.9 76.3

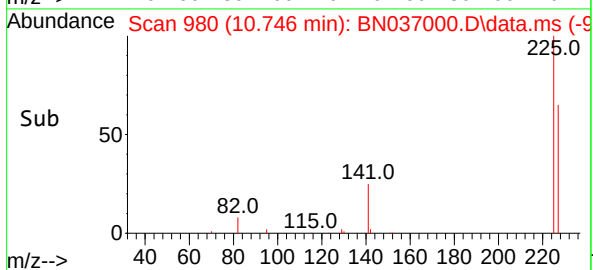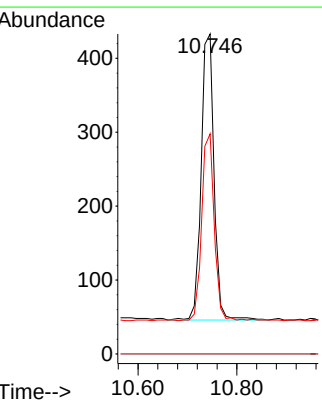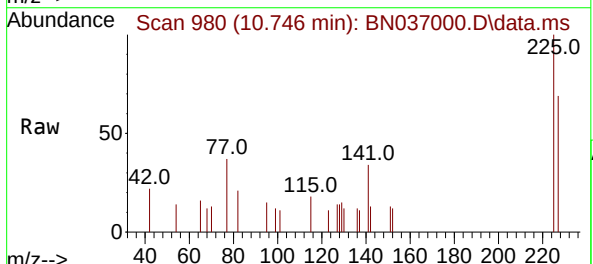

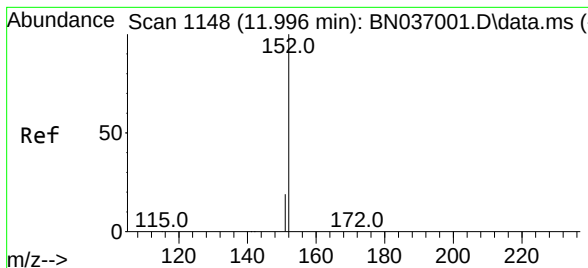

#11
2-Methylnaphthalene-d10
Concen: 0.194 ng
RT: 11.996 min Scan# 1148
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

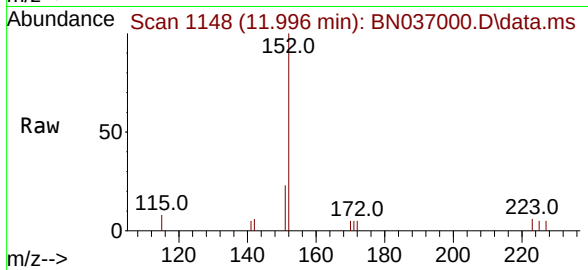

Tgt Ion:152 Resp: 154
Ion Ratio Lower Upper
152 100
151 22.0 17.5 26.3




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 05/15/2025
Supervised By :Jagrut Upadhyay 05/15/2025

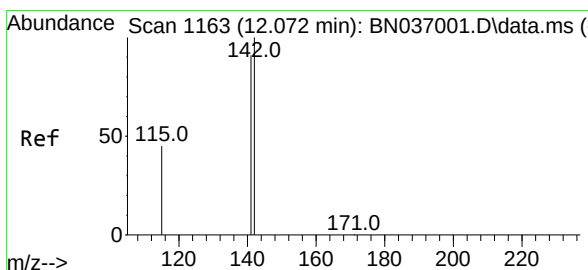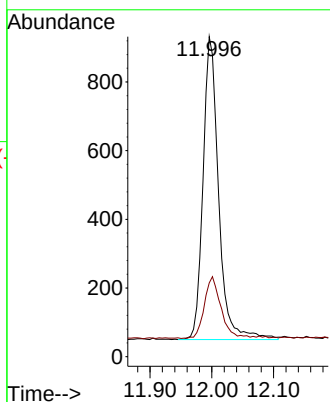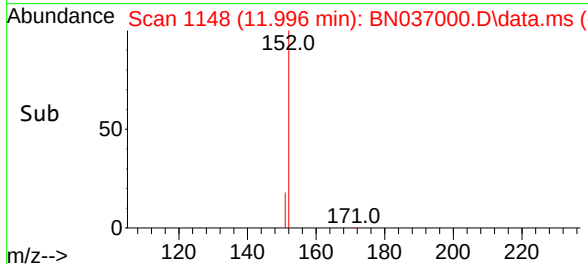

#12
2-Methylnaphthalene
Concen: 0.191 ng
RT: 12.072 min Scan# 1163
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17


Tgt Ion:142 Resp: 2041
Ion Ratio Lower Upper
142 100
141 91.1 73.3 109.9
115 49.5 38.4 57.6

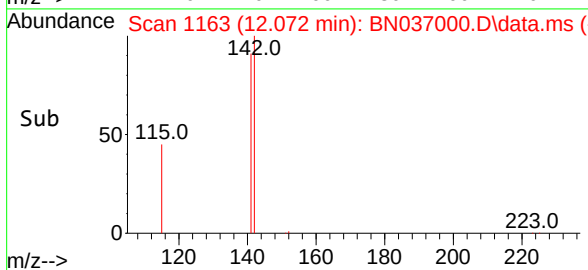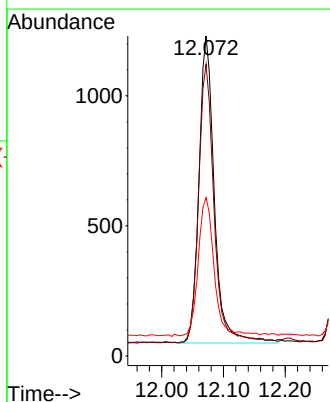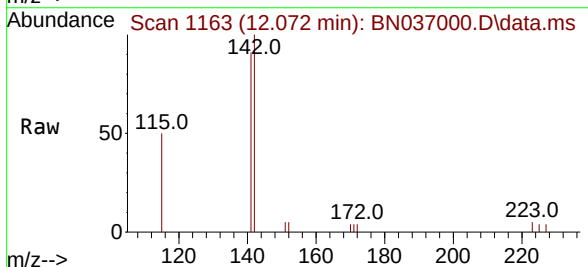



#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.266 min Scan# 1465
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2




Tgt Ion:164 Resp: 3174
Ion Ratio Lower Upper
164 100
162 105.4 84.2 126.4
160 52.6 42.6 63.8

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 05/15/2025
Supervised By :Jagrut Upadhyay 05/15/2025

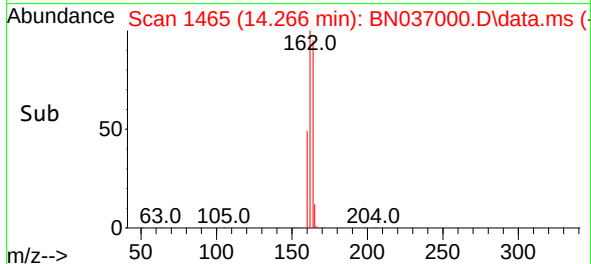


#14
2,4,6-Tribromophenol
Concen: 0.192 ng
RT: 15.767 min Scan# 1602
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17

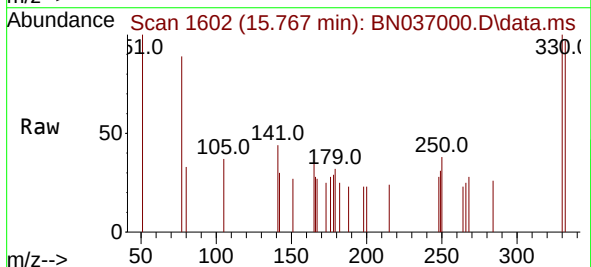


Tgt Ion:330 Resp: 267
Ion Ratio Lower Upper
330 100
332 93.3 73.8 110.8
141 58.1 43.9 65.9

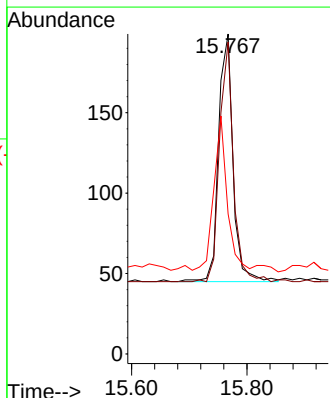

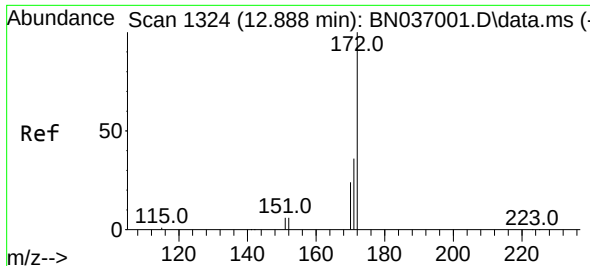

#15
2-Fluorobiphenyl
Concen: 0.197 ng
RT: 12.888 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

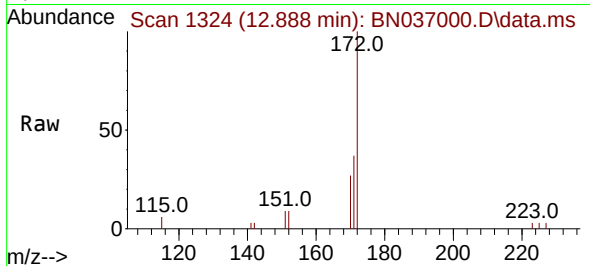

Tgt Ion:172 Resp: 285
Ion Ratio Lower Upper
172 100
171 37.4 29.2 43.8
170 26.9 20.5 30.7




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 05/15/2025
Supervised By :Jagrut Upadhyay 05/15/2025

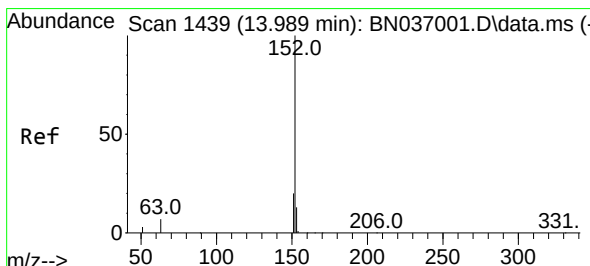

#16
Acenaphthylene
Concen: 0.189 ng
RT: 13.978 min Scan# 1438
Delta R.T. -0.011 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17


Tgt Ion:152 Resp: 2917
Ion Ratio Lower Upper
152 100
151 20.6 16.1 24.1
153 13.7 10.5 15.7

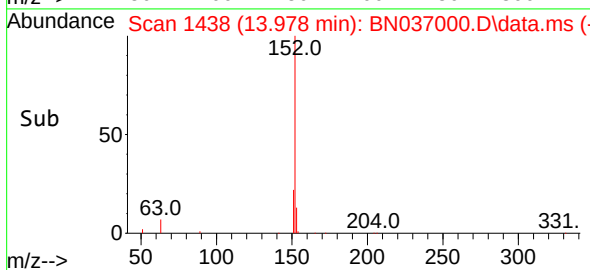



#17
Acenaphthene
Concen: 0.193 ng
RT: 14.331 min Scan# 1471
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2




Tgt Ion:154 Resp: 1950
Ion Ratio Lower Upper
154 100
153 117.0 94.2 141.4
152 62.3 49.4 74.0

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 05/15/2025
Supervised By :Jagrut Upadhyay 05/15/2025

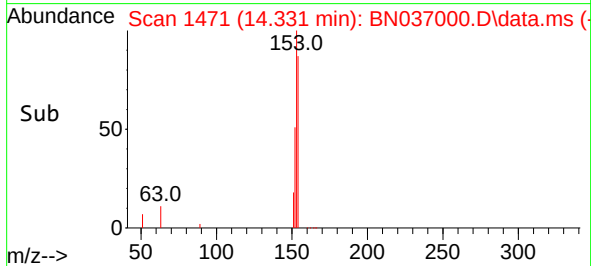


#18
Fluorene
Concen: 0.189 ng
RT: 15.325 min Scan# 1564
Delta R.T. 0.011 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17

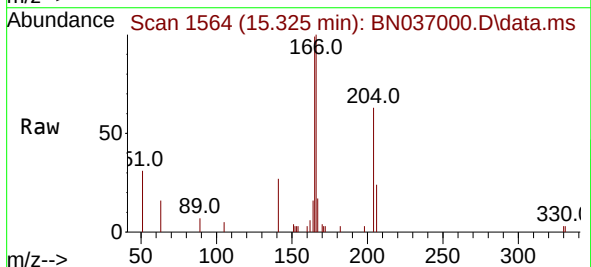


Tgt Ion:166 Resp: 2509
Ion Ratio Lower Upper
166 100
165 99.9 80.6 120.8
167 14.1 10.6 16.0

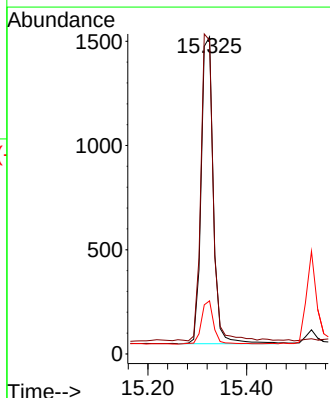



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.009 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2




Tgt Ion:188 Resp: 625
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 16.7 13.4 20.0

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 05/15/2025
Supervised By :Jagrut Upadhyay 05/15/2025




#20
4,6-Dinitro-2-methylphenol
Concen: 0.167 ng
RT: 15.410 min Scan# 1572
Delta R.T. 0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17

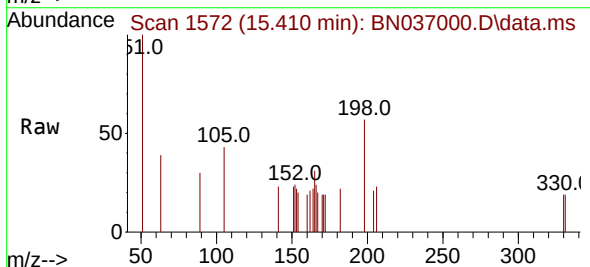

Tgt Ion:198 Resp: 187
Ion Ratio Lower Upper
198 100
51 176.6 87.8 131.6#
105 76.6 44.2 66.4#

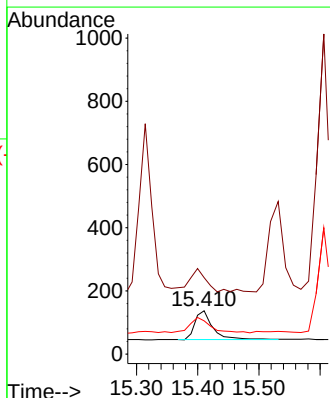




#21
4-Bromophenyl-phenylether
Concen: 0.195 ng
RT: 16.214 min Scan# 1638
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2

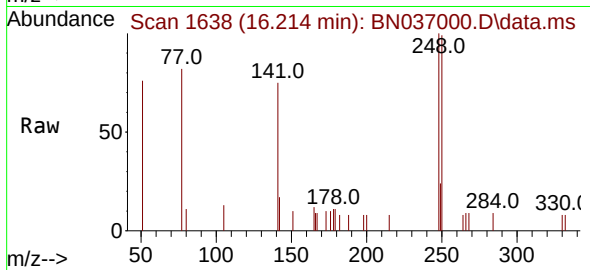




Tgt Ion:248 Resp: 770
Ion Ratio Lower Upper
248 100
250 99.5 78.1 117.1
141 75.0 59.7 89.5

Manual Integrations


APPROVED

Reviewed By :Rahul Chavli 05/15/2025



Supervised By :Jagrut Upadhyay 05/15/2025

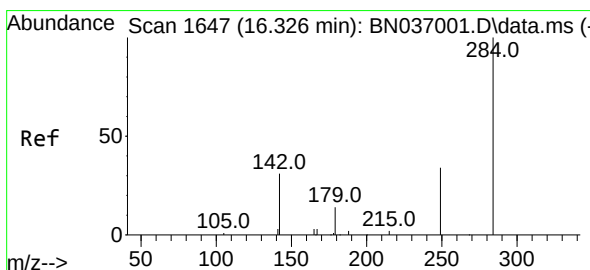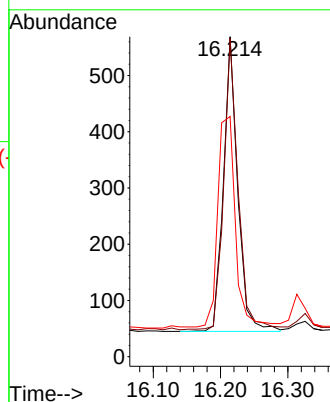


#22
Hexachlorobenzene
Concen: 0.199 ng
RT: 16.326 min Scan# 1647
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17

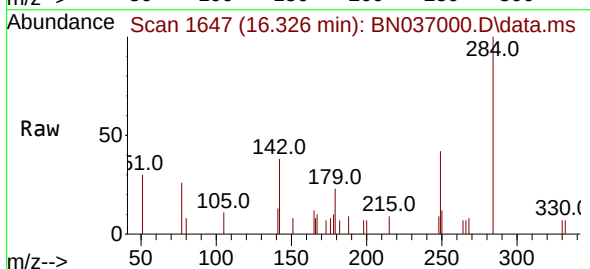

Tgt Ion:284 Resp: 840
Ion Ratio Lower Upper
284 100
142 52.3 41.2 61.8
249 37.9 28.7 43.1

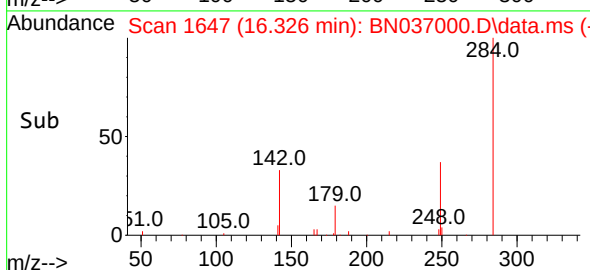



#23

Atrazine

Concen: 0.188 ng

RT: 16.487 min Scan# 1660

Delta R.T. -0.000 min

Lab File: BN037000.D

Acq: 13 May 2025 18:17

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:	200	Resp:	64
Ion Ratio	Lower	Upper	
200	100		
173	32.1	25.2	37.8
215	47.1	39.3	58.9

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 05/15/2025

Supervised By :Jagrut Upadhyay 05/15/2025

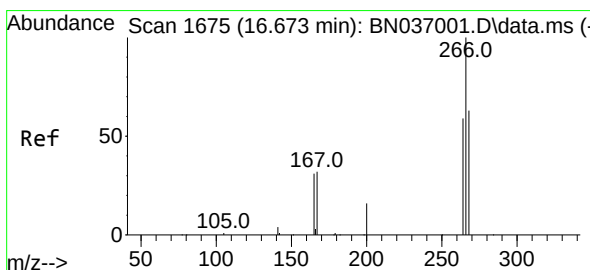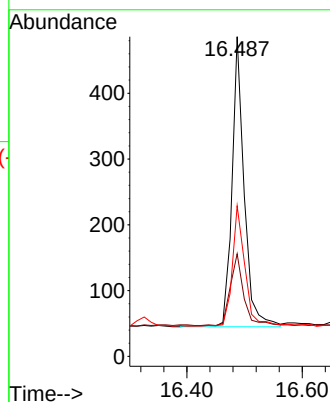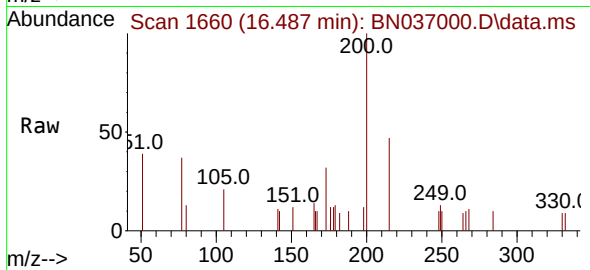

#24

Pentachlorophenol

Concen: 0.178 ng




RT: 16.673 min Scan# 1675


Delta R.T. -0.000 min

Lab File: BN037000.D

Acq: 13 May 2025 18:17

Tgt Ion:	266	Resp:	419
Ion Ratio	Lower	Upper	
266	100		
264	62.8	47.9	71.9
268	62.8	50.0	75.0

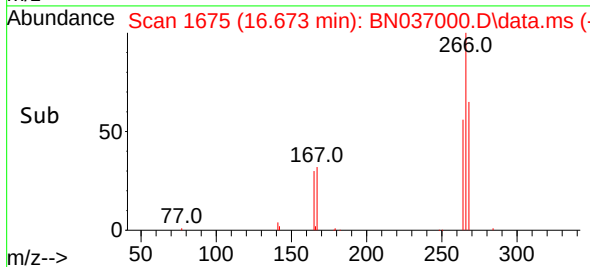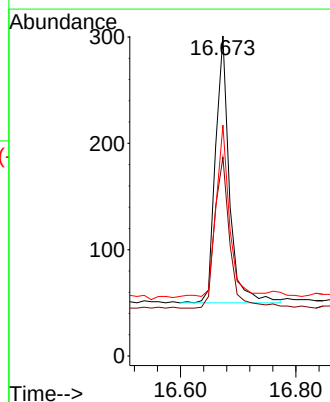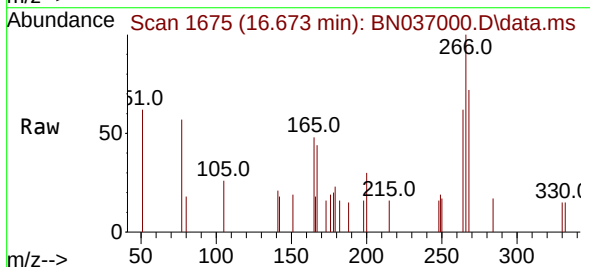

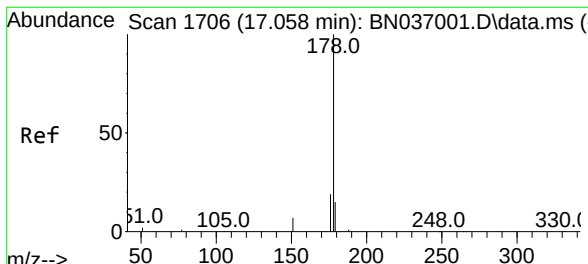





#25
 Phenanthrene
 Concen: 0.195 ng
 RT: 17.058 min Scan# 1706
 Delta R.T. -0.000 min
 Lab File: BN037000.D
 Acq: 13 May 2025 18:17

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion:	178	Resp:	397
Ion Ratio	Lower	Upper	
178	100		
176	19.6	15.7	23.5
179	15.6	12.2	18.2




Manual Integrations
 APPROVED


Reviewed By :Rahul Chavli 05/15/2025
 Supervised By :Jagrut Upadhyay 05/15/2025

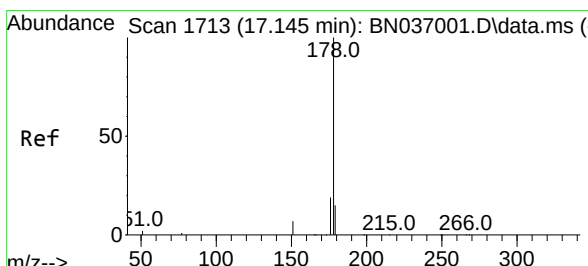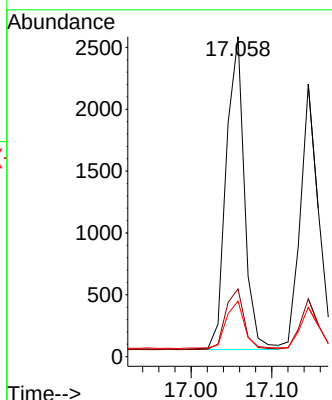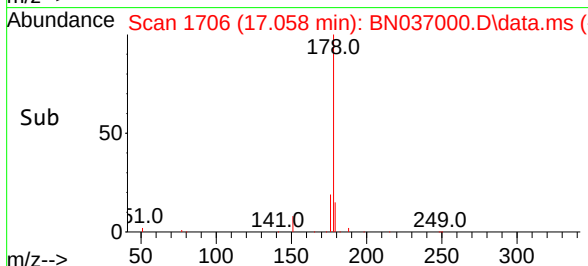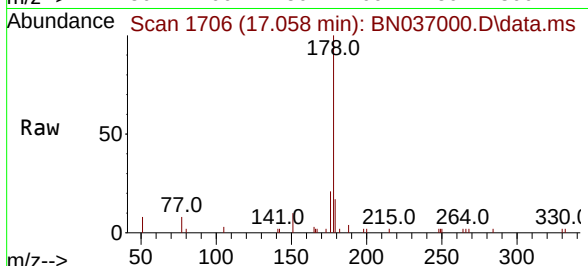

#26
 Anthracene
 Concen: 0.186 ng
 RT: 17.145 min Scan# 1713
 Delta R.T. -0.000 min
 Lab File: BN037000.D
 Acq: 13 May 2025 18:17


Tgt Ion:	178	Resp:	3452
Ion Ratio	Lower	Upper	
178	100		
176	18.8	15.0	22.6
179	15.9	12.3	18.5

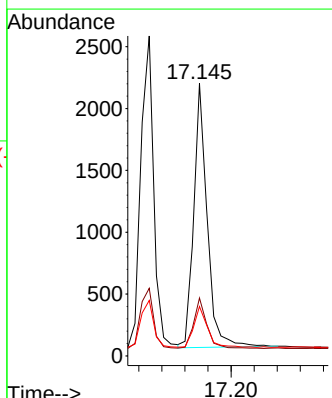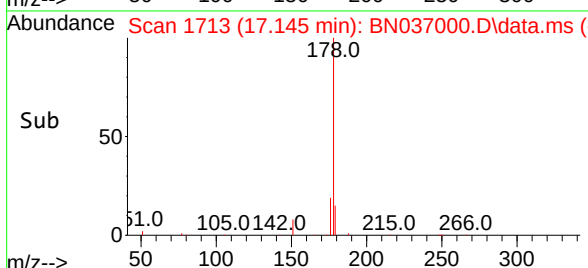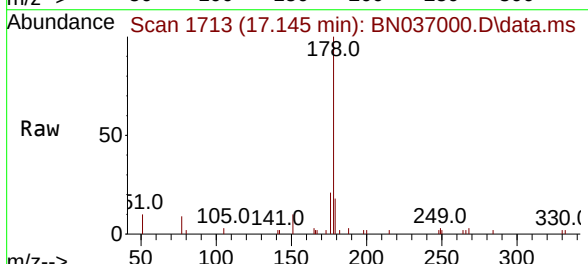

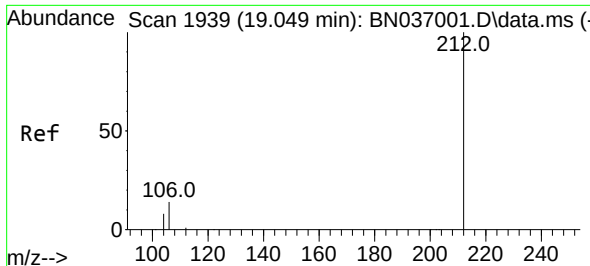

#27
Fluoranthene-d10
Concen: 0.188 ng
RT: 19.049 min Scan# 1939
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2




Tgt Ion:212 Resp: 323
Ion Ratio Lower Upper
212 100
106 14.3 11.3 16.9
104 9.5 6.7 10.1

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 05/15/2025
Supervised By :Jagrut Upadhyay 05/15/2025




#28
Fluoranthene
Concen: 0.184 ng
RT: 19.082 min Scan# 1946
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17

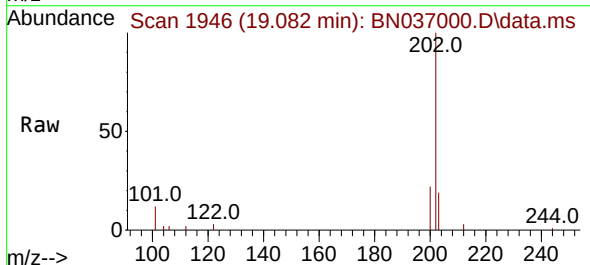


Tgt Ion:202 Resp: 4499
Ion Ratio Lower Upper
202 100
101 11.5 8.9 13.3
203 17.6 13.8 20.8

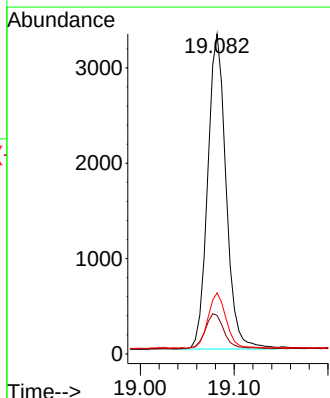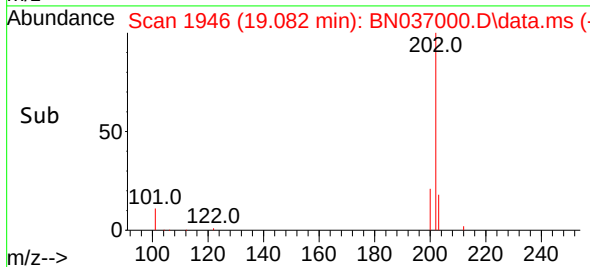

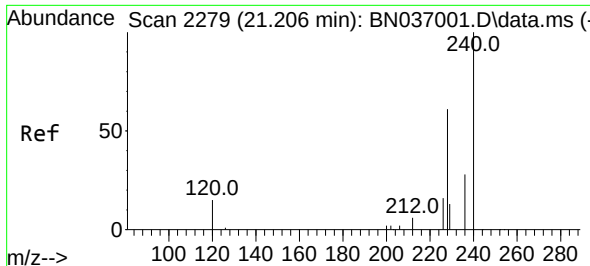

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.206 min Scan# 2127
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

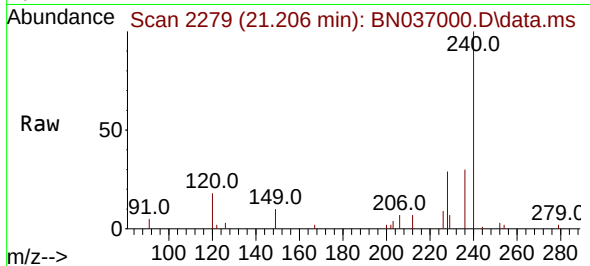


Tgt Ion:240 Resp: 5420
Ion Ratio Lower Upper
240 100
120 18.3 15.1 22.7
236 30.2 24.0 36.0

Manual Integrations
APPROVED



Reviewed By :Rahul Chavli 05/15/2025
Supervised By :Jagrut Upadhyay 05/15/2025

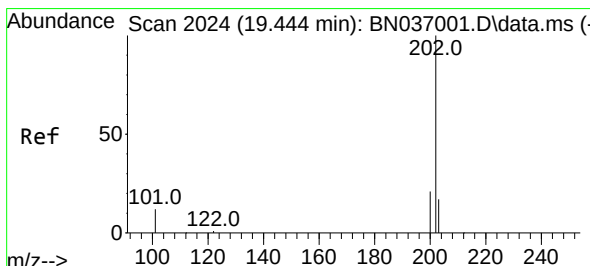


#30
Pyrene
Concen: 0.200 ng
RT: 19.444 min Scan# 2024
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17



Tgt Ion:202 Resp: 4629
Ion Ratio Lower Upper
202 100
200 21.3 17.1 25.7
203 17.7 14.2 21.4

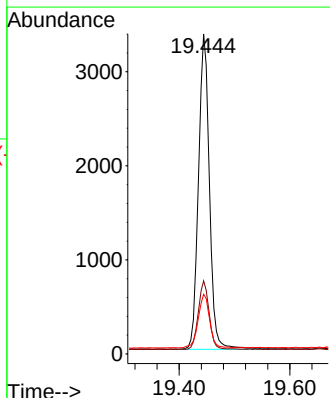




#31
 Terphenyl-d14
 Concen: 0.197 ng
 RT: 19.658 min Scan# 2070
 Delta R.T. -0.000 min
 Lab File: BN037000.D
 Acq: 13 May 2025 18:17

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2






Tgt Ion:244 Resp: 228
 Ion Ratio Lower Upper
 244 100
 212 12.5 9.7 14.5
 122 17.7 13.4 20.0

Manual Integrations


APPROVED

Reviewed By :Rahul Chavli 05/15/2025



Supervised By :Jagrut Upadhyay 05/15/2025

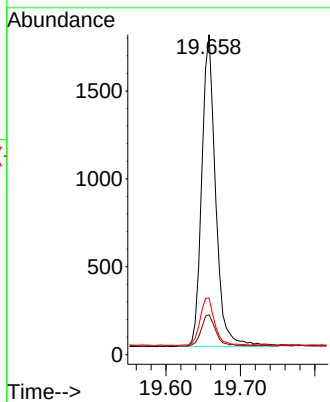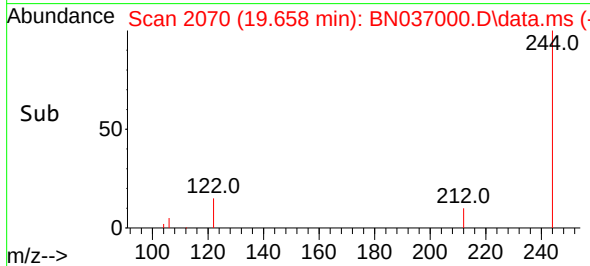


#32
 Benzo(a)anthracene
 Concen: 0.190 ng
 RT: 21.197 min Scan# 2278
 Delta R.T. -0.000 min
 Lab File: BN037000.D
 Acq: 13 May 2025 18:17

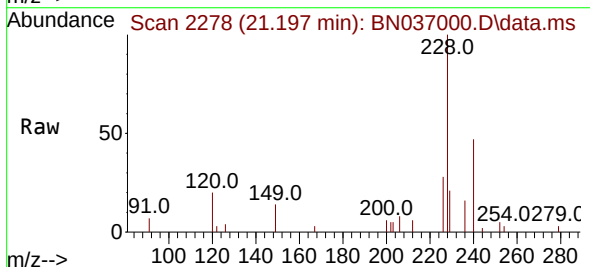

Tgt Ion:228 Resp: 3882
 Ion Ratio Lower Upper
 228 100
 226 28.3 22.2 33.4
 229 21.4 16.0 24.0

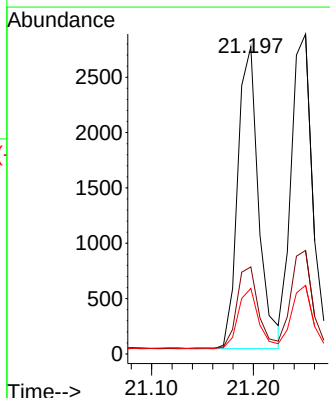

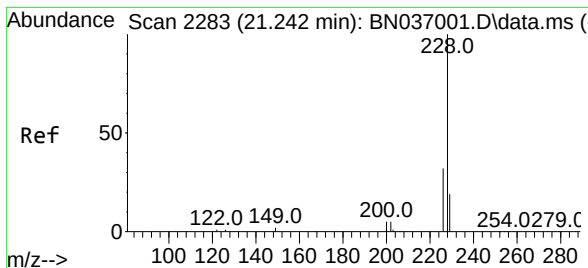

#33

Chrysene

Concen: 0.196 ng

RT: 21.251 min Scan# 2128

Delta R.T. 0.009 min

Lab File: BN037000.D


Acq: 13 May 2025 18:17

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2

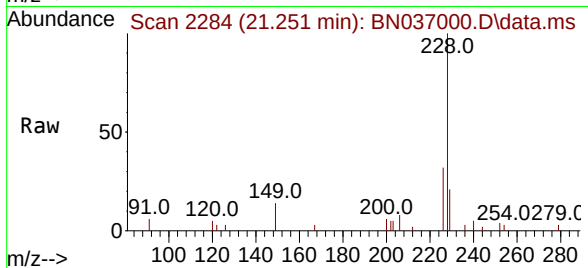




Tgt Ion:	228	Resp:	4220
Ion Ratio	Lower	Upper	
228	100		
226	32.3	26.3	39.5
229	21.4	16.2	24.2

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 05/15/2025

Supervised By :Jagrut Upadhyay 05/15/2025

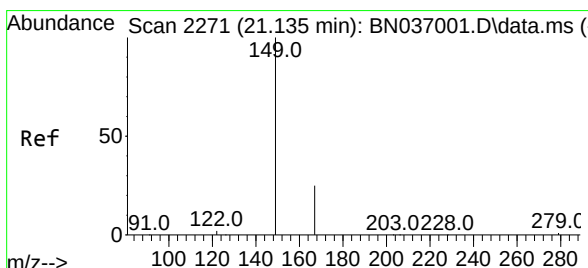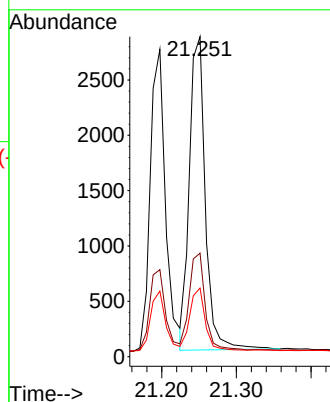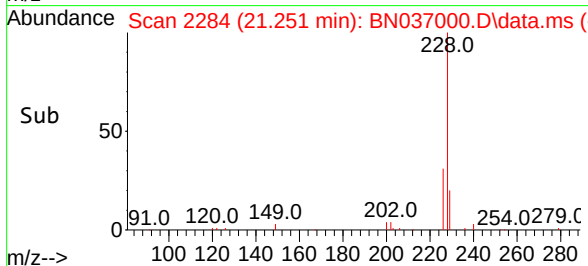

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.198 ng




RT: 21.135 min Scan# 2271


Delta R.T. -0.000 min

Lab File: BN037000.D

Acq: 13 May 2025 18:17


Tgt Ion:	149	Resp:	2490
Ion Ratio	Lower	Upper	
149	100		
167	26.4	20.6	30.8
279	3.8	2.6	3.8

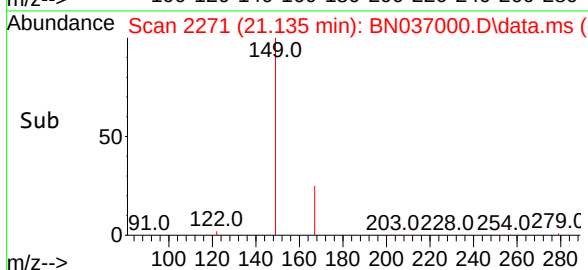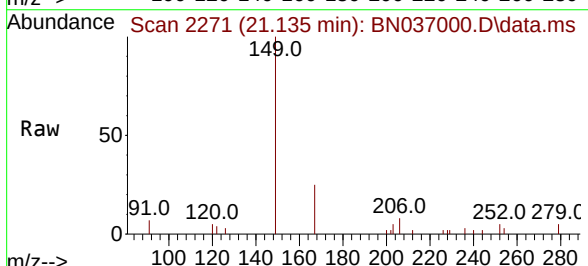

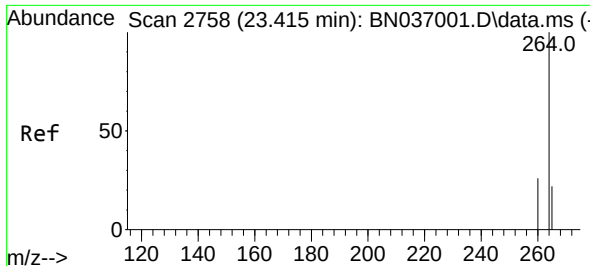

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.415 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN037000.D
 Acq: 13 May 2025 18:17




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2




Tgt Ion:264 Resp: 548
 Ion Ratio Lower Upper
 264 100
 260 26.6 21.9 32.9
 265 56.5 51.6 77.4

Manual Integrations
 APPROVED



Reviewed By :Rahul Chavli 05/15/2025
 Supervised By :Jagrut Upadhyay 05/15/2025




#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.198 ng
 RT: 25.628 min Scan# 3515
 Delta R.T. -0.003 min
 Lab File: BN037000.D
 Acq: 13 May 2025 18:17

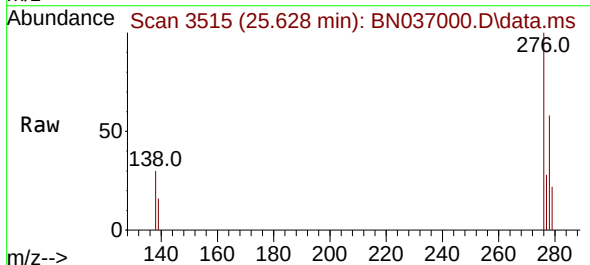


Tgt Ion:276 Resp: 4426
 Ion Ratio Lower Upper
 276 100
 138 27.9 22.7 34.1
 277 24.6 20.0 30.0

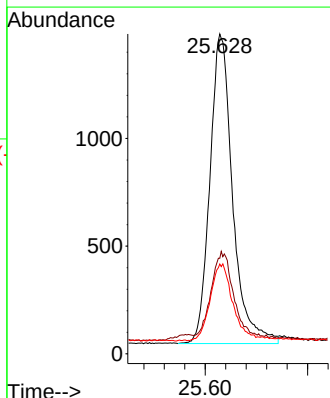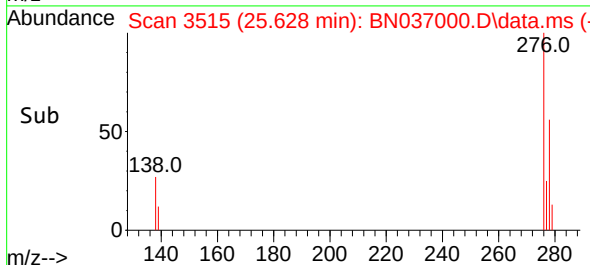

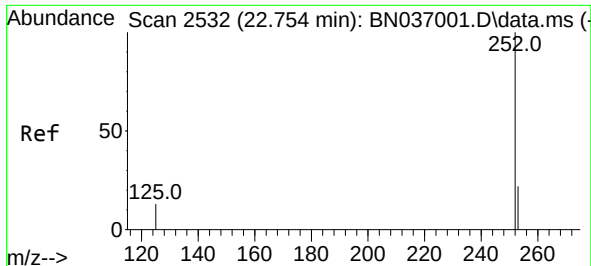

#37
Benzo(b)fluoranthene
Concen: 0.189 ng m
RT: 22.757 min Scan# 2533
Delta R.T. 0.003 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2



Tgt Ion:252 Resp: 4300
Ion Ratio Lower Upper
252 100
253 31.3 21.8 32.6
125 23.0 14.6 21.8




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 05/15/2025
Supervised By :Jagrut Upadhyay 05/15/2025

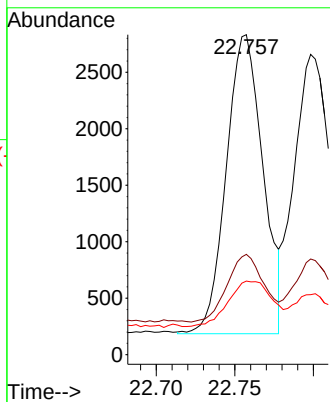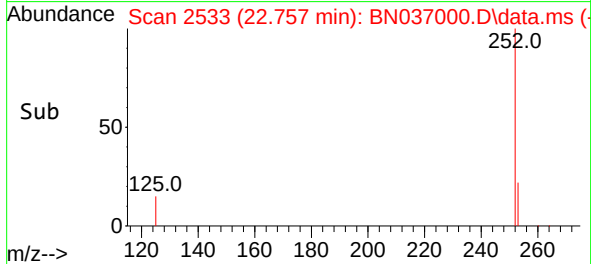

#38
Benzo(k)fluoranthene
Concen: 0.188 ng
RT: 22.798 min Scan# 2547
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17


Tgt Ion:252 Resp: 4219
Ion Ratio Lower Upper
252 100
253 31.9 21.4 32.2
125 20.0 13.0 19.4

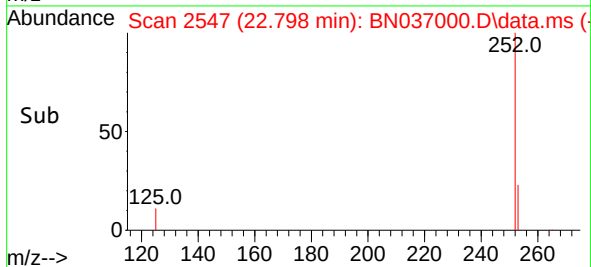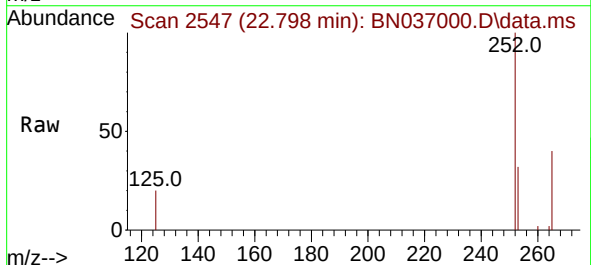



#39
Benzo(a)pyrene
Concen: 0.191 ng
RT: 23.322 min Scan# 2726
Delta R.T. 0.003 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

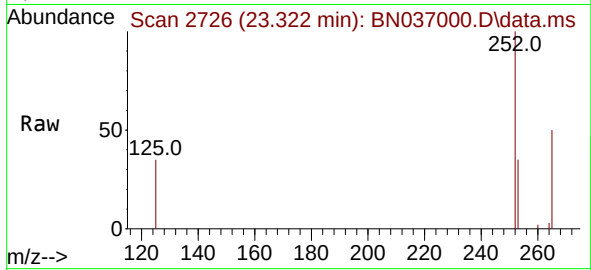

Tgt Ion:252 Resp: 368
Ion Ratio Lower Upper
252 100
253 34.9 23.8 35.6
125 35.0 21.8 32.6




Manual Integrations
APPROVED


Reviewed By :Rahul Chavli 05/15/2025
Supervised By :Jagrut Upadhyay 05/15/2025

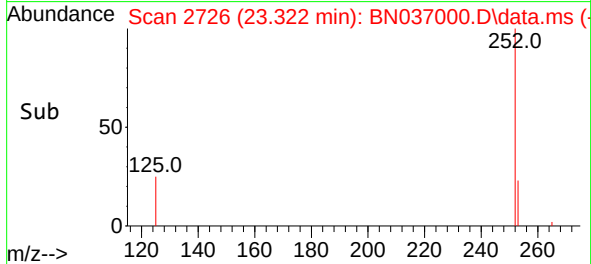

#40
Dibenzo(a,h)anthracene
Concen: 0.194 ng
RT: 25.646 min Scan# 3521
Delta R.T. -0.000 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17


Tgt Ion:278 Resp: 3380
Ion Ratio Lower Upper
278 100
139 24.5 17.4 26.0
279 33.7 24.6 37.0

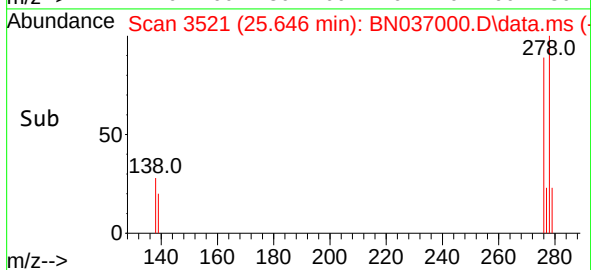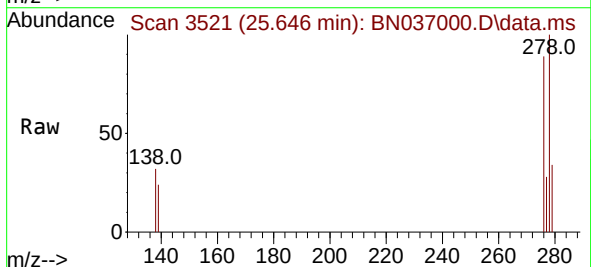

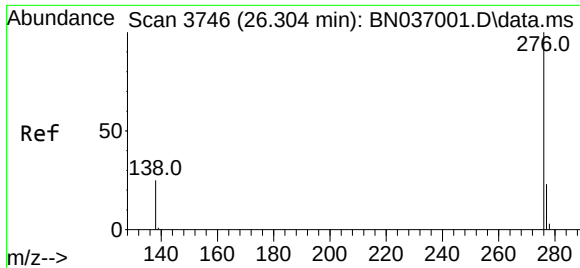

#41
Benzo(g,h,i)perylene
Concen: 0.204 ng
RT: 26.301 min Scan# 31
Delta R.T. -0.003 min
Lab File: BN037000.D
Acq: 13 May 2025 18:17

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

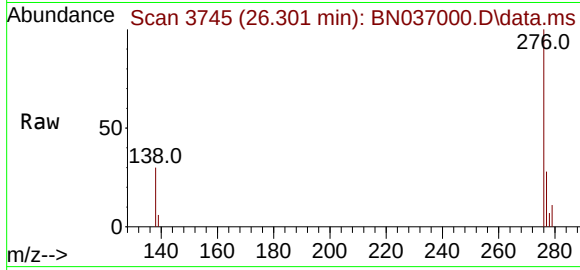

Tgt Ion:276 Resp: 386
Ion Ratio Lower Upper
276 100
277 27.6 20.2 30.4
138 29.6 22.0 33.0

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 05/15/2025
Supervised By :Jagrut Upadhyay 05/15/2025

