


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051925\
Data File : BN037037.D
Acq On : 19 May 2025 10:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 14 11:26:32 2025

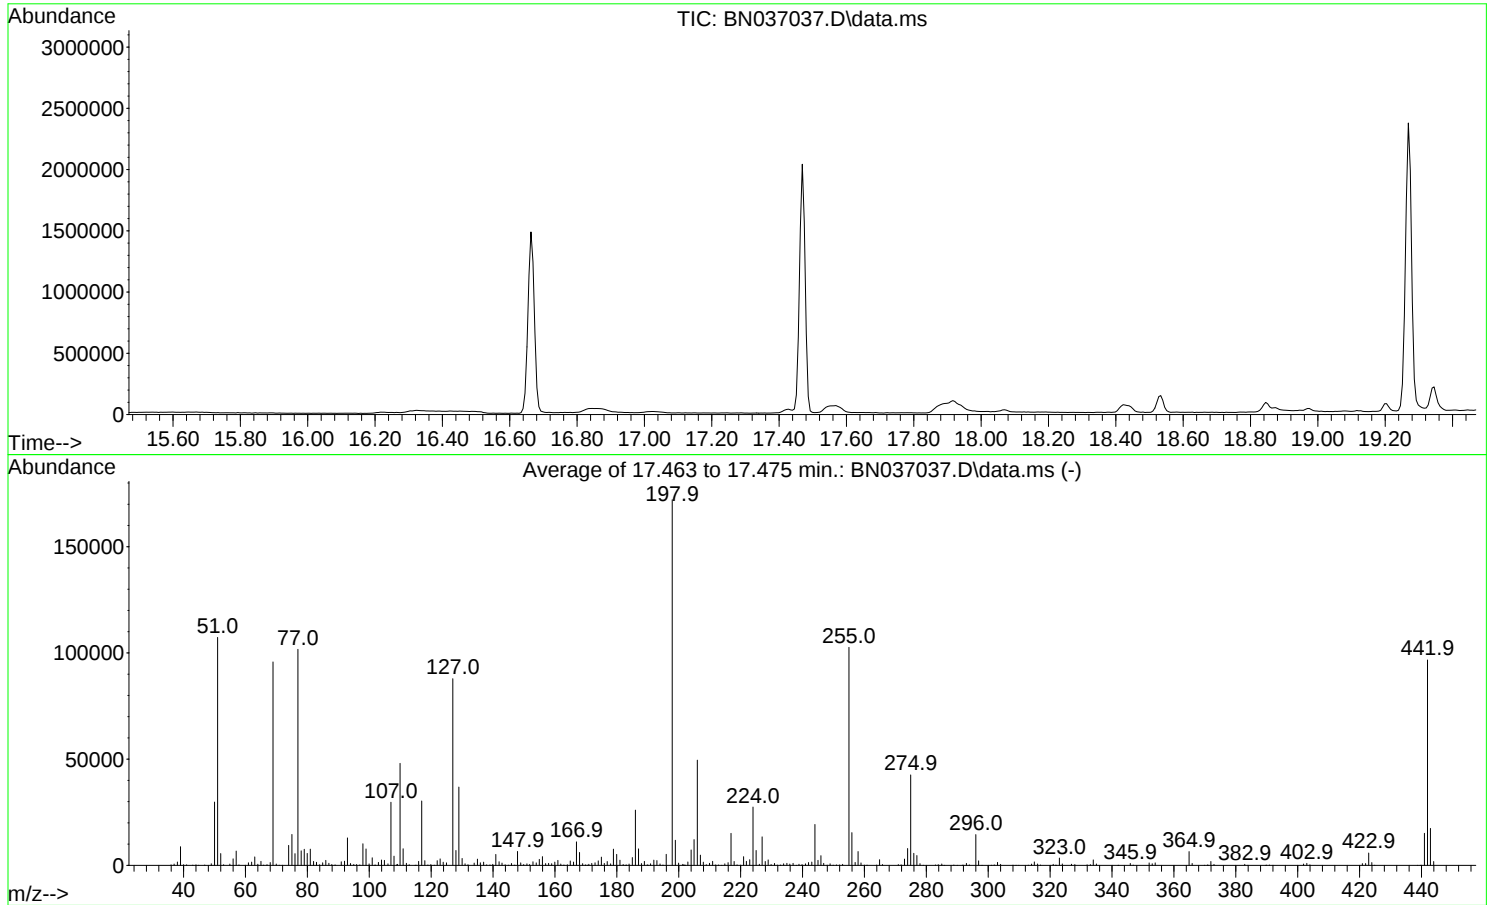

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.3	107312	PASS
68	69	0.00	2	1.4	1334	PASS
69	198	0.00	100	55.6	95774	PASS
70	69	0.00	2	0.7	629	PASS
127	198	10	80	51.1	87883	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	172139	PASS
199	198	5	9	6.9	11809	PASS
275	198	10	60	24.7	42579	PASS
365	198	1	100	3.8	6488	PASS
441	198	0.01	100	8.8	15091	PASS
442	442	50	100	100.0	96701	PASS
443	442	15	24	18.0	17401	PASS