

6C

SEMIVOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name: CHEMTECH Contract: TETR06  
Lab Code: CHEM Case No.: Q2063 SAS No.: Q2063 SDG No.: Q2063  
Instrument ID: BNA\_N Calibration Date(s): 05/13/2025 05/13/2025  
Calibration Time(s): 17:41 21:17

| LAB FILE ID:            |        | RRF0.1 = BN036999.D |        |        | RRF0.2 = BN037000.D |        | RRF0.4 = BN037001.D |       |
|-------------------------|--------|---------------------|--------|--------|---------------------|--------|---------------------|-------|
|                         |        | RRF0.8 = BN037002.D |        |        | RRF1.6 = BN037003.D |        | RRF3.2 = BN037004.D |       |
| COMPOUND                | RRF0.1 | RRF0.2              | RRF0.4 | RRF0.8 | RRF1.6              | RRF3.2 | RRF                 | % RSD |
| 2-Methylnaphthalene-d10 | 0.529  | 0.547               | 0.552  | 0.548  | 0.603               | 0.574  | 0.563               | 4.7   |
| Fluoranthene-d10        | 1.033  | 1.033               | 1.078  | 1.042  | 1.153               | 1.161  | 1.097               | 5.9   |
| 2-Fluorophenol          |        | 1.101               | 1.134  | 1.024  | 1.093               | 0.964  | 1.048               | 6.9   |
| Phenol-d6               |        | 1.304               | 1.385  | 1.236  | 1.392               | 1.259  | 1.311               | 4.9   |
| Nitrobenzene-d5         | 0.546  | 0.383               | 0.398  | 0.400  | 0.452               | 0.426  | 0.436               | 12.6  |
| 2-Fluorobiphenyl        | 1.912  | 1.801               | 1.901  | 1.802  | 1.927               | 1.672  | 1.832               | 4.9   |
| 2,4,6-Tribromophenol    | 0.174  | 0.168               | 0.178  | 0.160  | 0.186               | 0.175  | 0.176               | 5.8   |
| Terphenyl-d14           | 0.897  | 0.844               | 0.871  | 0.822  | 0.891               | 0.816  | 0.856               | 3.7   |
| 1,4-Dioxane             |        | 0.510               | 0.512  | 0.487  | 0.514               | 0.467  | 0.491               | 5.2   |

All other compounds must meet a minimum RRF of 0.010.

Form VI SV-1

Method Path : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\  
 Method File : 8270-SIM-BN051425.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed May 14 11:26:32 2025  
 Response Via : Initial Calibration

## Calibration Files

0.1 =BN036999.D 0.2 =BN037000.D 0.4 =BN037001.D 0.8 =BN037002.D 1.6 =BN037003.D 3.2 =BN037004.D 5.0 =BN037005.D

|          | Compound              | 0.1            | 0.2   | 0.4   | 0.8   | 1.6   | 3.2   | 5.0   | Avg   | %RSD  |
|----------|-----------------------|----------------|-------|-------|-------|-------|-------|-------|-------|-------|
| 1) I     | 1,4-Dichlorobenzen... | -----ISTD----- |       |       |       |       |       |       |       |       |
| 2)       | 1,4-Dioxane           | 0.510          | 0.512 | 0.487 | 0.514 | 0.467 | 0.454 | 0.491 | 5.25  |       |
| 3)       | n-Nitrosodimet...     | 1.465          | 0.974 | 0.980 | 0.971 | 1.075 | 0.967 | 0.950 | 1.054 | 17.59 |
| 4) S     | 2-Fluorophenol        | 1.101          | 1.134 | 1.024 | 1.093 | 0.964 | 0.971 | 1.048 | 6.87  |       |
| 5) S     | Phenol-d6             | 1.304          | 1.385 | 1.236 | 1.392 | 1.259 | 1.292 | 1.311 | 4.91  |       |
| 6)       | bis(2-Chloroet...     | 1.441          | 1.163 | 1.153 | 1.135 | 1.240 | 1.168 | 1.148 | 1.207 | 9.02  |
| 7) I     | Naphthalene-d8        | -----ISTD----- |       |       |       |       |       |       |       |       |
| 8) S     | Nitrobenzene-d5       | 0.546          | 0.383 | 0.398 | 0.400 | 0.452 | 0.426 | 0.442 | 0.436 | 12.60 |
| 9)       | Naphthalene           | 1.326          | 1.140 | 1.144 | 1.122 | 1.226 | 1.152 | 1.165 | 1.182 | 6.05  |
| 10)      | Hexachlorobuta...     | 0.286          | 0.248 | 0.244 | 0.235 | 0.256 | 0.236 | 0.233 | 0.248 | 7.47  |
| 11) SURR | 2-Methylnaphth...     | 0.529          | 0.547 | 0.552 | 0.548 | 0.603 | 0.574 | 0.588 | 0.563 | 4.65  |
| 12)      | 2-Methylnaphth...     | 0.754          | 0.724 | 0.736 | 0.733 | 0.814 | 0.770 | 0.790 | 0.760 | 4.34  |
| 13) I    | Acenaphthene-d10      | -----ISTD----- |       |       |       |       |       |       |       |       |
| 14) S    | 2,4,6-Tribromo...     | 0.174          | 0.168 | 0.178 | 0.160 | 0.186 | 0.175 | 0.189 | 0.176 | 5.77  |
| 15) S    | 2-Fluorobiphenyl      | 1.912          | 1.801 | 1.901 | 1.802 | 1.927 | 1.672 | 1.807 | 1.832 | 4.90  |
| 16)      | Acenaphthylene        | 1.906          | 1.838 | 1.894 | 1.849 | 2.071 | 1.997 | 2.075 | 1.947 | 5.14  |
| 17)      | Acenaphthene          | 1.255          | 1.229 | 1.243 | 1.217 | 1.350 | 1.298 | 1.315 | 1.272 | 3.89  |
| 18)      | Fluorene              | 1.602          | 1.581 | 1.635 | 1.611 | 1.779 | 1.721 | 1.752 | 1.669 | 4.80  |
| 19) I    | Phenanthrene-d10      | -----ISTD----- |       |       |       |       |       |       |       |       |
| 20)      | 4,6-Dinitro-2-...     | 0.060          | 0.073 | 0.079 | 0.102 | 0.103 | 0.124 | 0.090 | 26.02 |       |
| 21)      | 4-Bromophenyl-...     | 0.243          | 0.246 | 0.250 | 0.247 | 0.262 | 0.261 | 0.259 | 0.253 | 3.13  |
| 22)      | Hexachlorobenzene     | 0.267          | 0.269 | 0.281 | 0.259 | 0.281 | 0.270 | 0.267 | 0.270 | 3.03  |
| 23)      | Atrazine              | 0.199          | 0.207 | 0.211 | 0.213 | 0.237 | 0.234 | 0.242 | 0.220 | 7.64  |
| 24)      | Pentachlorophenol     | 0.133          | 0.134 | 0.141 | 0.137 | 0.159 | 0.162 | 0.177 | 0.149 | 11.45 |
| 25)      | Phenanthrene          | 1.259          | 1.272 | 1.292 | 1.263 | 1.367 | 1.337 | 1.361 | 1.307 | 3.56  |
| 26)      | Anthracene            | 1.099          | 1.104 | 1.166 | 1.130 | 1.269 | 1.259 | 1.300 | 1.190 | 7.13  |
| 27) SURR | Fluoranthene-d10      | 1.033          | 1.033 | 1.078 | 1.042 | 1.153 | 1.161 | 1.178 | 1.097 | 5.95  |
| 28)      | Fluoranthene          | 1.461          | 1.439 | 1.500 | 1.496 | 1.670 | 1.672 | 1.693 | 1.562 | 7.13  |
| 29) I    | Chrysene-d12          | -----ISTD----- |       |       |       |       |       |       |       |       |
| 30)      | Pyrene                | 1.744          | 1.708 | 1.727 | 1.656 | 1.790 | 1.641 | 1.711 | 1.711 | 2.96  |
| 31) S    | Terphenyl-d14         | 0.897          | 0.844 | 0.871 | 0.822 | 0.891 | 0.816 | 0.848 | 0.856 | 3.73  |
| 32)      | Benzo(a)anthra...     | 1.463          | 1.432 | 1.485 | 1.438 | 1.594 | 1.521 | 1.609 | 1.506 | 4.77  |
| 33)      | Chrysene              | 1.655          | 1.559 | 1.616 | 1.532 | 1.653 | 1.560 | 1.576 | 1.593 | 3.05  |
| 34)      | Bis(2-ethylhex...     | 0.955          | 0.919 | 0.906 | 0.855 | 0.941 | 0.903 | 1.011 | 0.927 | 5.27  |
| 35) I    | Perylene-d12          | -----ISTD----- |       |       |       |       |       |       |       |       |

Method Path : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\


Method File : 8270-SIM-BN051425.M

|       |                   |       |       |       |       |       |       |       |       |      |
|-------|-------------------|-------|-------|-------|-------|-------|-------|-------|-------|------|
| 36)   | Indeno(1,2,3-c... | 1.511 | 1.613 | 1.645 | 1.568 | 1.687 | 1.732 | 1.680 | 1.634 | 4.65 |
| 37)   | Benzo(b)fluora... | 1.631 | 1.570 | 1.602 | 1.599 | 1.749 | 1.698 | 1.765 | 1.659 | 4.71 |
| 38)   | Benzo(k)fluora... | 1.539 | 1.538 | 1.642 | 1.601 | 1.770 | 1.661 | 1.719 | 1.639 | 5.34 |
| 39) C | Benzo(a)pyrene    | 1.380 | 1.343 | 1.381 | 1.331 | 1.486 | 1.444 | 1.486 | 1.407 | 4.59 |
| 40)   | Dibenzo(a,h)an... | 1.116 | 1.232 | 1.273 | 1.237 | 1.340 | 1.376 | 1.334 | 1.272 | 6.90 |
| 41)   | Benzo(g,h,i)pe... | 1.299 | 1.407 | 1.424 | 1.330 | 1.403 | 1.439 | 1.376 | 1.383 | 3.72 |

-----  
(#) = Out of Range

# 4,6-Dinitro-2-methylphenol

Response Ratio

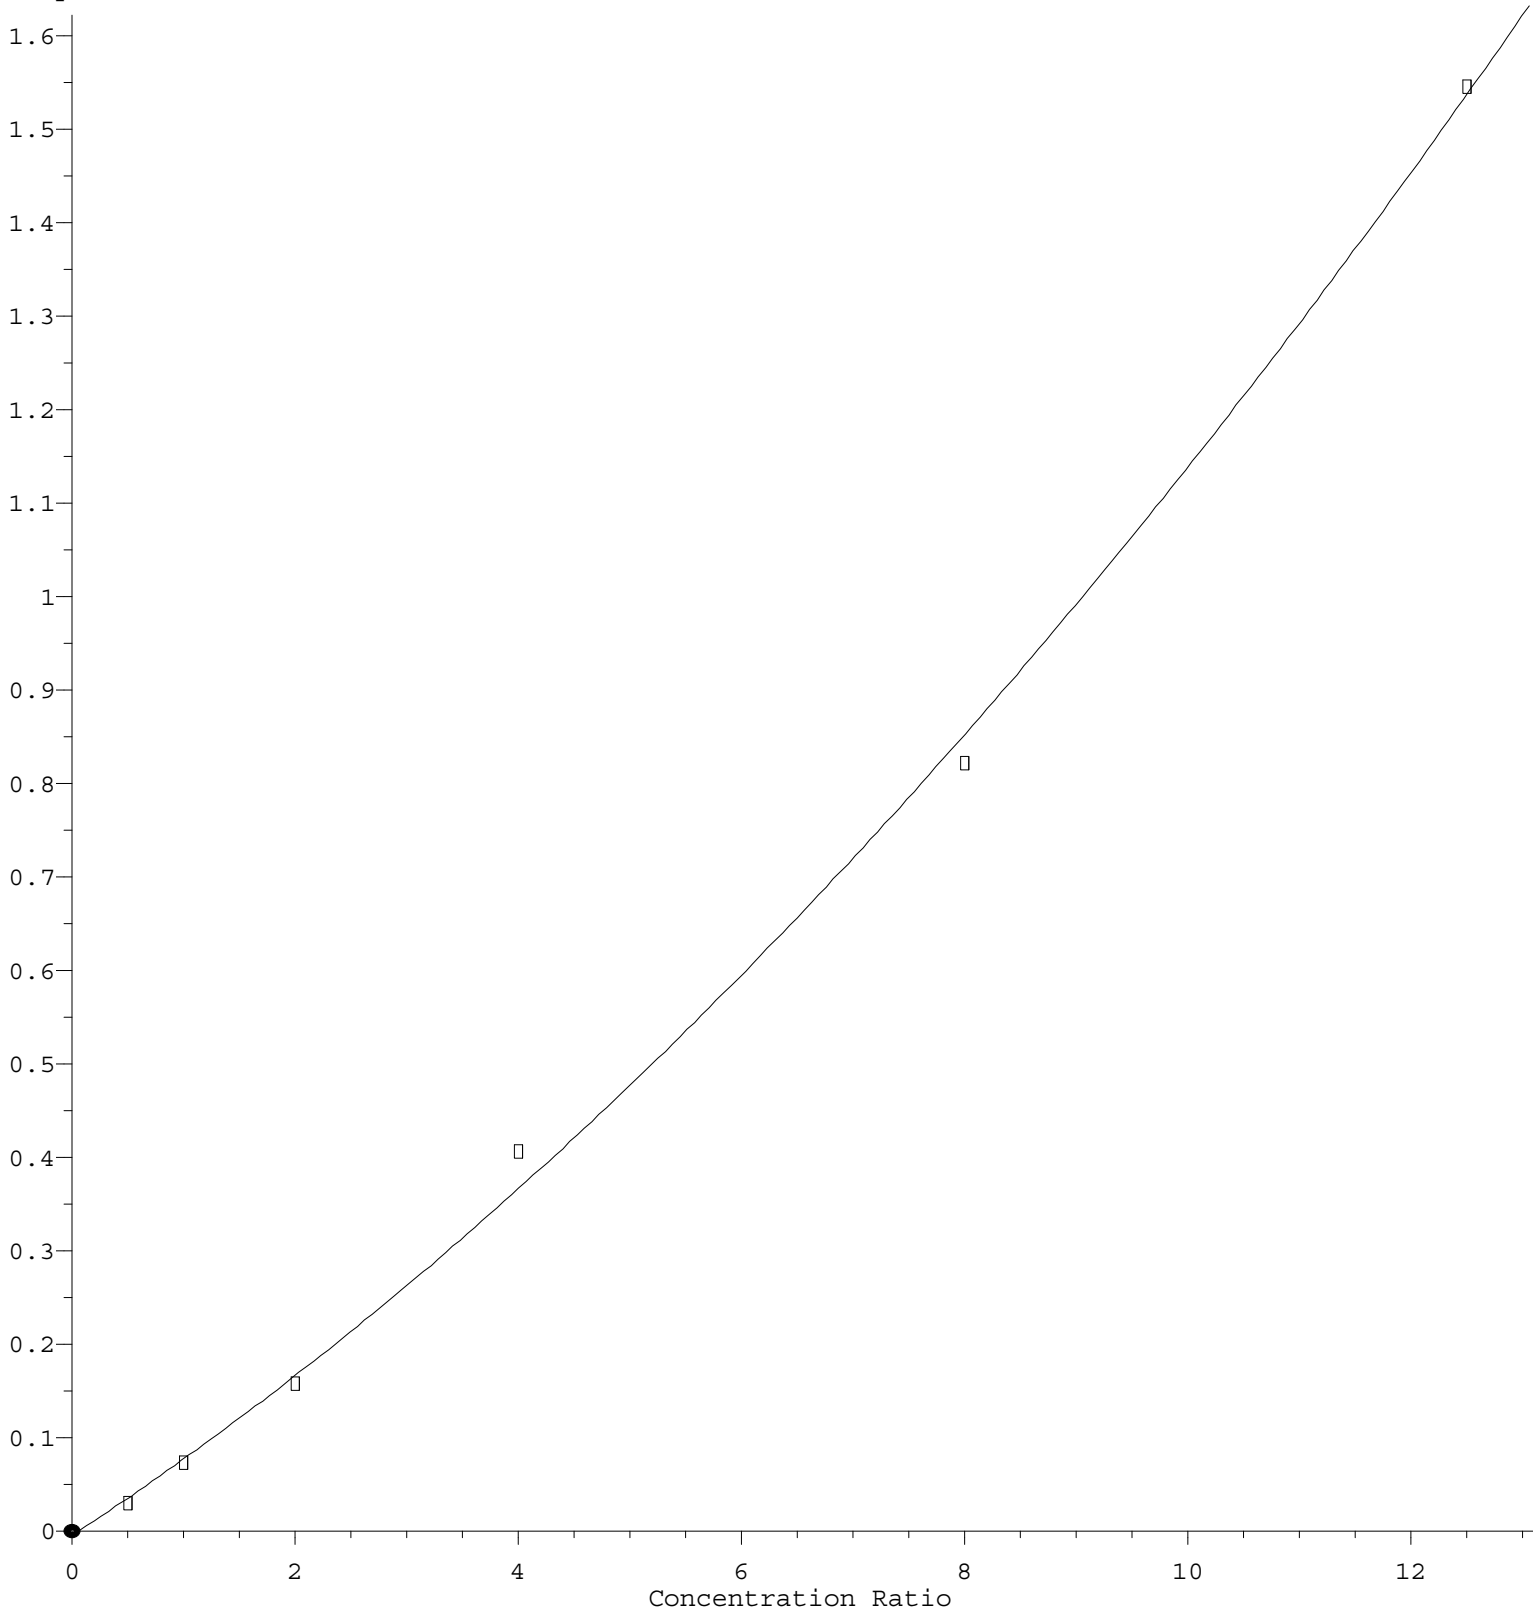

$R = 3.599e-003 A^2 + 7.833e-002 A - 4.644e-003$   
 Coef of Det ( $r^2$ ) = 0.998418    Curve Fit: Quadratic  
 Method Name: Z:\svoasrv\HPCHEM1\BNA N\Methods\8270-SIM-BN051425.M  
 Calibration Table Last Updated: Wed May 14 11:26:32 2025