
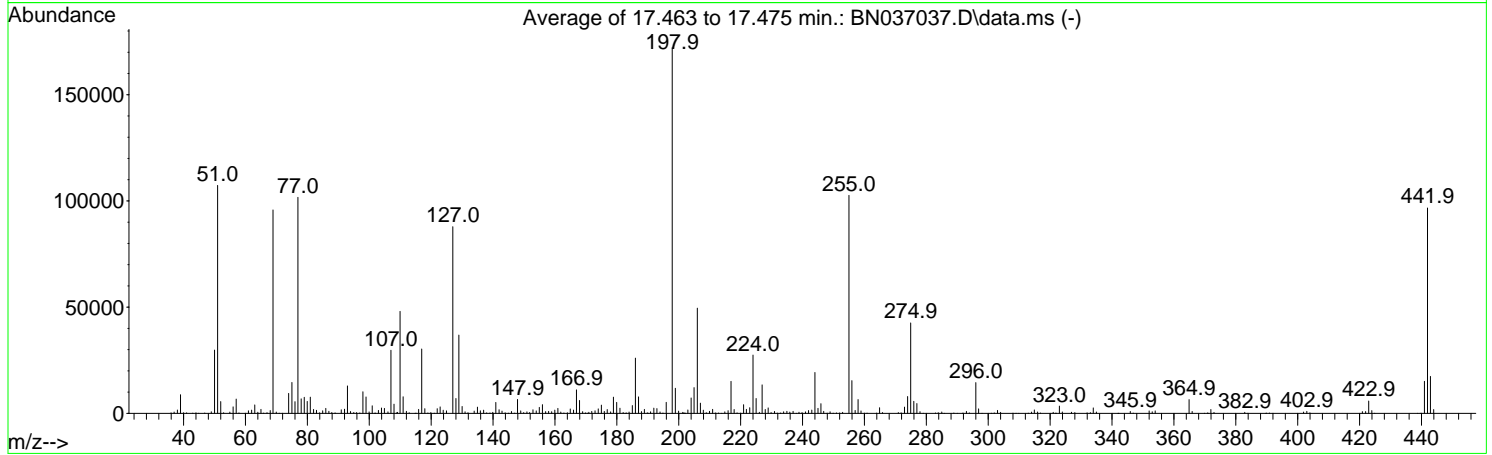


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051925\
 Data File : BN037037.D
 Acq On : 19 May 2025 10:08
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051425.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 14 11:26:32 2025

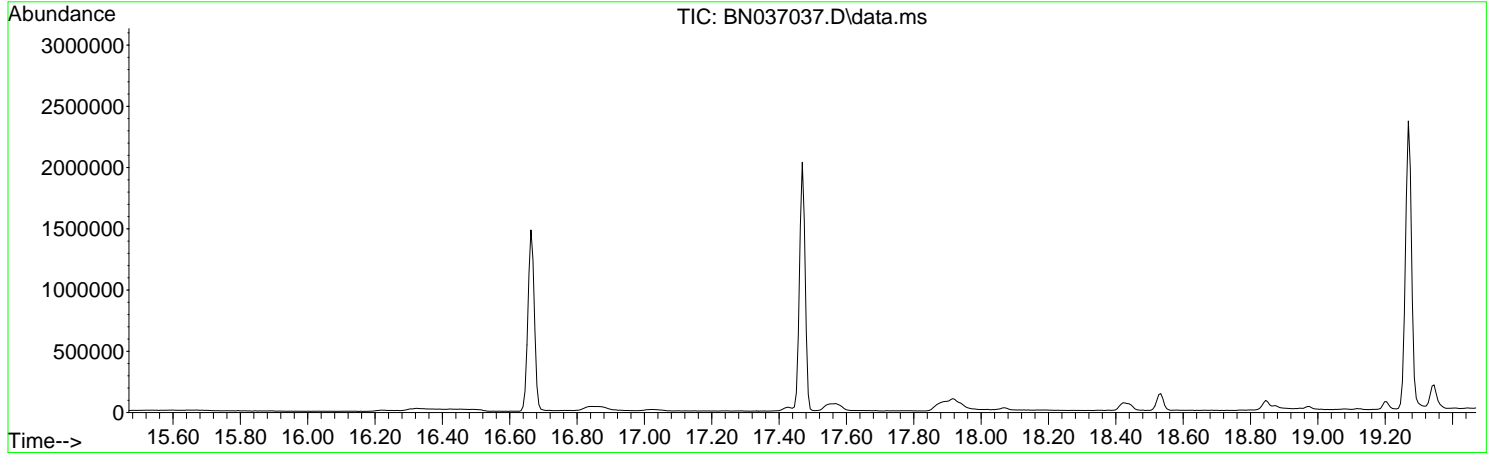




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result
51	198	10	80	62.3	107312	PASS
68	69	0.00	2	1.4	1334	PASS
69	198	0.00	100	55.6	95774	PASS
70	69	0.00	2	0.7	629	PASS
127	198	10	80	51.1	87883	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	172139	PASS
199	198	5	9	6.9	11809	PASS
275	198	10	60	24.7	42579	PASS
365	198	1	100	3.8	6488	PASS
441	198	0.01	100	8.8	15091	PASS
442	442	50	100	100.0	96701	PASS
443	442	15	24	18.0	17401	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051925\
 Data File : BN037037.D
 Acq On : 19 May 2025 10:08
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 DFTPP

Quant Time: May 19 20:15:09 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 16 02:43:29 2025
 Response via : Initial Calibration

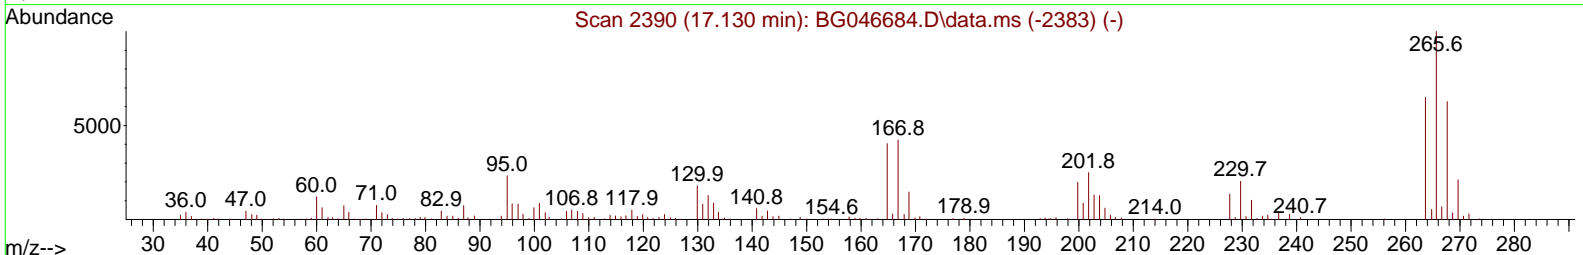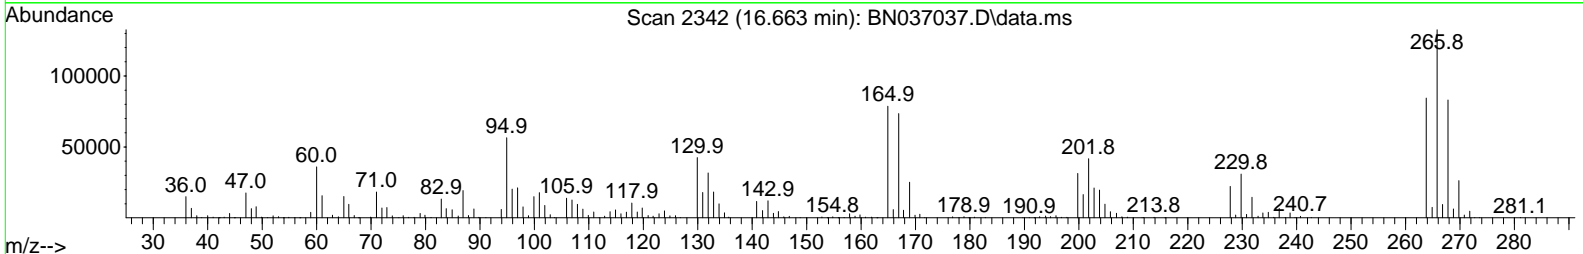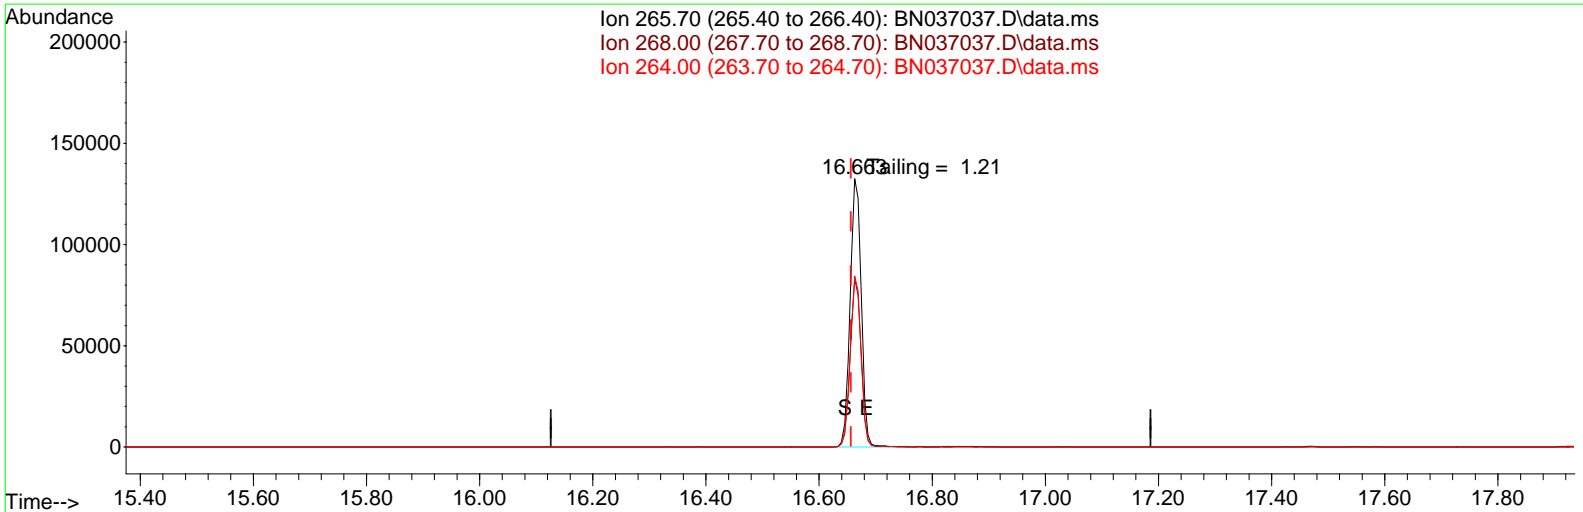

TIC: BN037037.D\data.ms

(70) Pentachlorophenol (C)

16.663min (+ 0.007) 18901.49 ng




response 181116

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.64
264.00	61.60	63.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051925\
 Data File : BN037037.D
 Acq On : 19 May 2025 10:08
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 19 20:15:09 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 16 02:43:29 2025
 Response via : Initial Calibration

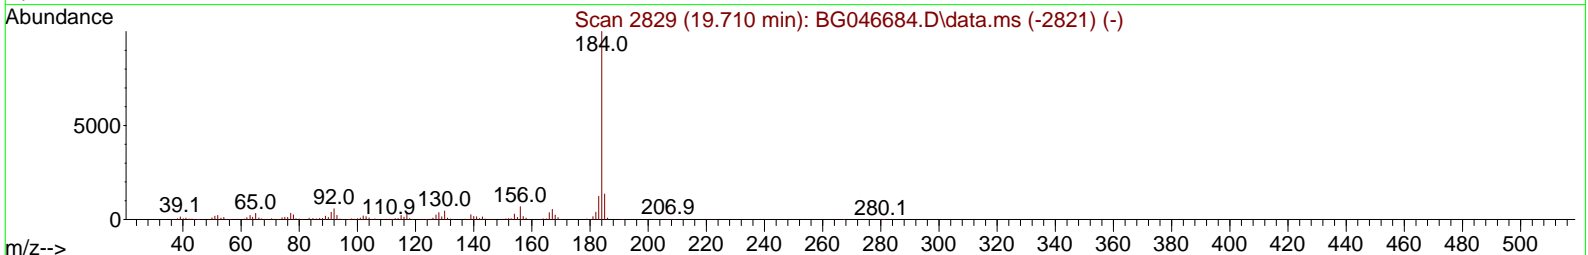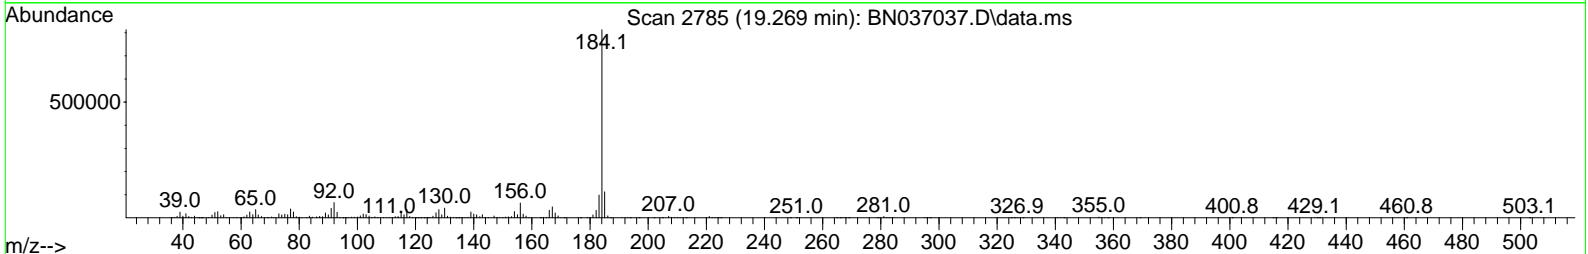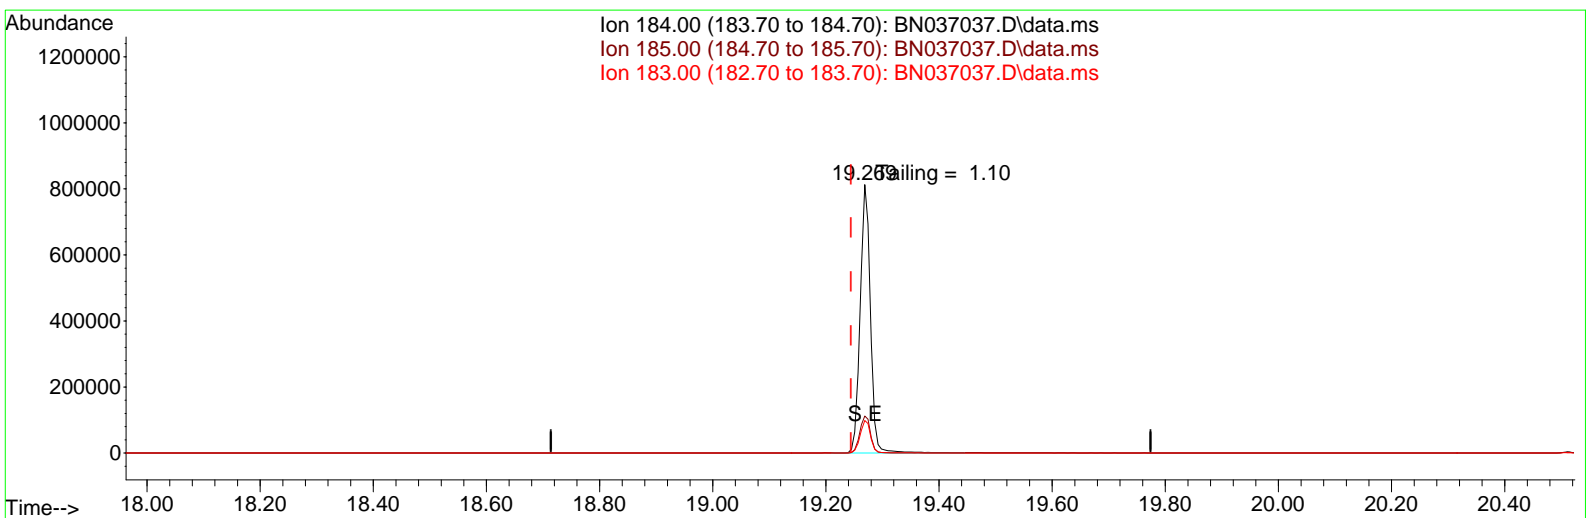

TIC: BN037037.D\data.ms

(77) Benzidine

19.269min (+ 0.025) 0.00 ng

response 1031617

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.80
183.00	13.20	12.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/19/2025	BNA_N	<u>BN037037.D</u>
Compound Name	Response	Retention Time
DDT	563666	20.51
DDD	17637	20.069
DDE	881	19.557
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18518	582184	3.18

Instrument :
 BNA_N
 Client:Sampled :
 DFTPP