
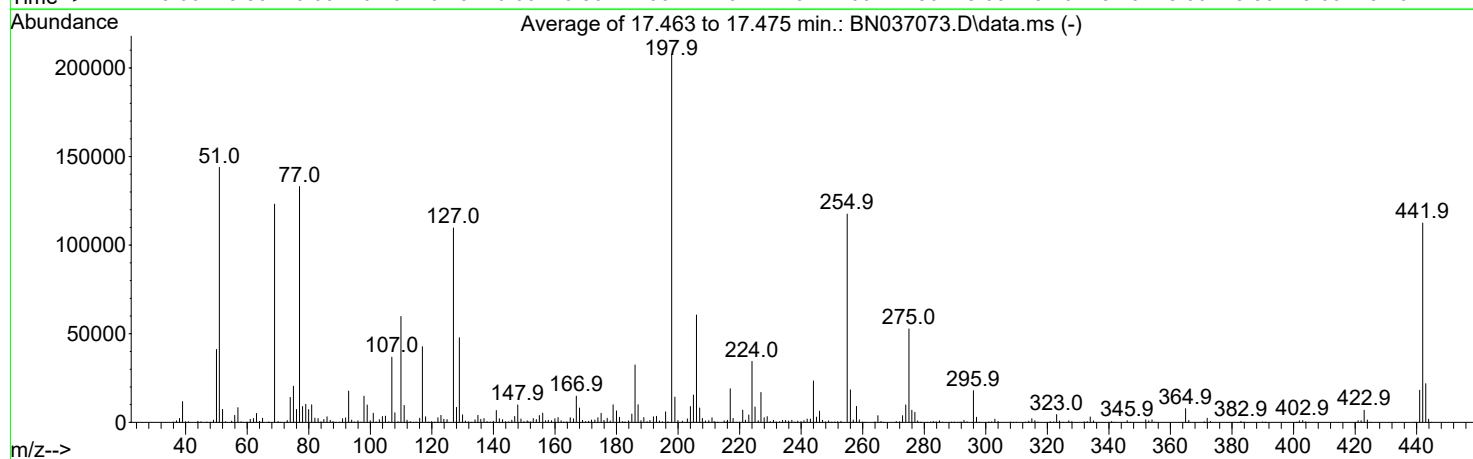


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052125\
Data File : BN037073.D
Acq On : 20 May 2025 14:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 14 11:26:32 2025

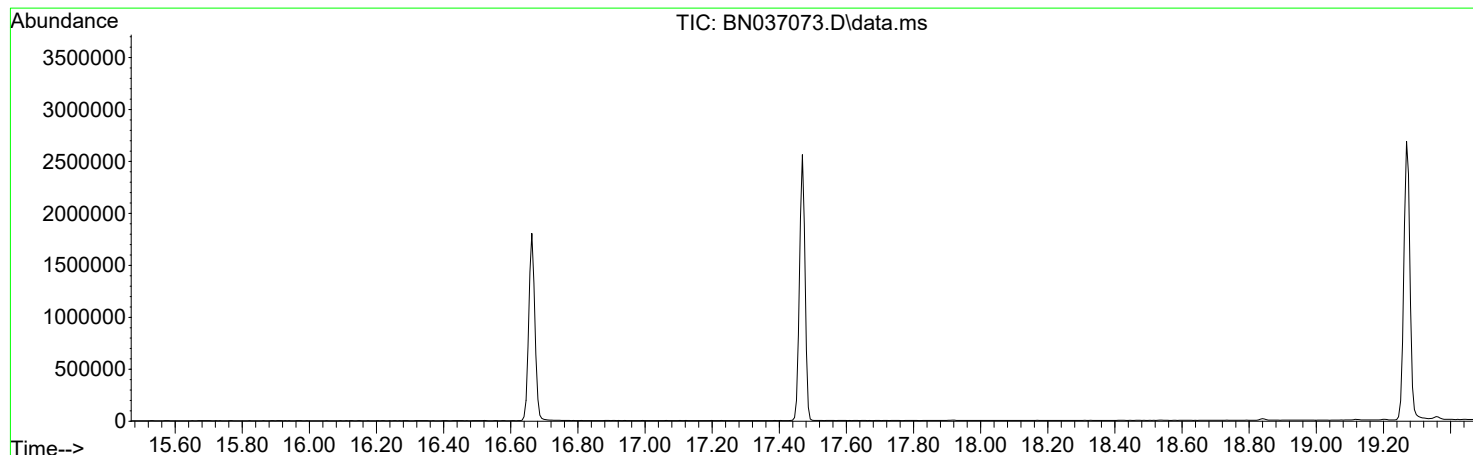

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	69.3	143915	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	59.3	123171	PASS
70	69	0.00	2	0.4	548	PASS
127	198	10	80	52.8	109691	PASS
197	198	0.00	2	0.2	410	PASS
198	198	100	100	100.0	207573	PASS
199	198	5	9	6.9	14234	PASS
275	198	10	60	25.4	52744	PASS
365	198	1	100	3.7	7760	PASS
441	198	0.01	100	8.8	18185	PASS
442	442	50	100	100.0	112477	PASS
443	442	15	24	19.4	21852	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/21/2025	BNA_N	<u>BN037073.D</u>
Compound Name	Response	Retention Time
DDT	609749	20.51
DDD	18109	20.069
DDE	634	19.557
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18743	628492	2.98

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052125\
Data File : BN037073.D
Acq On : 20 May 2025 14:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 21 01:54:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 21 01:54:36 2025
Response via : Initial Calibration

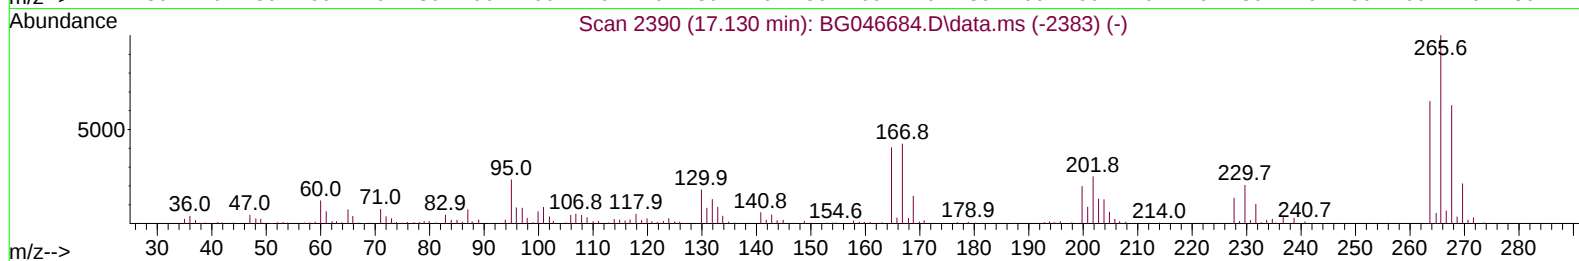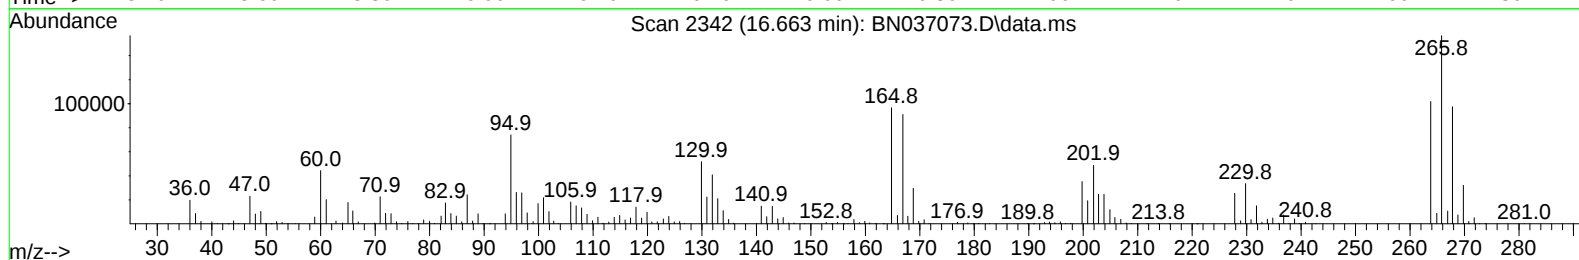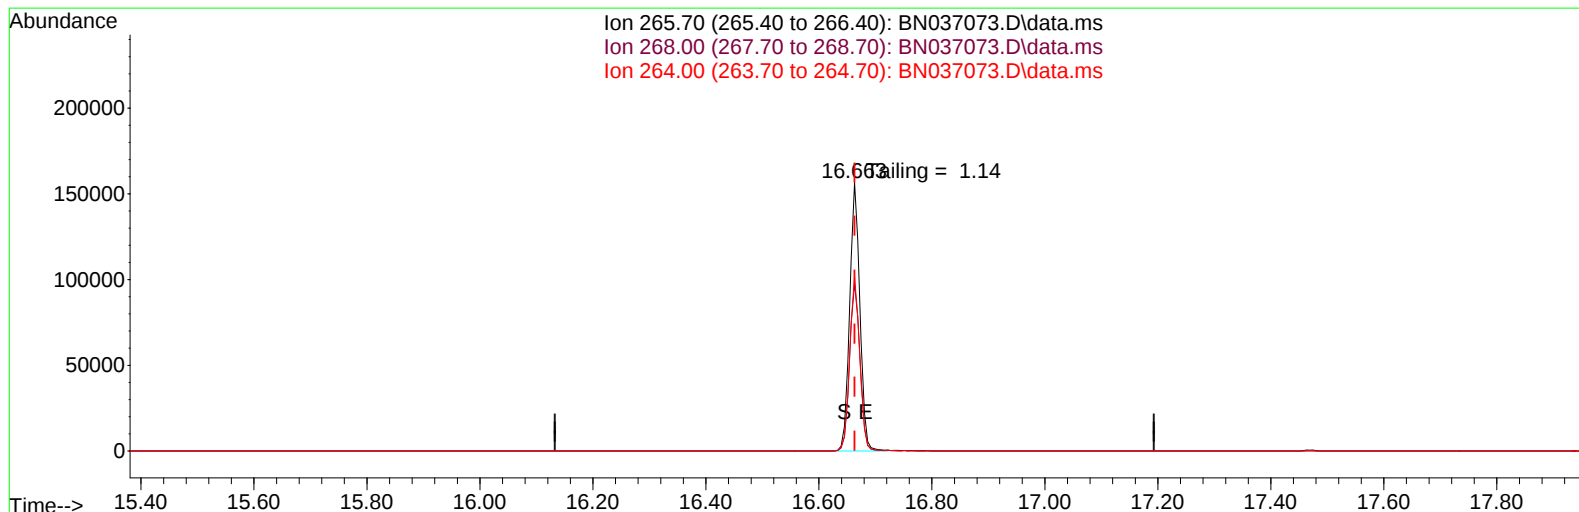

TIC: BN037073.D\data.ms

(70) Pentachlorophenol (C)

16.663min (0.000) 18354.59 ng




response 197914

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.23
264.00	61.60	65.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052125\
Data File : BN037073.D
Acq On : 20 May 2025 14:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 21 01:54:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 21 01:54:36 2025
Response via : Initial Calibration

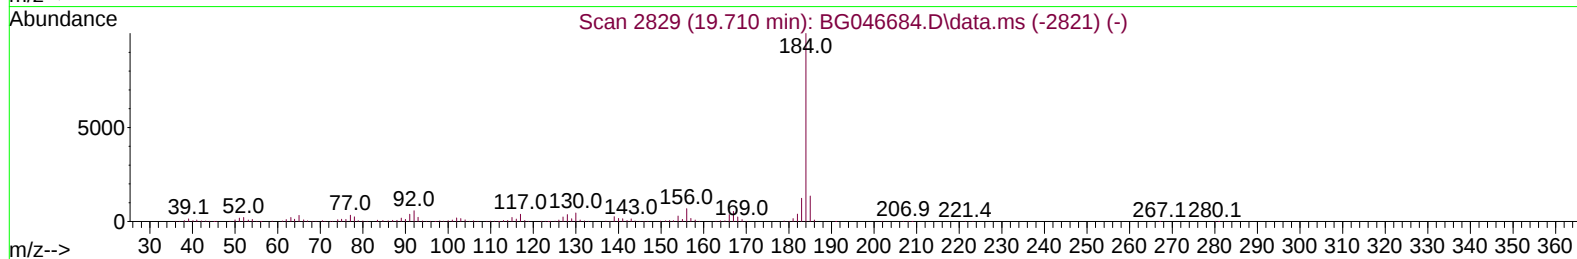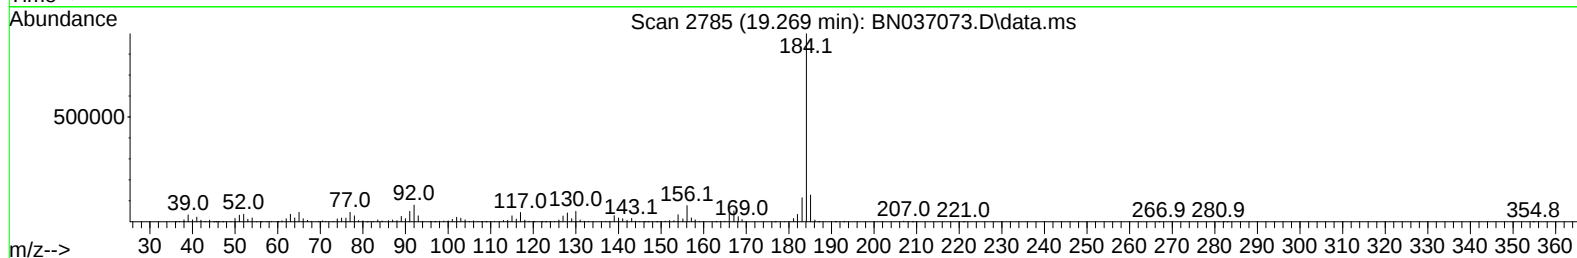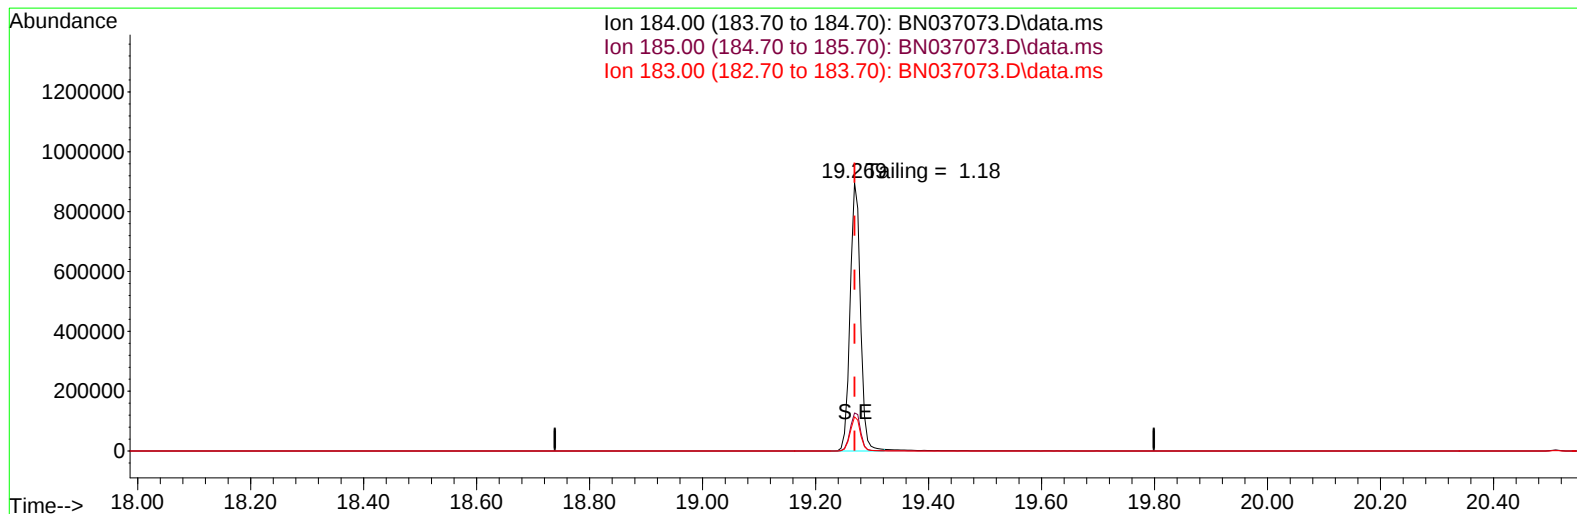

TIC: BN037073.D\data.ms

(77) Benzidine

19.269min (0.000) 0.00 ng

response 1157281

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.21
183.00	13.20	12.75
0.00	0.00	0.00