
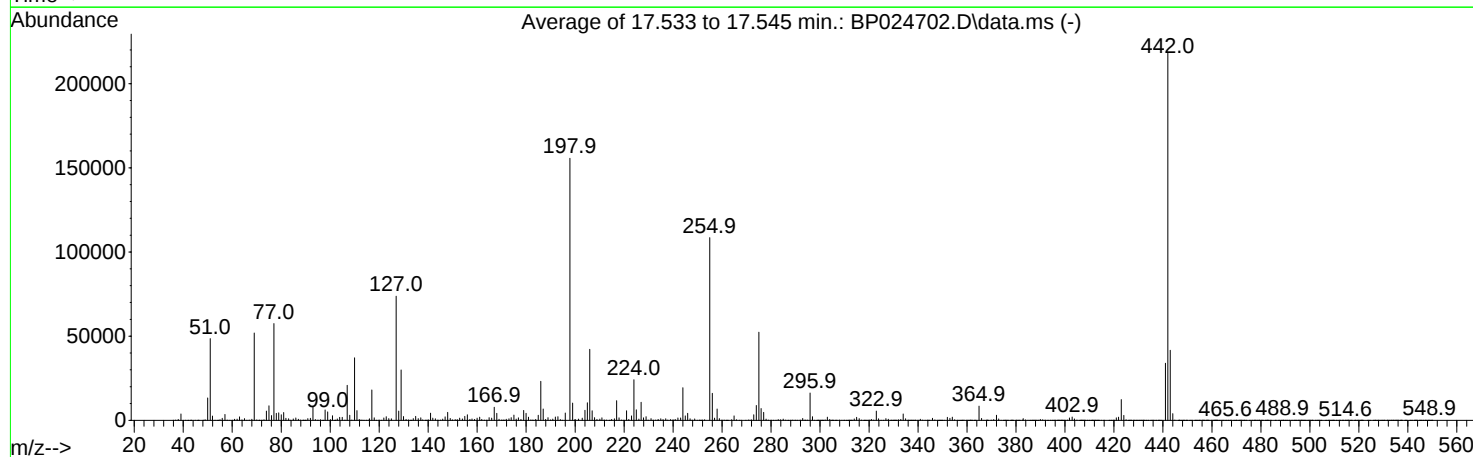


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024702.D
Acq On : 20 May 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 13 16:21:39 2025

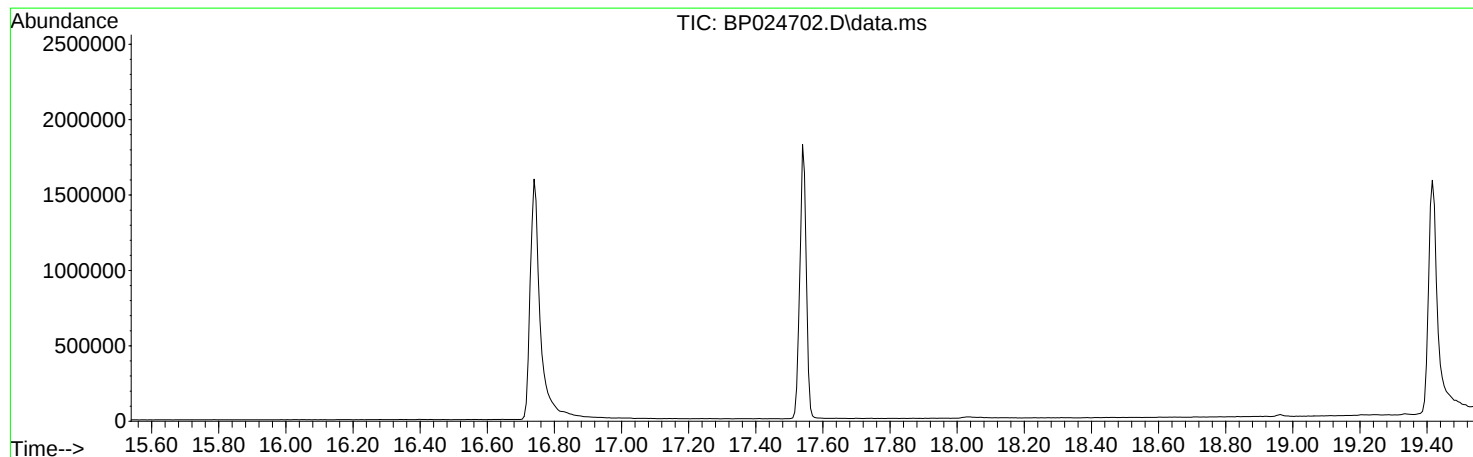




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	48558	PASS
68	69	0.00	2	1.3	692	PASS
69	198	0.00	100	33.3	51898	PASS
70	69	0.00	2	0.6	286	PASS
127	198	10	80	47.4	73724	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	155659	PASS
199	198	5	9	6.6	10281	PASS
275	198	10	60	33.6	52370	PASS
365	198	1	100	5.4	8455	PASS
441	198	0.01	100	21.8	33949	PASS
442	442	100	100	100.0	218491	PASS
443	442	15	24	19.0	41616	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024702.D
Acq On : 20 May 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 20 12:58:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

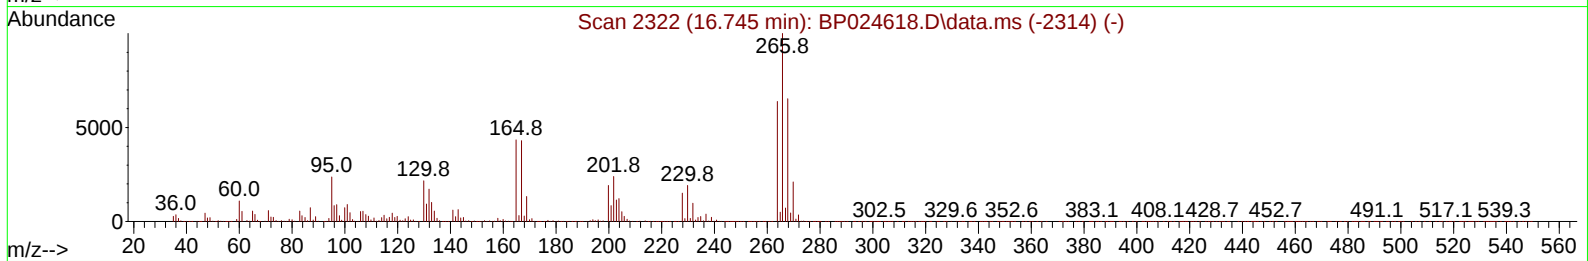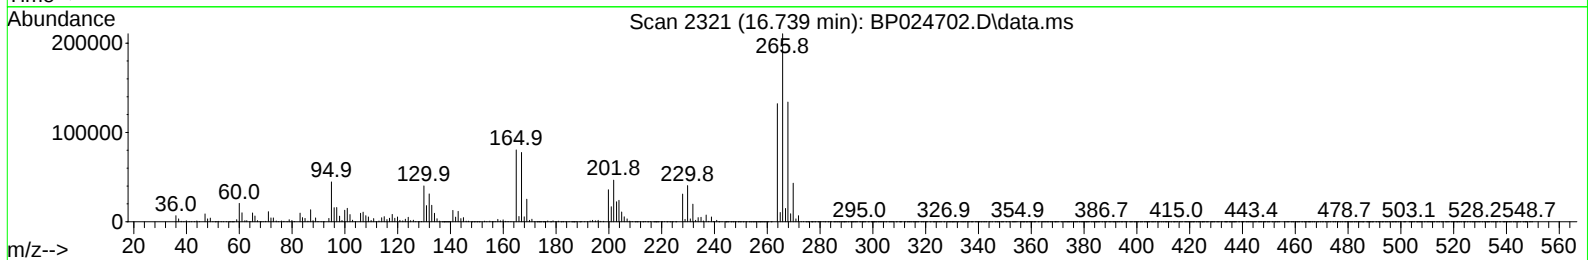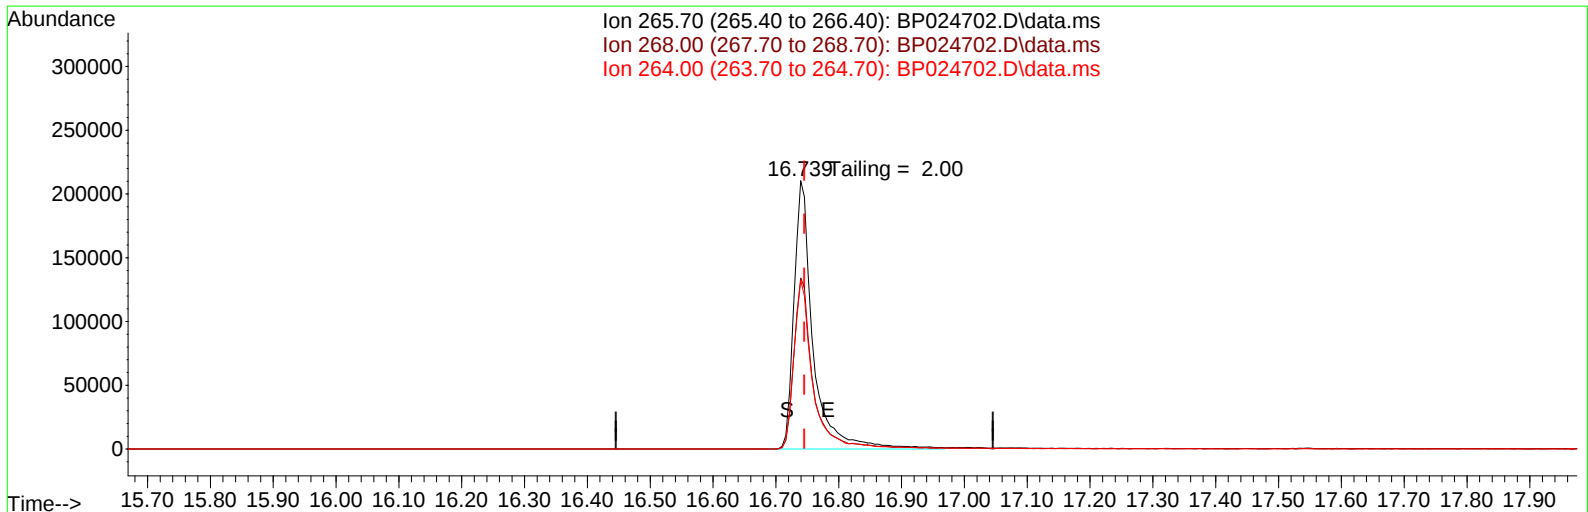

TIC: BP024702.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.006) 1977139.32 ng




response 448686

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.67
264.00	63.90	62.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052025\
Data File : BP024702.D
Acq On : 20 May 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 20 12:58:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

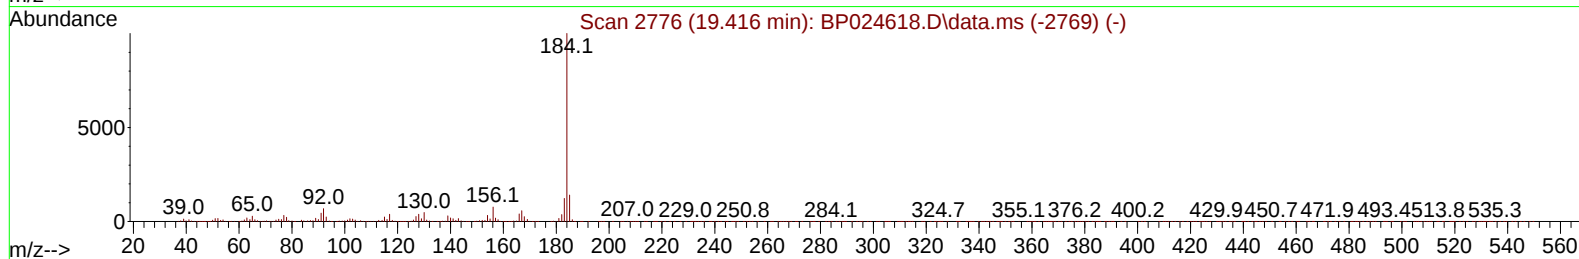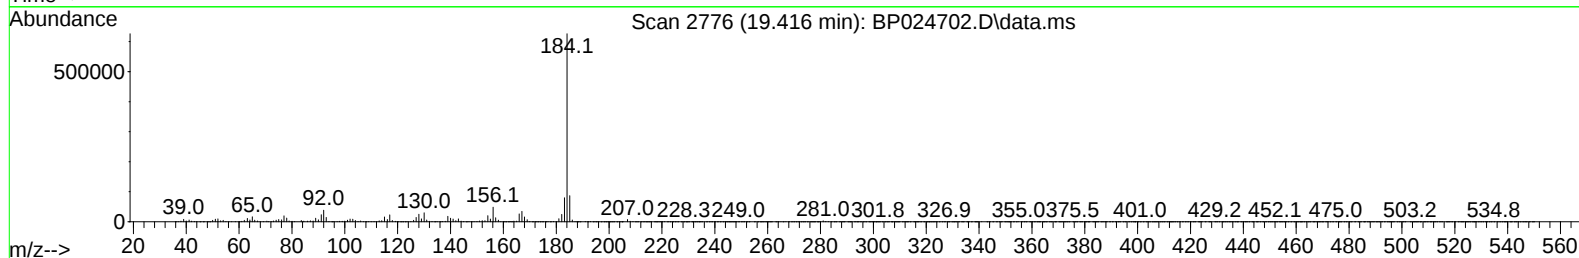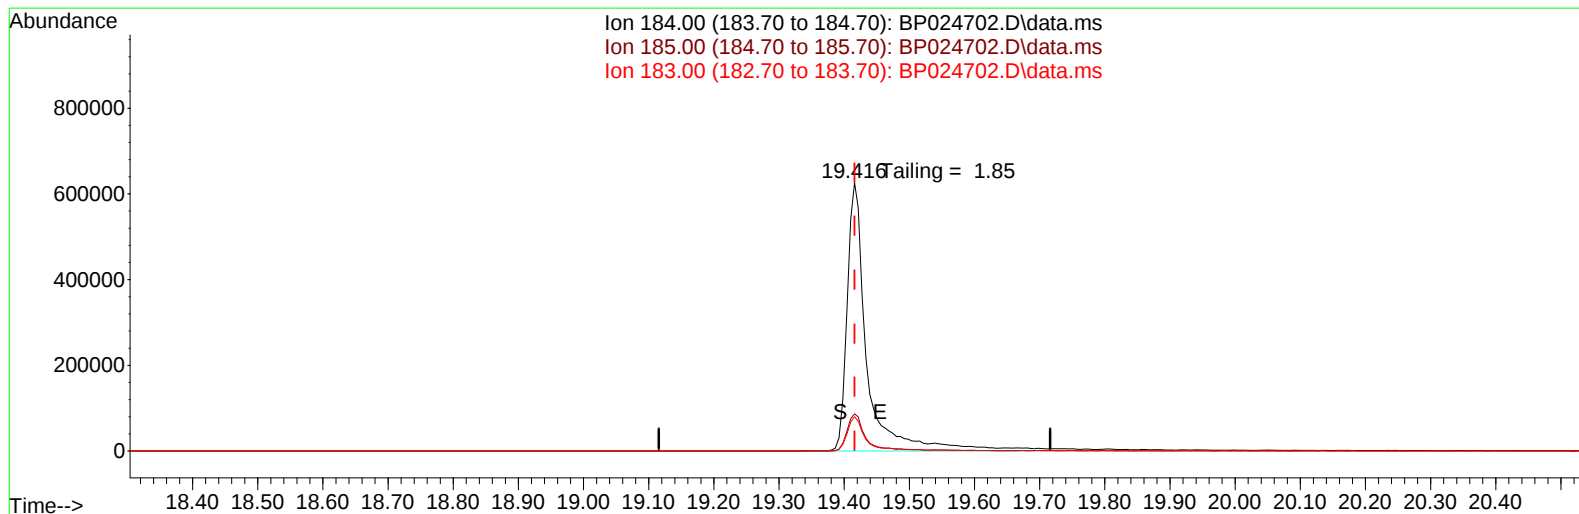

TIC: BP024702.D\data.ms

(77) Benzidine

19.416min (-0.000) 89911.52 ng

response 1248901

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.86
183.00	12.30	12.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/20/2025	BNA_P	<u>BP024702.D</u>
Compound Name	Response	Retention Time
DDT	589251	20.698
DDD	22194	20.239
DDE	3176	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25370	614621	4.13

Instrument :
BNA_P
ClientSampleId :
DFTPP