

Method Path : Z:\svoasrv\HPCHEM1\BNA_N\Methods\
 Method File : 8270-SIM-BN051425.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 14 11:26:32 2025
 Response Via : Initial Calibration

Calibration Files

0.1 =BN036999.D 0.2 =BN037000.D 0.4 =BN037001.D 0.8 =BN037002.D 1.6 =BN037003.D 3.2 =BN037004.D 5.0 =BN037005.D

Compound	0.1	0.2	0.4	0.8	1.6	3.2	5.0	Avg	%RSD

1) I 1,4-Dichlorobenzen...	-----ISTD-----								
2) 1,4-Dioxane	0.510	0.512	0.487	0.514	0.467	0.454	0.491		5.25
3) n-Nitrosodimet...	1.465	0.974	0.980	0.971	1.075	0.967	0.950	1.054	17.59
4) S 2-Fluorophenol	1.101	1.134	1.024	1.093	0.964	0.971	1.048		6.87
5) S Phenol-d6	1.304	1.385	1.236	1.392	1.259	1.292	1.311		4.91
6) bis(2-Chloroet...	1.441	1.163	1.153	1.135	1.240	1.168	1.148	1.207	9.02

7) I Naphthalene-d8	-----ISTD-----								
8) S Nitrobenzene-d5	0.546	0.383	0.398	0.400	0.452	0.426	0.442	0.436	12.60
9) Naphthalene	1.326	1.140	1.144	1.122	1.226	1.152	1.165	1.182	6.05
10) Hexachlorobuta...	0.286	0.248	0.244	0.235	0.256	0.236	0.233	0.248	7.47
11) SURR2-Methylnaphth...	0.529	0.547	0.552	0.548	0.603	0.574	0.588	0.563	4.65
12) 2-Methylnaphth...	0.754	0.724	0.736	0.733	0.814	0.770	0.790	0.760	4.34

13) I Acenaphthene-d10	-----ISTD-----								
14) S 2,4,6-Tribromo...	0.174	0.168	0.178	0.160	0.186	0.175	0.189	0.176	5.77
15) S 2-Fluorobiphenyl	1.912	1.801	1.901	1.802	1.927	1.672	1.807	1.832	4.90
16) Acenaphthylene	1.906	1.838	1.894	1.849	2.071	1.997	2.075	1.947	5.14
17) Acenaphthene	1.255	1.229	1.243	1.217	1.350	1.298	1.315	1.272	3.89
18) Fluorene	1.602	1.581	1.635	1.611	1.779	1.721	1.752	1.669	4.80

19) I Phenanthrene-d10	-----ISTD-----								
20) 4,6-Dinitro-2-...	0.060	0.073	0.079	0.102	0.103	0.124	0.090		26.02
21) 4-Bromophenyl-...	0.243	0.246	0.250	0.247	0.262	0.261	0.259	0.253	3.13
22) Hexachlorobenzene	0.267	0.269	0.281	0.259	0.281	0.270	0.267	0.270	3.03
23) Atrazine	0.199	0.207	0.211	0.213	0.237	0.234	0.242	0.220	7.64
24) Pentachlorophenol	0.133	0.134	0.141	0.137	0.159	0.162	0.177	0.149	11.45
25) Phenanthrene	1.259	1.272	1.292	1.263	1.367	1.337	1.361	1.307	3.56
26) Anthracene	1.099	1.104	1.166	1.130	1.269	1.259	1.300	1.190	7.13
27) SURRFluoranthene-d10	1.033	1.033	1.078	1.042	1.153	1.161	1.178	1.097	5.95
28) Fluoranthene	1.461	1.439	1.500	1.496	1.670	1.672	1.693	1.562	7.13

29) I Chrysene-d12	-----ISTD-----								
30) Pyrene	1.744	1.708	1.727	1.656	1.790	1.641	1.711	1.711	2.96
31) S Terphenyl-d14	0.897	0.844	0.871	0.822	0.891	0.816	0.848	0.856	3.73
32) Benzo(a)anthra...	1.463	1.432	1.485	1.438	1.594	1.521	1.609	1.506	4.77
33) Chrysene	1.655	1.559	1.616	1.532	1.653	1.560	1.576	1.593	3.05
34) Bis(2-ethylhex...	0.955	0.919	0.906	0.855	0.941	0.903	1.011	0.927	5.27

35) I Perylene-d12	-----ISTD-----								


Method Path : Z:\svoasrv\HPCHEM1\BNA_N\Methods\
Method File : 8270-SIM-BN051425.M

36)	Indeno(1,2,3-c...	1.511	1.613	1.645	1.568	1.687	1.732	1.680	1.634	4.65
37)	Benzo(b)fluora...	1.631	1.570	1.602	1.599	1.749	1.698	1.765	1.659	4.71
38)	Benzo(k)fluora...	1.539	1.538	1.642	1.601	1.770	1.661	1.719	1.639	5.34
39) C	Benzo(a)pyrene	1.380	1.343	1.381	1.331	1.486	1.444	1.486	1.407	4.59
40)	Dibenzo(a,h)an...	1.116	1.232	1.273	1.237	1.340	1.376	1.334	1.272	6.90
41)	Benzo(g,h,i)pe...	1.299	1.407	1.424	1.330	1.403	1.439	1.376	1.383	3.72

(#) = Out of Range

4,6-Dinitro-2-methylphenol

Response Ratio

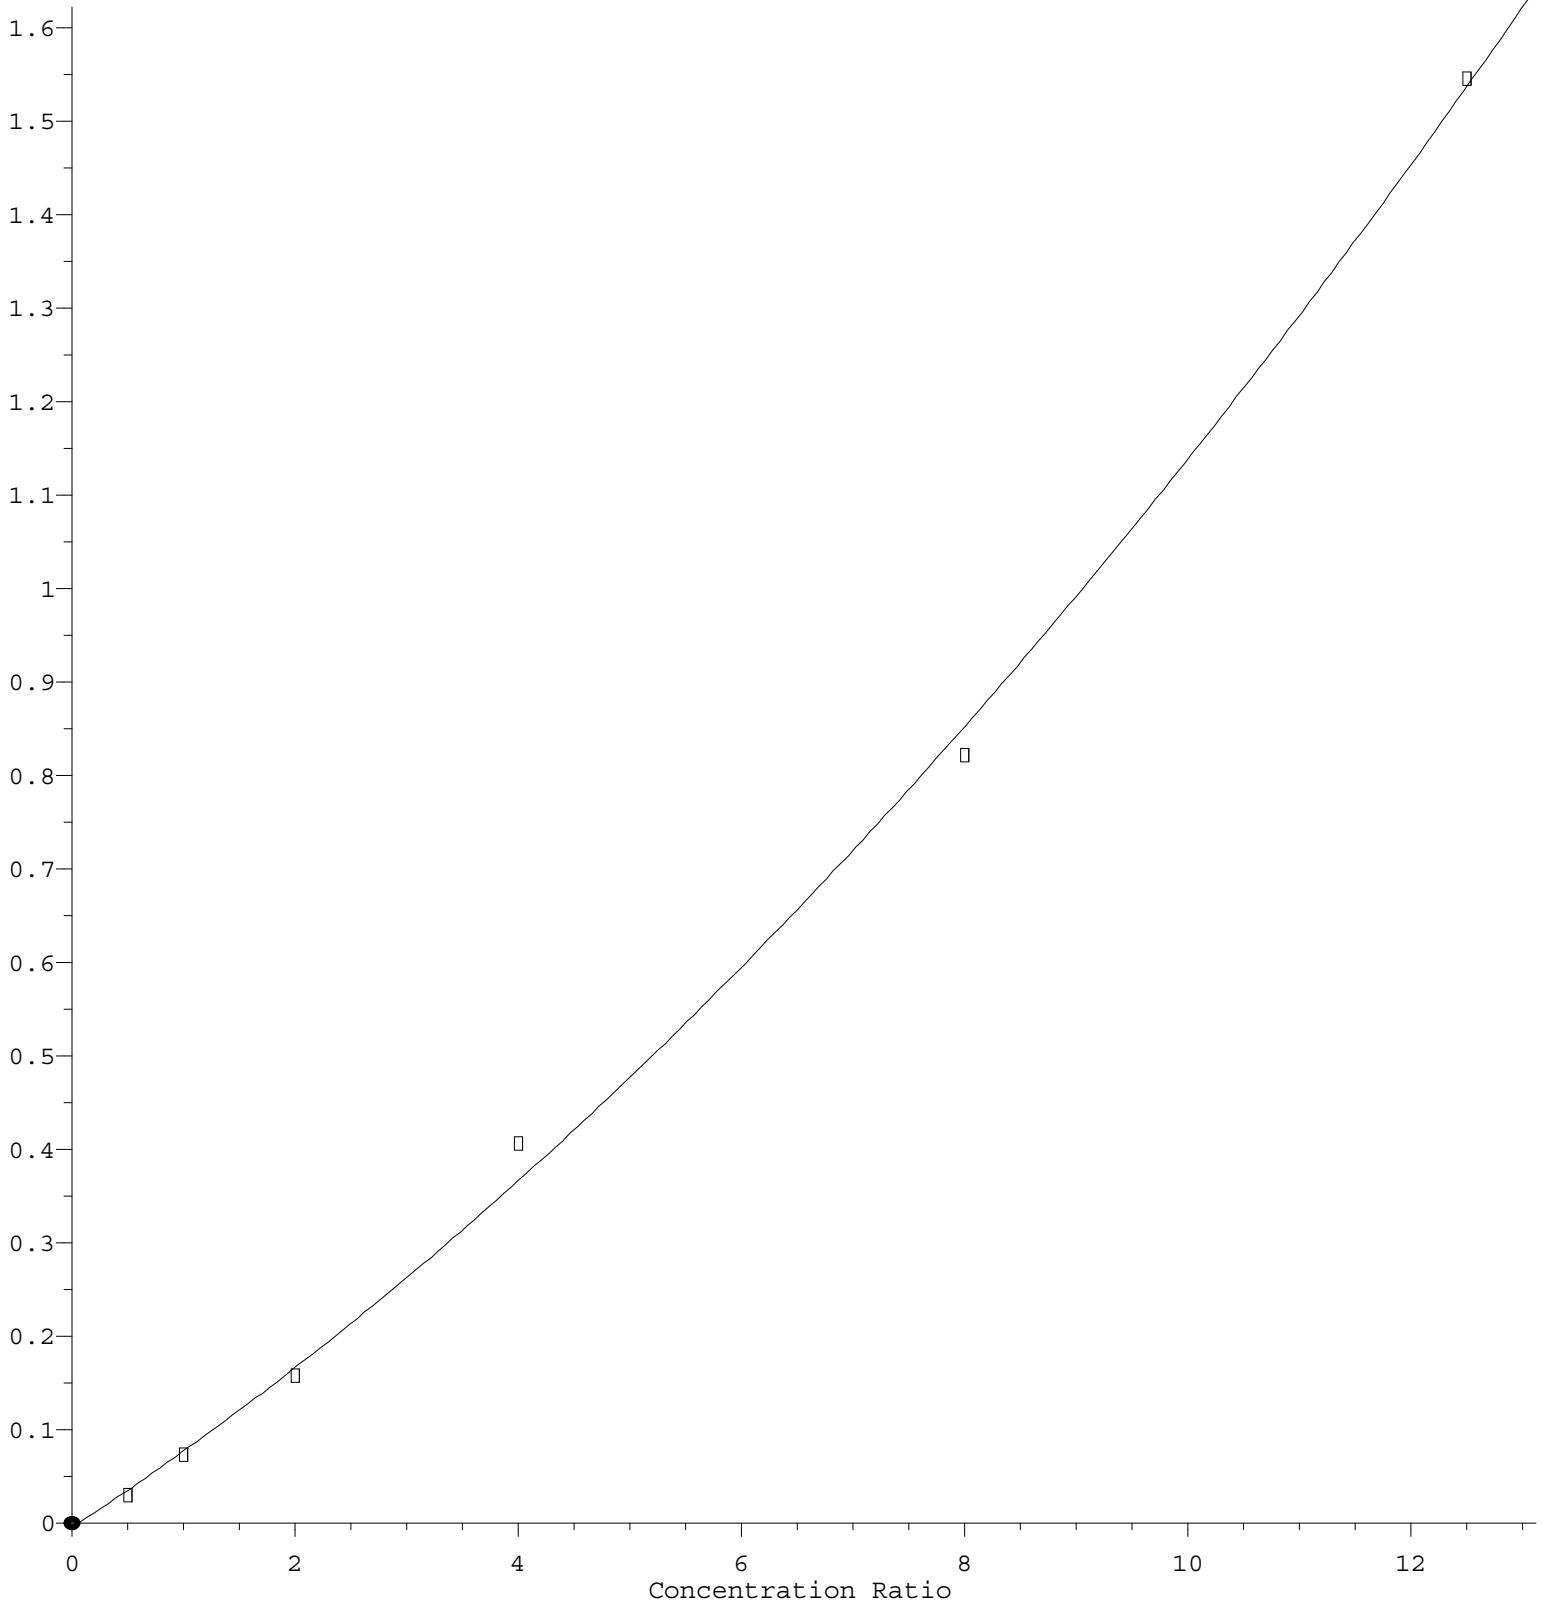

R = 3.599e-003 A*A + 7.833e-002 A - 4.644e-003
Coef of Det (r^2) = 0.998418 Curve Fit: Quadratic
Method Name: Z:\svoasrv\HPCHEM1\BNA N\Methods\8270-SIM-BN051425.M
Calibration Table Last Updated: Wed May 14 11:26:32 2025