
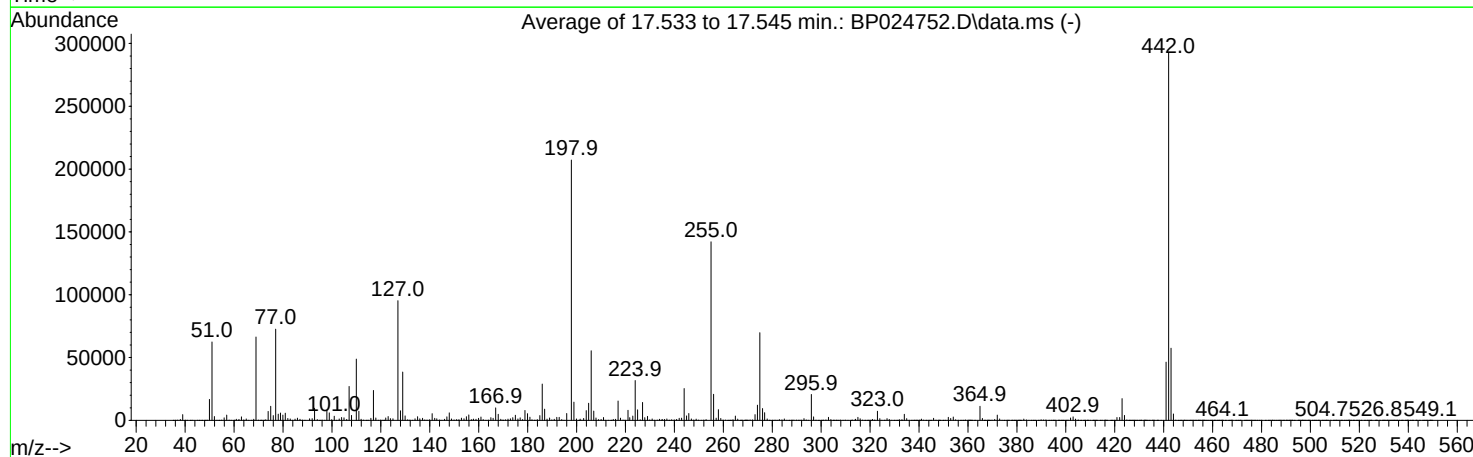


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024752.D
Acq On : 22 May 2025 09:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 13 16:21:39 2025

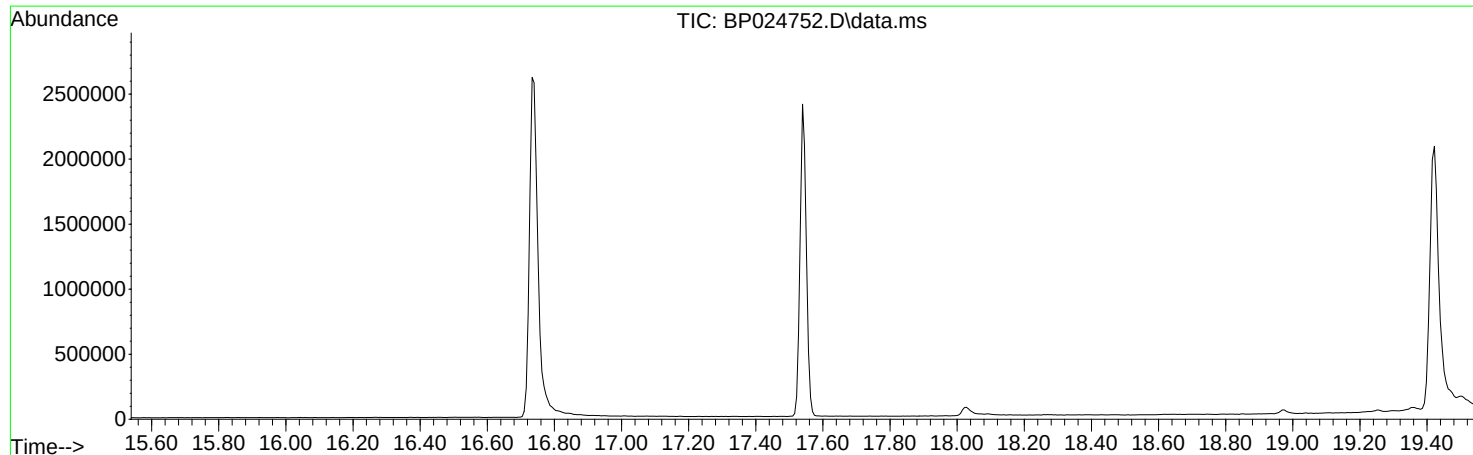




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	62396	PASS
68	69	0.00	2	1.3	886	PASS
69	198	0.00	100	32.0	66316	PASS
70	69	0.00	2	0.5	312	PASS
127	198	10	80	46.0	95339	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	207249	PASS
199	198	5	9	7.0	14476	PASS
275	198	10	60	33.7	69755	PASS
365	198	1	100	5.4	11230	PASS
441	198	0.01	100	22.4	46360	PASS
442	442	100	100	100.0	292800	PASS
443	442	15	24	19.6	57458	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024752.D
Acq On : 22 May 2025 09:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 22 11:25:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

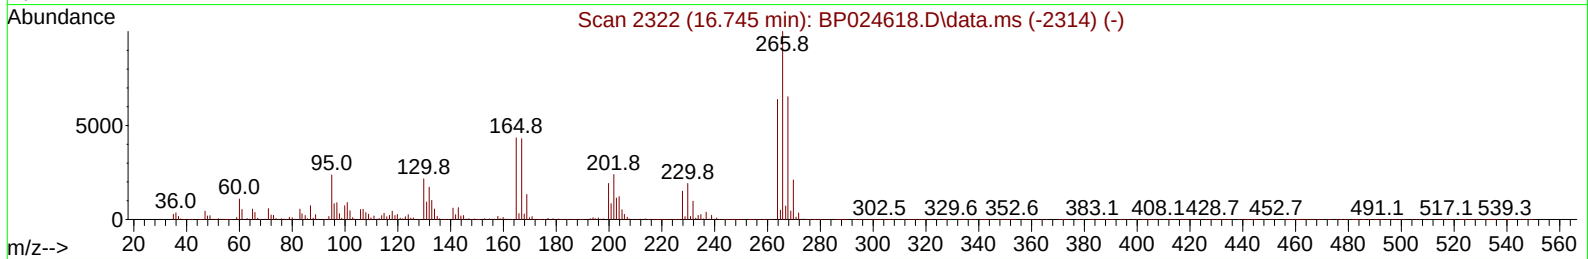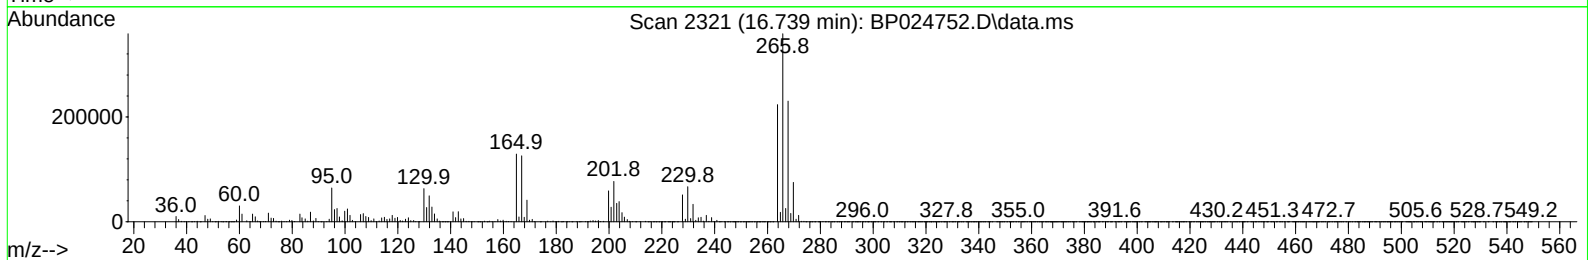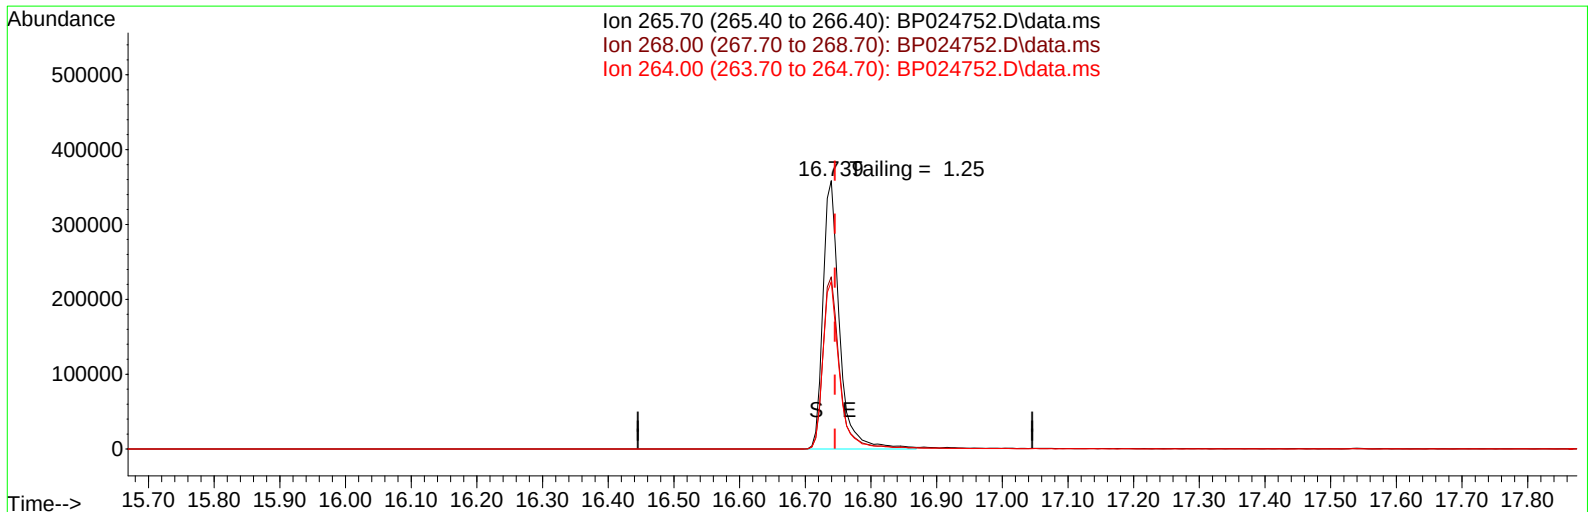

TIC: BP024752.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.006) 136502.62 ng




response 627581

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.18
264.00	63.90	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052225\
Data File : BP024752.D
Acq On : 22 May 2025 09:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 22 11:25:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

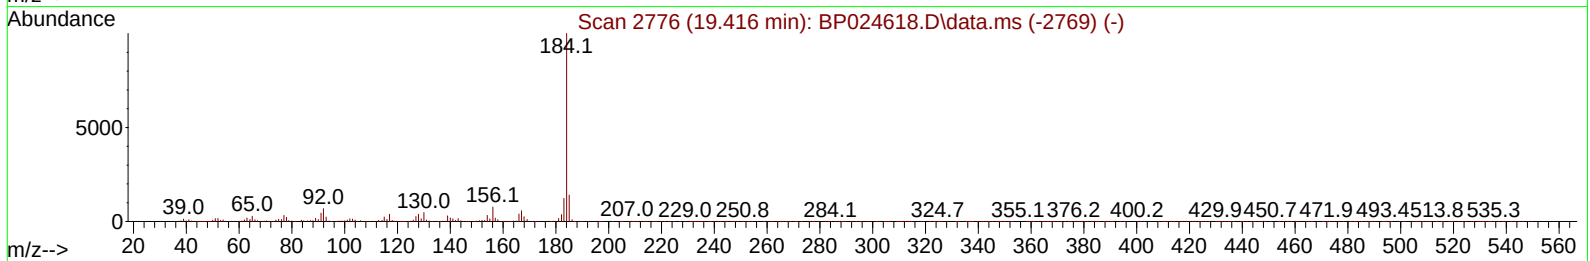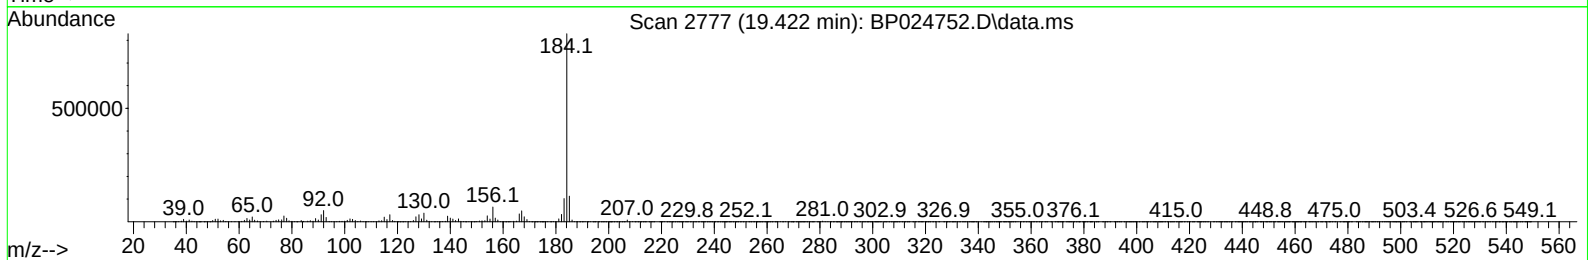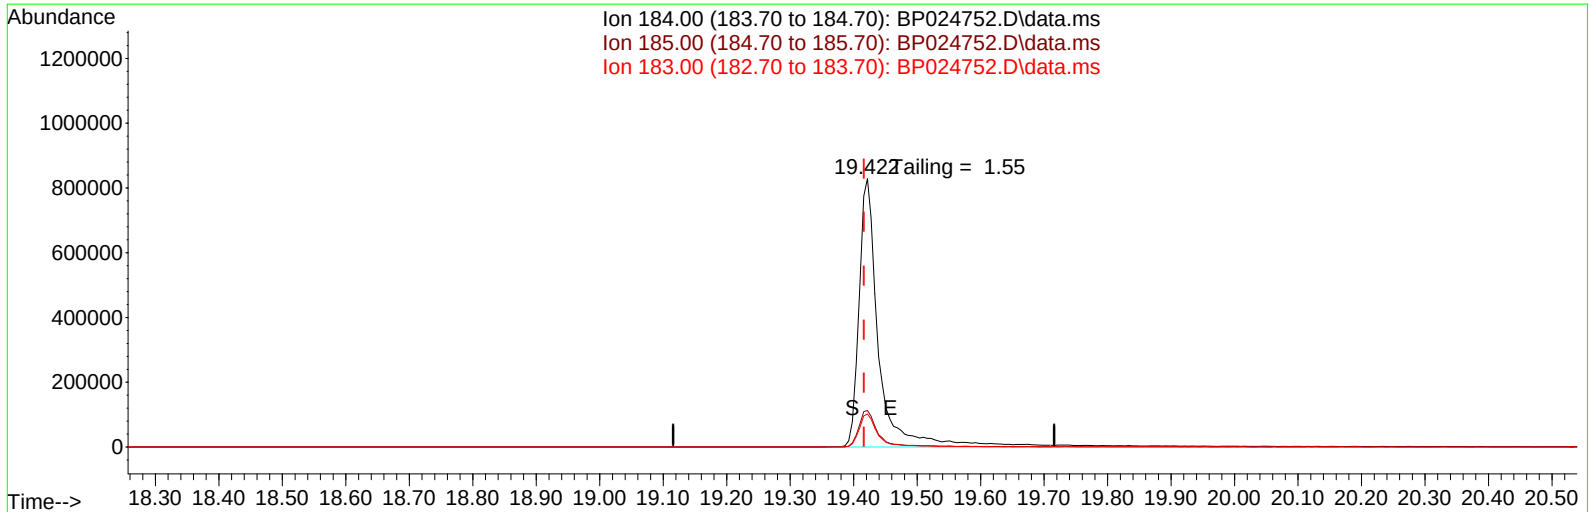

TIC: BP024752.D\data.ms

(77) Benzidine

19.422min (+ 0.006) 65290.51 ng

response 1700006

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.62
183.00	12.30	12.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/22/2025	BNA_P	<u>BP024752.D</u>
Compound Name	Response	Retention Time
DDT	762668	20.704
DDD	29290	20.239
DDE	2824	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32114	794782	4.04

Instrument :
BNA_P
ClientSampleId :
DFTPP