
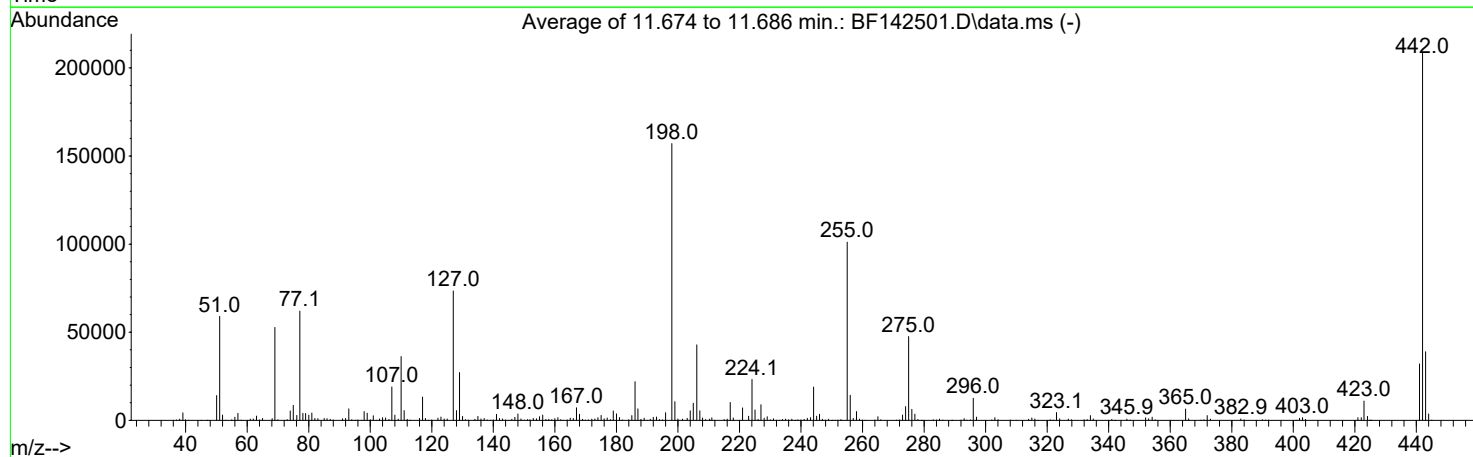


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF052225\  
Data File : BF142501.D  
Acq On : 22 May 2025 10:43  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF052025.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue May 20 16:26:47 2025

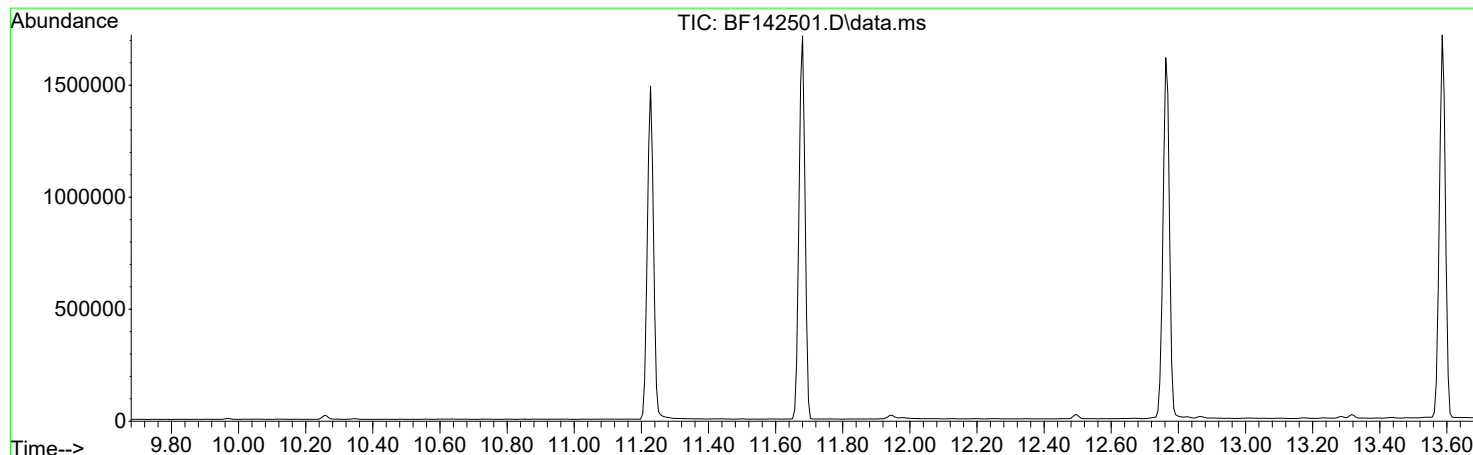

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1605

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 37.5         | 58985      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 974        | PASS                |
| 69             | 198             | 0.00            | 100             | 33.6         | 52773      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 339        | PASS                |
| 127            | 198             | 10              | 80              | 46.8         | 73475      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 157088     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 10630      | PASS                |
| 275            | 198             | 10              | 60              | 30.3         | 47603      | PASS                |
| 365            | 198             | 1               | 100             | 4.1          | 6420       | PASS                |
| 441            | 198             | 0.01            | 100             | 20.4         | 32069      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 208725     | PASS                |
| 443            | 442             | 15              | 24              | 18.7         | 38941      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 5/22/2025     | BNA_F            | <u>BF142501.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 439631           | 13.586             |
| DDD           | 7071             | 13.316             |
| DDE           | 359              | 12.951             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 7430          | 447061           | 1.66               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF052225\  
Data File : BF142501.D  
Acq On : 22 May 2025 10:43  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: May 22 12:24:21 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF052025.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 20 16:26:47 2025  
Response via : Initial Calibration

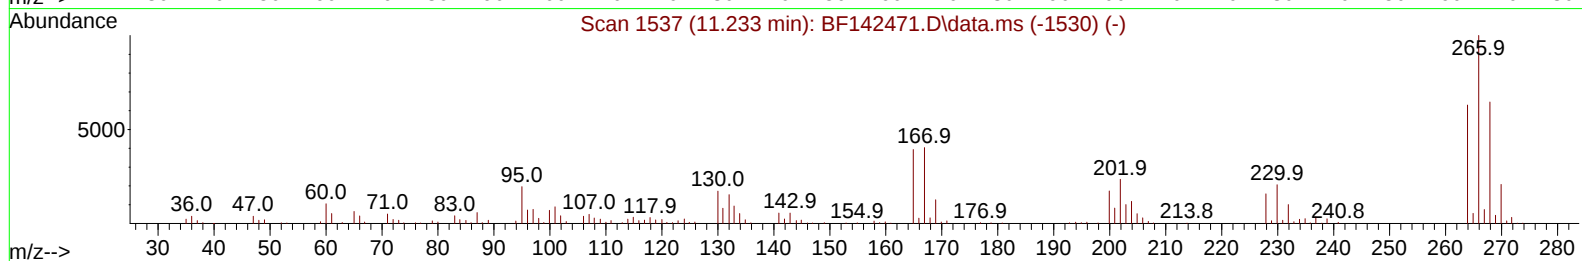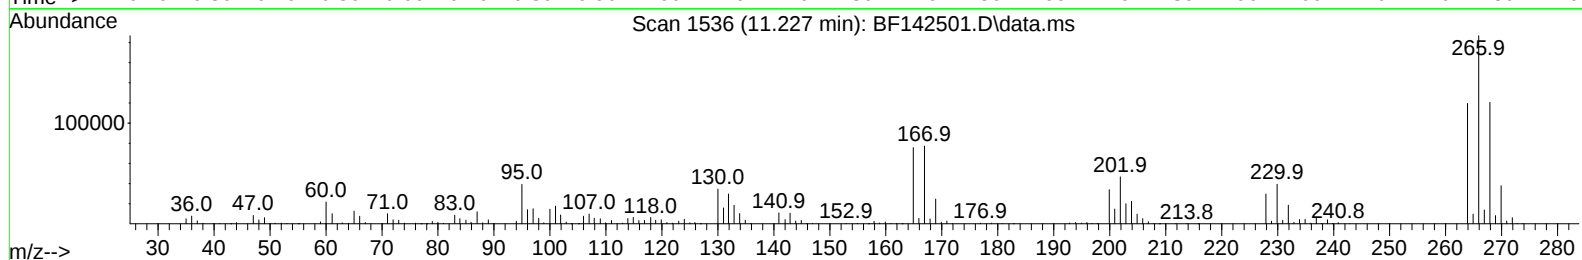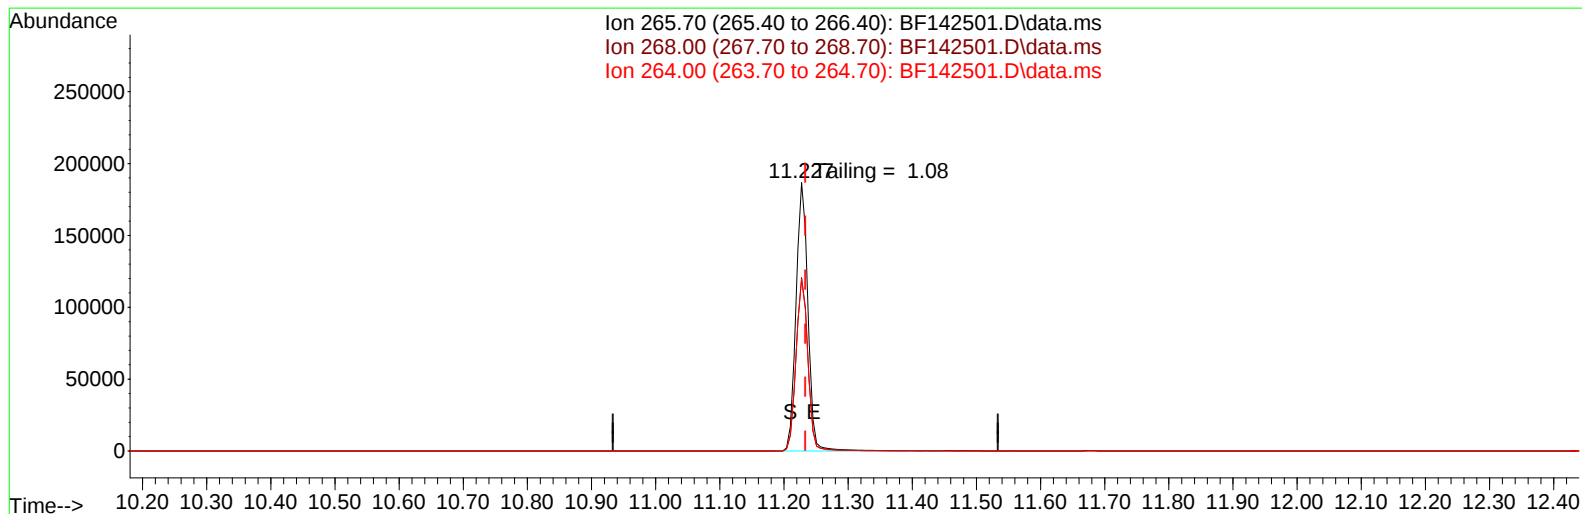

TIC: BF142501.D\data.ms

**(70) Pentachlorophenol (C)**

**11.227min (-0.006) 79510.36 ng**

**response 243635**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.60  | 64.59  |
| 264.00 | 63.00  | 64.05  |
| 0.00   | 0.00   | 0.00   |

