
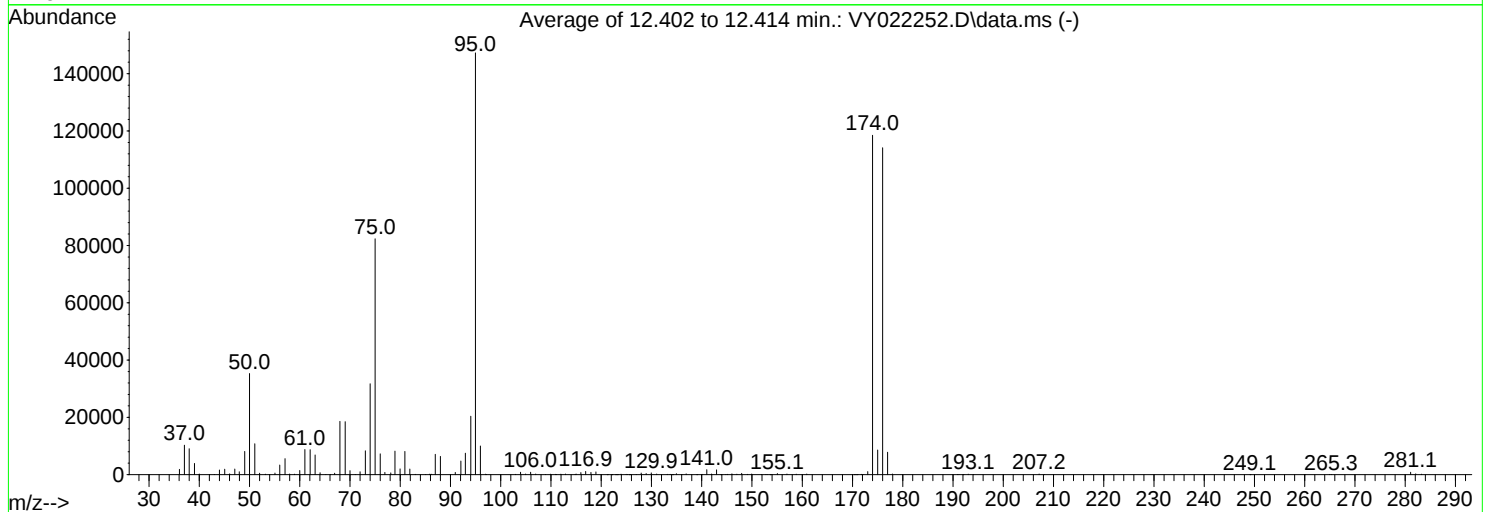


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051525\
 Data File : VY022252.D
 Acq On : 15 May 2025 07:52
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051525S.M
 Title : SW846 8260
 Last Update : Fri May 16 01:42:09 2025

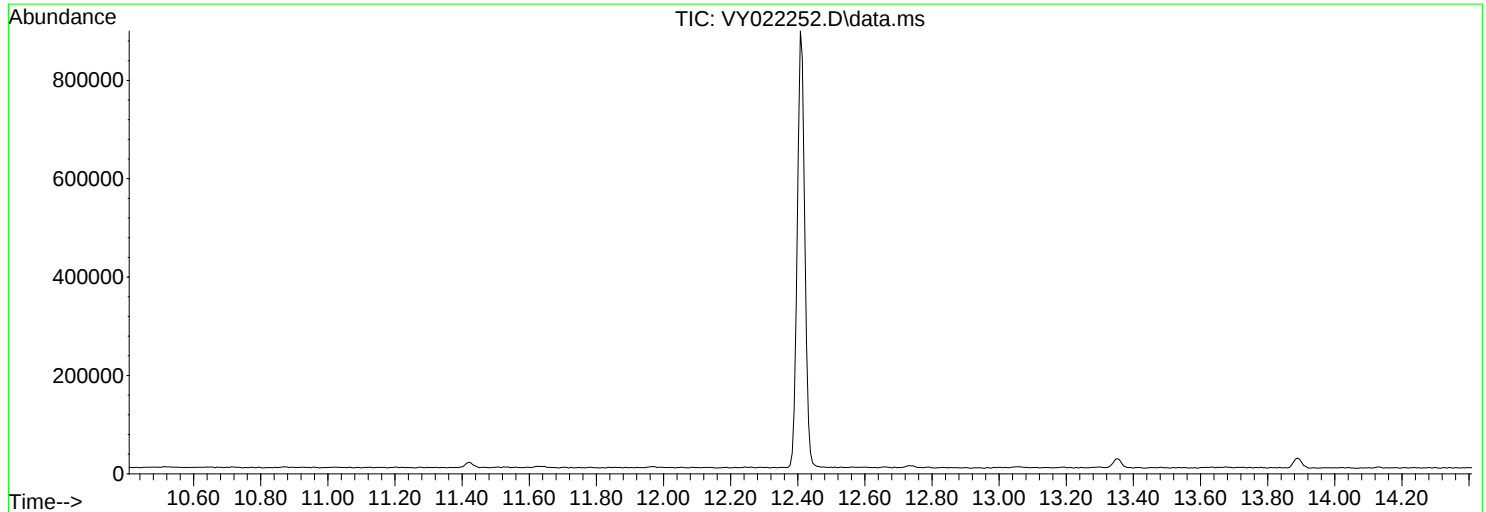

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	35318	PASS
75	95	30	60	55.9	82344	PASS
95	95	100	100	100.0	147275	PASS
96	95	5	9	6.8	9993	PASS
173	174	0.00	2	0.9	1042	PASS
174	95	50	100	80.5	118504	PASS
175	174	5	9	7.3	8635	PASS
176	174	95	101	96.3	114157	PASS
177	176	5	9	6.8	7810	PASS