
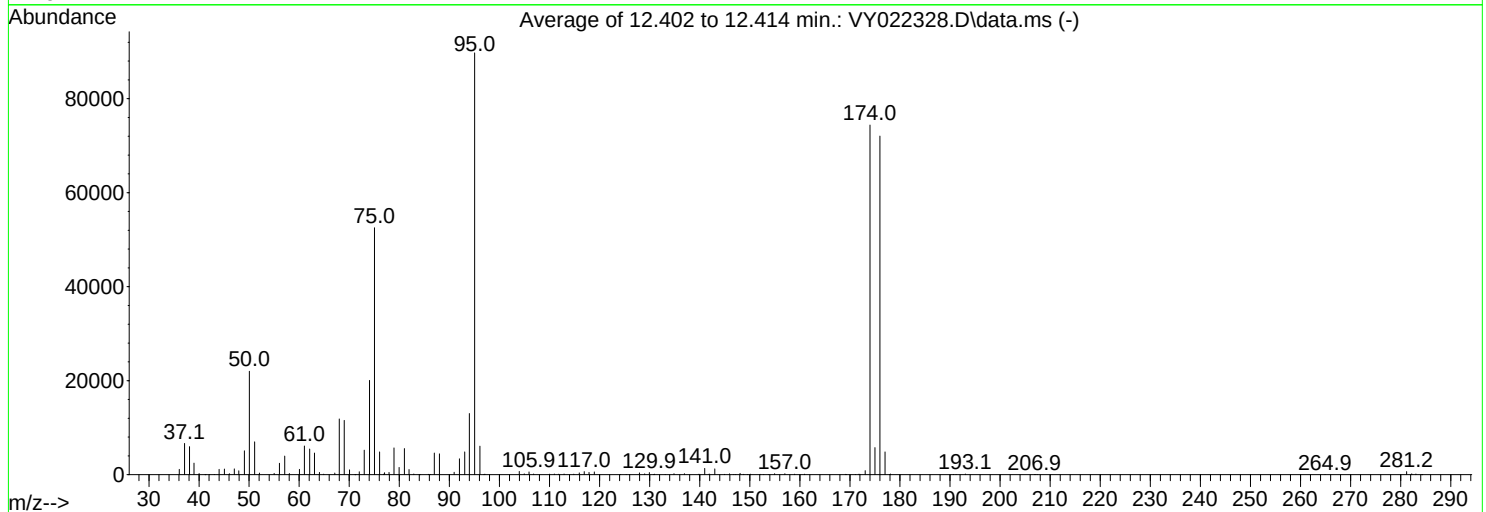


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052025\
Data File : VY022328.D
Acq On : 20 May 2025 08:09
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051525S.M
Title : SW846 8260
Last Update : Fri May 16 01:42:09 2025

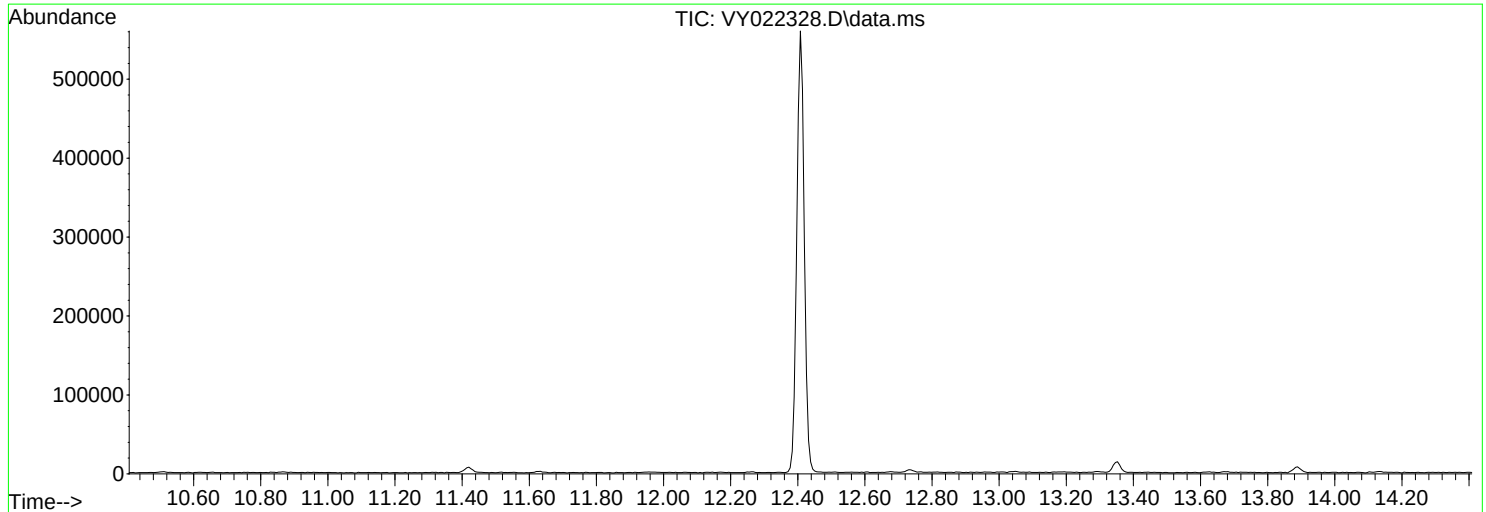

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	21987	PASS
75	95	30	60	58.5	52528	PASS
95	95	100	100	100.0	89755	PASS
96	95	5	9	6.7	6051	PASS
173	174	0.00	2	1.2	859	PASS
174	95	50	100	82.9	74379	PASS
175	174	5	9	7.7	5741	PASS
176	174	95	101	96.8	72035	PASS
177	176	5	9	6.7	4837	PASS