
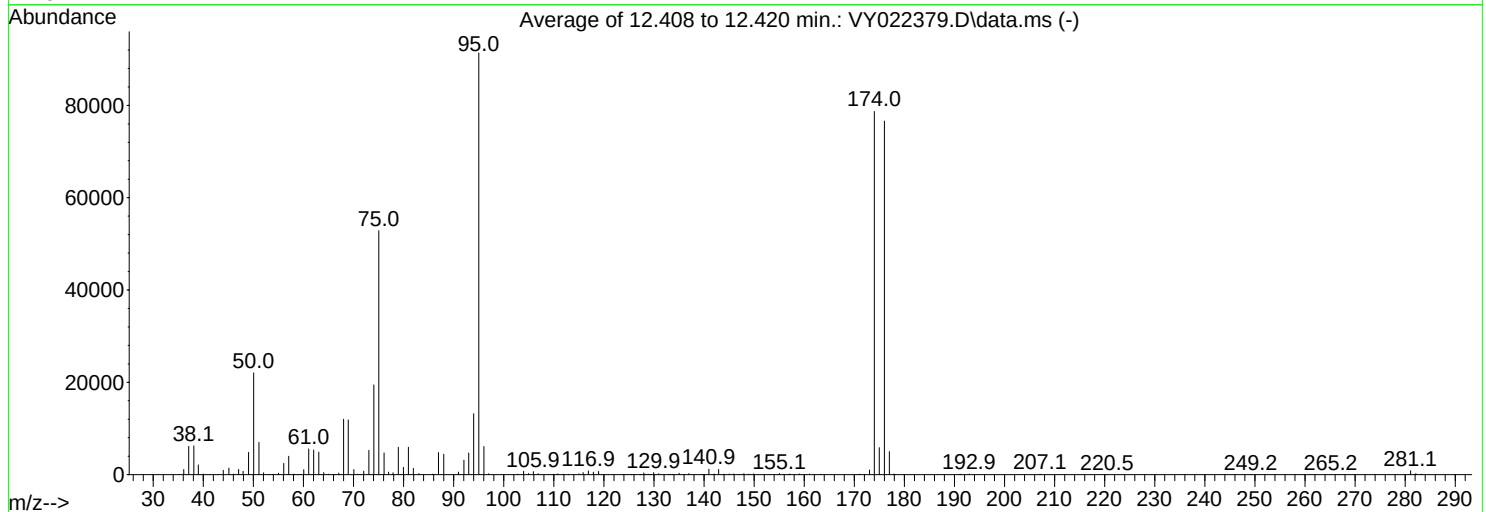


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052225\
Data File : VY022379.D
Acq On : 22 May 2025 08:05
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051525S.M
Title : SW846 8260
Last Update : Fri May 16 01:42:09 2025

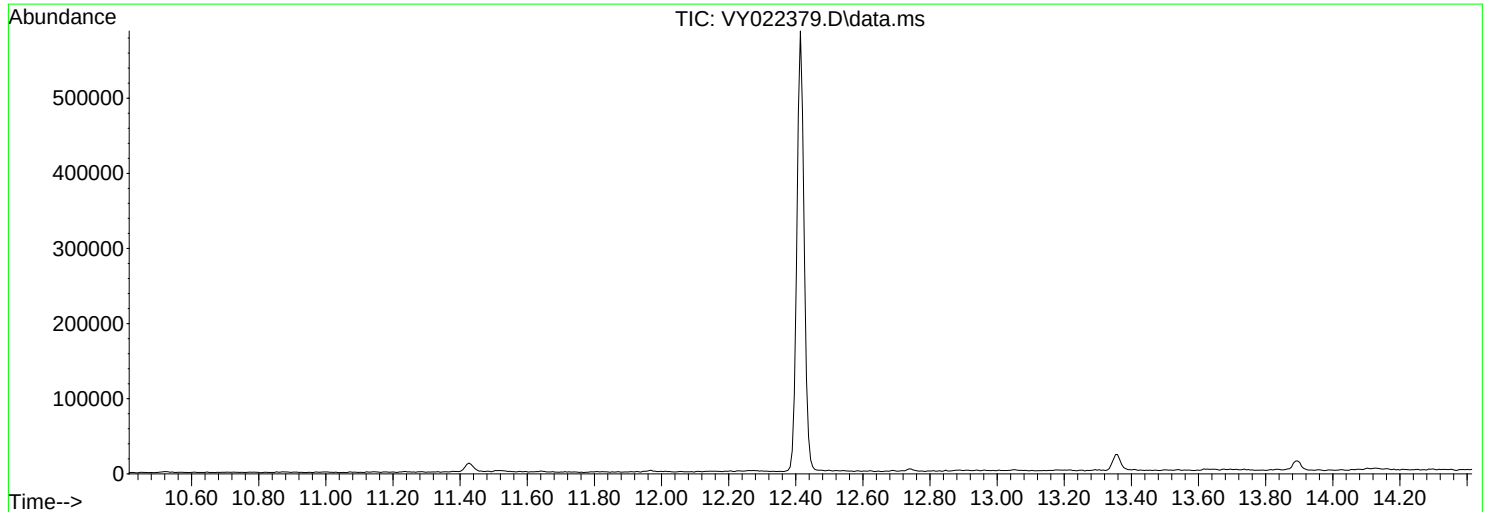

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.1	22056	PASS
75	95	30	60	57.8	52859	PASS
95	95	100	100	100.0	91380	PASS
96	95	5	9	6.7	6119	PASS
173	174	0.00	2	1.3	1000	PASS
174	95	50	100	86.1	78696	PASS
175	174	5	9	7.5	5864	PASS
176	174	95	101	97.4	76611	PASS
177	176	5	9	6.5	4987	PASS