


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051625\
Data File : VN086668.D
Acq On : 16 May 2025 15:33
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
Title : SW846 8260
Last Update : Sat May 17 00:46:13 2025

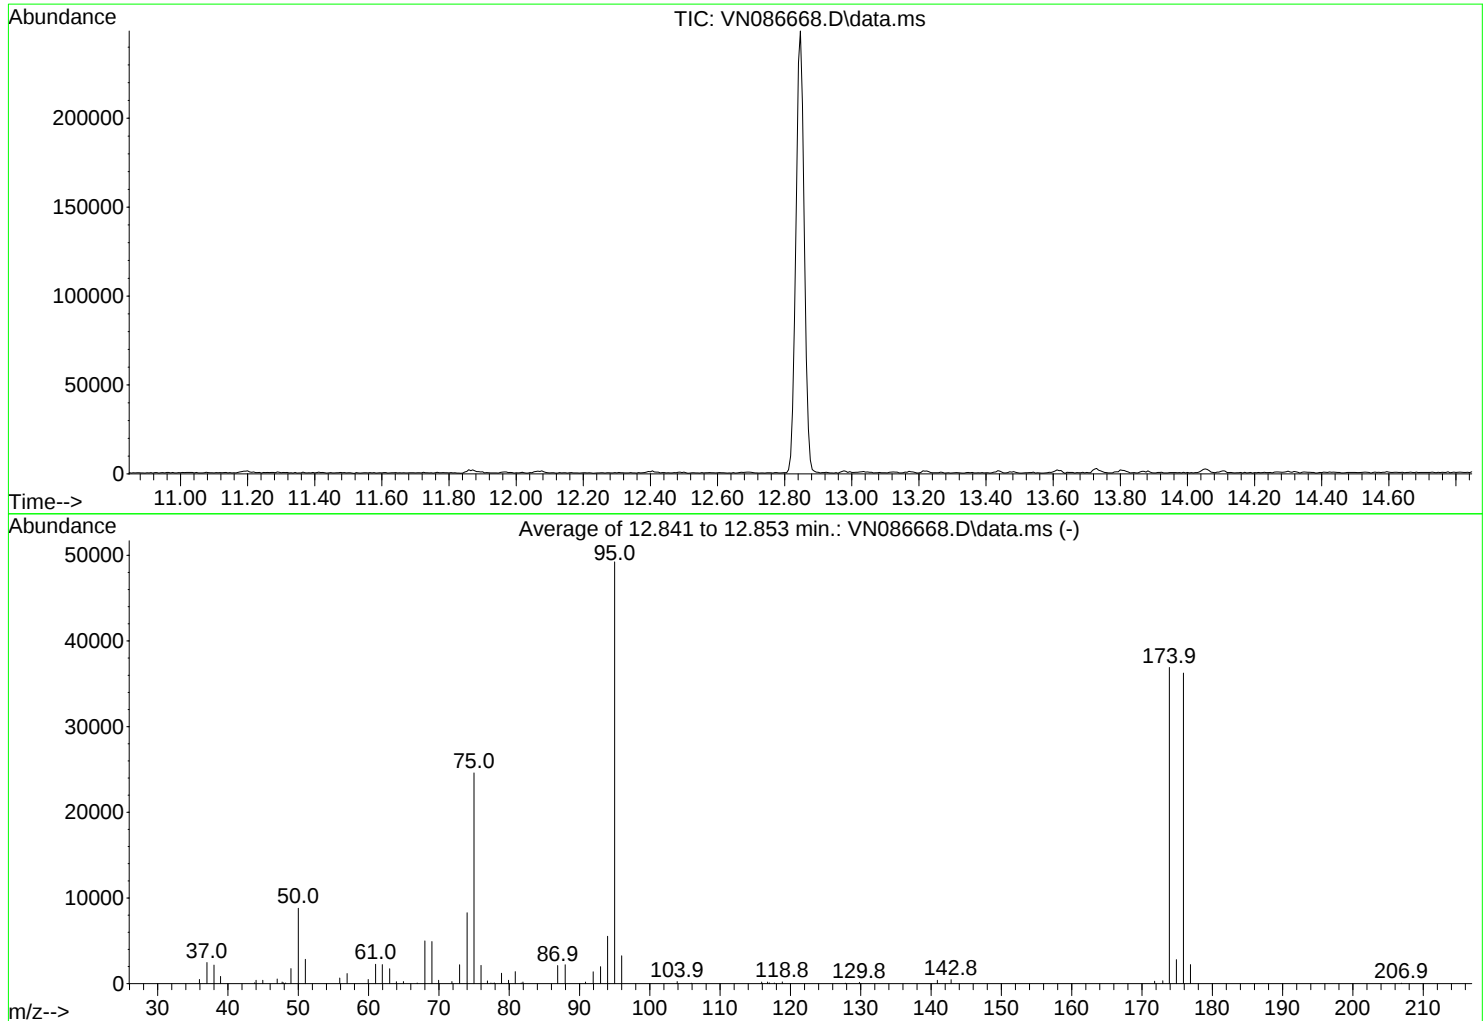

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	8802	PASS
75	95	30	60	50.0	24603	PASS
95	95	100	100	100.0	49237	PASS
96	95	5	9	6.6	3255	PASS
173	174	0.00	2	0.9	345	PASS
174	95	50	100	74.9	36899	PASS
175	174	5	9	7.6	2805	PASS
176	174	95	101	98.2	36248	PASS
177	176	5	9	6.1	2226	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	491	48.95	1758	66.90	77	77.70	61
37.00	2471	50.00	8802	68.00	4985	77.90	81
38.00	2170	51.00	2842	69.00	4914	78.90	122
38.95	848	55.90	650	69.95	392	79.90	39
43.80	90	56.95	1184	71.85	240	80.85	1395
44.00	384	59.95	482	72.95	2211	81.70	66
44.95	402	61.00	2266	74.00	8274	81.95	184
47.00	538	61.95	2229	75.00	24603	86.90	2121
47.70	193	63.00	1738	76.00	2136	87.95	2202
47.90	98	63.95	231	76.90	315	90.85	195
48.20	75	64.95	248	77.40	73	91.95	1382

Average of 12.841 to 12.853 min.: VN086668.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.00	1974	127.80	58				
94.00	5539	129.80	148				
95.00	49237	140.90	397				
96.00	3255	142.85	470				
103.90	249	171.80	278				
105.90	60	172.95	345				
115.90	181	173.90	36899				
116.75	181	174.90	2805				
117.00	86	175.90	36248				
117.70	68	176.90	2226				
118.85	214	206.90	58				

Instrument :
MSVOA_N
ClientSampleId :
BFB