
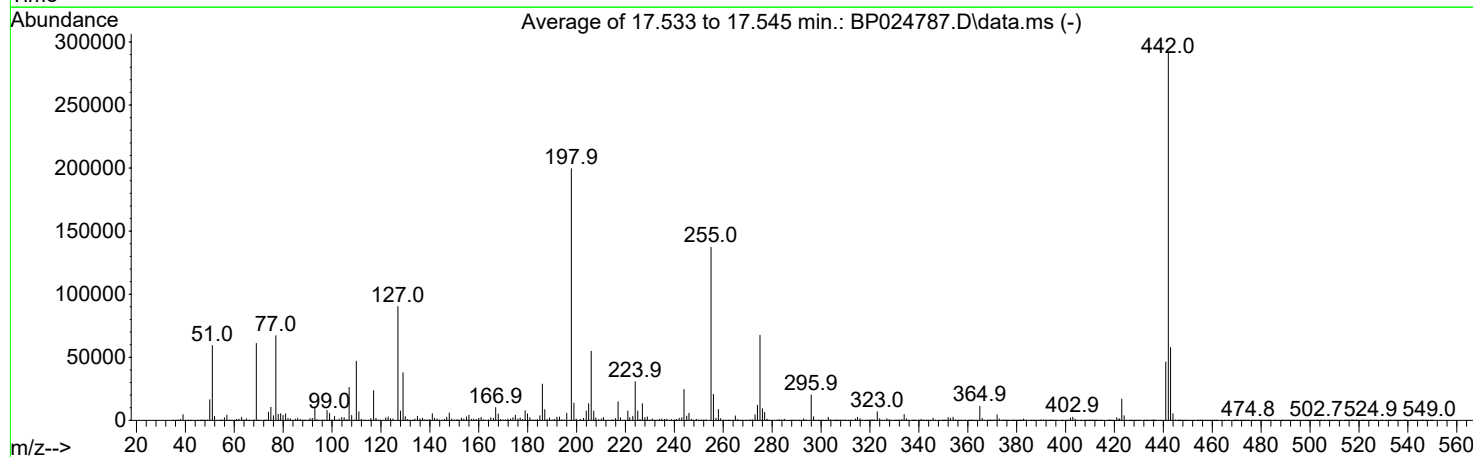


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052325\  
Data File : BP024787.D  
Acq On : 23 May 2025 10:59  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP051325.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue May 13 16:21:39 2025

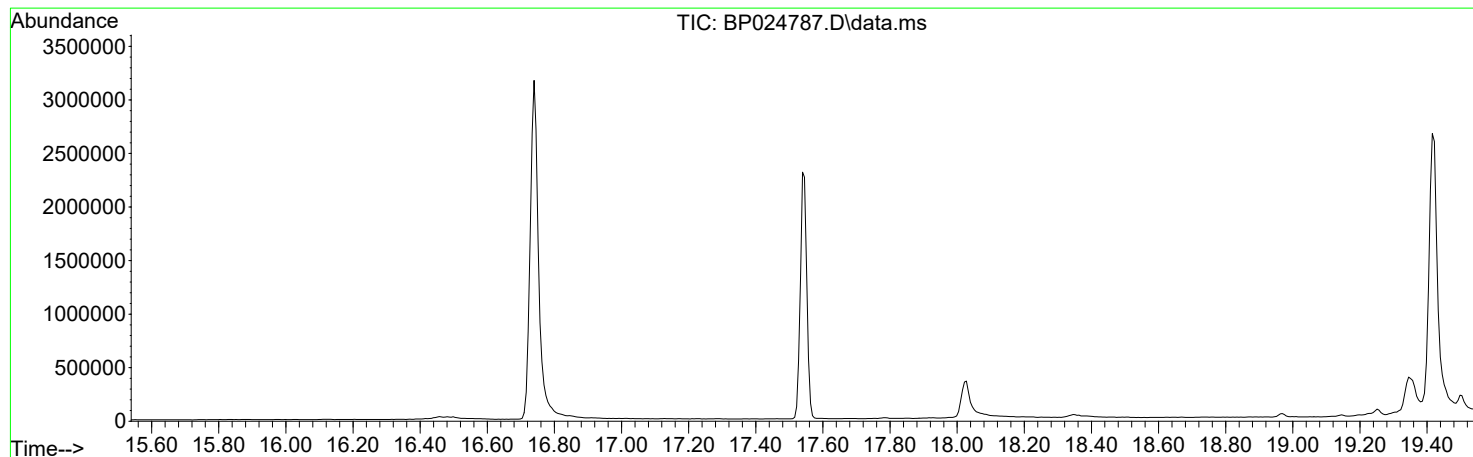

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2447

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 29.8         | 59362      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.7          | 401        | PASS                |
| 69             | 198             | 0.00            | 100             | 30.6         | 61074      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 290        | PASS                |
| 127            | 198             | 10              | 80              | 45.2         | 90179      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 199477     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 13702      | PASS                |
| 275            | 198             | 10              | 60              | 33.8         | 67505      | PASS                |
| 365            | 198             | 1               | 100             | 5.6          | 11114      | PASS                |
| 441            | 198             | 0.01            | 100             | 23.2         | 46297      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 291624     | PASS                |
| 443            | 442             | 15              | 24              | 19.8         | 57675      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 5/23/2025     | BNA_P            | <u>BP024787.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 889984           | 20.698             |
| DDD           | 15428            | 20.286             |
| DDE           | 1954             | 19.71              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 17382         | 907366           | 1.92               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP052325\  
Data File : BP024787.D  
Acq On : 23 May 2025 10:59  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: May 23 12:13:37 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP051325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 13 16:21:39 2025  
Response via : Initial Calibration

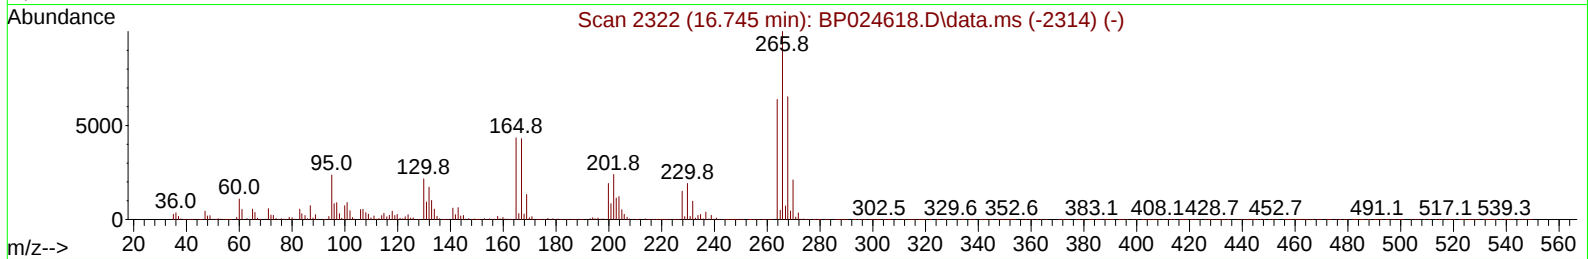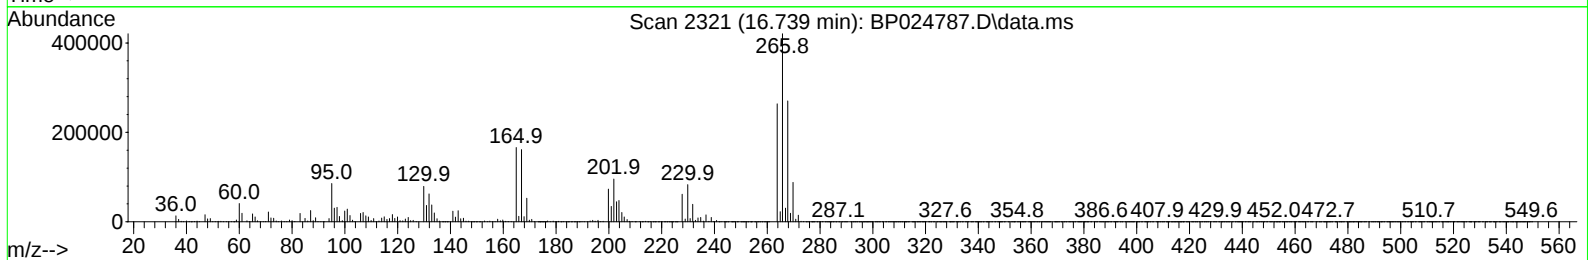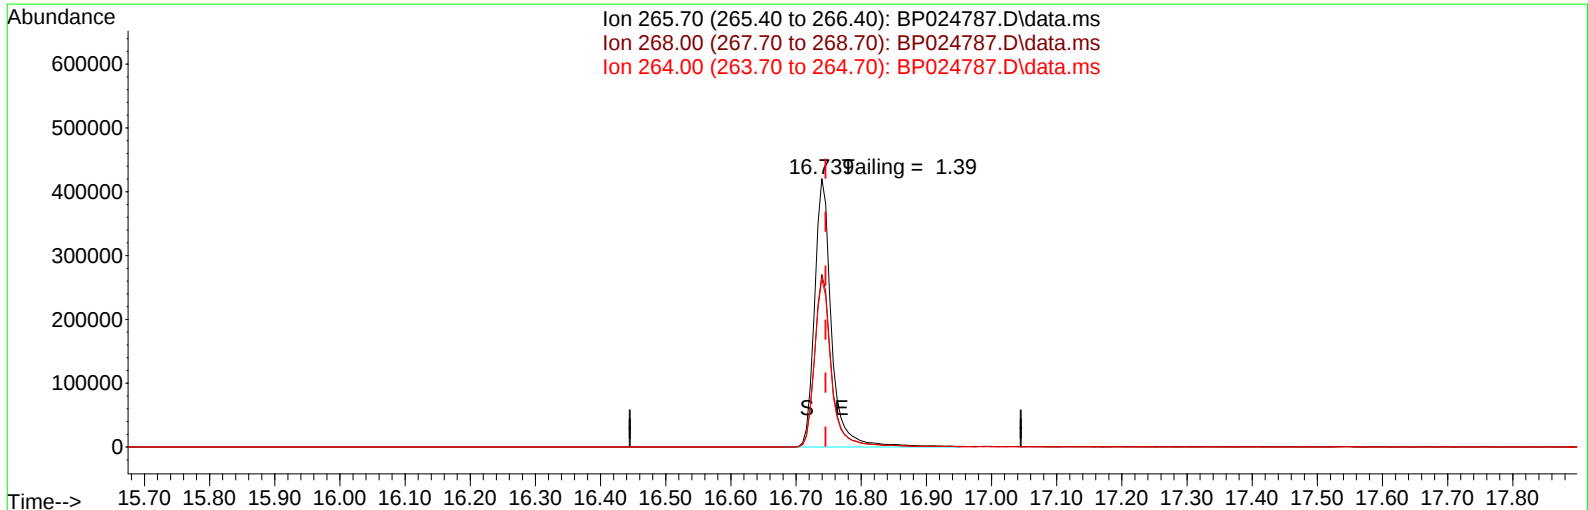

TIC: BP024787.D\data.ms

**(70) Pentachlorophenol (C)**

**16.739min (-0.006) 1289316.61 ng**




**response 758576**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.30  | 64.26  |
| 264.00 | 63.90  | 62.71  |
| 0.00   | 0.00   | 0.00   |

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052325\  
Data File : BP024787.D  
Acq On    : 23 May 2025  10:59  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

**Instrument :**  
BNA\_P  
**ClientSampleId :**  
DFTPP

Quant Time: May 23 12:13:37 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP051325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 13 16:21:39 2025  
Response via : Initial Calibration

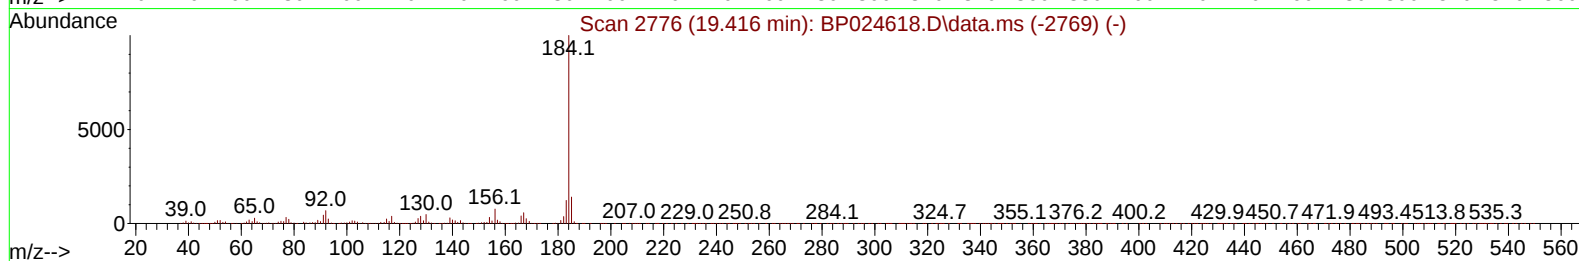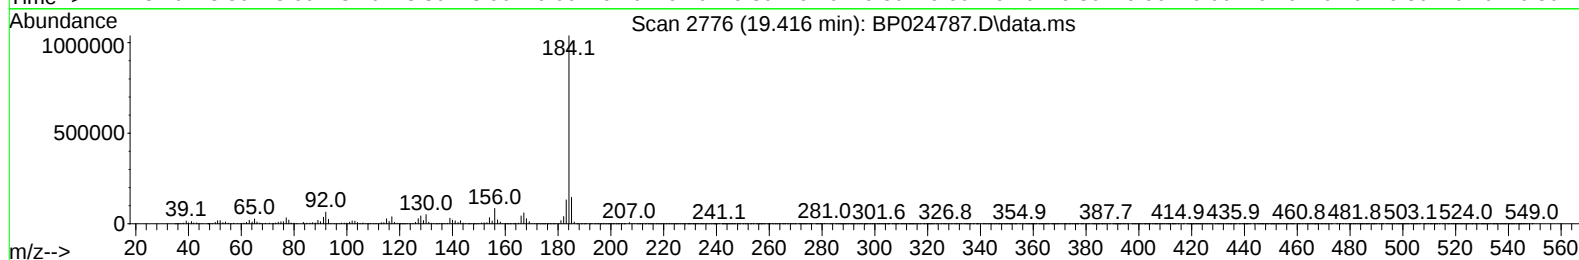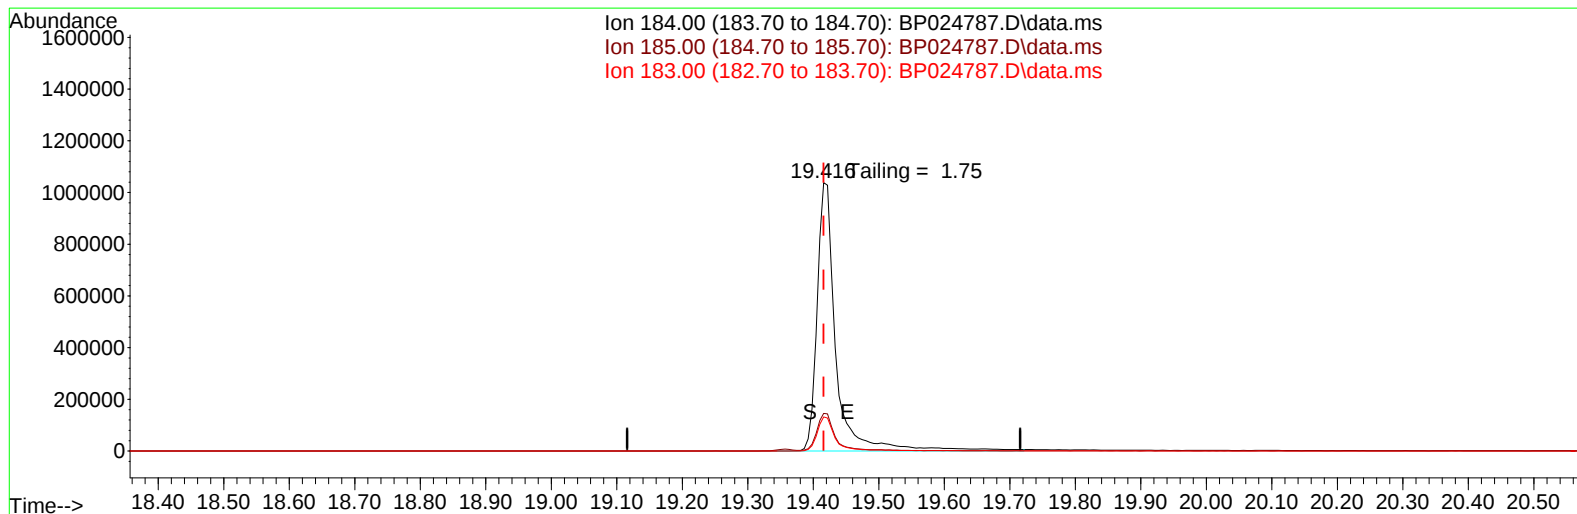

TIC: BP024787.D\data.ms

(77) Benzidine

**19.416min (-0.000) 1952689.30 ng**

**response**      **2020967**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.00  | 14.02  |
| 183.00 | 12.30  | 12.71  |
| 0.00   | 0.00   | 0.00   |