


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052325\
Data File : VN086765.D
Acq On : 23 May 2025 08:37
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
Title : SW846 8260
Last Update : Sat May 17 00:46:13 2025

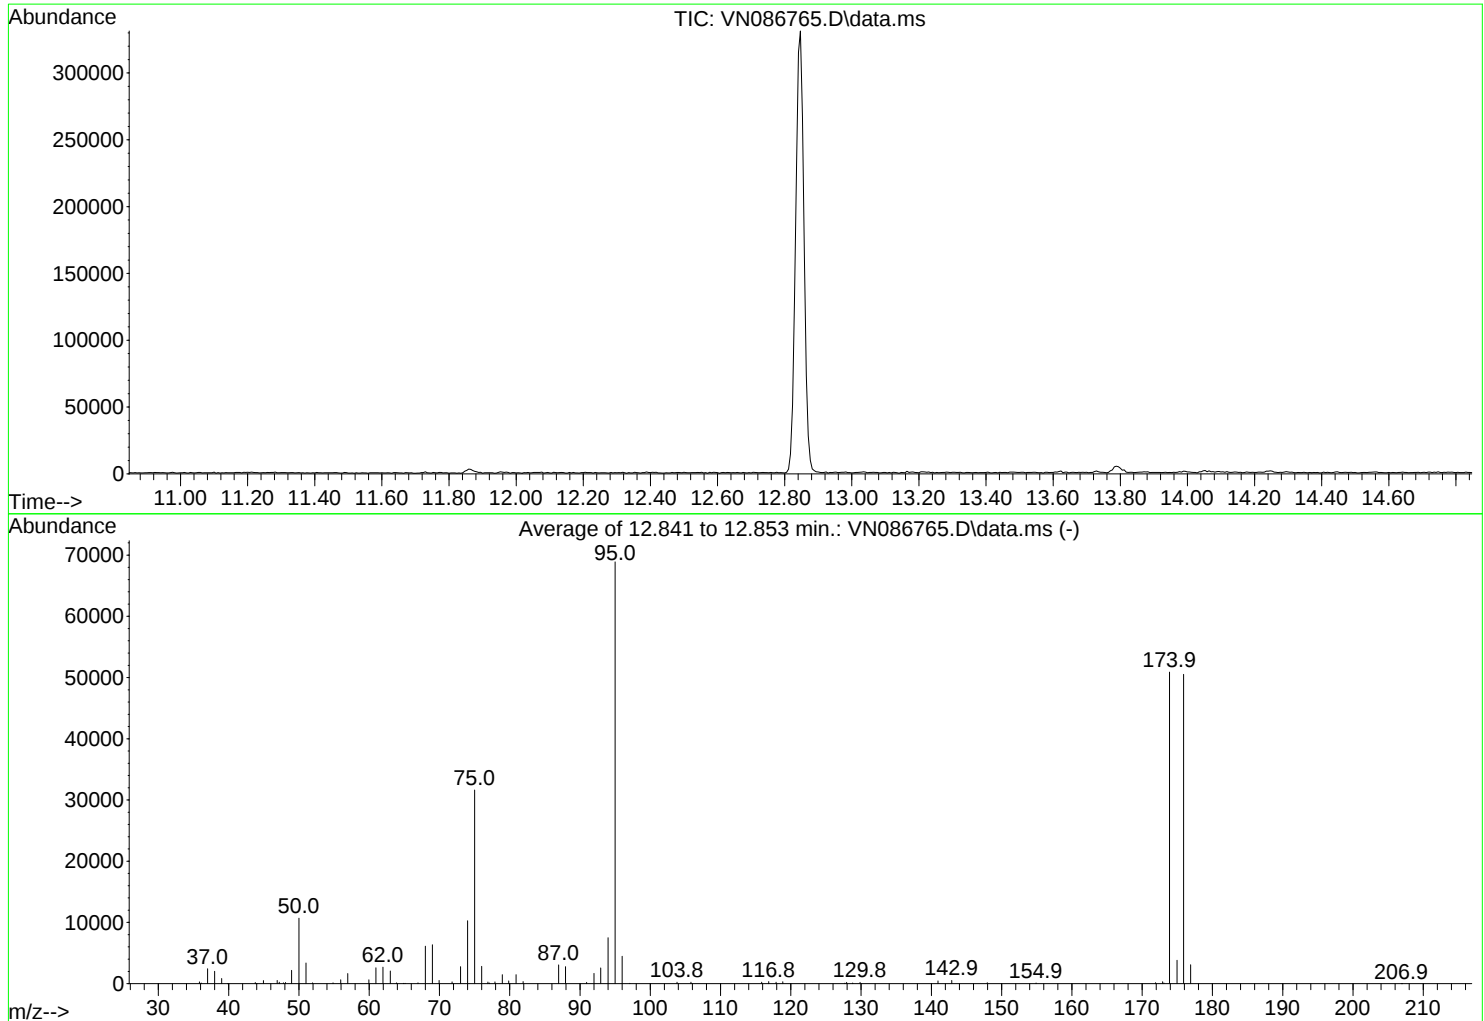

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.5	10690	PASS
75	95	30	60	45.9	31621	PASS
95	95	100	100	100.0	68904	PASS
96	95	5	9	6.5	4467	PASS
173	174	0.00	2	0.6	311	PASS
174	95	50	100	73.8	50883	PASS
175	174	5	9	7.5	3816	PASS
176	174	95	101	99.3	50515	PASS
177	176	5	9	6.1	3097	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	297	47.80	126	61.95	2695	74.00	1028
36.10	118	48.10	191	63.00	2074	75.00	3162
37.00	2436	48.95	2164	63.90	123	76.00	281
38.00	2020	50.00	10690	64.90	58	76.90	26
39.00	848	51.00	3361	65.10	58	77.10	111
39.85	5	51.95	133	66.95	132	77.90	280
43.80	196	54.85	144	68.00	6104	78.95	1465
43.90	11	55.95	643	69.00	6359	79.85	445
44.95	497	56.95	1663	69.95	518	80.90	1470
46.90	522	59.95	637	71.80	283	81.90	338
47.20	228	60.95	2594	73.00	2776	86.95	3053

Average of 12.841 to 12.853 min.: VN086765.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	2773	116.85	355	171.90	168		
90.95	208	117.90	241	172.90	311		
92.00	1664	118.85	322	173.10	113		
92.95	2562	127.70	84	173.90	50883		
94.00	7515	127.95	215	174.95	3816		
95.00	68904	128.80	107	175.90	50515		
96.00	4467	129.85	222	176.90	3097		
97.10	57	140.95	456	206.90	10		
103.80	236	142.90	524				
105.80	225	147.95	155				
115.85	245	154.90	105				

Instrument :

MSVOA_N

ClientSampleId :

BFB