


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN052925\  
Data File : BN037127.D  
Acq On : 29 May 2025 09:28  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN051425.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed May 14 11:26:32 2025

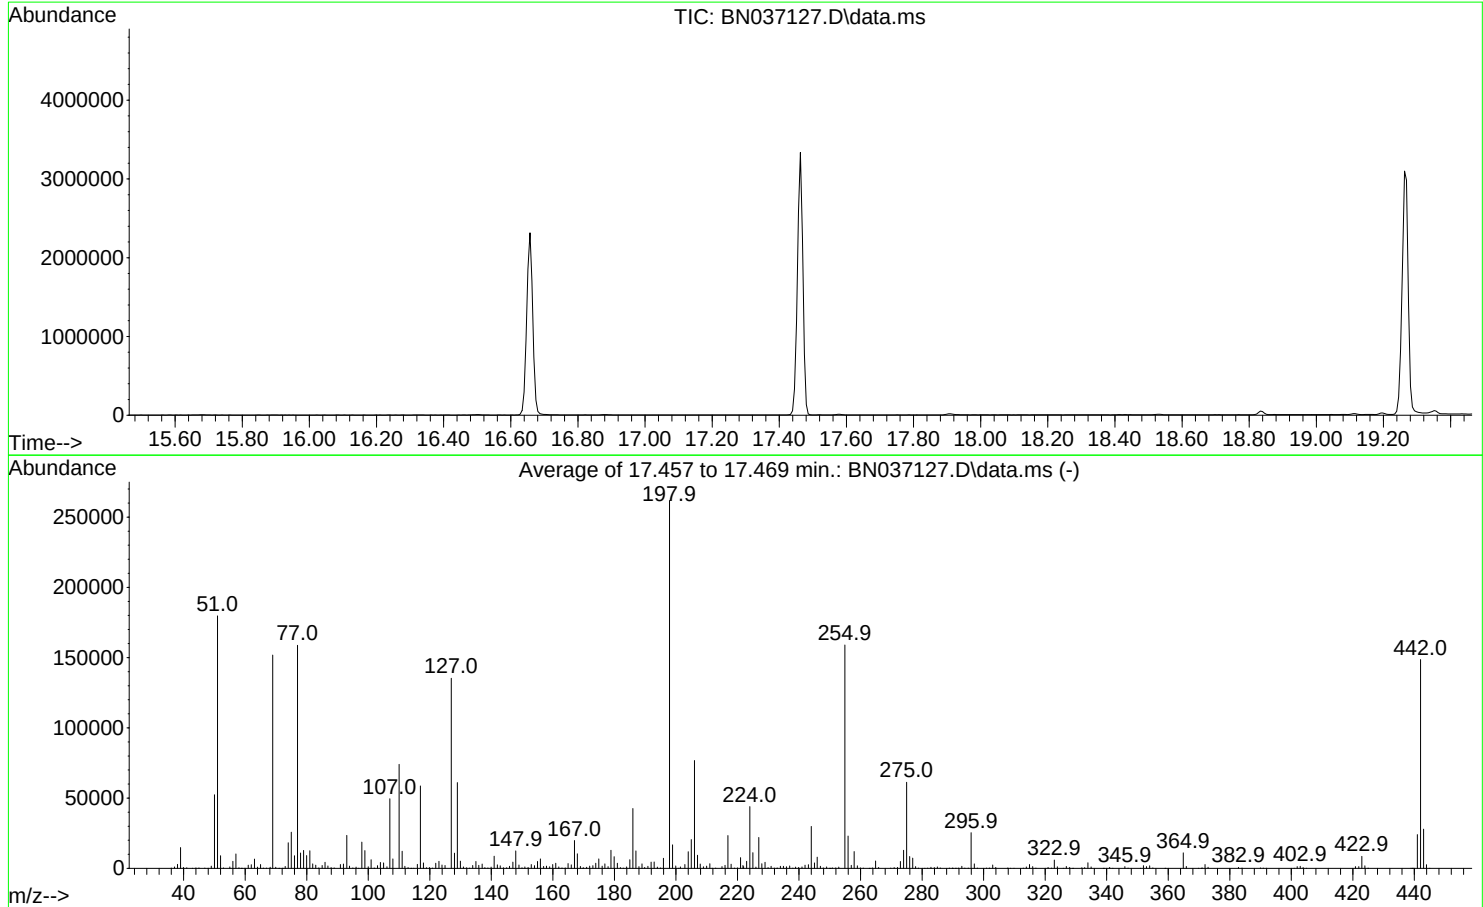




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 68.7         | 179763     | PASS                |
| 68             | 69              | 0.00            | 2               | 0.5          | 810        | PASS                |
| 69             | 198             | 0.00            | 100             | 58.0         | 151837     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 774        | PASS                |
| 127            | 198             | 10              | 80              | 51.7         | 135352     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 261824     | PASS                |
| 199            | 198             | 5               | 9               | 6.4          | 16719      | PASS                |
| 275            | 198             | 10              | 60              | 23.4         | 61272      | PASS                |
| 365            | 198             | 1               | 100             | 4.2          | 11025      | PASS                |
| 441            | 198             | 0.01            | 100             | 9.2          | 23996      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 148611     | PASS                |
| 443            | 442             | 15              | 24              | 18.8         | 27931      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN052925\  
Data File : BN037127.D  
Acq On : 29 May 2025 09:28  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: May 29 16:10:02 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 27 07:40:28 2025  
Response via : Initial Calibration

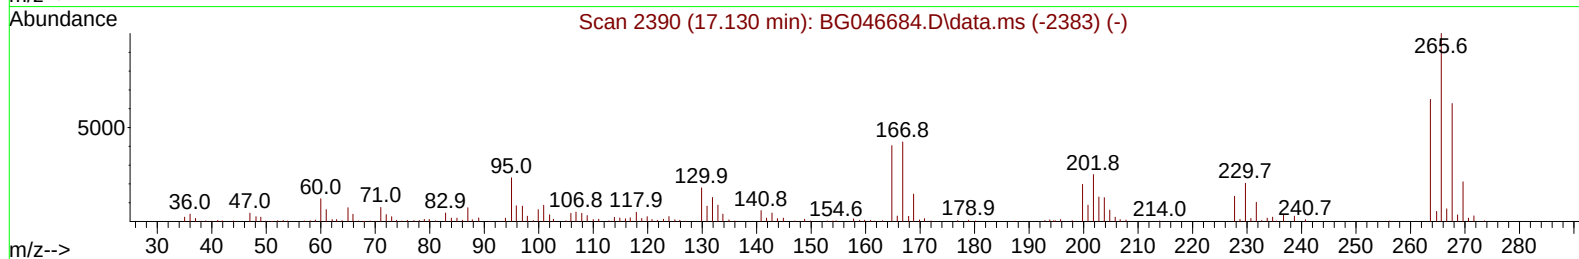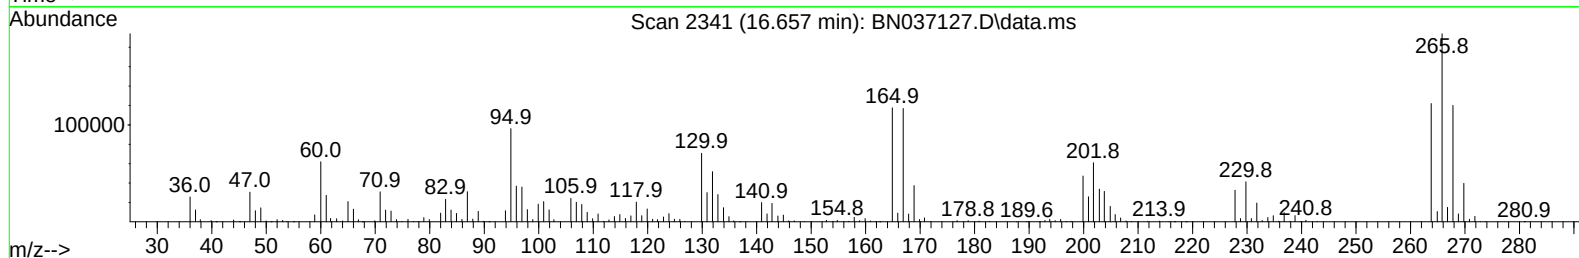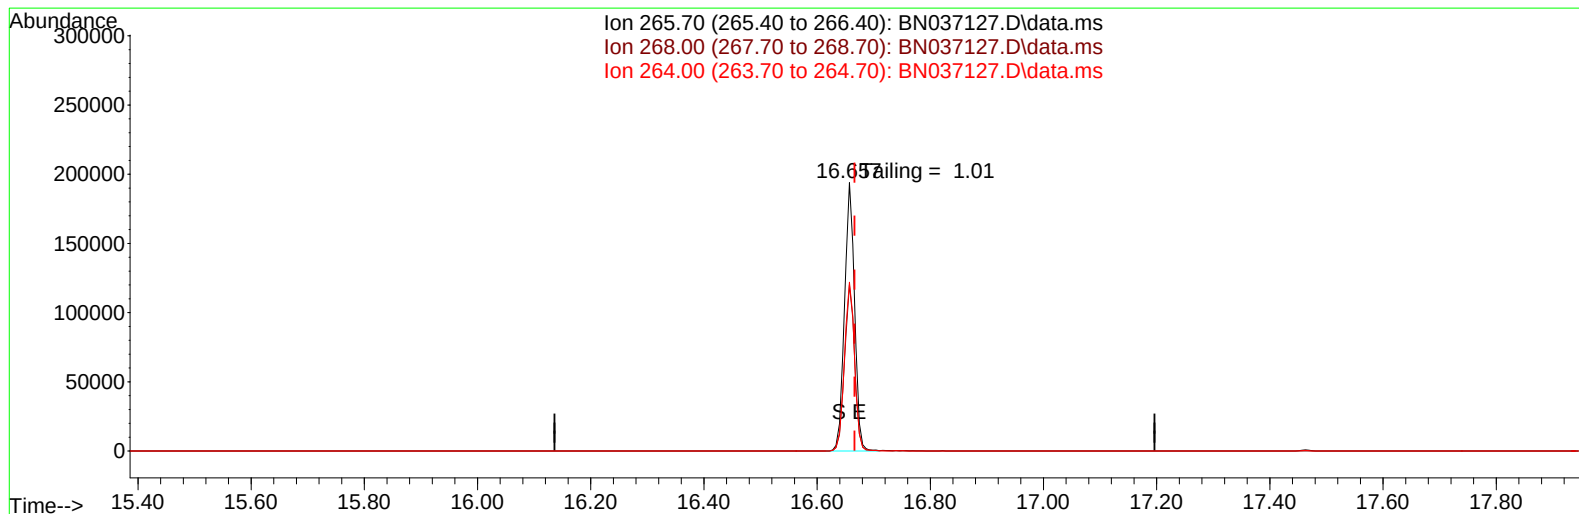

TIC: BN037127.D\data.ms

**(70) Pentachlorophenol (C)**

16.657min (-0.009) 17413.96 ng




response 239839

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 61.88  |
| 264.00 | 61.60  | 62.90  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN052925\  
Data File : BN037127.D  
Acq On : 29 May 2025 09:28  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: May 29 16:10:02 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 27 07:40:28 2025  
Response via : Initial Calibration

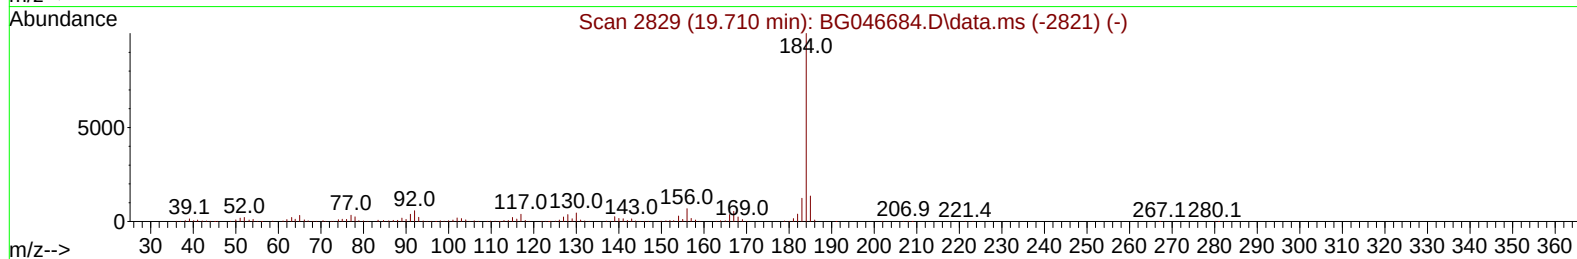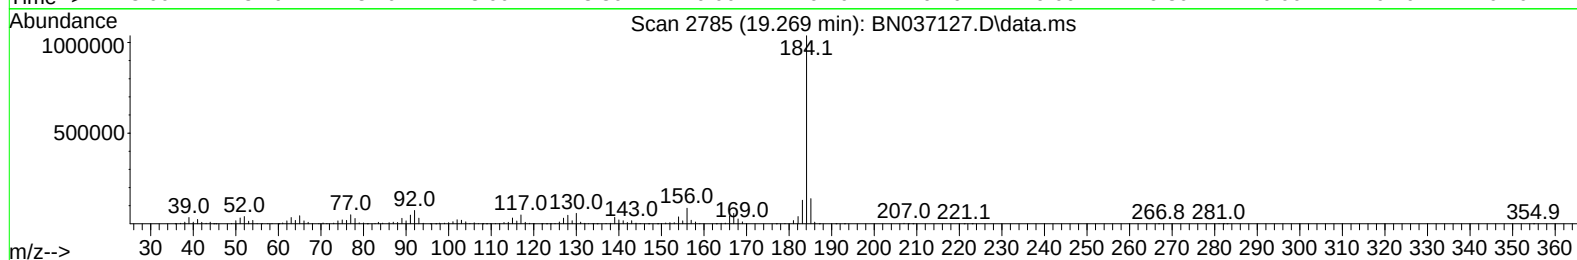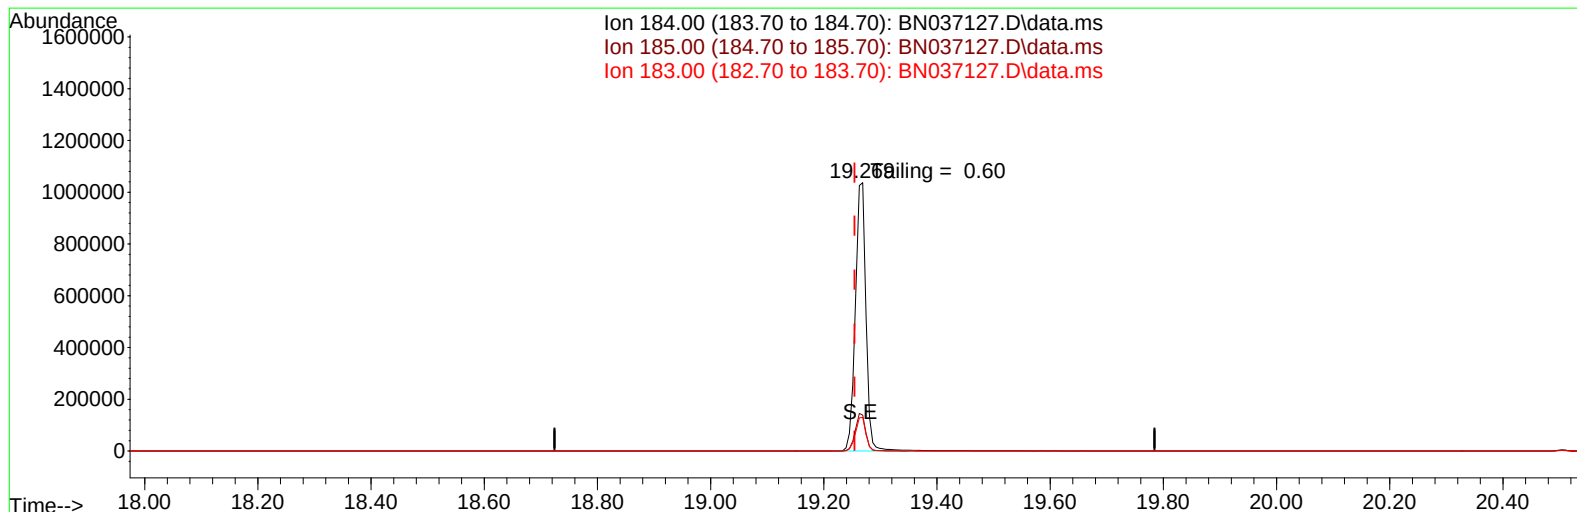

TIC: BN037127.D\data.ms

**(77) Benzidine**

19.269min (+ 0.015) 0.00 ng m

response 1341629

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.40  |
| 183.00 | 13.20  | 12.52  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 5/29/2025     | BNA_N            | <u>BN037127.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 789740           | 20.504             |
| DDD           | 15689            | 20.063             |
| DDE           | 611              | 19.557             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 16300         | 806040           | 2.02               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP