


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050235.D
Acq On : 09 Jun 2025 10:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 09 11:54:38 2025

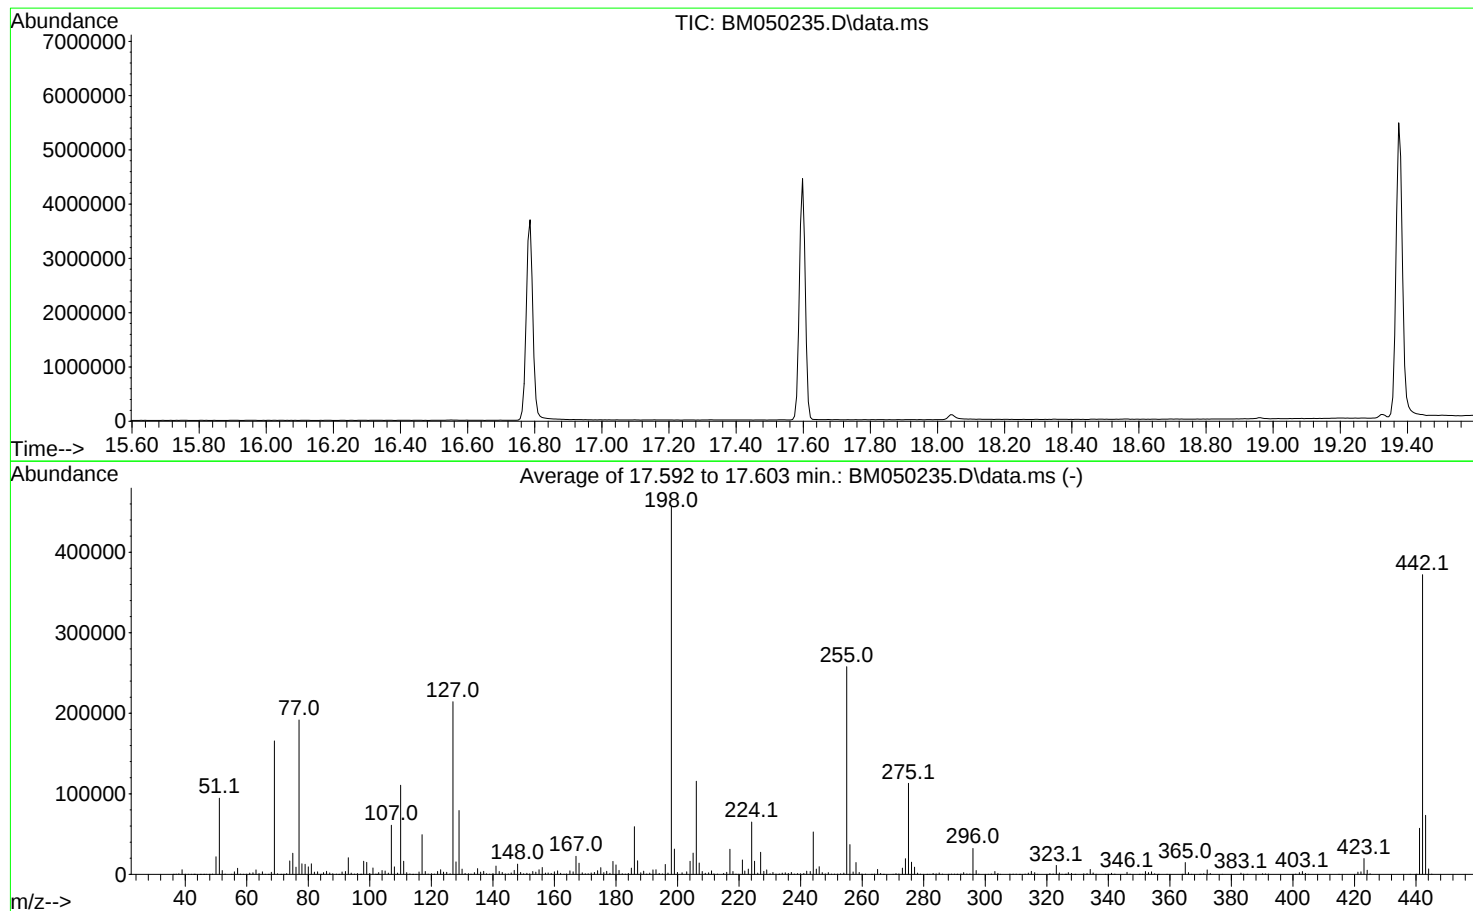




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	20.7	94583	PASS
68	69	0.00	2	1.6	2624	PASS
69	198	0.00	100	36.3	165736	PASS
70	69	0.00	2	0.5	805	PASS
127	198	10	80	46.9	214315	PASS
197	198	0.00	2	0.4	1683	PASS
198	198	100	100	100.0	456747	PASS
199	198	5	9	6.9	31357	PASS
275	198	10	60	24.7	112981	PASS
365	198	1	100	3.2	14692	PASS
441	198	0.01	100	12.5	57299	PASS
442	442	50	100	100.0	372181	PASS
443	442	15	24	19.7	73325	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050235.D
Acq On : 09 Jun 2025 10:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 09 13:03:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

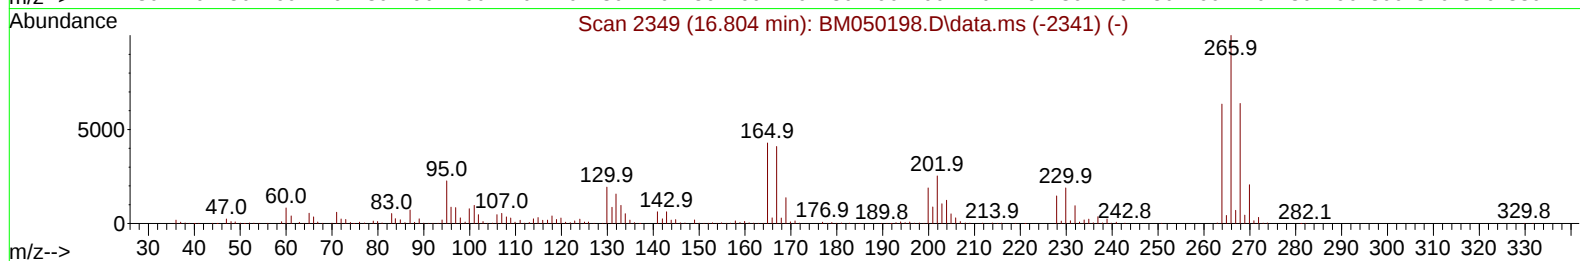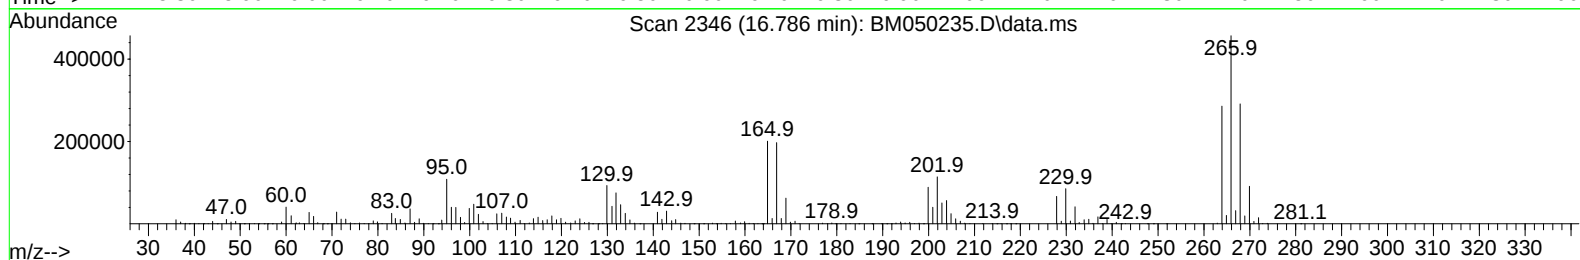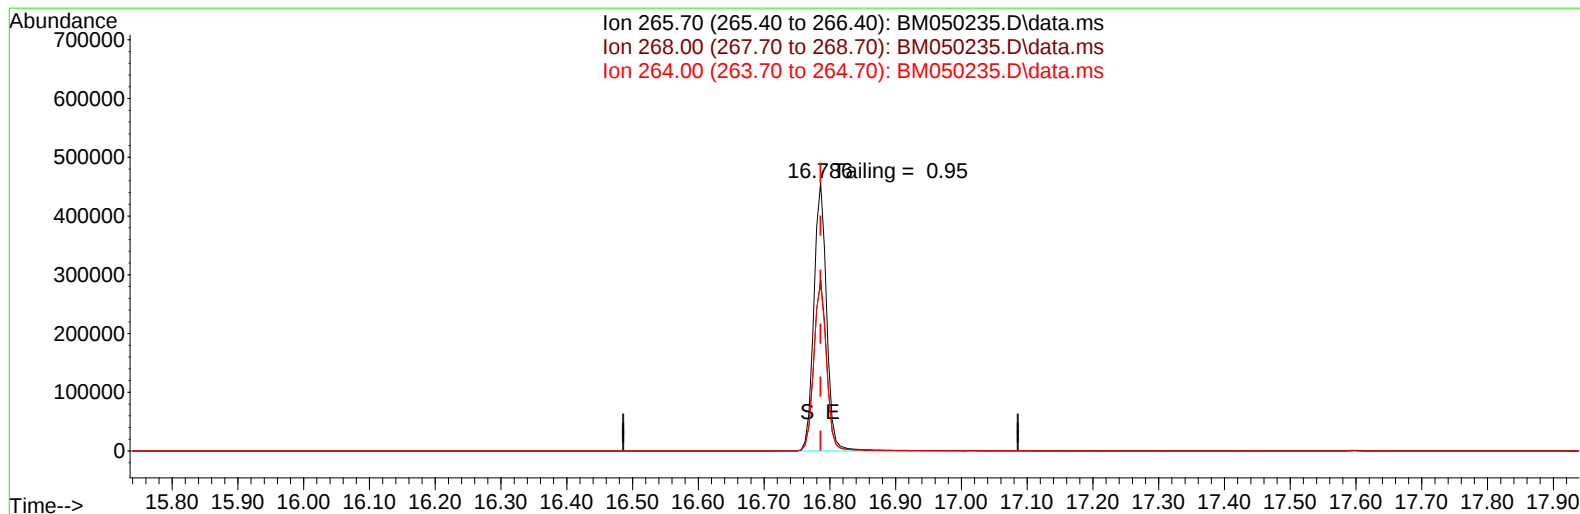

TIC: BM050235.D\data.ms

(70) Pentachlorophenol (C)

16.786min (-0.000) 0.00 ng




response 616214

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.75
264.00	63.50	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050235.D
Acq On : 09 Jun 2025 10:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 09 13:03:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

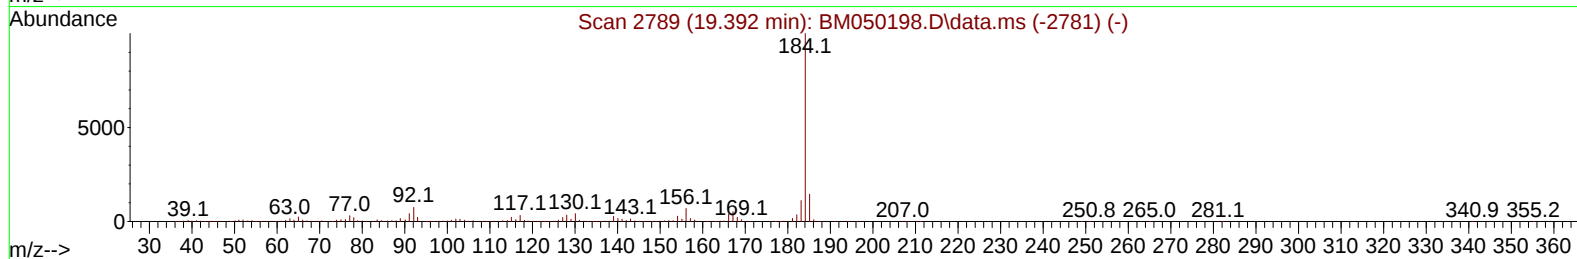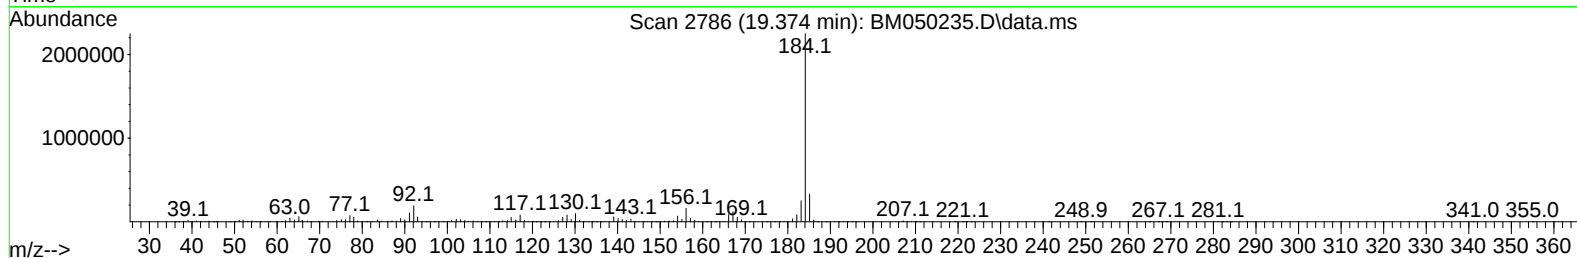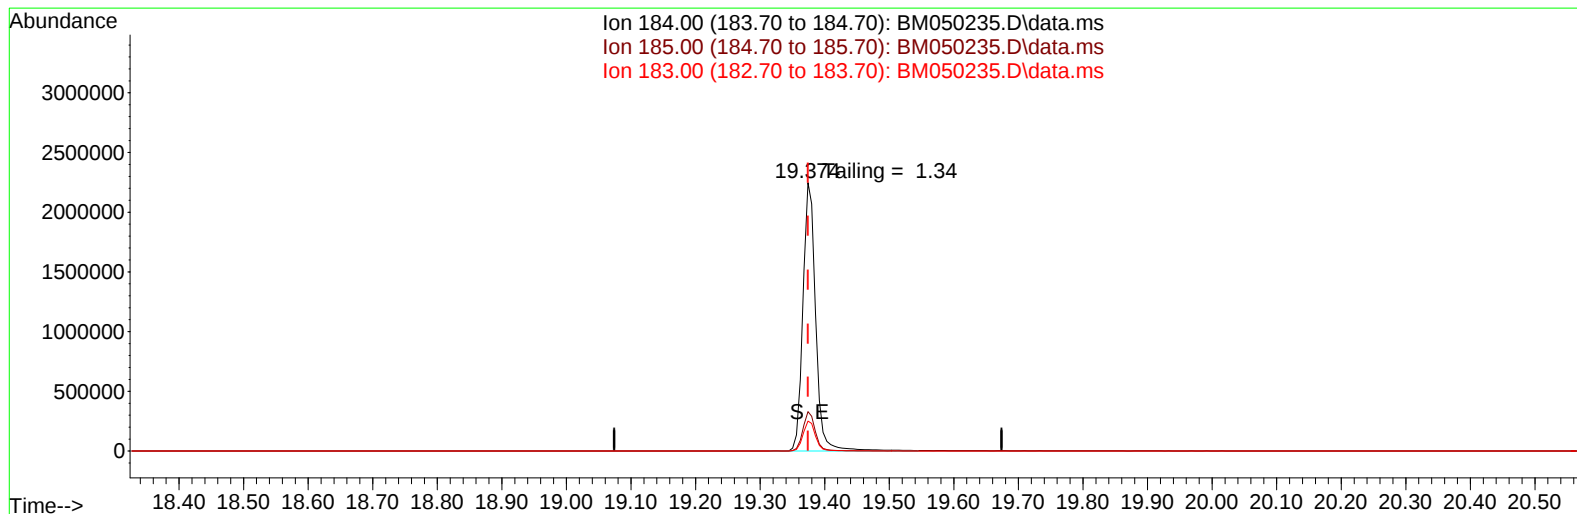

TIC: BM050235.D\data.ms

(77) Benzidine

19.374min (-0.000) 298883.97 ng

response 3092988

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.66
183.00	11.20	11.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/9/2025	BNA_M	<u>BM050235.D</u>
Compound Name	Response	Retention Time
DDT	15270008	20.621
DDD	18649	20.233
DDE	1319	19.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19968	15289976	0.13

Instrument :
BNA_M
ClientSampleId :
DFTPP