

SOP ID: M3510C,3580A-Extraction SVOC-20

Clean Up SOP #: N/A

Matrix : Water

Weigh By: N/A

Balance check: N/A

Balance ID: N/A

pH Strip Lot#: E3880

Extraction By: RS

Filter By: RS

pH Meter ID: N/A

Hood ID: 4,6,7

Extraction Start Date : 06/06/2025

Extraction Start Time : 09:15

Extraction End Date : 06/06/2025

Extraction End Time : 14:15

Concentration By: EH

Supervisor By : rajesh

Extraction Method: ☒ Separatory Funnel

☐ Continuous Liquid/Liquid

☐ Sonication

☐ Waste Dilution

☐ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	50/100 PPM	SP6794
Surrogate	1.0ML	100/150 PPM	SP6754
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Methylene Chloride	N/A	E3939
Baked Na2SO4	N/A	EP2620
H2SO4 1:1	N/A	EP2610
10N NaOH	N/A	EP2609
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

1.5 ML Vial lot# 2210443. pH Adjusted<2 with 1:1 H2SO4 &>11 with 10 N NaOH.

KD Bath ID: WATER BATH-1,2

Envap ID: NE VAP-02

KD Bath Temperature: 60 °C


Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
6/6/25	RS (Ext-9th)	J4/SVOC
1h-20	Preparation Group	Analysis Group

Analytical Method: M3510C,3580A-Extraction SVOC-20

Concentration Date: 06/06/2025

Sample ID	Client Sample ID	Test	g / mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB168340BL	PB168340BL	SPLP BNA Group1	1000	6	RUPESH	ritesh	1			SEP-1
PB168340BS	PB168340BS	SPLP BNA Group1	1000	6	RUPESH	ritesh	1			2
PB168340TB	PB168340TB	SPLP BNA Group1	1000	6	RUPESH	ritesh	1			3
Q2125-08	GSB3	SPLP BNA Group1	1000	6	RUPESH	ritesh	1	A		4
Q2125-08MS	GSB3MS	SPLP BNA Group1	1000	6	RUPESH	ritesh	1	A		5
Q2125-08MS D	GSB3MSD	SPLP BNA Group1	1000	6	RUPESH	ritesh	1	A		6

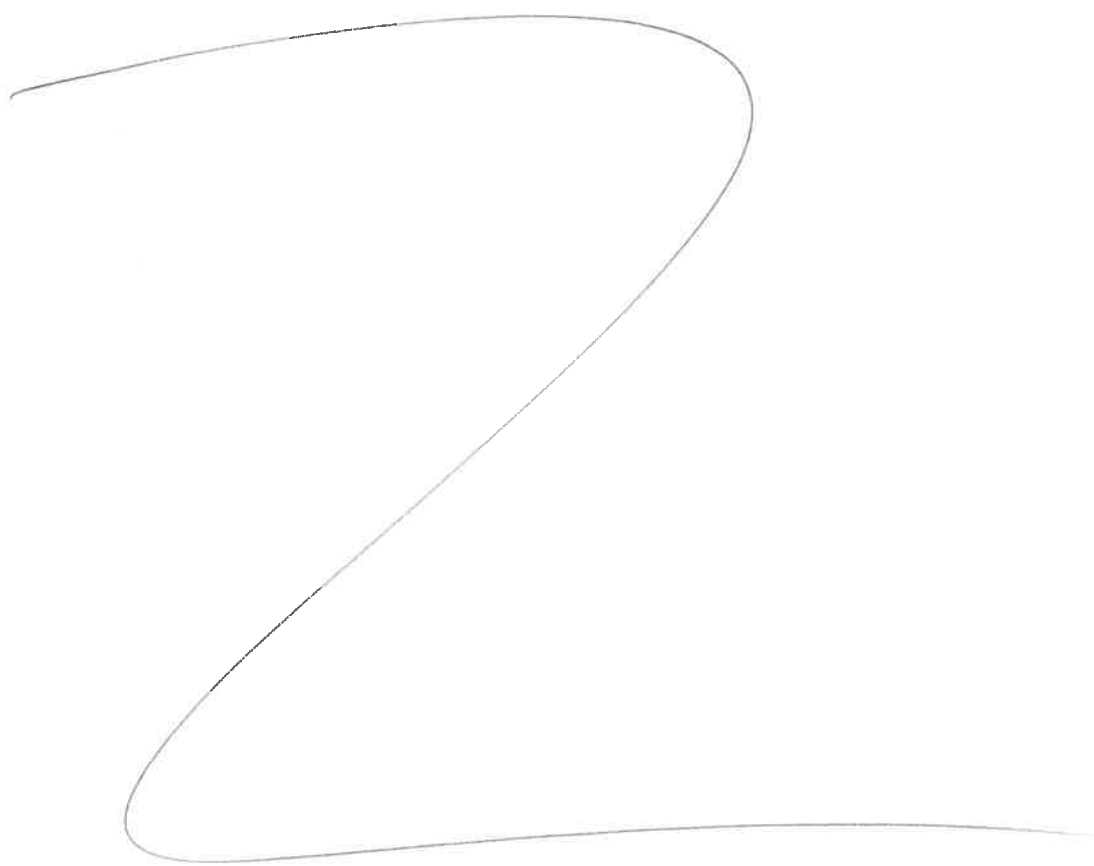

RS
6/6

* Extracts relinquished on the same date as received.