


h	Instrument IC-1				Analyst: NF		Method: 300.0 / 9056A		Initial Analyst	
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/22/2025 11:09	10 NF/IZ
STD2	0.430	0.640	0.649	2.129	0.543	1.098	3.287	IC1-052225	5/22/2025 11:30	10 NF/IZ
STD3	0.795	1.207	1.205	4.018	1.004	1.867	6.069	IC1-052225	5/22/2025 11:52	10 NF/IZ
STD4	0.977	1.480	1.479	4.929	1.229	2.477	7.415	IC1-052225	5/22/2025 12:13	10 NF/IZ
STD5	1.991	2.968	2.960	9.916	2.467	5.110	14.621	IC1-052225	5/22/2025 12:35	10 NF/IZ
STD6	4.001	5.967	5.959	19.868	4.966	9.870	29.848	IC1-052225	5/22/2025 12:56	10 NF/IZ
STD7	5.006	7.539	7.548	25.140	6.290	12.578	37.260	IC1-052225	5/22/2025 13:17	10 NF/IZ
ICV	2.054	3.101	3.056	10.229	2.610	5.286	15.128	IC1-052225	5/22/2025 13:39	10 NF/IZ
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/22/2025 14:22	10 NF/IZ
CCV	2.173	3.234	3.183	10.665	2.719	5.177	15.946	IC1-052225	5/28/2025 11:29	10 NF/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/28/2025 11:51	10 NF/IZ
LB135928BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/28/2025 12:12	10 NF/IZ
LB135928BSW	2.169	3.277	3.196	10.743	2.741	5.407	15.912	IC1-052225	5/28/2025 13:29	10 NF/IZ
Q2126-08	0.429	0.652	0.665	2.168	0.555	1.098	3.376	IC1-052225	5/28/2025 13:51	10 NF/IZ
Q2126-07	0.227	0.350	0.365	1.172	0.300	0.580	1.871	IC1-052225	5/28/2025 14:12	10 NF/IZ
Q2126-07RE 0.25ML	0.131	0.204	0.221	0.677	0.176	0.327	1.162	IC1-052225	5/28/2025 14:34	10 NF/IZ
Q2133-01	0.142	894.317	0.000	0.000	0.058	0.000	23.378	IC1-052225	5/28/2025 14:55	10 NF/IZ
Q2133-02	0.365	6224.982	0.000	0.716	0.117	0.000	40.826	IC1-052225	5/28/2025 15:17	10 NF/IZ
Q2133-03	0.225	297.983	0.080	0.220	1.302	0.000	23.282	IC1-052225	5/28/2025 15:38	10 NF/IZ
Q2133-03MS	2.334	286.238	3.096	10.452	3.847	5.265	38.231	IC1-052225	5/28/2025 16:00	10 NF/IZ
Q2133-03MSD	2.221	287.399	2.997	10.102	3.749	5.143	37.638	IC1-052225	5/28/2025 16:21	10 NF/IZ
CCV	2.052	3.104	3.050	10.194	2.603	5.254	15.139	IC1-052225	5/28/2025 16:43	10 NF/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/28/2025 17:05	10 NF/IZ
Q2133-01DLX100	0.000	5.817	0.000	0.000	0.000	0.000	0.683	IC1-052225	5/28/2025 17:26	10 NF/IZ
Q2133-02DLX100	0.000	46.339	0.000	0.000	0.000	0.000	0.839	IC1-052225	5/28/2025 18:09	10 NF/IZ
Q2133-02DL2X1000	0.000	3.856	0.000	0.000	0.000	0.000	0.490	IC1-052225	5/28/2025 18:52	10 NF/IZ
Q2133-0DLX100	0.000	2.061	0.000	0.000	0.060	0.000	0.651	IC1-052225	5/28/2025 19:35	10 NF/IZ
CCV	2.066	3.109	3.057	10.203	2.604	5.259	15.206	IC1-052225	5/28/2025 19:56	10 NF/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/28/2025 20:18	10 NF/IZ

Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A									
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	Initial wt/ Final
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-052225	10 NF/IZ
STD2	0.4300	0.6400	0.6490	2.1290	0.5430	1.0980	3.2870	IC1-052225	10 NF/IZ
STD3	0.7950	1.2070	1.2050	4.0180	1.0040	1.8670	6.0690	IC1-052225	10 NF/IZ
STD4	0.9770	1.4800	1.4790	4.9290	1.2290	2.4770	7.4150	IC1-052225	10 NF/IZ
STD5	1.9910	2.9680	2.9600	9.9160	2.4670	5.1100	14.6210	IC1-052225	10 NF/IZ
STD6	4.0010	5.9670	5.9590	19.8680	4.9660	9.8700	29.8480	IC1-052225	10 NF/IZ
STD7	5.0060	7.5390	7.5480	25.1400	6.2900	12.5780	37.2600	IC1-052225	10 NF/IZ
True Value CL- NO2 BR- NO3 HPO4 SO4									
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1	7.5000	6.6667	8.1667	6.4500	8.6000	9.8000	9.5667		
STD2	-0.6250	0.5833	0.4167	0.4500	0.4000	-6.6500	1.1500		
STD3	-2.3000	-1.3333	-1.4000	-1.4200	-1.6800	-0.9200	-1.1333		
STD4	-0.4500	-1.0667	-1.3333	-0.8400	-1.3200	2.2000	-2.5267		
STD5	0.0250	-0.5500	-0.6833	-0.6600	-0.6800	-1.3000	-0.5067		
STD6	0.1200	0.5200	0.6400	0.5600	0.6400	0.6240	0.7027		

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

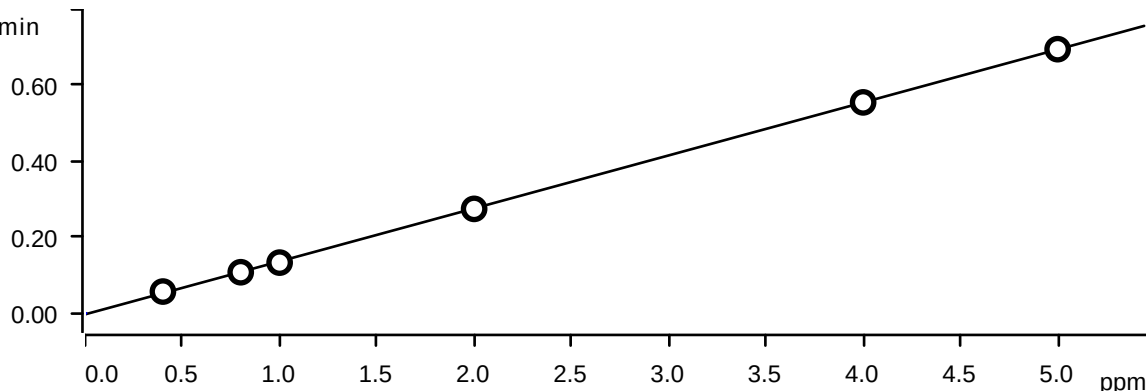

Function: $A = -2.82659E-3 + 0.0139492 \times Q$


Relative standard deviation 0.920519 %

Correlation coefficient 0.999955

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.057	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.108	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.133	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.275	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.555	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.695	STD7	2025-05-22 13:17:57 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

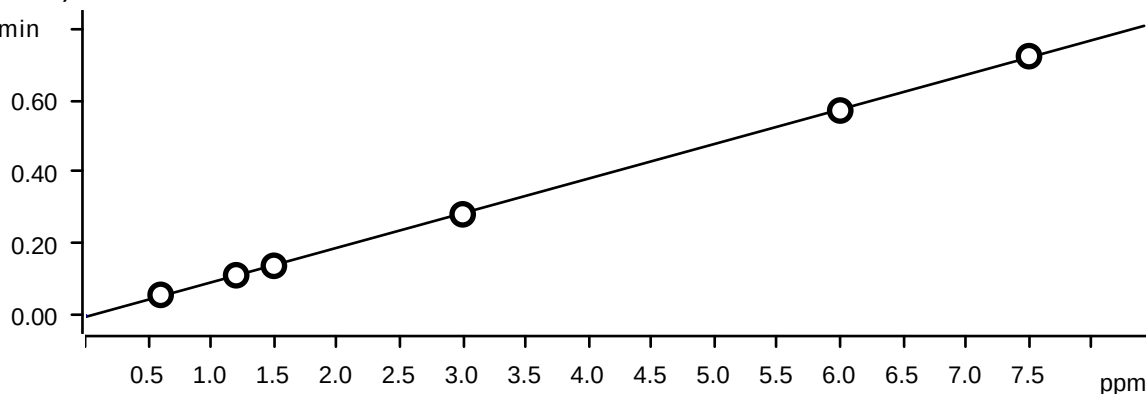

Function: $A = -4.33057E-3 + 9.64673E-3 \times Q$


Relative standard deviation 1.154335 %

Correlation coefficient 0.999929

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.057	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.112	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.138	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.282	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.571	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.723	STD7	2025-05-22 13:17:57 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

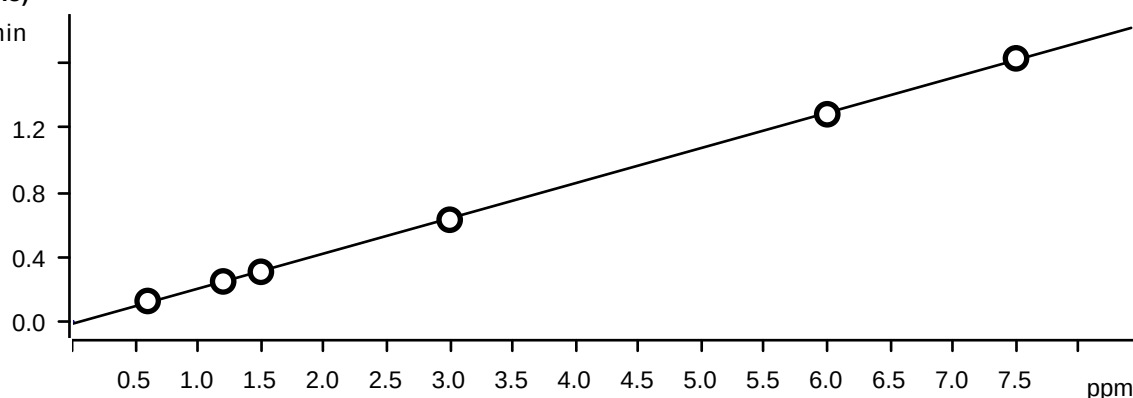Function: $A = -0.0150155 + 0.0217890 \times Q$


Relative standard deviation 1.428639 %

Correlation coefficient 0.999893

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.126	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.248	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.307	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.630	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.283	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.630	STD7	2025-05-22 13:17:57 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

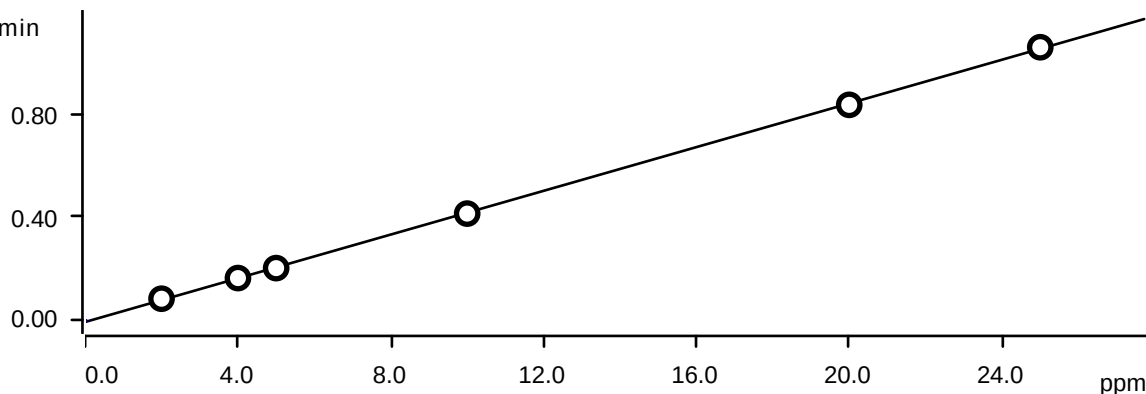

Function: $A = -6.27114E-3 + 4.23162E-3 \times Q$


Relative standard deviation: 1.185575 %

Correlation coefficient: 0.999925

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.084	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.164	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.202	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.413	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.834	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.058	STD7	2025-05-22 13:17:57 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

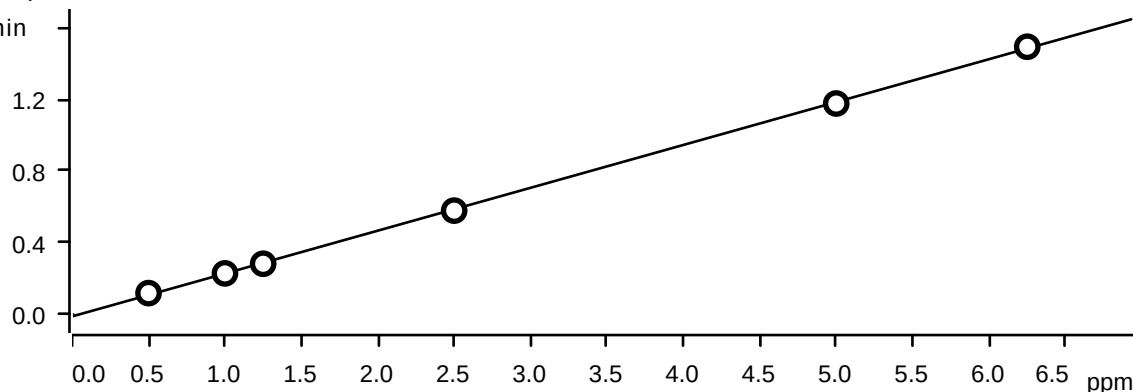


Function: $A = -0.0109593 + 0.0239055 \times Q$

Relative standard deviation: 1.451672 %

Correlation coefficient 0.999889


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.119	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.229	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.283	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.579	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.176	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.493	STD7	2025-05-22 13:17:57 UTC-4	used

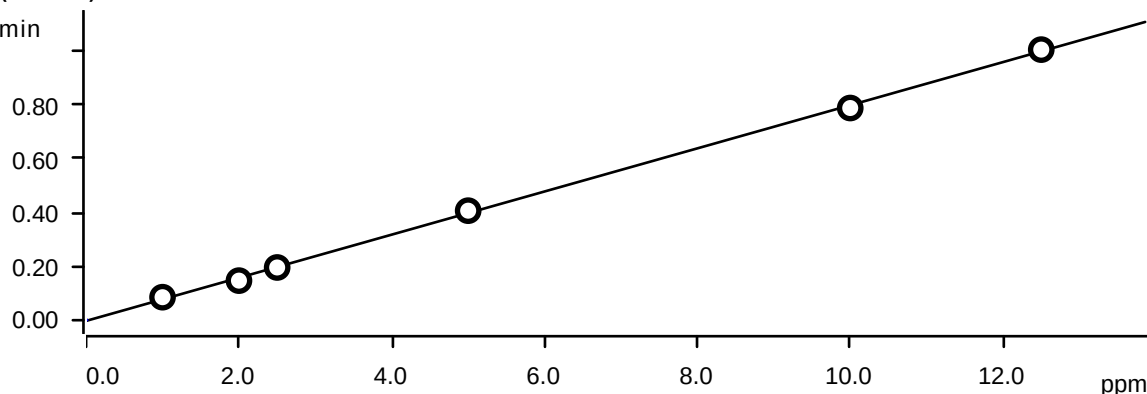Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.02035E-3 + 8.01761E-3 \times Q$

Relative standard deviation 2.297726 %

Correlation coefficient 0.999716

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.085	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.147	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.196	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.407	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.788	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.005	STD7	2025-05-22 13:17:57 UTC-4	used

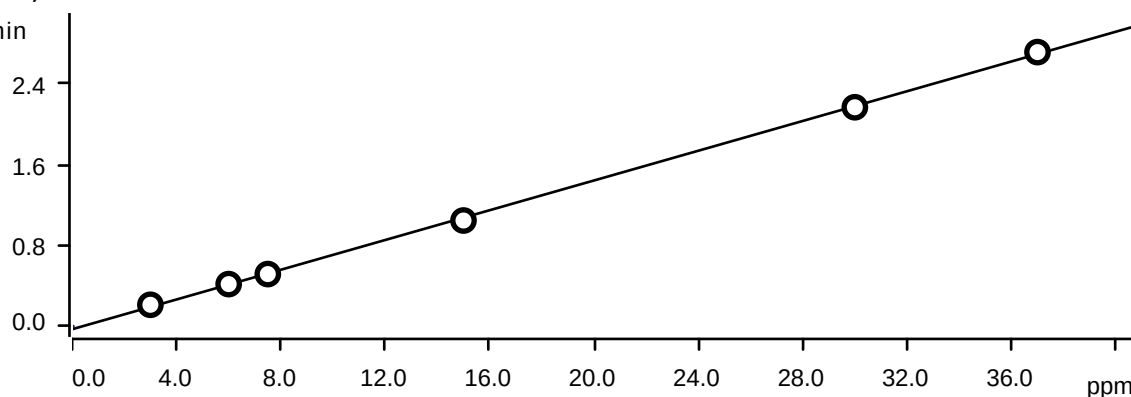Sulfate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0303663 + 7.37295E-3 \times Q$

Relative standard deviation 1.792871 %

Correlation coefficient 0.999832


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.212	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.417	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.516	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.048	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.170	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.717	STD7	2025-05-22 13:17:57 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-05-22 11:09:38 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

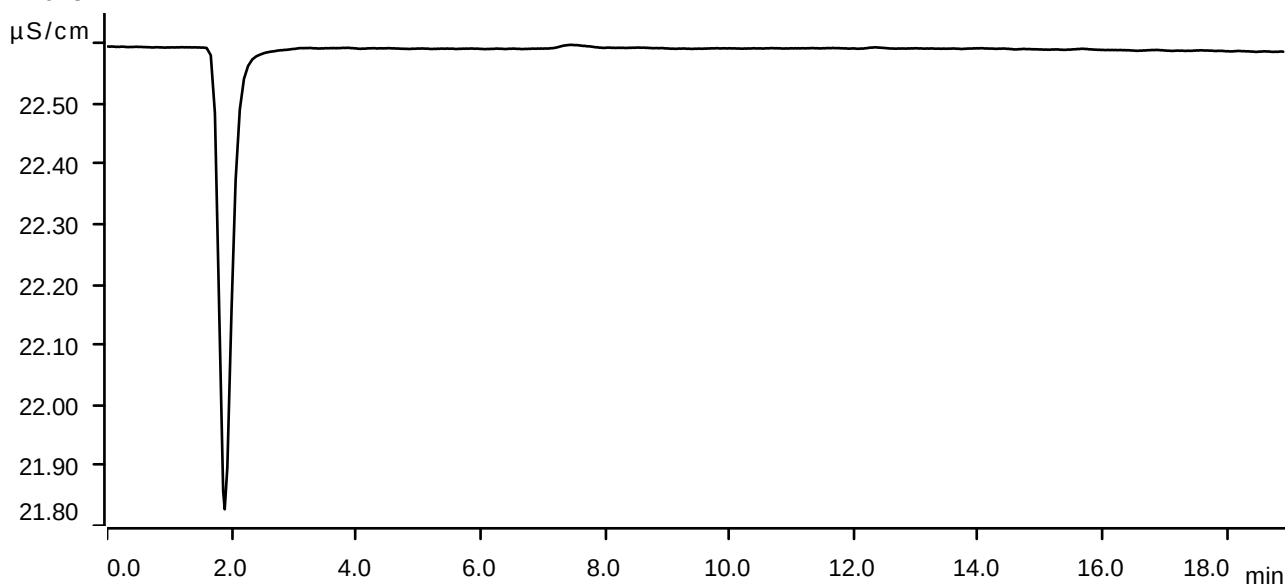Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-05-22 11:30:53 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

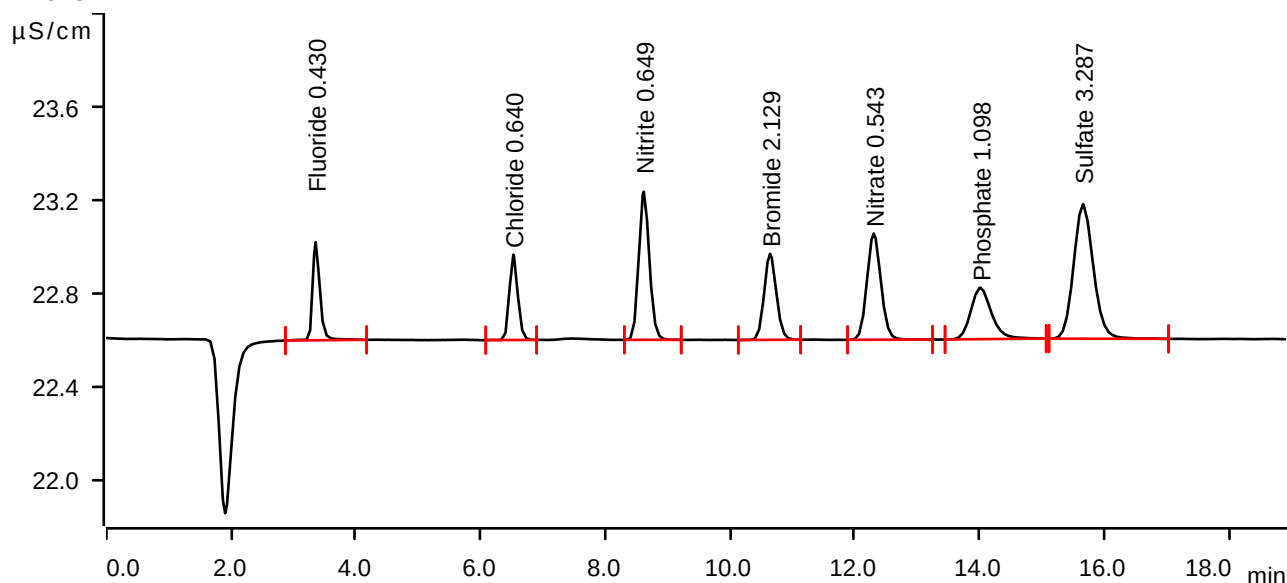

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.0572	0.421	0.430	Fluoride
2	6.525	0.0574	0.366	0.640	Chloride
3	8.617	0.1264	0.636	0.649	Nitrite
4	10.642	0.0838	0.369	2.129	Bromide
5	12.303	0.1190	0.456	0.543	Nitrate
6	14.013	0.0850	0.221	1.098	Phosphate
7	15.657	0.2120	0.577	3.287	Sulfate


Sample data

Ident STD3
 Sample type Standard 3
 Determination start 2025-05-22 11:52:16 UTC-4
 Method IC1-052225
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.71 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

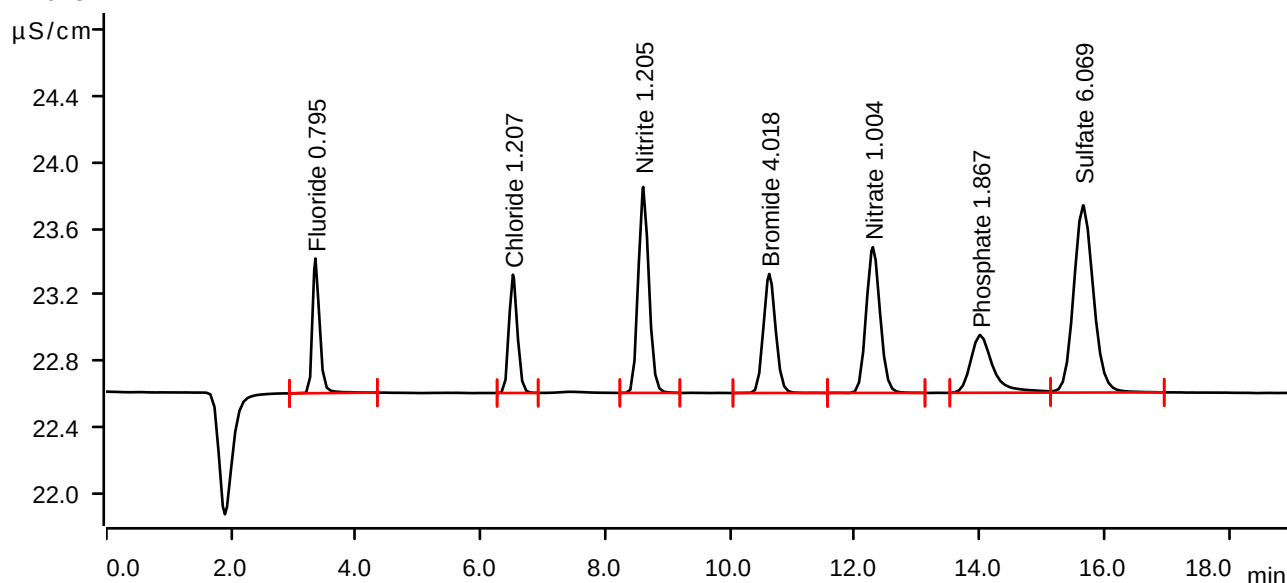

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.1081	0.814	0.795	Fluoride
2	6.518	0.1121	0.716	1.207	Chloride
3	8.608	0.2475	1.247	1.205	Nitrite
4	10.628	0.1637	0.720	4.018	Bromide
5	12.290	0.2290	0.882	1.004	Nitrate
6	14.008	0.1467	0.350	1.867	Phosphate
7	15.660	0.4171	1.133	6.069	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-05-22 12:13:41 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

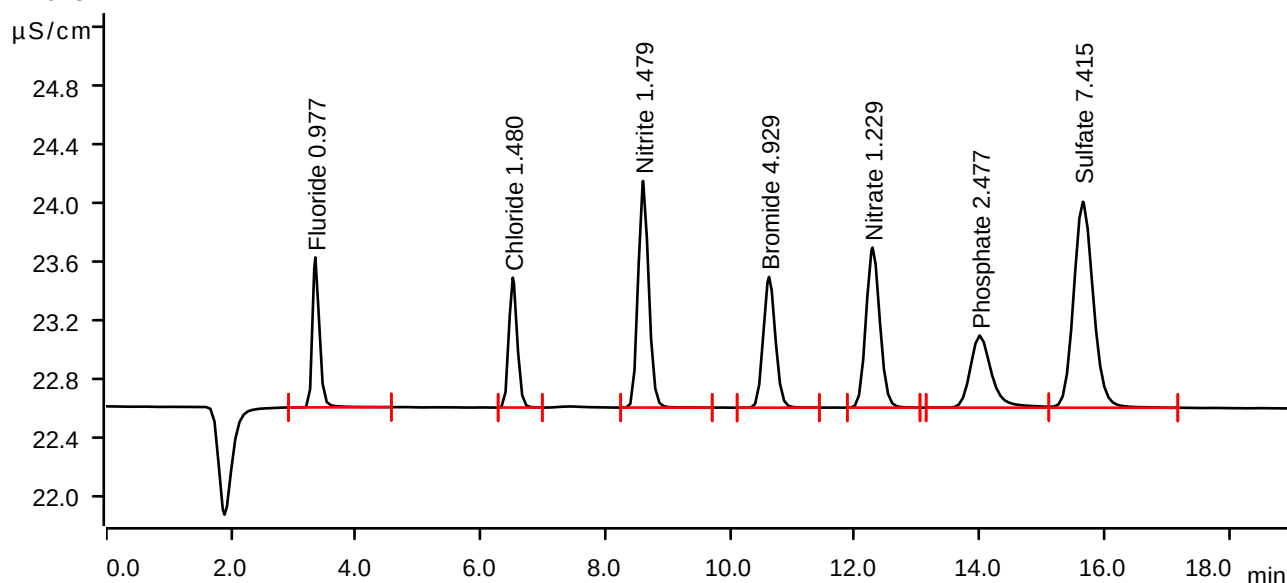

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.1334	1.024	0.977	Fluoride
2	6.517	0.1384	0.888	1.480	Chloride
3	8.607	0.3073	1.549	1.479	Nitrite
4	10.625	0.2023	0.894	4.929	Bromide
5	12.285	0.2828	1.094	1.229	Nitrate
6	14.003	0.1955	0.493	2.477	Phosphate
7	15.657	0.5164	1.408	7.415	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-05-22 12:35:06 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

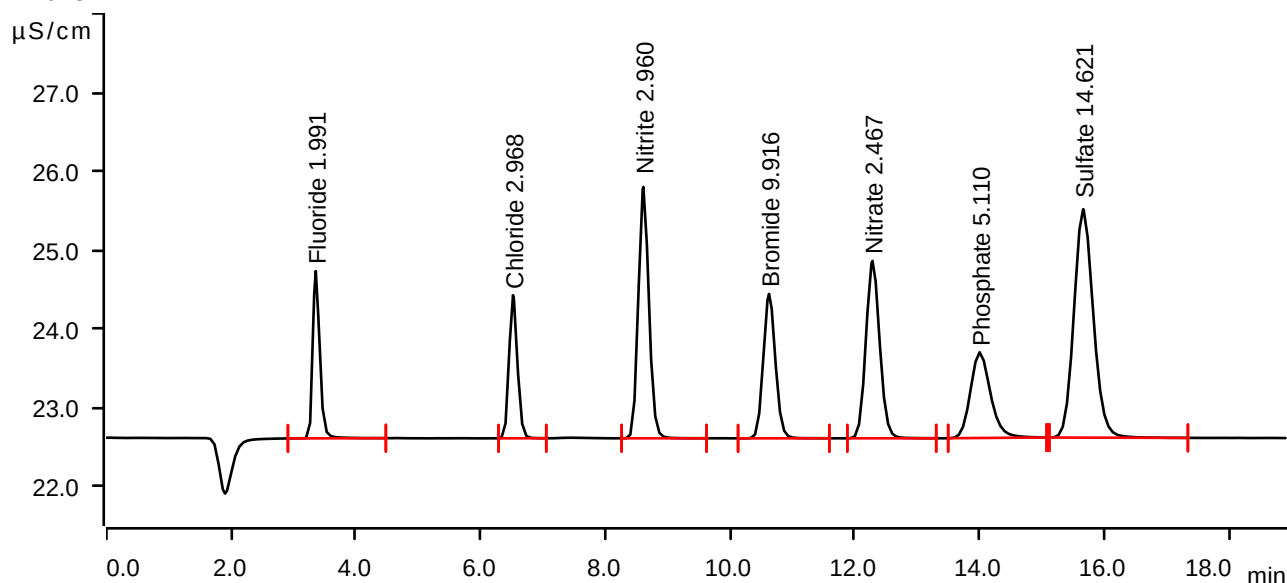

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.2749	2.123	1.991	Fluoride
2	6.520	0.2820	1.816	2.968	Chloride
3	8.610	0.6298	3.190	2.960	Nitrite
4	10.625	0.4133	1.833	9.916	Bromide
5	12.283	0.5789	2.251	2.467	Nitrate
6	14.002	0.4067	1.087	5.110	Phosphate
7	15.660	1.0476	2.898	14.621	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-05-22 12:56:31 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

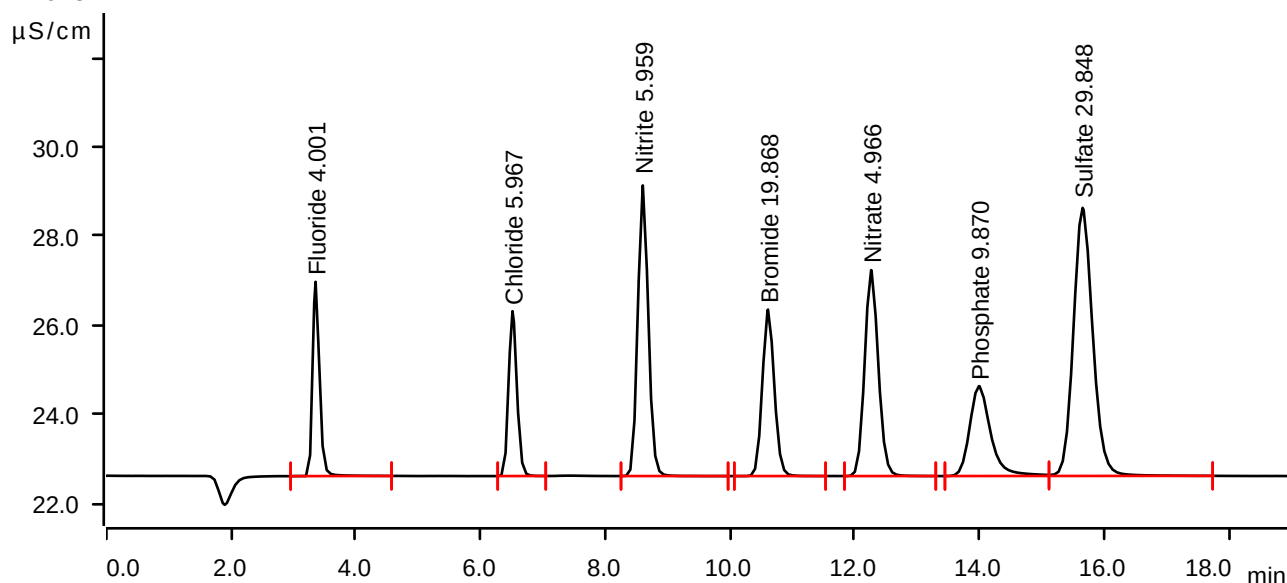

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.5553	4.361	4.001	Fluoride
2	6.512	0.5713	3.701	5.967	Chloride
3	8.602	1.2834	6.525	5.959	Nitrite
4	10.608	0.8345	3.739	19.868	Bromide
5	12.262	1.1762	4.624	4.966	Nitrate
6	13.990	0.7883	2.019	9.870	Phosphate
7	15.652	2.1703	6.019	29.848	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-05-22 13:17:57 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

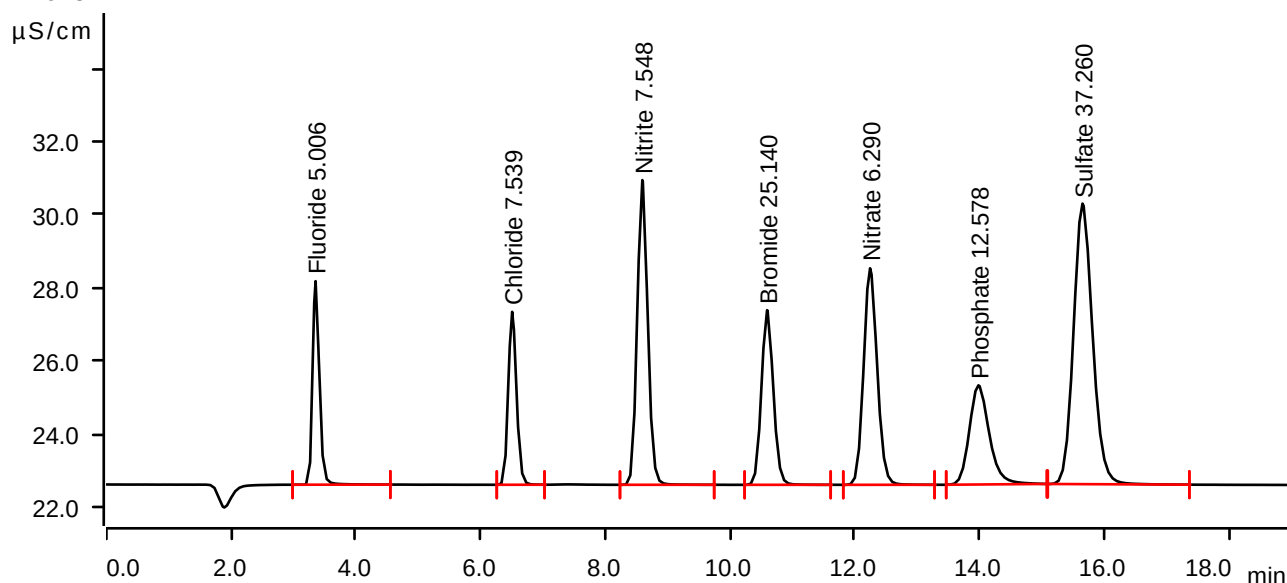

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.6954	5.562	5.006	Fluoride
2	6.507	0.7229	4.726	7.539	Chloride
3	8.593	1.6297	8.328	7.548	Nitrite
4	10.593	1.0576	4.774	25.140	Bromide
5	12.245	1.4927	5.918	6.290	Nitrate
6	13.982	1.0054	2.711	12.578	Phosphate
7	15.650	2.7168	7.668	37.260	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-05-22 13:39:25 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

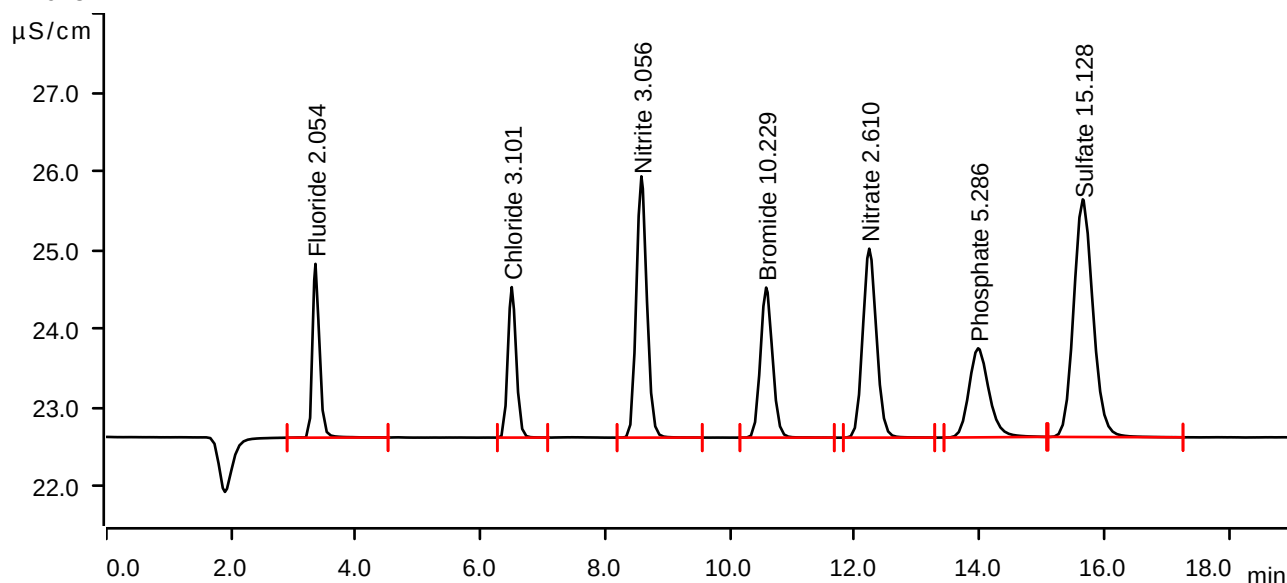


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.2837	2.205	2.054	Fluoride
2	6.500	0.2948	1.910	3.101	Chloride
3	8.578	0.6509	3.316	3.056	Nitrite
4	10.578	0.4266	1.904	10.229	Bromide
5	12.232	0.6129	2.398	2.610	Nitrate
6	13.977	0.4208	1.130	5.286	Phosphate
7	15.655	1.0850	3.016	15.128	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2025-05-22 14:22:21 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

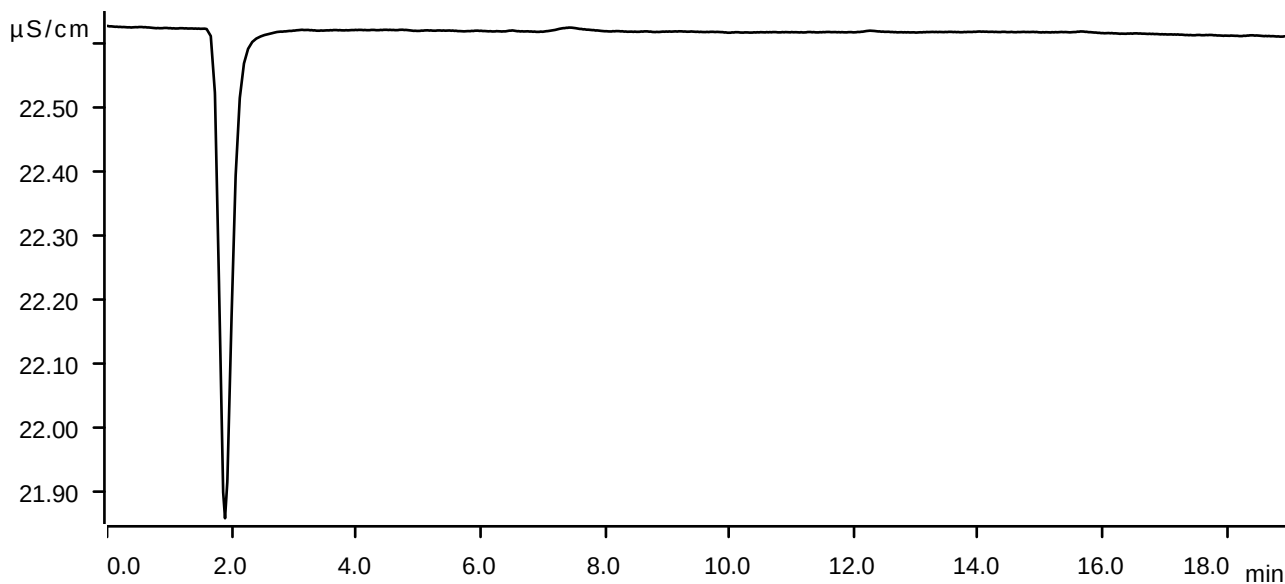Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-05-28 11:29:37 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

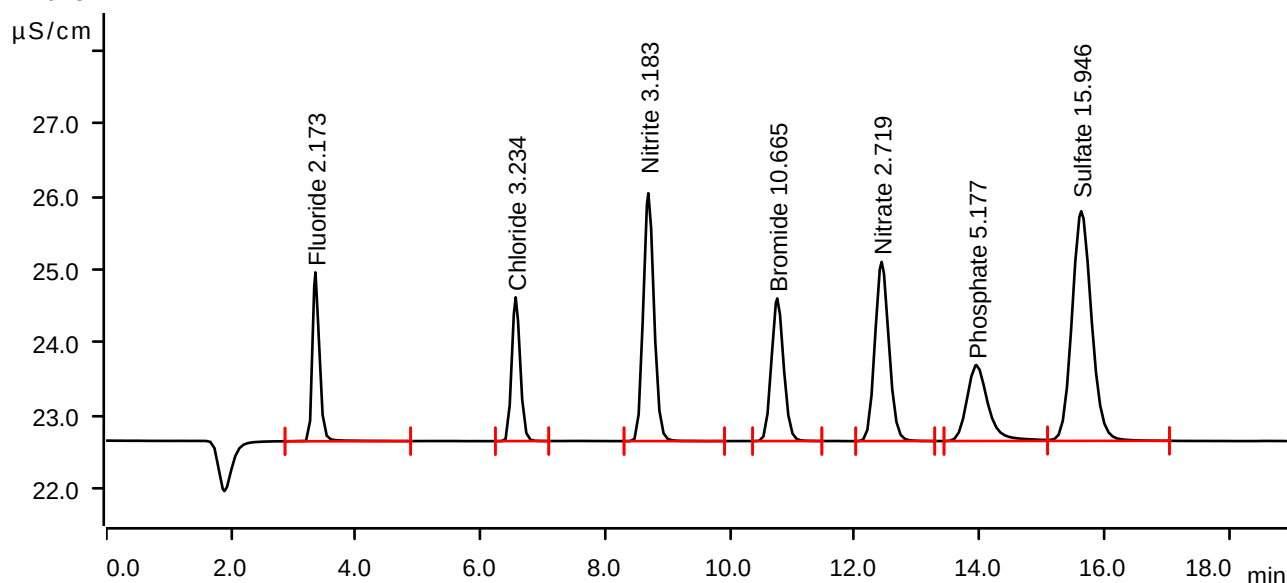


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.3003	2.307	2.173	Fluoride
2	6.563	0.3076	1.965	3.234	Chloride
3	8.690	0.6784	3.387	3.183	Nitrite
4	10.757	0.4450	1.949	10.665	Bromide
5	12.430	0.6390	2.449	2.719	Nitrate
6	13.948	0.4121	1.039	5.177	Phosphate
7	15.630	1.1453	3.138	15.946	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-05-28 11:51:07 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

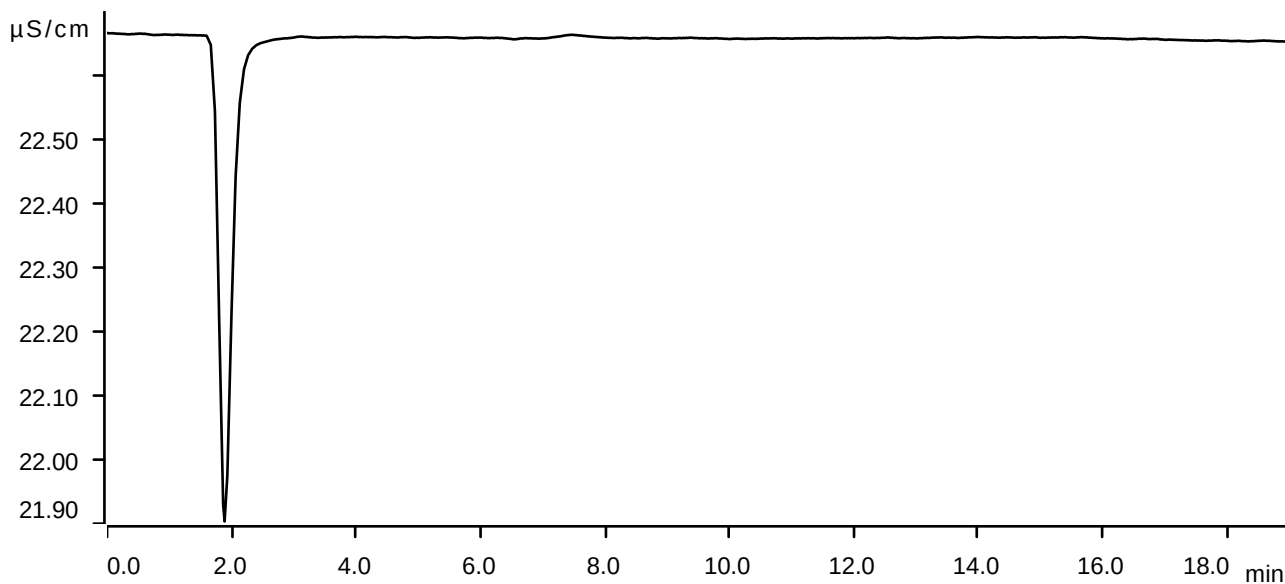Anions


Sample data

Ident LB135928BLW
Sample type Sample
Determination start 2025-05-28 12:12:37 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

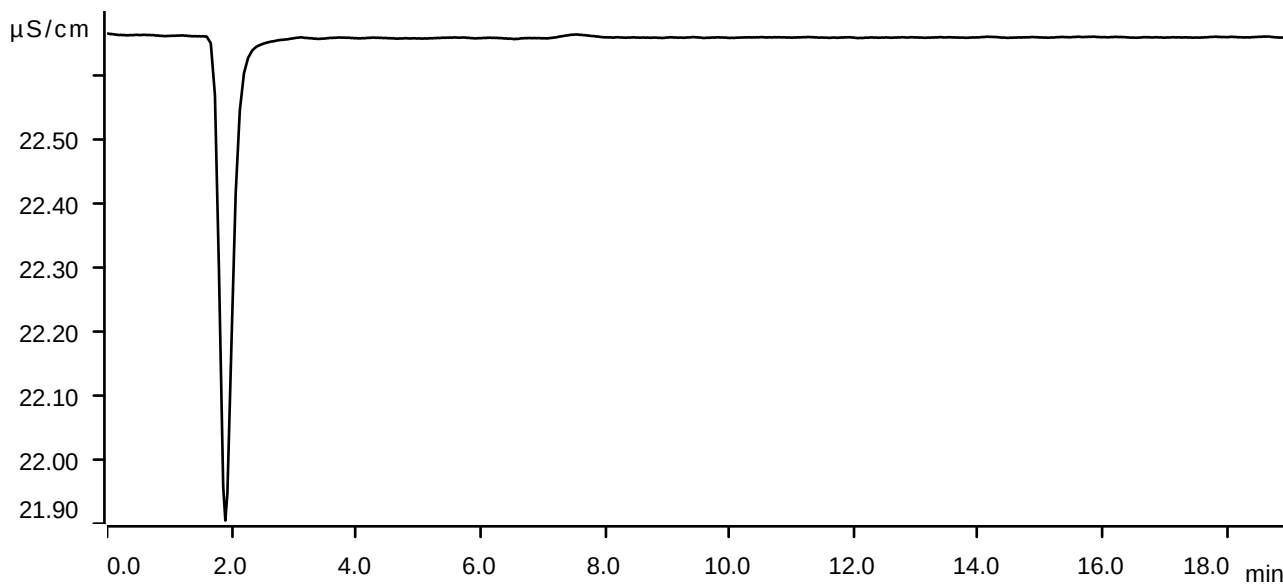


Sample data

Ident LB135928BSW
Sample type Check standard 1
Determination start 2025-05-28 13:29:42 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

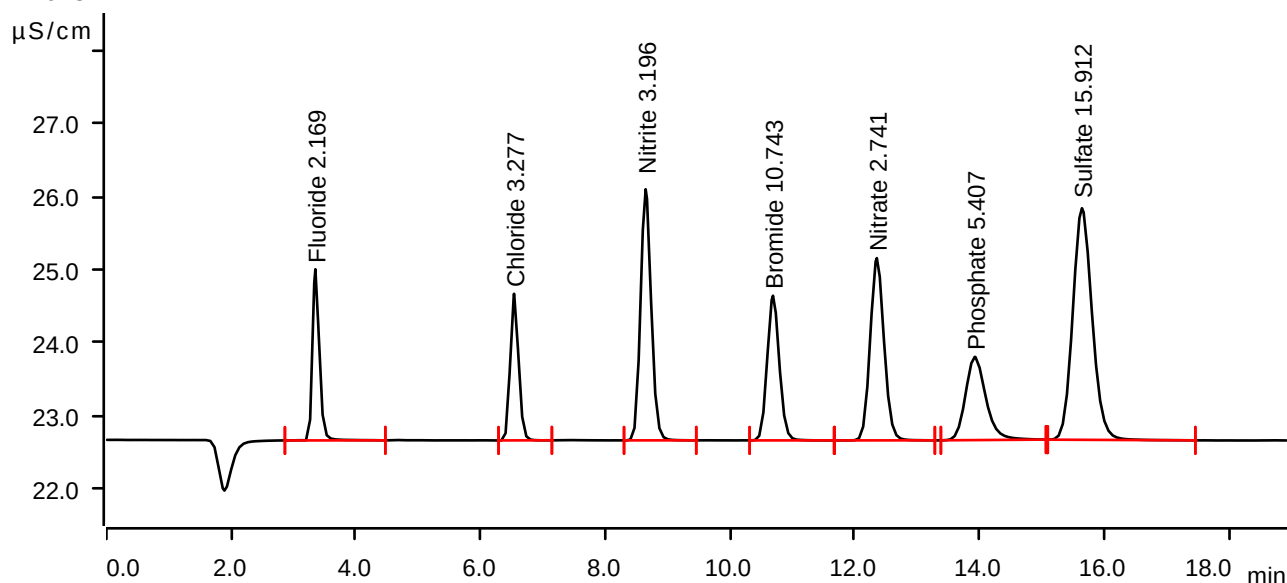

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.2997	2.339	2.169	Fluoride
2	6.538	0.3118	2.003	3.277	Chloride
3	8.647	0.6814	3.431	3.196	Nitrite
4	10.688	0.4483	1.978	10.743	Bromide
5	12.353	0.6443	2.491	2.741	Nitrate
6	13.923	0.4305	1.138	5.407	Phosphate
7	15.642	1.1428	3.165	15.912	Sulfate


Sample data

Ident Q2126-08
Sample type Sample
Determination start 2025-05-28 13:51:14 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

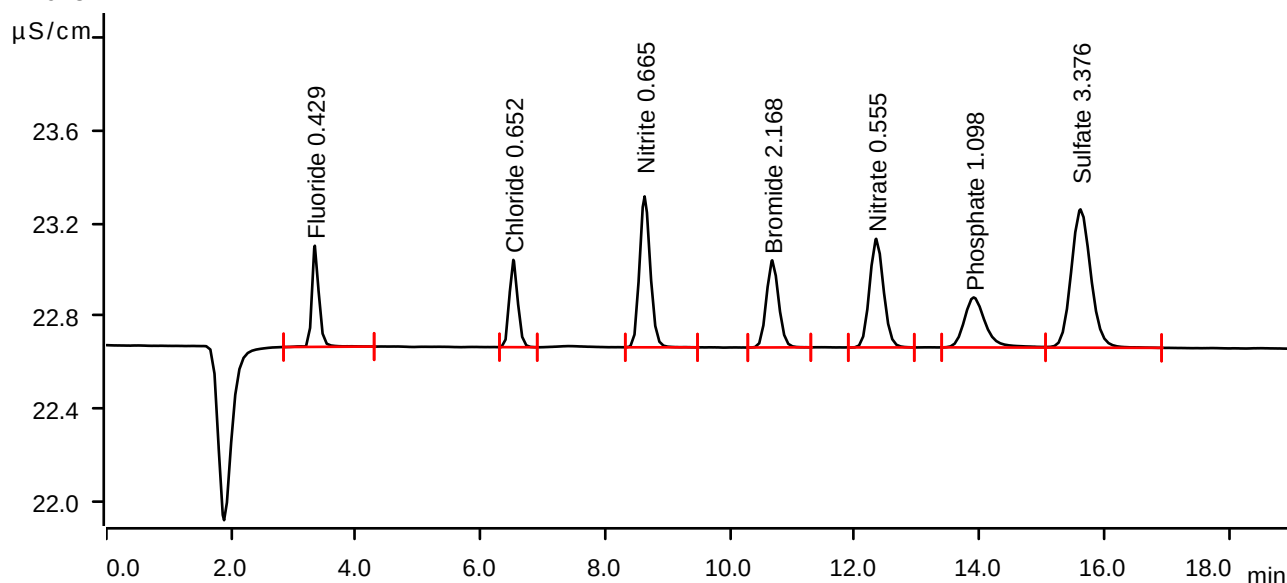

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.343	0.0571	0.434	0.429	Fluoride
2	6.525	0.0586	0.375	0.652	Chloride
3	8.630	0.1299	0.648	0.665	Nitrite
4	10.677	0.0855	0.374	2.168	Bromide
5	12.343	0.1218	0.466	0.555	Nitrate
6	13.907	0.0850	0.215	1.098	Phosphate
7	15.618	0.2185	0.594	3.376	Sulfate


Sample data

Ident Q2126-07
Sample type Sample
Determination start 2025-05-28 14:12:46 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.67 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

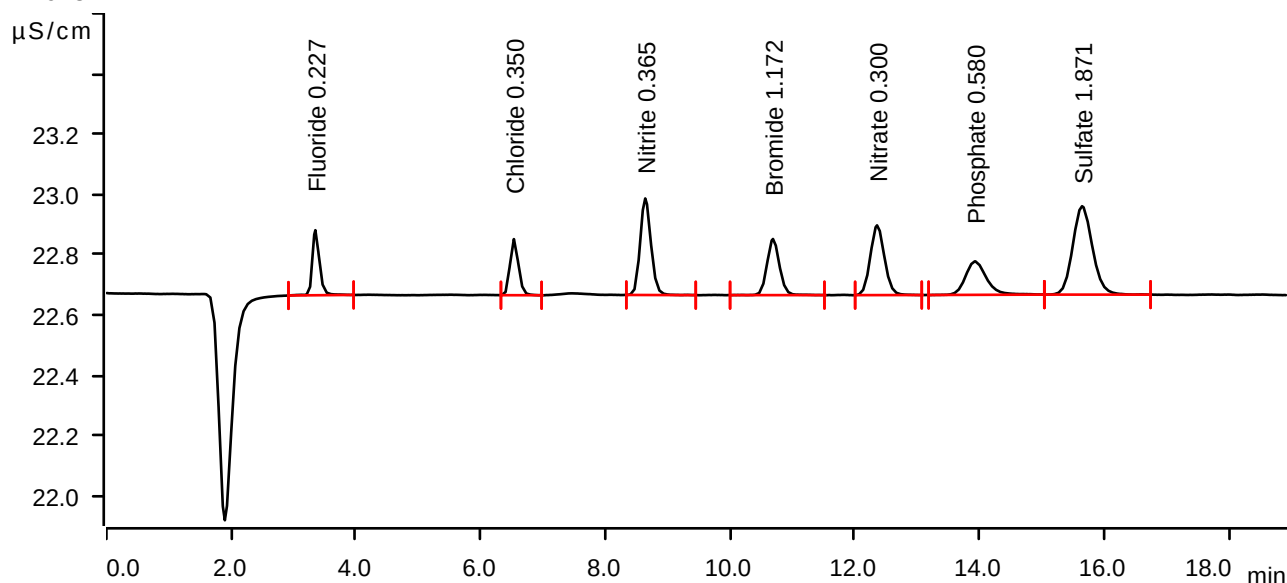

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.0288	0.216	0.227	Fluoride
2	6.535	0.0294	0.186	0.350	Chloride
3	8.640	0.0645	0.320	0.365	Nitrite
4	10.688	0.0433	0.186	1.172	Bromide
5	12.357	0.0609	0.231	0.300	Nitrate
6	13.923	0.0435	0.111	0.580	Phosphate
7	15.643	0.1076	0.294	1.871	Sulfate


Sample data

Ident Q2126-07RE 0.25ML
Sample type Sample
Determination start 2025-05-28 14:34:20 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

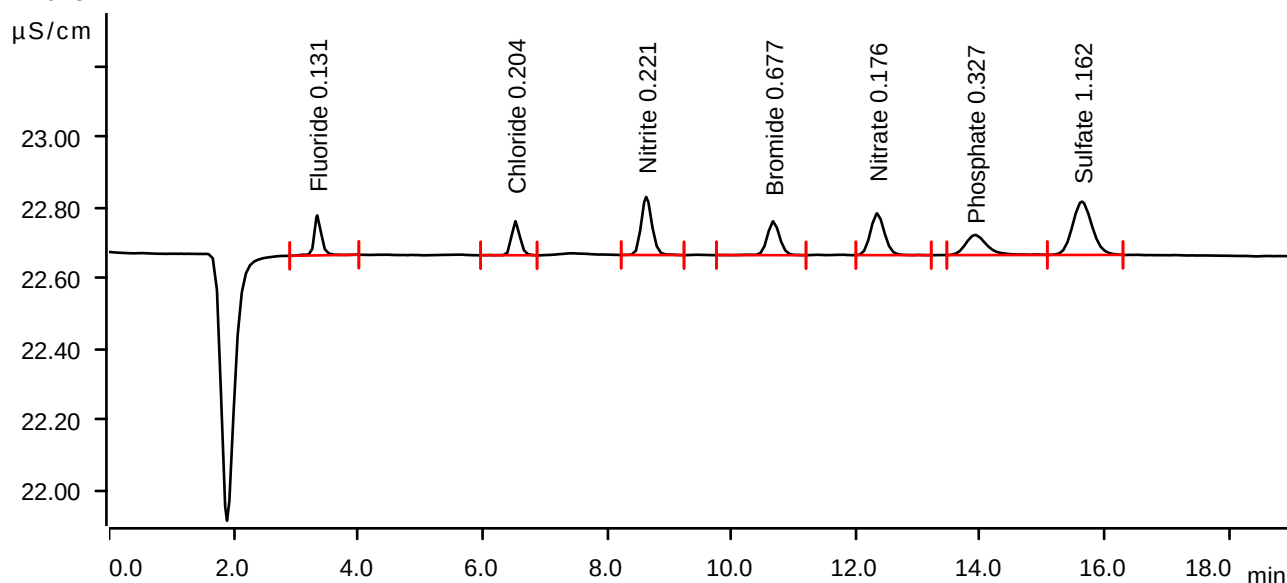

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.347	0.0155	0.113	0.131	Fluoride
2	6.530	0.0154	0.096	0.204	Chloride
3	8.632	0.0332	0.165	0.221	Nitrite
4	10.672	0.0224	0.096	0.677	Bromide
5	12.343	0.0311	0.118	0.176	Nitrate
6	13.910	0.0232	0.057	0.327	Phosphate
7	15.635	0.0553	0.151	1.162	Sulfate


Sample data

Ident Q2133-01
Sample type Sample
Determination start 2025-05-28 14:55:42 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

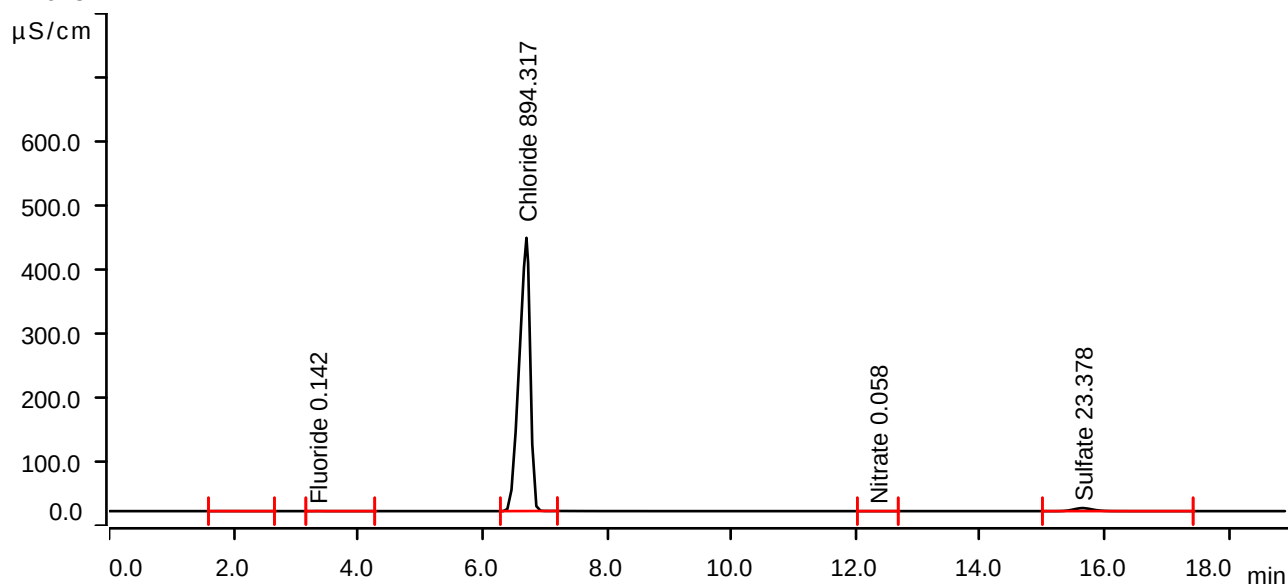

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.843	0.0157	0.056	invalid	
2	3.343	0.0170	0.121	0.142	Fluoride
3	6.708	86.2680	426.735	894.317	Chloride
4	12.350	0.0030	0.011	0.058	Nitrate
5	15.642	1.6933	4.736	23.378	Sulfate


Sample data

Ident Q2133-02
Sample type Sample
Determination start 2025-05-28 15:17:17 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

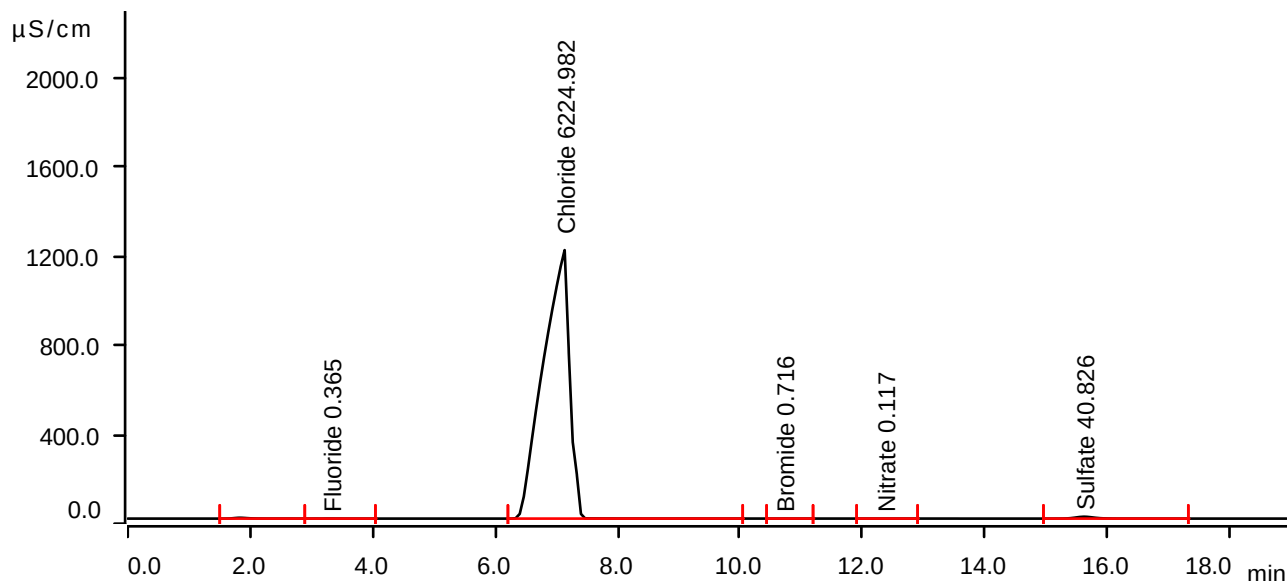

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.832	1.0247	3.812	invalid	
2	3.323	0.0481	0.234	0.365	Fluoride
3	7.135	600.5027	1205.532	6224.982	Chloride
4	10.720	0.0240	0.109	0.716	Bromide
5	12.363	0.0170	0.065	0.117	Nitrate
6	15.615	2.9797	8.397	40.826	Sulfate


Sample data

Ident Q2133-03
Sample type Sample
Determination start 2025-05-28 15:38:51 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

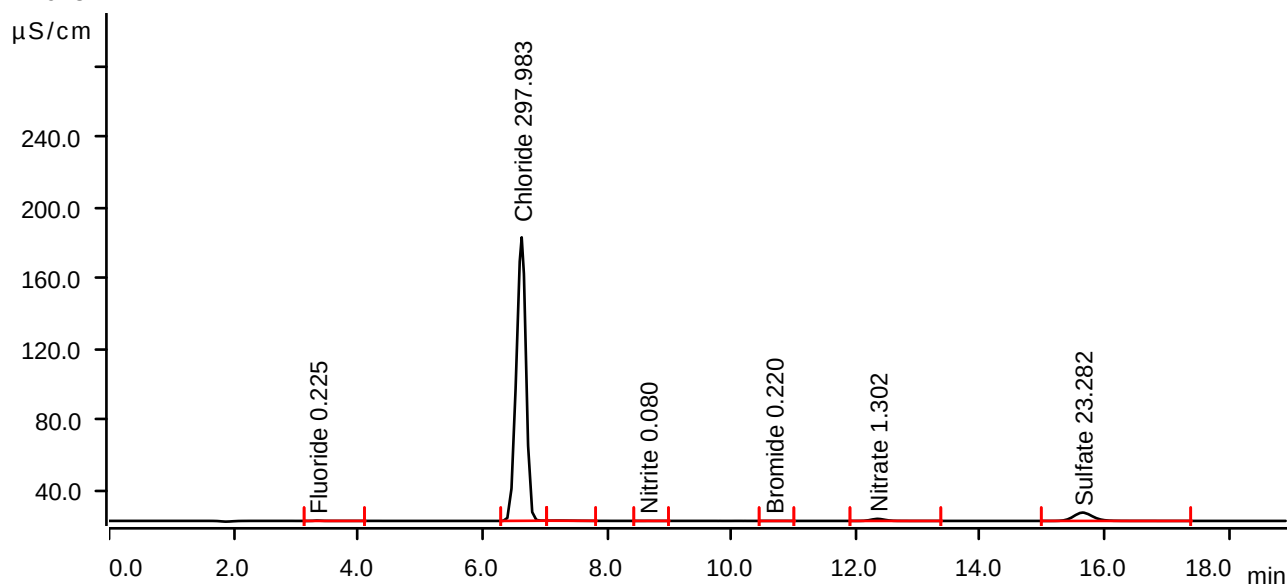

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.345	0.0286	0.194	0.225	Fluoride
2	6.632	28.7413	160.500	297.983	Chloride
3	7.238	0.0275	0.077	invalid	
4	8.652	0.0023	0.012	0.080	Nitrite
5	10.675	0.0031	0.014	0.220	Bromide
6	12.350	0.3003	1.166	1.302	Nitrate
7	15.645	1.6862	4.722	23.282	Sulfate


Sample data

Ident Q2133-03MS
Sample type Sample
Determination start 2025-05-28 16:00:25 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.84 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

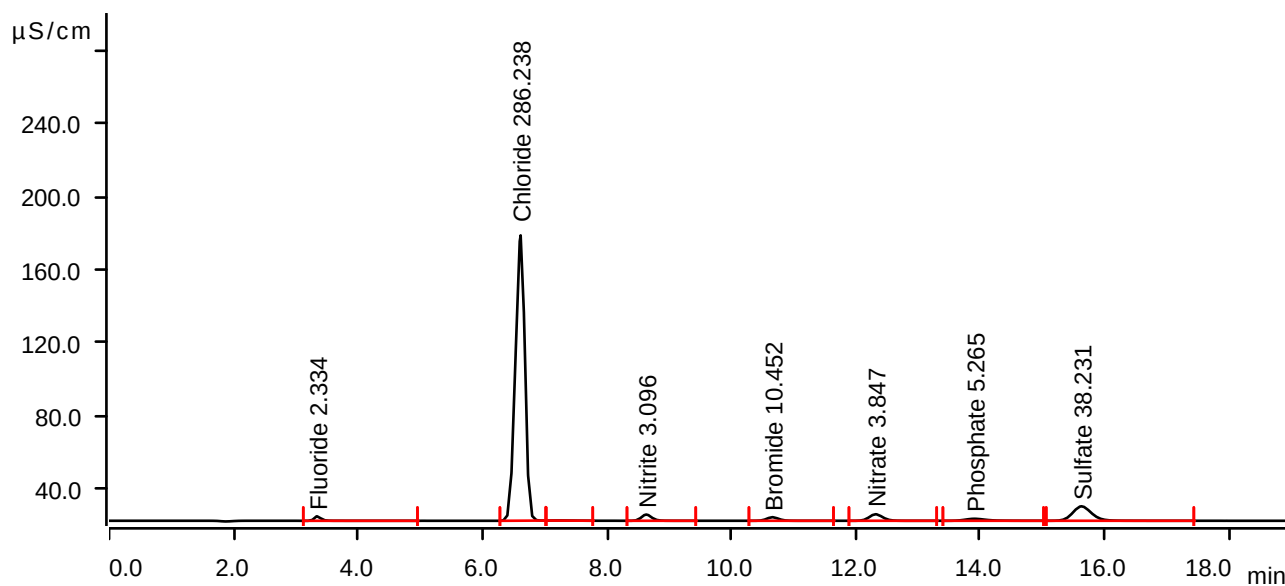

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.343	0.3228	2.452	2.334	Fluoride
2	6.615	27.6083	155.967	286.238	Chloride
3	7.217	0.0257	0.071	invalid	
4	8.633	0.6595	3.400	3.096	Nitrite
5	10.660	0.4360	1.954	10.452	Bromide
6	12.318	0.9087	3.571	3.847	Nitrate
7	13.907	0.4191	1.089	5.265	Phosphate
8	15.627	2.7884	7.899	38.231	Sulfate


Sample data

Ident Q2133-03MSD
Sample type Sample
Determination start 2025-05-28 16:21:57 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

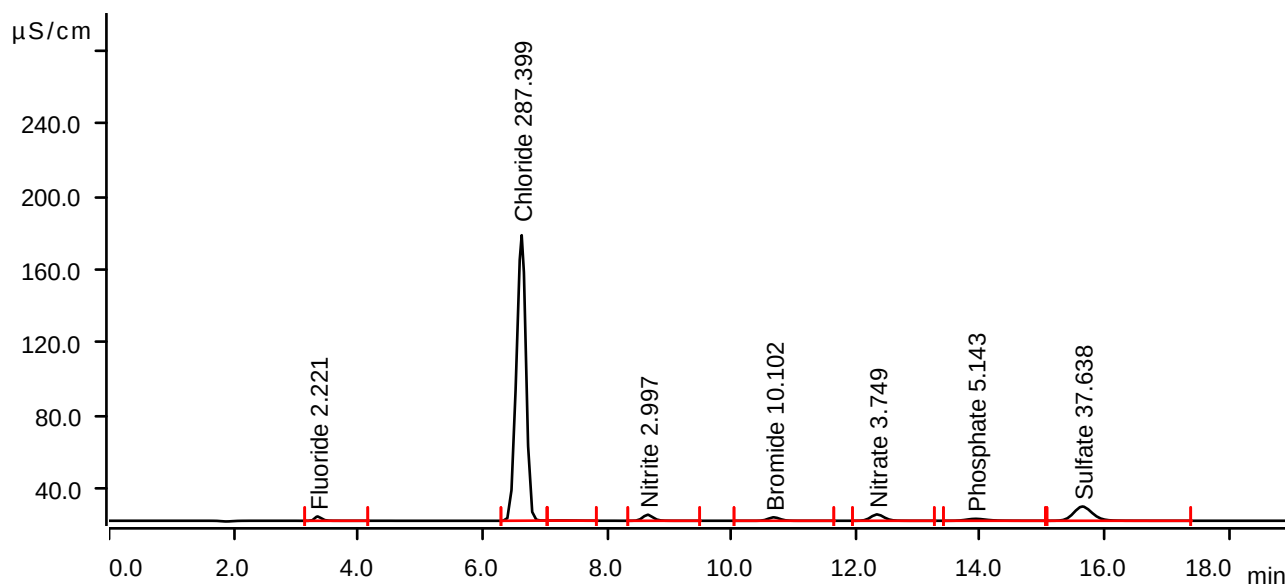

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.3070	2.378	2.221	Fluoride
2	6.632	27.7202	156.048	287.399	Chloride
3	7.242	0.0259	0.072	invalid	
4	8.657	0.6381	3.279	2.997	Nitrite
5	10.682	0.4212	1.886	10.102	Bromide
6	12.342	0.8852	3.479	3.749	Nitrate
7	13.925	0.4093	1.068	5.143	Phosphate
8	15.642	2.7446	7.783	37.638	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-05-28 16:43:30 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

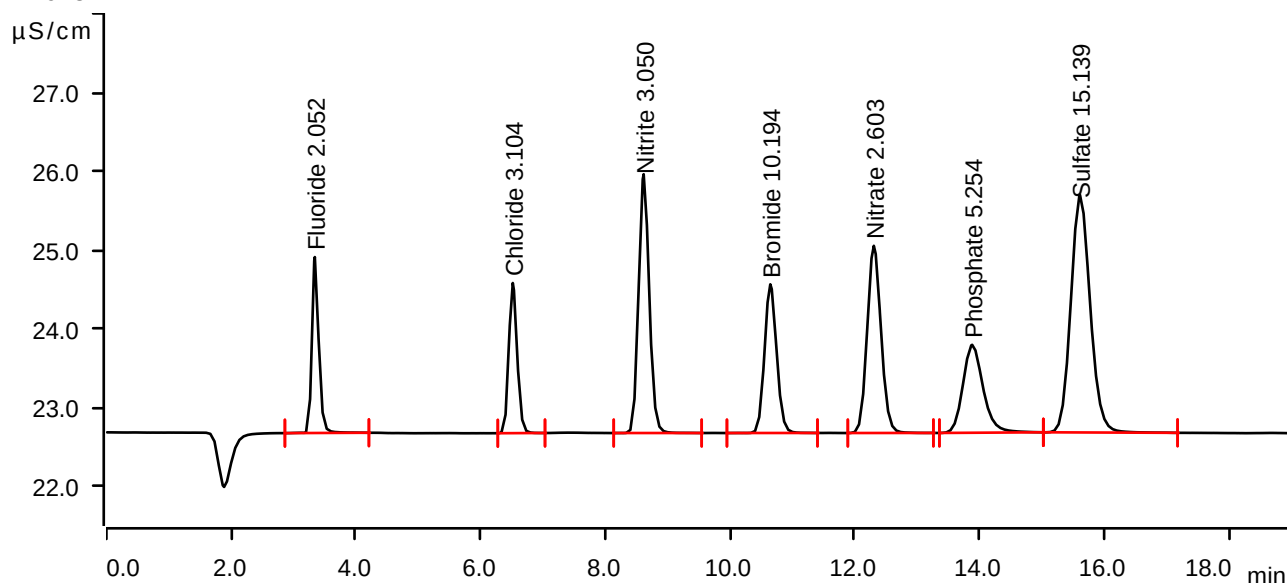


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.343	0.2834	2.232	2.052	Fluoride
2	6.517	0.2951	1.905	3.104	Chloride
3	8.615	0.6495	3.284	3.050	Nitrite
4	10.645	0.4251	1.887	10.194	Bromide
5	12.305	0.6113	2.376	2.603	Nitrate
6	13.882	0.4182	1.116	5.254	Phosphate
7	15.610	1.0858	3.015	15.139	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-05-28 17:05:00 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

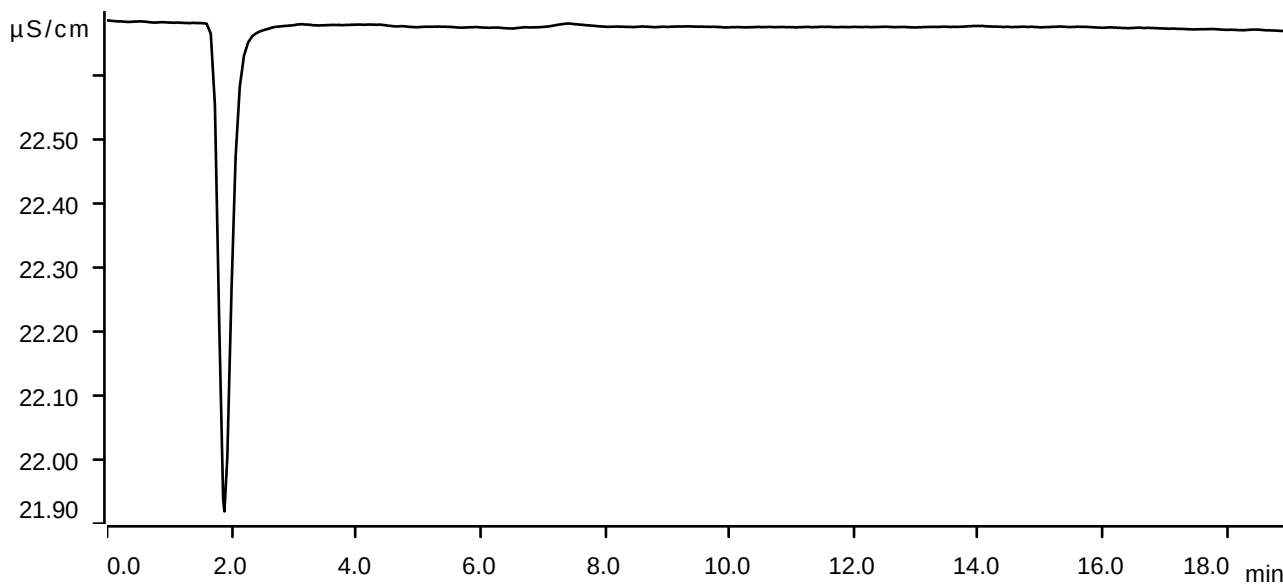Anions


Sample data

Ident Q2133-01DLX100
Sample type Sample
Determination start 2025-05-28 17:26:29 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

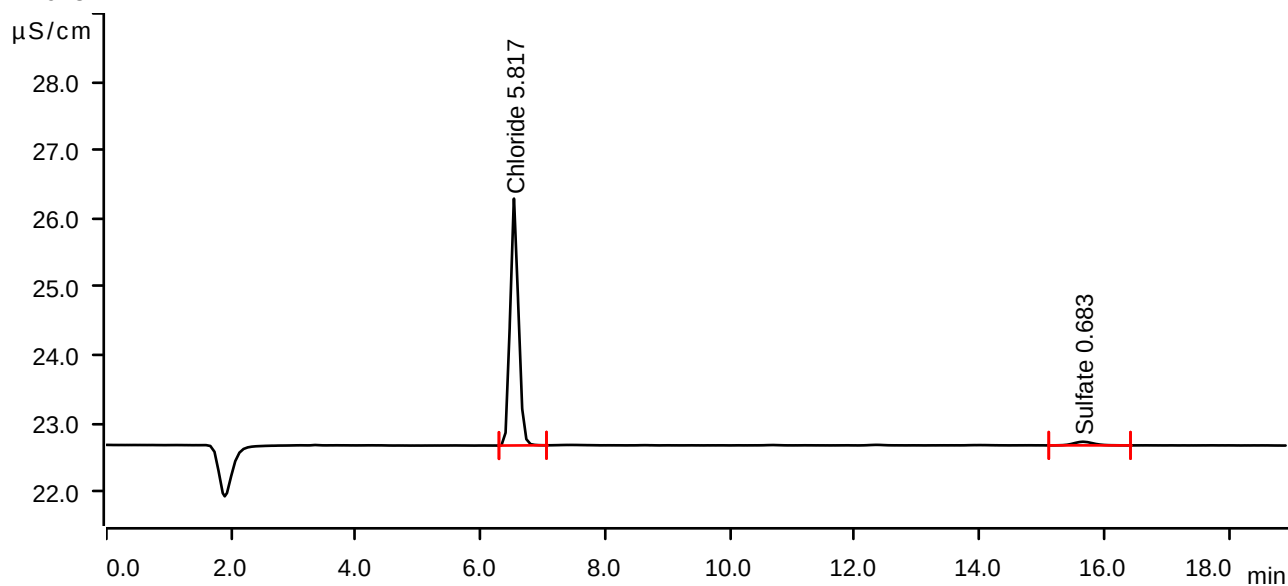

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.537	0.5568	3.615	5.817	Chloride
2	15.653	0.0200	0.053	0.683	Sulfate


Sample data

Ident Q2133-02DLX100
Sample type Sample
Determination start 2025-05-28 18:09:31 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

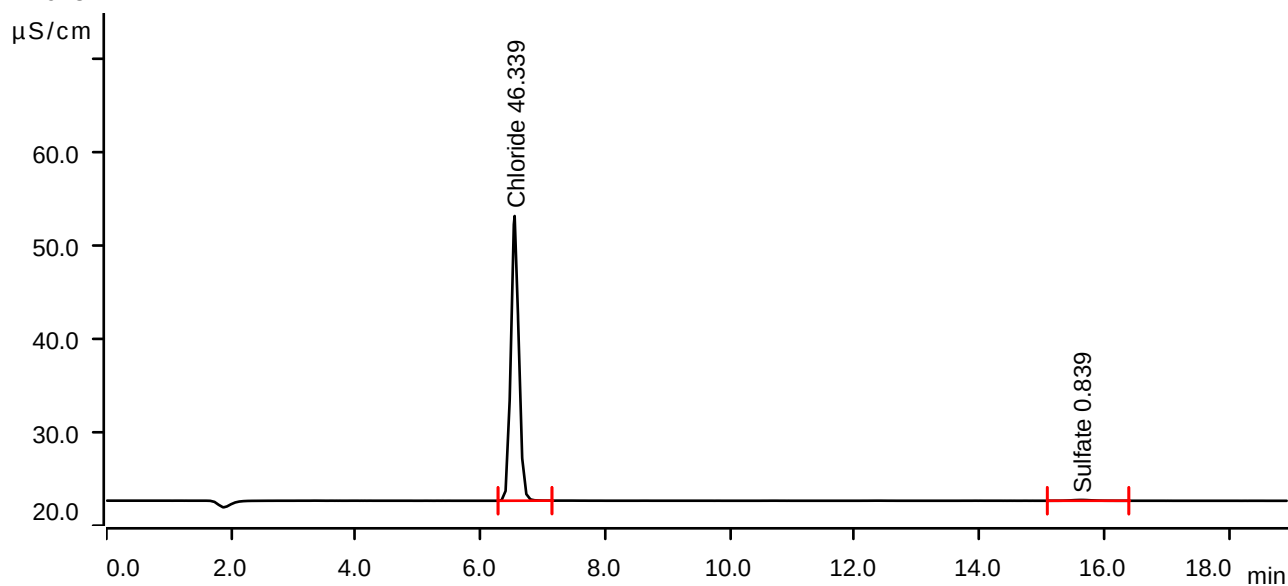

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.547	4.4659	30.568	46.339	Chloride
2	15.625	0.0315	0.085	0.839	Sulfate


Sample data

Ident Q2133-02DL2X1000
Sample type Sample
Determination start 2025-05-28 18:52:28 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.56 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

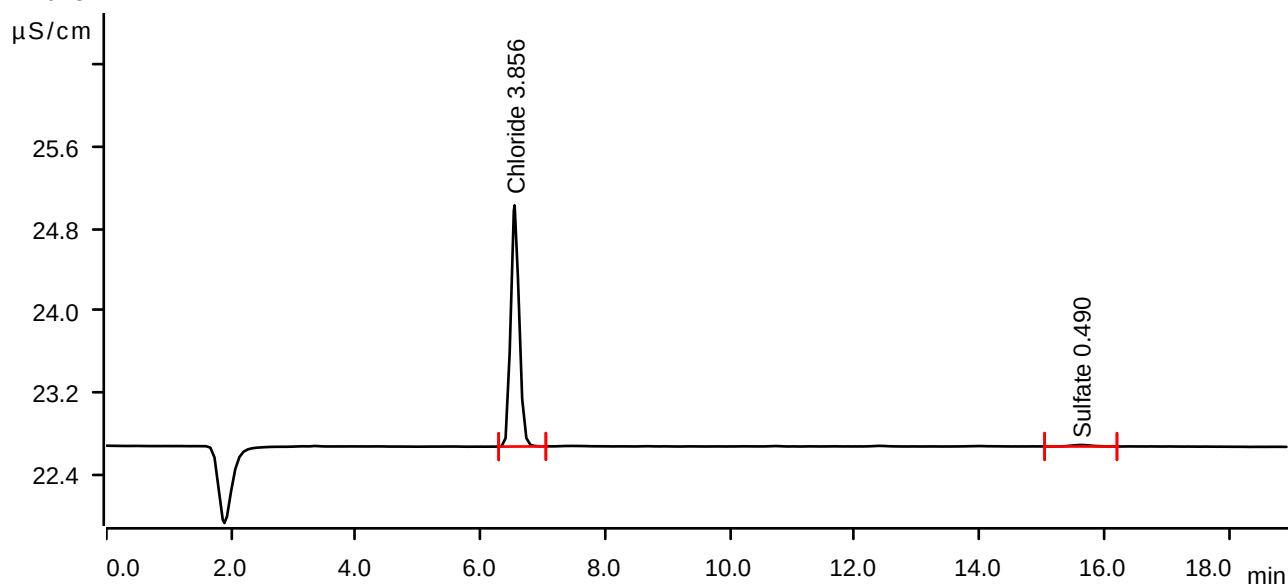

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.547	0.3677	2.355	3.856	Chloride
2	15.618	0.0058	0.015	0.490	Sulfate


Sample data

Ident Q2133-0DLX100
Sample type Sample
Determination start 2025-05-28 19:35:24 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

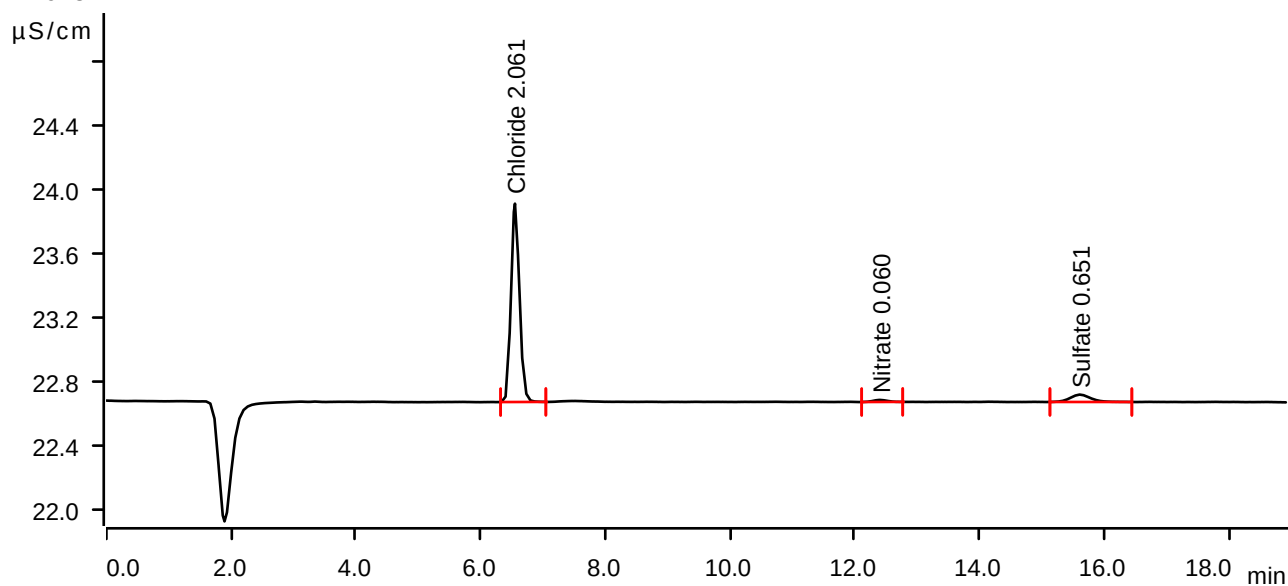

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.552	0.1945	1.239	2.061	Chloride
2	12.405	0.0033	0.013	0.060	Nitrate
3	15.607	0.0176	0.046	0.651	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-05-28 19:56:50 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

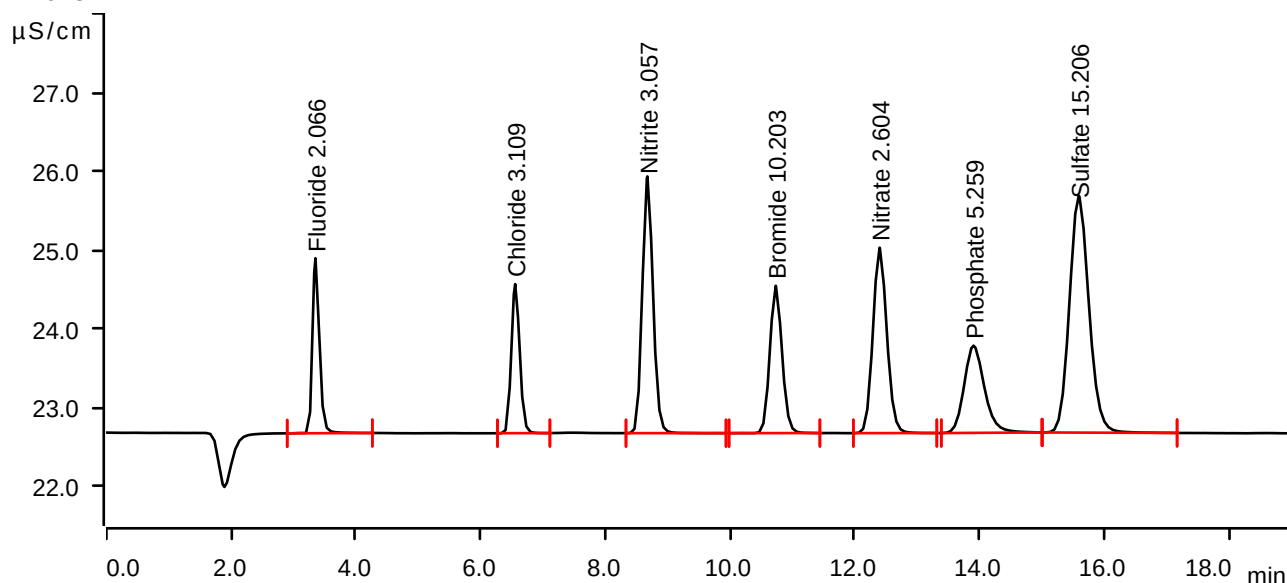

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.2854	2.220	2.066	Fluoride
2	6.555	0.2956	1.892	3.109	Chloride
3	8.675	0.6510	3.258	3.057	Nitrite
4	10.732	0.4255	1.870	10.203	Bromide
5	12.397	0.6116	2.353	2.604	Nitrate
6	13.903	0.4186	1.107	5.259	Phosphate
7	15.590	1.0908	3.005	15.206	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-05-28 20:18:21 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions