

Cover Page

Order ID : Q2133

Project ID : Banker

Client : G Environmental

Lab Sample Number

Q2133-01
Q2133-02
Q2133-03

Client Sample Number

MW1
MW5
SUPPLY

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature : _____

Date: 5/30/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

CASE NARRATIVE

G Environmental

Project Name: Banker

Project # N/A

Order ID # Q2133

Test Name: Anions Group1

A. Number of Samples and Date of Receipt:

3 Water samples were received on 05/28/2025.

B. Parameters:

According to the Chain of Custody document, the following analyses were requested: Anions Group1 and Metals Group4. This data package contains results for Anions Group1.

C. Analytical Techniques:

The analysis of Anions Group1 was based on method 300.0.

D. QA/ QC Samples:

The Holding Times were met for all analysis.

Sample MW1 was diluted due to high concentrations for Chloride & Sample MW5 was diluted due to high concentrations for Chloride & Sample MW5DL was diluted due to high concentrations for Chloride & Sample SUPPLY was diluted due to high concentrations for Chloride.

The Blank Spike met requirements for all samples.

The Duplicate analysis met criteria for all samples.

The Matrix Spike (SUPPLYMS) analysis met criteria for all samples except for Chloride due to sample matrix interference.

The Matrix Spike Duplicate (SUPPLYMSD) analysis met criteria for all samples except for Chloride due to sample matrix interference.

The Blank analysis did not indicate the presence of lab contamination.

The Calibration met the requirements.

E. Additional Comments:

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

Signature_____

DATA REPORTING QUALIFIERS- INORGANIC

For reporting results, the following “ Results Qualifiers” are used:

J	Indicates the reported value was obtained from a reading that was less than the Contract Required Detection Limit (CRDL), but greater than or equal to the Instrument Detection Limit (IDL).
U	Indicates the analyte was analyzed for, but not detected.
ND	Indicates the analyte was analyzed for, but not detected
E	Indicates the reported value is estimated because of the presence of interference
M	Indicates Duplicate injection precision not met.
N	Indicates the spiked sample recovery is not within control limits.
S	Indicates the reported value was determined by the Method of Standard Addition (MSA).
*	Indicates that the duplicate analysis is not within control limits.
+	Indicates the correlation coefficient for the MSA is less than 0.995.
D	Indicates the reported value is from a secondary analysis with a dilution factor. The original analysis exceeded the calibration range.
M	Method qualifiers “P” for ICP instrument “PM” for ICP when Microwave Digestion is used “CV” for Manual Cold Vapor AA “AV” for automated Cold Vapor AA “CA” for MIDI-Distillation Spectrophotometric “AS” for Semi -Automated Spectrophotometric “C” for Manual Spectrophotometric “T” for Titrimetric “NR” for analyte not required to be analyzed
OR	Indicates the analyte’s concentration exceeds the calibrated range of the instrument for that specific analysis.
Q	Indicates the LCS did not meet the control limits requirements
H	Sample Analysis Out Of Hold Time

APPENDIX A

QA REVIEW GENERAL DOCUMENTATION

Project #: Q2133

Completed

For thorough review, the report must have the following:

GENERAL:

Are all original paperwork present (chain of custody, record of communication,airbill, sample management lab chronicle, login page)

✓

Check chain-of-custody for proper relinquish/return of samples

✓

Is the chain of custody signed and complete

✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts

✓

Collect information for each project id from server. Were all requirements followed

✓

COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page

✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody

✓

CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results

✓

Do requested analyses on Chain of Custody agree with the log-in page

✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Castody

✓

Were the samples received within hold time

✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle

✓

ANALYTICAL:

Was method requirement followed?

✓

Was client requirement followed?

✓

Does the case narrative summarize all QC failure?

✓

All runlogs and manual integration are reviewed for requirements

✓

All manual calculations and /or hand notations verified

✓

QA Review Signature: KETAN PATEL

Date: 05/30/2025

LAB CHRONICLE

OrderID:	Q2133	OrderDate:	5/28/2025 11:41:01 AM
Client:	G Environmental	Project:	Banker
Contact:	Gary Landis	Location:	L41

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q2133-01	MW1	WATER			05/27/25 10:00			05/28/25
			Anions Group1	300.0			05/28/25 14:55	
Q2133-01DL	MW1DL	WATER			05/27/25 10:00			05/28/25
			Anions Group1	300.0			05/28/25 17:26	
Q2133-02	MW5	WATER			05/27/25 11:30			05/28/25
			Anions Group1	300.0			05/28/25 15:17	
Q2133-02DL	MW5DL	WATER			05/27/25 11:30			05/28/25
			Anions Group1	300.0			05/28/25 18:09	
Q2133-02DL 2	MW5DL2	WATER			05/27/25 11:30			05/28/25
			Anions Group1	300.0			05/28/25 18:52	
Q2133-03	SUPPLY	WATER			05/27/25 12:09			05/28/25
			Anions Group1	300.0			05/28/25 15:38	
Q2133-03DL	SUPPLYDL	WATER			05/27/25 12:09			05/28/25
			Anions Group1	300.0			05/28/25 19:35	



SAMPLE DATA

Report of Analysis

Client:	G Environmental	Date Collected:	05/27/25 10:00
Project:	Banker	Date Received:	05/28/25
Client Sample ID:	MW1	SDG No.:	Q2133
Lab Sample ID:	Q2133-01	Matrix:	WATER
		% Solid:	0

Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Prep Date	Date Ana.	Ana Met.
Chloride	894	OR	1	0.19	0.60	mg/L		05/28/25 14:55	300.0

Comments: _____

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

D = Dilution

Q = indicates LCS control criteria did not meet requirements

H = Sample Analysis Out Of Hold Time

J = Estimated Value

B = Analyte Found in Associated Method Blank

* = indicates the duplicate analysis is not within control limits.

E = Indicates the reported value is estimated because of the presence of interference.

OR = Over Range

N =Spiked sample recovery not within control limits

Report of Analysis

Client:	G Environmental	Date Collected:	05/27/25 10:00
Project:	Banker	Date Received:	05/28/25
Client Sample ID:	MW1DL	SDG No.:	Q2133
Lab Sample ID:	Q2133-01DL	Matrix:	WATER
		% Solid:	0

Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Prep Date	Date Ana.	Ana Met.
Chloride	582	D	100	19.0	60.0	mg/L		05/28/25 17:26	300.0

Comments: _____

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

D = Dilution

Q = indicates LCS control criteria did not meet requirements

H = Sample Analysis Out Of Hold Time

J = Estimated Value

B = Analyte Found in Associated Method Blank

* = indicates the duplicate analysis is not within control limits.

E = Indicates the reported value is estimated because of the presence of interference.

OR = Over Range

N =Spiked sample recovery not within control limits

Report of Analysis

Client:	G Environmental	Date Collected:	05/27/25 11:30
Project:	Banker	Date Received:	05/28/25
Client Sample ID:	MW5	SDG No.:	Q2133
Lab Sample ID:	Q2133-02	Matrix:	WATER
		% Solid:	0

Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Prep Date	Date Ana.	Ana Met.
Chloride	6220	OR	1	0.19	0.60	mg/L		05/28/25 15:17	300.0

Comments: _____

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

D = Dilution

Q = indicates LCS control criteria did not meet requirements

H = Sample Analysis Out Of Hold Time

J = Estimated Value

B = Analyte Found in Associated Method Blank

* = indicates the duplicate analysis is not within control limits.

E = Indicates the reported value is estimated because of the presence of interference.

OR = Over Range

N = Spiked sample recovery not within control limits

Report of Analysis

Client:	G Environmental	Date Collected:	05/27/25 11:30
Project:	Banker	Date Received:	05/28/25
Client Sample ID:	MW5DL	SDG No.:	Q2133
Lab Sample ID:	Q2133-02DL	Matrix:	WATER
		% Solid:	0

Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Prep Date	Date Ana.	Ana Met.
Chloride	4630	OR	100	19.0	60.0	mg/L		05/28/25 18:09	300.0

Comments: _____

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

D = Dilution

Q = indicates LCS control criteria did not meet requirements

H = Sample Analysis Out Of Hold Time

J = Estimated Value

B = Analyte Found in Associated Method Blank

* = indicates the duplicate analysis is not within control limits.

E = Indicates the reported value is estimated because of the presence of interference.

OR = Over Range

N = Spiked sample recovery not within control limits

Report of Analysis

Client:	G Environmental	Date Collected:	05/27/25 11:30
Project:	Banker	Date Received:	05/28/25
Client Sample ID:	MW5DL2	SDG No.:	Q2133
Lab Sample ID:	Q2133-02DL2	Matrix:	WATER
		% Solid:	0

Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Prep Date	Date Ana.	Ana Met.
Chloride	3860	D	1000	190	600	mg/L		05/28/25 18:52	300.0

Comments: _____

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

D = Dilution

Q = indicates LCS control criteria did not meet requirements

H = Sample Analysis Out Of Hold Time

J = Estimated Value

B = Analyte Found in Associated Method Blank

* = indicates the duplicate analysis is not within control limits.

E = Indicates the reported value is estimated because of the presence of interference.

OR = Over Range

N =Spiked sample recovery not within control limits

Report of Analysis

Client:	G Environmental	Date Collected:	05/27/25 12:09
Project:	Banker	Date Received:	05/28/25
Client Sample ID:	SUPPLY	SDG No.:	Q2133
Lab Sample ID:	Q2133-03	Matrix:	WATER
		% Solid:	0

Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Prep Date	Date Ana.	Ana Met.
Chloride	298	OR	1	0.19	0.60	mg/L		05/28/25 15:38	300.0

Comments: _____

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

D = Dilution

Q = indicates LCS control criteria did not meet requirements

H = Sample Analysis Out Of Hold Time

J = Estimated Value

B = Analyte Found in Associated Method Blank

* = indicates the duplicate analysis is not within control limits.

E = Indicates the reported value is estimated because of the presence of interference.

OR = Over Range

N =Spiked sample recovery not within control limits

Report of Analysis

Client:	G Environmental	Date Collected:	05/27/25 12:09
Project:	Banker	Date Received:	05/28/25
Client Sample ID:	SUPPLYDL	SDG No.:	Q2133
Lab Sample ID:	Q2133-03DL	Matrix:	WATER
		% Solid:	0

Parameter	Conc.	Qua.	DF	MDL	LOQ / CRQL	Units	Prep Date	Date Ana.	Ana Met.
Chloride	206	D	100	19.0	60.0	mg/L		05/28/25 19:35	300.0

Comments: _____

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

D = Dilution

Q = indicates LCS control criteria did not meet requirements

H = Sample Analysis Out Of Hold Time

J = Estimated Value

B = Analyte Found in Associated Method Blank

* = indicates the duplicate analysis is not within control limits.

E = Indicates the reported value is estimated because of the presence of interference.

OR = Over Range

N =Spiked sample recovery not within control limits



QC RESULT SUMMARY

Initial and Continuing Calibration Verification

Client: G Environmental

SDG No.: Q2133

Project: Banker

RunNo.: LB135928

Analyte	Units	Result	True Value	% Recovery	Acceptance Window (%R)	Analysis Date
Sample ID: ICV1						
Bromide	mg/L	10.2	10	102	90-110	05/22/2025
Chloride	mg/L	3.1	3	103	90-110	05/22/2025
Fluoride	mg/L	2.1	2	105	90-110	05/22/2025
Nitrite	mg/L	3.1	3	103	90-110	05/22/2025
Nitrate	mg/L	2.6	2.5	104	90-110	05/22/2025
Sulfate	mg/L	15.1	15	101	90-110	05/22/2025
Orthophosphate as P	mg/L	5.3	5	106	90-110	05/22/2025
Sample ID: CCV1						
Bromide	mg/L	10.7	10	107	90-110	05/28/2025
Chloride	mg/L	3.2	3	107	90-110	05/28/2025
Fluoride	mg/L	2.2	2	110	90-110	05/28/2025
Nitrite	mg/L	3.2	3	107	90-110	05/28/2025
Nitrate	mg/L	2.7	2.5	108	90-110	05/28/2025
Sulfate	mg/L	15.9	15	106	90-110	05/28/2025
Orthophosphate as P	mg/L	5.2	5	104	90-110	05/28/2025
Sample ID: CCV2						
Bromide	mg/L	10.2	10	102	90-110	05/28/2025
Chloride	mg/L	3.1	3	103	90-110	05/28/2025
Fluoride	mg/L	2.1	2	105	90-110	05/28/2025
Nitrite	mg/L	3.1	3	103	90-110	05/28/2025
Nitrate	mg/L	2.6	2.5	104	90-110	05/28/2025
Sulfate	mg/L	15.1	15	101	90-110	05/28/2025
Orthophosphate as P	mg/L	5.3	5	106	90-110	05/28/2025
Sample ID: CCV3						
Bromide	mg/L	10.2	10	102	90-110	05/28/2025
Chloride	mg/L	3.1	3	103	90-110	05/28/2025
Fluoride	mg/L	2.1	2	105	90-110	05/28/2025
Nitrite	mg/L	3.1	3	103	90-110	05/28/2025
Nitrate	mg/L	2.6	2.5	104	90-110	05/28/2025
Sulfate	mg/L	15.2	15	101	90-110	05/28/2025
Orthophosphate as P	mg/L	5.3	5	106	90-110	05/28/2025

Initial and Continuing Calibration Blank Summary

Client: G Environmental

SDG No.: Q2133

Project: Banker

RunNo.: LB135928

Analyte	Units	Result	Acceptance Limits	Conc Qual	MDL	RDL	Analysis Date
Sample ID: ICB1							
Bromide	mg/L	< 1.0000	1.0000	U	0.37	2	05/22/2025
Chloride	mg/L	< 0.3000	0.3000	U	0.19	0.6	05/22/2025
Fluoride	mg/L	< 0.2000	0.2000	U	0.11	0.4	05/22/2025
Nitrite	mg/L	< 0.3000	0.3000	U	0.074	0.6	05/22/2025
Nitrate	mg/L	< 0.2500	0.2500	U	0.095	0.5	05/22/2025
Sulfate	mg/L	< 1.5000	1.5000	U	0.46	3	05/22/2025
Orthophosphate as P	mg/L	< 0.5000	0.5000	U	0.34	1	05/22/2025
Sample ID: CCB1							
Bromide	mg/L	< 1.0000	1.0000	U	0.37	2	05/28/2025
Chloride	mg/L	< 0.3000	0.3000	U	0.19	0.6	05/28/2025
Fluoride	mg/L	< 0.2000	0.2000	U	0.11	0.4	05/28/2025
Nitrite	mg/L	< 0.3000	0.3000	U	0.074	0.6	05/28/2025
Nitrate	mg/L	< 0.2500	0.2500	U	0.095	0.5	05/28/2025
Sulfate	mg/L	< 1.5000	1.5000	U	0.46	3	05/28/2025
Orthophosphate as P	mg/L	< 0.5000	0.5000	U	0.34	1	05/28/2025
Sample ID: CCB2							
Bromide	mg/L	< 1.0000	1.0000	U	0.37	2	05/28/2025
Chloride	mg/L	< 0.3000	0.3000	U	0.19	0.6	05/28/2025
Fluoride	mg/L	< 0.2000	0.2000	U	0.11	0.4	05/28/2025
Nitrite	mg/L	< 0.3000	0.3000	U	0.074	0.6	05/28/2025
Nitrate	mg/L	< 0.2500	0.2500	U	0.095	0.5	05/28/2025
Sulfate	mg/L	< 1.5000	1.5000	U	0.46	3	05/28/2025
Orthophosphate as P	mg/L	< 0.5000	0.5000	U	0.34	1	05/28/2025
Sample ID: CCB3							
Bromide	mg/L	< 1.0000	1.0000	U	0.37	2	05/28/2025
Chloride	mg/L	< 0.3000	0.3000	U	0.19	0.6	05/28/2025
Fluoride	mg/L	< 0.2000	0.2000	U	0.11	0.4	05/28/2025
Nitrite	mg/L	< 0.3000	0.3000	U	0.074	0.6	05/28/2025
Nitrate	mg/L	< 0.2500	0.2500	U	0.095	0.5	05/28/2025
Sulfate	mg/L	< 1.5000	1.5000	U	0.46	3	05/28/2025
Orthophosphate as P	mg/L	< 0.5000	0.5000	U	0.34	1	05/28/2025

Preparation Blank Summary

Client: G Environmental

SDG No.: Q2133

Project: Banker

Analyte	Units	Result	Acceptance Limits	Conc Qual	MDL	RDL	Analysis Date
Sample ID: LB135928BLW							
Bromide	mg/L	< 1.0000	1.0000	U	0.37	2	05/28/2025
Chloride	mg/L	< 0.3000	0.3000	U	0.19	0.6	05/28/2025
Fluoride	mg/L	< 0.2000	0.2000	U	0.11	0.4	05/28/2025
Nitrite	mg/L	< 0.3000	0.3000	U	0.074	0.6	05/28/2025
Nitrate	mg/L	< 0.2500	0.2500	U	0.095	0.5	05/28/2025
Sulfate	mg/L	< 1.5000	1.5000	U	0.46	3	05/28/2025
Orthophosphate as P	mg/L	< 0.5000	0.5000	U	0.34	1	05/28/2025

Matrix Spike Summary

Client:	G Environmental	SDG No.:	Q2133
Project:	Banker	Sample ID:	Q2133-03
Client ID:	SUPPLYMS	Percent Solids for Spike Sample:	0

Analyte	Units	Acceptance Limit %R	Spiked Result	Conc. Qualifier	Sample Result	Conc. Qualifier	Spike Added	Dilution Factor	% Rec	Qual	Analysis Date
Bromide	mg/L	80-120	10.5		0.37	U	10	1	105		05/28/2025
Chloride	mg/L	80-120	286	OR	298	OR	3	1	-400	*	05/28/2025
Fluoride	mg/L	80-120	2.30		0.23	J	2	1	104		05/28/2025
Nitrite	mg/L	80-120	3.10		0.080	J	3	1	101		05/28/2025
Nitrate	mg/L	80-120	3.80		1.30		2.5	1	100		05/28/2025
Sulfate	mg/L	80-120	38.2	OR	23.3		15	1	99		05/28/2025
Orthophosphate as P	mg/L	80-120	5.30		0.34	U	5	1	106		05/28/2025

Matrix Spike Summary

Client:	G Environmental	SDG No.:	Q2133
Project:	Banker	Sample ID:	Q2133-03
Client ID:	SUPPLYMSD	Percent Solids for Spike Sample:	0

Analyte	Units	Acceptance Limit %R	Spiked Result	Conc. Qualifier	Sample Result	Conc. Qualifier	Spike Added	Dilution Factor	% Rec	Qual	Analysis Date
Bromide	mg/L	80-120	10.1		0.37	U	10	1	101		05/28/2025
Chloride	mg/L	80-120	287	OR	298	OR	3	1	-367	*	05/28/2025
Fluoride	mg/L	80-120	2.20		0.23	J	2	1	99		05/28/2025
Nitrite	mg/L	80-120	3.00		0.080	J	3	1	97		05/28/2025
Nitrate	mg/L	80-120	3.70		1.30		2.5	1	96		05/28/2025
Sulfate	mg/L	80-120	37.6	OR	23.3		15	1	95		05/28/2025
Orthophosphate as P	mg/L	80-120	5.10		0.34	U	5	1	102		05/28/2025

Duplicate Sample Summary

Client: G Environmental	SDG No.: Q2133
Project: Banker	Sample ID: Q2133-03
Client ID: SUPPLYMSD	Percent Solids for Spike Sample: 0

Analyte	Units	Acceptance Limit	Sample Result	Conc. Qualifier	Duplicate Result	Conc. Qualifier	Dilution Factor	RPD/AD	Qual	Analysis Date
Chloride	mg/L	+/-20	286	OR	287	OR	1	0		05/28/2025
Sulfate	mg/L	+/-20	38.2	OR	37.6	OR	1	2		05/28/2025
Nitrate	mg/L	+/-20	3.80		3.70		1	3		05/28/2025
Nitrite	mg/L	+/-20	3.10		3.00		1	3		05/28/2025
Bromide	mg/L	+/-20	10.5		10.1		1	4		05/28/2025
Fluoride	mg/L	+/-20	2.30		2.20		1	4		05/28/2025
Orthophosphate as P	mg/L	+/-20	5.30		5.10		1	4		05/28/2025

Laboratory Control Sample Summary

Client: G Environmental

SDG No.: Q2133

Project: Banker

Run No.: LB135928

Analyte	Units	True Value	Result	Conc. Qualifier	% Recovery	Dilution Factor	Acceptance Limit %R	Analysis Date
Sample ID	LB135928BSW							
Bromide	mg/L	10	10.7		107	1	90-110	05/28/2025
Chloride	mg/L	3	3.30		110	1	90-110	05/28/2025
Fluoride	mg/L	2	2.20		110	1	90-110	05/28/2025
Nitrite	mg/L	3	3.20		107	1	90-110	05/28/2025
Nitrate	mg/L	2.5	2.70		108	1	90-110	05/28/2025
Sulfate	mg/L	15	15.9		106	1	90-110	05/28/2025
Orthophosphate as P	mg/L	5	5.40		108	1	90-110	05/28/2025



RAW DATA


h	Instrument IC-1				Analyst: NF		Method: 300.0 / 9056A		Initial Analyst	
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	Initial Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/22/2025 11:09	10 NF/IZ
STD2	0.430	0.640	0.649	2.129	0.543	1.098	3.287	IC1-052225	5/22/2025 11:30	10 NF/IZ
STD3	0.795	1.207	1.205	4.018	1.004	1.867	6.069	IC1-052225	5/22/2025 11:52	10 NF/IZ
STD4	0.977	1.480	1.479	4.929	1.229	2.477	7.415	IC1-052225	5/22/2025 12:13	10 NF/IZ
STD5	1.991	2.968	2.960	9.916	2.467	5.110	14.621	IC1-052225	5/22/2025 12:35	10 NF/IZ
STD6	4.001	5.967	5.959	19.868	4.966	9.870	29.848	IC1-052225	5/22/2025 12:56	10 NF/IZ
STD7	5.006	7.539	7.548	25.140	6.290	12.578	37.260	IC1-052225	5/22/2025 13:17	10 NF/IZ
ICV	2.054	3.101	3.056	10.229	2.610	5.286	15.128	IC1-052225	5/22/2025 13:39	10 NF/IZ
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/22/2025 14:22	10 NF/IZ
CCV	2.173	3.234	3.183	10.665	2.719	5.177	15.946	IC1-052225	5/28/2025 11:29	10 NF/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/28/2025 11:51	10 NF/IZ
LB135928BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/28/2025 12:12	10 NF/IZ
LB135928BSW	2.169	3.277	3.196	10.743	2.741	5.407	15.912	IC1-052225	5/28/2025 13:29	10 NF/IZ
Q2126-08	0.429	0.652	0.665	2.168	0.555	1.098	3.376	IC1-052225	5/28/2025 13:51	10 NF/IZ
Q2126-07	0.227	0.350	0.365	1.172	0.300	0.580	1.871	IC1-052225	5/28/2025 14:12	10 NF/IZ
Q2126-07RE 0.25ML	0.131	0.204	0.221	0.677	0.176	0.327	1.162	IC1-052225	5/28/2025 14:34	10 NF/IZ
Q2133-01	0.142	894.317	0.000	0.000	0.058	0.000	23.378	IC1-052225	5/28/2025 14:55	10 NF/IZ
Q2133-02	0.365	6224.982	0.000	0.716	0.117	0.000	40.826	IC1-052225	5/28/2025 15:17	10 NF/IZ
Q2133-03	0.225	297.983	0.080	0.220	1.302	0.000	23.282	IC1-052225	5/28/2025 15:38	10 NF/IZ
Q2133-03MS	2.334	286.238	3.096	10.452	3.847	5.265	38.231	IC1-052225	5/28/2025 16:00	10 NF/IZ
Q2133-03MSD	2.221	287.399	2.997	10.102	3.749	5.143	37.638	IC1-052225	5/28/2025 16:21	10 NF/IZ
CCV	2.052	3.104	3.050	10.194	2.603	5.254	15.139	IC1-052225	5/28/2025 16:43	10 NF/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/28/2025 17:05	10 NF/IZ
Q2133-01DLX100	0.000	5.817	0.000	0.000	0.000	0.000	0.683	IC1-052225	5/28/2025 17:26	10 NF/IZ
Q2133-02DLX100	0.000	46.339	0.000	0.000	0.000	0.000	0.839	IC1-052225	5/28/2025 18:09	10 NF/IZ
Q2133-02DL2X1000	0.000	3.856	0.000	0.000	0.000	0.000	0.490	IC1-052225	5/28/2025 18:52	10 NF/IZ
Q2133-0DLX100	0.000	2.061	0.000	0.000	0.060	0.000	0.651	IC1-052225	5/28/2025 19:35	10 NF/IZ
CCV	2.066	3.109	3.057	10.203	2.604	5.259	15.206	IC1-052225	5/28/2025 19:56	10 NF/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/28/2025 20:18	10 NF/IZ

Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A											
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-052225	5/22/2025 11:09	10	NF/IZ
STD2	0.4300	0.6400	0.6490	2.1290	0.5430	1.0980	3.2870	IC1-052225	5/22/2025 11:30	10	NF/IZ
STD3	0.7950	1.2070	1.2050	4.0180	1.0040	1.8670	6.0690	IC1-052225	5/22/2025 11:52	10	NF/IZ
STD4	0.9770	1.4800	1.4790	4.9290	1.2290	2.4770	7.4150	IC1-052225	5/22/2025 12:13	10	NF/IZ
STD5	1.9910	2.9680	2.9600	9.9160	2.4670	5.1100	14.6210	IC1-052225	5/22/2025 12:35	10	NF/IZ
STD6	4.0010	5.9670	5.9590	19.8680	4.9660	9.8700	29.8480	IC1-052225	5/22/2025 12:56	10	NF/IZ
STD7	5.0060	7.5390	7.5480	25.1400	6.2900	12.5780	37.2600	IC1-052225	5/22/2025 13:17	10	NF/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000				
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000				
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000				
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000				
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000				
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000				
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000				
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4				
STD1	7.5000	6.6667	8.1667	6.4500	8.6000	9.8000	9.5667				
STD2	-0.6250	0.5833	0.4167	0.4500	0.4000	-6.6500	1.1500				
STD3	-2.3000	-1.3333	-1.4000	-1.4200	-1.6800	-0.9200	-1.1333				
STD4	-0.4500	-1.0667	-1.3333	-0.8400	-1.3200	2.2000	-2.5267				
STD5	0.0250	-0.5500	-0.6833	-0.6600	-0.6800	-1.3000	-0.5067				
STD6	0.1200	0.5200	0.6400	0.5600	0.6400	0.6240	0.7027				

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

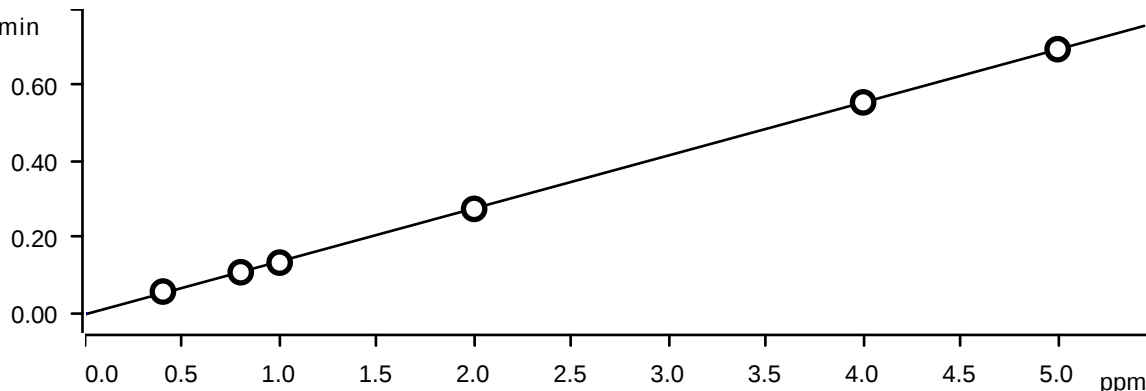

Function: $A = -2.82659E-3 + 0.0139492 \times Q$


Relative standard deviation 0.920519 %

Correlation coefficient 0.999955

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.057	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.108	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.133	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.275	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.555	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.695	STD7	2025-05-22 13:17:57 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

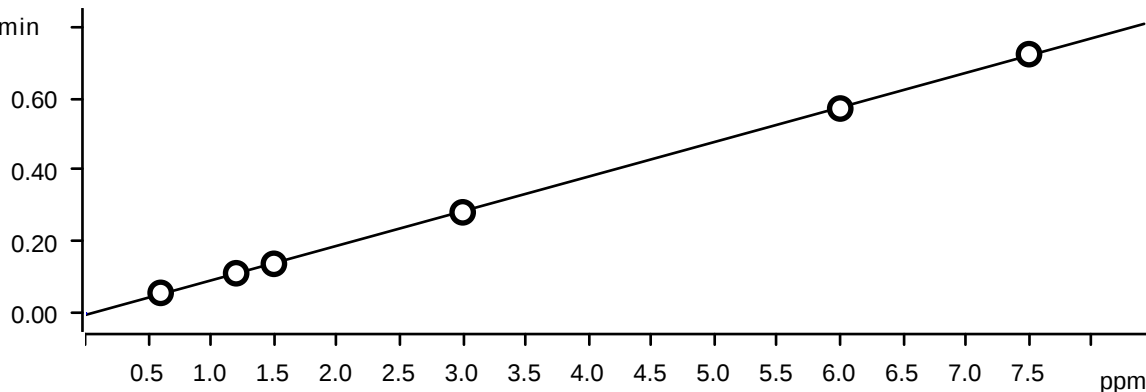

Function: $A = -4.33057E-3 + 9.64673E-3 \times Q$


Relative standard deviation 1.154335 %

Correlation coefficient 0.999929

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.057	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.112	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.138	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.282	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.571	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.723	STD7	2025-05-22 13:17:57 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

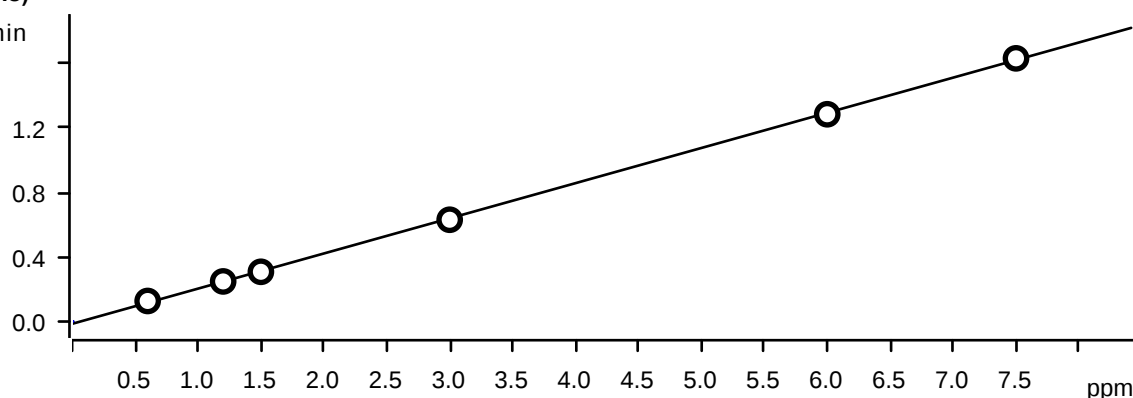Function: $A = -0.0150155 + 0.0217890 \times Q$


Relative standard deviation 1.428639 %

Correlation coefficient 0.999893

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.126	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.248	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.307	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.630	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.283	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.630	STD7	2025-05-22 13:17:57 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

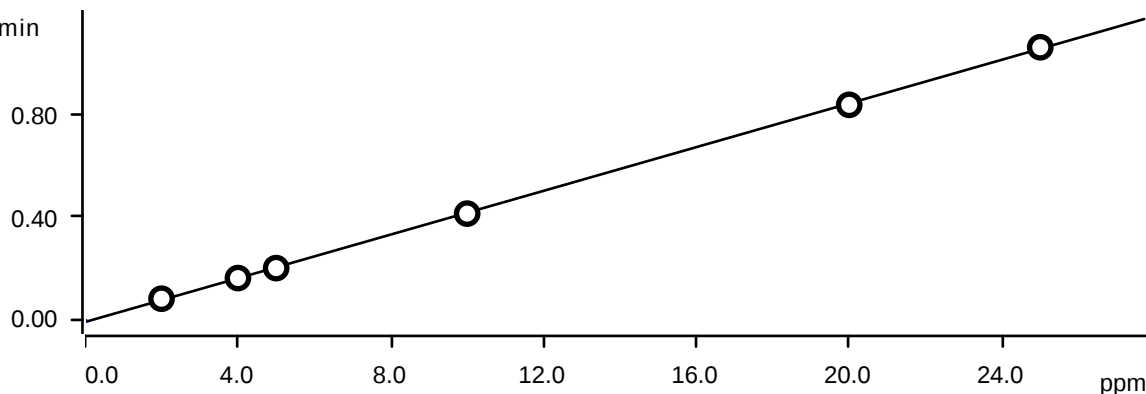

Function: $A = -6.27114E-3 + 4.23162E-3 \times Q$


Relative standard deviation: 1.185575 %

Correlation coefficient: 0.999925

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.084	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.164	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.202	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.413	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.834	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.058	STD7	2025-05-22 13:17:57 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

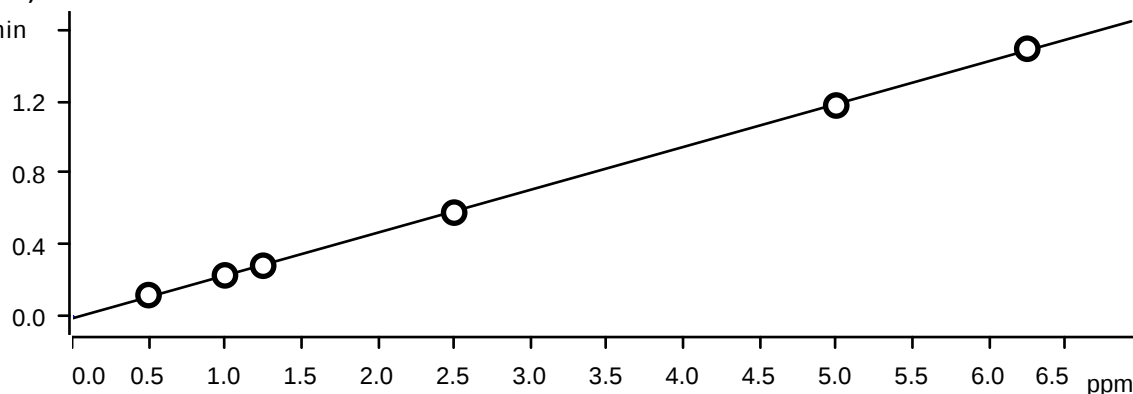


Function: $A = -0.0109593 + 0.0239055 \times Q$

Relative standard deviation: 1.451672 %

Correlation coefficient 0.999889

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.119	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.229	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.283	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.579	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.176	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.493	STD7	2025-05-22 13:17:57 UTC-4	used

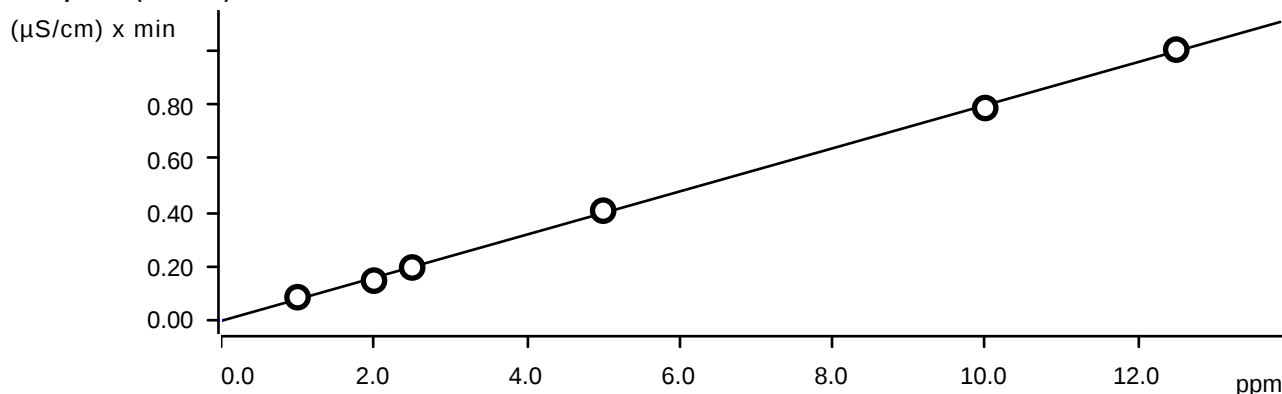
Phosphate (Anions)Function: $A = -3.02035E-3 + 8.01761E-3 \times Q$

Relative standard deviation 2.297726 %

Correlation coefficient 0.999716

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.085	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.147	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.196	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.407	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.788	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.005	STD7	2025-05-22 13:17:57 UTC-4	used

Sulfate (Anions)

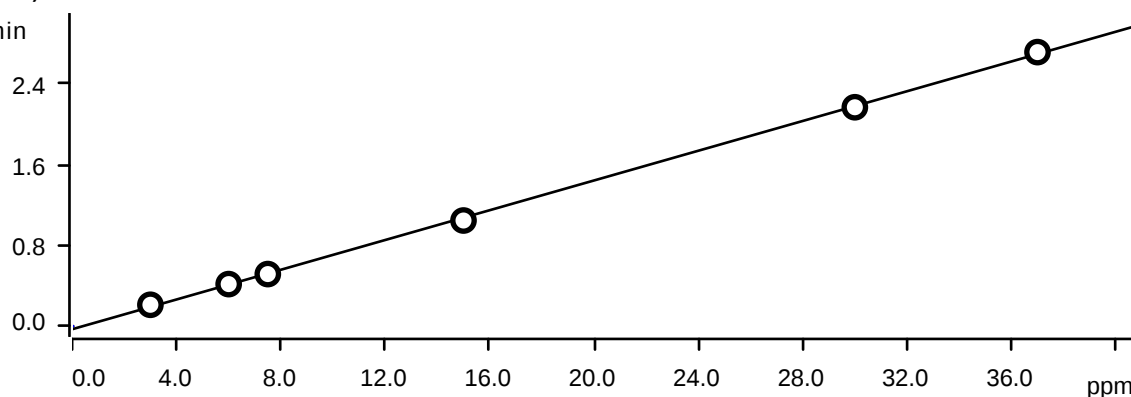 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0303663 + 7.37295E-3 \times Q$

Relative standard deviation 1.792871 %

Correlation coefficient 0.999832


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.212	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.417	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.516	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.048	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.170	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.717	STD7	2025-05-22 13:17:57 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-05-22 11:09:38 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

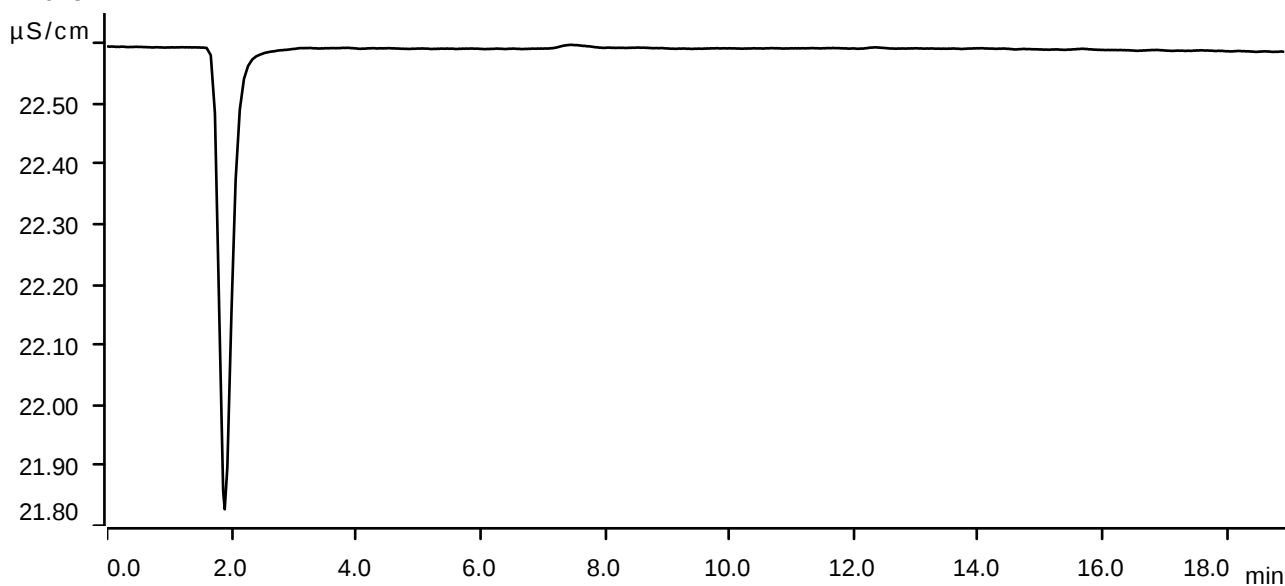Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-05-22 11:30:53 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

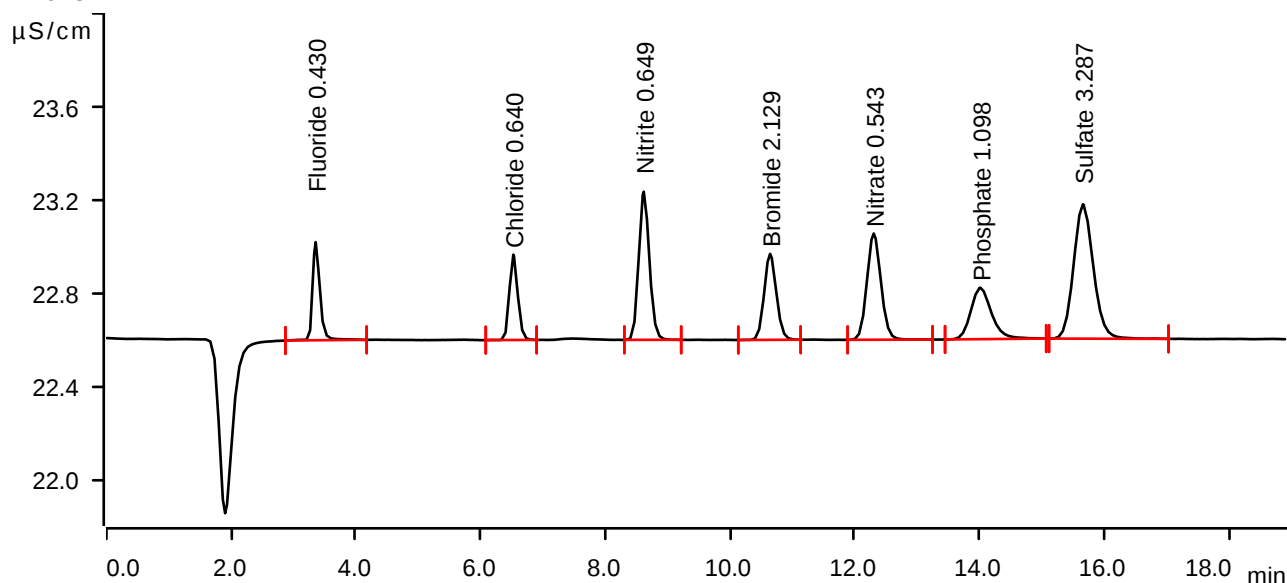

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.0572	0.421	0.430	Fluoride
2	6.525	0.0574	0.366	0.640	Chloride
3	8.617	0.1264	0.636	0.649	Nitrite
4	10.642	0.0838	0.369	2.129	Bromide
5	12.303	0.1190	0.456	0.543	Nitrate
6	14.013	0.0850	0.221	1.098	Phosphate
7	15.657	0.2120	0.577	3.287	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-05-22 11:52:16 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

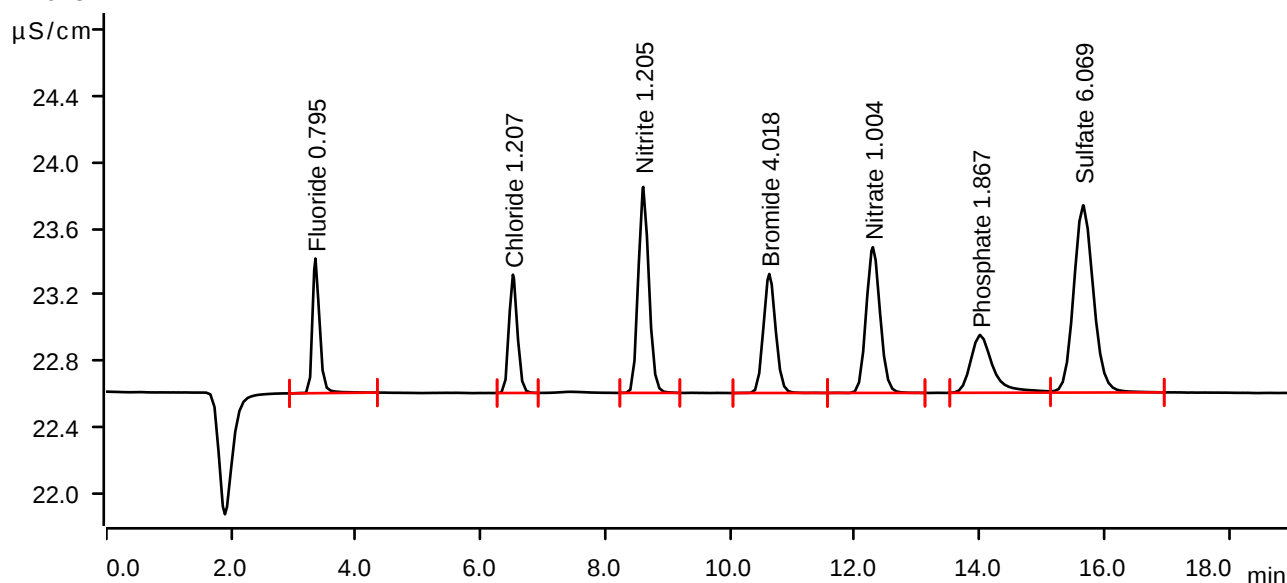

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.1081	0.814	0.795	Fluoride
2	6.518	0.1121	0.716	1.207	Chloride
3	8.608	0.2475	1.247	1.205	Nitrite
4	10.628	0.1637	0.720	4.018	Bromide
5	12.290	0.2290	0.882	1.004	Nitrate
6	14.008	0.1467	0.350	1.867	Phosphate
7	15.660	0.4171	1.133	6.069	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-05-22 12:13:41 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

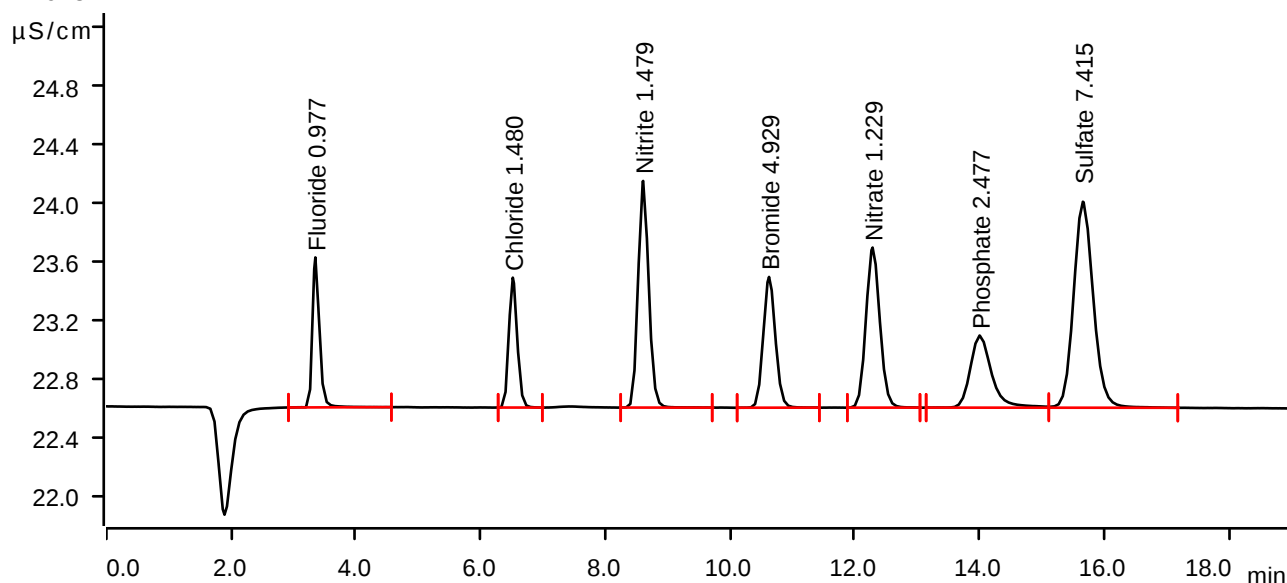

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	3.352	0.1334	1.024	0.977	Fluoride
2	6.517	0.1384	0.888	1.480	Chloride
3	8.607	0.3073	1.549	1.479	Nitrite
4	10.625	0.2023	0.894	4.929	Bromide
5	12.285	0.2828	1.094	1.229	Nitrate
6	14.003	0.1955	0.493	2.477	Phosphate
7	15.657	0.5164	1.408	7.415	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-05-22 12:35:06 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

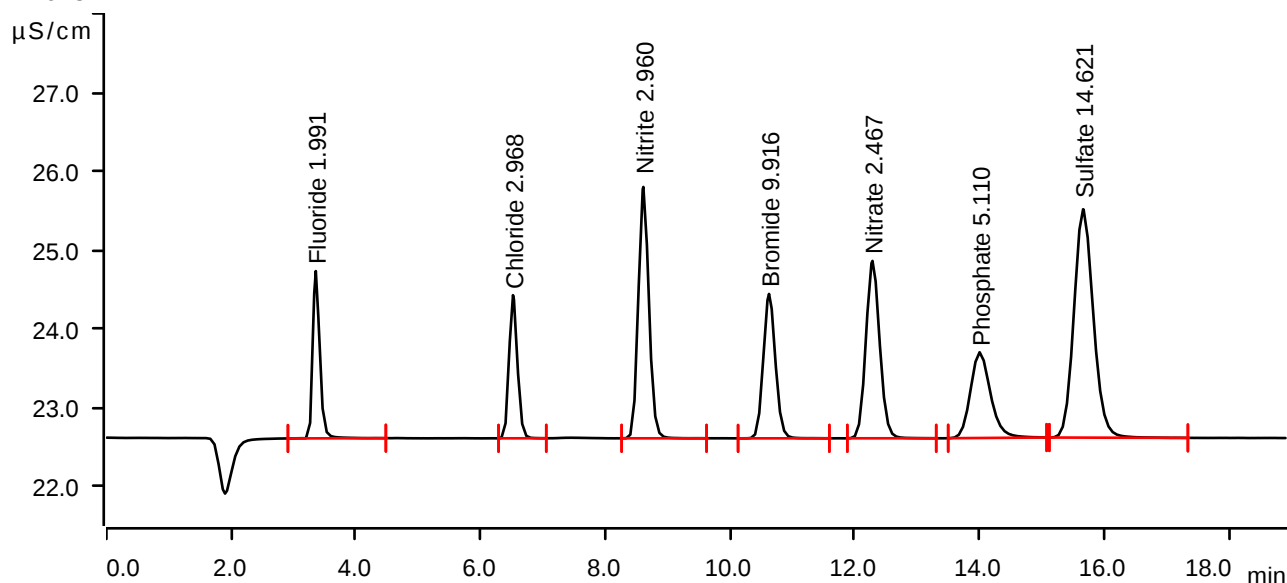

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.2749	2.123	1.991	Fluoride
2	6.520	0.2820	1.816	2.968	Chloride
3	8.610	0.6298	3.190	2.960	Nitrite
4	10.625	0.4133	1.833	9.916	Bromide
5	12.283	0.5789	2.251	2.467	Nitrate
6	14.002	0.4067	1.087	5.110	Phosphate
7	15.660	1.0476	2.898	14.621	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-05-22 12:56:31 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

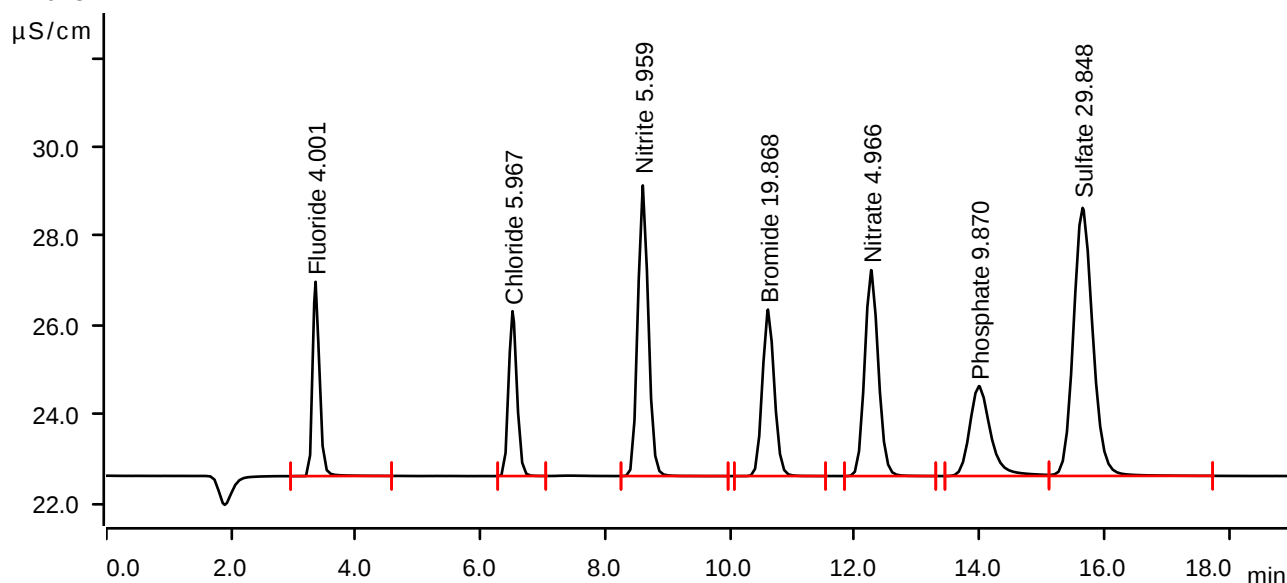

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.5553	4.361	4.001	Fluoride
2	6.512	0.5713	3.701	5.967	Chloride
3	8.602	1.2834	6.525	5.959	Nitrite
4	10.608	0.8345	3.739	19.868	Bromide
5	12.262	1.1762	4.624	4.966	Nitrate
6	13.990	0.7883	2.019	9.870	Phosphate
7	15.652	2.1703	6.019	29.848	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-05-22 13:17:57 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

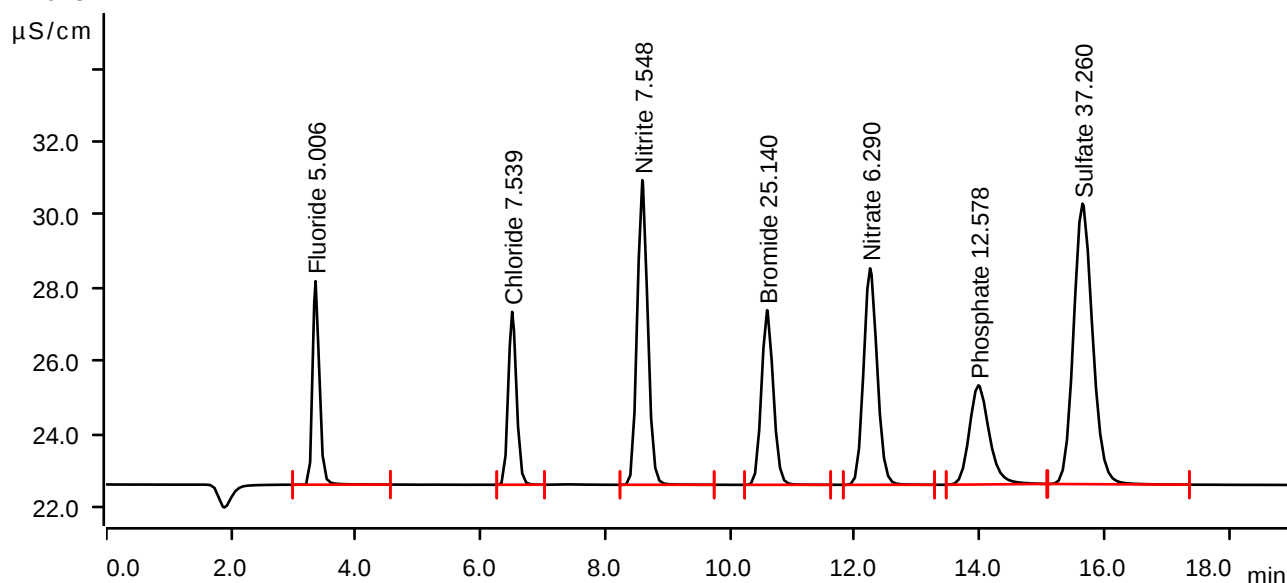

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.6954	5.562	5.006	Fluoride
2	6.507	0.7229	4.726	7.539	Chloride
3	8.593	1.6297	8.328	7.548	Nitrite
4	10.593	1.0576	4.774	25.140	Bromide
5	12.245	1.4927	5.918	6.290	Nitrate
6	13.982	1.0054	2.711	12.578	Phosphate
7	15.650	2.7168	7.668	37.260	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-05-22 13:39:25 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

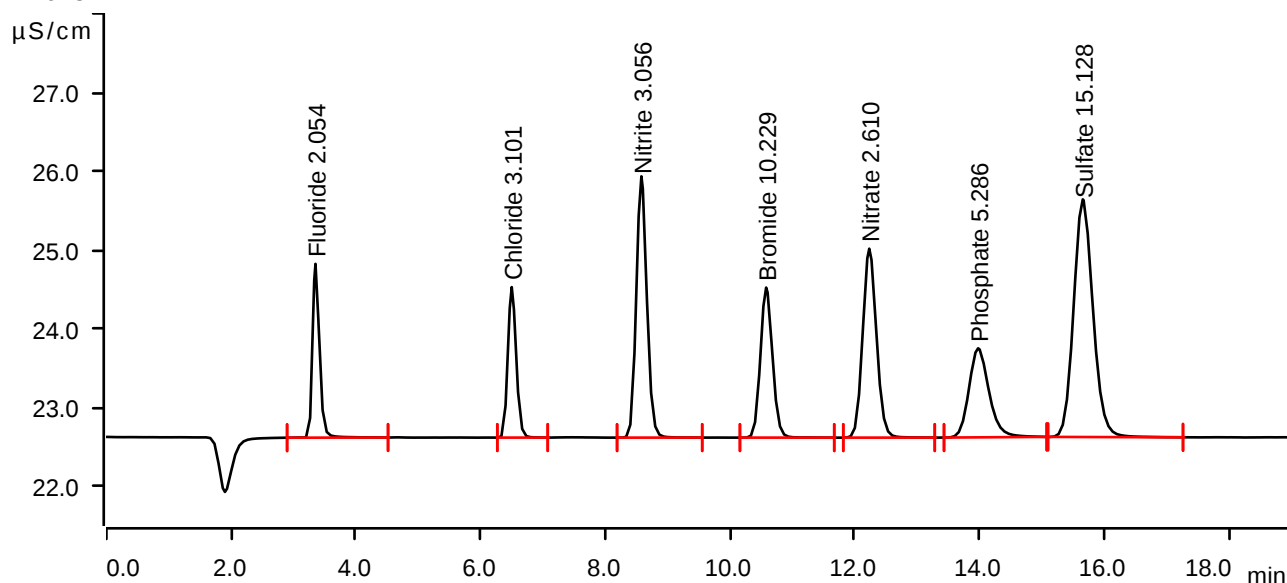


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.2837	2.205	2.054	Fluoride
2	6.500	0.2948	1.910	3.101	Chloride
3	8.578	0.6509	3.316	3.056	Nitrite
4	10.578	0.4266	1.904	10.229	Bromide
5	12.232	0.6129	2.398	2.610	Nitrate
6	13.977	0.4208	1.130	5.286	Phosphate
7	15.655	1.0850	3.016	15.128	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2025-05-22 14:22:21 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

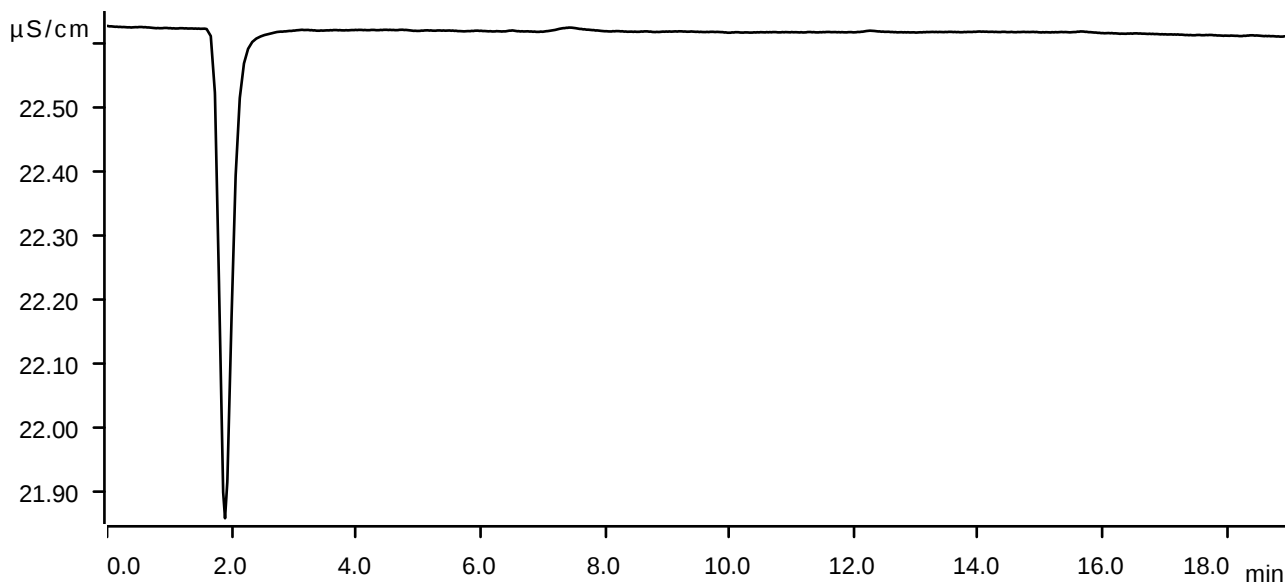Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-05-28 11:29:37 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

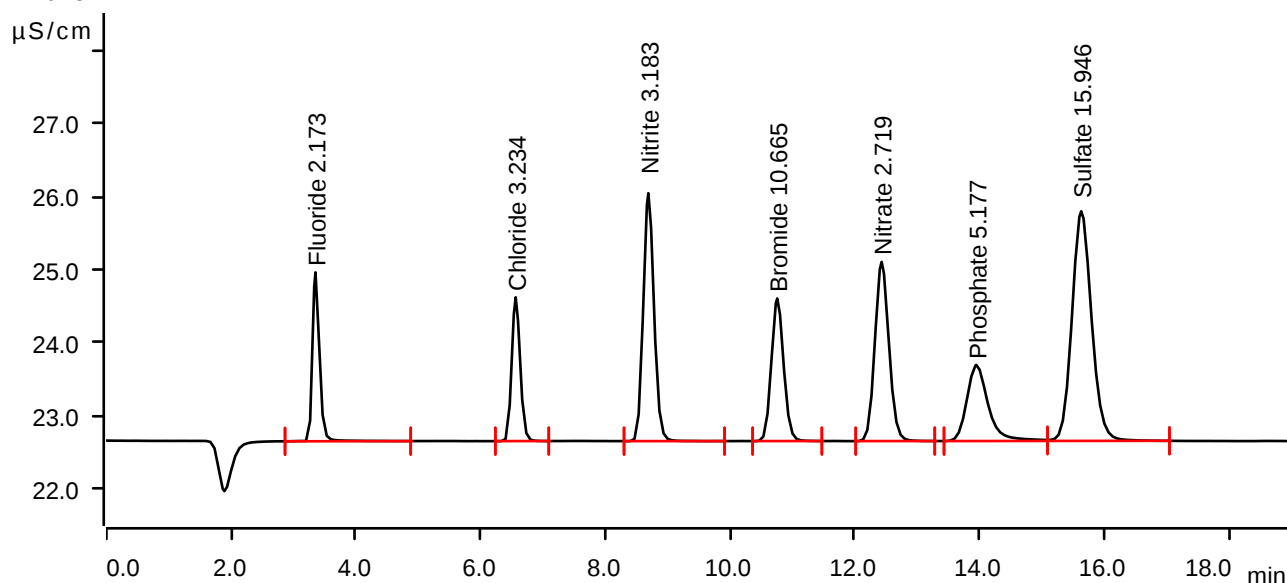


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.3003	2.307	2.173	Fluoride
2	6.563	0.3076	1.965	3.234	Chloride
3	8.690	0.6784	3.387	3.183	Nitrite
4	10.757	0.4450	1.949	10.665	Bromide
5	12.430	0.6390	2.449	2.719	Nitrate
6	13.948	0.4121	1.039	5.177	Phosphate
7	15.630	1.1453	3.138	15.946	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-05-28 11:51:07 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

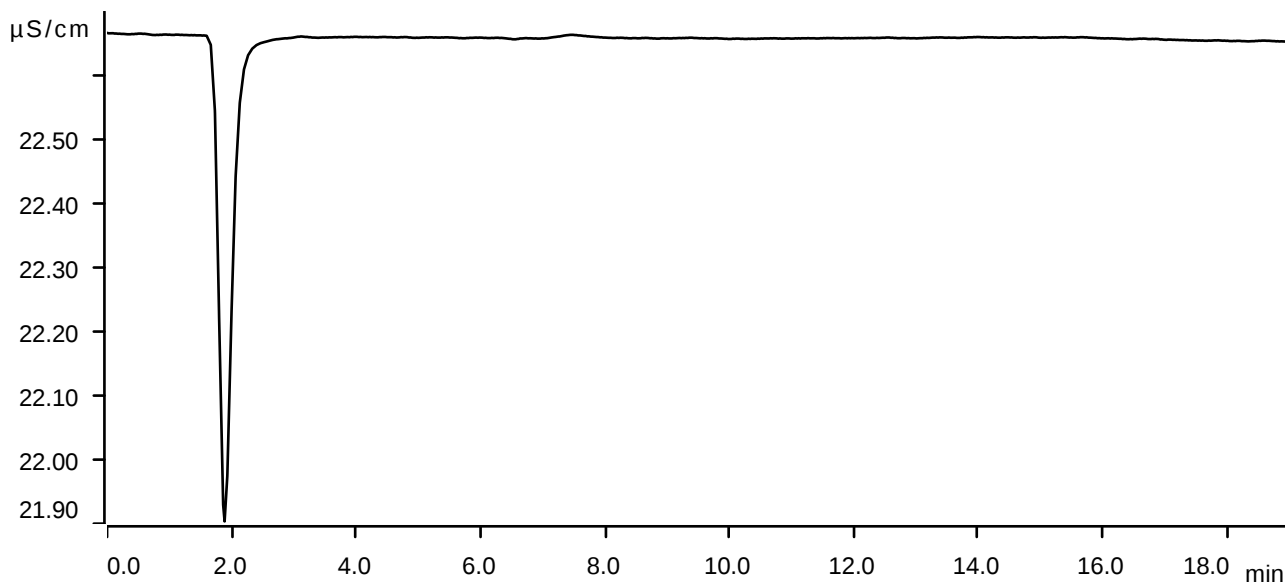
Anions

Sample data

Ident LB135928BLW
Sample type Sample
Determination start 2025-05-28 12:12:37 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

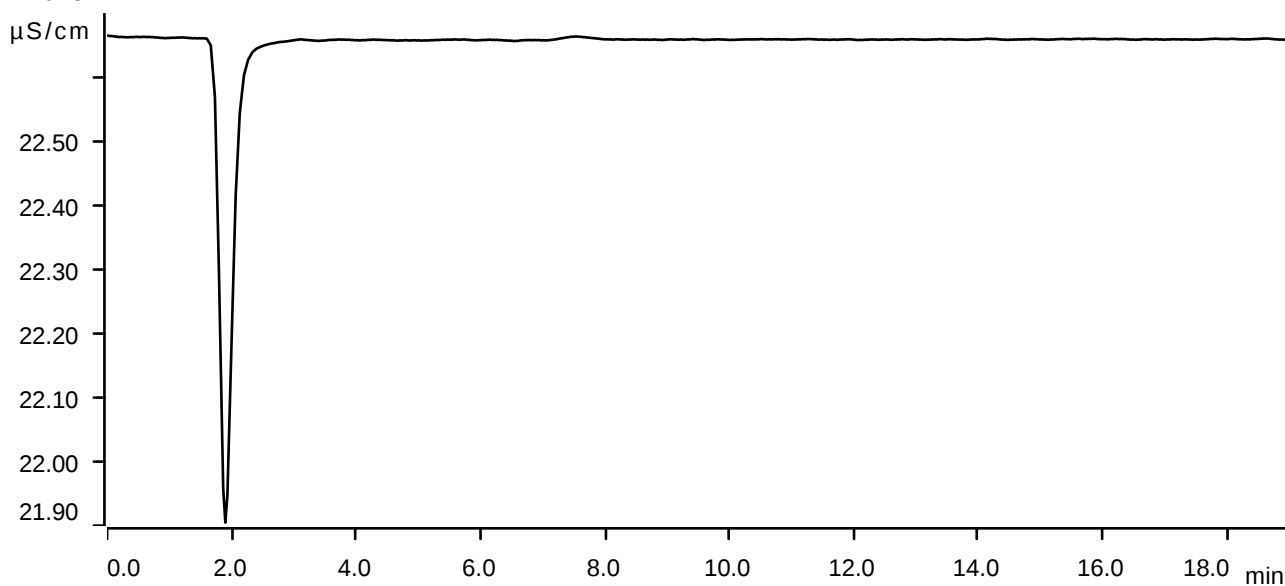Anions


Sample data

Ident LB135928BSW
Sample type Check standard 1
Determination start 2025-05-28 13:29:42 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

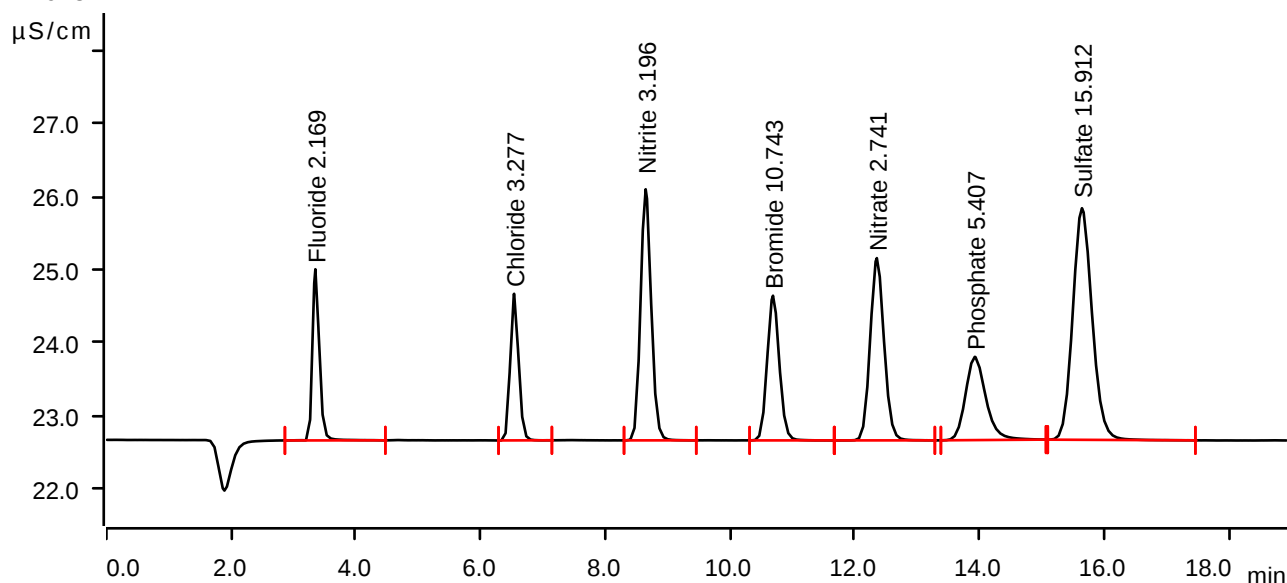

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.2997	2.339	2.169	Fluoride
2	6.538	0.3118	2.003	3.277	Chloride
3	8.647	0.6814	3.431	3.196	Nitrite
4	10.688	0.4483	1.978	10.743	Bromide
5	12.353	0.6443	2.491	2.741	Nitrate
6	13.923	0.4305	1.138	5.407	Phosphate
7	15.642	1.1428	3.165	15.912	Sulfate


Sample data

Ident Q2126-08
Sample type Sample
Determination start 2025-05-28 13:51:14 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

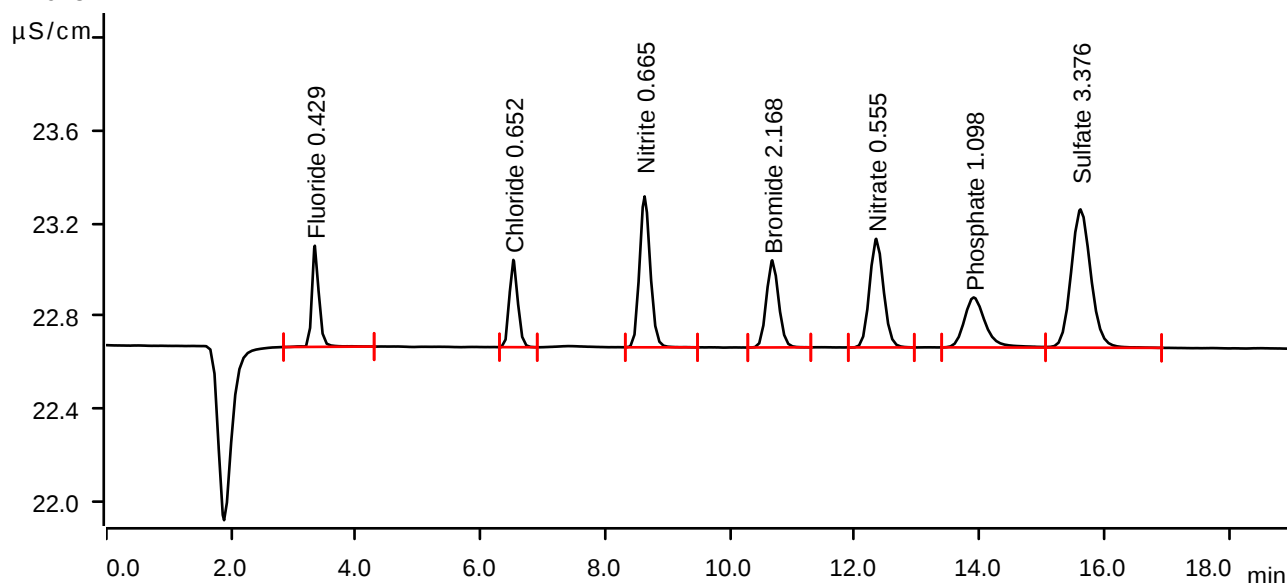

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.343	0.0571	0.434	0.429	Fluoride
2	6.525	0.0586	0.375	0.652	Chloride
3	8.630	0.1299	0.648	0.665	Nitrite
4	10.677	0.0855	0.374	2.168	Bromide
5	12.343	0.1218	0.466	0.555	Nitrate
6	13.907	0.0850	0.215	1.098	Phosphate
7	15.618	0.2185	0.594	3.376	Sulfate


Sample data

Ident Q2126-07
Sample type Sample
Determination start 2025-05-28 14:12:46 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.67 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

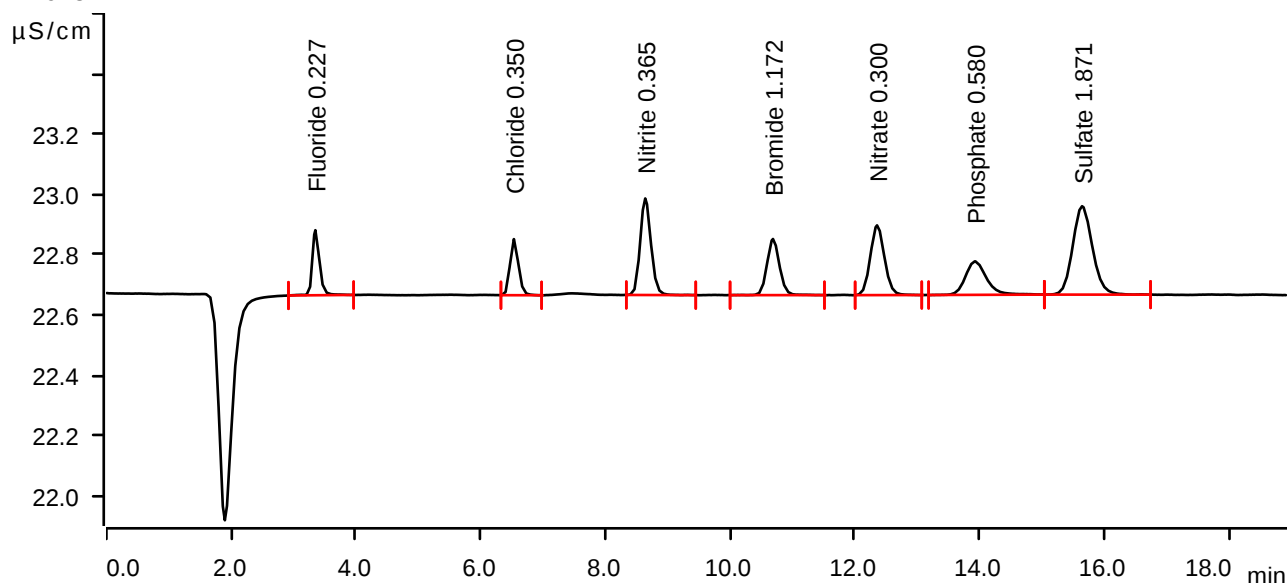

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.0288	0.216	0.227	Fluoride
2	6.535	0.0294	0.186	0.350	Chloride
3	8.640	0.0645	0.320	0.365	Nitrite
4	10.688	0.0433	0.186	1.172	Bromide
5	12.357	0.0609	0.231	0.300	Nitrate
6	13.923	0.0435	0.111	0.580	Phosphate
7	15.643	0.1076	0.294	1.871	Sulfate


Sample data

Ident Q2126-07RE 0.25ML
Sample type Sample
Determination start 2025-05-28 14:34:20 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

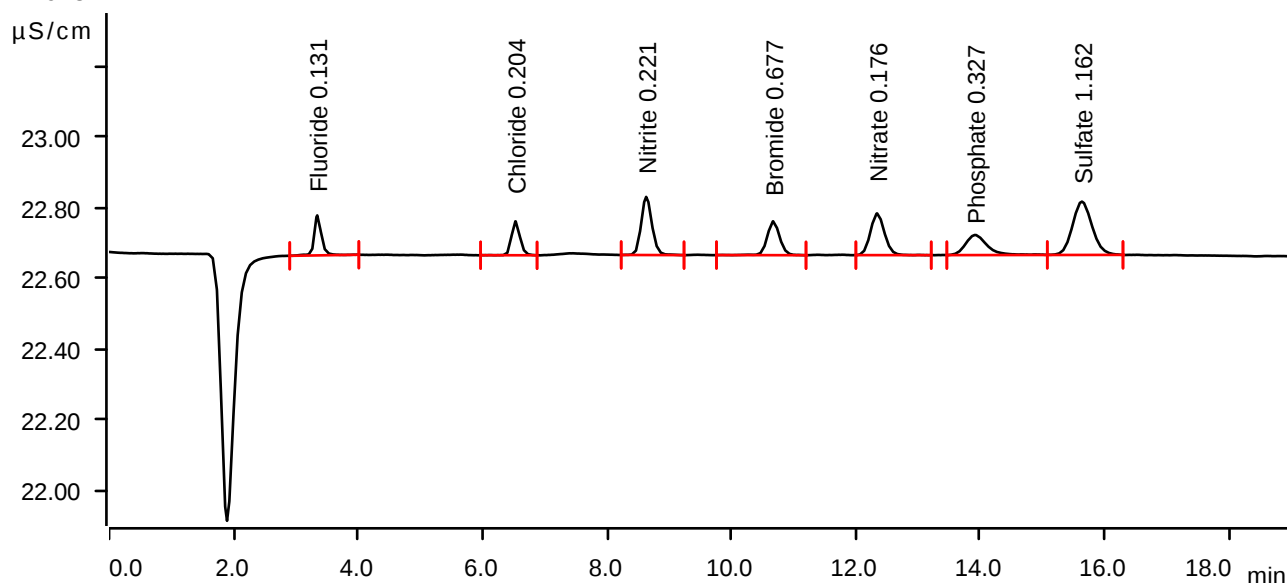

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.347	0.0155	0.113	0.131	Fluoride
2	6.530	0.0154	0.096	0.204	Chloride
3	8.632	0.0332	0.165	0.221	Nitrite
4	10.672	0.0224	0.096	0.677	Bromide
5	12.343	0.0311	0.118	0.176	Nitrate
6	13.910	0.0232	0.057	0.327	Phosphate
7	15.635	0.0553	0.151	1.162	Sulfate


Sample data

Ident Q2133-01
Sample type Sample
Determination start 2025-05-28 14:55:42 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

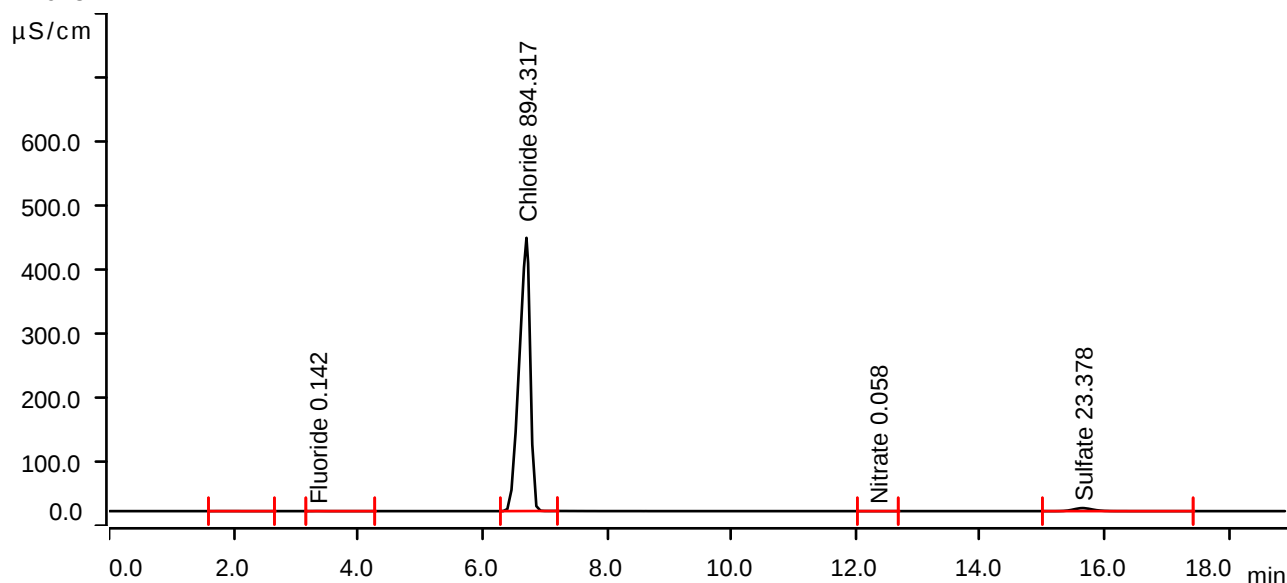

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.843	0.0157	0.056	invalid	
2	3.343	0.0170	0.121	0.142	Fluoride
3	6.708	86.2680	426.735	894.317	Chloride
4	12.350	0.0030	0.011	0.058	Nitrate
5	15.642	1.6933	4.736	23.378	Sulfate


Sample data

Ident Q2133-02
Sample type Sample
Determination start 2025-05-28 15:17:17 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

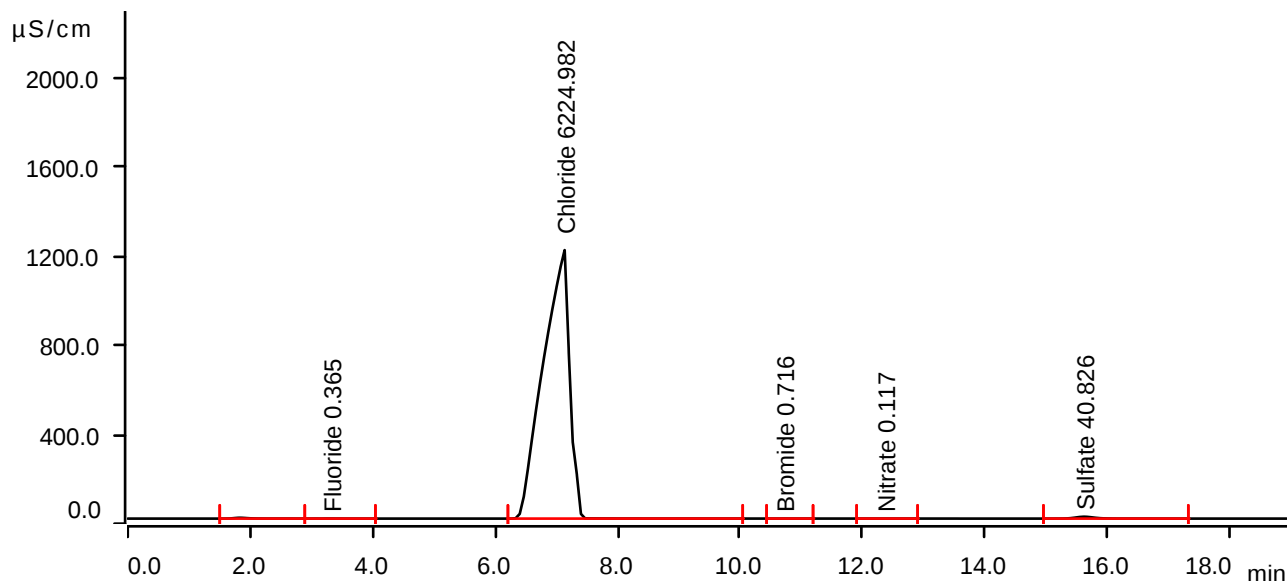

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.832	1.0247	3.812	invalid	
2	3.323	0.0481	0.234	0.365	Fluoride
3	7.135	600.5027	1205.532	6224.982	Chloride
4	10.720	0.0240	0.109	0.716	Bromide
5	12.363	0.0170	0.065	0.117	Nitrate
6	15.615	2.9797	8.397	40.826	Sulfate


Sample data

Ident Q2133-03
Sample type Sample
Determination start 2025-05-28 15:38:51 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

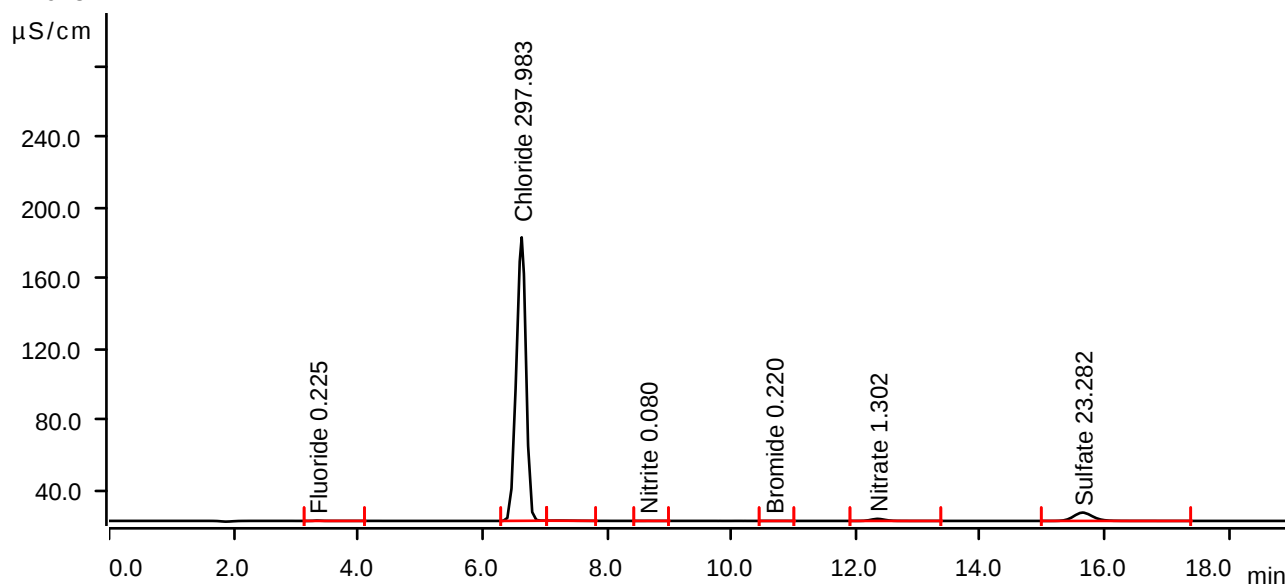

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.345	0.0286	0.194	0.225	Fluoride
2	6.632	28.7413	160.500	297.983	Chloride
3	7.238	0.0275	0.077	invalid	
4	8.652	0.0023	0.012	0.080	Nitrite
5	10.675	0.0031	0.014	0.220	Bromide
6	12.350	0.3003	1.166	1.302	Nitrate
7	15.645	1.6862	4.722	23.282	Sulfate


Sample data

Ident Q2133-03MS
Sample type Sample
Determination start 2025-05-28 16:00:25 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.84 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

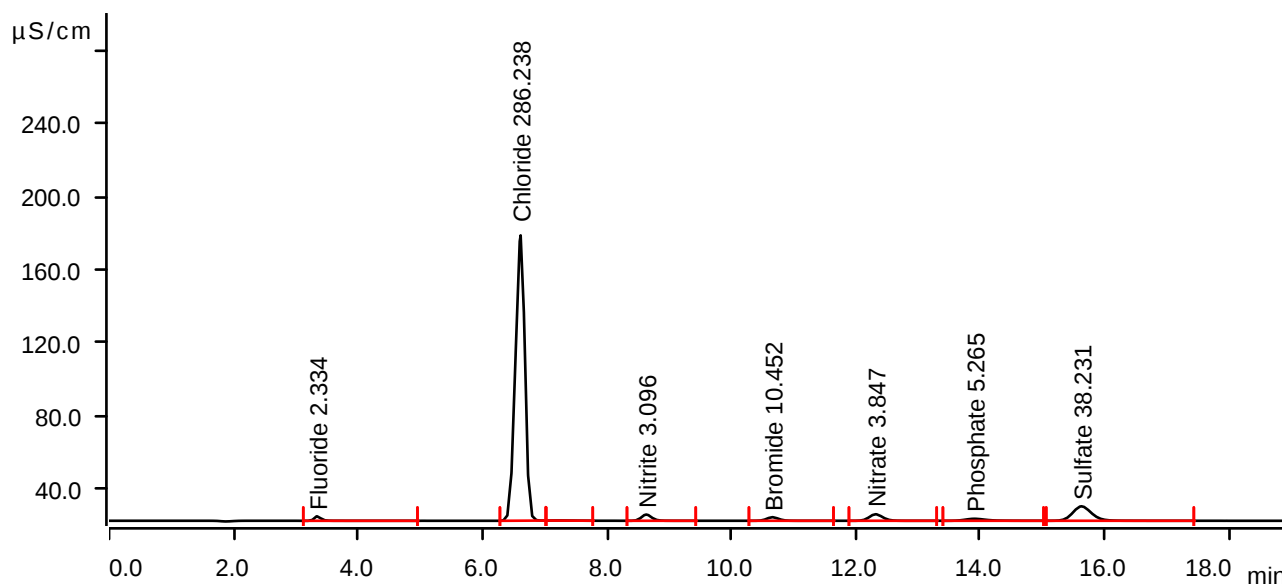

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.343	0.3228	2.452	2.334	Fluoride
2	6.615	27.6083	155.967	286.238	Chloride
3	7.217	0.0257	0.071	invalid	
4	8.633	0.6595	3.400	3.096	Nitrite
5	10.660	0.4360	1.954	10.452	Bromide
6	12.318	0.9087	3.571	3.847	Nitrate
7	13.907	0.4191	1.089	5.265	Phosphate
8	15.627	2.7884	7.899	38.231	Sulfate


Sample data

Ident Q2133-03MSD
Sample type Sample
Determination start 2025-05-28 16:21:57 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

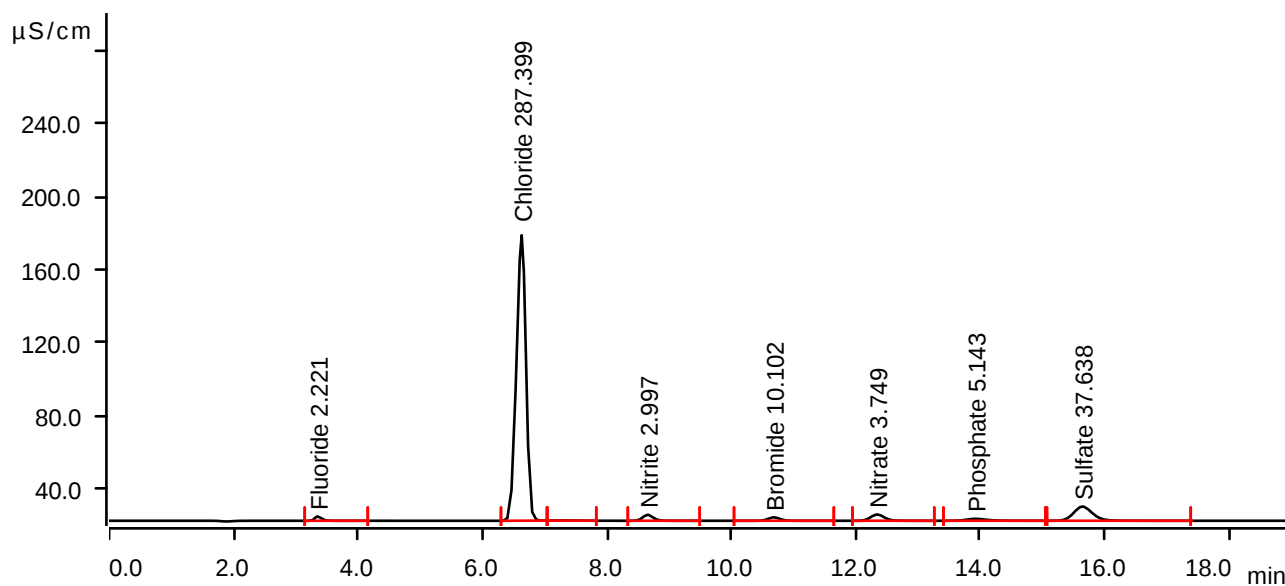

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.353	0.3070	2.378	2.221	Fluoride
2	6.632	27.7202	156.048	287.399	Chloride
3	7.242	0.0259	0.072	invalid	
4	8.657	0.6381	3.279	2.997	Nitrite
5	10.682	0.4212	1.886	10.102	Bromide
6	12.342	0.8852	3.479	3.749	Nitrate
7	13.925	0.4093	1.068	5.143	Phosphate
8	15.642	2.7446	7.783	37.638	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-05-28 16:43:30 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

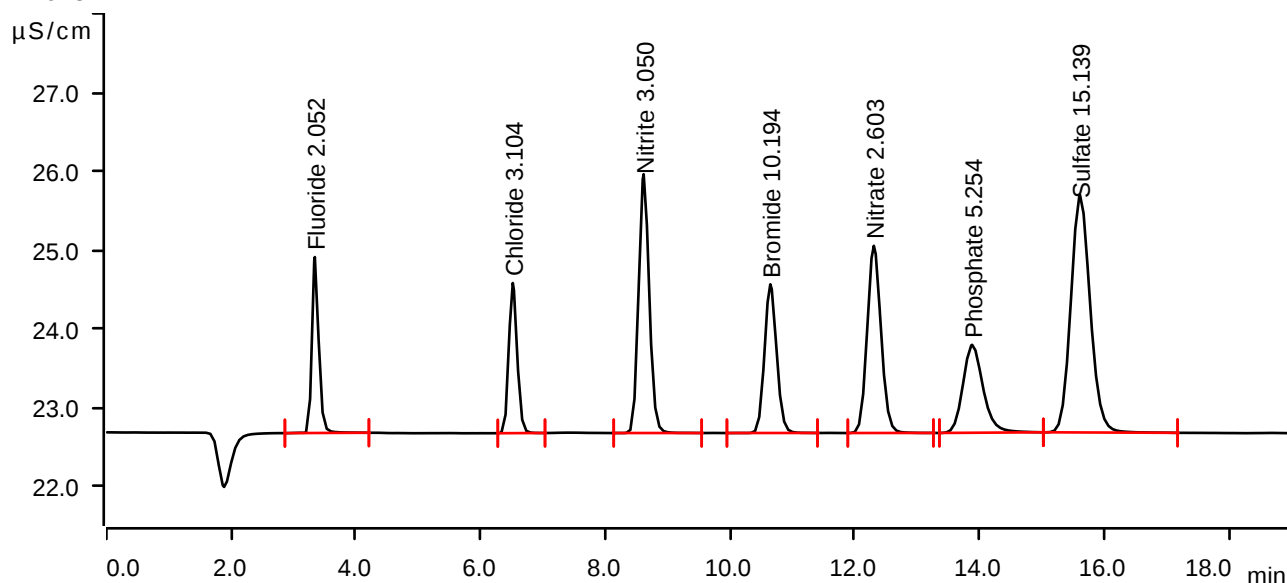

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.343	0.2834	2.232	2.052	Fluoride
2	6.517	0.2951	1.905	3.104	Chloride
3	8.615	0.6495	3.284	3.050	Nitrite
4	10.645	0.4251	1.887	10.194	Bromide
5	12.305	0.6113	2.376	2.603	Nitrate
6	13.882	0.4182	1.116	5.254	Phosphate
7	15.610	1.0858	3.015	15.139	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2025-05-28 17:05:00 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

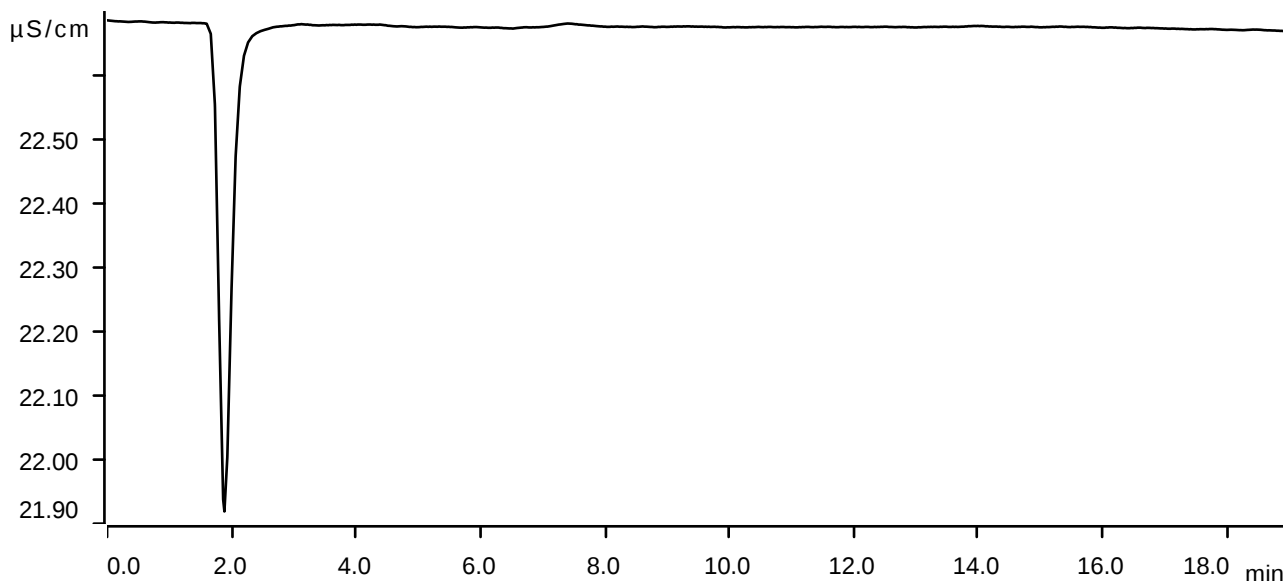


Sample data

Ident Q2133-01DLX100
Sample type Sample
Determination start 2025-05-28 17:26:29 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

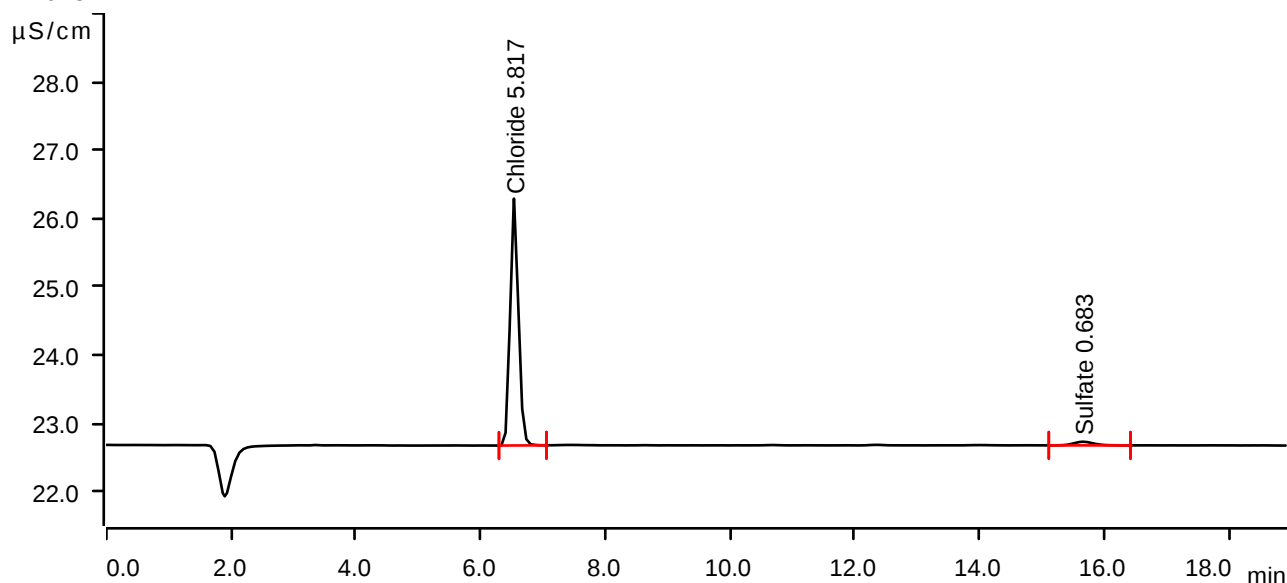

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.537	0.5568	3.615	5.817	Chloride
2	15.653	0.0200	0.053	0.683	Sulfate


Sample data

Ident Q2133-02DLX100
Sample type Sample
Determination start 2025-05-28 18:09:31 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

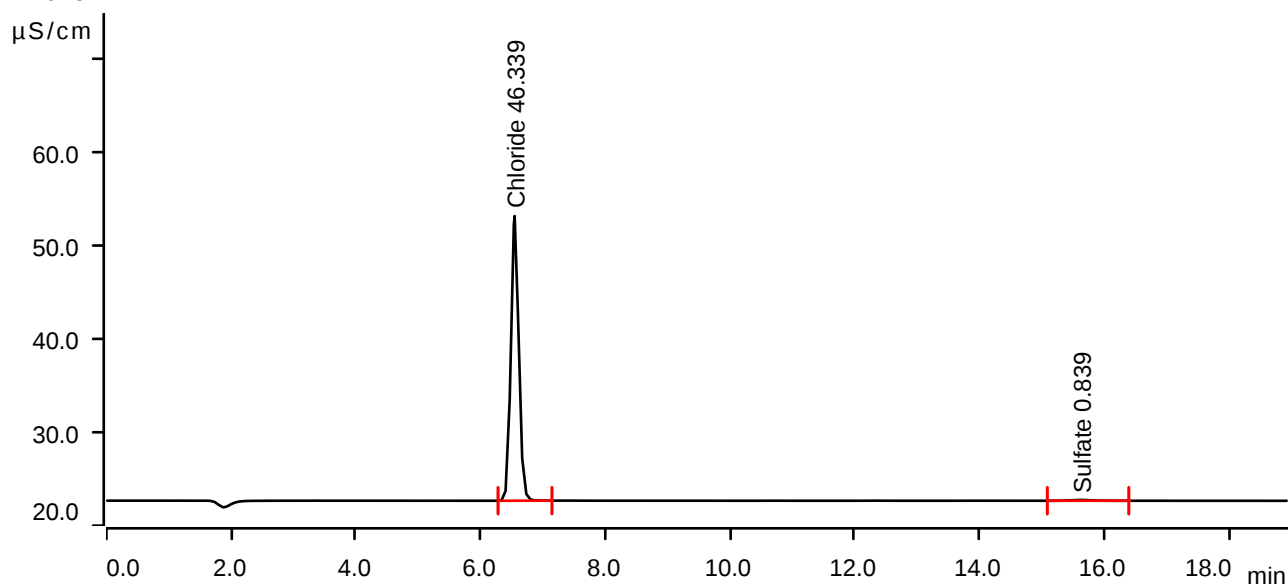

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.547	4.4659	30.568	46.339	Chloride
2	15.625	0.0315	0.085	0.839	Sulfate


Sample data

Ident Q2133-02DL2X1000
Sample type Sample
Determination start 2025-05-28 18:52:28 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.56 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

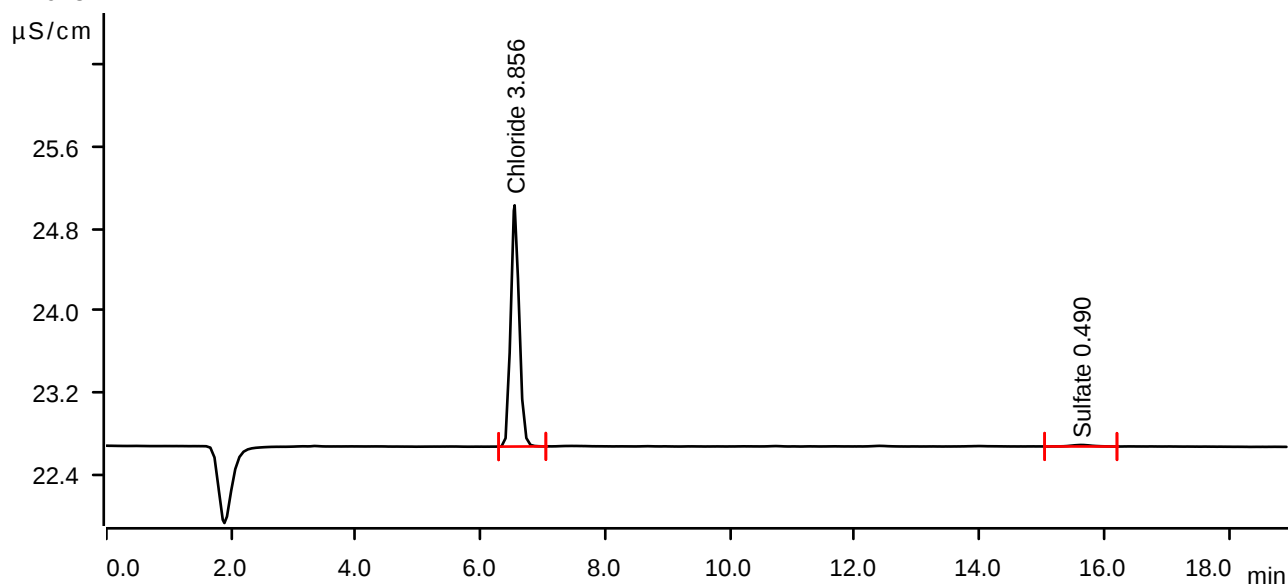

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.547	0.3677	2.355	3.856	Chloride
2	15.618	0.0058	0.015	0.490	Sulfate


Sample data

Ident Q2133-0DLX100
Sample type Sample
Determination start 2025-05-28 19:35:24 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

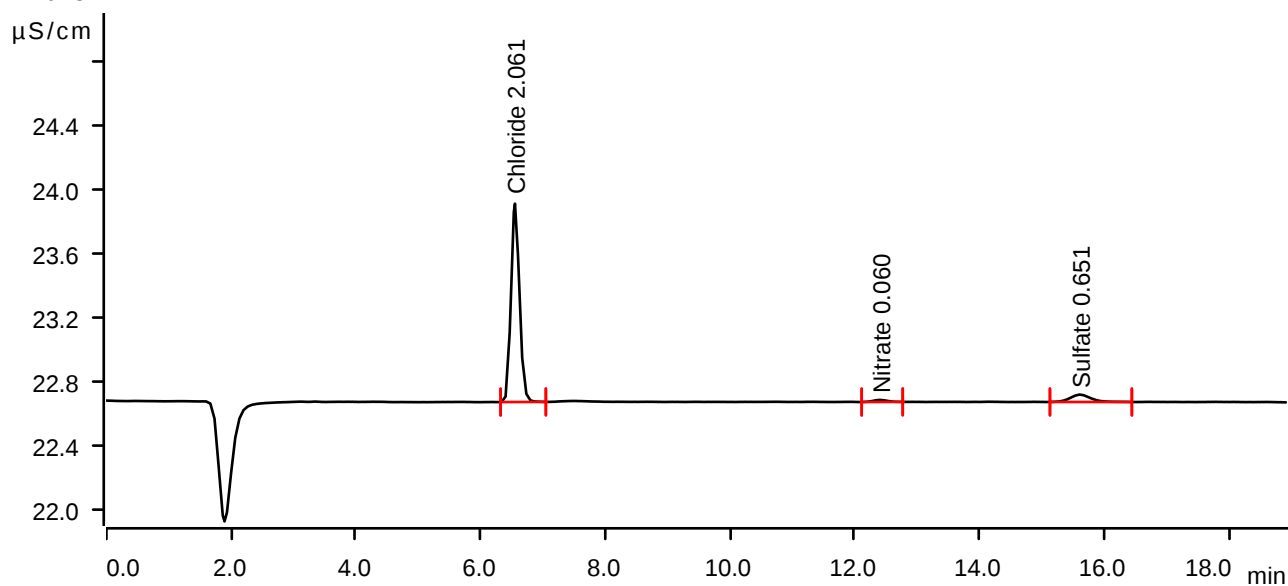

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.552	0.1945	1.239	2.061	Chloride
2	12.405	0.0033	0.013	0.060	Nitrate
3	15.607	0.0176	0.046	0.651	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-05-28 19:56:50 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

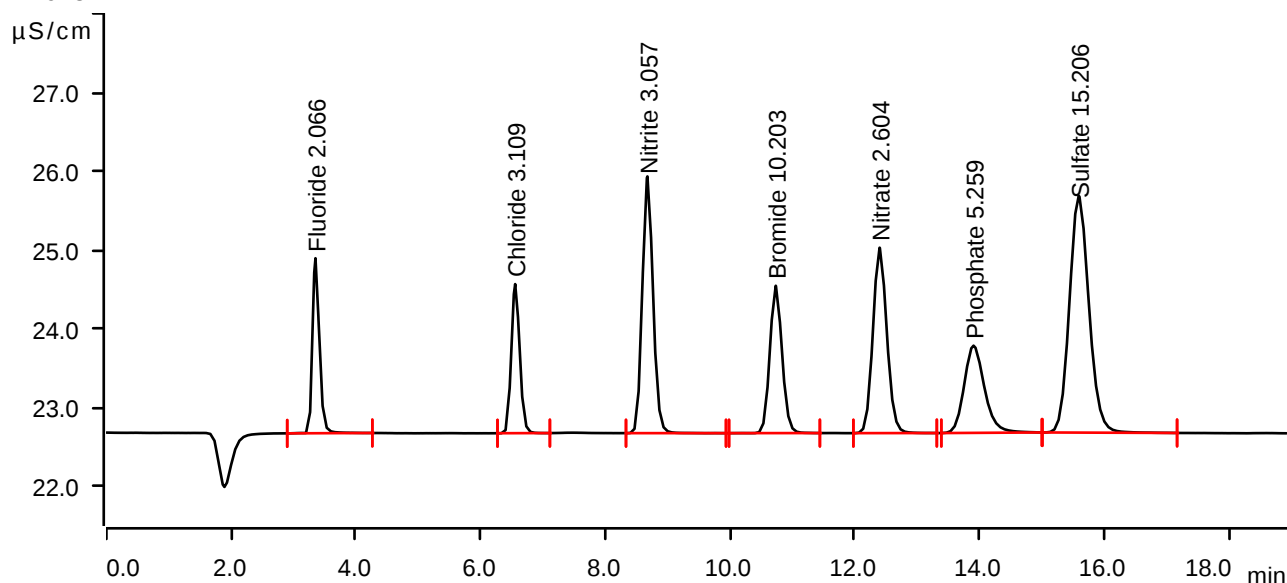


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.2854	2.220	2.066	Fluoride
2	6.555	0.2956	1.892	3.109	Chloride
3	8.675	0.6510	3.258	3.057	Nitrite
4	10.732	0.4255	1.870	10.203	Bromide
5	12.397	0.6116	2.353	2.604	Nitrate
6	13.903	0.4186	1.107	5.259	Phosphate
7	15.590	1.0908	3.005	15.206	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-05-28 20:18:21 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

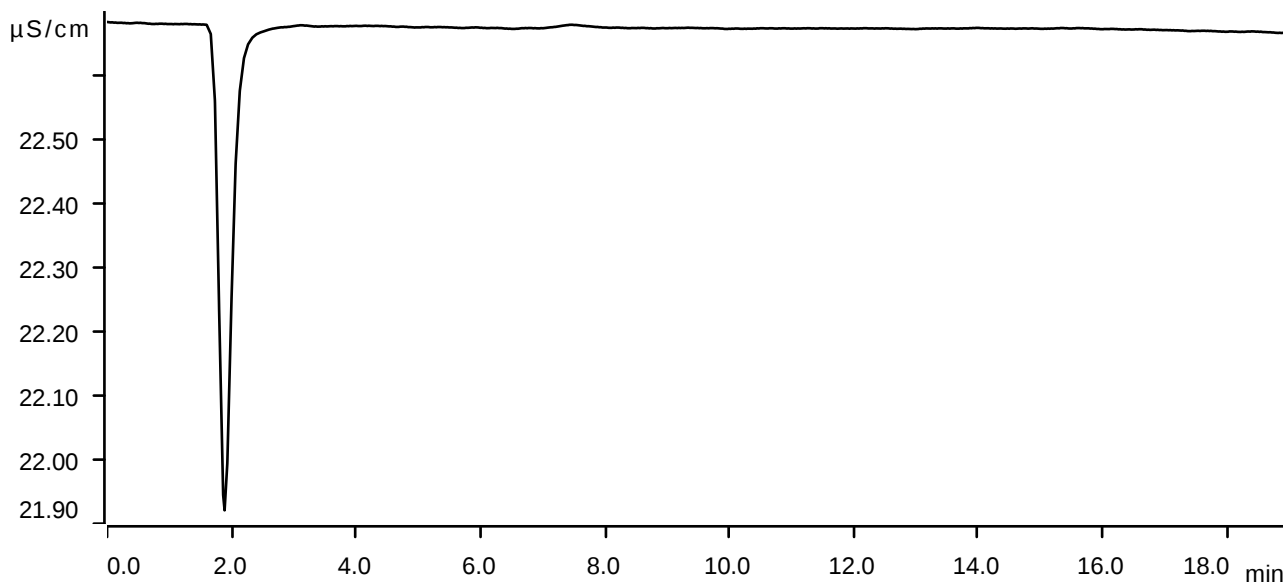Anions

Instrument ID: IC-1

Daily Analysis Runlog For Sequence/QC Batch ID # LB135928

Review By	rubina	Review On	5/30/2025 11:40:18 AM
Supervise By	Iwona	Supervise On	5/30/2025 12:35:36 PM
SubDirectory	LB135928	Test	Anions
STD. NAME	STD REF.#		
ICAL Standard	WP113186,WP113187,WP113188,WP113189,WP113190,WP113191,WP113192		
ICV Standard	WP113193		
CCV Standard	WP113251		
ICSA Standard	N/A		
CRI Standard	N/A		
LCS Standard	WP113252		
Chk Standard	WP113194,WP113195,WP113252,WP113254,WP113255		

Sr#	SampleId	ClientID	QcType	Date	Comment	Operator	Status
1	STD1	STD1	CAL1	05/22/25 11:09	All standards, samples, and	NF/IZ	OK
2	STD2	STD2	CAL2	05/22/25 11:30	QC are filtered through	NF/IZ	OK
3	STD3	STD3	CAL3	05/22/25 11:52	0.45um, filter lot W3160	NF/IZ	OK
4	STD4	STD4	CAL4	05/22/25 12:13		NF/IZ	OK
5	STD5	STD5	CAL5	05/22/25 12:35		NF/IZ	OK
6	STD6	STD6	CAL6	05/22/25 12:56		NF/IZ	OK
7	STD7	STD7	CAL7	05/22/25 13:17		NF/IZ	OK
8	ICV1	ICV1	ICV	05/22/25 13:39		NF/IZ	OK
9	ICB1	ICB1	ICB	05/22/25 14:22		NF/IZ	OK
10	CCV1	CCV1	CCV	05/28/25 11:29		NF/IZ	OK
11	CCB1	CCB1	CCB	05/28/25 11:51		NF/IZ	OK
12	LB135928BLW	LB135928BLW	MB	05/28/25 12:12		NF/IZ	OK
13	LB135928BSW	LB135928BSW	LCS	05/28/25 13:29		NF/IZ	OK
14	Q2126-08	LOQ-WATER-02-QT2	LOQ	05/28/25 13:51		NF/IZ	OK
15	Q2126-07	LOD-MDL-WATER-01	SAM	05/28/25 14:12		NF/IZ	OK
16	Q2126-07RE	LOD-MDL-WATER-01	SAM	05/28/25 14:34		NF/IZ	OK
17	Q2133-01	MW1	SAM	05/28/25 14:55	Cl is high	NF/IZ	Dilution
18	Q2133-02	MW5	SAM	05/28/25 15:17	Cl and SO4 is high	NF/IZ	Dilution

Instrument ID: IC-1

Daily Analysis Runlog For Sequence/QC Batch ID # LB135928

Review By	rubina	Review On	5/30/2025 11:40:18 AM
Supervise By	Iwona	Supervise On	5/30/2025 12:35:36 PM
SubDirectory	LB135928	Test	Anions
STD. NAME	STD REF.#		
ICAL Standard	WP113186,WP113187,WP113188,WP113189,WP113190,WP113191,WP113192		
ICV Standard	WP113193		
CCV Standard	WP113251		
ICSA Standard	N/A		
CRI Standard	N/A		
LCS Standard	WP113252		
Chk Standard	WP113194,WP113195,WP113252,WP113254,WP113255		

19	Q2133-03	SUPPLY	SAM	05/28/25 15:38	Cl is high	NF/IZ	Dilution
20	Q2133-03MS	SUPPLYMS	MS	05/28/25 16:00	9.5ml of sample, 0.5mL W3092	NF/IZ	OK
21	Q2133-03MSD	SUPPLYMSD	MSD	05/28/25 16:21	9.5ml of sample, 0.5mL W3092	NF/IZ	OK
22	CCV2	CCV2	CCV	05/28/25 16:43		NF/IZ	OK
23	CCB2	CCB2	CCB	05/28/25 17:05		NF/IZ	OK
24	Q2133-01DL	MW1DL	SAM	05/28/25 17:26	100X For Cl	NF/IZ	Confirms
25	Q2133-02DL	MW5DL	SAM	05/28/25 18:09	100X for CL and SO4, still Cl is high	NF/IZ	Dilution
26	Q2133-02DL2	MW5DL2	SAM	05/28/25 18:52	1000X for Cl	NF/IZ	Confirms
27	Q2133-03DL	SUPPLYDL	SAM	05/28/25 19:35	100X for Cl	NF/IZ	Confirms
28	CCV3	CCV3	CCV	05/28/25 19:56		NF/IZ	OK
29	CCB3	CCB3	CCB	05/28/25 20:18		NF/IZ	OK

Prep Standard - Chemical Standard Summary

Order ID : Q2133

Test : Anions Group1

Prepbatch ID :

Sequence ID/Qc Batch ID: LB135928,

Standard ID :

WP112796,WP113186,WP113187,WP113188,WP113189,WP113190,WP113191,WP113192,WP113193,WP113194,WP113195,WP113251,WP113252,WP113254,WP113255,

Chemical ID :

M6041,W2647,W3112,W3163,W3180,W3197,



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4035	IC ELUENT CONCENTRATE FOR IC-1	WP112796	04/22/2025	10/22/2025	Iwona Zarych	WETCHEM_SCALE_5 (WCS-5)	None	Jignesh Parikh 04/22/2025
<u>FROM</u> 2.10000gram of W2647 + 84.75000gram of W3163 + 913.15000ml of W3112 = Final Quantity: 1000.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2487	Anions 300/9056 calibration standard 1	WP113186	05/22/2025	05/23/2025	Iwona Zarych	None	WETCHEM_PIPETTE_3 (WC)	Jignesh Parikh 05/22/2025
<u>FROM</u> 10.00000ml of W3112 = Final Quantity: 10.000 ml								



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
24	Anions 300/9056 calibration standard 2	WP113187	05/22/2025	05/23/2025	Iwona Zarych	None	WETCHEM_PIPETTE_3	Jignesh Parikh
(WC) FROM 0.20000ml of W3180 + 9.80000ml of W3112 = Final Quantity: 10.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
25	Anions 300/9056 calibration standard 3	WP113188	05/22/2025	05/23/2025	Iwona Zarych	None	WETCHEM_PIPETTE_3 (WC)	Jignesh Parikh 05/22/2025
<u>FROM</u> 0.40000ml of W3180 + 9.60000ml of W3112 = Final Quantity: 10.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
26	Anions 300/9056 calibration standard 4	WP113189	05/22/2025	05/23/2025	Iwona Zarych	None	WETCHEM_F IPETTE_3 (WC)	Jignesh Parikh 05/22/2025
FROM 0.50000ml of W3180 + 9.50000ml of W3112 = Final Quantity: 10.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3680	Anions 300/9056 calibration standard 5-CCV	WP113190	05/22/2025	05/23/2025	Iwona Zarych	None	WETCHEM_F IPETTE_3 (WC)	Jignesh Parikh 05/22/2025
FROM 5.00000ml of W3180 + 95.00000ml of W3112 = Final Quantity: 50.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3679	Anions 300/9056 calibration standard 6	WP113191	05/22/2025	05/23/2025	Iwona Zarych	None	WETCHEM_F IPETTE_3 (WC)	Jignesh Parikh 05/22/2025
FROM 2.00000ml of W3180 + 8.00000ml of W3112 = Final Quantity: 10.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3681	Anions 300/9056 calibration standard 7	WP113192	05/22/2025	05/23/2025	Iwona Zarych	None	WETCHEM_F IPETTE_3 (WC)	Jignesh Parikh 05/22/2025
FROM 2.50000ml of W3180 + 7.50000ml of W3112 = Final Quantity: 10.000 ml								

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3233	Anions 300/9056 ICV-LCS std	WP113193	05/22/2025	05/23/2025	Iwona Zarych	None	WETCHEM_F IPETTE_3 (WC)	Jignesh Parikh 05/22/2025

FROM 45.00000ml of W3112 + 5.00000ml of W3197 = Final Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4036	IC ELUENT FOR IC-1	WP113194	05/22/2025	06/22/2025	Iwona Zarych	None	Glass Pipette-A	Jignesh Parikh 05/22/2025

FROM 1980.00000ml of W3112 + 20.00000ml of WP112796 = Final Quantity: 2000.000 ml

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4037	IC H2SO4 FOR IC-1	WP113195	05/22/2025	06/22/2025	Iwona Zarych	None	Glass Pipette-A	Jignesh Parikh 05/22/2025

FROM 5.60000ml of M6041 + 994.40000ml of W3112 = Final Quantity: 1000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3680	Anions 300/9056 calibration standard 5-CCV	WP113251	05/28/2025	05/29/2025	Iwona Zarych	None	WETCHEM_F IPETTE_3 (WC)	Jignesh Parikh 05/28/2025

FROM 45.00000ml of W3112 + 5.00000ml of W3180 = Final Quantity: 50.000 ml

Wet Chemistry STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3233	Anions 300/9056 ICV-LCS std	WP113252	05/28/2025	05/29/2025	Iwona Zarych	None	WETCHEM_F IPETTE_3 (WC)	Jignesh Parikh 05/28/2025

FROM 45.00000ml of W3112 + 5.00000ml of W3197 = Final Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3912	Anions 300/9056 LOD Std	WP113254	05/28/2025	05/29/2025	Iwona Zarych	None	WETCHEM_F IPETTE_3 (WC)	Jignesh Parikh 05/28/2025

FROM 0.50000ml of W3180 + 49.50000ml of W3112 = Final Quantity: 50.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3983	Anions 300/9056 LOD std 0.25ml spike	WP113255	05/28/2025	05/29/2025	Iwona Zarych	None	WETCHEM_PIPETTE_3	Jignesh Parikh
(WC) FROM 0.25000ml of W3180 + 49.75000ml of W3112 = Final Quantity: 50.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	23D2462010	03/20/2028	08/16/2024 / mohan	08/16/2024 / mohan	M6041

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	J3506-5 / SODIUM BICARBONATE, PWD, ACS, 2.5KG	0000240594	06/03/2026	02/24/2020 / AMANDEEP	01/20/2020 / apatel	W2647

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	EM-SX0395-3 / SODIUM CARBONATE ANHYDR 2.5KG	24E3156178	09/30/2027	12/10/2024 / lwona	12/10/2024 / lwona	W3163

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	300-CAL-A-500ML / 300.0 Calibration Standard, 500 ml	V2-MEB742616	02/19/2026	02/19/2025 / lwona	01/27/2025 / lwona	W3180

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	300-CAL-A-500ML / 300.0 Calibration Standard, 500 ml	040525	04/05/2027	04/08/2025 / lwona	04/08/2025 / lwona	W3197

Sodium Bicarbonate, Powder
BAKER ANALYZED® A.C.S. Reagent

(sodium hydrogen carbonate)



Material No.: 3506-05
Batch No.: 0000240594
Manufactured Date: 2019/06/05
Retest Date: 2026/06/03
Revision No: 1

Certificate of Analysis

Meets ACS Reagent Chemical Requirements,

Test	Specification	Result
Assay (NaHCO ₃) (dried basis)	99.7 – 100.3 %	100.1
Insoluble Matter	<= 0.015 %	< 0.002
Chloride (Cl)	<= 0.003 %	0.003
Phosphate (PO ₄)	<= 0.001 %	0.001
Sulfur Compounds (as SO ₄)	<= 0.003 %	0.003
Calcium (Ca)	<= 0.02 %	0.02
Trace Impurities – Iron (Fe)	<= 0.001 %	0.001
Magnesium (Mg)	<= 0.005 %	0.005
Potassium (K)	<= 0.005 %	0.005
Ammonium (NH ₄)	<= 5 ppm	5
Trace Impurities – ACS – Heavy Metals (as Pb)	<= 5 ppm	5

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

James Ethier
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium

avantor™



M 6041-4b
MS

Material No.: 9673-33
Batch No.: 23D2462010
Manufactured Date: 2023-03-22
Retest Date: 2028-03-20
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
ACS – Assay (H ₂ SO ₄)	95.0 – 98.0 %	96.1 %
Appearance	Passes Test	Passes Test
ACS – Color (APHA)	≤ 10	5
ACS – Residue after Ignition	≤ 3 ppm	< 1 ppm
ACS – Substances Reducing Permanganate (as SO ₂)	≤ 2 ppm	< 2 ppm
Ammonium (NH ₄)	≤ 1 ppm	1 ppm
Chloride (Cl)	≤ 0.1 ppm	< 0.1 ppm
Nitrate (NO ₃)	≤ 0.2 ppm	< 0.1 ppm
Phosphate (PO ₄)	≤ 0.5 ppm	< 0.1 ppm
Trace Impurities – Aluminum (Al)	≤ 30.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 4.0 ppb	< 2.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	8.5 ppb
Trace Impurities – Cadmium (Cd)	≤ 2.0 ppb	< 0.3 ppb
Trace Impurities – Chromium (Cr)	≤ 6.0 ppb	< 0.4 ppb
Trace Impurities – Cobalt (Co)	≤ 0.5 ppb	< 0.3 ppb
Trace Impurities – Copper (Cu)	≤ 1.0 ppb	< 0.1 ppb
Trace Impurities – Gold (Au)	≤ 10.0 ppb	0.5 ppb
Heavy Metals (as Pb)	≤ 500.0 ppb	< 100.0 ppb
Trace Impurities – Iron (Fe)	≤ 50.0 ppb	1.3 ppb
Trace Impurities – Lead (Pb)	≤ 0.5 ppb	< 0.5 ppb
Trace Impurities – Magnesium (Mg)	≤ 7.0 ppb	0.8 ppb
Trace Impurities – Manganese (Mn)	≤ 1.0 ppb	< 0.4 ppb
Trace Impurities – Mercury (Hg)	≤ 0.5 ppb	< 0.1 ppb
Trace Impurities – Nickel (Ni)	≤ 2.0 ppb	0.3 ppb
Trace Impurities – Potassium (K)	≤ 500.0 ppb	< 2.0 ppb
Trace Impurities – Selenium (Se)	≤ 50.0 ppb	< 0.1 ppb
Trace Impurities – Silicon (Si)	≤ 100.0 ppb	31.5 ppb
Trace Impurities – Silver (Ag)	≤ 1.0 ppb	< 0.3 ppb

>>> Continued on page 2 >>>

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium

 **avantor™**




Material No.: 9673-33
Batch No.: 23D2462010

Test	Specification	Result
Trace Impurities – Sodium (Na)	≤ 500.0 ppb	5.4 ppb
Trace Impurities – Strontium (Sr)	≤ 5.0 ppb	< 0.2 ppb
Trace Impurities – Tin (Sn)	≤ 5.0 ppb	< 0.8 ppb
Trace Impurities – Zinc (Zn)	≤ 5.0 ppb	0.4 ppb

For Laboratory, Research, or Manufacturing Use

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality



W3163 Rec. on 12/10/24 by IZ

Certificate of Analysis



Material BDH9284-2.5KG
Material Description BDH SODIUM CARB ANHYD ACS 2.5KG
Grade U S P REAGENT (ACS GRADE)

Batch 24E3156178
Reassay Date 09/30/2027
CAS Number 497-19-8
Molecular Formula Na_2CO_3
Molecular Mass 105.99

Date of Manufacture 09/01/2023
Storage Room Temperature
Material is hygroscopic. Protect from Moisture.
Additional Product Description:

Characteristics	Specifications	Measured Values
Appearance	Fine white granular powder	Fine white granular powder
Calcium	$\leq 0.03 \%$	0.003 %
Chloride	$\leq 0.001 \%$	0.0003 %
Heavy Metals (as Pb)	$\leq 0.0005 \%$	0.0001 %
Insolubles	$\leq 0.01 \%$	0.001 %
Iron	$\leq 0.0005 \%$	0.0001 %
Loss on Heating	$\leq 1.0 \%$	0.03 %
Magnesium	$\leq 0.005 \%$	0.001 %
Phosphate	$\leq 0.001 \%$	0.001 %
Potassium	$\leq 0.005 \%$	0.003 %
Purity	$\geq 99.5 \%$	100.0 %
Silica	$\leq 0.005 \%$	0.001 %
Sulfur Compounds	$\leq 0.003 \%$	0.002 %
Extra Description:	Meets Reagent Specifications for testing USP/NF monographs	

Internal ID #: 710

Signature	Additional Information
We certify that this batch conforms to the specifications listed above. This document has been electronically produced and is valid without a signature. Leona Edwardson, Quality Control Sr. Manager - Solon VWR Chemicals, LLC. 28600 Fountain Parkway, Solon OH 44139 USA	Analysis may have been rounded to significant digits in specification limits Product meets analytical specifications of the grades listed.



Refine your results. Redefine your industry.

Certificate of Analysis

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Ion Chromatography Solution
Catalog Number: 300-CAL-A
Lot Number: V2-MEB742616
Matrix: H₂O
Value / Analyte(s):
150 µg/mL ea:
Sulfate,
100 µg/mL ea:
Bromide,
50 µg/mL ea:
o-Phosphate as P,
30 µg/mL ea:
Chloride, Nitrite as N,
25 µg/mL ea:
Nitrate as N,
20 µg/mL ea:
Fluoride

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Bromide, Br	100.0 ± 0.5 µg/mL	Chloride, Cl	30.01 ± 0.13 µg/mL
Fluoride, F-	20.00 ± 0.07 µg/mL	Nitrate as N, NNO ₃ -	25.00 ± 0.10 µg/mL
Nitrite as N, NNO ₂ -	30.00 ± 0.10 µg/mL	o-Phosphate as P, PPO ₄	50.00 ± 0.18 µg/mL
Sulfate, SO ₄	150.0 ± 0.8 µg/mL		

Density: 0.999 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
Br	IC Assay	3184	151130
Br	Fajans	999c	999c
Cl	IC Assay	3182	190830
Cl	Fajans	999c	999c
F-	IC Assay	3183	140203
NNO3-	IC Assay	3185	170309
NNO2-	IC Assay	Traceable to 40H	08228TH-H2
NNO2-	Calculated	40h	40h
PPO4	IC Assay	3186	170606
SO4	IC Assay	3181	080603

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum (1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = [\sum (w_i)^2 (u_{\text{char } i}^2)]^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a) (u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 CHROMATOGRAM

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures [Terms and Conditions of Sale](https://www.inorganicventures.com/terms-and-conditions-sale). The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.
- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.
- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

April 02, 2024

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- **April 02, 2029**

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Prepared By:

Uyen Truong
Custom Processing Supervisor



Certificate Approved By:

Thomas Kozikowski
Stock VS Manager



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



Ident	Instrument IC-1				Analyst : NF		Method: 300.0 / 9056A		Initial Analyst		
	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4				
STD1	0	0	0	0	0	0	0	0	IC1-032125	3/21/2025 10:45	10 NF/IZ
STD2	0.421	0.619	0.631	2.075	0.523	1.052	3.247	IC1-032125	3/21/2025 11:07	10 NF/IZ	
STD3	0.795	1.199	1.203	3.994	1.001	1.993	5.998	IC1-032125	3/21/2025 11:28	10 NF/IZ	
STD4	0.977	1.475	1.468	4.904	1.226	2.407	7.216	IC1-032125	3/21/2025 11:50	10 NF/IZ	
STD5	1.993	3.009	2.995	10.03	2.493	4.968	14.842	IC1-032125	3/21/2025 12:11	10 NF/IZ	
STD6	4.034	5.988	5.986	19.975	5.011	10.256	30.502	IC1-032125	3/21/2025 12:32	10 NF/IZ	
STD7	4.979	7.51	7.517	25.022	6.247	12.323	36.695	IC1-032125	3/21/2025 12:54	10 NF/IZ	
ICV	2.031	3.038	3.08	10.364	2.568	5.199	15.269	IC1-032125	3/21/2025 13:37	10 NF/IZ	
ICB	0	0.122	0.08	0	0	0	0	IC1-032125	3/21/2025 13:58	10 NF/IZ	
CCV	2.034	3.119	3.093	10.383	2.559	5.188	15.179	IC1-032125	4/3/2025 9:38	10 NF/IZ	
CCB	0	0	0	0	0	0	0	IC1-032125	4/3/2025 9:59	10 NF/IZ	
LB135296BSW	2.028	3.121	3.103	10.387	2.561	5.226	15.185	IC1-032125	4/3/2025 10:43	10 NF/IZ	
LB135296BLW	0	0	0	0	0	0	0	IC1-032125	4/3/2025 11:04	10 NF/IZ	
Q1711-01	0.332	26.59	0	0.215	0	2.108	10.666	IC1-032125	4/3/2025 12:29	10 NF/IZ	
Q1711-02MS	2.301	28.881	3.076	10.43	2.571	2.367	24.892	IC1-032125	4/3/2025 12:50	10 NF/IZ	
Q1711-03MSD	2.172	28.857	2.983	10.101	2.479	1.573	24.485	IC1-032125	4/3/2025 13:12	10 NF/IZ	
Q1711-04	0.275	20.1	0	0.221	0	0	4.529	IC1-032125	4/3/2025 13:55	10 NF/IZ	
Q1711-08	0	0.047	0	0	0	0	0	IC1-032125	4/3/2025 14:16	10 NF/IZ	
Q1716-01	0.433	427.687	0	0.63	0.296	0	54.697	IC1-032125	4/3/2025 14:38	10 NF/IZ	
Q1711-01DLX10	0.054	2.364	0	0	0	0	1.413	IC1-032125	4/3/2025 14:59	10 NF/IZ	
Q1711-04DLX5	0.071	3.687	0	0	0	0	1.238	IC1-032125	4/3/2025 15:21	10 NF/IZ	
CCV	2.072	3.107	3.112	10.418	2.589	5.237	15.386	IC1-032125	4/3/2025 15:43	10 NF/IZ	
CCB	0	0	0	0	0	0	0	IC1-032125	4/3/2025 17:16	10 NF/IZ	



SHIPPING DOCUMENTS

CLIENT INFORMATION

CLIENT PROJECT INFORMATION

CLIENT BILLING INFORMATION

REPORT TO BE SENT TO:
COMPANY: G Environmental
ADDRESS: 8 CARRAGE
CITY: Succesuna STATE: NJ ZIP:
ATTENTION:
PHONE: FAX:

PROJECT NAME: BANKER
PROJECT NO.: LOCATION:
PROJECT MANAGER: GL
e-mail:
PHONE: FAX:

BILL TO: G Environmental PO#:
ADDRESS: 8 CARRAGE
CITY: Succesuna STATE: NJ ZIP:
ATTENTION: PHONE:
ANALYSIS

DATA TURNAROUND INFORMATION

DATA DELIVERABLE INFORMATION

FAX (RUSH) DAYS*
HARDCOPY (DATA PACKAGE): DAYS*
EDD: DAYS*
*TO BE APPROVED BY CHEMTECH
STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS

☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)
☐ Level 2 (Results + QC) ☒ NJ Reduced ☐ US EPA CLP
☐ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B
+ Raw Data ☐ Other
☒ EDD FORMAT has 25k edel

Sodium Chloride
1 2 3 4 5 6 7 8 9

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES									COMMENTS
			COMP	GRAB	DATE	TIME		1	2	3	4	5	6	7	8	9	
1.	MW1	GW		X	5/27/25	1000	2	X	X								
2.	MW5	GW		X	5/27/25	1130	2	X	X								
3.	Supply	GW		X	5/27/25	1209	2	X	X								
4.																	
5.																	
6.																	
7.																	
8.																	
9.																	
10.																	

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER: 1. <u>AKD</u>	DATE/TIME: <u>9:37</u> <u>5/28/25</u>	RECEIVED BY: 1. <u>AKD</u>	Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP <u>2-1°C</u>
RELINQUISHED BY SAMPLER: 2.	DATE/TIME:	RECEIVED BY: 2.	Comments: <u>IR-GW #1</u>
RELINQUISHED BY SAMPLER: 3.	DATE/TIME:	RECEIVED BY: 3.	Page ____ of CLIENT: ☐ Hand Delivered ☐ Other Shipment Complete ☐ YES ☐ NO

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488