

## Prep Standard - Chemical Standard Summary

**Order ID :** Q2147

**Test :** EPH\_F2

**Prepbatch ID :** PB168239,

**Sequence ID/Qc Batch ID:** FE060325AL,

**Standard ID :**

EP2612,EP2620,PP24170,PP24174,PP24175,PP24176,PP24177,PP24178,PP24179,PP24573,PP24591,

**Chemical ID :**

E2865,E3551,E3930,E3932,E3939,P12363,P12981,P12983,P13279,P13601,P13603,P13650,P13671,P13676,P13677,  
P13710,P13711,P13712,P13713,P13714,P13716,P13822,P13825,P13827,P13902,P13904,P13914,P13922,P13924,P1  
3978,P13979,P13980,P13981,P13988,P13989,W3177,

### Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2017	1:1 ACETONE/METHYLENE CHLORIDE	<a href="#">EP2612</a>	05/09/2025	11/05/2025	RUPESHKUMAR SHAH	None	None	Riteshkumar Patel 05/09/2025

**FROM** 8000.00000ml of E3930 + 8000.00000ml of E3932 = Final Quantity: 16000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	<a href="#">EP2620</a>	05/30/2025	07/01/2025	RUPESHKUMAR SHAH	Extraction_SC ALE_2 (EX-SC-2)	None	Riteshkumar Patel 05/30/2025

**FROM** 4000.00000gram of E3551 = Final Quantity: 4000.000 gram

### Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
781	100 PPM Aliphatic HC Working STD (Restek)	<a href="#">PP24170</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani 02/03/2025

**FROM** 0.25000ml of P12981 + 0.25000ml of P13671 + 1.25000ml of P12363 + 23.25000ml of W3177 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2900	100 PPM Aliphatic HC STD (Absolute)	<a href="#">PP24174</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani 02/03/2025

**FROM** 0.25000ml of P12983 + 0.25000ml of P13650 + 2.50000ml of P13279 + 22.00000ml of W3177 = Final Quantity: 25.000 ml

### Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
783	50 PPM Aliphatic HC STD	<a href="#">PP24175</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani 02/03/2025

**FROM** 0.50000ml of W3177 + 0.50000ml of PP24170 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
784	20 PPM Aliphatic HC STD	<a href="#">PP24176</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani 02/03/2025

**FROM** 0.80000ml of W3177 + 0.20000ml of PP24170 = Final Quantity: 1.000 ml

### Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
785	10 PPM Aliphatic HC STD	<a href="#">PP24177</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani 02/03/2025

**FROM** 0.90000ml of W3177 + 0.10000ml of PP24170 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
786	5 PPM Aliphatic HC STD	<a href="#">PP24178</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani 02/03/2025

**FROM** 0.90000ml of W3177 + 0.10000ml of PP24175 = Final Quantity: 1.000 ml

### Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2901	20 PPM Aliphatic HC STD ICV (Absolute)	<a href="#">PP24179</a>	02/03/2025	08/03/2025	Yogesh Patel	None	None	Ankita Jodhani  02/03/2025

**FROM** 0.80000ml of W3177 + 0.20000ml of PP24174 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1330	100 PPM NJEPH Spike Solution	<a href="#">PP24573</a>	05/14/2025	11/14/2025	Abdul Mirza	None	None	Yogesh Patel  05/22/2025

**FROM** 5.00000ml of P13710 + 5.00000ml of P13711 + 5.00000ml of P13712 + 5.00000ml of P13713 + 5.00000ml of P13714 + 5.00000ml of P13716 + 5.00000ml of P13822 + 5.00000ml of P13825 + 5.00000ml of P13827 + 5.00000ml of P13902 + 5.00000ml of P13904 + 5.00000ml of P13914 + 5.00000ml of P13922 + 5.00000ml of P13924 + 5.00000ml of P13978 + 5.00000ml of P13979 + 5.00000ml of P13980 + 5.00000ml of P13981 + 5.00000ml of P13988 + 5.00000ml of P13989 = Final Quantity: 100.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1339	100 PPM NJEPH Surrogate Spike	<a href="#">PP24591</a>	05/19/2025	11/05/2025	Abdul Mirza	None	None	Yogesh Patel
								05/22/2025
<b>FROM</b>	1.00000ml of P13601 + 1.00000ml of P13603 + 1.00000ml of P13676 + 1.00000ml of P13677 + 196.00000ml of E3932 = Final Quantity: 200.000 ml							

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	06/30/2025	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	12/04/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	25A0262002	02/20/2026	05/02/2025 / RUPESH	03/09/2025 / RUPESH	E3930

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	11/05/2025	05/05/2025 / RUPESH	04/23/2025 / RUPESH	E3932

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	25A2862010	11/22/2025	05/22/2025 / RUPESH	02/28/2025 / RUPESH	E3939

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30540 / Custom NJEPH Aliphatics Calibration Standard	A0190424	08/03/2025	02/03/2025 / yogesh	03/16/2023 / Yogesh	P12363

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0204989	08/03/2025	02/03/2025 / yogesh	12/20/2023 / Yogesh	P12981

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0204989	08/03/2025	02/03/2025 / yogesh	12/20/2023 / Yogesh	P12983

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95899 / NJ EPH Aliphatic n-Hydrocarbons-Revised, 1000 PPM	040524	08/03/2025	02/03/2025 / yogesh	04/11/2024 / yogesh	P13279

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0213283	11/19/2025	05/19/2025 / Abdul	10/16/2024 / yogesh	P13601

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0213283	11/19/2025	05/19/2025 / Abdul	10/16/2024 / yogesh	P13603

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	08/03/2025	02/03/2025 / yogesh	10/16/2024 / yogesh	P13650

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	08/03/2025	02/03/2025 / yogesh	10/16/2024 / yogesh	P13671

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	11/19/2025	05/19/2025 / Abdul	10/16/2024 / yogesh	P13676

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0216631	11/19/2025	05/19/2025 / Abdul	10/16/2024 / yogesh	P13677

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0211254	11/14/2025	05/14/2025 / Abdul	10/24/2024 / yogesh	P13710

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0211254	11/14/2025	05/14/2025 / Abdul	10/24/2024 / yogesh	P13711

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0211254	11/14/2025	05/14/2025 / Abdul	10/24/2024 / yogesh	P13712

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0211254	11/14/2025	05/14/2025 / Abdul	10/24/2024 / yogesh	P13713

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0211254	11/14/2025	05/14/2025 / Abdul	10/24/2024 / yogesh	P13714

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0211254	11/14/2025	05/14/2025 / Abdul	10/24/2024 / yogesh	P13716

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	11/14/2025	05/14/2025 / Abdul	12/09/2024 / yogesh	P13822

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	11/14/2025	05/14/2025 / Abdul	12/09/2024 / yogesh	P13825

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	11/14/2025	05/14/2025 / Abdul	12/09/2024 / yogesh	P13827

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	11/14/2025	05/14/2025 / Abdul	03/06/2025 / yogesh	P13902

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0217408	11/14/2025	05/14/2025 / Abdul	03/06/2025 / yogesh	P13904

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0220449	11/14/2025	05/14/2025 / Abdul	03/06/2025 / yogesh	P13914

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A022580	11/14/2025	05/14/2025 / Abdul	03/06/2025 / yogesh	P13922

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A022580	11/14/2025	05/14/2025 / Abdul	03/06/2025 / yogesh	P13924

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0220449	11/14/2025	05/14/2025 / Abdul	04/24/2025 / Rahul	P13978

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0220449	11/14/2025	05/14/2025 / Abdul	04/24/2025 / Rahul	P13979

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0220449	11/14/2025	05/14/2025 / Abdul	04/24/2025 / Rahul	P13980

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0220449	11/14/2025	05/14/2025 / Abdul	04/24/2025 / Rahul	P13981

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0220580	11/14/2025	05/14/2025 / Abdul	04/25/2025 / Rahul	P13988

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0220580	11/14/2025	05/14/2025 / Abdul	04/25/2025 / Rahul	P13989

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	08/22/2025	02/03/2025 / jignesh	01/31/2025 / jignesh	W3177

Sand  
Purified  
Washed and Ignited



Material No.: 3382-05  
Batch No.: 0000243821  
Manufactured Date: 2018/04/09  
Retest Date: 2025/04/07  
Revision No: 1

## Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use  
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US  
Packaging Site: Paris Mfg Ctr & DC

E 2865

*James Ethier*  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700  
Avantor Performance Materials, LLC  
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



**PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MEXICO  
CP 64070  
TEL +52 81 13 52 57 57  
www.pqm.com.mx

# CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na <sub>2</sub> SO <sub>4</sub>
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na <sub>2</sub> SO <sub>4</sub> )	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO <sub>4</sub> )	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

## COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/29/23 E 3551

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)

avantor



Material No.: 9266-A4  
Batch No.: 25A0262002  
Manufactured Date: 2024-11-21  
Expiration Date: 2026-02-20  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	$\leq 10$	4
Assay (CH <sub>2</sub> Cl <sub>2</sub> ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	99.9 %
Color (APHA)	$\leq 10$	10
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.8 ppm
Titration Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	$< 0.1$
Chloride (Cl)	$\leq 10 \text{ ppm}$	$< 5 \text{ ppm}$
Water (by KF, coulometric)	$\leq 0.02 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

E3930

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

Acetone  
BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis

Avantor™



Material No.: 9254-03  
Batch No.: 24H1462005  
Manufactured Date: 2024-05-24  
Expiration Date: 2027-05-24  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected forwater)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H <sub>2</sub> O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol)Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

RS

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3932

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 25A2862010  
Manufactured Date: 2024-12-18  
Expiration Date: 2026-03-19  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	2
Assay (CH <sub>2</sub> Cl <sub>2</sub> ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	99.9 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0$ ppm	0.3 ppm
Titration Acid ( $\mu$ eq/g)	$\leq 0.3$	<0.1
Chloride (Cl)	$\leq 10$ ppm	<5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	<0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

E3939

  
Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700  
Avantor Performance Materials, LLC  
100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700



110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: (800)356-1688  
 Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis



ISO 17034 Accredited  
 Reference Material Producer  
 Certificate #3222.01



ISO/IEC 17025 Accredited  
 Testing Laboratory  
 Certificate #3222.02



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30540 **Lot No.:** A0190424

**Description :** NJEPH Aliphatics Calibration Standard  
Aliphatics Calibration Standard 2000µg/mL, Hexane/Carbon Disulfide (80:20), 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** November 30, 2029 **Storage:** 25°C nominal

**Handling:** Sonicate prior to use. **Ship:** Ambient

P12361  
 ↓  
 P12370 } Y.P.  
 03/16/23

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)			
1	n-Nonane (C9)	2,014.0 µg/mL (Lot SHBN5361)	+/-	11.8193	µg/mL	Gravimetric
	CAS # 111-84-2		+/-	50.0027	µg/mL	Unstressed
	Purity 99%		+/-	59.9491	µg/mL	Stressed
2	n-Decane (C10)	2,014.7 µg/mL (Lot SHBN8619)	+/-	11.8232	µg/mL	Gravimetric
	CAS # 124-18-5		+/-	50.0193	µg/mL	Unstressed
	Purity 99%		+/-	59.9689	µg/mL	Stressed
3	Naphthalene	2,015.3 µg/mL (Lot MKCH0219)	+/-	11.8271	µg/mL	Gravimetric
	CAS # 91-20-3		+/-	50.0358	µg/mL	Unstressed
	Purity 99%		+/-	59.9888	µg/mL	Stressed
4	n-Dodecane (C12)	2,008.0 µg/mL (Lot SHBN7174)	+/-	11.7841	µg/mL	Gravimetric
	CAS # 112-40-3		+/-	49.8538	µg/mL	Unstressed
	Purity 99%		+/-	59.7705	µg/mL	Stressed
5	2-Methylnaphthalene	2,007.0 µg/mL (Lot STBK0259)	+/-	11.7784	µg/mL	Gravimetric
	CAS # 91-57-6		+/-	49.8299	µg/mL	Unstressed
	Purity 96%		+/-	59.7419	µg/mL	Stressed
6	n-Tetradecane (C14)	2,016.7 µg/mL (Lot STBK2282)	+/-	11.8349	µg/mL	Gravimetric
	CAS # 629-59-4		+/-	50.0689	µg/mL	Unstressed
	Purity 99%		+/-	60.0284	µg/mL	Stressed
7	n-Hexadecane (C16)	2,014.9 µg/mL (Lot SHBM4146)	+/-	11.8244	µg/mL	Gravimetric
	CAS # 544-76-3		+/-	50.0246	µg/mL	Unstressed
	Purity 98%		+/-	59.9753	µg/mL	Stressed

8	n-Octadecane (C18) CAS # 593-45-3 Purity 97%	(Lot VZKOJ)	2,004.7 µg/mL	+/- 11.7645 +/- 49.7710 +/- 59.6712	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Eicosane (C20) CAS # 112-95-8 Purity 99%	(Lot MKCF7888)	2,018.0 µg/mL	+/- 11.8428 +/- 50.1020 +/- 60.0681	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Heneicosane (C21) CAS # 629-94-7 Purity 99%	(Lot MKCL3226)	2,000.7 µg/mL	+/- 11.7410 +/- 49.6717 +/- 59.5522	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	2,005.3 µg/mL	+/- 11.7684 +/- 49.7876 +/- 59.6911	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	2,018.0 µg/mL	+/- 11.8428 +/- 50.1020 +/- 60.0681	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	2,014.0 µg/mL	+/- 11.8193 +/- 50.0027 +/- 59.9491	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	2,002.0 µg/mL	+/- 11.7489 +/- 49.7048 +/- 59.5919	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Triacontane (C30) CAS # 638-68-6 Purity 97%	(Lot MKCQ9436)	2,011.1 µg/mL	+/- 11.8025 +/- 49.9316 +/- 59.8637	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	2,012.0 µg/mL	+/- 11.8075 +/- 49.9531 +/- 59.8895	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	2,006.7 µg/mL	+/- 11.7762 +/- 49.8207 +/- 59.7308	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
18	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot Z27H018)	2,017.3 µg/mL	+/- 11.8388 +/- 50.0855 +/- 60.0483	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
19	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 96%	(Lot 0000145137)	2,017.3 µg/mL	+/- 11.8385 +/- 50.0842 +/- 60.0467	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
20	n-Tetracontane (C40) CAS # 4181-95-7 Purity 99%	(Lot BSBME)	2,008.7 µg/mL	+/- 11.7880 +/- 49.8703 +/- 59.7903	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed

**Solvent:** Hexane/Carbon disulfide (80:20)  
CAS # 110-54-3/75-15-0  
Purity 99%

**Column:**  
30m x 0.25mm x 0.25µm  
Plex-5 (cat.#10223)


**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

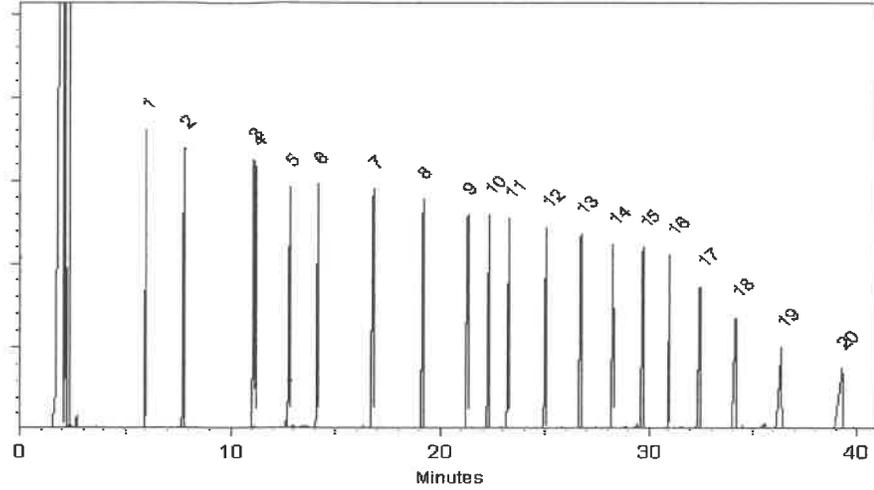

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Morgan Craighead - Mix Technician

Date Mixed: 10-Oct-2022      Balance: 1128360905

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Oct-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31098 Lot No.: A0204989  
 Description : 1-Chlorooctadecane Standard  
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride,  
1mL/ampul  
 Container Size : 2 mL Pkg Amt: > 1 mL  
 Expiration Date : January 31, 2031 Storage: 10°C or colder  
 Ship: Ambient

P12960 } Y.P.  
 ↓ }  
 P12991 } 12/21/2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	14738400	99%	10,097.3 µg/mL	+/- 567.2675

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride  
 CAS # 75-09-2  
 Purity 99%

# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

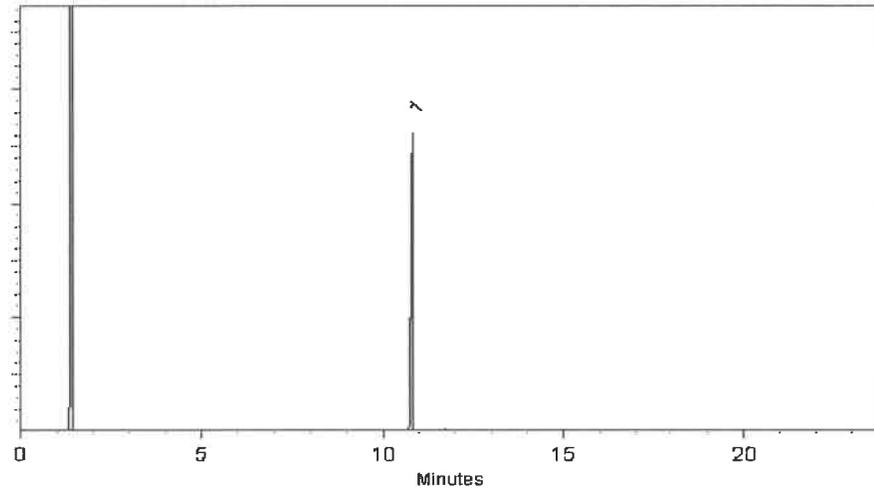

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 02-Dec-2023

Balance Serial # B345965662

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Dec-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31098 Lot No.: A0204989  
 Description : 1-Chlorooctadecane Standard  
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride,  
1mL/ampul  
 Container Size : 2 mL Pkg Amt: > 1 mL  
 Expiration Date : January 31, 2031 Storage: 10°C or colder  
 Ship: Ambient

P12960 } Y.P.  
 ↓  
 P12991 } 12/21/2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	14738400	99%	10,097.3 µg/mL	+/- 567.2675

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride  
 CAS # 75-09-2  
 Purity 99%

# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

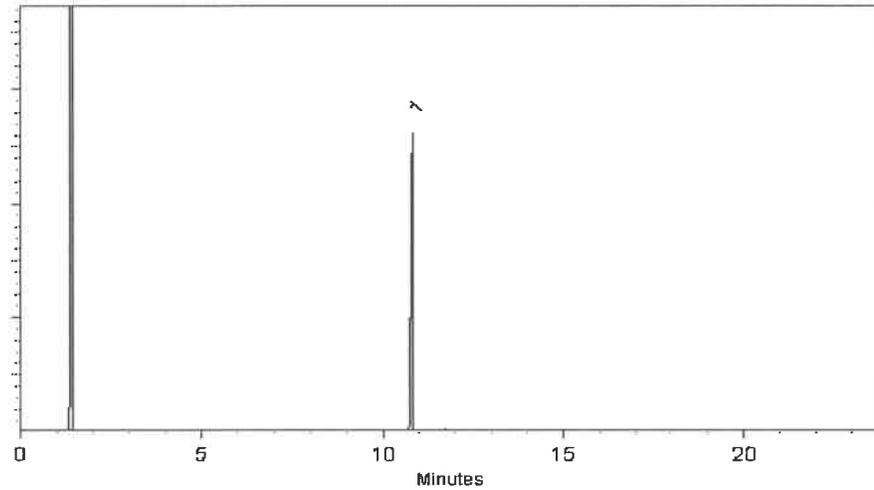

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Peter Robbins - Operations Technician I

Date Mixed: 02-Dec-2023

Balance Serial # B345965662

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Dec-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.


### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.


### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





**Certified Reference Material CRM**



**CERTIFIED WEIGHT REPORT**

Part Number: **95999**  
Lot Number: **040524**  
Description: **NJ EPH Aliphatic n-Hydrocarbons - Revised**  
20 components  
Expiration Date: **040534**  
Recommended Storage: **Ambient (20 °C)**  
Nominal Concentration (µg/mL): **1000**  
NIST Test ID#: **6UTB**  
5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

Solvent(s): **Cyclohexane**  
Lot# **28930**

Formulated By: <i>Anthony Mahoney</i>	040524
DATE	DATE
Reviewed By: <i>Pedro L. Rentas</i>	040524
DATE	DATE

*P13278*  
*Y.P.*  
*P13287*  
*04/11/24*

Weight(s) shown below were combined and diluted to (mL):  
**CAUTION: Sonicate Before Use**

Compound	(RM#)	Lot Number	DIL Factor	Initial Vol. (mL)	Initial Conc. (µg/mL)	Nominal Conc. (µg/mL)	Purity (%)	Purity Uncertainty	Pipette	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)	LD50
1. 2-Methylnaphthalene	(0214)	MKBF3783V	NA	NA	NA	1000	97	0.2	NA	0.02579	0.02594	1005.7	5.7	91-57-6	N/A	N/A	or-rat 1630mg/kg
2. Naphthalene	(0222)	MKBZ8680V	NA	NA	NA	1000	100	0.2	NA	0.02502	0.02511	1003.7	5.7	91-20-3	10 ppm (50mg/m <sup>3</sup> /8H)	or-trat 490mg/kg	
3. n-Nonane	95708	120222	1.00	25.00	1000.7	1000	NA	0.013	NA	NA	NA	1000.0	4.2	111-84-2	200 ppm (1050mg/m <sup>3</sup> /8H)	ivt-rms 218mg/kg	
4. n-Decane	95708	120222	1.00	25.00	1000.9	1000	NA	0.013	NA	NA	NA	1000.2	4.2	124-18-5	N/A	N/A	
5. n-Dodecane	95708	120222	1.00	25.00	1000.7	1000	NA	0.013	NA	NA	NA	1000.0	4.2	112-40-3	N/A	N/A	ivt-rms 3494mg/kg
6. n-Tetradecane	95708	120222	1.00	25.00	1002.1	1000	NA	0.013	NA	NA	NA	1001.3	4.2	629-59-4	N/A	N/A	
7. n-Hexadecane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	999.7	4.2	544-76-3	N/A	N/A	
8. n-Octadecane	95708	120222	1.00	25.00	1001.0	1000	NA	0.013	NA	NA	NA	1000.3	4.1	593-45-3	N/A	N/A	
9. n-Eicosane	95708	120222	1.00	25.00	1001.0	1000	NA	0.013	NA	NA	NA	1000.3	4.2	112-95-8	N/A	N/A	
10. n-Heneicosane	95708	120222	1.00	25.00	1002.4	1000	NA	0.013	NA	NA	NA	1001.6	4.2	629-94-7	N/A	N/A	
11. n-Docosane	95708	120222	1.00	25.00	1001.9	1000	NA	0.013	NA	NA	NA	1001.2	4.2	629-97-0	N/A	N/A	
12. n-Tetracosane	95708	120222	1.00	25.00	1000.8	1000	NA	0.013	NA	NA	NA	1000.1	4.2	646-31-1	N/A	N/A	
13. n-Hexacosane	95708	120222	1.00	25.00	1001.2	1000	NA	0.013	NA	NA	NA	1000.4	4.2	690-01-3	N/A	N/A	
14. n-Octacosane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	999.8	4.2	630-02-4	N/A	N/A	
15. n-Triacontane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	999.8	4.2	638-68-6	N/A	N/A	
16. n-Dotriacontane	95708	120222	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	999.8	4.3	544-85-4	N/A	N/A	
17. n-Tetracontane	95708	120222	1.00	25.00	1000.4	1000	NA	0.013	NA	NA	NA	999.7	4.2	14167-59-0	N/A	N/A	
18. n-Hexatriacontane	95708	120222	1.00	25.00	1001.5	1000	NA	0.013	NA	NA	NA	1000.8	4.2	630-06-8	N/A	N/A	
19. n-Octatriacontane	95708	120222	1.00	25.00	1000.3	1000	NA	0.013	NA	NA	NA	999.6	4.3	7184-86-6	N/A	N/A	
20. n-Tetracontane	95708	120222	1.00	25.00	1000.6	1000	NA	0.013	NA	NA	NA	999.9	4.3	4181-95-7	N/A	N/A	

\* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
 \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
 \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.  
 \* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
 \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31098 Lot No.: A0213283  
 Description : 1-Chlorooctadecane Standard  
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride,  
1mL/ampul  
 Container Size : 2 mL Pkg Amt: > 1 mL  
 Expiration Date : July 31, 2031 Storage: 10°C or colder  
 Ship: Ambient

P13595 } Y.P.  
 ↓  
 P13624 } 10/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	15018900	99%	10,058.0 µg/mL	+/- 565.0578

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride  
 CAS # 75-09-2  
 Purity 99%



# Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
10 ml/min.

**Inj. Vol**  
1µl

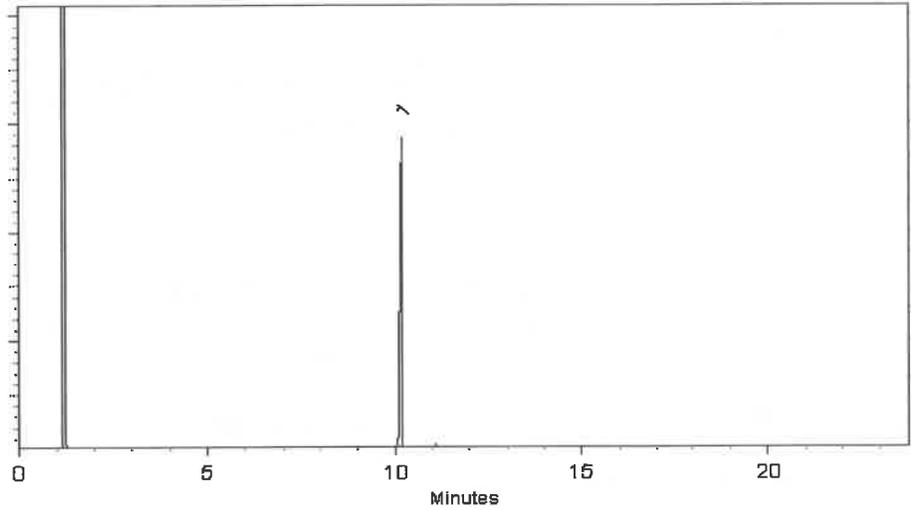

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Stacey S. Wann*

Stacey Wann - Operations Technician I

Date Mixed: 28-Jun-2024

Balance Serial # B345965662

*Dylan Murphy*

Dylan Murphy - Operations Technician I

Date Passed: 01-Jul-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31098 Lot No.: A0213283  
 Description : 1-Chlorooctadecane Standard  
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul  
 Container Size : 2 mL Pkg Amt: > 1 mL  
 Expiration Date : July 31, 2031 Storage: 10°C or colder  
 Ship: Ambient

P13595 } Y.P.  
 ↓  
 P13624 } 10/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Chlorooctadecane	3386-33-2	15018900	99%	10,058.0 µg/mL	+/- 565.0578

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride  
 CAS # 75-09-2  
 Purity 99%



# Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
10 ml/min.

**Inj. Vol**  
1µl

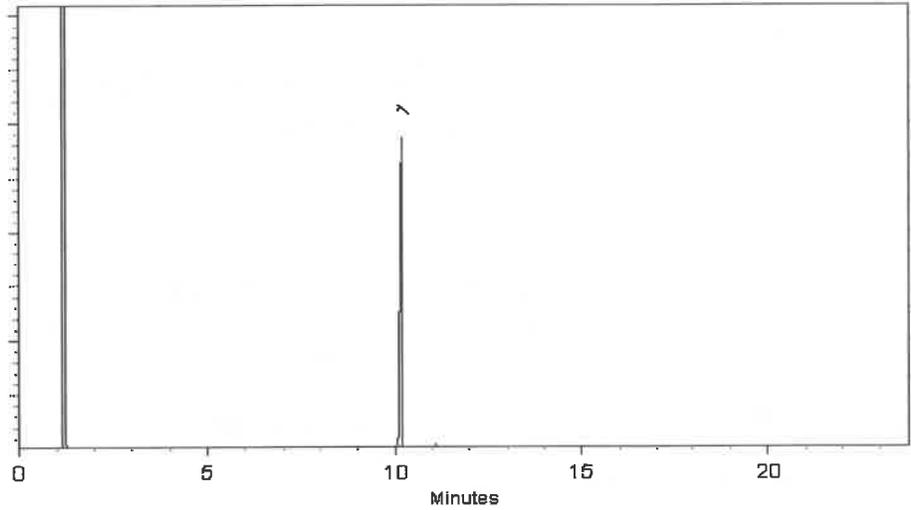

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wannner - Operations Technician I

Date Mixed: 28-Jun-2024

Balance Serial # B345965662

Dillan Murphy - Operations Technician I

Date Passed: 01-Jul-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31097 Lot No.: A0216631  
 Description : o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
 Container Size : 2 mL Pkg Amt: > 1 mL  
 Expiration Date : April 30, 2028 Storage: 10°C or colder  
 Handling: Sonicate prior to use. Ship: Ambient

P13645 } Y.P.  
 ↓  
 P13694 } 10/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,065.0 µg/mL	+/- 453.3336

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride  
 CAS # 75-09-2  
 Purity 99%



# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rbx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

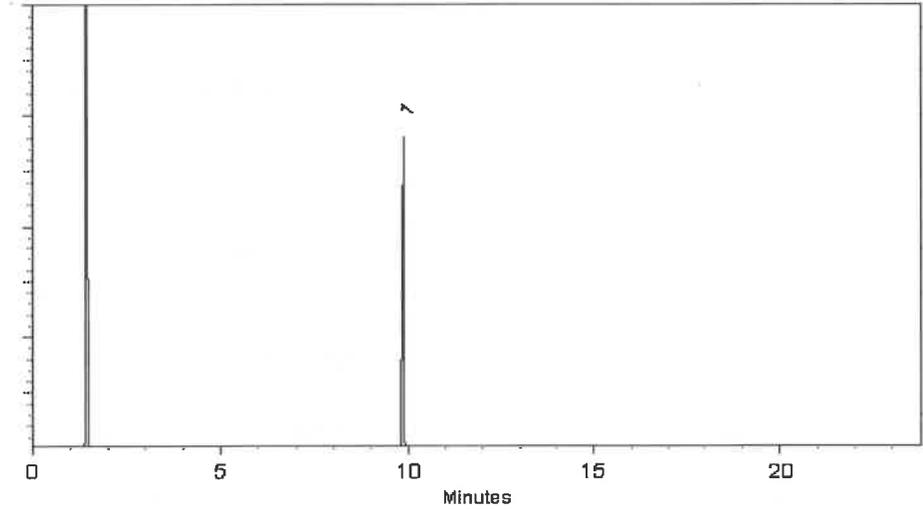

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ven Kelley*

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

*Dillon Murphy*

Dillon Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31097 Lot No.: A0216631  
 Description : o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
 Container Size : 2 mL Pkg Amt: > 1 mL  
 Expiration Date : April 30, 2028 Storage: 10°C or colder  
 Handling: Sonicate prior to use. Ship: Ambient

P13645 } Y.P.  
 ↓  
 P13694 } 10/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,065.0 µg/mL	+/- 453.3336

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride  
 CAS # 75-09-2  
 Purity 99%



# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rbx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

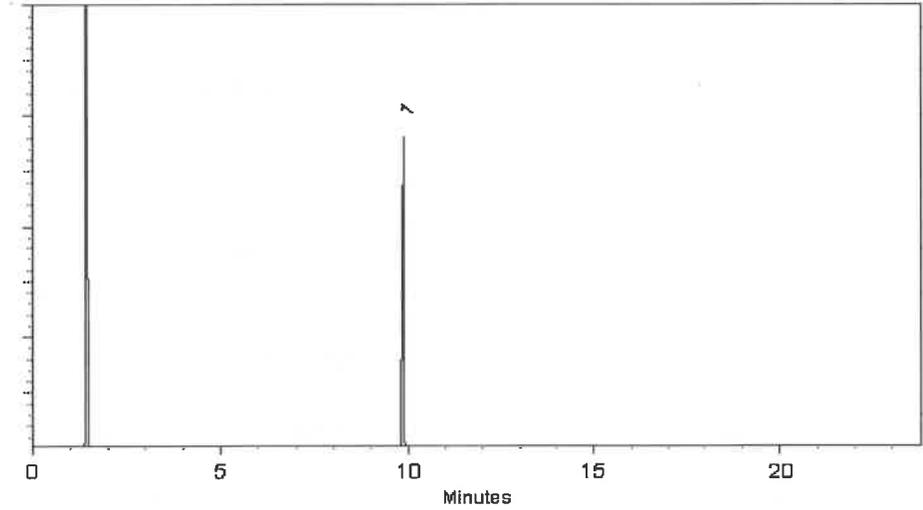

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ven Kelley*

**Ven Kelley - Operations Tech I**

**Date Mixed:** 17-Sep-2024

**Balance Serial #** 1128353505

*Dillon Murphy*

**Dillon Murphy - Operations Technician I**

**Date Passed:** 23-Sep-2024

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31097 Lot No.: A0216631  
 Description : o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
 Container Size : 2 mL Pkg Amt: > 1 mL  
 Expiration Date : April 30, 2028 Storage: 10°C or colder  
 Handling: Sonicate prior to use. Ship: Ambient

P13645 } Y.P.  
 ↓  
 P13694 } 10/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,065.0 µg/mL	+/- 453.3336

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride  
 CAS # 75-09-2  
 Purity 99%



# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rbx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

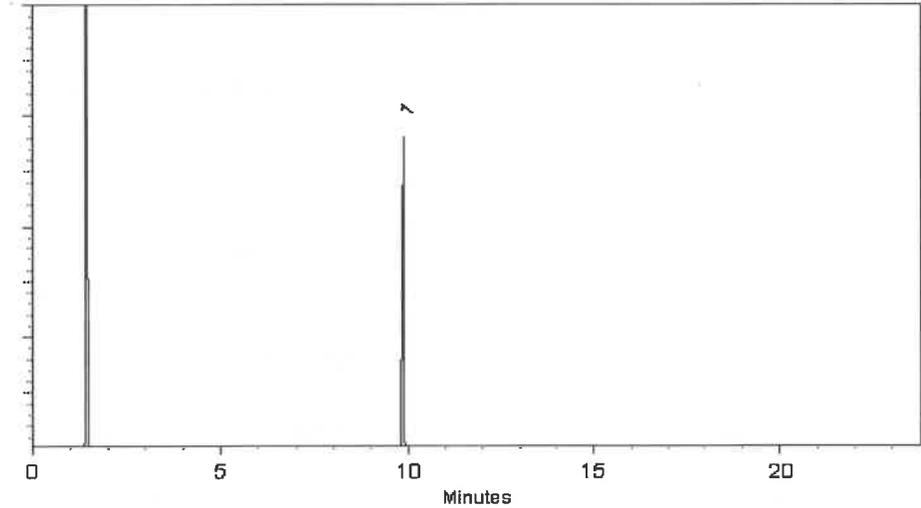

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ven Kelley*

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

*Dillon Murphy*

Dillon Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31097 Lot No.: A0216631  
 Description : o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
 Container Size : 2 mL Pkg Amt: > 1 mL  
 Expiration Date : April 30, 2028 Storage: 10°C or colder  
 Handling: Sonicate prior to use. Ship: Ambient

P13645 } Y.P.  
 ↓  
 P13694 } 10/16/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	GKSSA	99%	10,065.0 µg/mL	+/- 453.3336

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride  
 CAS # 75-09-2  
 Purity 99%



# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rbx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

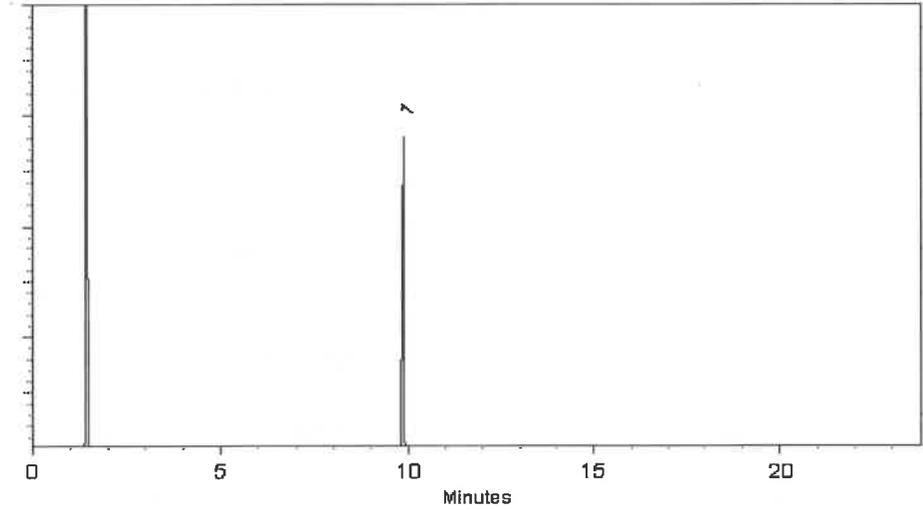

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ven Kelley*

Ven Kelley - Operations Tech I

Date Mixed: 17-Sep-2024

Balance Serial # 1128353505

*Dillon Murphy*

Dillon Murphy - Operations Technician I

Date Passed: 23-Sep-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



**FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.**

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543 **Lot No.:** A0211254  
**Description :** NJEPH Aromatics Matrix Spike Mix  
NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** April 30, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13408  
 ↓  
 P13716 } Y.P.  
 10/26/26

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.0 µg/mL	+/- 9.0114
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0316
4	Acenaphthylene	208-96-8	214935L31M	98%	200.3 µg/mL	+/- 9.0255
5	Acenaphthene	83-32-9	MKCR7169	99%	202.0 µg/mL	+/- 9.1015
6	Fluorene	86-73-7	10241100	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCS5188	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCR0570	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.8 µg/mL	+/- 9.0474
10	Pyrene	129-00-0	BCCK2592	99%	201.2 µg/mL	+/- 9.0655
11	Benz(a)anthracene	56-55-3	I30012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP231206RSR	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.0 µg/mL	+/- 9.0114
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.8 µg/mL	+/- 9.0033



17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240105ECS	99%	200.8 µg/mL	+/- 9.0474

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

### Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

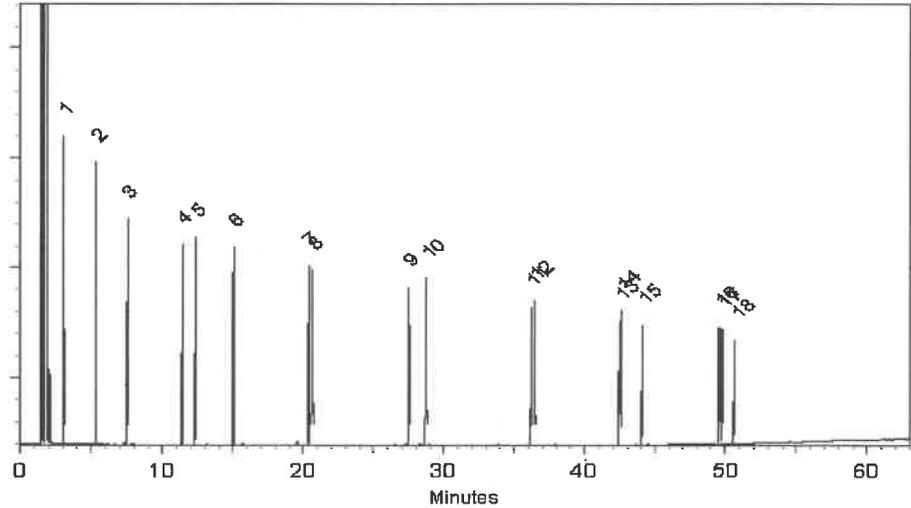

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Michael Maye*  
**Michael Maye - Operations Tech I**

**Date Mixed:** 09-May-2024    **Balance Serial #** 1128353505

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 13-May-2024

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**



## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



**FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.**

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543 **Lot No.:** A0211254  
**Description :** NJEPH Aromatics Matrix Spike Mix  
NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** April 30, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13408  
 ↓  
 P13716 } Y.P.  
 10/26/26

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.0 µg/mL	+/- 9.0114
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0316
4	Acenaphthylene	208-96-8	214935L31M	98%	200.3 µg/mL	+/- 9.0255
5	Acenaphthene	83-32-9	MKCR7169	99%	202.0 µg/mL	+/- 9.1015
6	Fluorene	86-73-7	10241100	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCS5188	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCR0570	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.8 µg/mL	+/- 9.0474
10	Pyrene	129-00-0	BCCK2592	99%	201.2 µg/mL	+/- 9.0655
11	Benz(a)anthracene	56-55-3	I30012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP231206RSR	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.0 µg/mL	+/- 9.0114
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.8 µg/mL	+/- 9.0033



17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240105ECS	99%	200.8 µg/mL	+/- 9.0474

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

### Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

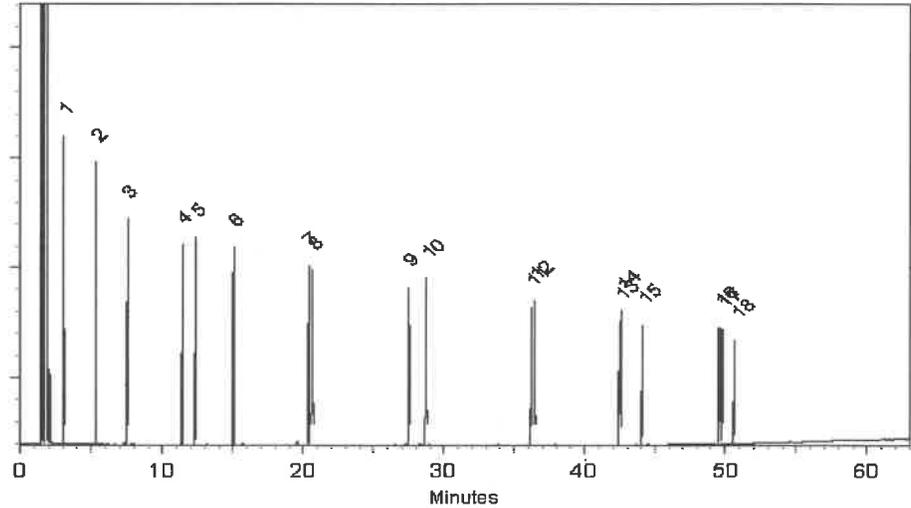

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Michael Maye*  
**Michael Maye - Operations Tech I**

**Date Mixed:** 09-May-2024 **Balance Serial #** 1128353505

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 13-May-2024

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



**FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.**

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543 **Lot No.:** A0211254  
**Description :** NJEPH Aromatics Matrix Spike Mix  
NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** April 30, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13408  
 ↓  
 P13716 } Y.P.  
 10/26/26

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.0 µg/mL	+/- 9.0114
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0316
4	Acenaphthylene	208-96-8	214935L31M	98%	200.3 µg/mL	+/- 9.0255
5	Acenaphthene	83-32-9	MKCR7169	99%	202.0 µg/mL	+/- 9.1015
6	Fluorene	86-73-7	10241100	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCS5188	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCR0570	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.8 µg/mL	+/- 9.0474
10	Pyrene	129-00-0	BCCK2592	99%	201.2 µg/mL	+/- 9.0655
11	Benz(a)anthracene	56-55-3	I30012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP231206RSR	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.0 µg/mL	+/- 9.0114
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.8 µg/mL	+/- 9.0033



17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240105ECS	99%	200.8 µg/mL	+/- 9.0474

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

### Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

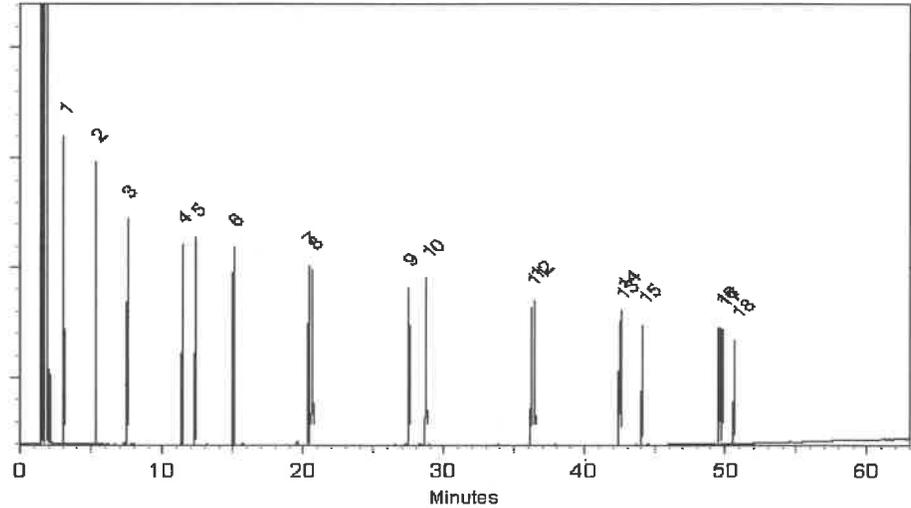

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Michael Maye*  
**Michael Maye - Operations Tech I**

**Date Mixed:** 09-May-2024 **Balance Serial #** 1128353505

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 13-May-2024

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**



## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



**FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.**

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543 **Lot No.:** A0211254  
**Description :** NJEPH Aromatics Matrix Spike Mix  
NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** April 30, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13408  
 ↓  
 P13716 } Y.P.  
 10/26/26

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.0 µg/mL	+/- 9.0114
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0316
4	Acenaphthylene	208-96-8	214935L31M	98%	200.3 µg/mL	+/- 9.0255
5	Acenaphthene	83-32-9	MKCR7169	99%	202.0 µg/mL	+/- 9.1015
6	Fluorene	86-73-7	10241100	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCS5188	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCR0570	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.8 µg/mL	+/- 9.0474
10	Pyrene	129-00-0	BCCK2592	99%	201.2 µg/mL	+/- 9.0655
11	Benz(a)anthracene	56-55-3	I30012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP231206RSR	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.0 µg/mL	+/- 9.0114
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.8 µg/mL	+/- 9.0033



17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240105ECS	99%	200.8 µg/mL	+/- 9.0474

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

### Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

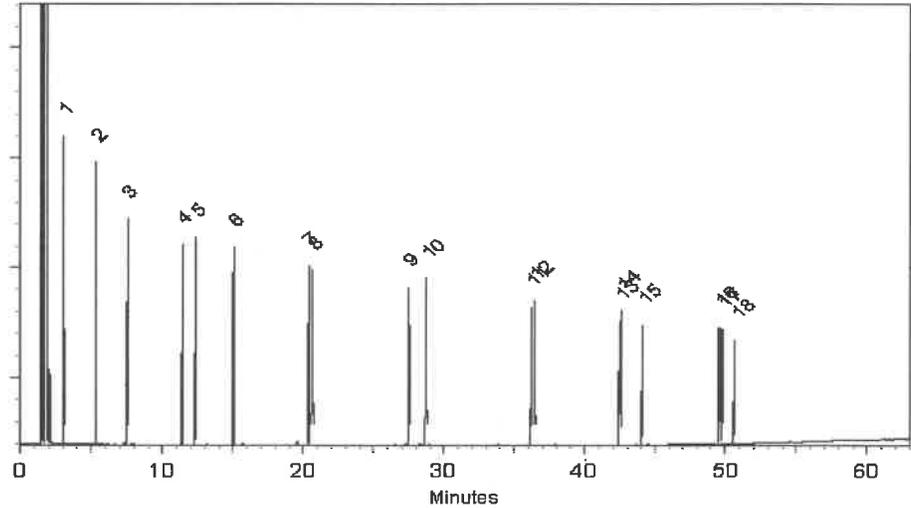

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Michael Maye*  
**Michael Maye - Operations Tech I**

**Date Mixed:** 09-May-2024    **Balance Serial #** 1128353505

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 13-May-2024

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
 chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543 **Lot No.:** A0211254  
**Description :** NJEPH Aromatics Matrix Spike Mix  
 NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** April 30, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13408  
 ↓  
 P13716 } Y.P.  
 10/26/26

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.0 µg/mL	+/- 9.0114
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0316
4	Acenaphthylene	208-96-8	214935L31M	98%	200.3 µg/mL	+/- 9.0255
5	Acenaphthene	83-32-9	MKCR7169	99%	202.0 µg/mL	+/- 9.1015
6	Fluorene	86-73-7	10241100	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCS5188	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCR0570	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.8 µg/mL	+/- 9.0474
10	Pyrene	129-00-0	BCCK2592	99%	201.2 µg/mL	+/- 9.0655
11	Benz(a)anthracene	56-55-3	I30012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP231206RSR	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.0 µg/mL	+/- 9.0114
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.8 µg/mL	+/- 9.0033



17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240105ECS	99%	200.8 µg/mL	+/- 9.0474

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

### Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

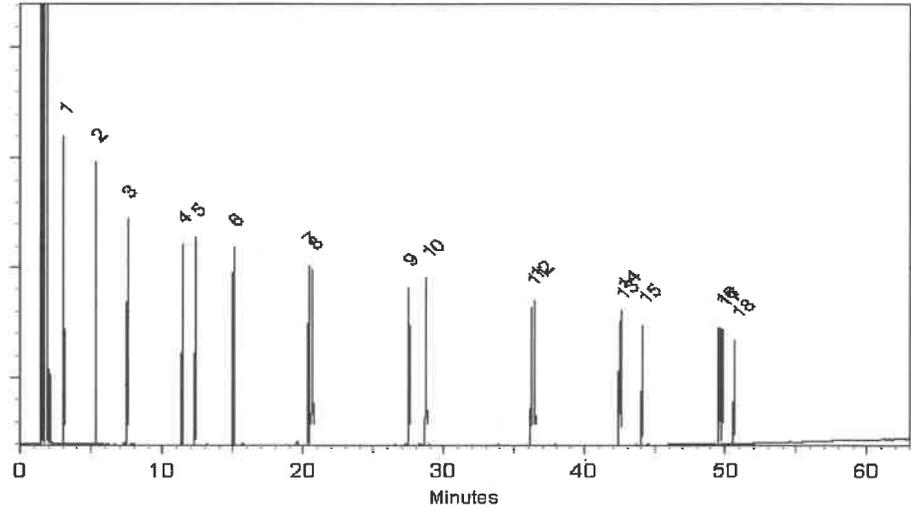

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Michael Maye*  
**Michael Maye - Operations Tech I**

**Date Mixed:** 09-May-2024    **Balance Serial #** 1128353505

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 13-May-2024

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**



## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



**FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.**

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30543 **Lot No.:** A0211254  
**Description :** NJEPH Aromatics Matrix Spike Mix  
NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** April 30, 2030 **Storage:** 10°C or colder  
**Handling:** Sonication required. Mix is photosensitive. **Ship:** Ambient

P13408  
 ↓  
 P13716 } Y.P.  
 10/26/26

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-38	99%	200.0 µg/mL	+/- 9.0114
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.4 µg/mL	+/- 9.0316
4	Acenaphthylene	208-96-8	214935L31M	98%	200.3 µg/mL	+/- 9.0255
5	Acenaphthene	83-32-9	MKCR7169	99%	202.0 µg/mL	+/- 9.1015
6	Fluorene	86-73-7	10241100	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCS5188	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCR0570	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.8 µg/mL	+/- 9.0474
10	Pyrene	129-00-0	BCCK2592	99%	201.2 µg/mL	+/- 9.0655
11	Benz(a)anthracene	56-55-3	I30012022BAA	99%	200.8 µg/mL	+/- 9.0474
12	Chrysene	218-01-9	RP231206RSR	99%	200.4 µg/mL	+/- 9.0294
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.4 µg/mL	+/- 9.0294
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.0 µg/mL	+/- 9.0114
15	Benzo(a)pyrene	50-32-8	O45GL	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	199.8 µg/mL	+/- 9.0033



17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	200.0 µg/mL	+/- 9.0114
18	Benzo(g,h,i)perylene	191-24-2	RP240105ECS	99%	200.8 µg/mL	+/- 9.0474

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

### Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

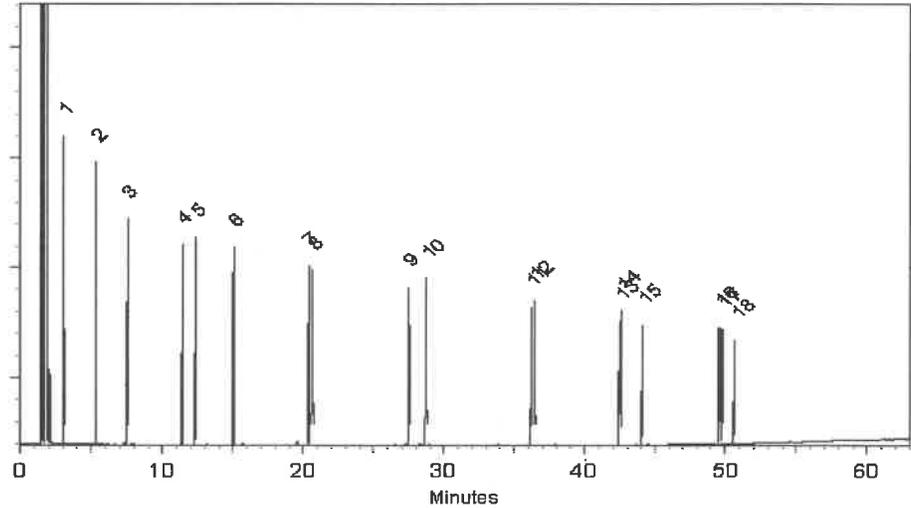

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Michael Maye*  
**Michael Maye - Operations Tech I**

**Date Mixed:** 09-May-2024    **Balance Serial #** 1128353505

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 13-May-2024

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**



## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30542 Lot No.: A0217408  
 Description : NJEPH Aliphatics Matrix Spike Mix  
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul  
 Container Size : 5 mL Pkg Amt: > 5 mL  
 Expiration Date : November 30, 2031 Storage: 10°C or colder  
 Handling: Sonicate prior to use. Ship: Ambient

P13800  
 ↓  
 P13829 } YIP  
 12/09/20

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477



\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
 30m x 0.25mm x 0.25µm  
 Rtx-5 (cat.#10223)

**Carrier Gas:**  
 hydrogen-constant pressure 10 psi.

**Temp. Program:**  
 40°C (hold 2 min.) to 330°C  
 @ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
 250°C

**Det. Temp:**  
 330°C

**Det. Type:**  
 FID

**Split Vent:**  
 2 ml/min.

**Inj. Vol**  
 1µl

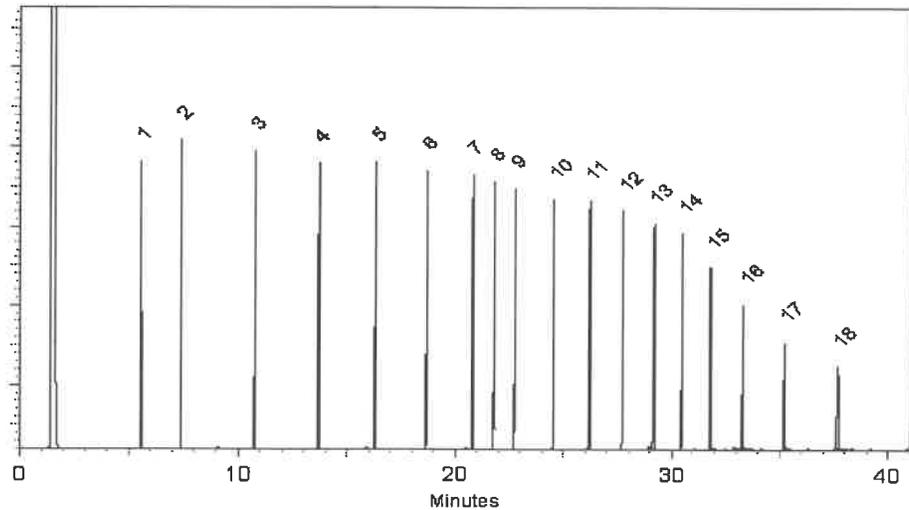

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope S. Riglin*

Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024

**Balance Serial #** 1128353505

*Jennifer S. Pollino*

Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
 Registered Quality System  
 Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30542 **Lot No.:** A0217408  
**Description :** NJEPH Aliphatics Matrix Spike Mix  
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul  
**Container Size :** 5 mL **Pkg Amt:** > 5 mL  
**Expiration Date :** November 30, 2031 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

P13800  
 ↓  
 P13829 } YIP  
 12/09/20

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477



\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
 30m x 0.25mm x 0.25µm  
 Rtx-5 (cat.#10223)

**Carrier Gas:**  
 hydrogen-constant pressure 10 psi.

**Temp. Program:**  
 40°C (hold 2 min.) to 330°C  
 @ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
 250°C

**Det. Temp:**  
 330°C

**Det. Type:**  
 FID

**Split Vent:**  
 2 ml/min.

**Inj. Vol**  
 1µl

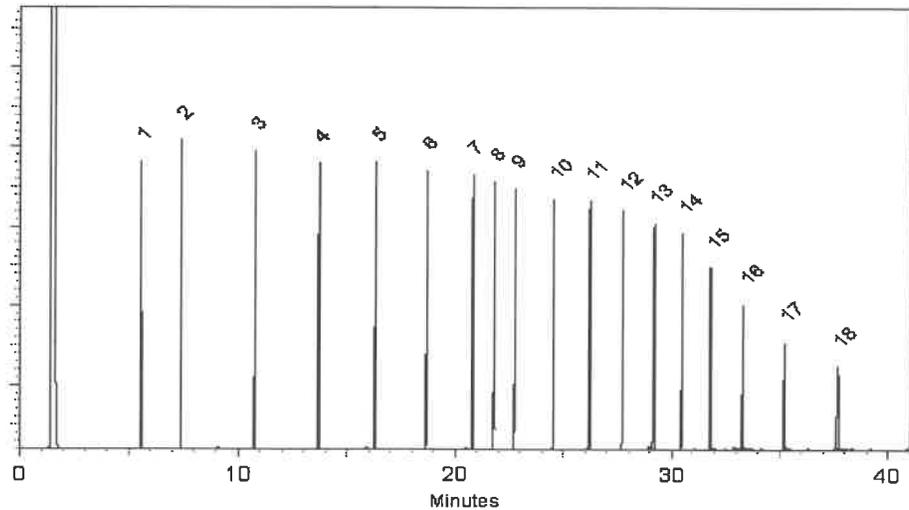

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope S. Riglin*

Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024

**Balance Serial #** 1128353505

*Jennifer Pollino*

Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
 Registered Quality System  
 Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30542 Lot No.: A0217408  
 Description : NJEPH Aliphatics Matrix Spike Mix  
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul  
 Container Size : 5 mL Pkg Amt: > 5 mL  
 Expiration Date : November 30, 2031 Storage: 10°C or colder  
 Handling: Sonicate prior to use. Ship: Ambient

P13800  
 ↓  
 P13829 } YIP  
 12/09/20

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477



\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
 30m x 0.25mm x 0.25µm  
 Rtx-5 (cat.#10223)

**Carrier Gas:**  
 hydrogen-constant pressure 10 psi.

**Temp. Program:**  
 40°C (hold 2 min.) to 330°C  
 @ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
 250°C

**Det. Temp:**  
 330°C

**Det. Type:**  
 FID

**Split Vent:**  
 2 ml/min.

**Inj. Vol**  
 1µl

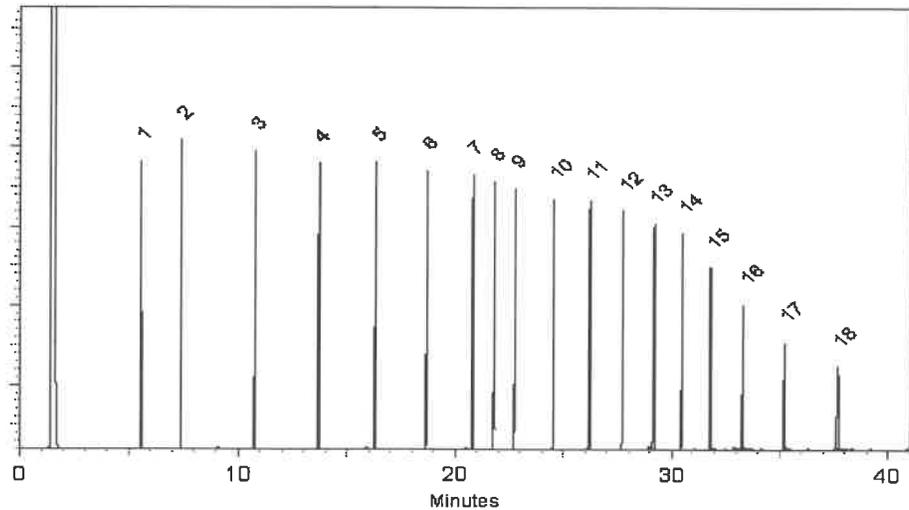

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope S. Riglin*

Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024

**Balance Serial #** 1128353505

*Jennifer Pollino*

Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
 Registered Quality System  
 Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30542 Lot No.: A0217408  
 Description : NJEPH Aliphatics Matrix Spike Mix  
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul  
 Container Size : 5 mL Pkg Amt: > 5 mL  
 Expiration Date : November 30, 2031 Storage: 10°C or colder  
 Handling: Sonicate prior to use. Ship: Ambient

P13896  
 ↓  
 P13906 } Y.P.  
 03/06/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
 Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
 @ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

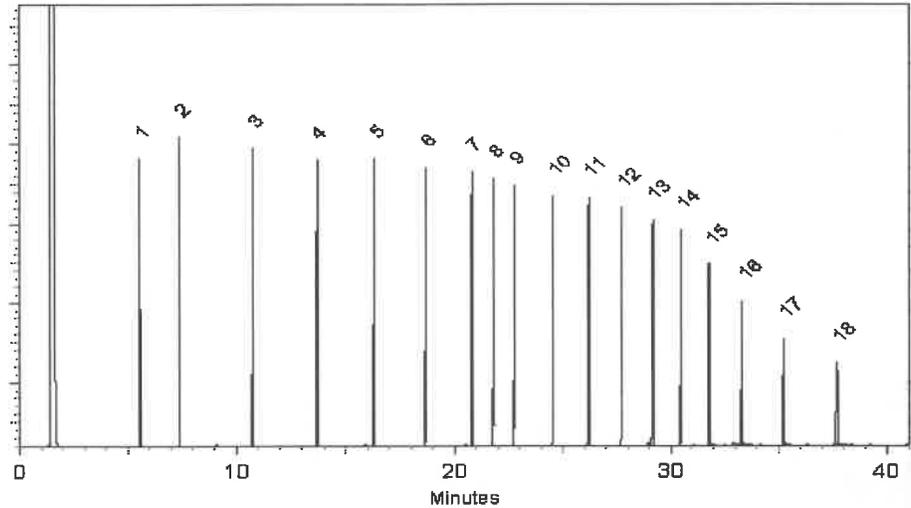

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope S. Riglin*

Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024

**Balance Serial #** 1128353505

*Jennifer Pollino*

Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
 Registered Quality System  
 Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30542 Lot No.: A0217408  
 Description : NJEPH Aliphatics Matrix Spike Mix  
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul  
 Container Size : 5 mL Pkg Amt: > 5 mL  
 Expiration Date : November 30, 2031 Storage: 10°C or colder  
 Handling: Sonicate prior to use. Ship: Ambient

P13896  
 ↓  
 P13906 } Y.P.  
 03/06/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	200.7 µg/mL	+/- 5.1839
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.0 µg/mL	+/- 5.1917
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	200.5 µg/mL	+/- 5.1805
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.5 µg/mL	+/- 5.1805
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.7 µg/mL	+/- 5.1857
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1857
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.9 µg/mL	+/- 5.1888
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.5 µg/mL	+/- 5.1805
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.5 µg/mL	+/- 5.1788
10	n-Tetracosane (C24)	646-31-1	MKCS9978	99%	200.6 µg/mL	+/- 5.1822
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	200.5 µg/mL	+/- 5.1796
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.6 µg/mL	+/- 5.1822
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.1 µg/mL	+/- 5.1942
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	200.9 µg/mL	+/- 5.1891
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	200.8 µg/mL	+/- 5.1865
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	200.6 µg/mL	+/- 5.1814
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	199.3 µg/mL	+/- 5.1477

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
 Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
 @ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

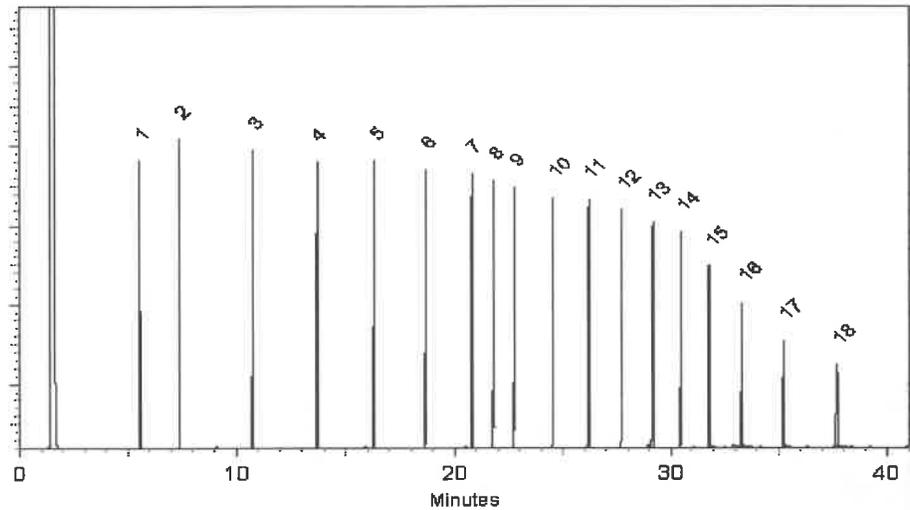

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope S. Riglin*

Penelope Riglin - Operations Tech I

**Date Mixed:** 03-Oct-2024

**Balance Serial #** 1128353505

*Jennifer Pollino*

Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 07-Oct-2024

Manufactured under Restek's ISO 9001:2015  
 Registered Quality System  
 Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30542 Lot No.: A0220449  
 Description : NJEPH Aliphatics Matrix Spike Mix  
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul  
 Container Size : 5 mL Pkg Amt: > 5 mL  
 Expiration Date : January 31, 2032 Storage: 10°C or colder  
 Handling: Sonicate prior to use. Ship: Ambient

P13909  
 ↓  
 P1395 } Y.P.  
 03106/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	201.3 µg/mL	+/- 5.2012
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.7 µg/mL	+/- 5.2098
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	201.3 µg/mL	+/- 5.2012
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.3 µg/mL	+/- 5.1753
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1839
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.1 µg/mL	+/- 5.1704
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.7 µg/mL	+/- 5.1839
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.3 µg/mL	+/- 5.1753
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	201.3 µg/mL	+/- 5.2012
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	201.0 µg/mL	+/- 5.1926
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.3 µg/mL	+/- 5.1753
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.2 µg/mL	+/- 5.1984
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	201.7 µg/mL	+/- 5.2098
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	201.3 µg/mL	+/- 5.2012
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	201.7 µg/mL	+/- 5.2098
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	201.6 µg/mL	+/- 5.2081

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
 Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
 @ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

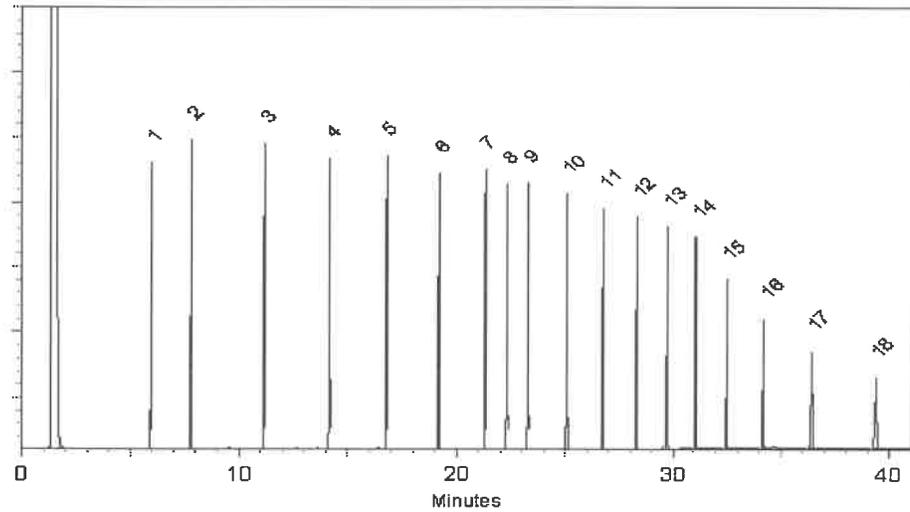

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Brandon Reish*  
 Brandon Reish - Operations Technician III

**Date Mixed:** 23-Dec-2024

**Balance Serial #** C322230531

*Dillian Murphy*  
 Dillian Murphy - Operations Technician I

**Date Passed:** 27-Dec-2024

Manufactured under Restek's ISO 9001:2015  
 Registered Quality System  
 Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30543 Lot No.: A0220580  
 Description : NJEPH Aromatics Matrix Spike Mix  
NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul  
 Container Size : 5 mL Pkg Amt: > 5 mL  
 Expiration Date : November 30, 2030 Storage: 10°C or colder  
 Handling: Sonication required. Mix is photosensitive. Ship: Ambient

P13916 } Y.P.  
 ↓  
 P13935 } 08/06/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	201.9 µg/mL	+/- 9.0961
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	RP241029RSR	98%	201.9 µg/mL	+/- 9.0961
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.9 µg/mL	+/- 9.0961
7	Phenanthrene	85-01-8	MKCT3391	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	MKCW9141	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCL8032	99%	201.6 µg/mL	+/- 9.0835
11	Benz(a)anthracene	56-55-3	I220012022BAA	99%	202.0 µg/mL	+/- 9.1015
12	Chrysene	218-01-9	RP240719RSR	99%	202.0 µg/mL	+/- 9.1015
13	Benzo(b)fluoranthene	205-99-2	SBS-BBF-FINAL-2	99%	202.0 µg/mL	+/- 9.1015
14	Benzo(k)fluoranthene	207-08-9	012022K	98%	201.5 µg/mL	+/- 9.0784
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383



17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	201.2 µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	200.3 µg/mL	+/- 9.0255

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

### Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

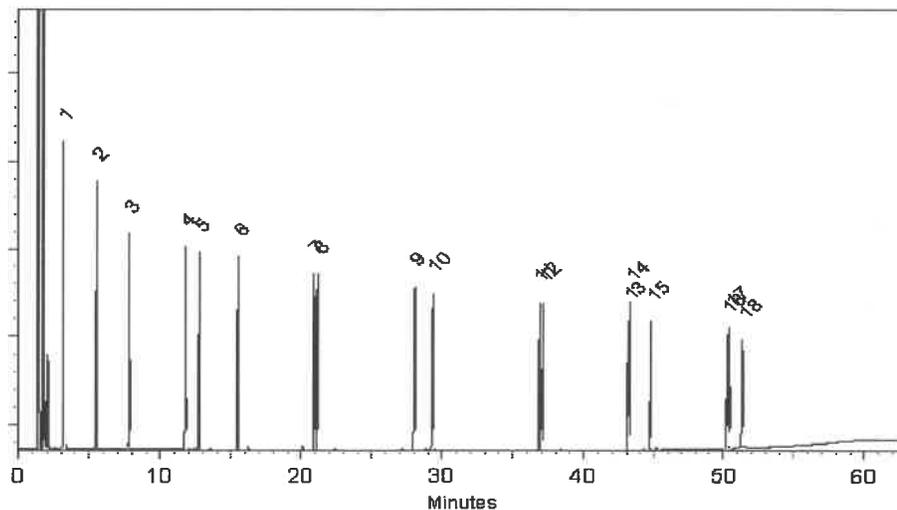

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024      **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30543 Lot No.: A0220580  
 Description : NJEPH Aromatics Matrix Spike Mix  
NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul  
 Container Size : 5 mL Pkg Amt: > 5 mL  
 Expiration Date : November 30, 2030 Storage: 10°C or colder  
 Handling: Sonication required. Mix is photosensitive. Ship: Ambient

P13916 } Y.P.  
 ↓  
 P13935 } 08106125

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	201.9 µg/mL	+/- 9.0961
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	RP241029RSR	98%	201.9 µg/mL	+/- 9.0961
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.9 µg/mL	+/- 9.0961
7	Phenanthrene	85-01-8	MKCT3391	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	MKCW9141	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCL8032	99%	201.6 µg/mL	+/- 9.0835
11	Benz(a)anthracene	56-55-3	I220012022BAA	99%	202.0 µg/mL	+/- 9.1015
12	Chrysene	218-01-9	RP240719RSR	99%	202.0 µg/mL	+/- 9.1015
13	Benzo(b)fluoranthene	205-99-2	SBS-BBF-FINAL-2	99%	202.0 µg/mL	+/- 9.1015
14	Benzo(k)fluoranthene	207-08-9	012022K	98%	201.5 µg/mL	+/- 9.0784
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383



17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	201.2 µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	200.3 µg/mL	+/- 9.0255

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

### Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

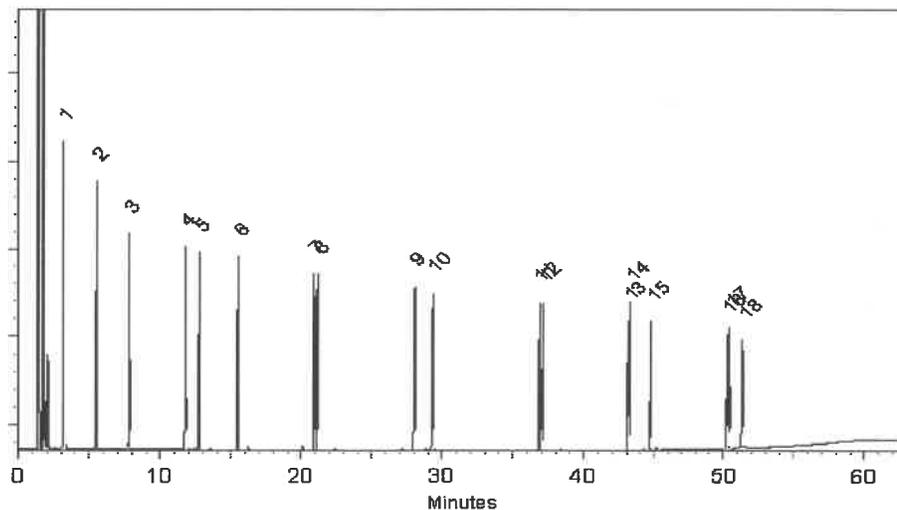

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*VenKelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024      **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30542 Lot No.: A0220449  
 Description : NJEPH Aliphatics Matrix Spike Mix  
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul  
 Container Size : 5 mL Pkg Amt: > 5 mL  
 Expiration Date : January 31, 2032 Storage: 10°C or colder  
 Handling: Sonicate prior to use. Ship: Ambient

P13978 } RC/  
 ↓  
 P13987 } 04/24/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	201.3 µg/mL	+/- 5.2012
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.7 µg/mL	+/- 5.2098
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	201.3 µg/mL	+/- 5.2012
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.3 µg/mL	+/- 5.1753
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1839
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.1 µg/mL	+/- 5.1704
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.7 µg/mL	+/- 5.1839
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.3 µg/mL	+/- 5.1753
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	201.3 µg/mL	+/- 5.2012
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	201.0 µg/mL	+/- 5.1926
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.3 µg/mL	+/- 5.1753
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.2 µg/mL	+/- 5.1984
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	201.7 µg/mL	+/- 5.2098
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	201.3 µg/mL	+/- 5.2012
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	201.7 µg/mL	+/- 5.2098
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	201.6 µg/mL	+/- 5.2081



\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

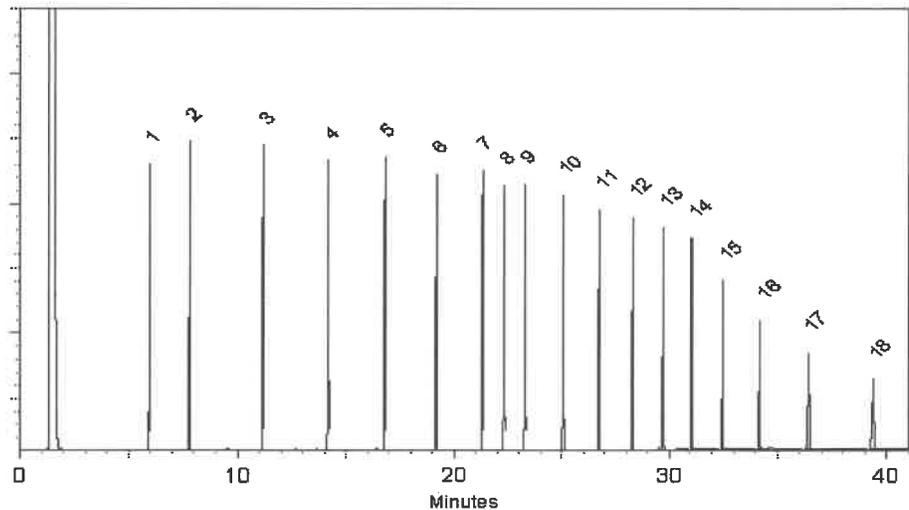

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brandon Reish - Operations Technician III

**Date Mixed:** 23-Dec-2024 **Balance Serial #** C322230531

Dillan Murphy - Operations Technician I

**Date Passed:** 27-Dec-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30542 Lot No.: A0220449  
 Description : NJEPH Aliphatics Matrix Spike Mix  
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul  
 Container Size : 5 mL Pkg Amt: > 5 mL  
 Expiration Date : January 31, 2032 Storage: 10°C or colder  
 Handling: Sonicate prior to use. Ship: Ambient

P13978 } RC/  
 ↓  
 P13987 } 04/24/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	201.3 µg/mL	+/- 5.2012
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.7 µg/mL	+/- 5.2098
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	201.3 µg/mL	+/- 5.2012
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.3 µg/mL	+/- 5.1753
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1839
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.1 µg/mL	+/- 5.1704
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.7 µg/mL	+/- 5.1839
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.3 µg/mL	+/- 5.1753
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	201.3 µg/mL	+/- 5.2012
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	201.0 µg/mL	+/- 5.1926
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.3 µg/mL	+/- 5.1753
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.2 µg/mL	+/- 5.1984
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	201.7 µg/mL	+/- 5.2098
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	201.3 µg/mL	+/- 5.2012
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	201.7 µg/mL	+/- 5.2098
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	201.6 µg/mL	+/- 5.2081



\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

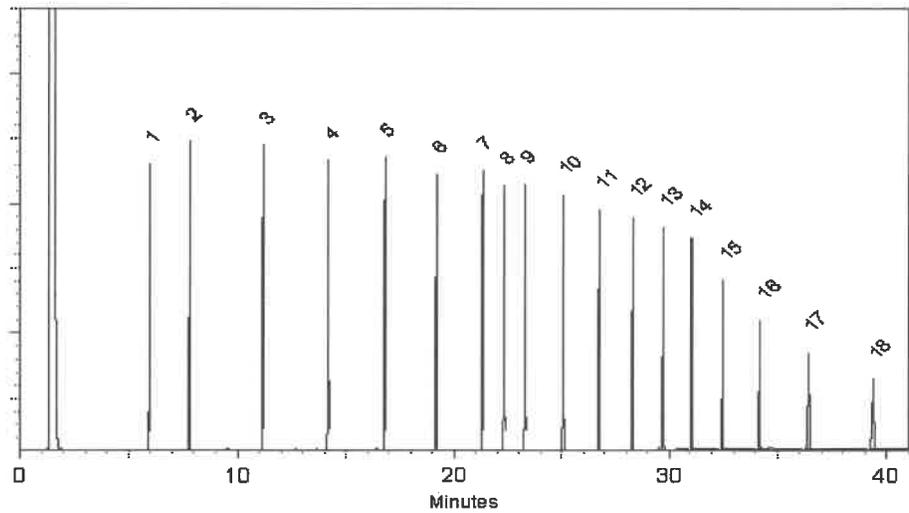

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brandon Reish - Operations Technician III

**Date Mixed:** 23-Dec-2024 **Balance Serial #** C322230531

Dillan Murphy - Operations Technician I

**Date Passed:** 27-Dec-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30542 Lot No.: A0220449  
 Description : NJEPH Aliphatics Matrix Spike Mix  
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul  
 Container Size : 5 mL Pkg Amt: > 5 mL  
 Expiration Date : January 31, 2032 Storage: 10°C or colder  
 Handling: Sonicate prior to use. Ship: Ambient

P13978 } RC/  
 ↓  
 P13987 } 04/24/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	201.3 µg/mL	+/- 5.2012
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.7 µg/mL	+/- 5.2098
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	201.3 µg/mL	+/- 5.2012
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.3 µg/mL	+/- 5.1753
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1839
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.1 µg/mL	+/- 5.1704
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.7 µg/mL	+/- 5.1839
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.3 µg/mL	+/- 5.1753
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	201.3 µg/mL	+/- 5.2012
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	201.0 µg/mL	+/- 5.1926
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.3 µg/mL	+/- 5.1753
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.2 µg/mL	+/- 5.1984
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	201.7 µg/mL	+/- 5.2098
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	201.3 µg/mL	+/- 5.2012
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	201.7 µg/mL	+/- 5.2098
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	201.6 µg/mL	+/- 5.2081



\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: n-Pentane  
CAS # 109-66-0  
Purity 99%

### Quality Confirmation Test

Column:  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)  
Carrier Gas:  
hydrogen-constant pressure 10 psi.

Temp. Program:  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


Inj. Temp:  
250°C

Det. Temp:  
330°C

Det. Type:  
FID

Split Vent:  
2 ml/min.

Inj. Vol  
1µl

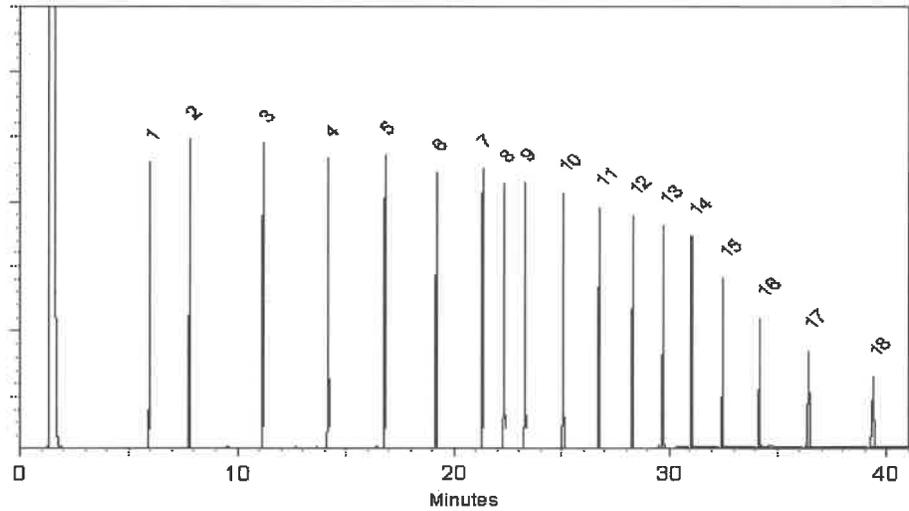

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Brandon Reish*  
Brandon Reish - Operations Technician III

Date Mixed: 23-Dec-2024 Balance Serial # C322230531

*Dylan Murphy*  
Dylan Murphy - Operations Technician I

Date Passed: 27-Dec-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30542 Lot No.: A0220449  
 Description : NJEPH Aliphatics Matrix Spike Mix  
NJEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul  
 Container Size : 5 mL Pkg Amt: > 5 mL  
 Expiration Date : January 31, 2032 Storage: 10°C or colder  
 Handling: Sonicate prior to use. Ship: Ambient

P13978 } RC/  
 ↓  
 P13987 } 04/24/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C9)	111-84-2	SHBP9752	99%	201.3 µg/mL	+/- 5.2012
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	201.7 µg/mL	+/- 5.2098
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	201.3 µg/mL	+/- 5.2012
4	n-Tetradecane (C14)	629-59-4	STBL0465	99%	200.7 µg/mL	+/- 5.1839
5	n-Hexadecane (C16)	544-76-3	SHBR0669	99%	200.3 µg/mL	+/- 5.1753
6	n-Octadecane (C18)	593-45-3	UE5NG	99%	200.7 µg/mL	+/- 5.1839
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	200.1 µg/mL	+/- 5.1704
8	n-Heneicosane (C21)	629-94-7	MKCP1960	99%	200.7 µg/mL	+/- 5.1839
9	n-Docosane (C22)	629-97-0	MKCQ3882	99%	200.3 µg/mL	+/- 5.1753
10	n-Tetracosane (C24)	646-31-1	UH5GN	99%	201.3 µg/mL	+/- 5.2012
11	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	201.0 µg/mL	+/- 5.1926
12	n-Octacosane (C28)	630-02-4	BCCJ4566	99%	200.3 µg/mL	+/- 5.1753
13	n-Triacontane (C30)	638-68-6	MKCV7007	98%	201.2 µg/mL	+/- 5.1984
14	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	201.7 µg/mL	+/- 5.2098
15	n-Tetratriacontane (C34)	14167-59-0	6JNHB	99%	201.3 µg/mL	+/- 5.2012
16	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	201.7 µg/mL	+/- 5.2098
17	n-Octatriacontane (C38)	7194-85-6	0000207852	96%	201.6 µg/mL	+/- 5.2081



\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

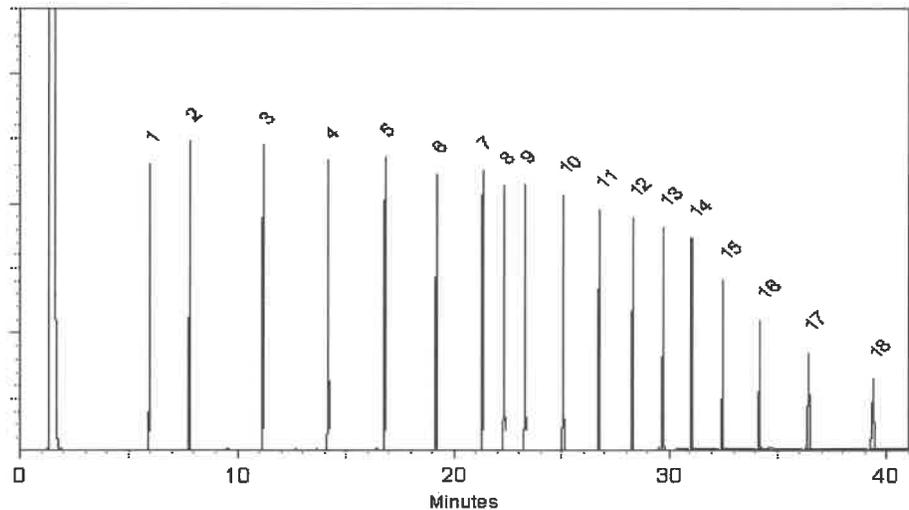

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brandon Reish - Operations Technician III

**Date Mixed:** 23-Dec-2024 **Balance Serial #** C322230531

Dillan Murphy - Operations Technician I

**Date Passed:** 27-Dec-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30543 Lot No.: A0220580  
 Description : NJEPH Aromatics Matrix Spike Mix  
NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul  
 Container Size : 5 mL Pkg Amt: > 5 mL  
 Expiration Date : November 30, 2030 Storage: 10°C or colder  
 Handling: Sonication required. Mix is photosensitive. Ship: Ambient

P13988 } RCL  
 ↓  
 P13993 } 4/25/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	201.9 µg/mL	+/- 9.0961
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	RP241029RSR	98%	201.9 µg/mL	+/- 9.0961
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.9 µg/mL	+/- 9.0961
7	Phenanthrene	85-01-8	MKCT3391	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	MKCW9141	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCL8032	99%	201.6 µg/mL	+/- 9.0835
11	Benz(a)anthracene	56-55-3	I220012022BAA	99%	202.0 µg/mL	+/- 9.1015
12	Chrysene	218-01-9	RP240719RSR	99%	202.0 µg/mL	+/- 9.1015
13	Benzo(b)fluoranthene	205-99-2	SBS-BBF-FINAL-2	99%	202.0 µg/mL	+/- 9.1015
14	Benzo(k)fluoranthene	207-08-9	012022K	98%	201.5 µg/mL	+/- 9.0784
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383


17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	201.2 µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	200.3 µg/mL	+/- 9.0255

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

### Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)  
**Carrier Gas:**  
hydrogen-constant pressure 10 psi.  
**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)  
**Inj. Temp:**  
250°C  
**Det. Temp:**  
330°C  
**Det. Type:**  
FID  
**Split Vent:**  
20 ml/min.  
**Inj. Vol**  
1µl

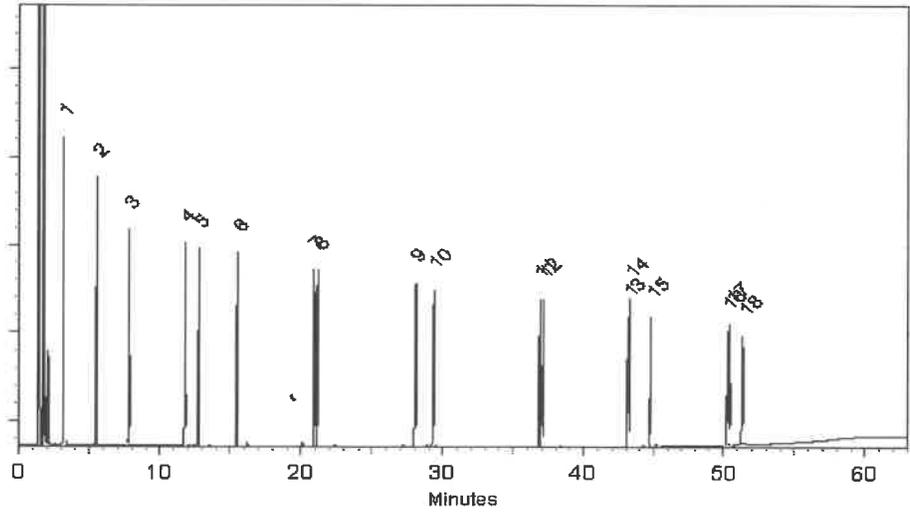

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ven Kelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024    **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**



110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: 1-814-353-1300  
 Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis  
*chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30543 Lot No.: A0220580  
 Description : NJEPH Aromatics Matrix Spike Mix  
NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul  
 Container Size : 5 mL Pkg Amt: > 5 mL  
 Expiration Date : November 30, 2030 Storage: 10°C or colder  
 Handling: Sonication required. Mix is photosensitive. Ship: Ambient

P13988 } RCL  
 ↓  
 P13993 } 4/25/25

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-39	98%	201.9 µg/mL	+/- 9.0961
2	Naphthalene	91-20-3	STBL1057	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBL3028	99%	200.4 µg/mL	+/- 9.0294
4	Acenaphthylene	208-96-8	RP241029RSR	98%	201.9 µg/mL	+/- 9.0961
5	Acenaphthene	83-32-9	MKCR7169	99%	200.4 µg/mL	+/- 9.0294
6	Fluorene	86-73-7	10246250	98%	201.9 µg/mL	+/- 9.0961
7	Phenanthrene	85-01-8	MKCT3391	99%	200.8 µg/mL	+/- 9.0474
8	Anthracene	120-12-7	MKCW9141	99%	200.4 µg/mL	+/- 9.0294
9	Fluoranthene	206-44-0	MKCQ4728	99%	200.4 µg/mL	+/- 9.0294
10	Pyrene	129-00-0	BCCL8032	99%	201.6 µg/mL	+/- 9.0835
11	Benz(a)anthracene	56-55-3	I220012022BAA	99%	202.0 µg/mL	+/- 9.1015
12	Chrysene	218-01-9	RP240719RSR	99%	202.0 µg/mL	+/- 9.1015
13	Benzo(b)fluoranthene	205-99-2	SBS-BBF-FINAL-2	99%	202.0 µg/mL	+/- 9.1015
14	Benzo(k)fluoranthene	207-08-9	012022K	98%	201.5 µg/mL	+/- 9.0784
15	Benzo(a)pyrene	50-32-8	NQLXA	98%	200.7 µg/mL	+/- 9.0431
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	200.6 µg/mL	+/- 9.0383

17	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	201.2 µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	200.3 µg/mL	+/- 9.0255

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

### Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
20 ml/min.

**Inj. Vol**  
1µl

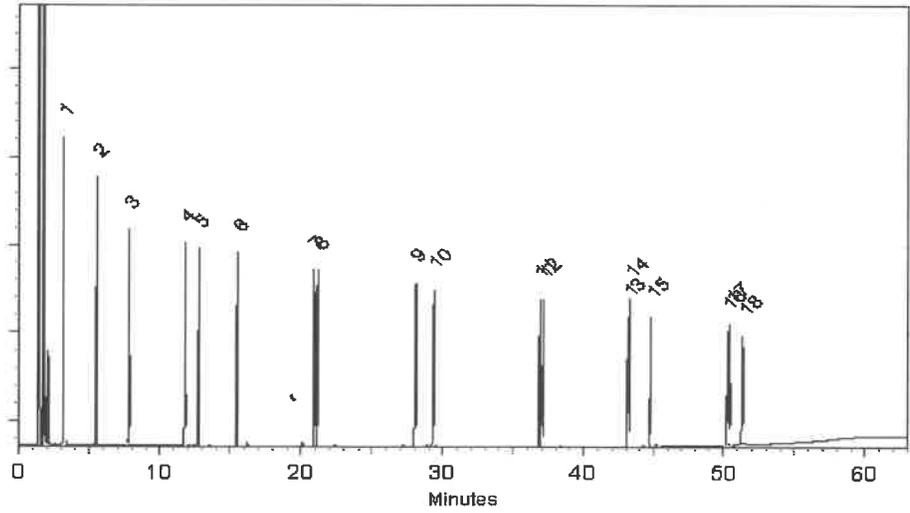

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ven Kelley*  
**Ven Kelley - Operations Tech I**

**Date Mixed:** 30-Dec-2024    **Balance Serial #** 1128360905

*Jennifer Pollino*  
**Jennifer Pollino - Operations Tech III - ARM QC**

**Date Passed:** 03-Jan-2025

**Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397**



n-Hexane 95%  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis

avantor™



Material No.: 9262-03  
Batch No.: 24G1962003  
Manufactured Date: 2024-05-23  
Expiration Date: 2025-08-22  
Revision No.: 0

W3147  
W3147  
CP4TE1. 02/03/2023  
JP

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H <sub>2</sub> SO <sub>4</sub>	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Croak  
Director Quality Operations, Bioscience Production