
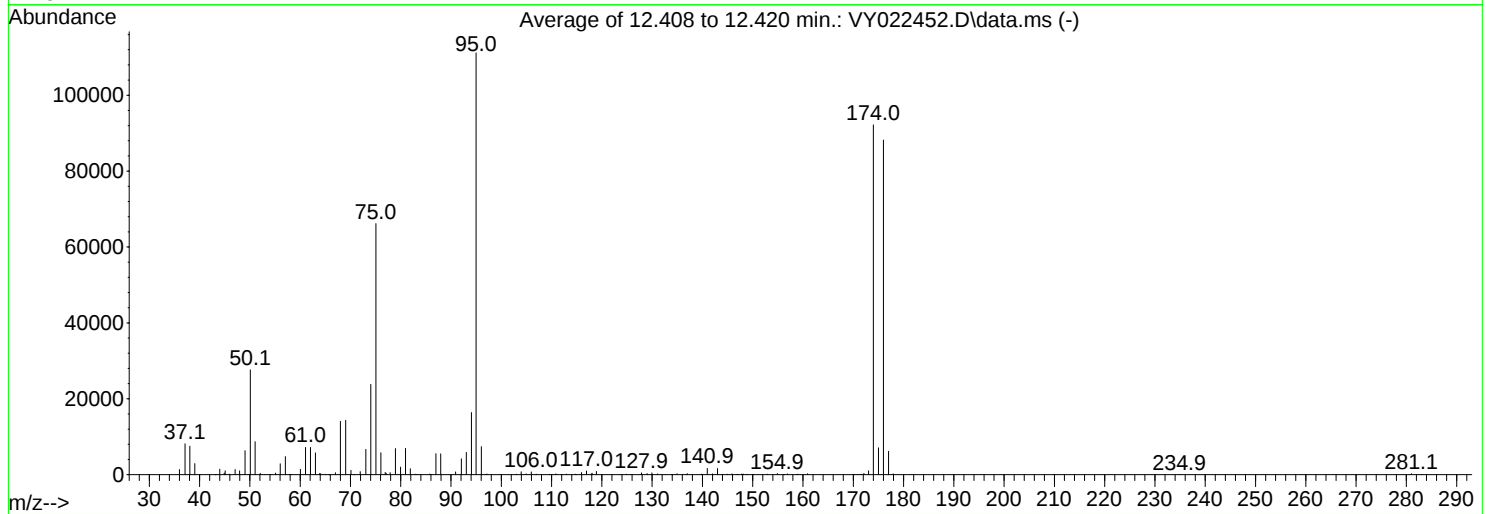


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052925\
Data File : VY022452.D
Acq On : 29 May 2025 07:54
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052725S.M
Title : SW846 8260
Last Update : Wed May 28 10:34:06 2025

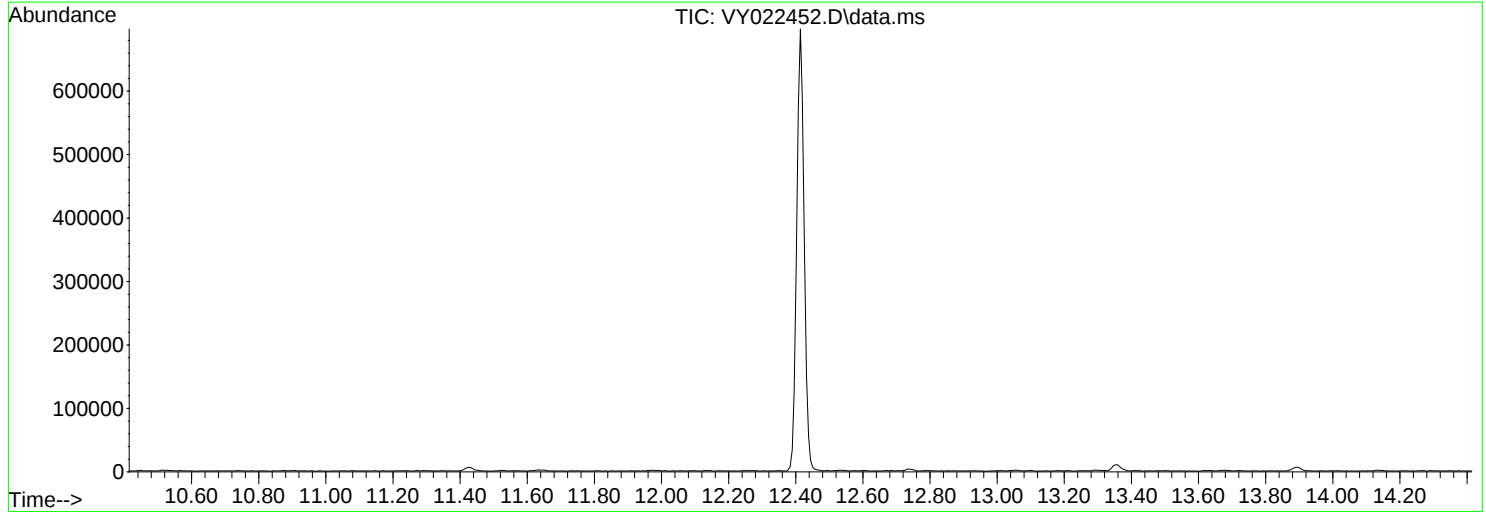

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.8	27616	PASS
75	95	30	60	59.5	66192	PASS
95	95	100	100	100.0	111184	PASS
96	95	5	9	6.6	7367	PASS
173	174	0.00	2	1.1	1032	PASS
174	95	50	100	82.9	92195	PASS
175	174	5	9	7.7	7073	PASS
176	174	95	101	95.6	88176	PASS
177	176	5	9	7.0	6175	PASS