

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060325\
Data File : FB031860.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2025 11:18
Operator : YP/AJ
Sample : Q2150-09
Misc : 7.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-54

Integration File: Calibration.e
Quant Time: Jun 04 01:20:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB053025.M
Quant Title :
QLast Update : Fri May 30 15:30:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	293932	24.088 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB060325\
Data File : FB031860.D
Signal(s) : FID2B.CH
Acq On : 3 Jun 2025 11:18
Operator : YP/AJ
Sample : Q2150-09
Misc : 7.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-54

Integration File: Calibration.e
Quant Time: Jun 04 01:20:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB053025.M
Quant Title :
QLast Update : Fri May 30 15:30:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

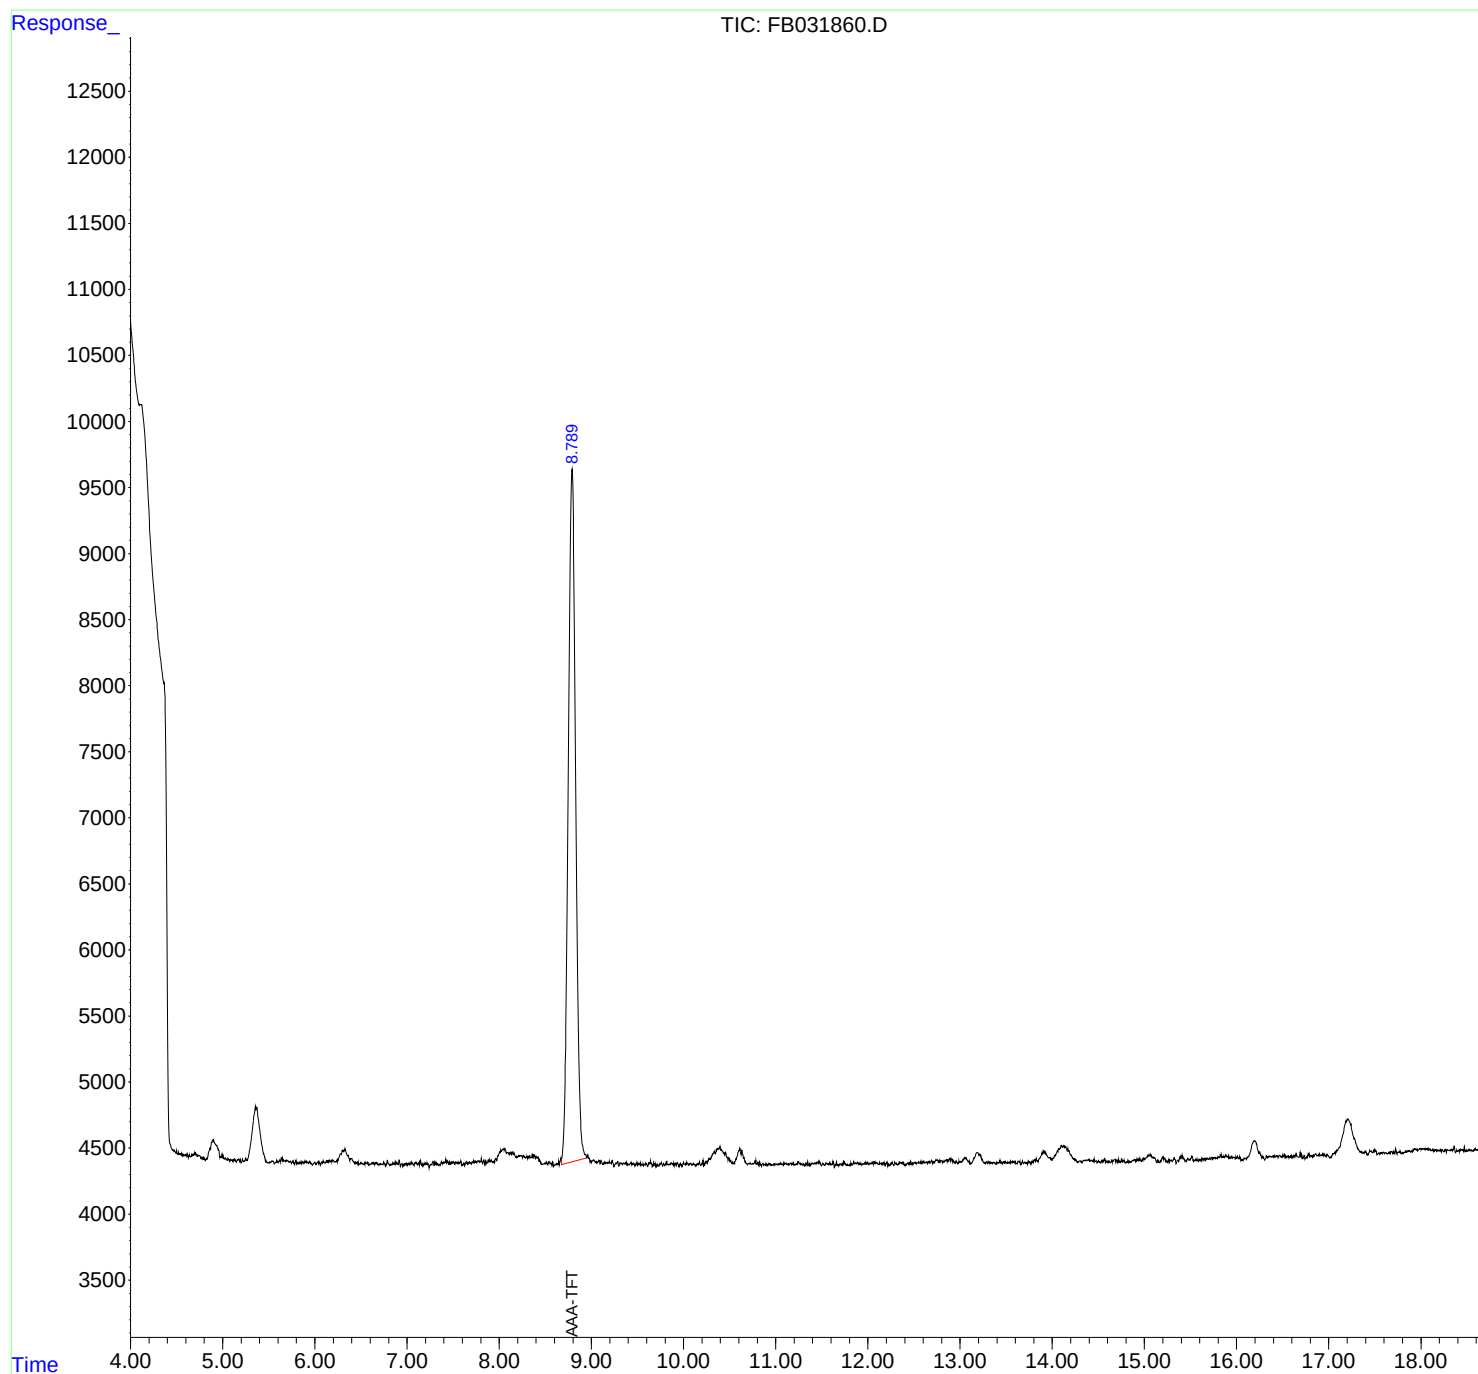

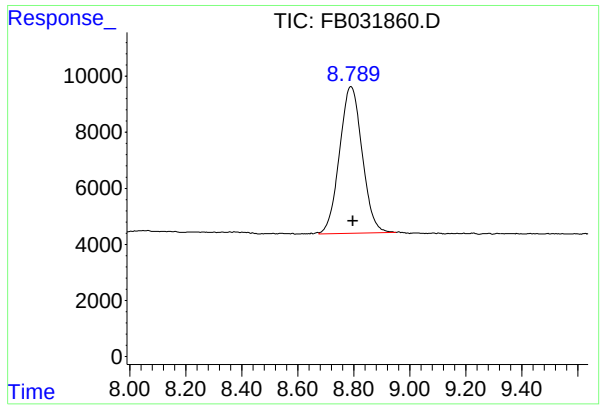

#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: -0.007 min
Response: 293932
Conc: 24.09 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-54