
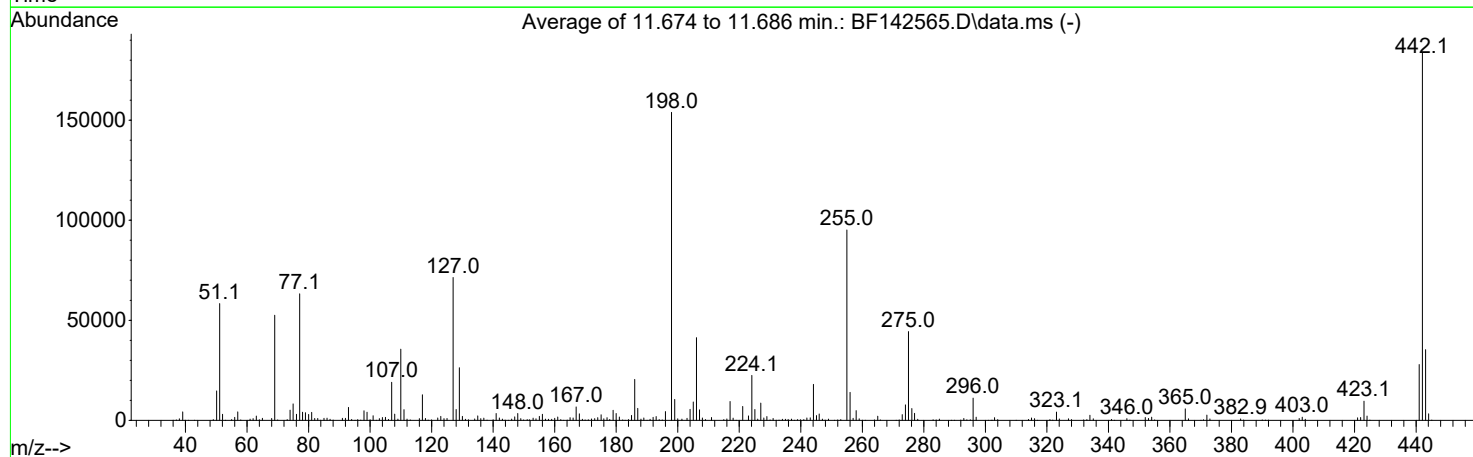


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053025\
Data File : BF142565.D
Acq On : 30 May 2025 12:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 20 16:26:47 2025

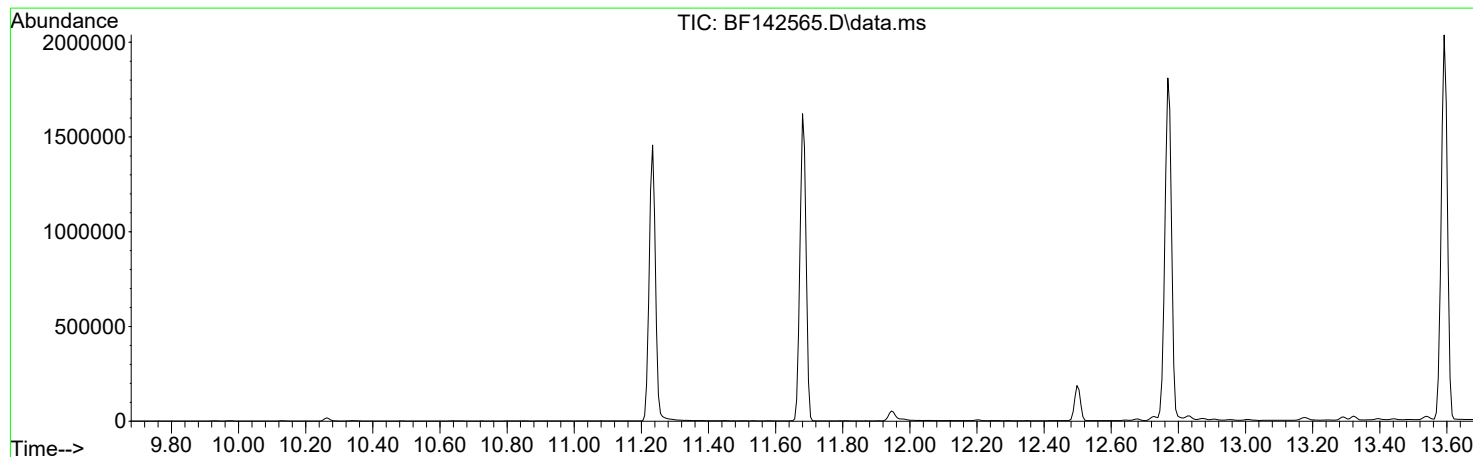

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	58331	PASS
68	69	0.00	2	1.8	964	PASS
69	198	0.00	100	34.2	52549	PASS
70	69	0.00	2	0.5	281	PASS
127	198	10	80	46.4	71373	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	153872	PASS
199	198	5	9	6.8	10478	PASS
275	198	10	60	28.8	44389	PASS
365	198	1	100	3.8	5787	PASS
441	198	0.01	100	18.2	27936	PASS
442	442	50	100	100.0	183816	PASS
443	442	15	24	19.2	35315	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/30/2025	BNA_F	<u>BF142565.D</u>
Compound Name	Response	Retention Time
DDT	529591	13.592
DDD	11584	13.321
DDE	806	12.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12390	541981	2.29

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF053025\
Data File : BF142565.D
Acq On : 30 May 2025 12:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 30 13:07:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

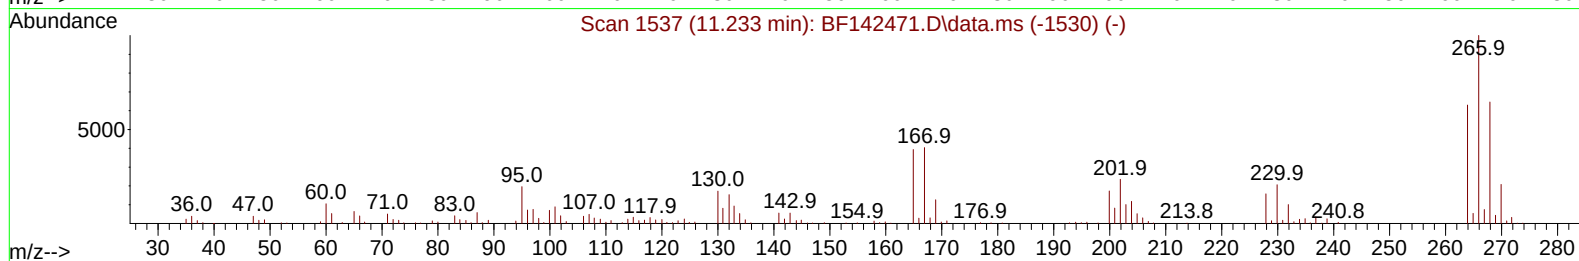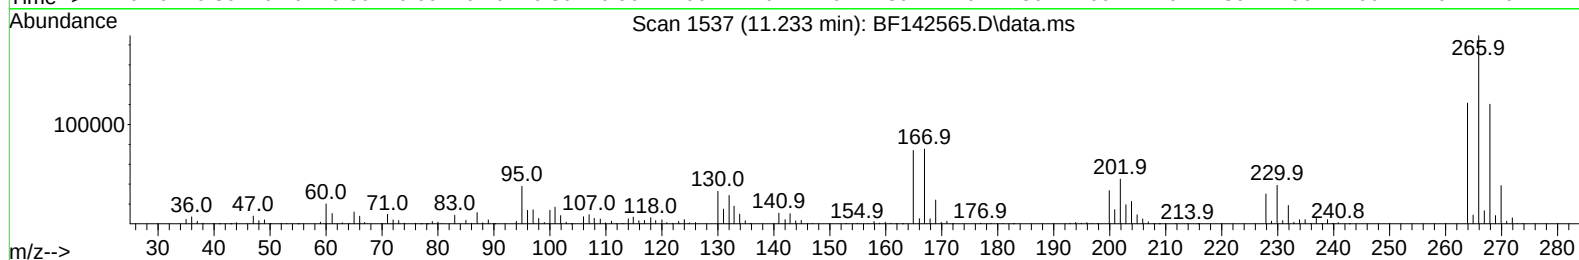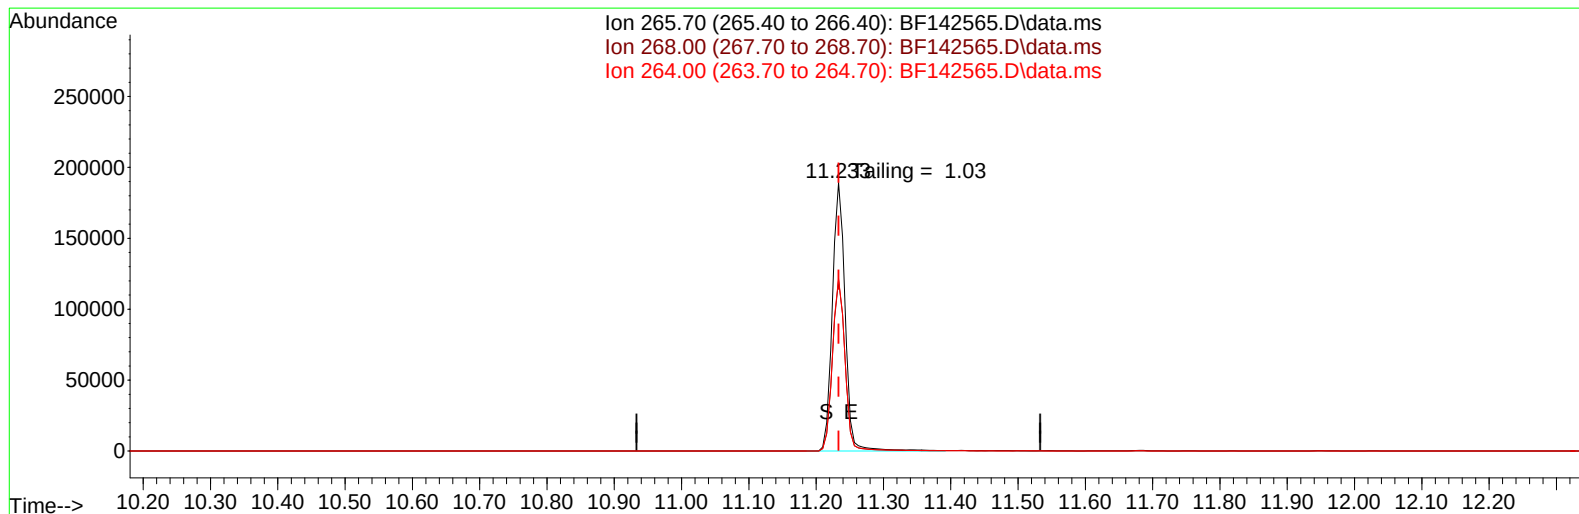

TIC: BF142565.D\data.ms

(70) Pentachlorophenol (C)




11.233min (+ 0.000) 56283.72 ng

response 248099

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	63.62
264.00	63.00	64.21
0.00	0.00	0.00

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 30 13:07:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

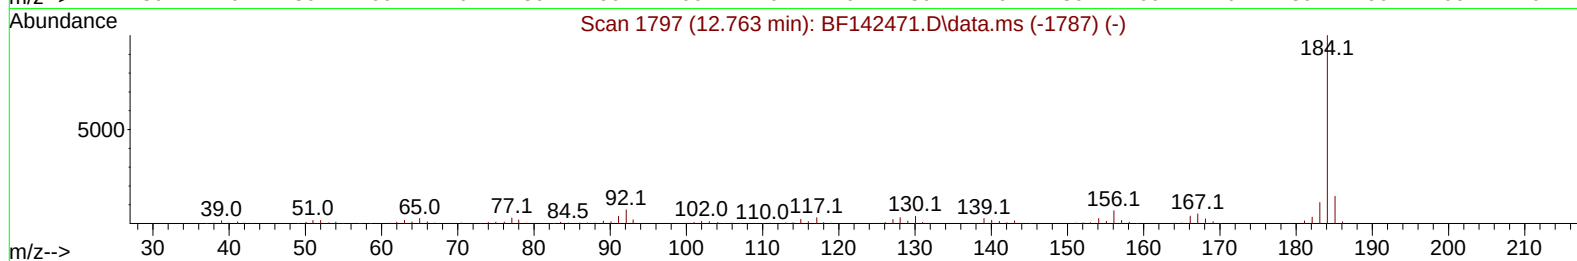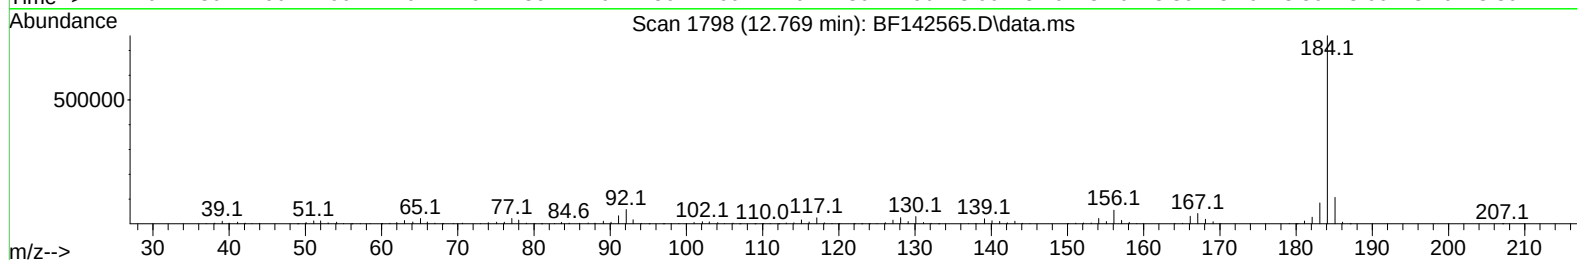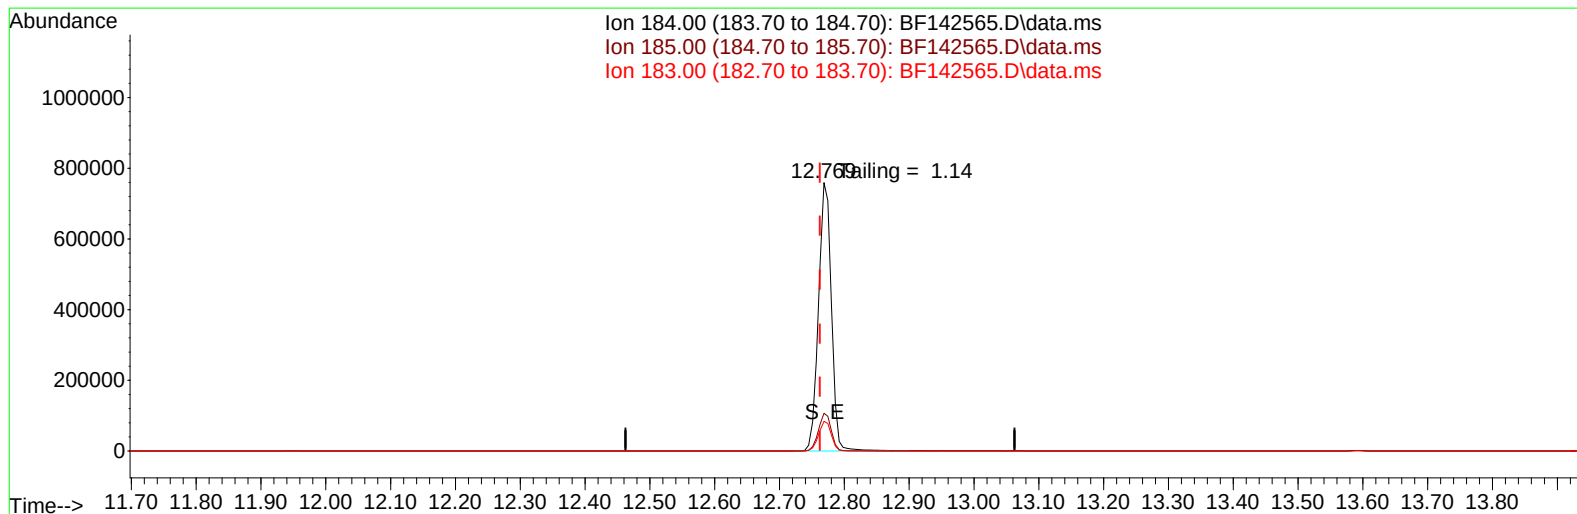

TIC: BF142565.D\data.ms

(77) Benzidine

12.769min (+ 0.006) 59056.94 ng

response **1057087**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.09
183.00	11.20	11.08
0.00	0.00	0.00