
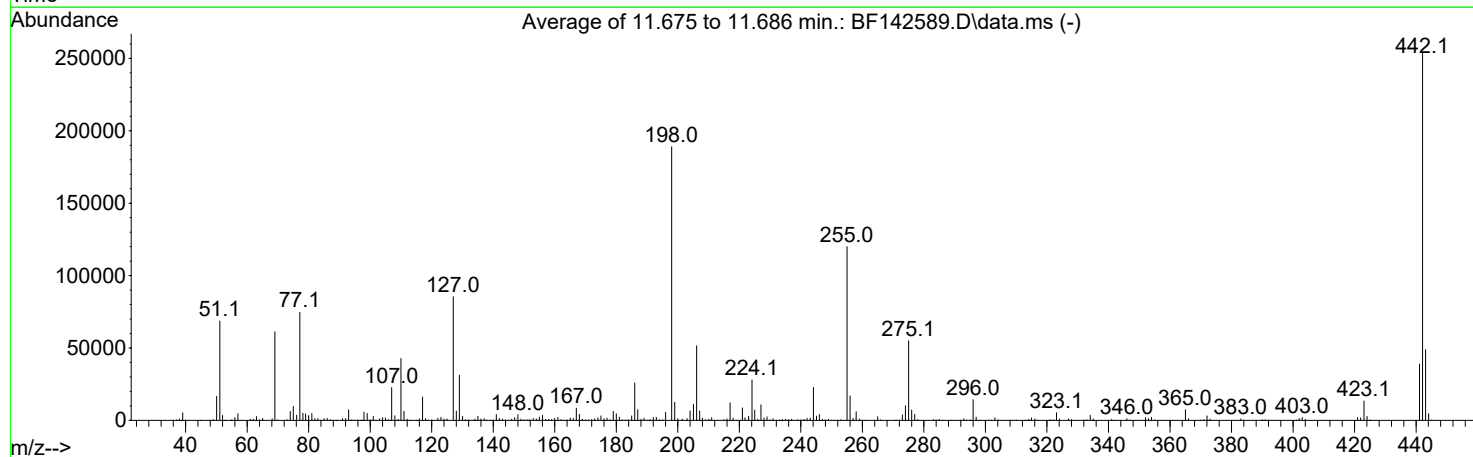


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060225\
Data File : BF142589.D
Acq On : 02 Jun 2025 11:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 20 16:26:47 2025

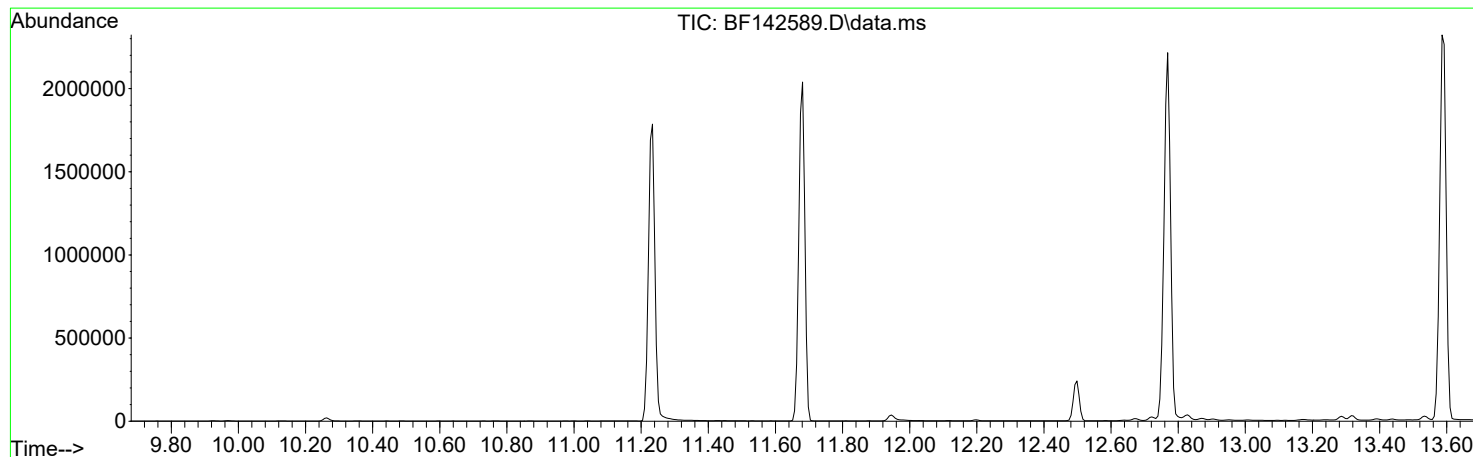

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	68579	PASS
68	69	0.00	2	1.8	1095	PASS
69	198	0.00	100	32.4	61195	PASS
70	69	0.00	2	0.6	380	PASS
127	198	10	80	45.2	85403	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	188992	PASS
199	198	5	9	6.6	12531	PASS
275	198	10	60	29.1	54928	PASS
365	198	1	100	3.9	7435	PASS
441	198	0.01	100	20.6	38853	PASS
442	442	50	100	100.0	254059	PASS
443	442	15	24	19.3	49003	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/2/2025	BNA_F	<u>BF142589.D</u>
Compound Name	Response	Retention Time
DDT	635948	13.592
DDD	13787	13.316
DDE	1005	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14792	650740	2.27

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060225\
Data File : BF142589.D
Acq On : 02 Jun 2025 11:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 02 12:45:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

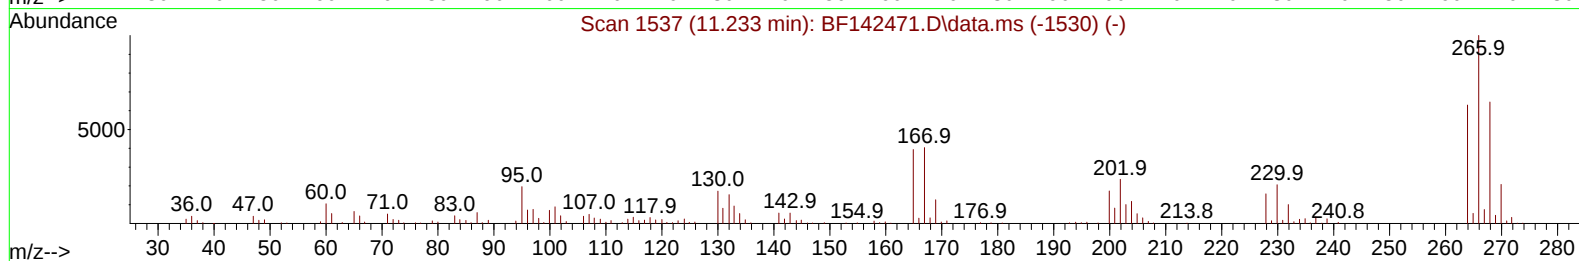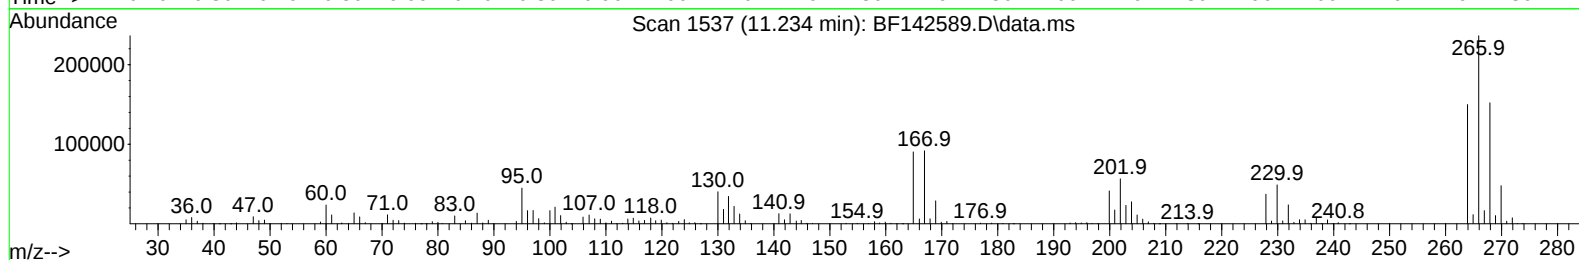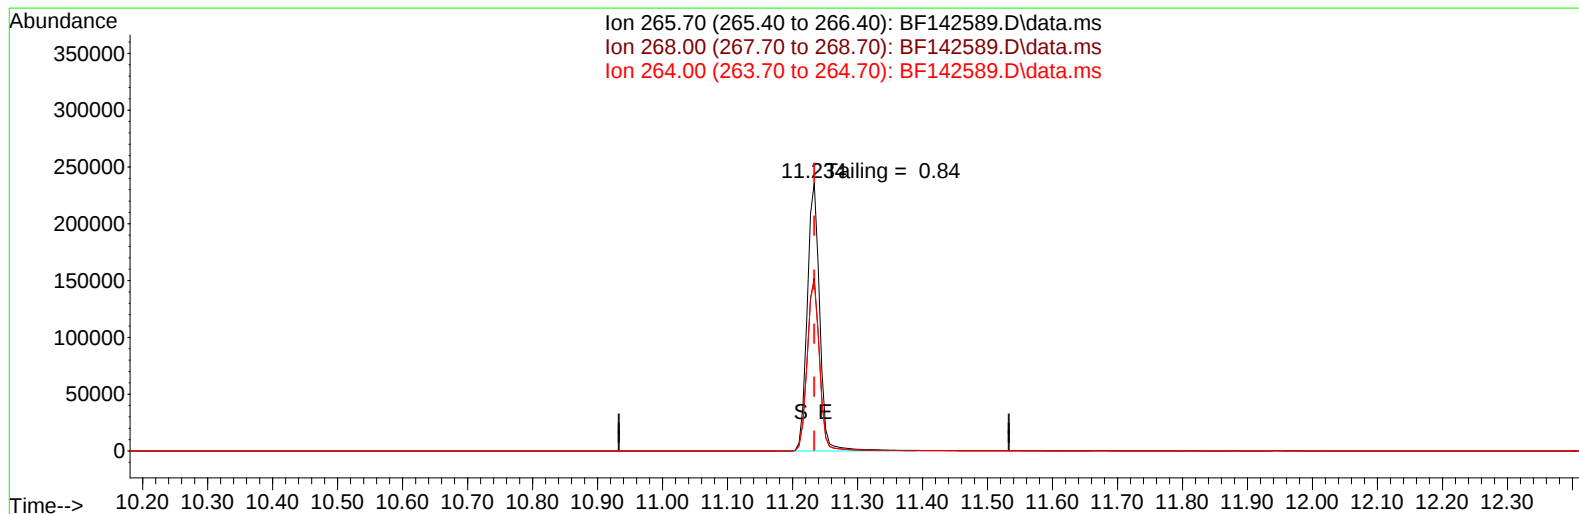

TIC: BF142589.D\data.ms

(70) Pentachlorophenol (C)

11.234min (+ 0.000) 81847.51 ng m




response 317877

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.41
264.00	63.00	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060225\
Data File : BF142589.D
Acq On : 02 Jun 2025 11:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 02 12:45:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

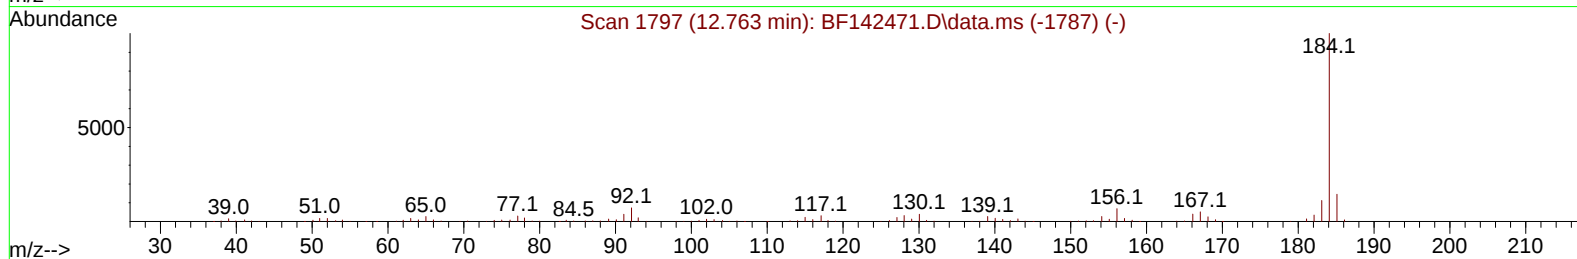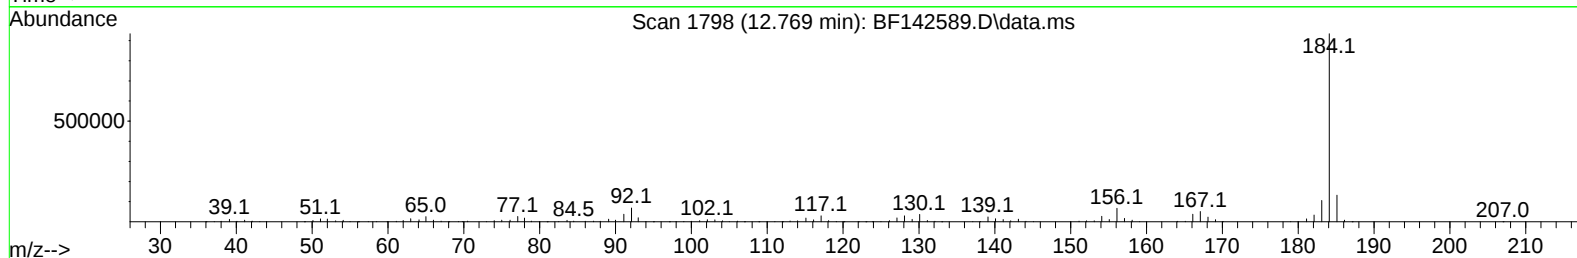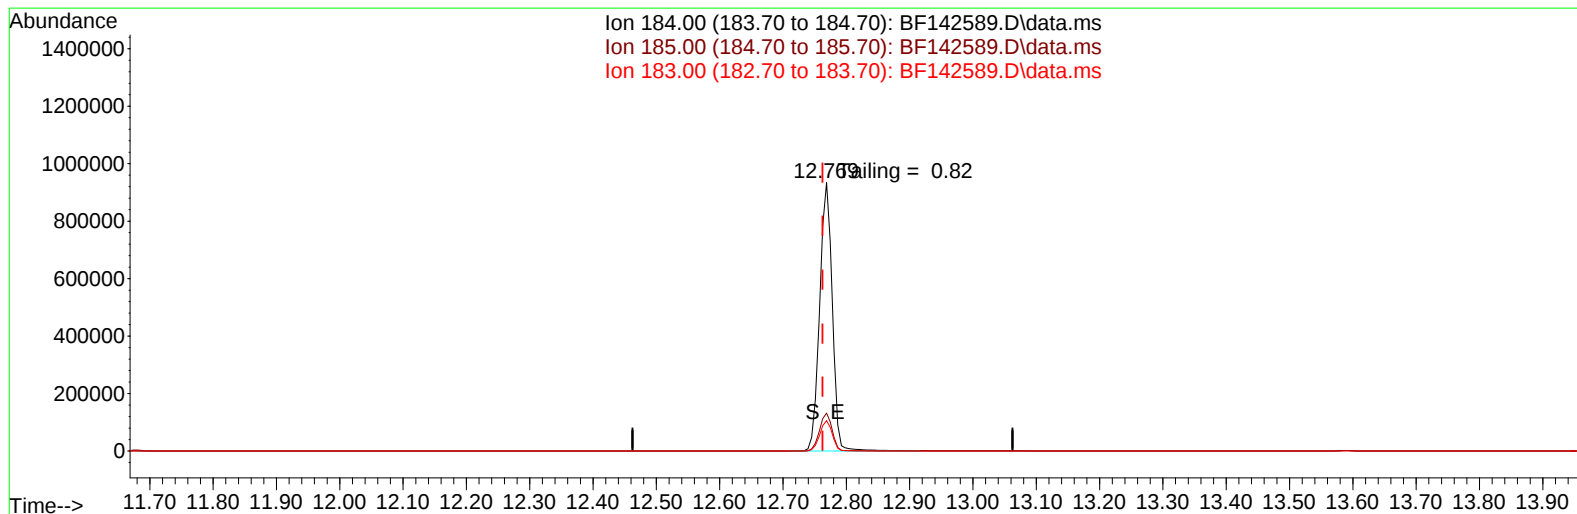

TIC: BF142589.D\data.ms

(77) Benzidine

12.769min (+ 0.006) 63416.49 ng

response 1295595

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.12
183.00	11.20	11.33
0.00	0.00	0.00