

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060225\
 Data File : VY022499.D
 Acq On : 02 Jun 2025 16:00
 Operator : SY/MD
 Sample : VY0602SBL02
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0602SBL02

Quant Time: Jun 03 04:06:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 03 03:22:04 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	309051	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	557091	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	442919	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	162489	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	183940	53.215	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	106.420%
35) Dibromofluoromethane	7.634	113	169603	51.006	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.020%
50) Toluene-d8	10.109	98	667368	49.671	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	99.340%
62) 4-Bromofluorobenzene	12.408	95	171494	42.839	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	85.680%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060225\
Data File : VY022499.D
Acq On : 02 Jun 2025 16:00
Operator : SY/MD
Sample : VY0602SBL02
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0602SBL02

Quant Time: Jun 03 04:06:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 03 03:22:04 2025
Response via : Initial Calibration




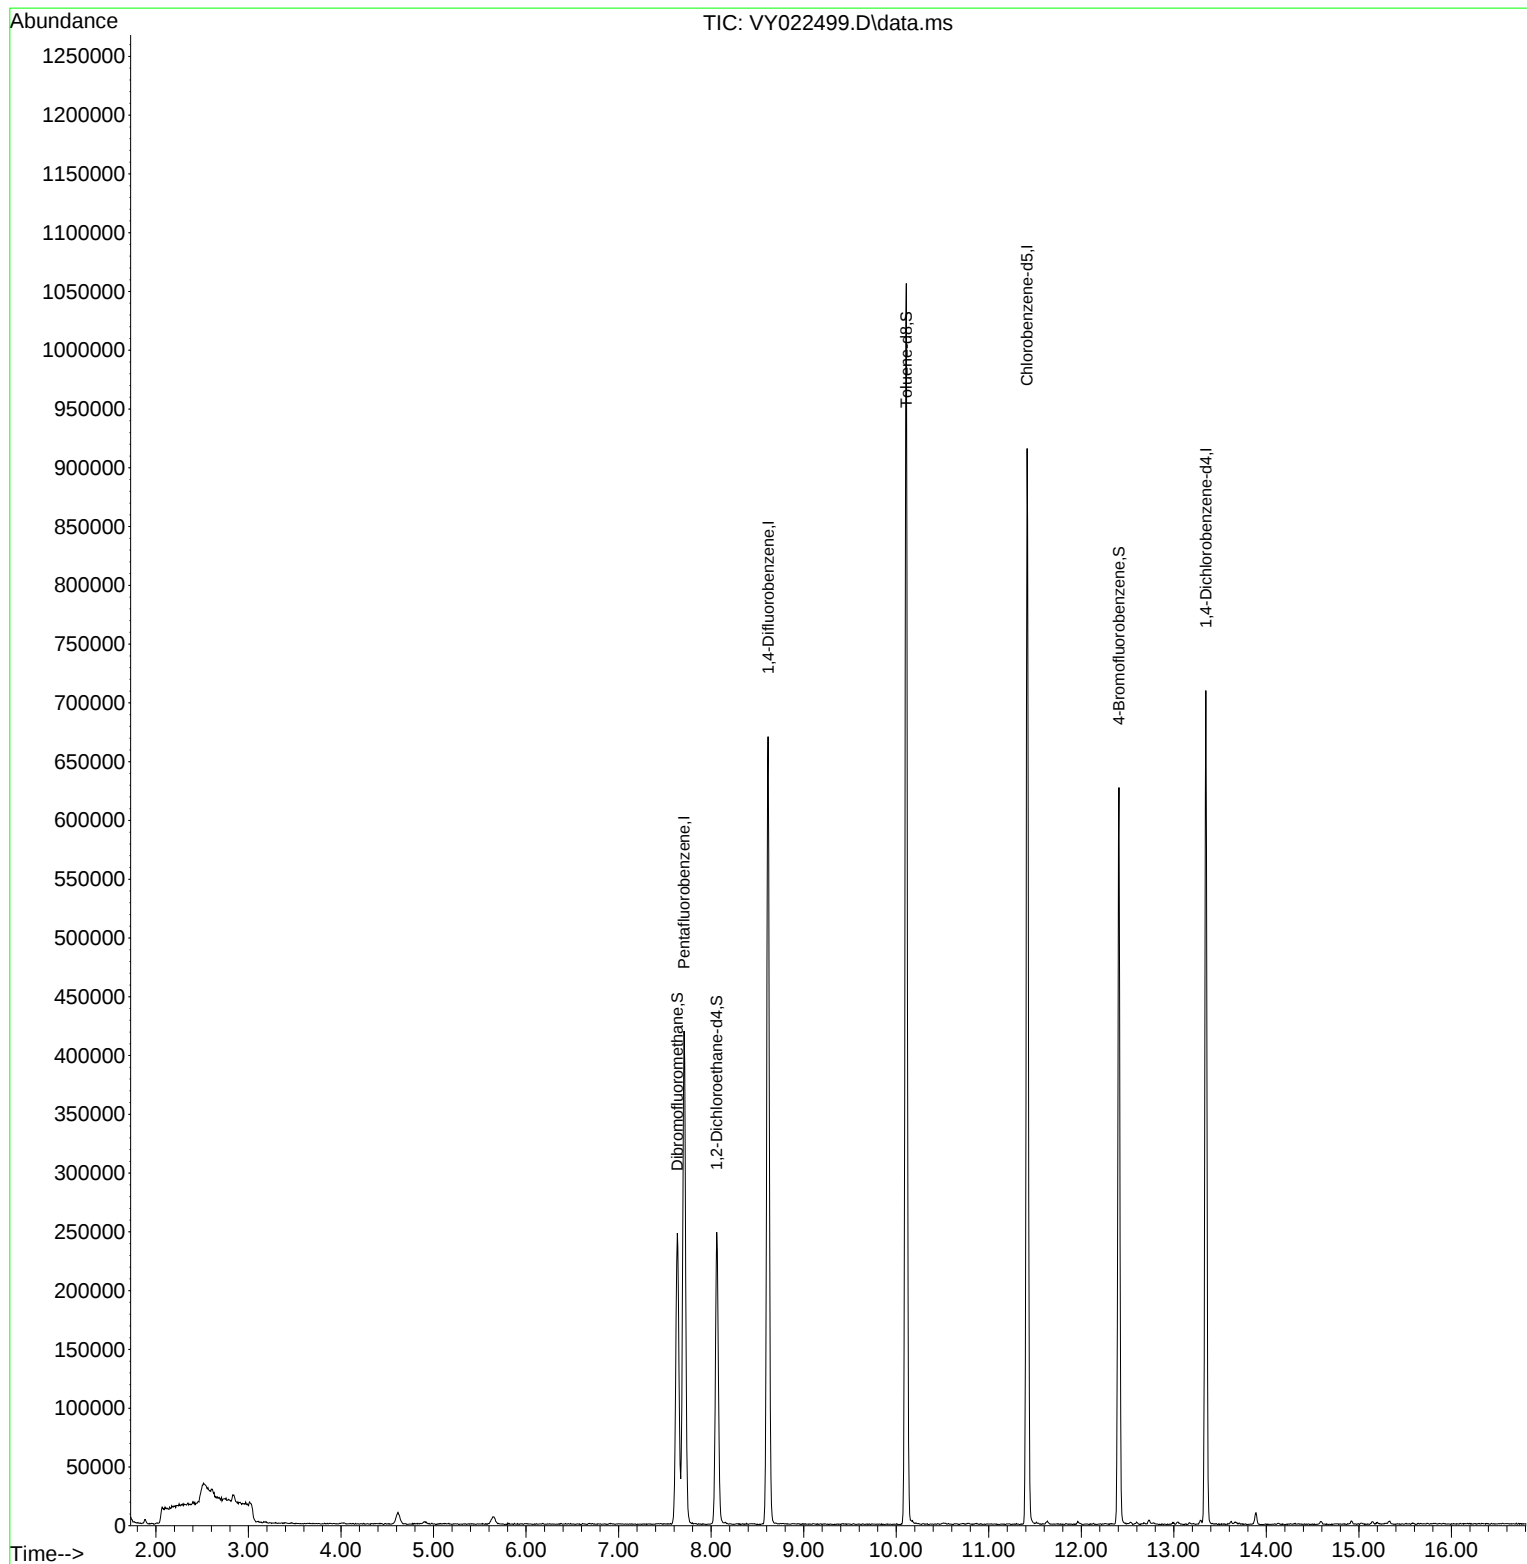


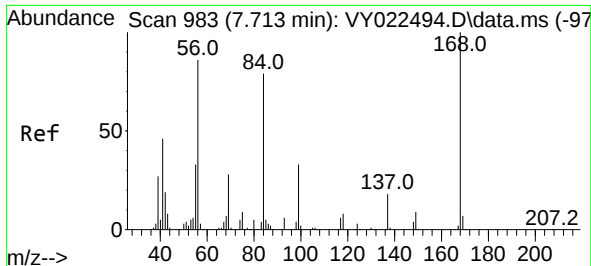

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY022499.D
Acq: 02 Jun 2025 16:00




Instrument :
MSVOA_Y
ClientSampleId :
VY0602SBL02

Tgt Ion:168 Resp: 309051
Ion Ratio Lower Upper
168 100
99 54.8 44.3 66.5

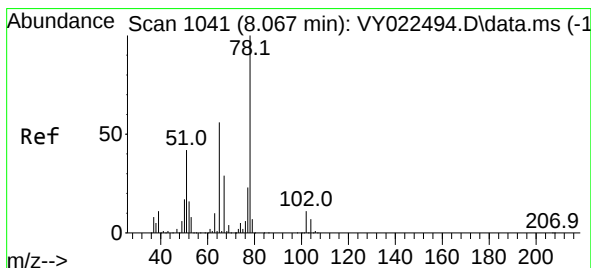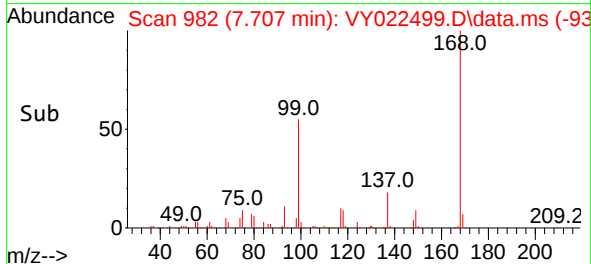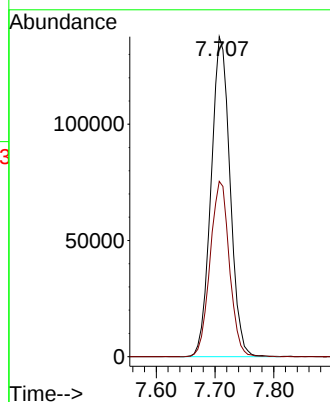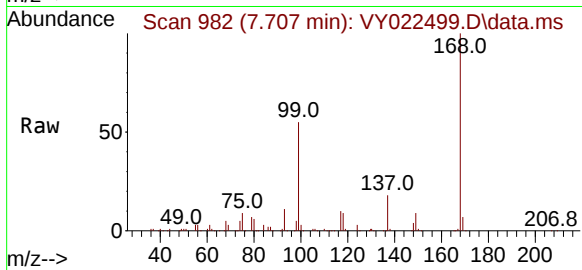

#33
1,2-Dichloroethane-d4
Concen: 53.215 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.006 min
Lab File: VY022499.D
Acq: 02 Jun 2025 16:00

Tgt Ion: 65 Resp: 183940
Ion Ratio Lower Upper
65 100
67 53.1 0.0 103.4


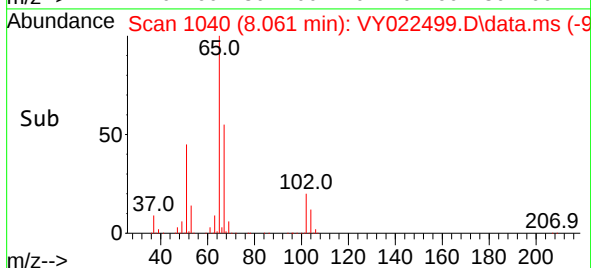
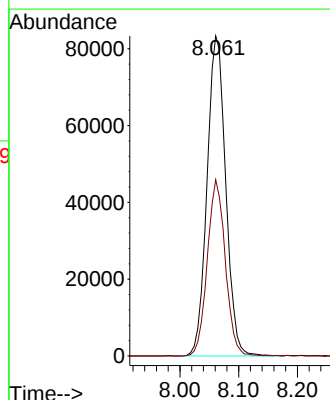
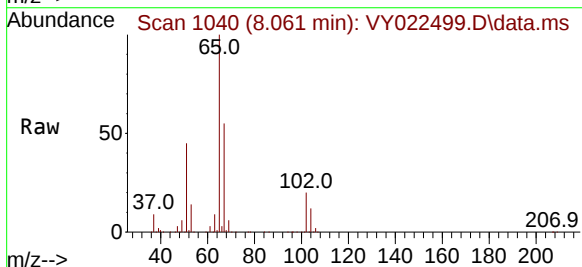




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. -0.000 min
Lab File: VY022499.D
Acq: 02 Jun 2025 16:00




Instrument :
MSVOA_Y
ClientSampleId :
VY0602SBL02

Tgt Ion:114 Resp: 557091
Ion Ratio Lower Upper
114 100
63 20.4 0.0 40.8
88 13.9 0.0 27.8

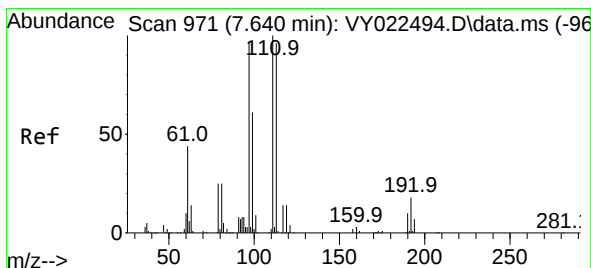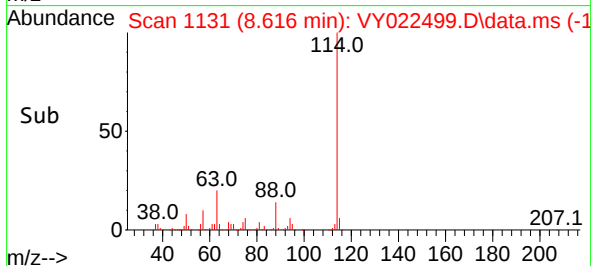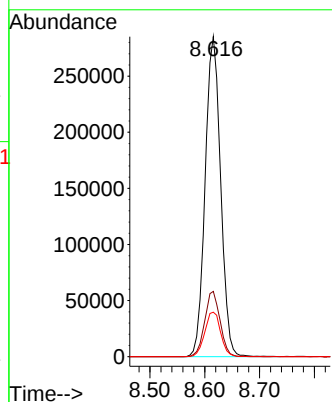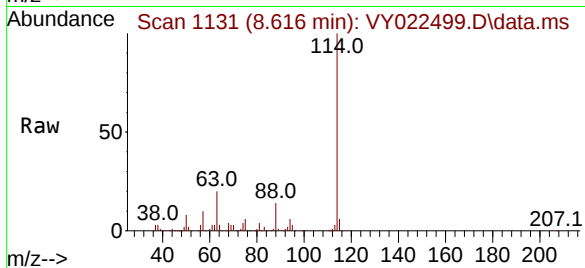

#35
Dibromofluoromethane
Concen: 51.006 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.006 min
Lab File: VY022499.D
Acq: 02 Jun 2025 16:00

Tgt Ion:113 Resp: 169603
Ion Ratio Lower Upper
113 100
111 102.8 81.1 121.7
192 18.4 14.2 21.2


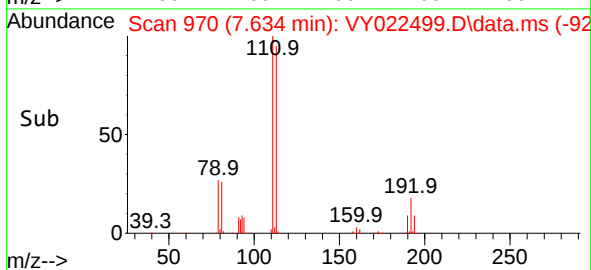
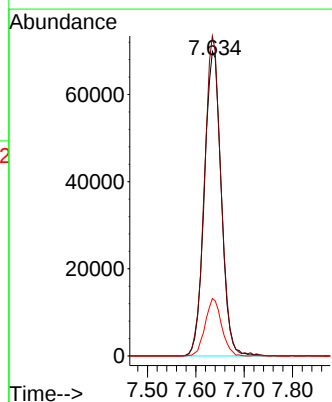
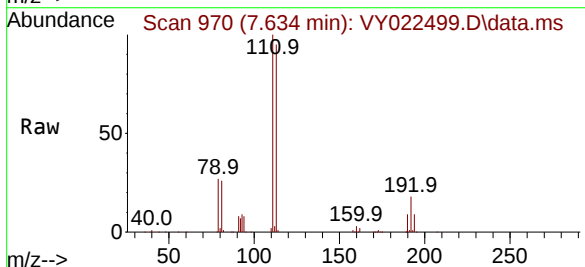




#50
Toluene-d8
Concen: 49.671 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. -0.000 min
Lab File: VY022499.D
Acq: 02 Jun 2025 16:00




Instrument :
MSVOA_Y
ClientSampleId :
VY0602SBL02


Tgt Ion: 98 Resp: 667368
Ion Ratio Lower Upper
98 100
100 63.9 51.4 77.0

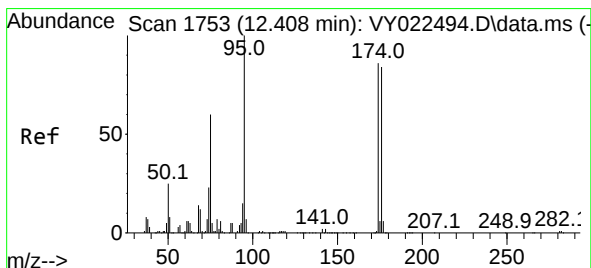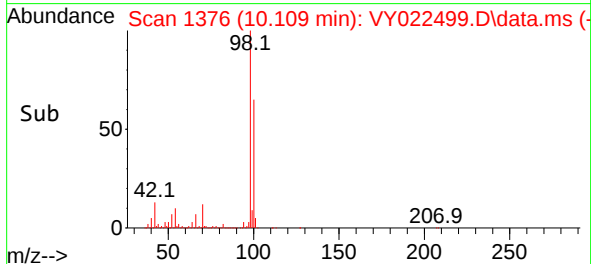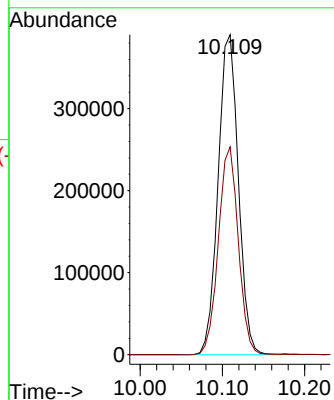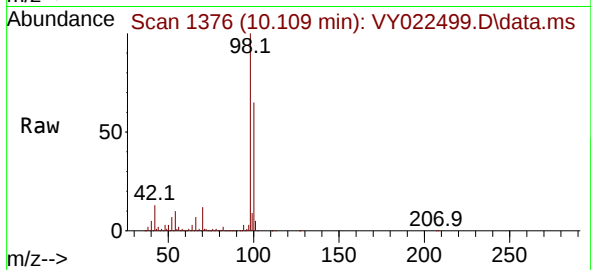

#62
4-Bromofluorobenzene
Concen: 42.839 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. -0.000 min
Lab File: VY022499.D
Acq: 02 Jun 2025 16:00

Tgt Ion: 95 Resp: 171494
Ion Ratio Lower Upper
95 100
174 84.7 0.0 170.0
176 82.6 0.0 166.2

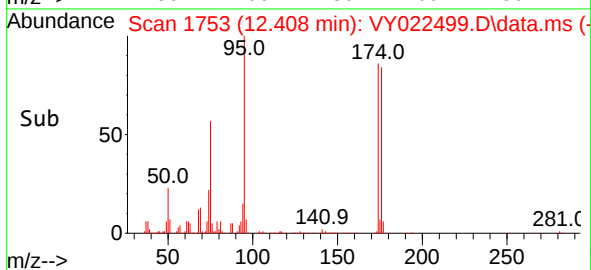
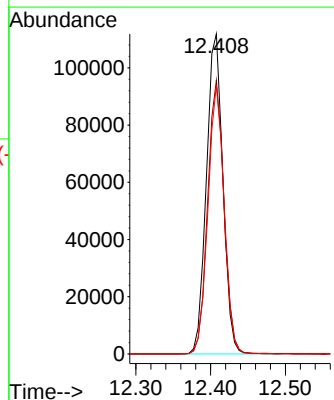
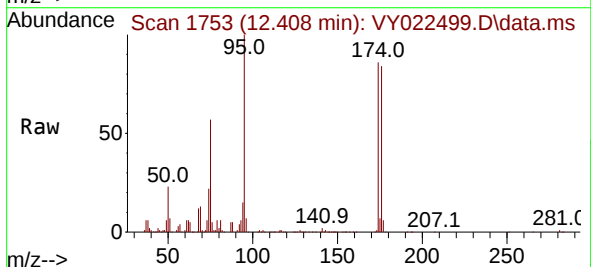


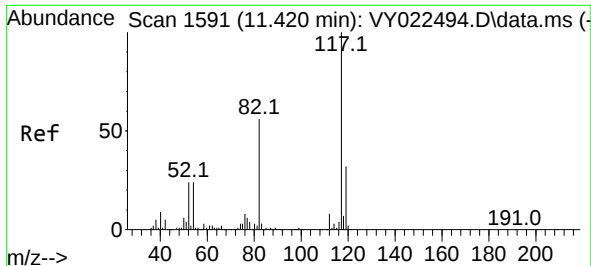

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 117
Delta R.T. -0.006 min
Lab File: VY022499.D
Acq: 02 Jun 2025 16:00

Instrument :
MSVOA_Y
ClientSampleId :
VY0602SBL02

Tgt Ion:117 Resp: 442919
Ion Ratio Lower Upper
117 100
82 57.2 44.6 66.8
119 32.0 25.4 38.0

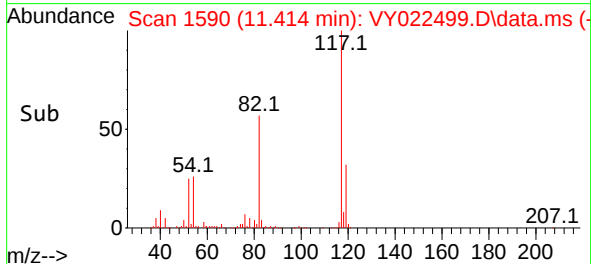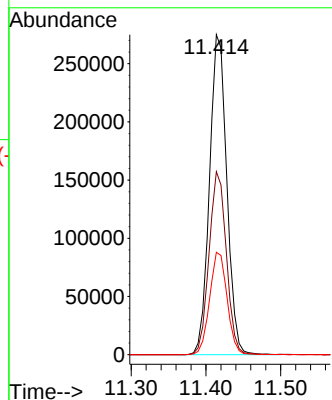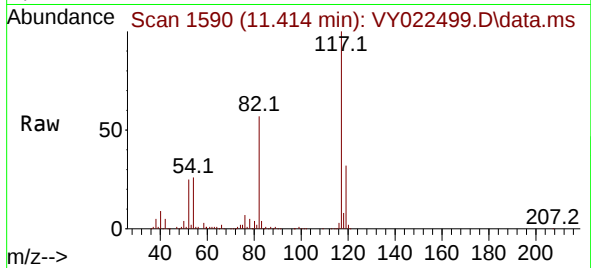

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.347 min Scan# 1907
Delta R.T. -0.000 min
Lab File: VY022499.D
Acq: 02 Jun 2025 16:00

Tgt Ion:152 Resp: 162489
Ion Ratio Lower Upper
152 100
115 57.4 28.9 86.7
150 158.3 0.0 349.6

