
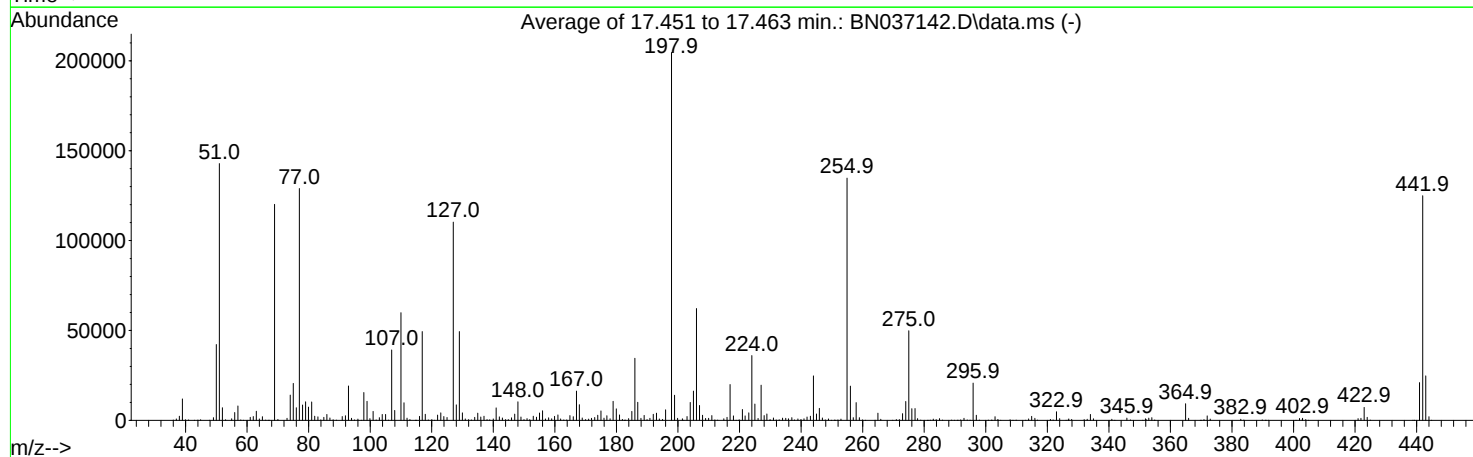


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060325\
Data File : BN037142.D
Acq On : 03 Jun 2025 10:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN060325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 04 01:52:03 2025

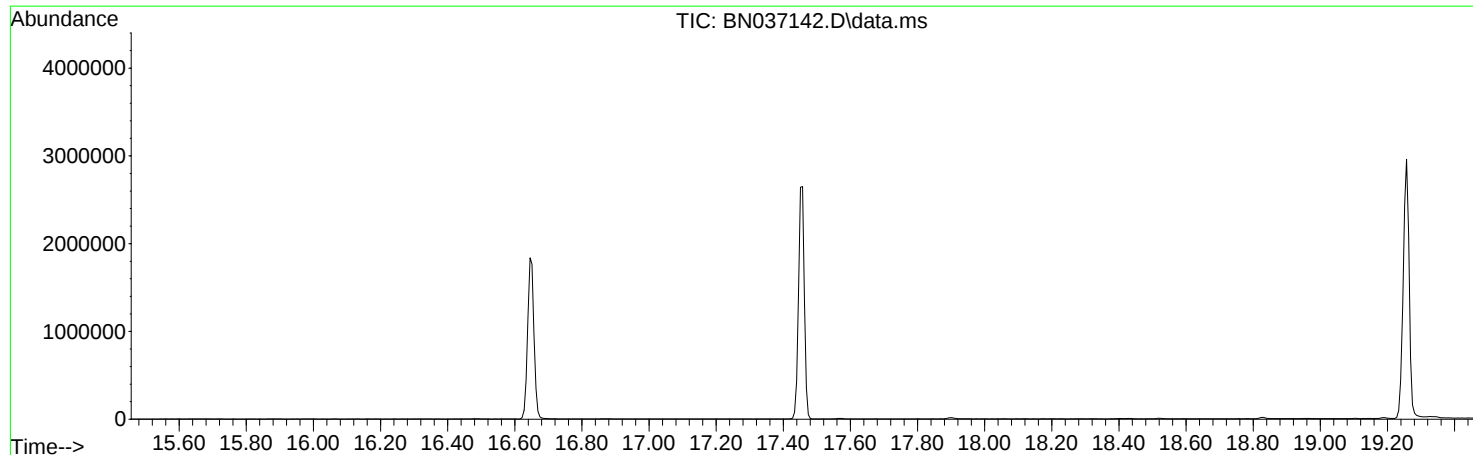




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	69.8	142869	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	58.7	120176	PASS
70	69	0.00	2	0.5	575	PASS
127	198	10	80	53.9	110283	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	204619	PASS
199	198	5	9	6.8	13950	PASS
275	198	10	60	24.4	49829	PASS
365	198	1	100	4.5	9270	PASS
441	198	0.01	100	10.3	21027	PASS
442	442	50	100	100.0	124989	PASS
443	442	15	24	19.8	24771	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060325\
Data File : BN037142.D
Acq On : 03 Jun 2025 10:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 03 13:49:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

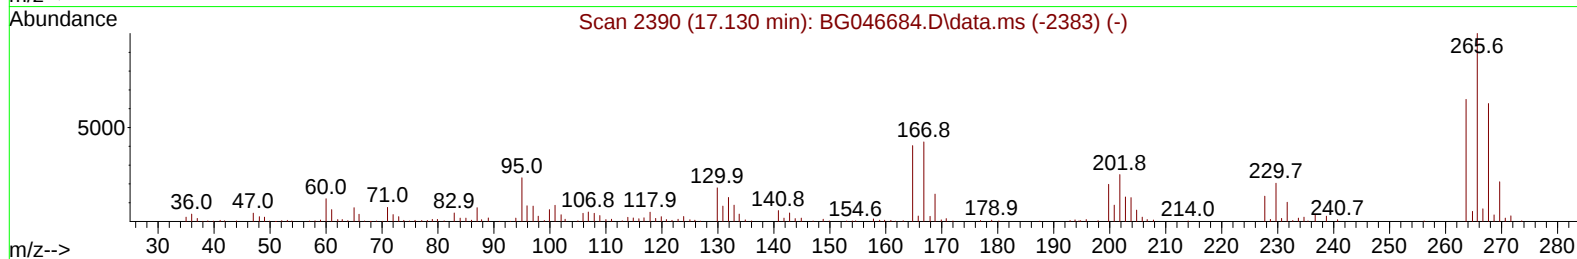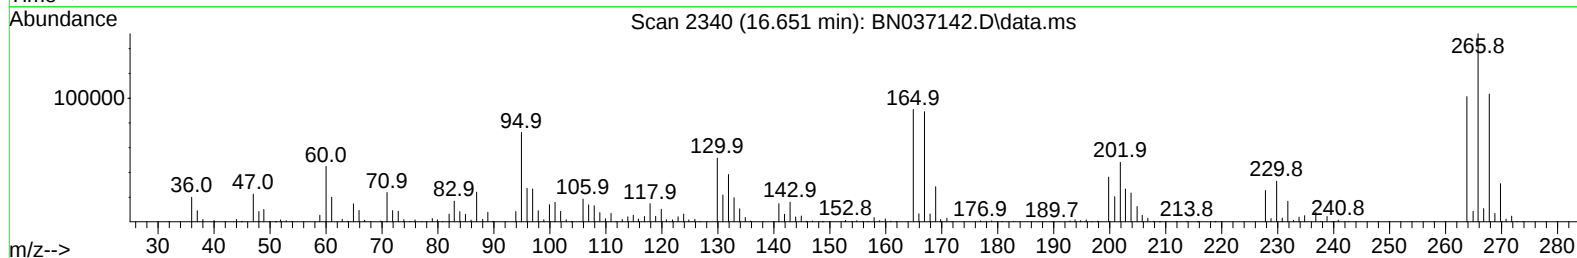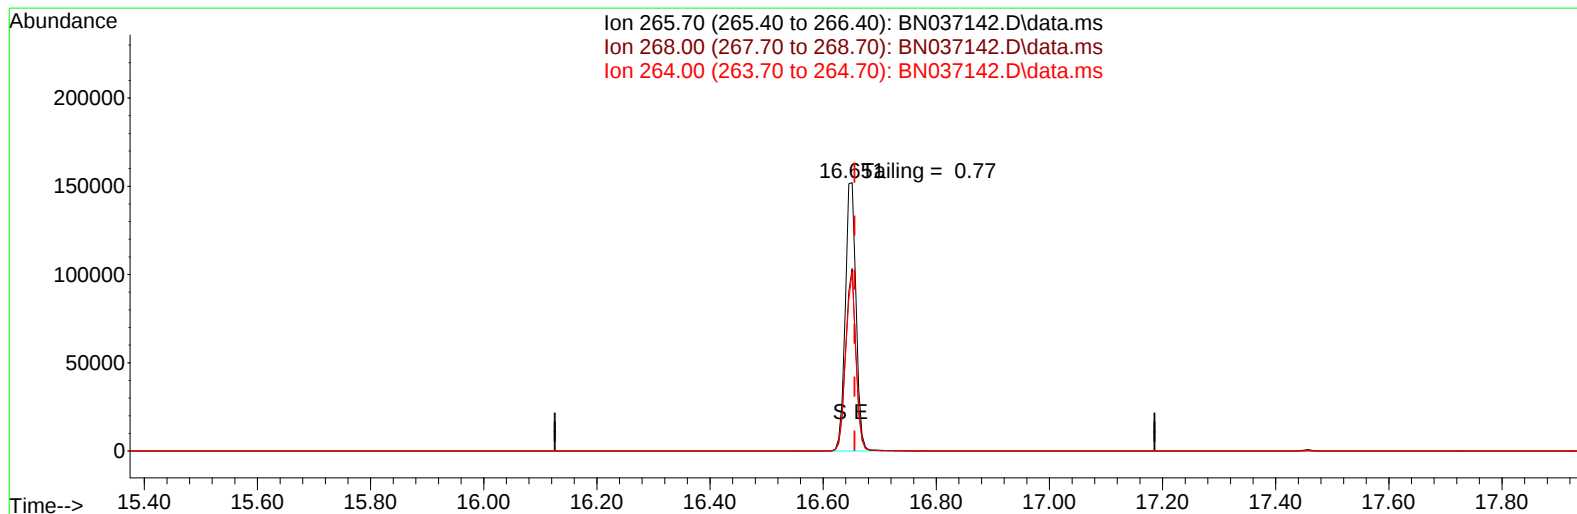

TIC: BN037142.D\data.ms

(70) Pentachlorophenol (C)

16.651min (-0.005) 16176.78 ng




response 200710

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.97
264.00	61.60	66.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060325\
Data File : BN037142.D
Acq On : 03 Jun 2025 10:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 03 13:56:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

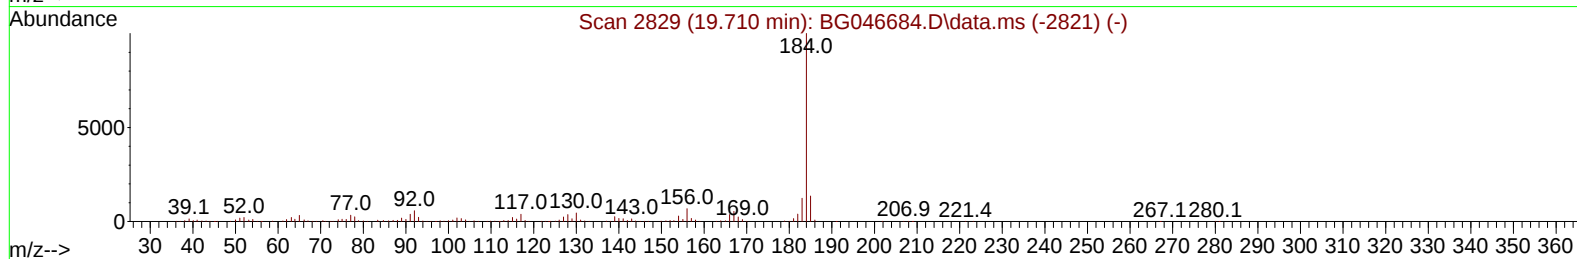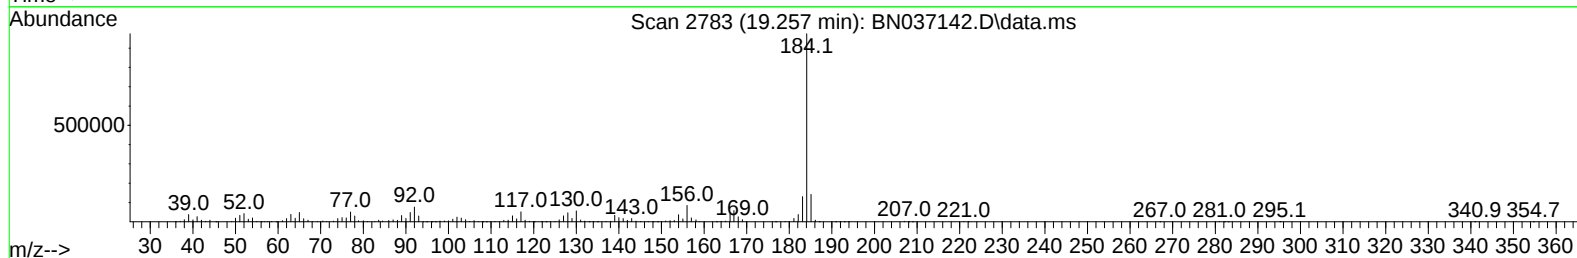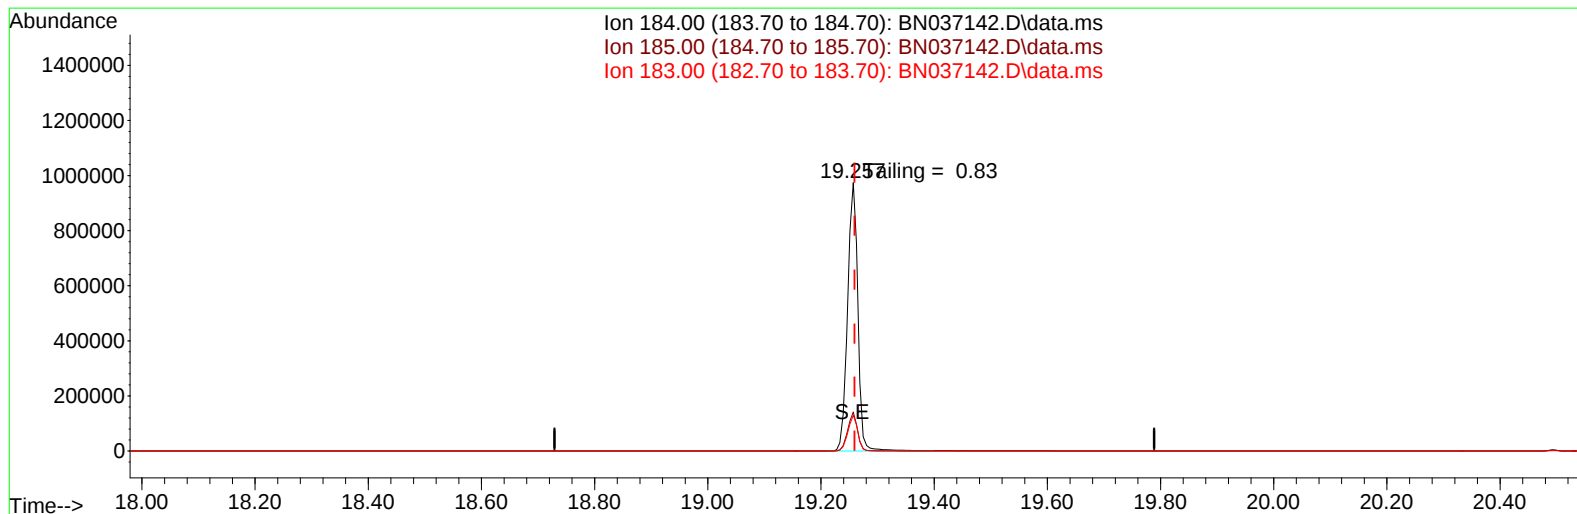

TIC: BN037142.D\data.ms

(77) Benzidine

19.257min (-0.002) 0.00 ng

response 1234162

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.54
183.00	13.20	13.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/3/2025	BNA_N	<u>BN037142.D</u>
Compound Name	Response	Retention Time
DDT	724224	20.492
DDD	9498	20.104
DDE	658	19.545
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10156	734380	1.38

Instrument :
BNA_N
ClientSampleId :
DFTPP