
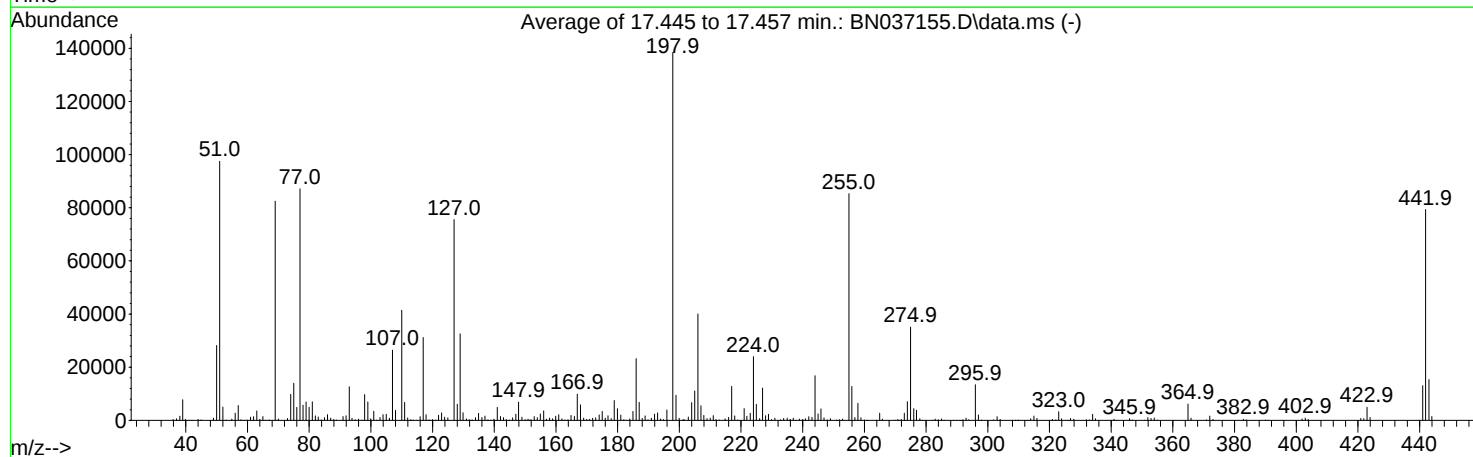


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060325\
Data File : BN037155.D
Acq On : 03 Jun 2025 20:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN060325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 04 01:52:03 2025

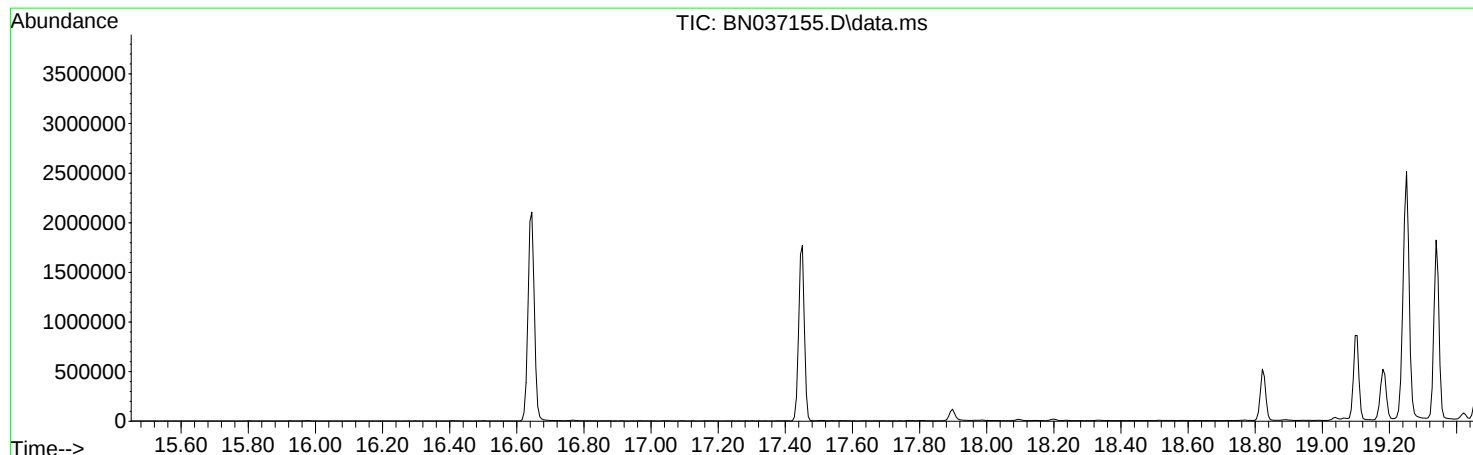




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	70.4	97493	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	59.6	82515	PASS
70	69	0.00	2	0.6	524	PASS
127	198	10	80	54.6	75568	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	138427	PASS
199	198	5	9	6.8	9434	PASS
275	198	10	60	25.3	35085	PASS
365	198	1	100	4.4	6127	PASS
441	198	0.01	100	9.5	13103	PASS
442	442	50	100	100.0	79381	PASS
443	442	15	24	19.4	15390	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060325\
Data File : BN037155.D
Acq On : 03 Jun 2025 20:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 04 02:36:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:35:39 2025
Response via : Initial Calibration

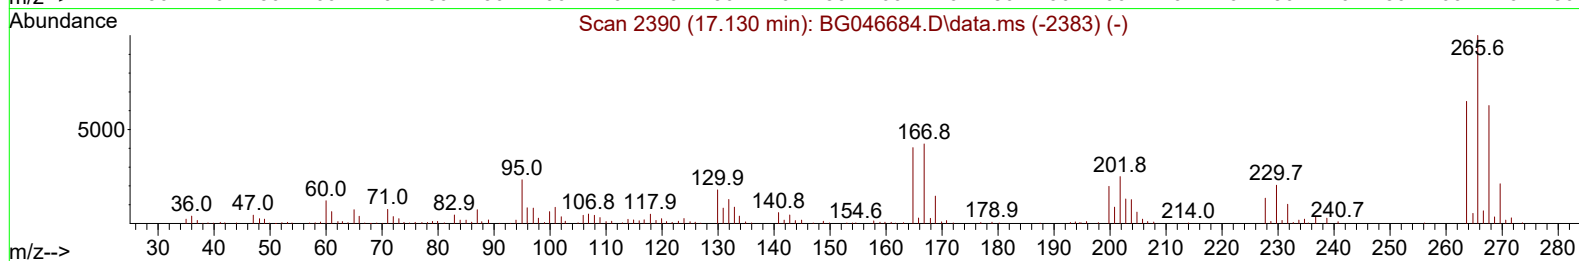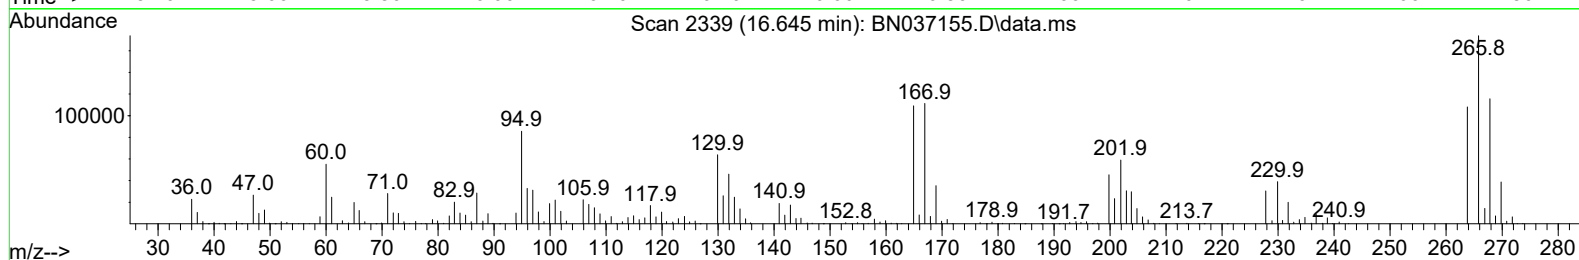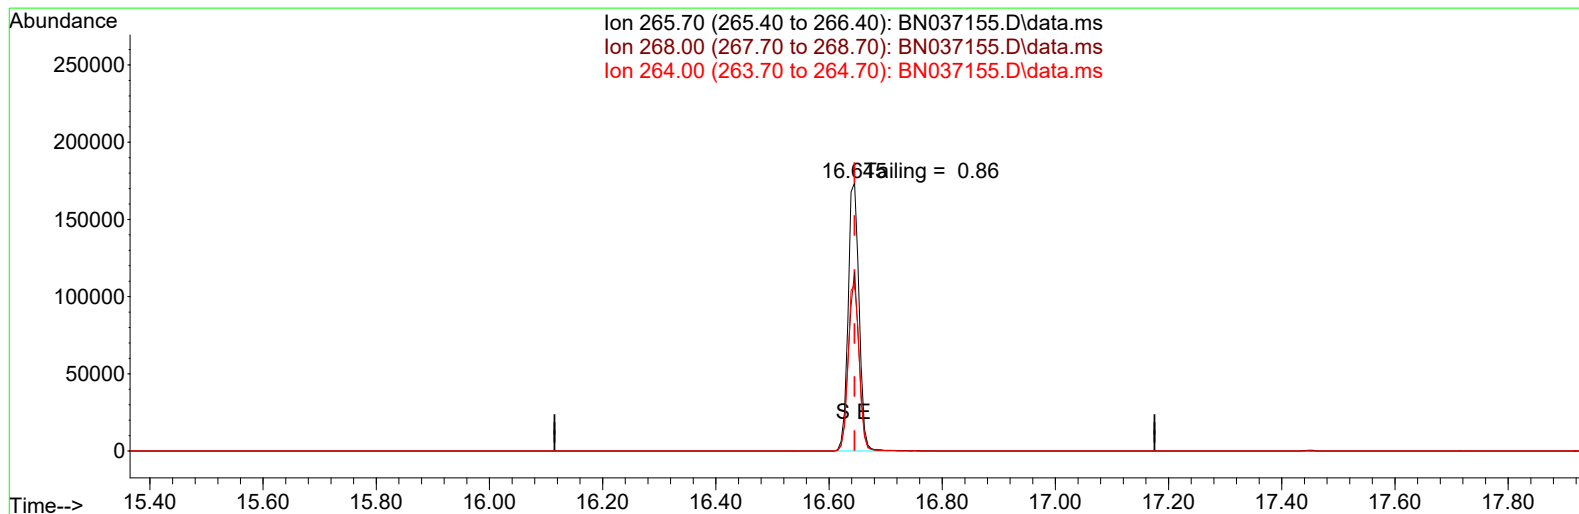

TIC: BN037155.D\data.ms

(70) Pentachlorophenol (C)

16.645min (0.000) 277.78 ng




response 233660

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.51
264.00	61.60	62.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060325\
Data File : BN037155.D
Acq On : 03 Jun 2025 20:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 04 02:36:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:35:39 2025
Response via : Initial Calibration

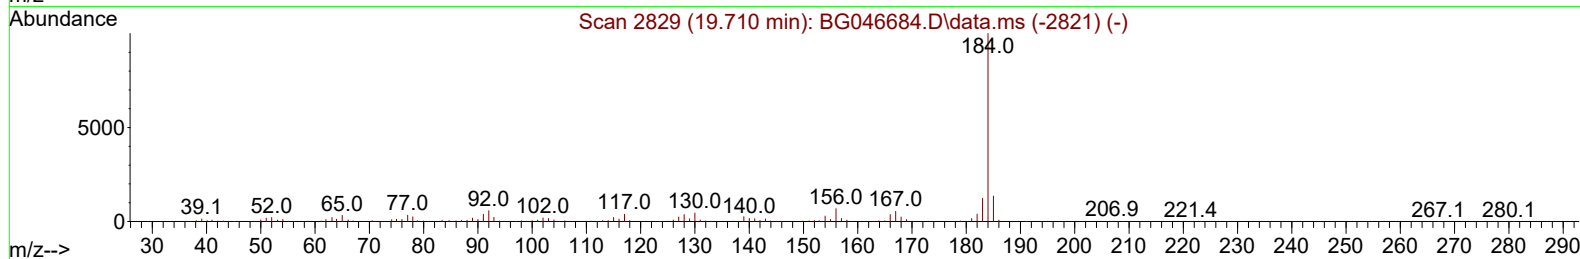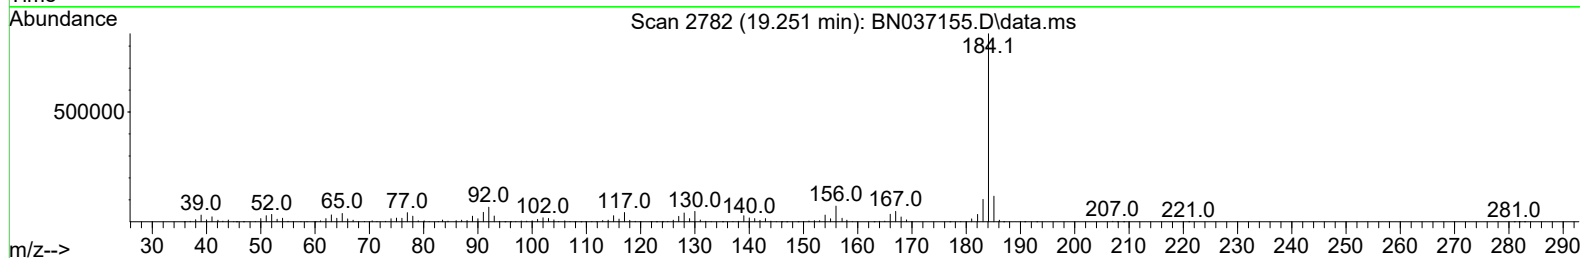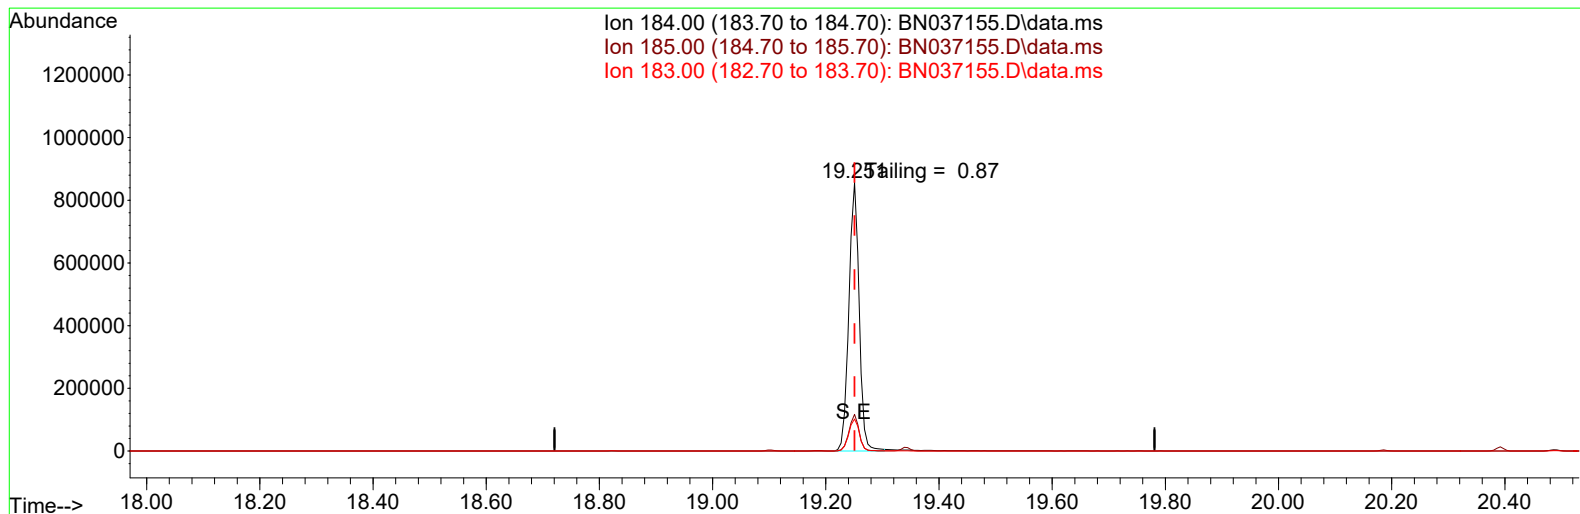

TIC: BN037155.D\data.ms

(77) Benzidine

19.251min (0.000) 0.00 ng

response 1091920

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.66
183.00	13.20	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/3/2025	BNA_N	<u>BN037155.D</u>
Compound Name	Response	Retention Time
DDT	668516	20.492
DDD	9485	20.098
DDE	192	19.539
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9677	678193	1.43

Instrument :
BNA_N
ClientSampleId :
DFTPP