


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060425\
Data File : BN037165.D
Acq On : 04 Jun 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN060325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 04 01:52:03 2025

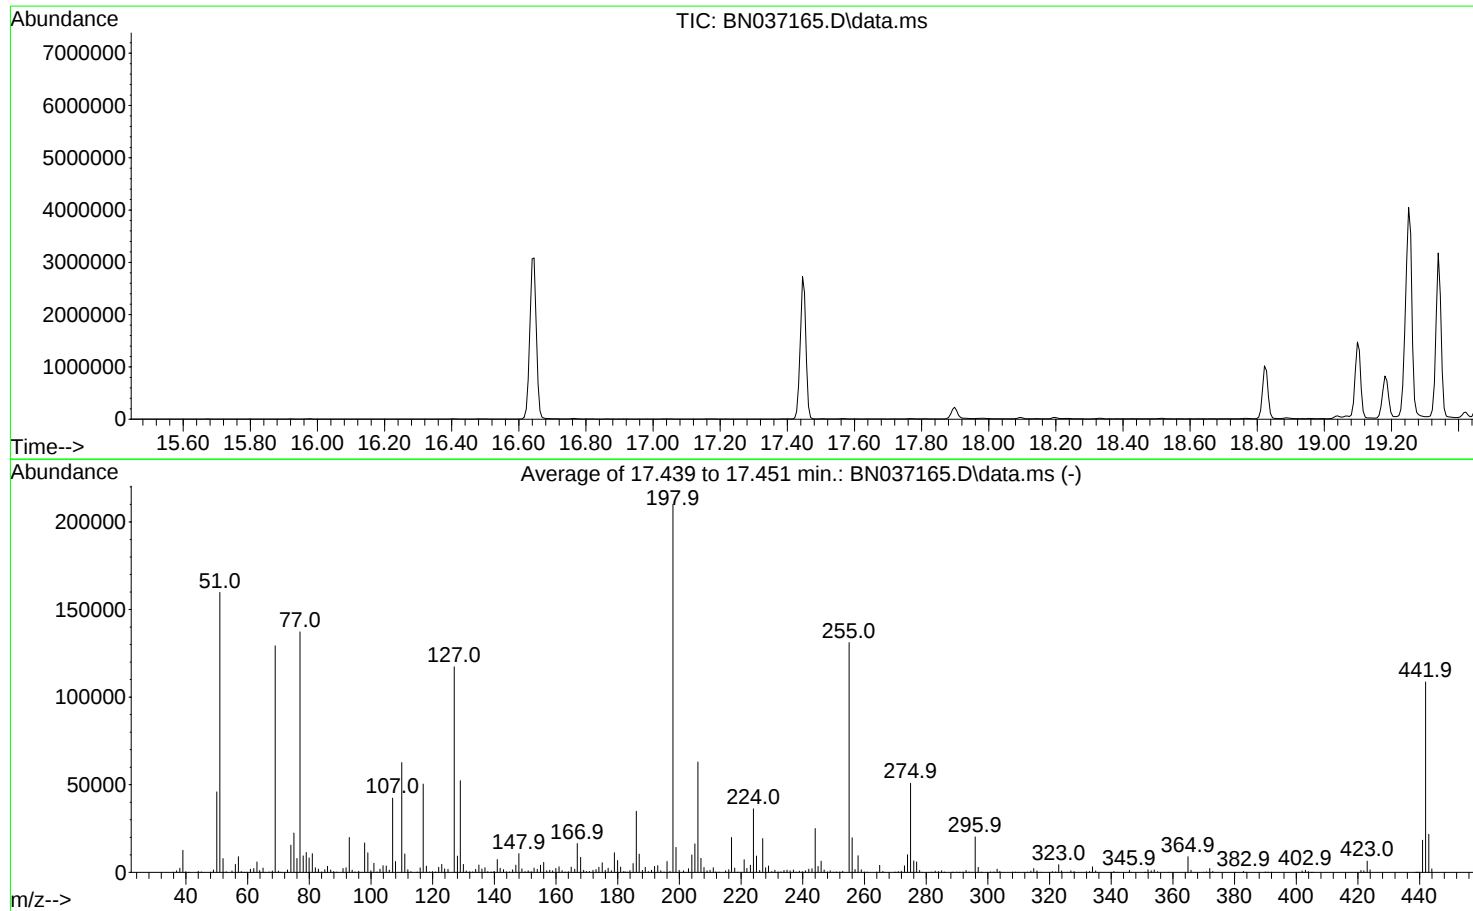




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	76.1	159787	PASS
68	69	0.00	2	0.6	809	PASS
69	198	0.00	100	61.6	129340	PASS
70	69	0.00	2	0.5	691	PASS
127	198	10	80	55.9	117328	PASS
197	198	0.00	2	0.2	516	PASS
198	198	100	100	100.0	209941	PASS
199	198	5	9	6.8	14242	PASS
275	198	10	60	24.2	50891	PASS
365	198	1	100	4.3	8935	PASS
441	198	0.01	100	8.7	18355	PASS
442	442	50	100	100.0	108645	PASS
443	442	15	24	20.0	21721	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060425\
Data File : BN037165.D
Acq On : 04 Jun 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 04 15:38:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:36:29 2025
Response via : Initial Calibration

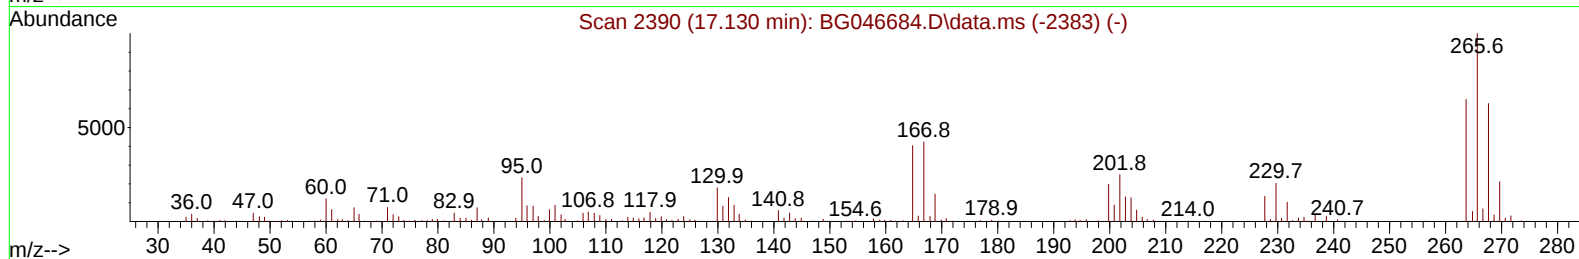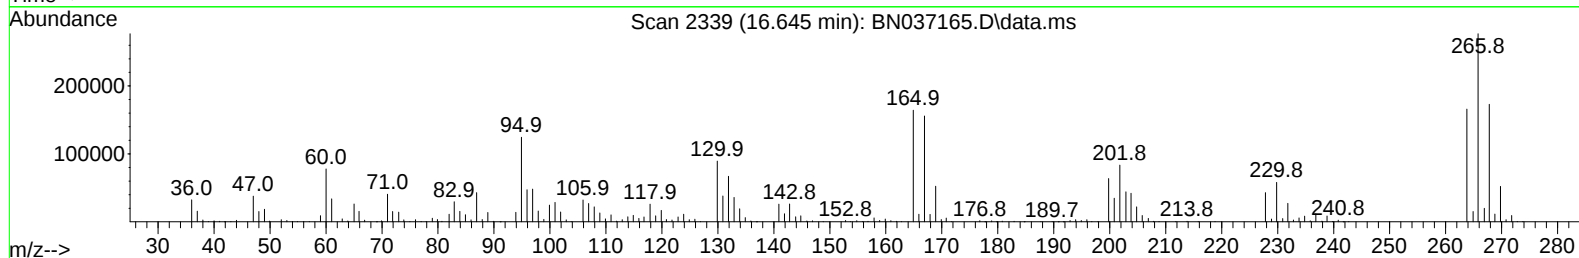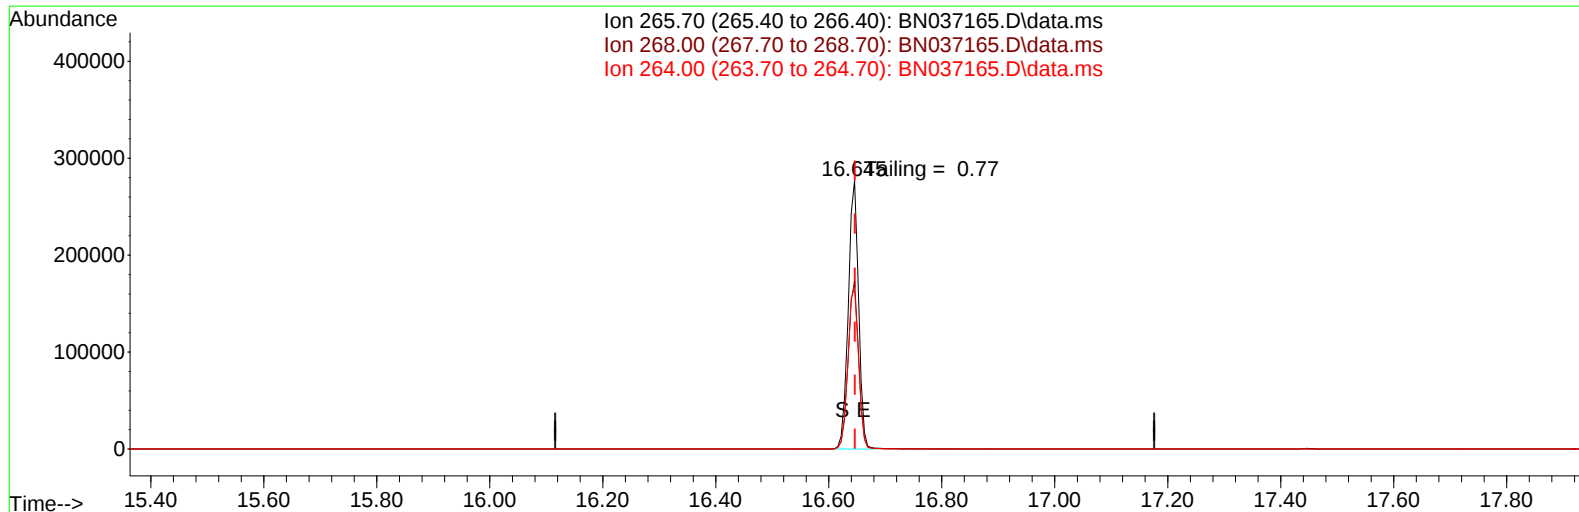

TIC: BN037165.D\data.ms

(70) Pentachlorophenol (C)

16.645min (-0.001) 30128.98 ng




response 352539

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.46
264.00	61.60	59.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060425\
Data File : BN037165.D
Acq On : 04 Jun 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 04 15:36:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:36:29 2025
Response via : Initial Calibration

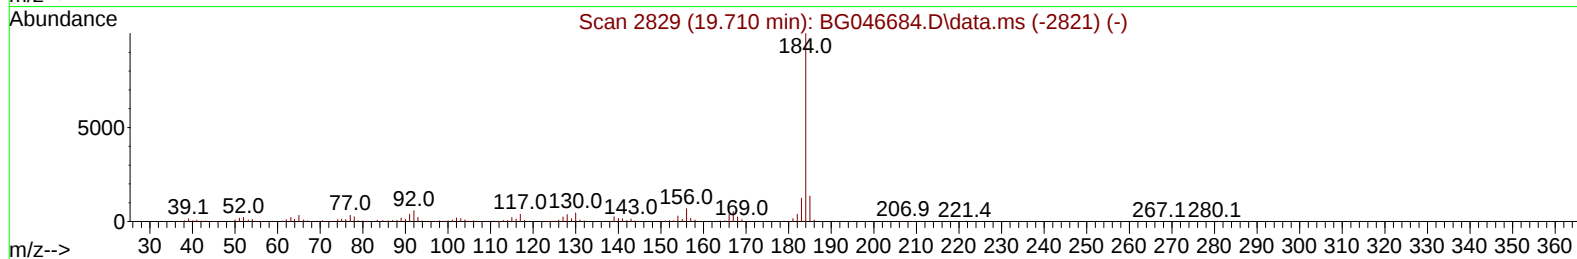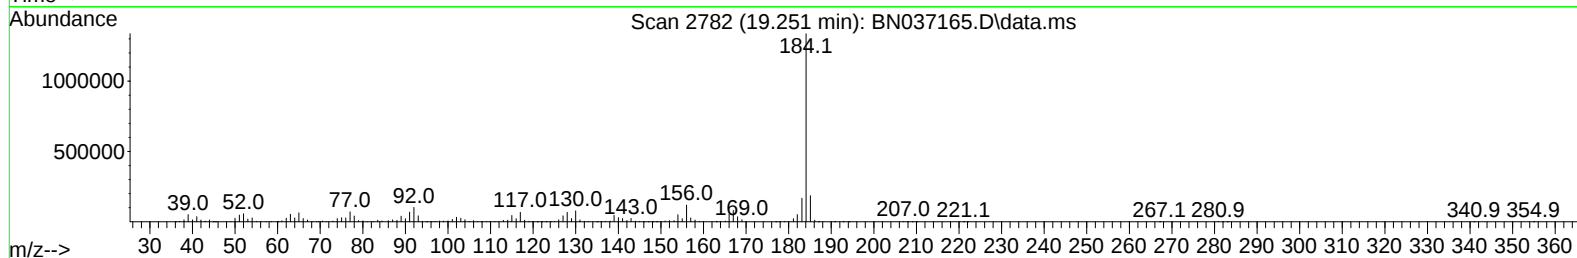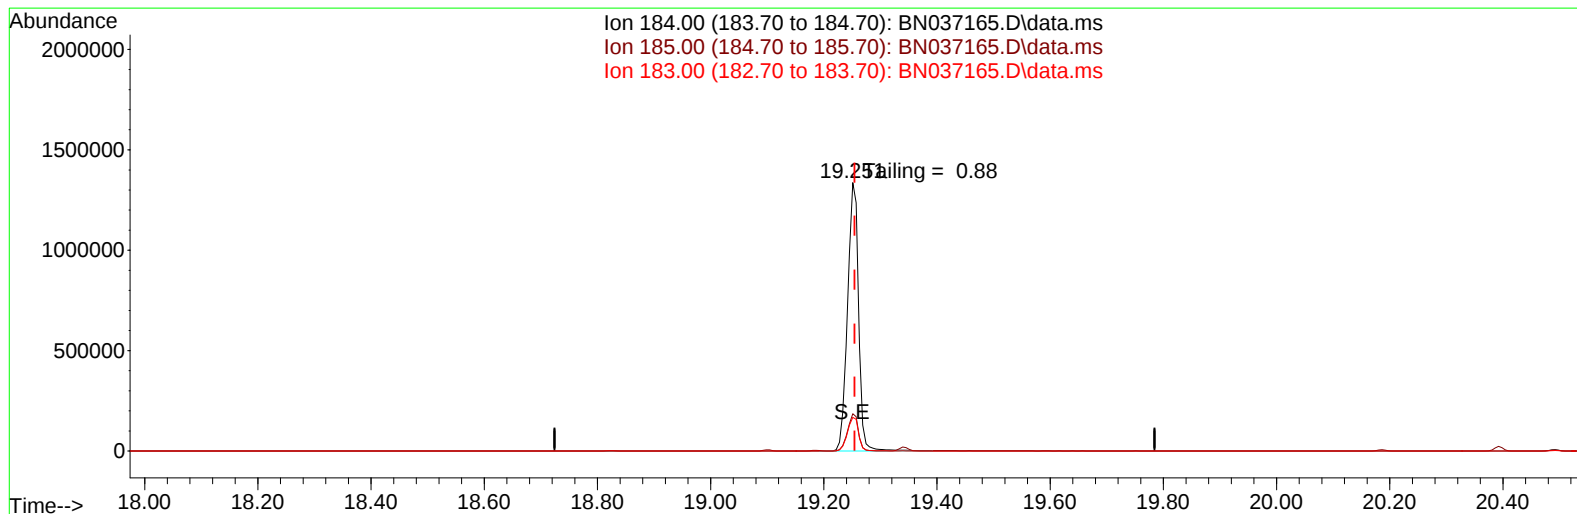

TIC: BN037165.D\data.ms

(77) Benzidine

19.251min (-0.003) 0.00 ng

response 1811758

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.92
183.00	13.20	12.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/4/2025	BNA_N	<u>BN037165.D</u>
Compound Name	Response	Retention Time
DDT	1237139	20.492
DDD	19824	20.098
DDE	602	19.539
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20426	1257565	1.62

Instrument :
BNA_N
ClientSampleId :
DFTPP