
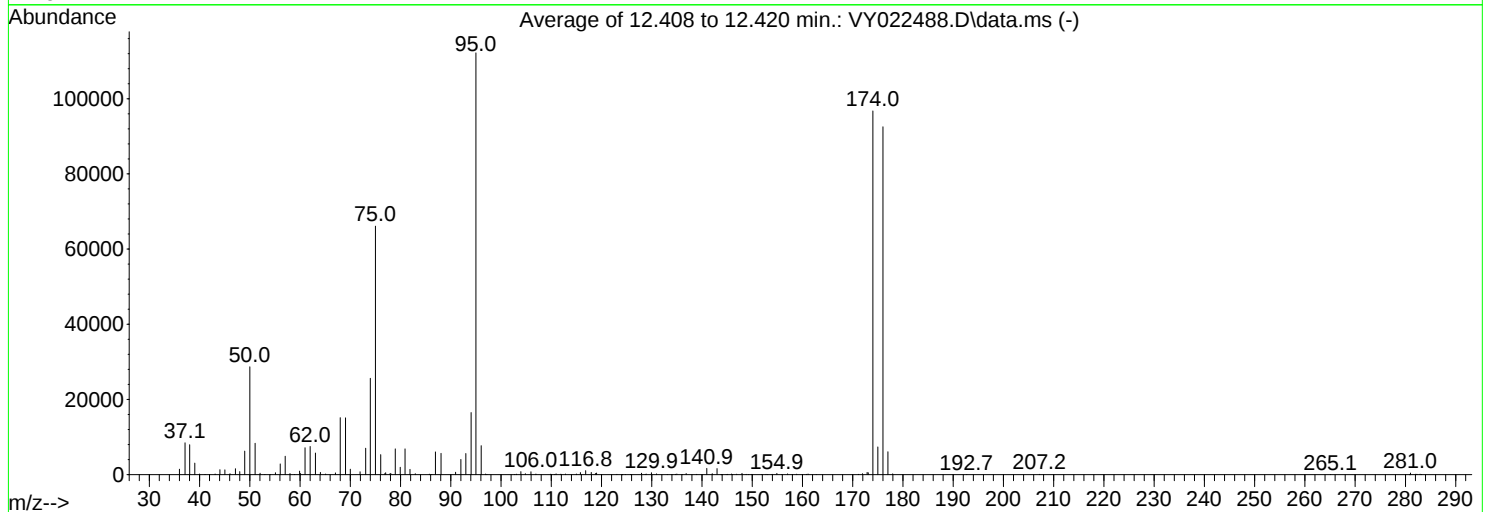


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060225\
Data File : VY022488.D
Acq On : 02 Jun 2025 08:31
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Title : SW846 8260
Last Update : Tue Jun 03 03:22:04 2025

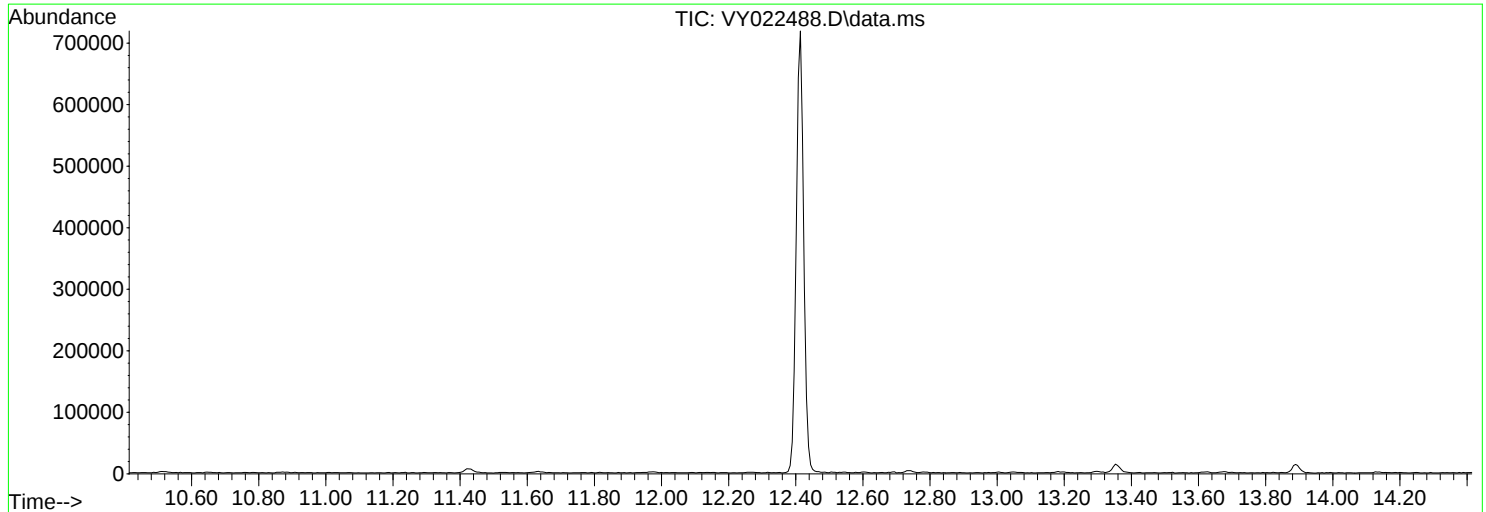

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	25.6	28688	PASS
75	95	30	60	58.9	66115	PASS
95	95	100	100	100.0	112208	PASS
96	95	5	9	6.9	7706	PASS
173	174	0.00	2	0.6	591	PASS
174	95	50	100	86.2	96760	PASS
175	174	5	9	7.6	7372	PASS
176	174	95	101	95.6	92520	PASS
177	176	5	9	6.6	6076	PASS