

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060325\
 Data File : PL095891.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2025 15:36
 Operator : AR\AJ
 Sample : Q2176-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-28

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 01:37:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
 Quant Title : GC Extractables
 QLast Update : Thu May 22 06:29:30 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.573	2.886	85533514	71309865	27.108	18.219 #
28)	SA Decachlor...	9.099	8.060	33392280	51917428	14.171	11.868
Target Compounds							
9)	A Endosulfan I	0.000	5.260f	0	10129882	N.D.	2.126 #
20)	A Methoxychlor	0.000	6.776f	0	7213538	N.D.	2.757 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL060325\
Data File : PL095891.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2025 15:36
Operator : AR\AJ
Sample : Q2176-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-28

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 01:37:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052125.M
Quant Title : GC Extractables
QLast Update : Thu May 22 06:29:30 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

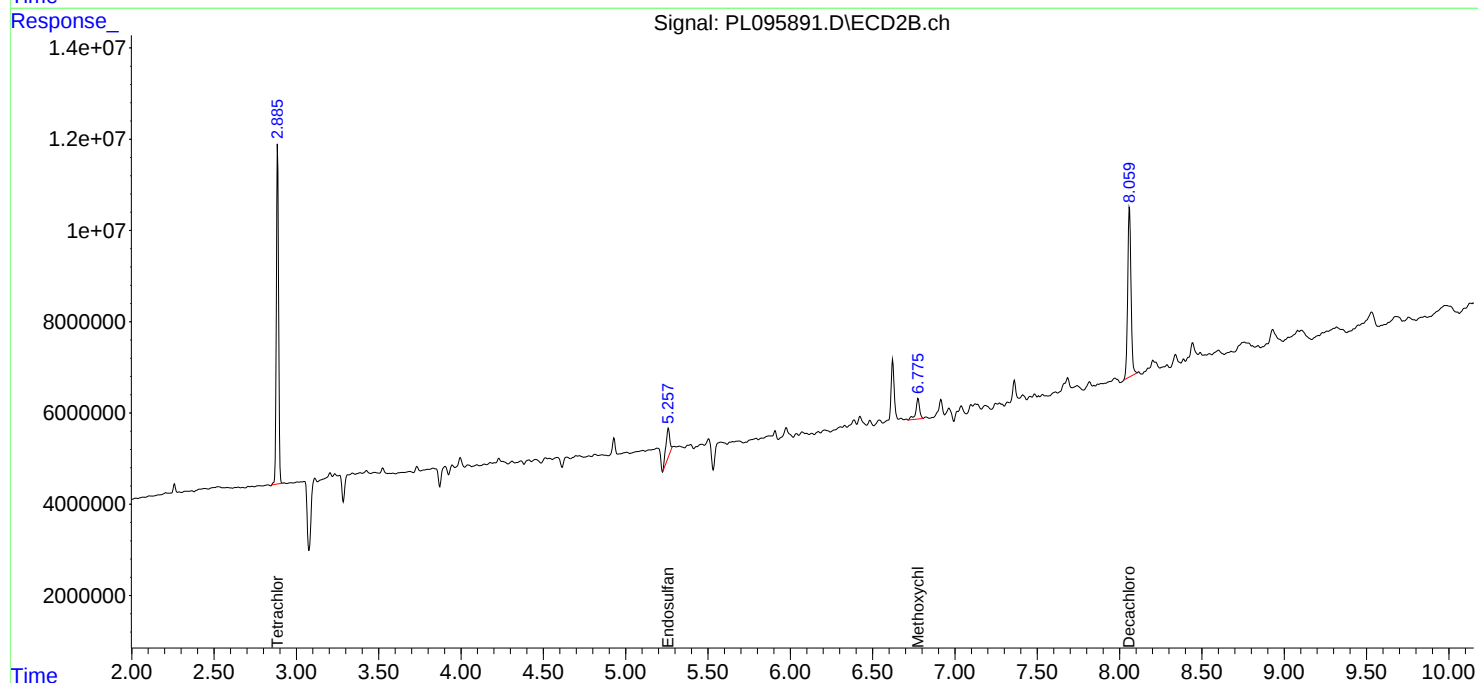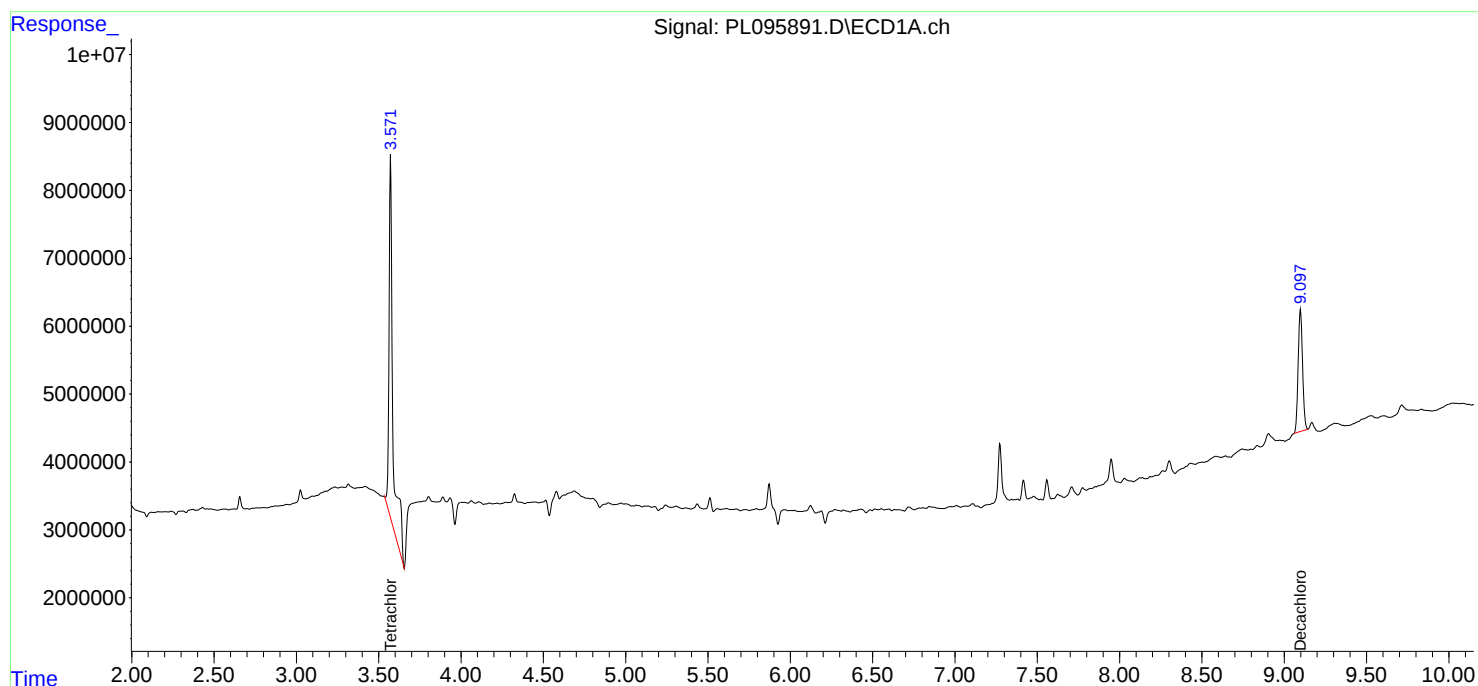


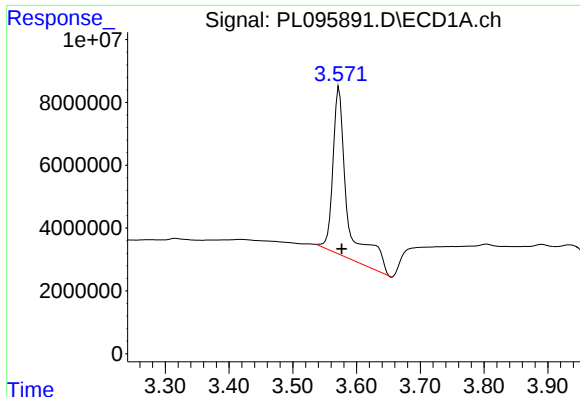

#1 Tetrachloro-m-xylene


R.T.: 3.573 min
Delta R.T.: -0.004 min
Response: 85533514
Conc: 27.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-28

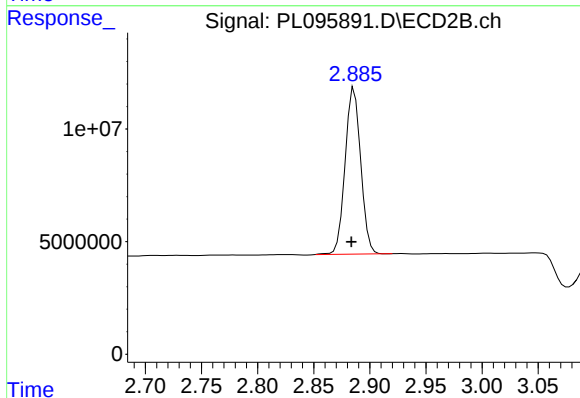


#1 Tetrachloro-m-xylene

R.T.: 2.886 min
Delta R.T.: 0.003 min
Response: 71309865
Conc: 18.22 ng/ml

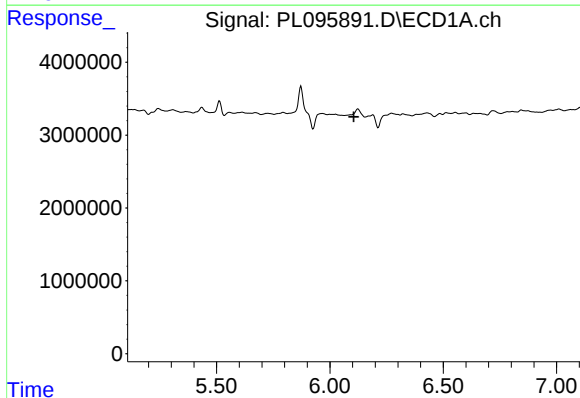


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.106 min
Response: 0
Conc: N.D.

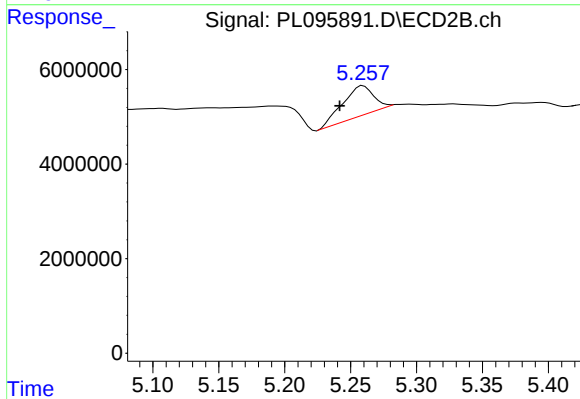

#9 Endosulfan I


R.T.: 5.260 min
Delta R.T.: 0.018 min
Response: 10129882
Conc: 2.13 ng/ml

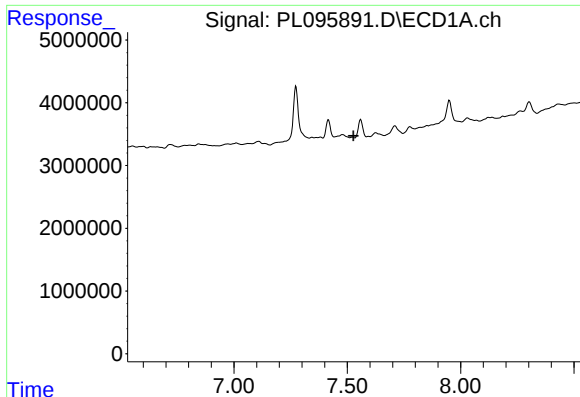

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-28

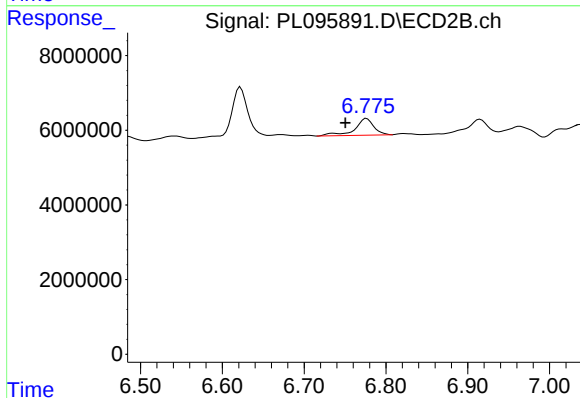


#20 Methoxychlor

R.T.: 6.776 min
Delta R.T.: 0.026 min
Response: 7213538
Conc: 2.76 ng/ml

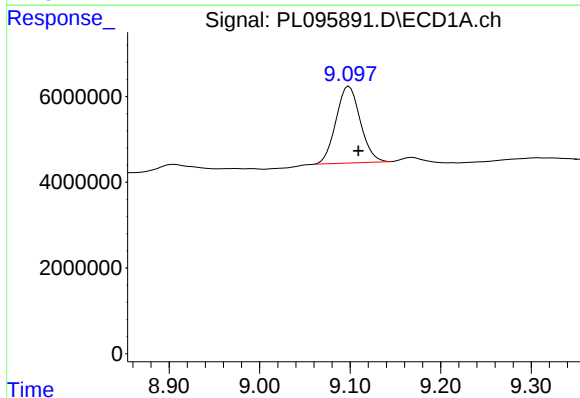

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.010 min
Response: 33392280
Conc: 14.17 ng/ml

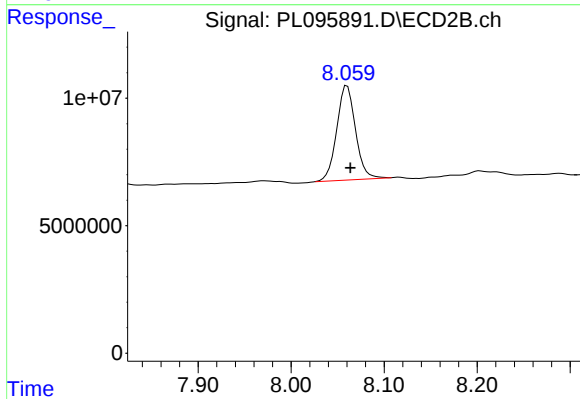

#28 Decachlorobiphenyl

R.T.: 8.060 min
Delta R.T.: -0.004 min
Response: 51917428
Conc: 11.87 ng/ml