
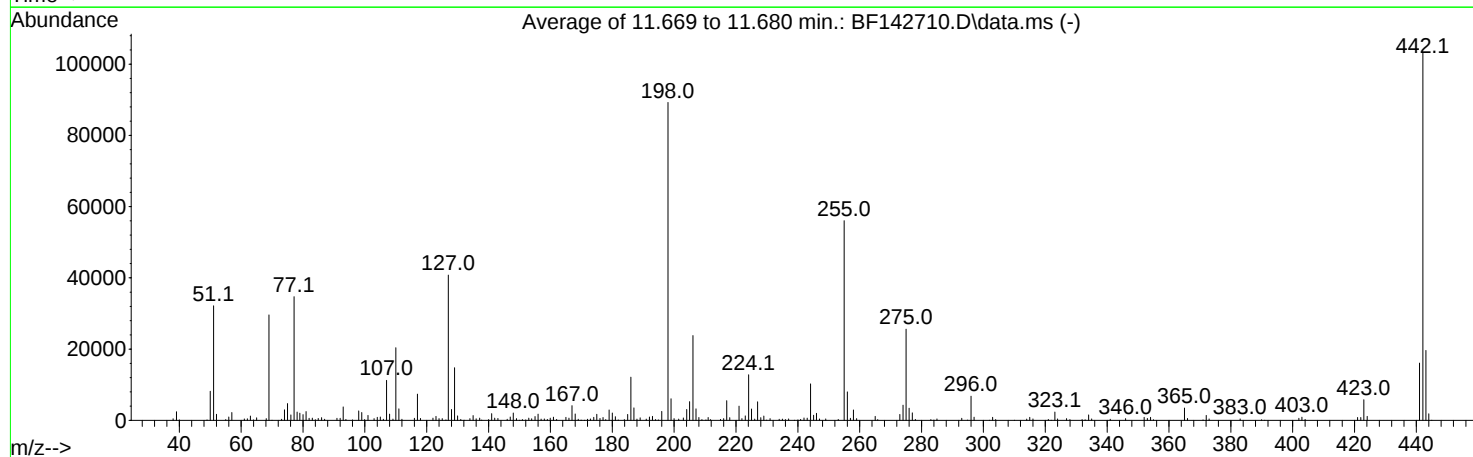


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061125\
Data File : BF142710.D
Acq On : 10 Jun 2025 15:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 11 05:56:09 2025

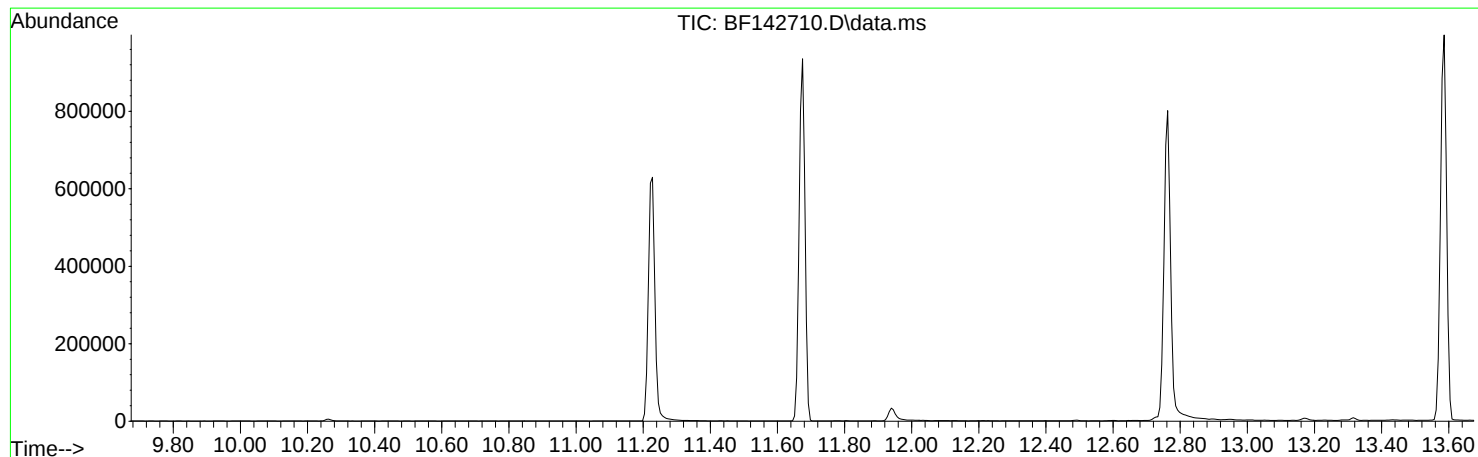

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	32160	PASS
68	69	0.00	2	1.7	514	PASS
69	198	0.00	100	33.2	29603	PASS
70	69	0.00	2	0.2	55	PASS
127	198	10	80	45.7	40781	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89240	PASS
199	198	5	9	6.8	6083	PASS
275	198	10	60	28.7	25613	PASS
365	198	1	100	3.9	3449	PASS
441	198	0.01	100	18.0	16079	PASS
442	442	50	100	100.0	103267	PASS
443	442	15	24	19.0	19634	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/11/2025	BNA_F	<u>BF142710.D</u>
Compound Name	Response	Retention Time
DDT	258255	13.586
DDD	3816	13.316
DDE	597	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4413	262668	1.68

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061125\
Data File : BF142710.D
Acq On : 10 Jun 2025 15:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 11 06:08:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

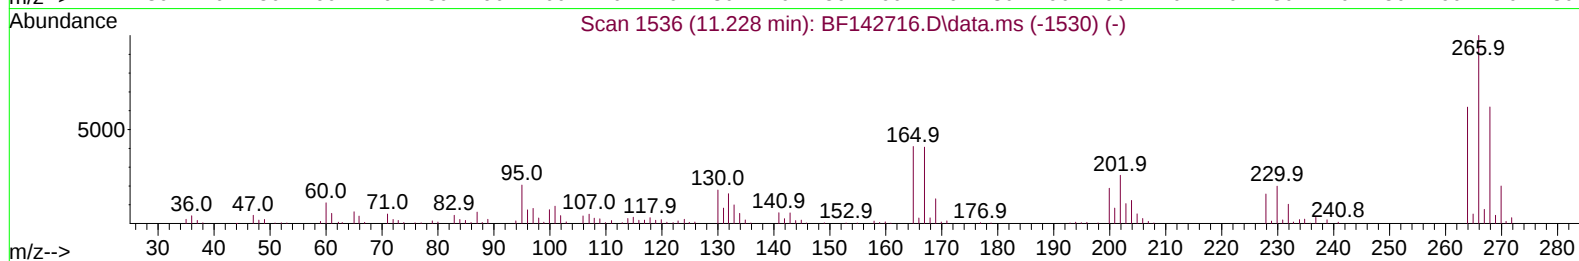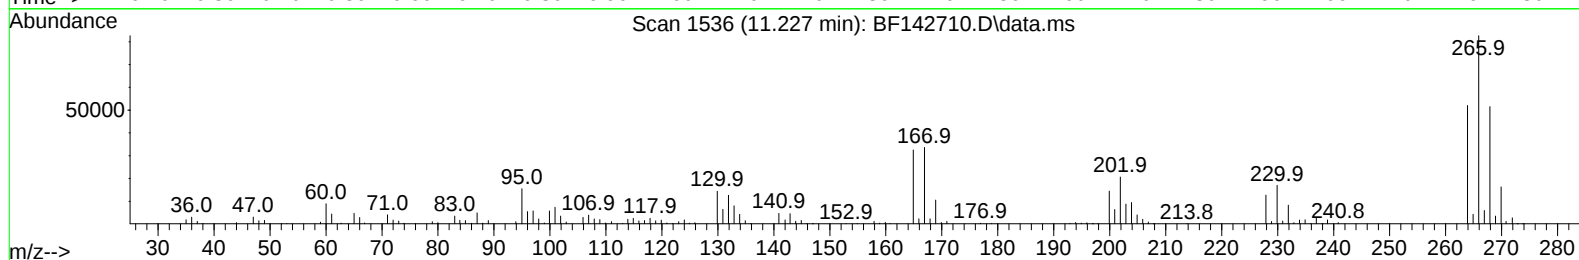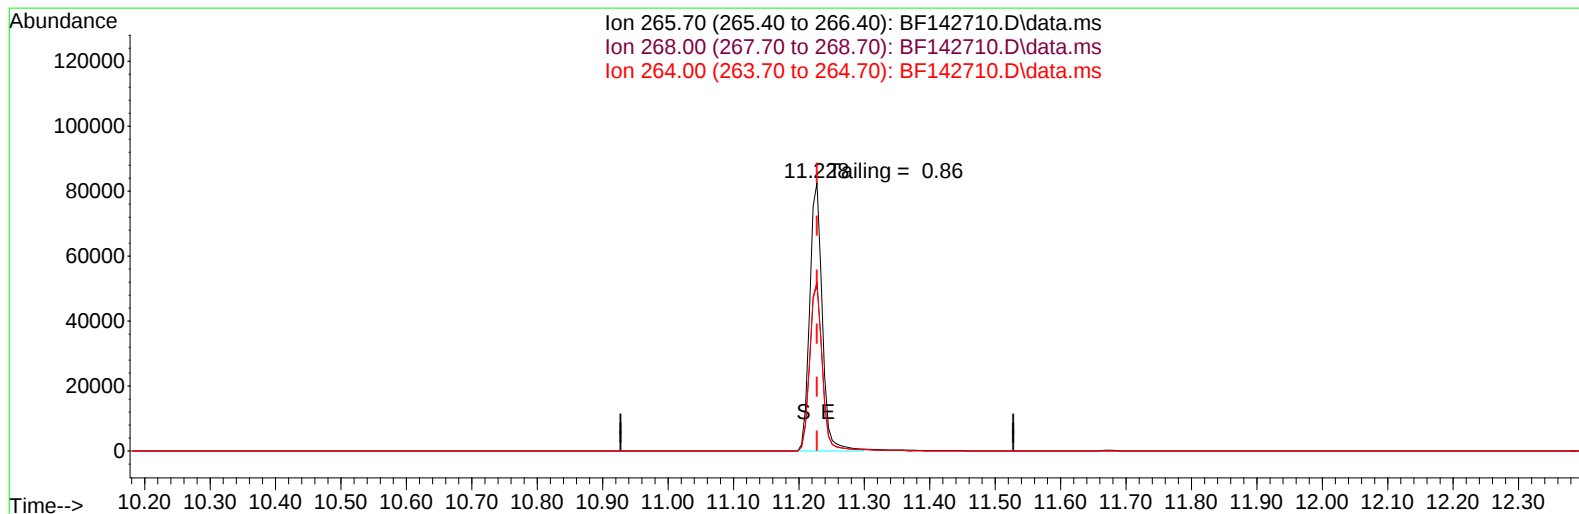

TIC: BF142710.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 33796.57 ng




response 112116

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.00	62.35
264.00	61.90	62.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061125\
Data File : BF142710.D
Acq On : 10 Jun 2025 15:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 11 06:08:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

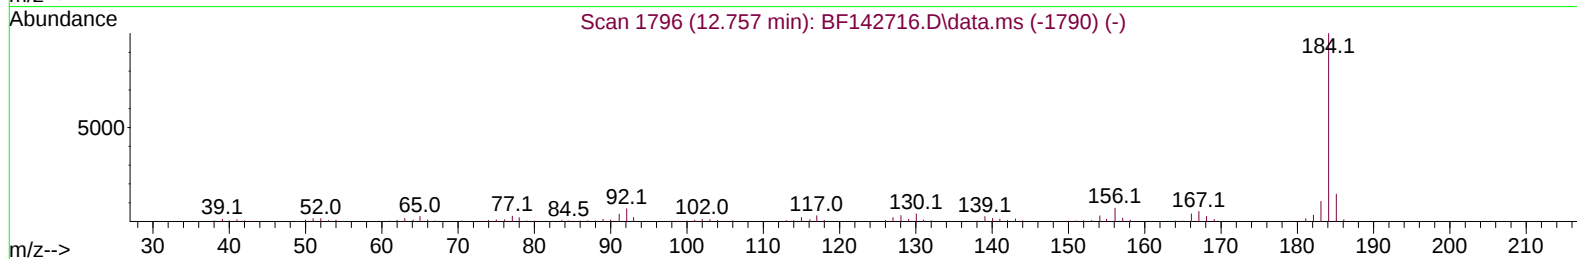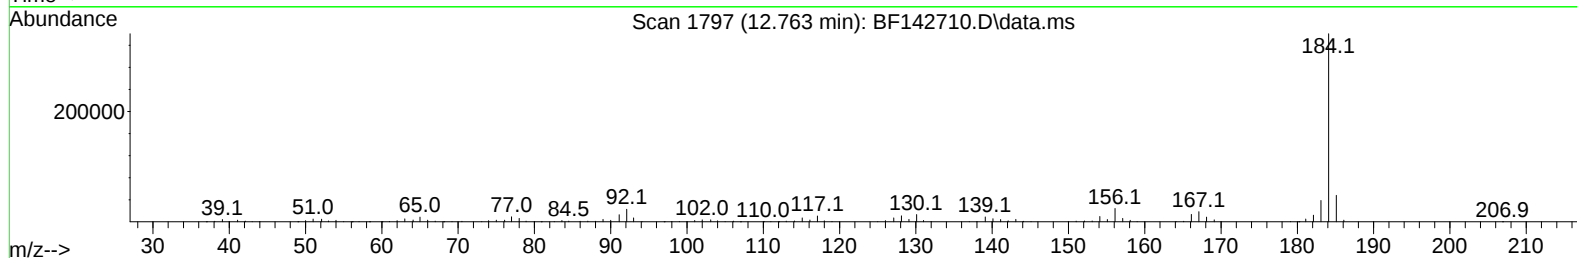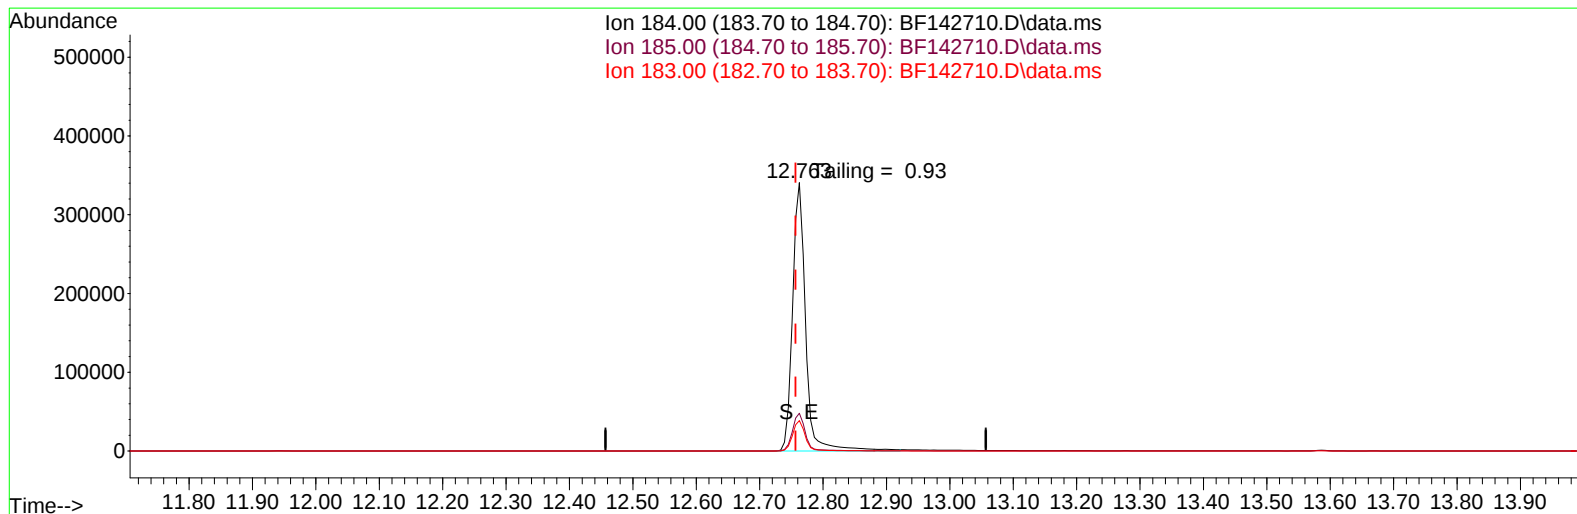

TIC: BF142710.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng

response 494727

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.07
183.00	10.70	11.33
0.00	0.00	0.00