
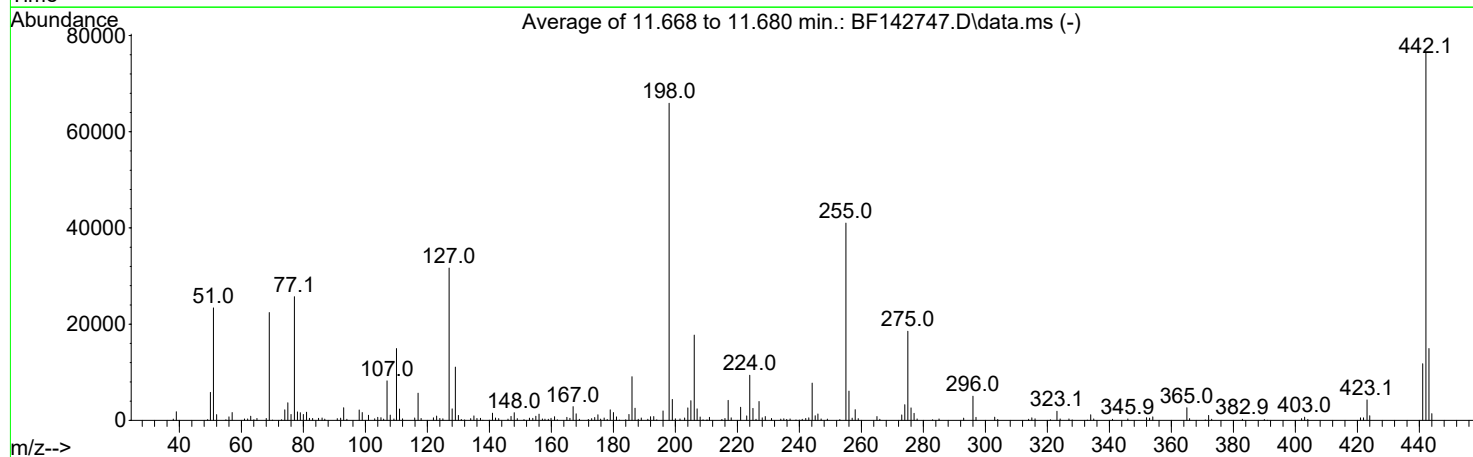


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
Data File : BF142747.D
Acq On : 12 Jun 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 11 05:56:09 2025

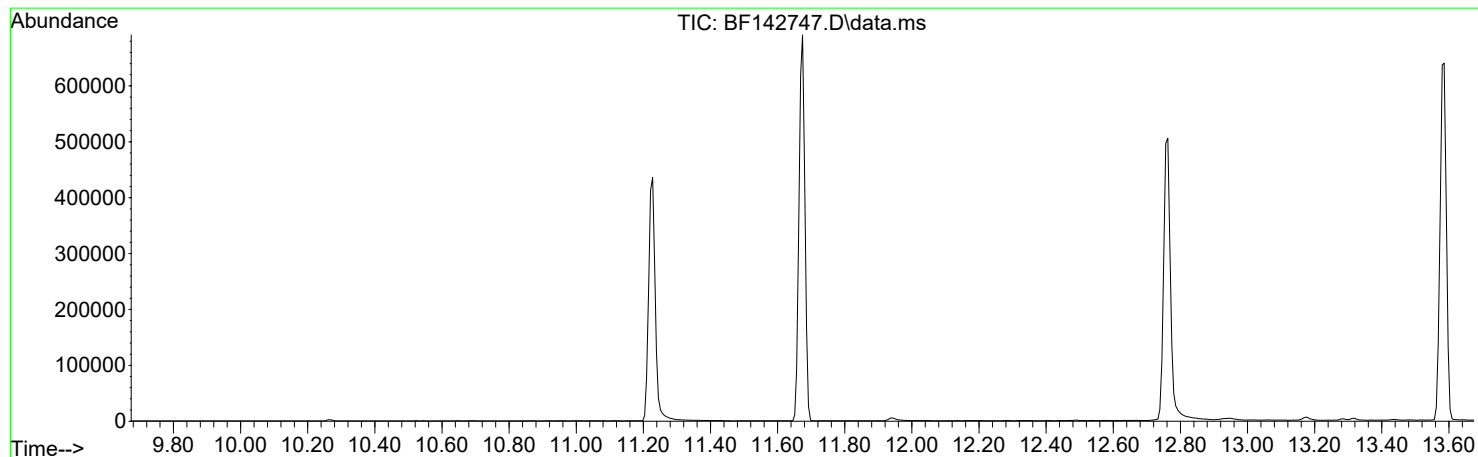

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	23396	PASS
68	69	0.00	2	1.8	411	PASS
69	198	0.00	100	34.0	22436	PASS
70	69	0.00	2	0.2	55	PASS
127	198	10	80	48.0	31656	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65912	PASS
199	198	5	9	6.6	4373	PASS
275	198	10	60	28.1	18539	PASS
365	198	1	100	4.0	2616	PASS
441	198	0.01	100	17.8	11765	PASS
442	442	50	100	100.0	76475	PASS
443	442	15	24	19.5	14940	PASS

DDT Breakdown



Date	Instrument Name	DFTPP Data File
6/12/2025	BNA_F	<u>BF142747.D</u>
Compound Name	Response	Retention Time
DDT	171550	13.586
DDD	3049	13.315
DDE	593	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3642	175192	2.08

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
Data File : BF142747.D
Acq On : 12 Jun 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 12 11:59:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

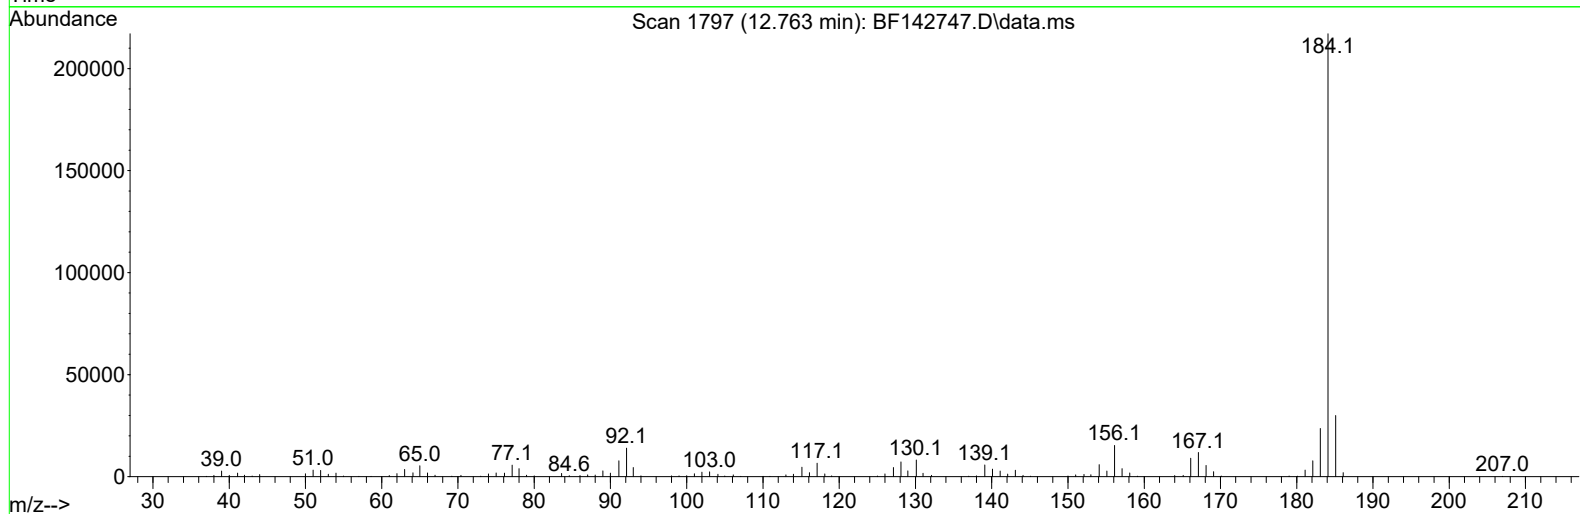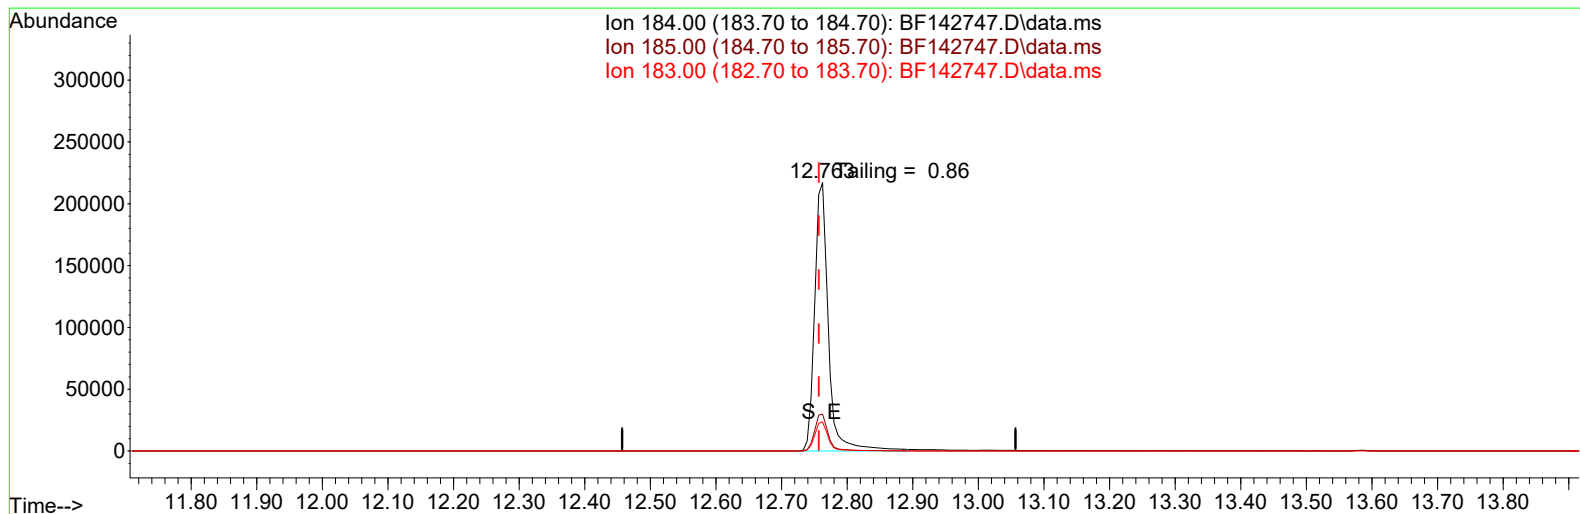

TIC: BF142747.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng



response 319051

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.81
183.00	10.70	10.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061225\
Data File : BF142747.D
Acq On : 12 Jun 2025 09:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 12 11:59:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

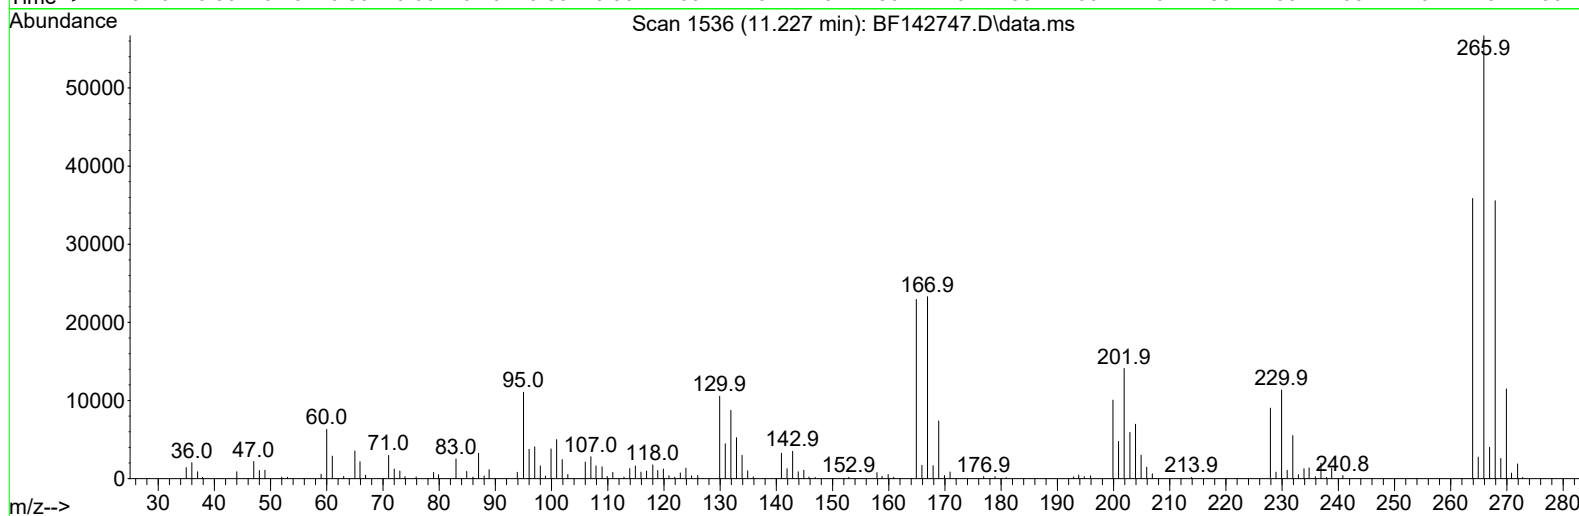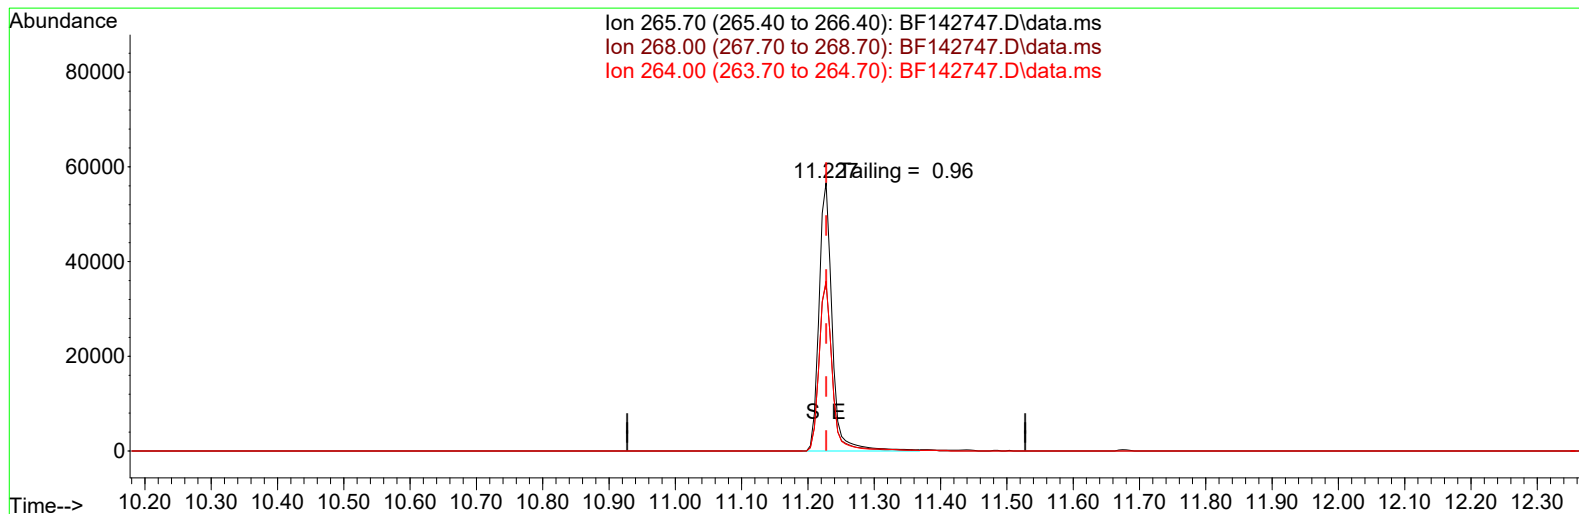

TIC: BF142747.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 48564.59 ng

response 78719

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.00	62.77
264.00	61.90	63.25
0.00	0.00	0.00