
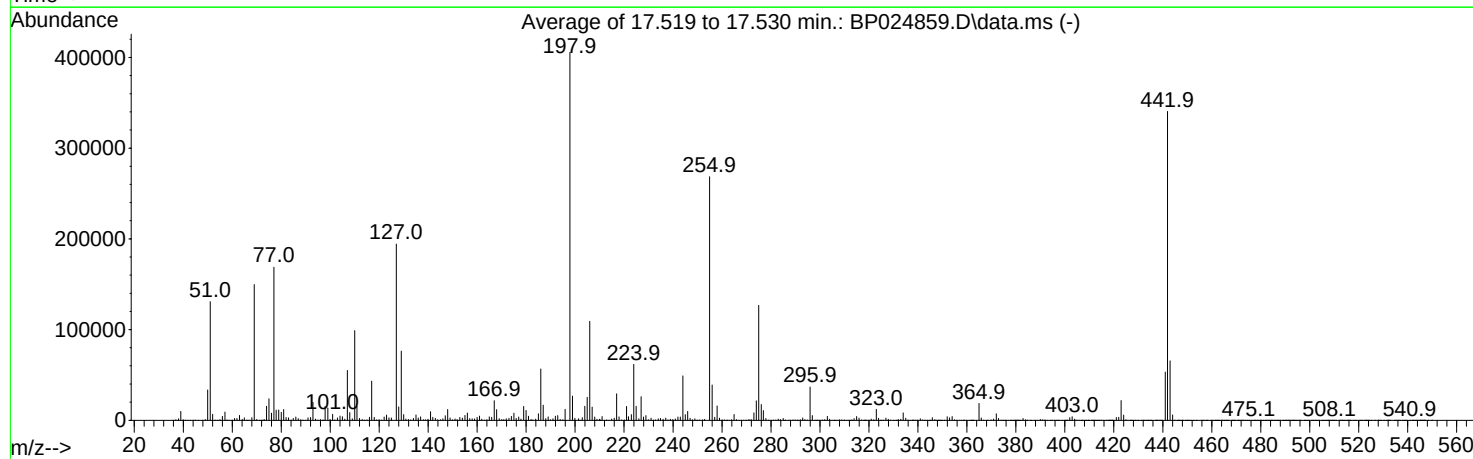


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060625\
Data File : BP024859.D
Acq On : 06 Jun 2025 09:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 06 16:20:27 2025

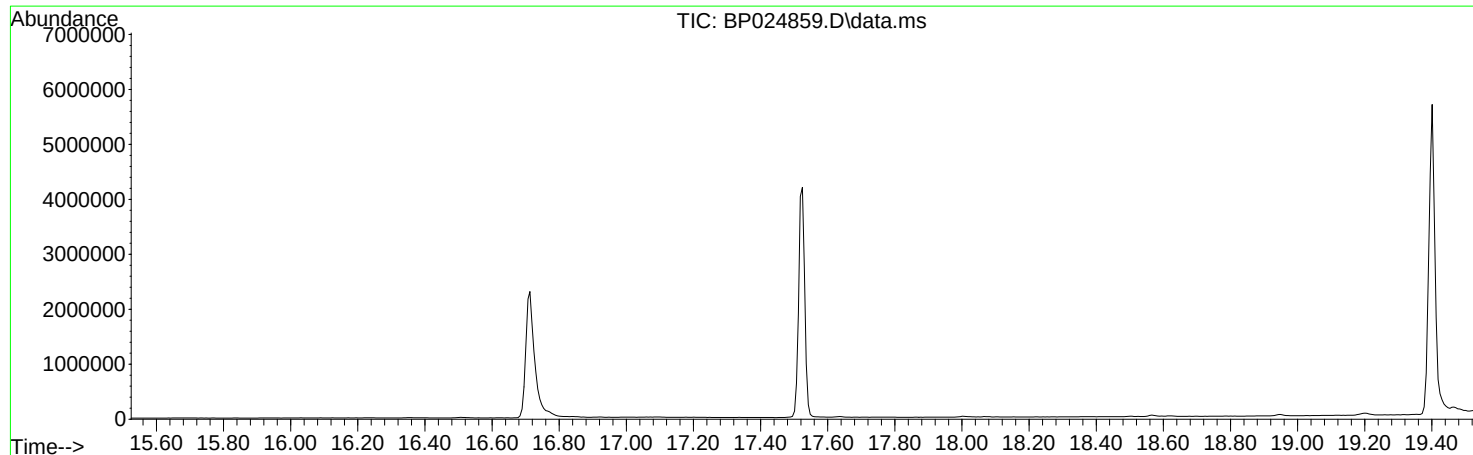




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	130762	PASS
68	69	0.00	2	1.9	2882	PASS
69	198	0.00	100	36.9	149759	PASS
70	69	0.00	2	0.6	956	PASS
127	198	10	80	47.9	194356	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	405520	PASS
199	198	5	9	6.6	26790	PASS
275	198	10	60	31.2	126715	PASS
365	198	1	100	4.6	18586	PASS
441	198	0.01	100	13.1	53196	PASS
442	442	100	100	100.0	340484	PASS
443	442	15	24	19.2	65481	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060625\
Data File : BP024859.D
Acq On : 06 Jun 2025 09:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 06 16:23:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

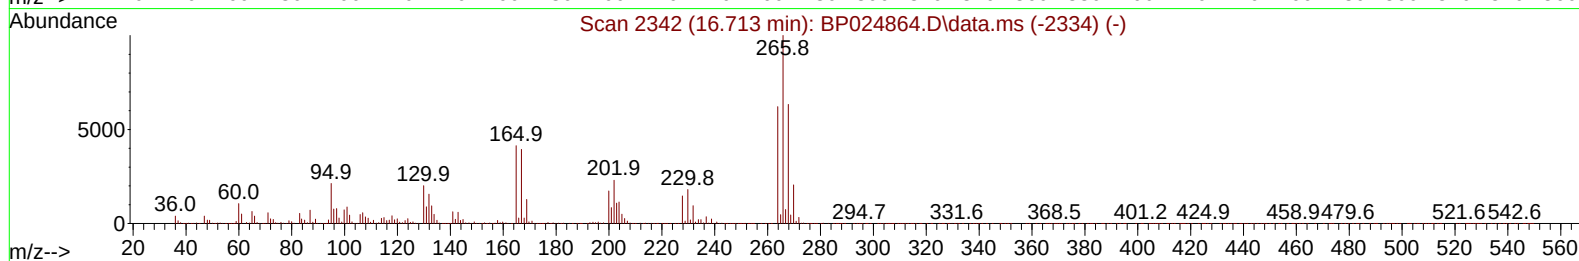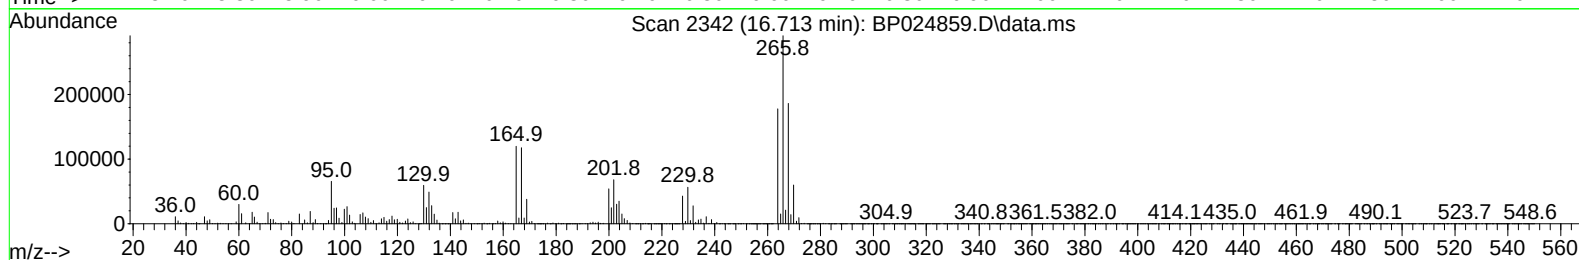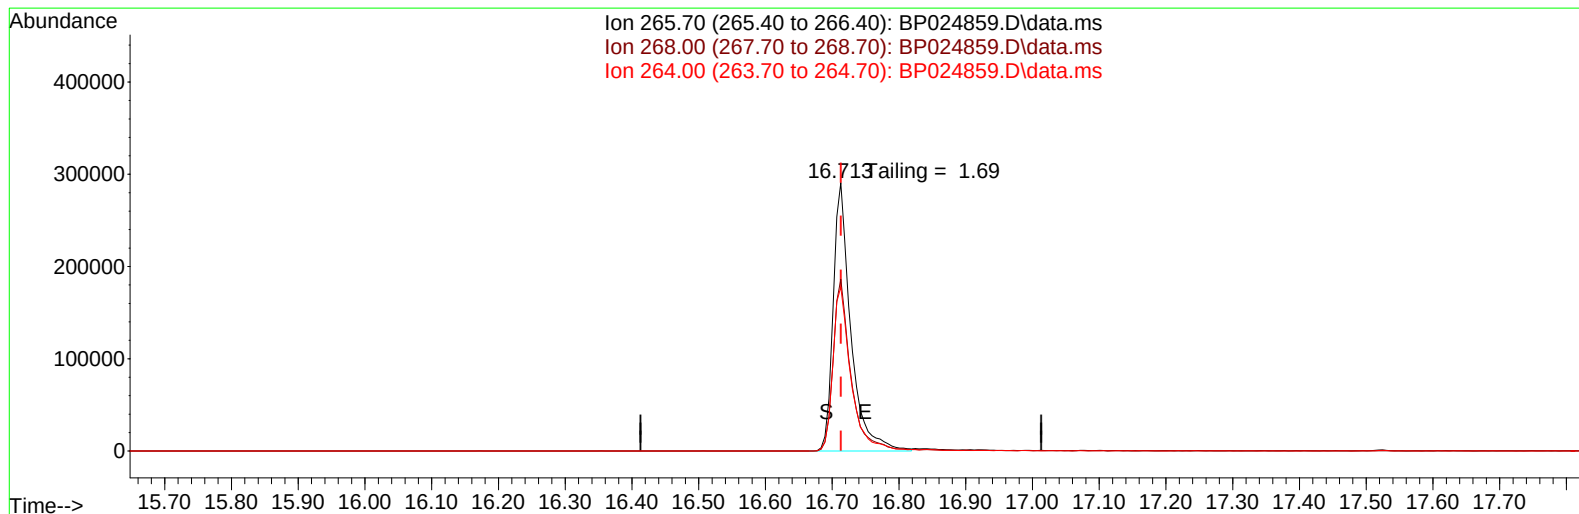

TIC: BP024859.D\data.ms

(70) Pentachlorophenol (C)

16.713min (-0.000) 25022.31 ng




response 535499

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.99
264.00	62.10	61.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060625\
Data File : BP024859.D
Acq On : 06 Jun 2025 09:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 06 16:23:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

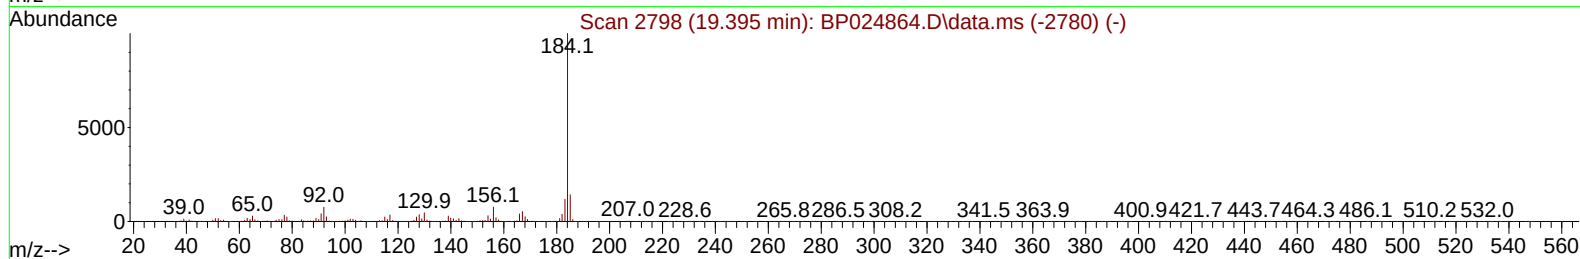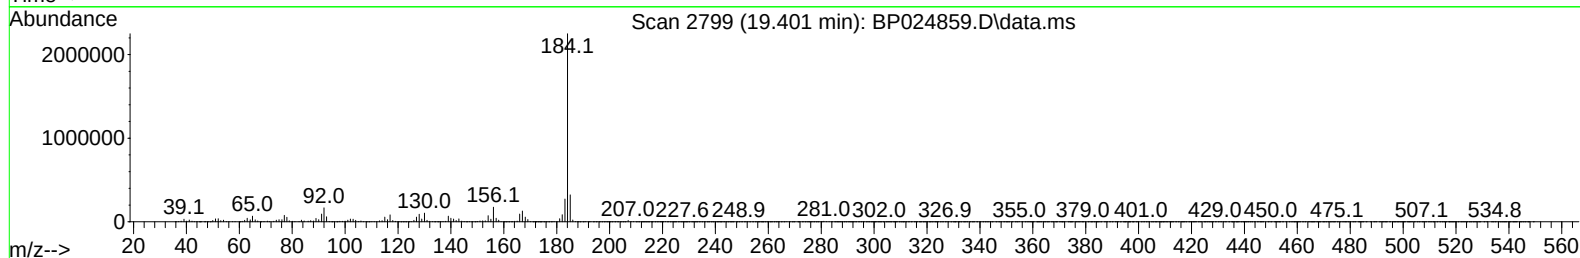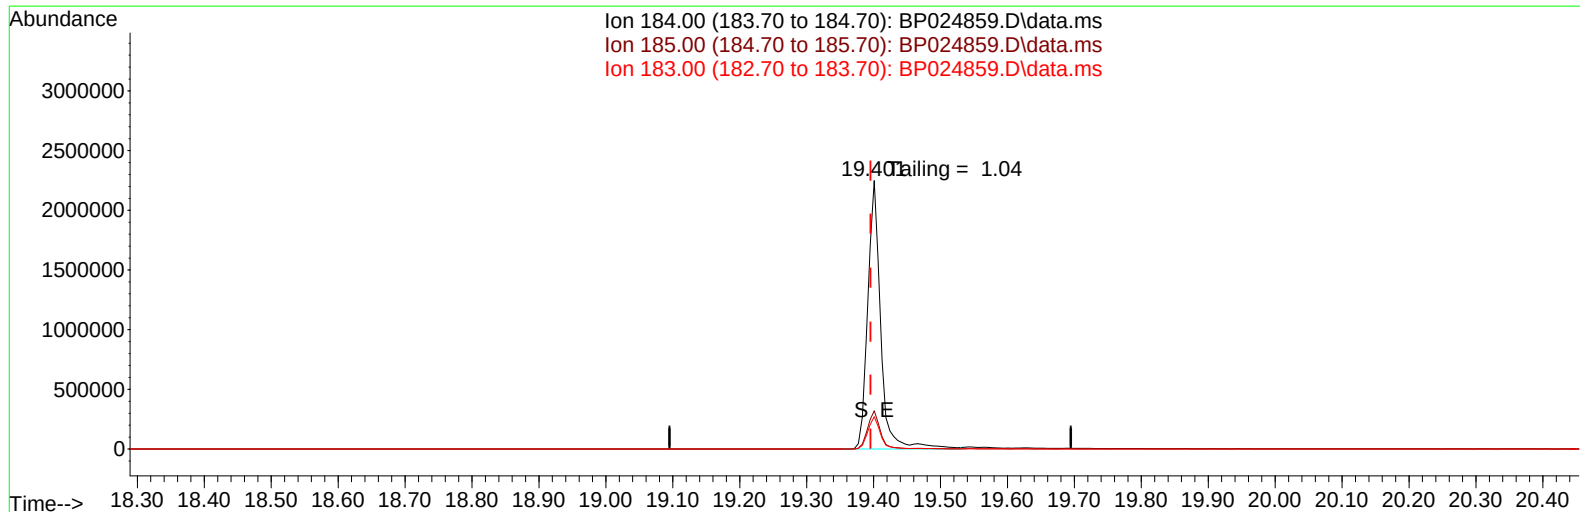

TIC: BP024859.D\data.ms

(77) Benzidine

19.401min (+ 0.006) 4191.40 ng

response 2912892

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.27
183.00	11.90	12.06
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/6/2025	BNA_P	<u>BP024859.D</u>
Compound Name	Response	Retention Time
DDT	1572545	20.677
DDD	21912	20.26
DDE	1833	19.695
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23745	1596290	1.49

Instrument :
BNA_P
ClientSampleId :
DFTPP