
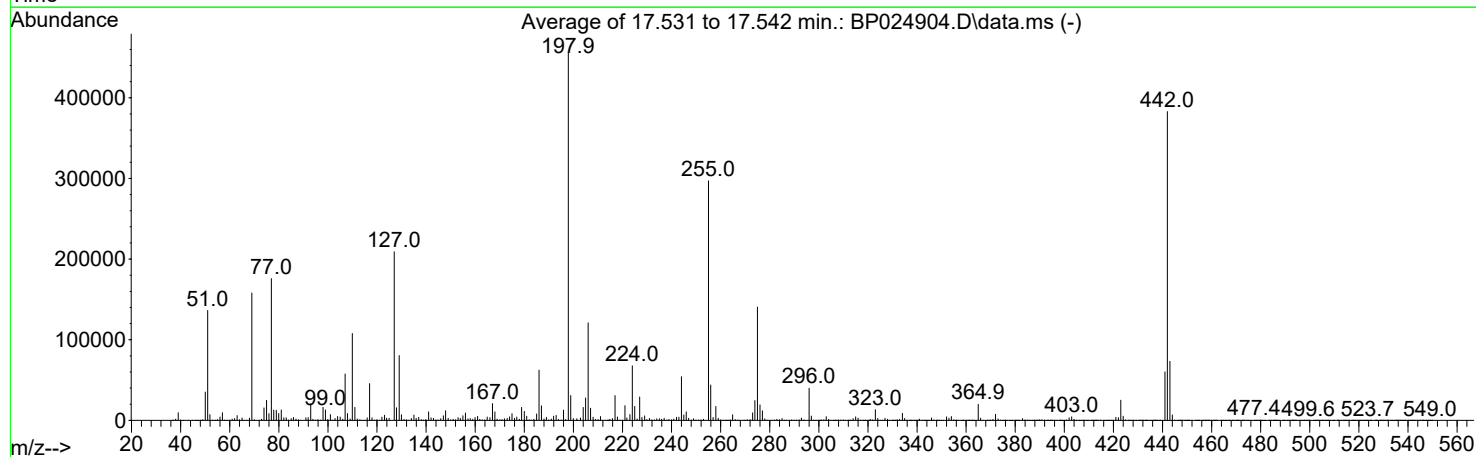


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061125\
Data File : BP024904.D
Acq On : 11 Jun 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 06 16:20:27 2025

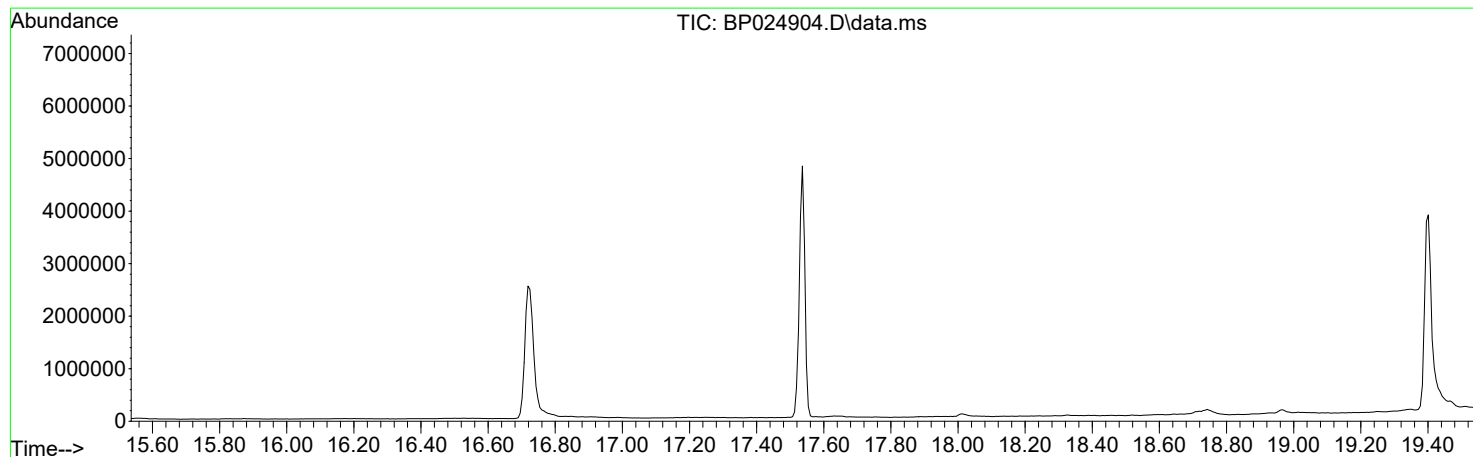

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	136312	PASS
68	69	0.00	2	1.8	2821	PASS
69	198	0.00	100	34.6	157942	PASS
70	69	0.00	2	0.5	729	PASS
127	198	10	80	45.8	209121	PASS
197	198	0.00	2	0.2	948	PASS
198	198	100	100	100.0	456177	PASS
199	198	5	9	6.7	30695	PASS
275	198	10	60	30.8	140518	PASS
365	198	1	100	4.4	19899	PASS
441	198	0.01	100	13.2	60071	PASS
442	442	100	100	100.0	383019	PASS
443	442	15	24	19.1	73251	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/11/2025	BNA_P	<u>BP024904.D</u>
Compound Name	Response	Retention Time
DDT	1545458	20.683
DDD	50136	20.236
DDE	2461	19.701
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
52597	1598055	3.29

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061125\
Data File : BP024904.D
Acq On : 11 Jun 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 11 10:56:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

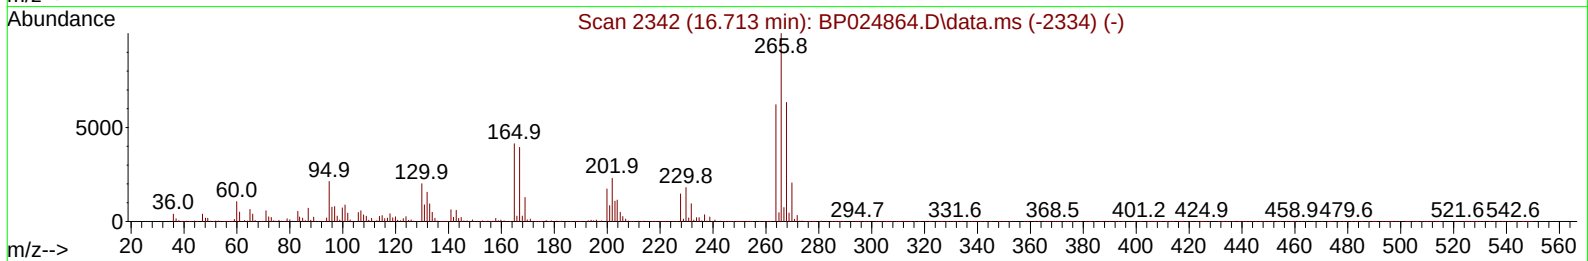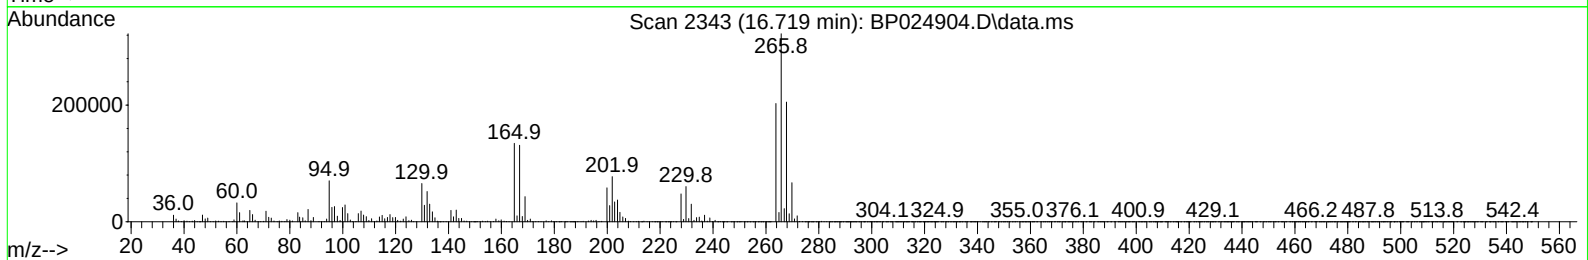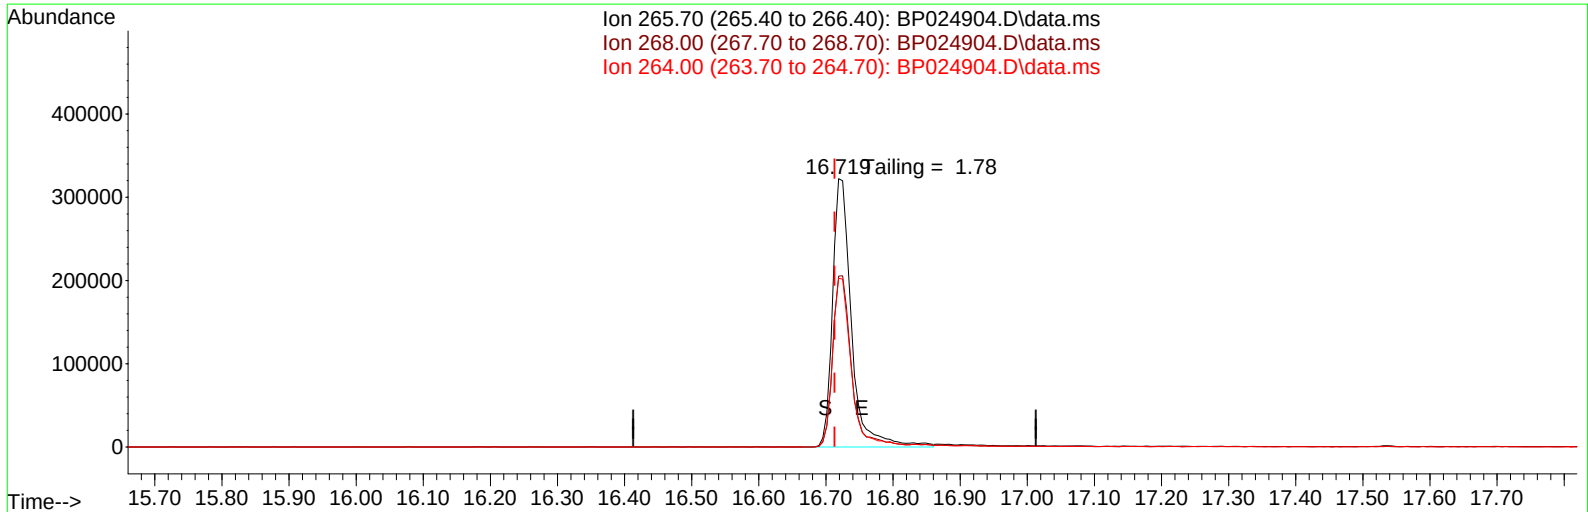

TIC: BP024904.D\data.ms

(70) Pentachlorophenol (C)

16.719min (+ 0.006) 642668.97 ng




response 532312

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.68
264.00	62.10	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061125\
Data File : BP024904.D
Acq On : 11 Jun 2025 09:29
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 11 10:56:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

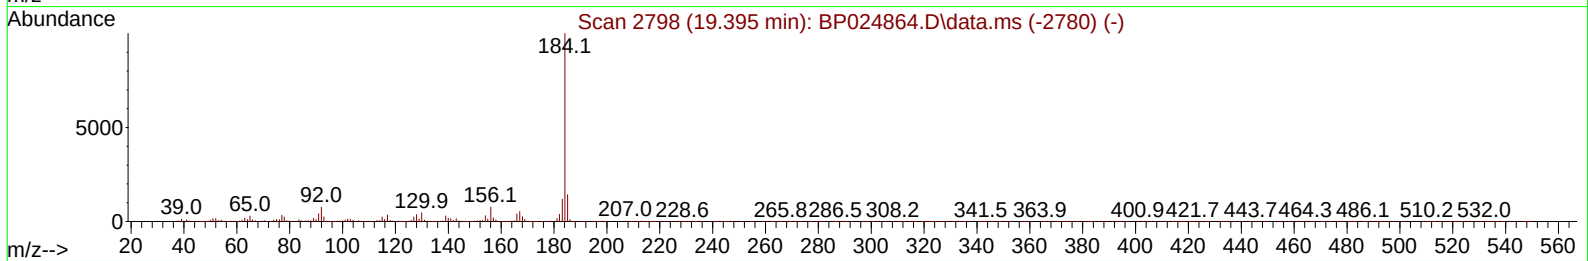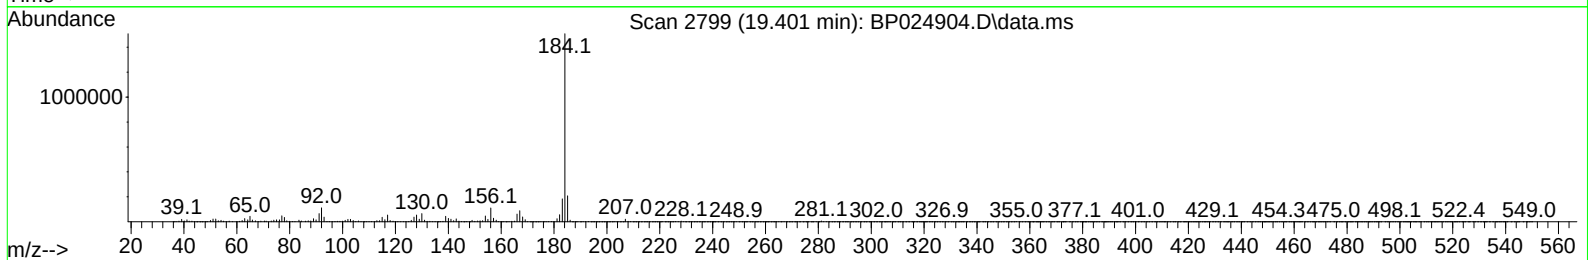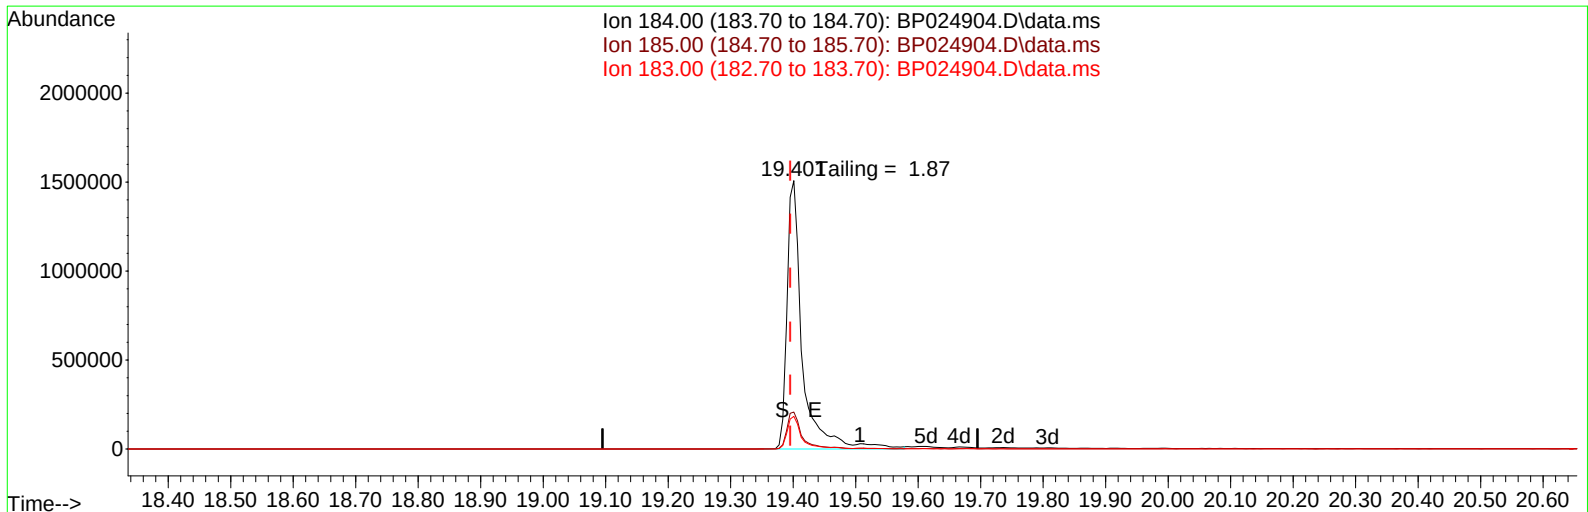

TIC: BP024904.D\data.ms

(77) Benzidine

19.401min (+ 0.006) 505291.00 ng m

response 2629132

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.77
183.00	11.90	12.20
0.00	0.00	0.00