

LB135995 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 04 Jun 2025 09:44:10


Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	9	-	0.0000	7470A	PPB	04 Jun 2025 10:02:01	S	Std
0.2 - 1	50.2	1061	-	0.2000	7470A	PPB	04 Jun 2025 10:04:17	S	Std
2.5 - 1	52.5	11354	-	2.5000	7470A	PPB	04 Jun 2025 10:06:34	S	Std
5.0 - 1	55	21246	-	5.0000	7470A	PPB	04 Jun 2025 10:08:51	S	Std
7.5 - 1	57.5	33122	-	7.5000	7470A	PPB	04 Jun 2025 10:11:10	S	Std
10.0 - 1	59	43131	-	10.0000	7470A	PPB	04 Jun 2025 10:13:30	S	Std
ICV26 - 1	ICV26	17171	3.9340	-	7470A	PPB	04 Jun 2025 10:25:12	U	SMPL
ICB26 - 1	ICB26	-162	-0.0769	-	7470A	PPB	04 Jun 2025 10:30:10	U	SMPL
CCV95 - 1	CCV95	21160	4.8571	-	7470A	PPB	04 Jun 2025 10:32:25	U	SMPL
CCB95 - 1	CCB95	-128	-0.0690	-	7470A	PPB	04 Jun 2025 10:34:40	U	SMPL
CRA - 1	CRA	1129	0.2218	-	7470A	PPB	04 Jun 2025 10:36:59	U	SMPL
HighStd - 1	HighStd	41519	9.5682	-	7470A	PPB	04 Jun 2025 10:39:14	U	SMPL
ChkStd - 1	ChkStd	28374	6.5264	-	7470A	PPB	04 Jun 2025 10:41:30	U	SMPL
PB168262BL - 1	PBW	20	-0.0348	-	7470A	PPB	04 Jun 2025 10:43:52	U	SMPL
PB168262BS - 1	LCSW	15662	3.5848	-	7470A	PPB	04 Jun 2025 10:48:21	U	SMPL
Q2159-04 - 1	TP05-MHO-WC	127	-0.0100	-	7470A	PPB	04 Jun 2025 10:50:37	U	SMPL
Q2160-04 - 1	TP04-MHG-WC	401	0.0534	-	7470A	PPB	04 Jun 2025 10:53:06	U	SMPL
Q2160-08 - 1	TP05-MHH-WC	409	0.0552	-	7470A	PPB	04 Jun 2025 10:55:23	U	SMPL
Q2168-02 - 1	SAN-A1-A3	531	0.0835	-	7470A	PPB	04 Jun 2025 10:57:40	U	SMPL
Q2168-06 - 1	SAN-B1-B3	530	0.0832	-	7470A	PPB	04 Jun 2025 10:59:55	U	SMPL
CCV96 - 1	CCV96	21021	4.8249	-	7470A	PPB	04 Jun 2025 11:02:12	U	SMPL
CCB96 - 1	CCB96	76	-0.0218	-	7470A	PPB	04 Jun 2025 11:04:27	U	SMPL
Q2168-10 - 1	SAN-C1-C2	796	0.1448	-	7470A	PPB	04 Jun 2025 11:06:46	U	SMPL
Q2172-04 - 1	TP06-MHQ	553	0.0885	-	7470A	PPB	04 Jun 2025 11:09:01	U	SMPL
Q2173-06 - 1	OR-400-CF-402B-COMP-23	809	0.1478	-	7470A	PPB	04 Jun 2025 11:11:18	U	SMPL
Q2173-12 - 1	OR-400-CF-402B-COMP-24	674	0.1165	-	7470A	PPB	04 Jun 2025 11:13:33	U	SMPL
Q2173-18 - 1	OR-400-CF-402B-COMP-25	592	0.0976	-	7470A	PPB	04 Jun 2025 11:15:49	U	SMPL
Q2177-03 - 1	B-187-SB01	461	0.0673	-	7470A	PPB	04 Jun 2025 11:18:05	U	SMPL
Q2177-05 - 1	B-187-SB02	337	0.0386	-	7470A	PPB	04 Jun 2025 11:20:22	U	SMPL
Q2177-07 - 1	B-202-SB01	308	0.0318	-	7470A	PPB	04 Jun 2025 11:22:38	U	SMPL
Q2185-04 - 1	TP02-MHB-WC	33	-0.0318	-	7470A	PPB	04 Jun 2025 11:24:55	U	SMPL
Q2185-08 - 1	TP01-MHB-WC	-37	-0.0480	-	7470A	PPB	04 Jun 2025 11:27:11	U	SMPL
CCV97 - 1	CCV97	20709	4.7527	-	7470A	PPB	04 Jun 2025 11:29:27	U	SMPL
CCB97 - 1	CCB97	173	0.0006	-	7470A	PPB	04 Jun 2025 11:31:42	U	SMPL
Q2185-08DUP - 1	TP01-MHB-WCDUP	393	0.0515	-	7470A	PPB	04 Jun 2025 11:34:01	U	SMPL
Q2185-08MS - 1	TP01-MHB-WCMS	18021	4.1307	-	7470A	PPB	04 Jun 2025 11:38:56	U	SMPL
Q2185-08MSD - 1	TP01-MHB-WCMSD	17438	3.9958	-	7470A	PPB	04 Jun 2025 11:41:13	U	SMPL
PB168224TB - 1		-54	-0.0519	-	7470A	PPB	04 Jun 2025 11:43:33	U	SMPL
Q2185-08LX5 - 1		38	-0.0306	-	7470A	PPB	04 Jun 2025 11:45:53	U	SMPL
Q2185-08A - 1		16845	3.8586	-	7470A	PPB	04 Jun 2025 11:48:10	U	SMPL
CCV98 - 1	CCV98	20300	4.6581	-	7470A	PPB	04 Jun 2025 11:53:09	U	SMPL
CCB98 - 1	CCB98	42	-0.0297	-	7470A	PPB	04 Jun 2025 11:55:27	U	SMPL

LB135995

7470A

INSTRUMENT ID: CV1

Linear

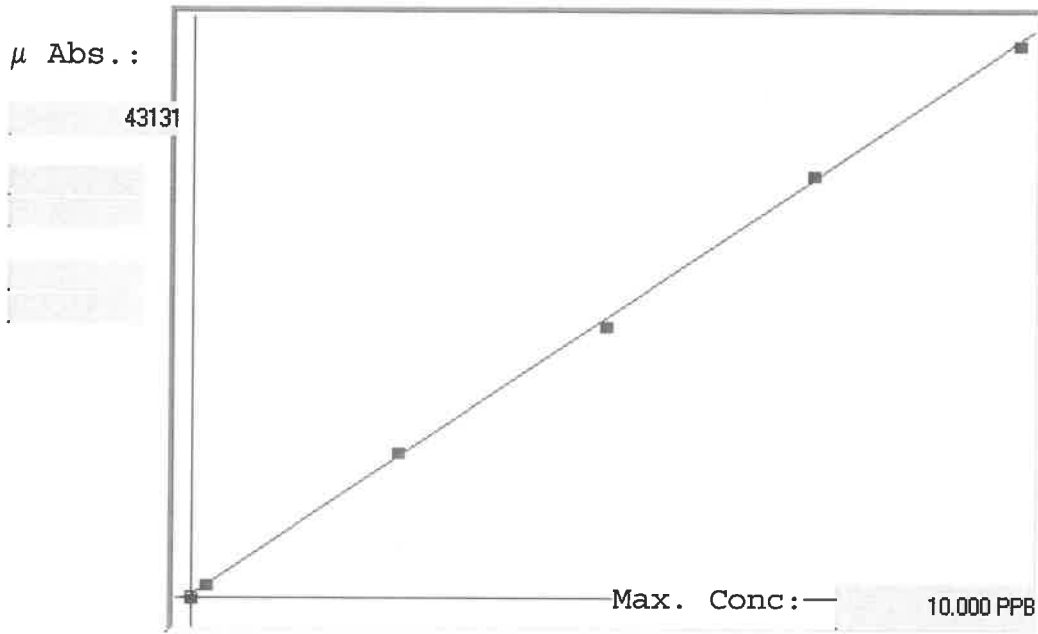

A= 0.0000e+000
B= 2.3140e-004
C= -3.9425e-002
Rho= 0.9997343
Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/2)
0.0	0.000	-0.037	-0.037	9	0.000	9	0				1
0.2	0.200	0.206	0.006	1061	0.0 %	1061					3
2.5	2.500	2.588	0.088	11354	0.0 %	11354					4
5.0	5.000	4.877	-0.123	21246	0.0 %	21246					2
7.5	7.500	7.625	0.125	33122	0.0 %	33122					2
10.0	10.000	9.941	-0.059	43131	0.0 %	43131					2