

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060325\
 Data File : PP072581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2025 20:48
 Operator : YP\AJ
 Sample : Q2177-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 B-202-SB01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/04/2025
 Supervised By :mohammad ahmed 06/05/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 01:38:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.502	3.795	41161641	38502501	20.470m	24.089
2) SA Decachlor...	10.200	8.810	30482591	23027738	18.711m	21.753m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060325\
Data File : PP072581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2025 20:48
Operator : YP\AJ
Sample : Q2177-06
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
B-202-SB01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/04/2025
Supervised By :mohammad ahmed 06/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 01:38:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

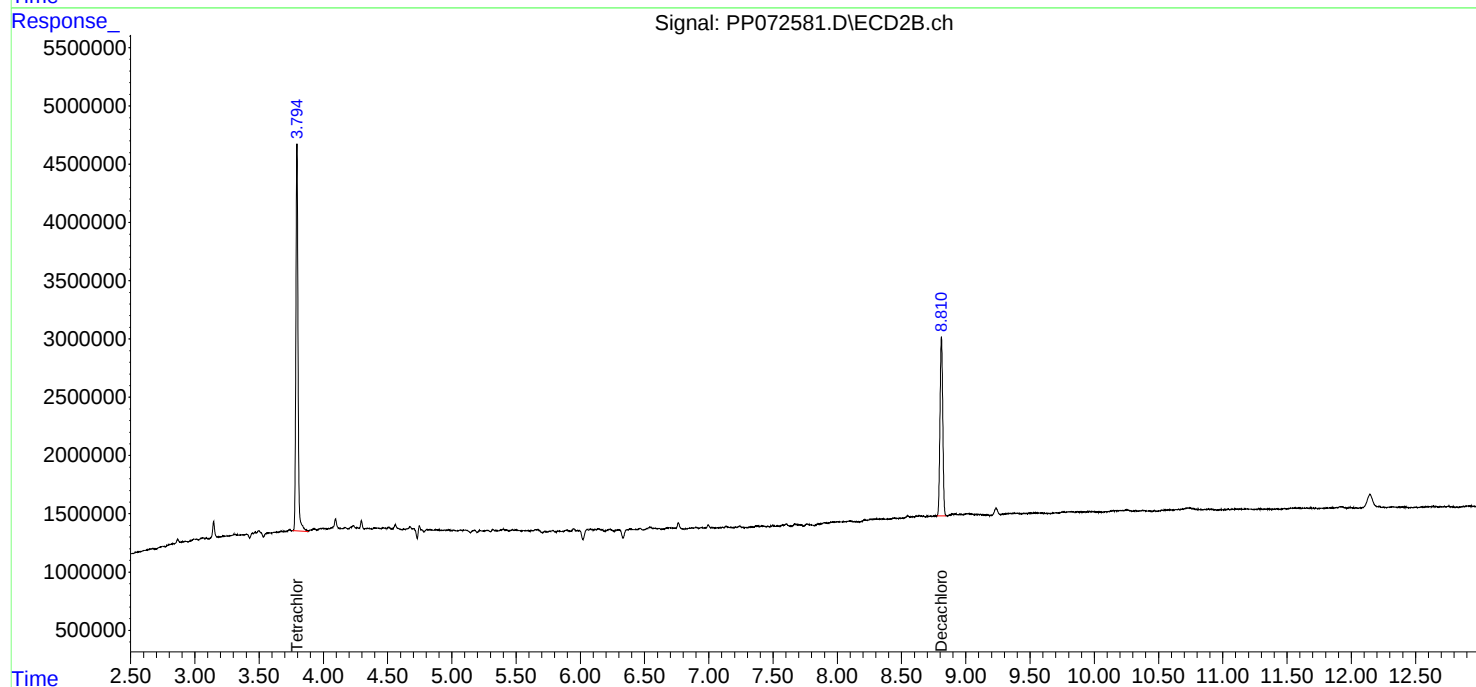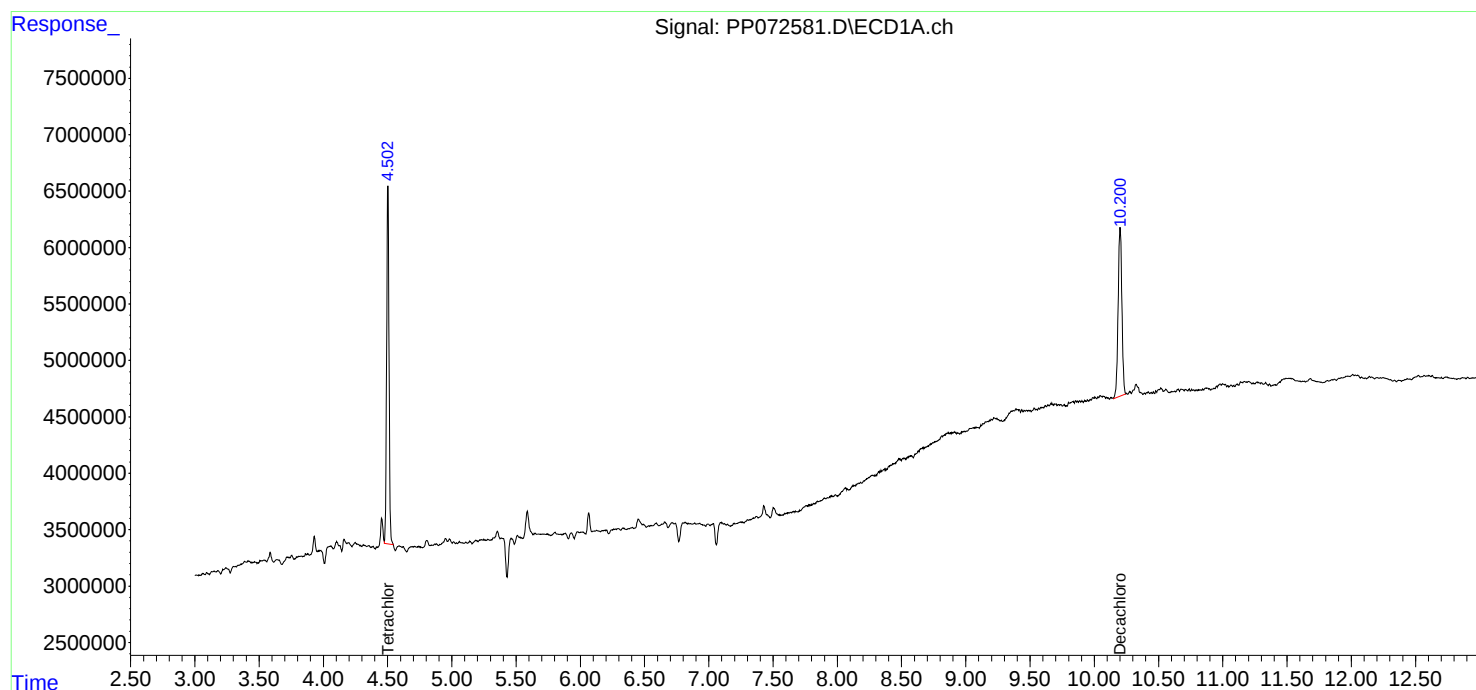

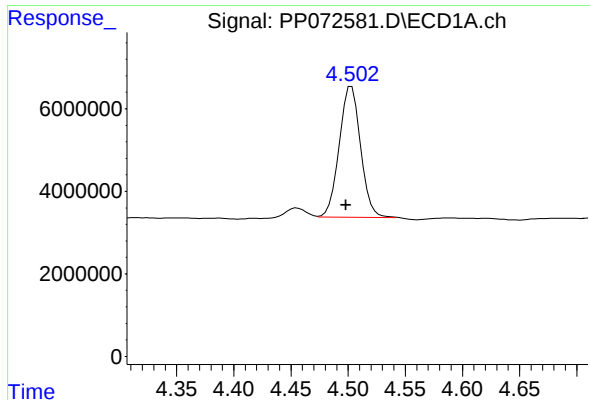


#1 Tetrachloro-m-xylene

R.T.: 4.502 min
Delta R.T.: 0.004 min
Response: 41161641
Conc: 20.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
B-202-SB01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/04/2025
Supervised By :mohammad ahmed 06/05/2025

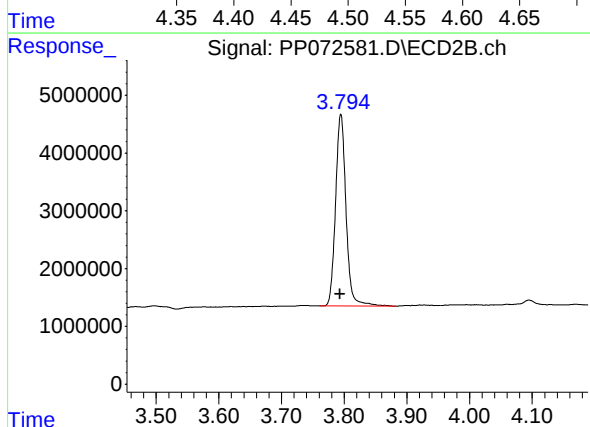


#1 Tetrachloro-m-xylene

R.T.: 3.795 min
Delta R.T.: 0.001 min
Response: 38502501
Conc: 24.09 ng/ml

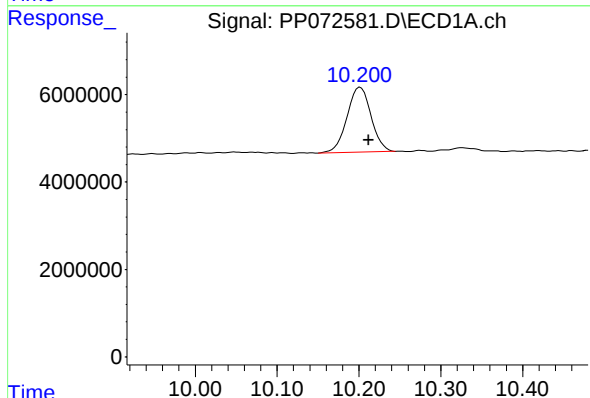

#2 Decachlorobiphenyl

R.T.: 10.200 min
Delta R.T.: -0.012 min
Response: 30482591
Conc: 18.71 ng/ml m

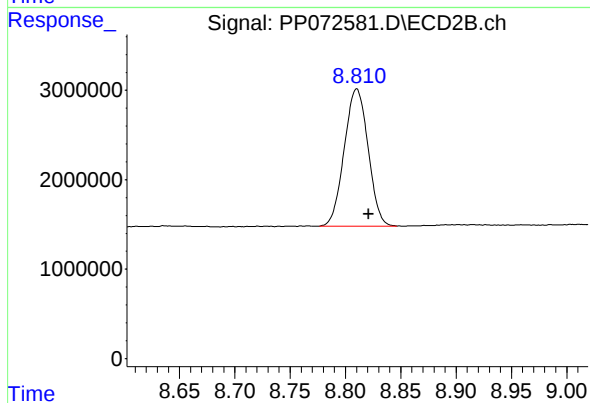

#2 Decachlorobiphenyl

R.T.: 8.810 min
Delta R.T.: -0.011 min
Response: 23027738
Conc: 21.75 ng/ml m