


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061025\
Data File : BP024887.D
Acq On : 10 Jun 2025 10:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 06 16:20:27 2025

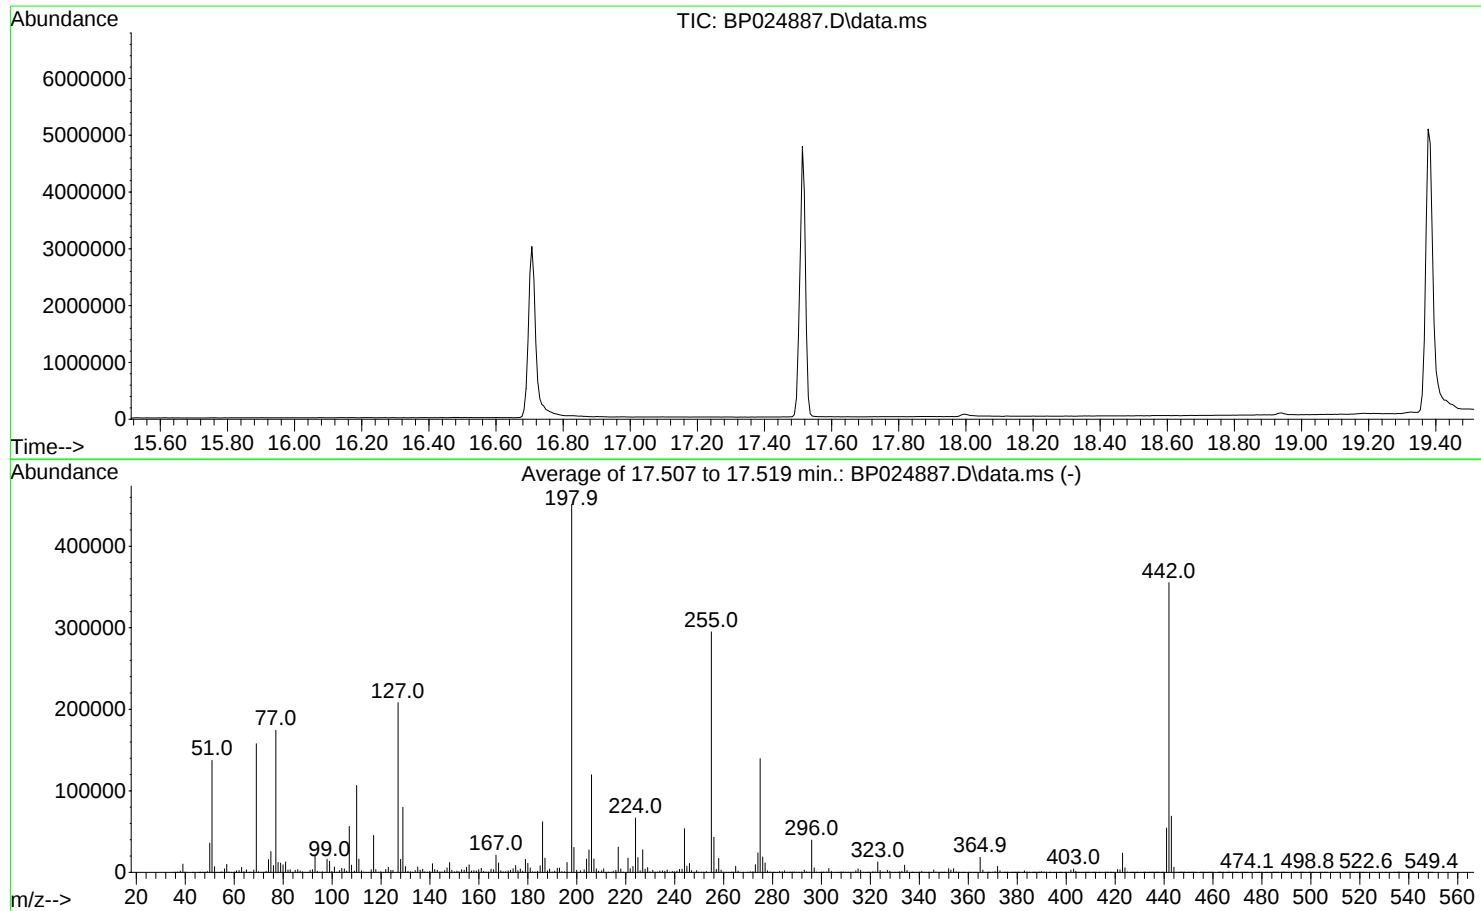

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	137404	PASS
68	69	0.00	2	1.8	2871	PASS
69	198	0.00	100	35.0	157844	PASS
70	69	0.00	2	0.6	870	PASS
127	198	10	80	46.2	208319	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	451221	PASS
199	198	5	9	6.8	30692	PASS
275	198	10	60	30.9	139559	PASS
365	198	1	100	4.1	18529	PASS
441	198	0.01	100	12.0	54291	PASS
442	442	100	100	100.0	355346	PASS
443	442	15	24	19.4	68941	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/10/2025	BNA_P	<u>BP024887.D</u>
Compound Name	Response	Retention Time
DDT	1552497	20.66
DDD	50681	20.207
DDE	2519	19.672
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
53200	1605697	3.31

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061025\
Data File : BP024887.D
Acq On : 10 Jun 2025 10:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 10 11:46:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

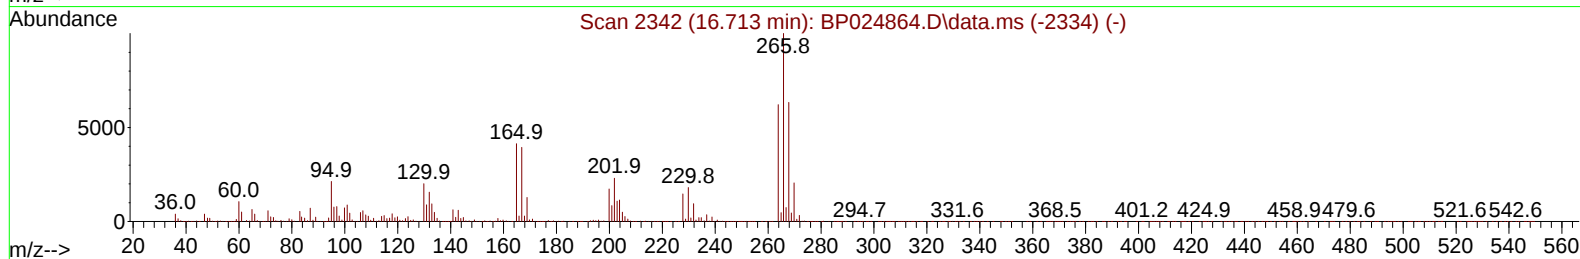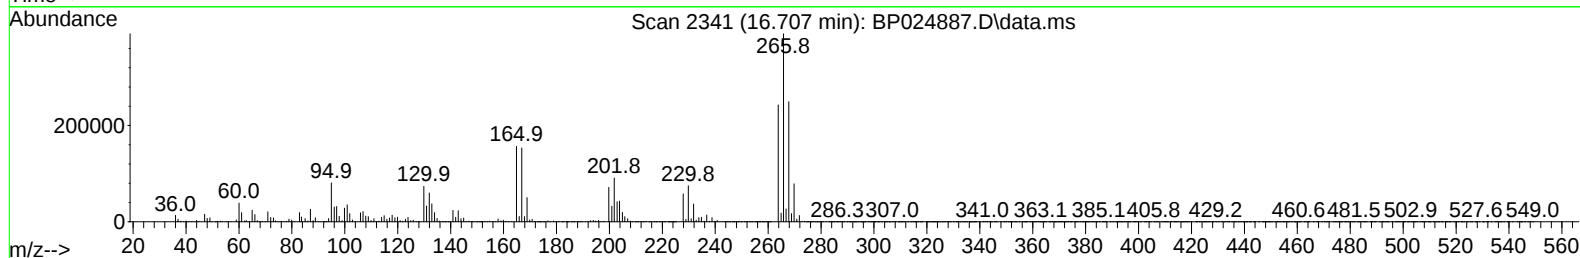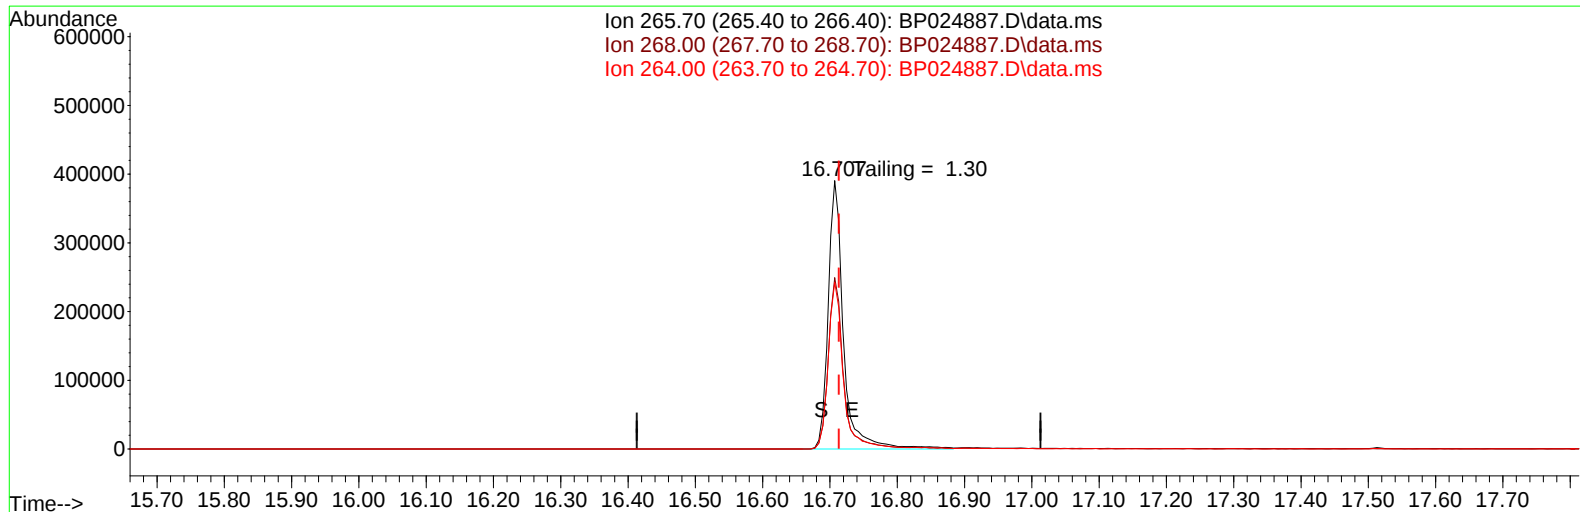

TIC: BP024887.D\data.ms

(70) Pentachlorophenol (C)

16.707min (-0.006) 2956989.98 ng




response 607073

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.85
264.00	62.10	62.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061025\
Data File : BP024887.D
Acq On : 10 Jun 2025 10:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 10 11:46:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

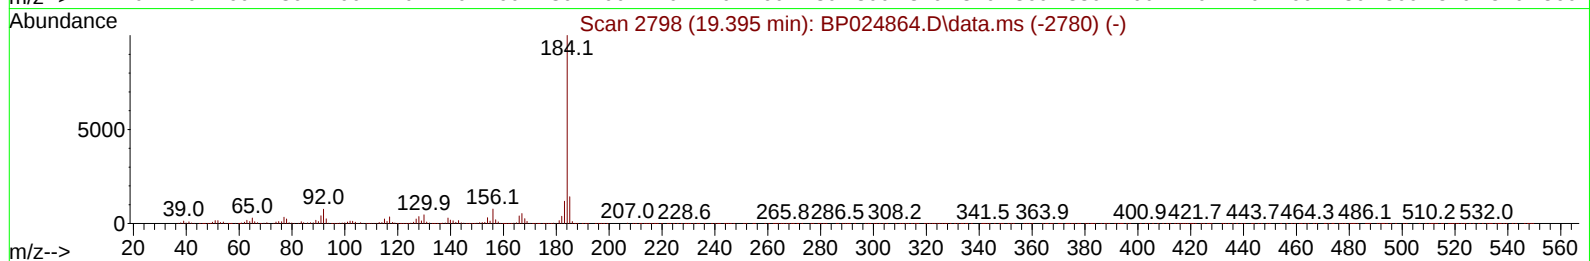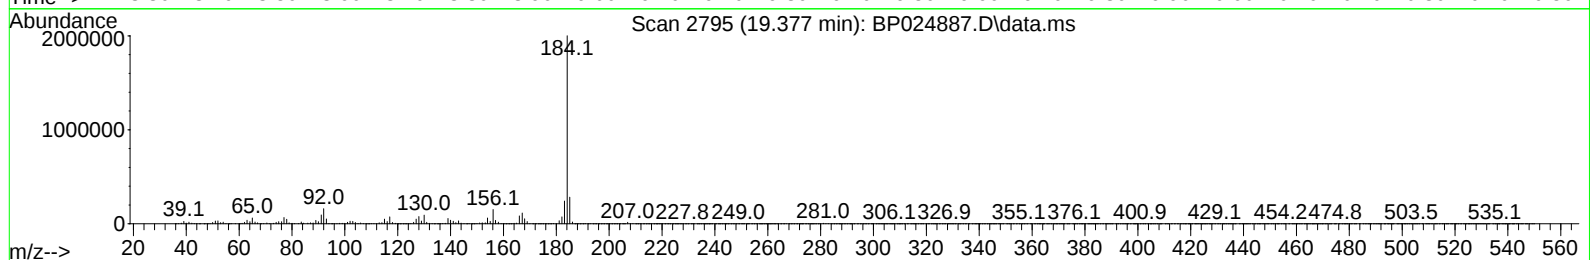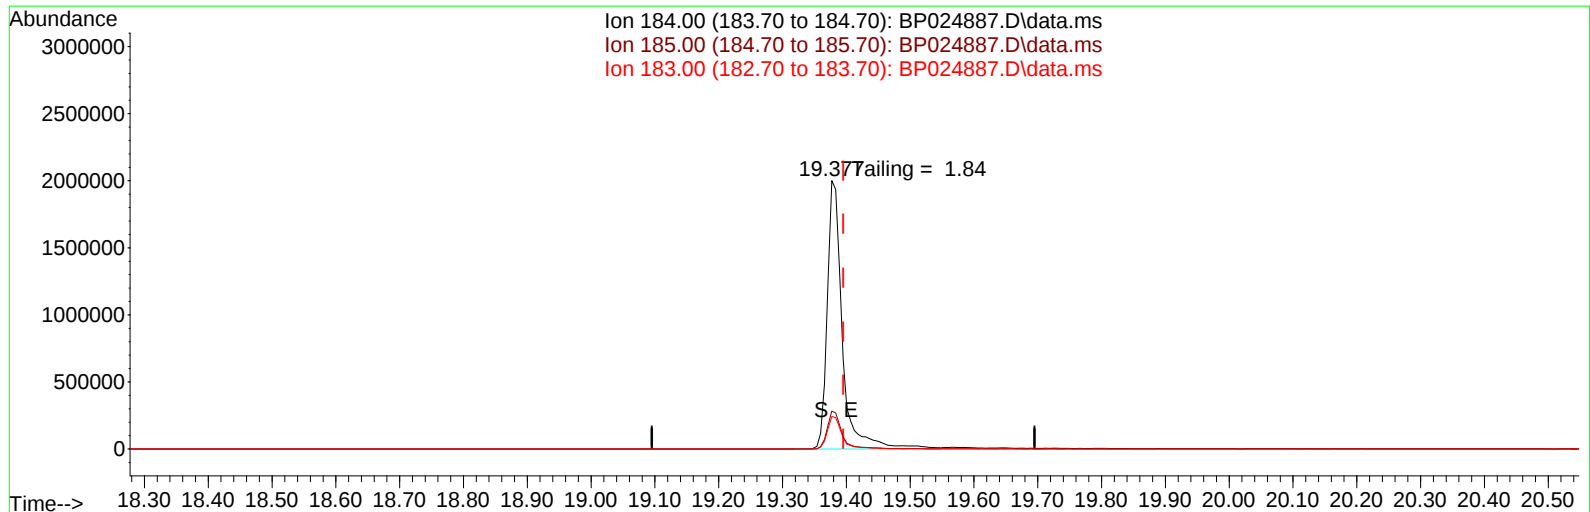

TIC: BP024887.D\data.ms

(77) Benzidine

19.377min (-0.018) 1369198.50 ng

response 3307673

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.14
183.00	11.90	12.13
0.00	0.00	0.00