
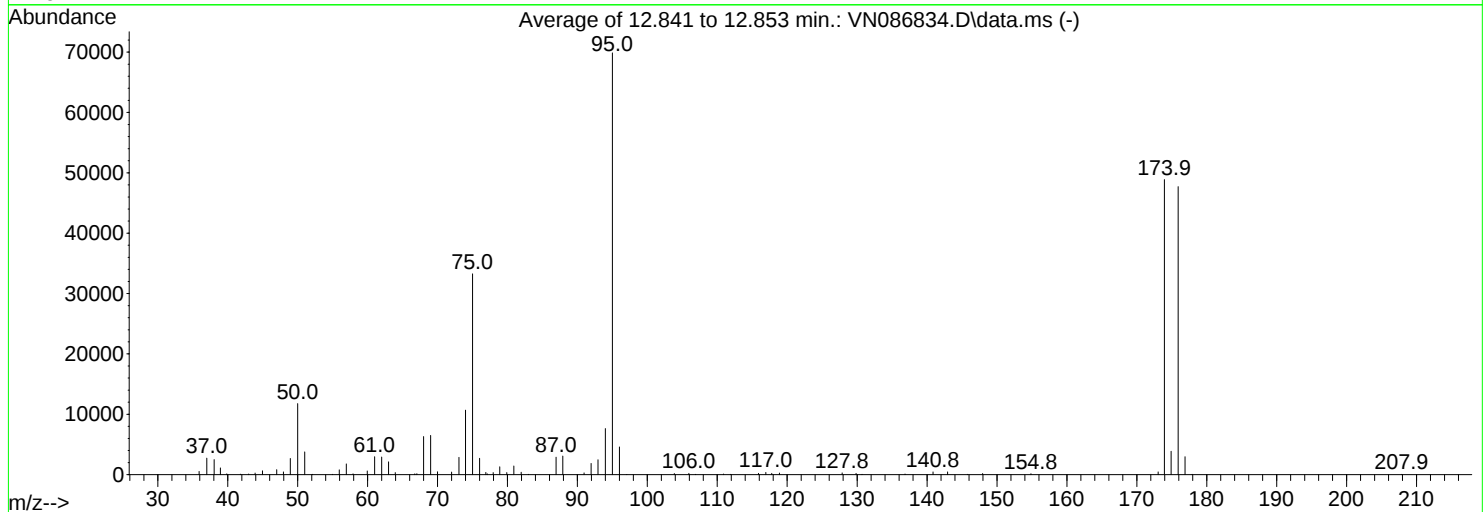


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN060325\  
Data File : VN086834.D  
Acq On : 03 Jun 2025 10:47  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N051625W.M  
Title : SW846 8260  
Last Update : Sat May 17 00:46:13 2025

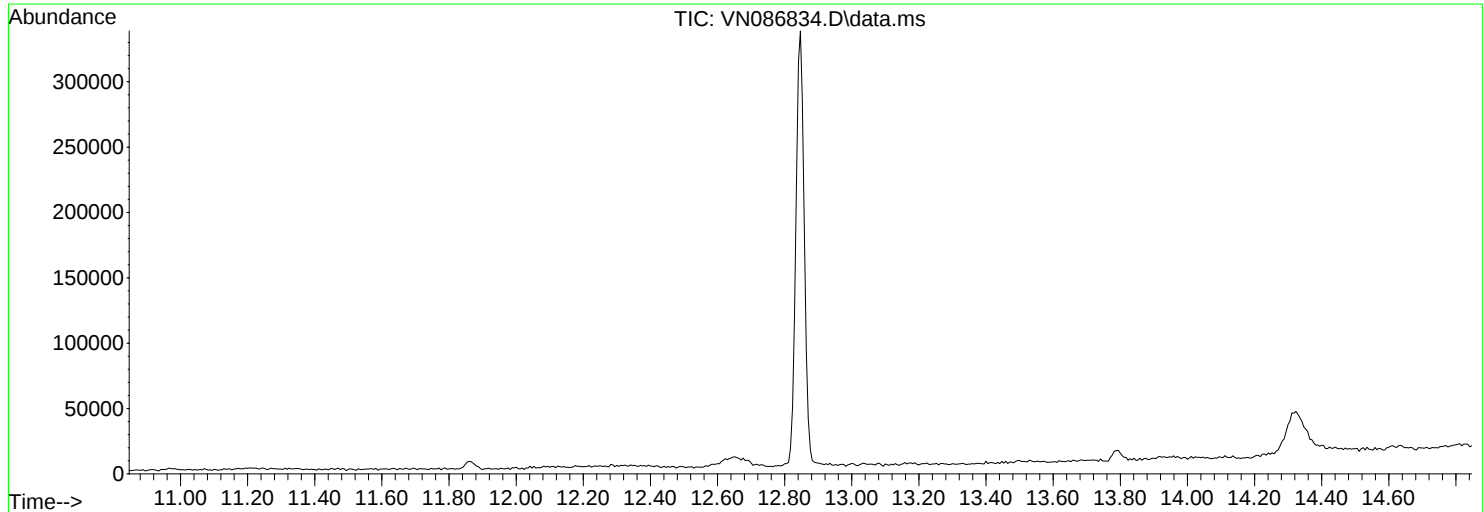

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 16.8         | 11764      | PASS                |
| 75             | 95              | 30              | 60              | 47.6         | 33277      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 69877      | PASS                |
| 96             | 95              | 5               | 9               | 6.6          | 4594       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.9          | 441        | PASS                |
| 174            | 95              | 50              | 100             | 69.9         | 48877      | PASS                |
| 175            | 174             | 5               | 9               | 7.9          | 3863       | PASS                |
| 176            | 174             | 95              | 101             | 97.6         | 47701      | PASS                |
| 177            | 176             | 5               | 9               | 6.2          | 2978       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 35.90 | 536    | 48.95 | 2681   | 63.00 | 2132   | 76.00 | 2711   |
| 37.00 | 2747   | 50.00 | 11764  | 63.95 | 342    | 76.90 | 360    |
| 38.05 | 2501   | 51.00 | 3775   | 66.75 | 147    | 77.10 | 14     |
| 38.95 | 1113   | 52.10 | 60     | 67.05 | 174    | 77.95 | 34     |
| 39.85 | 130    | 54.95 | 57     | 68.00 | 6320   | 78.90 | 1299   |
| 41.80 | 74     | 55.95 | 809    | 69.00 | 6498   | 79.90 | 356    |
| 43.00 | 103    | 56.95 | 1780   | 70.00 | 477    | 80.90 | 1437   |
| 43.90 | 263    | 57.90 | 128    | 72.00 | 435    | 81.95 | 401    |
| 44.95 | 630    | 59.95 | 611    | 73.05 | 2875   | 83.00 | 50     |
| 47.00 | 814    | 61.00 | 2974   | 74.00 | 10695  | 86.95 | 2901   |
| 47.95 | 463    | 62.00 | 2917   | 75.00 | 33277  | 87.90 | 3075   |

Average of 12.841 to 12.853 min.: VN086834.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z | abund. |
|--------|--------|--------|--------|--------|--------|-----|--------|
| 90.95  | 293    | 111.90 | 62     | 145.80 | 51     |     |        |
| 91.95  | 1844   | 115.90 | 219    | 147.95 | 187    |     |        |
| 92.95  | 2466   | 116.95 | 377    | 154.85 | 154    |     |        |
| 94.00  | 7644   | 117.80 | 220    | 173.05 | 441    |     |        |
| 95.00  | 69877  | 118.90 | 258    | 173.95 | 48877  |     |        |
| 96.00  | 4594   | 127.85 | 292    | 174.90 | 3863   |     |        |
| 97.05  | 38     | 129.85 | 202    | 175.90 | 47701  |     |        |
| 103.85 | 182    | 130.70 | 51     | 176.90 | 2978   |     |        |
| 105.95 | 227    | 136.85 | 120    | 177.90 | 57     |     |        |
| 106.90 | 63     | 140.85 | 466    | 207.90 | 61     |     |        |
| 110.90 | 104    | 142.95 | 465    |        |        |     |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB