

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060425\
 Data File : VY022539.D
 Acq On : 04 Jun 2025 10:24
 Operator : SY/MD
 Sample : VY0604SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0604SBL01

Quant Time: Jun 05 04:09:39 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 03 03:22:04 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	271205	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	498185	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	390593	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	137326	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	159828	52.692	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 105.380%	
35) Dibromofluoromethane	7.634	113	150711	50.684	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 101.360%	
50) Toluene-d8	10.109	98	592665	49.327	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 98.660%	
62) 4-Bromofluorobenzene	12.408	95	149151	41.664	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 83.320%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060425\
Data File : VY022539.D
Acq On : 04 Jun 2025 10:24
Operator : SY/MD
Sample : VY0604SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0604SBL01

Quant Time: Jun 05 04:09:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060225S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 03 03:22:04 2025
Response via : Initial Calibration




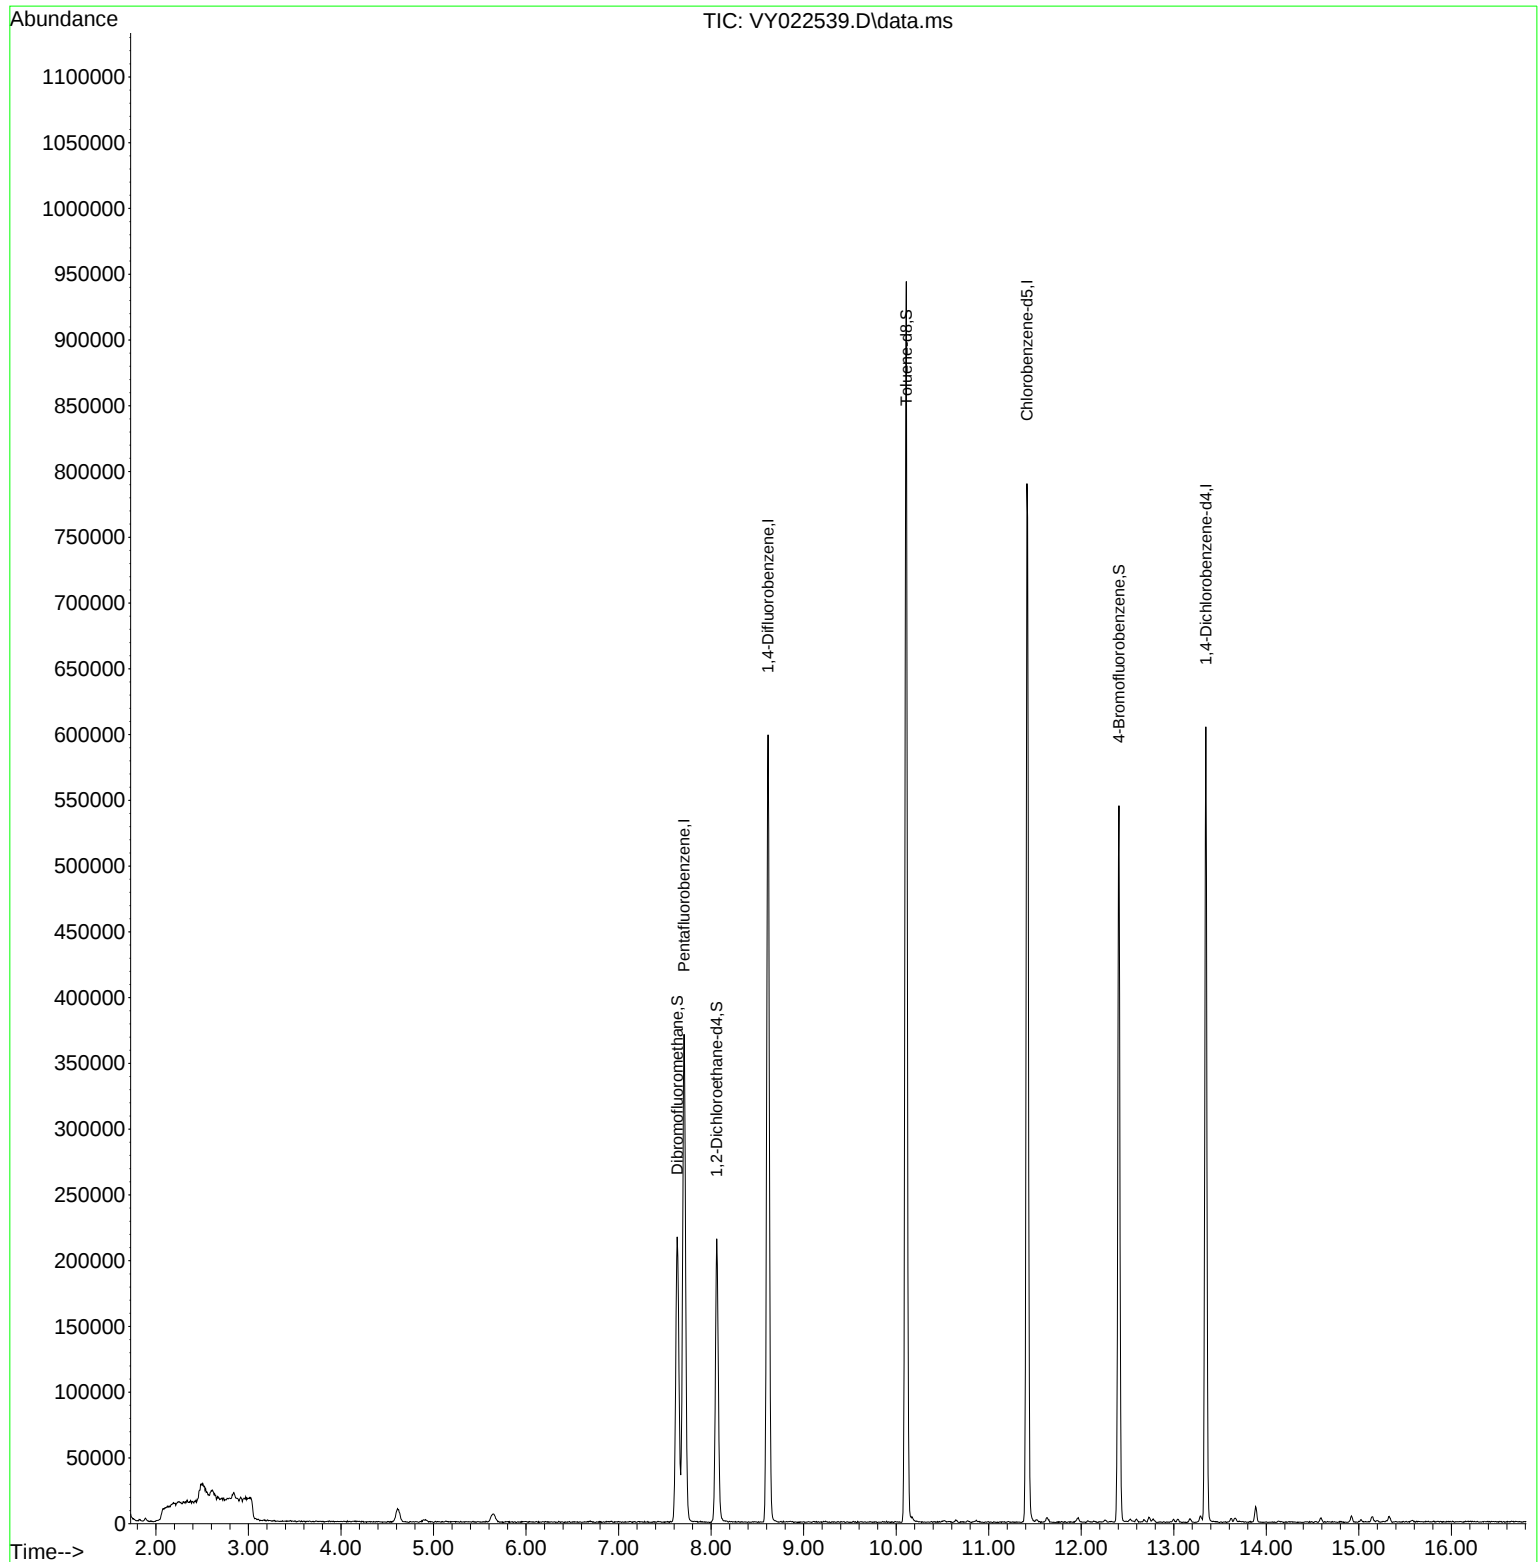




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 99
Delta R.T. -0.006 min
Lab File: VY022539.D
Acq: 04 Jun 2025 10:24




Instrument :
MSVOA_Y
ClientSampleId :
VY0604SBL01

Tgt Ion:168 Resp: 271205
Ion Ratio Lower Upper
168 100
99 55.5 44.3 66.5

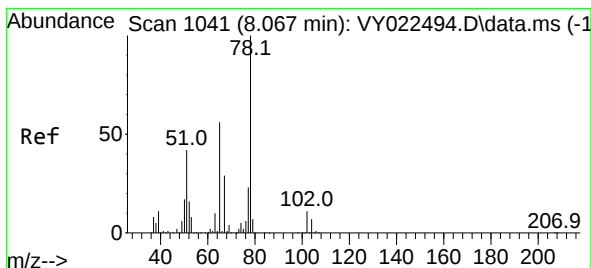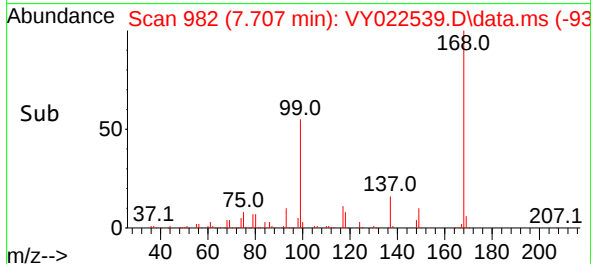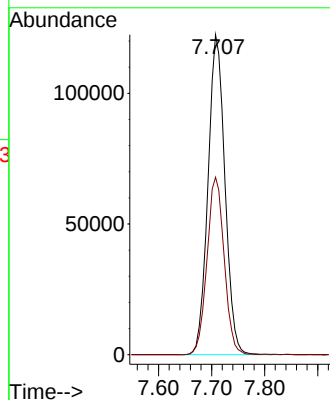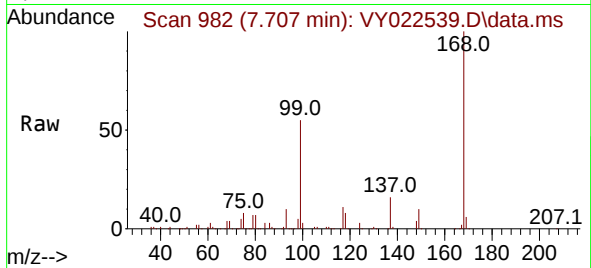

#33
1,2-Dichloroethane-d4
Concen: 52.692 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.006 min
Lab File: VY022539.D
Acq: 04 Jun 2025 10:24

Tgt Ion: 65 Resp: 159828
Ion Ratio Lower Upper
65 100
67 53.1 0.0 103.4

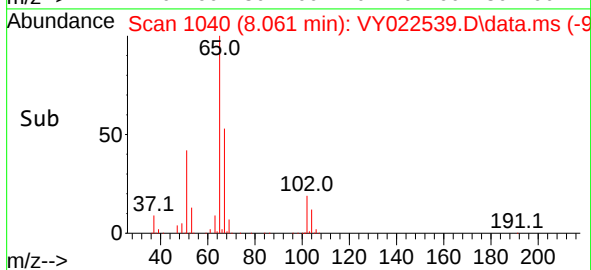
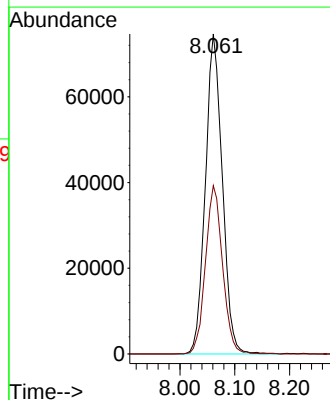
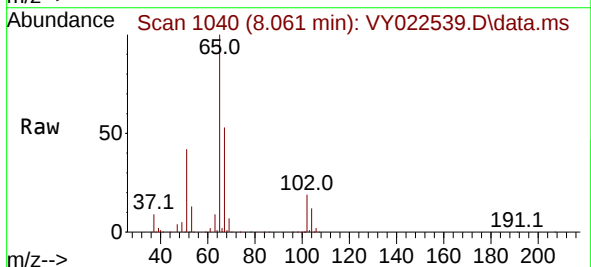




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.616 min Scan# 1131
Delta R.T. -0.000 min
Lab File: VY022539.D
Acq: 04 Jun 2025 10:24




Instrument :
MSVOA_Y
ClientSampleId :
VY0604SBL01


Tgt Ion:114 Resp: 498185
Ion Ratio Lower Upper
114 100
63 20.9 0.0 40.8
88 14.6 0.0 27.8

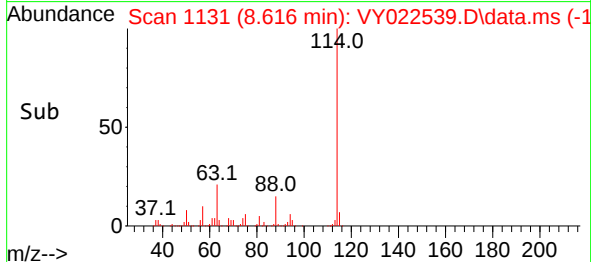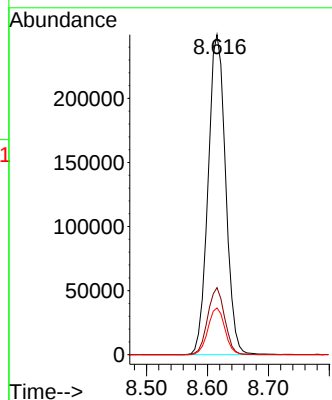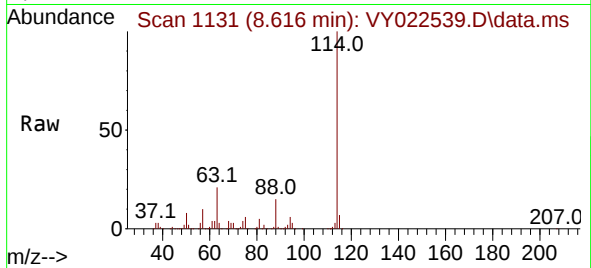

#35
Dibromofluoromethane
Concen: 50.684 ug/l
RT: 7.634 min Scan# 970
Delta R.T. -0.006 min
Lab File: VY022539.D
Acq: 04 Jun 2025 10:24

Tgt Ion:113 Resp: 150711
Ion Ratio Lower Upper
113 100
111 101.5 81.1 121.7
192 17.7 14.2 21.2


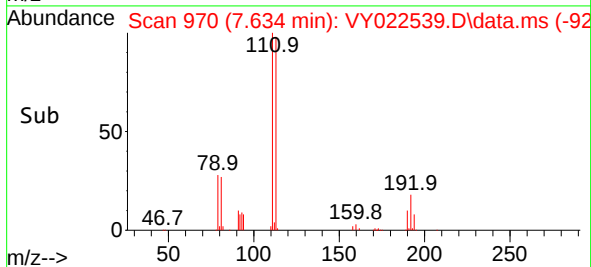
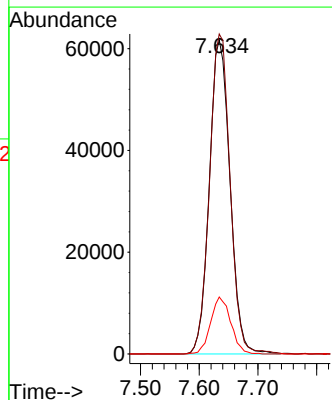
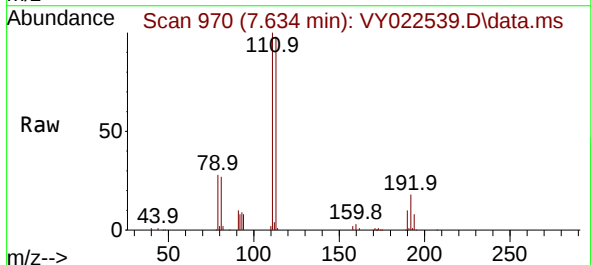


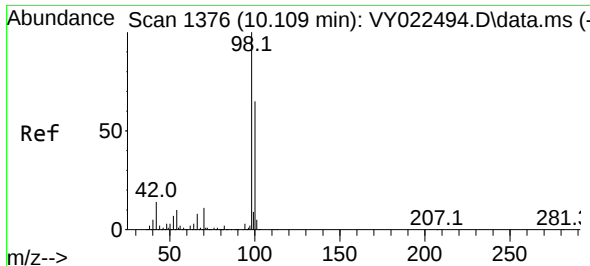

#50
Toluene-d8
Concen: 49.327 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. -0.000 min
Lab File: VY022539.D
Acq: 04 Jun 2025 10:24




Instrument :
MSVOA_Y
ClientSampleId :
VY0604SBL01


Tgt Ion: 98 Resp: 592665
Ion Ratio Lower Upper
98 100
100 64.0 51.4 77.0

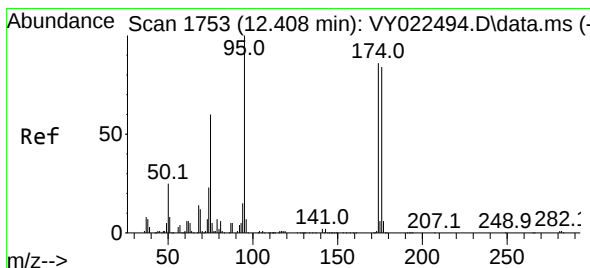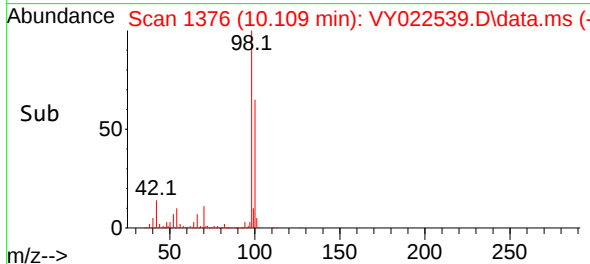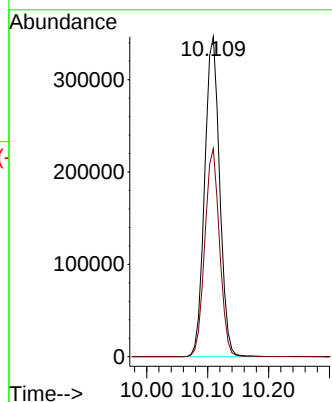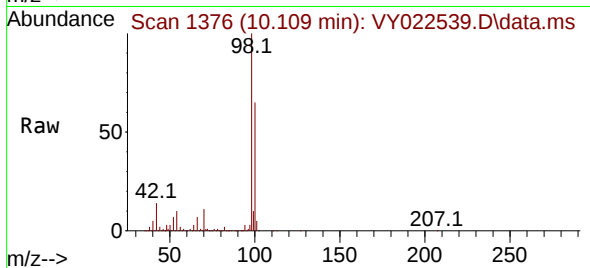

#62
4-Bromofluorobenzene
Concen: 41.664 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. -0.000 min
Lab File: VY022539.D
Acq: 04 Jun 2025 10:24

Tgt Ion: 95 Resp: 149151
Ion Ratio Lower Upper
95 100
174 82.8 0.0 170.0
176 80.6 0.0 166.2

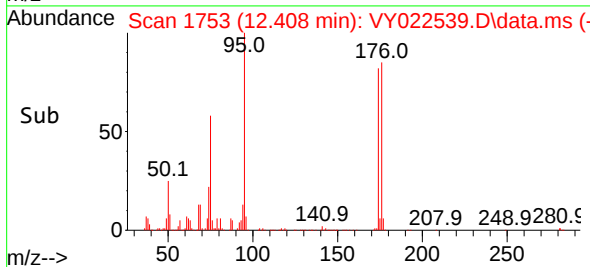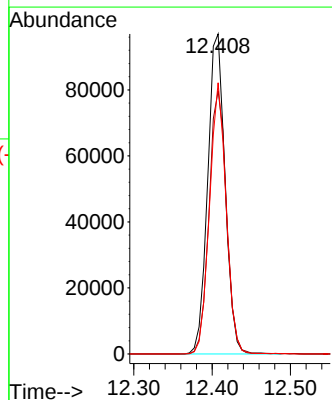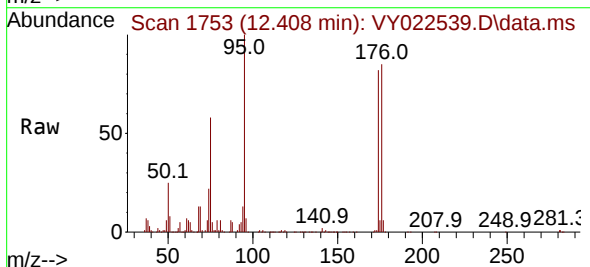

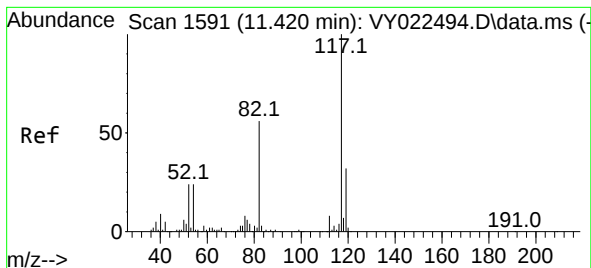

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 1

Delta R.T. -0.006 min

Lab File: VY022539.D

Acq: 04 Jun 2025 10:24

Instrument :

MSVOA_Y

ClientSampleId :

VY0604SBL01





Tgt Ion:117 Resp: 390593

Ion Ratio Lower Upper

117 100

82 57.7 44.6 66.8

119 32.2 25.4 38.0

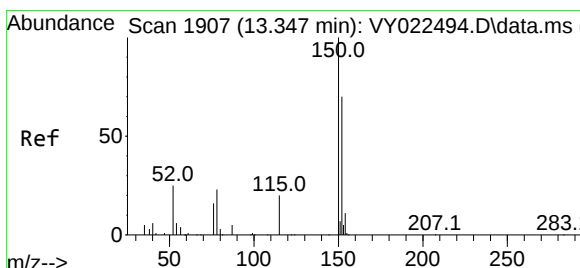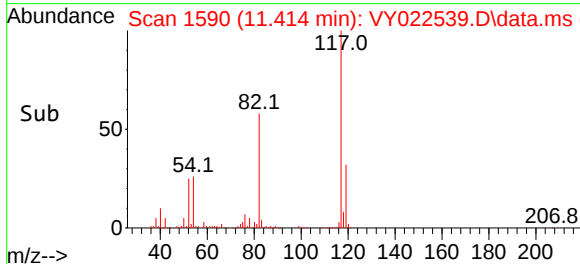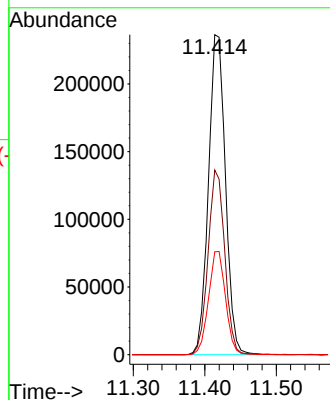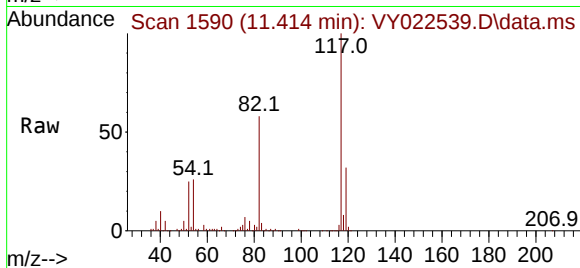

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. -0.000 min

Lab File: VY022539.D

Acq: 04 Jun 2025 10:24

Tgt Ion:152 Resp: 137326

Ion Ratio Lower Upper

152 100

115 58.1 28.9 86.7

150 156.5 0.0 349.6

