

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060525\
 Data File : BN037176.D
 Acq On : 05 Jun 2025 12:08
 Operator : RC/JU
 Sample : Q2186-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 VPB182-HYD-20250530

Quant Time: Jun 05 12:42:07 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN060325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 04 01:52:03 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.589	152	2282	0.400	ng	0.00
7) Naphthalene-d8	10.372	136	5466	0.400	ng	0.00
13) Acenaphthene-d10	14.234	164	2730	0.400	ng	0.00
19) Phenanthrene-d10	16.984	188	4699	0.400	ng	0.00
29) Chrysene-d12	21.180	240	3527	0.400	ng	# 0.00
35) Perylene-d12	23.374	264	3289	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	0.000	112	0d	0.000	ng	
5) Phenol-d6	0.000	99	0d	0.000	ng	
8) Nitrobenzene-d5	8.739	82	1940	0.336	ng	0.00
11) 2-Methylnaphthalene-d10	11.976	152	211	0.028	ng	0.00
14) 2,4,6-Tribromophenol	15.743	330	133	0.121	ng	0.00
15) 2-Fluorobiphenyl	12.858	172	4844	0.416	ng	0.00
27) Fluoranthene-d10	19.026	212	1985	0.166	ng	0.00
31) Terphenyl-d14	19.630	244	3730	0.449	ng	0.00
Target Compounds						
34) Bis(2-ethylhexyl)phtha...	21.108	149	672	0.083	ng	# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060525\
Data File : BN037176.D
Acq On : 05 Jun 2025 12:08
Operator : RC/JU
Sample : Q2186-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
VPB182-HYD-20250530


Quant Time: Jun 05 12:42:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN060325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 01:52:03 2025
Response via : Initial Calibration

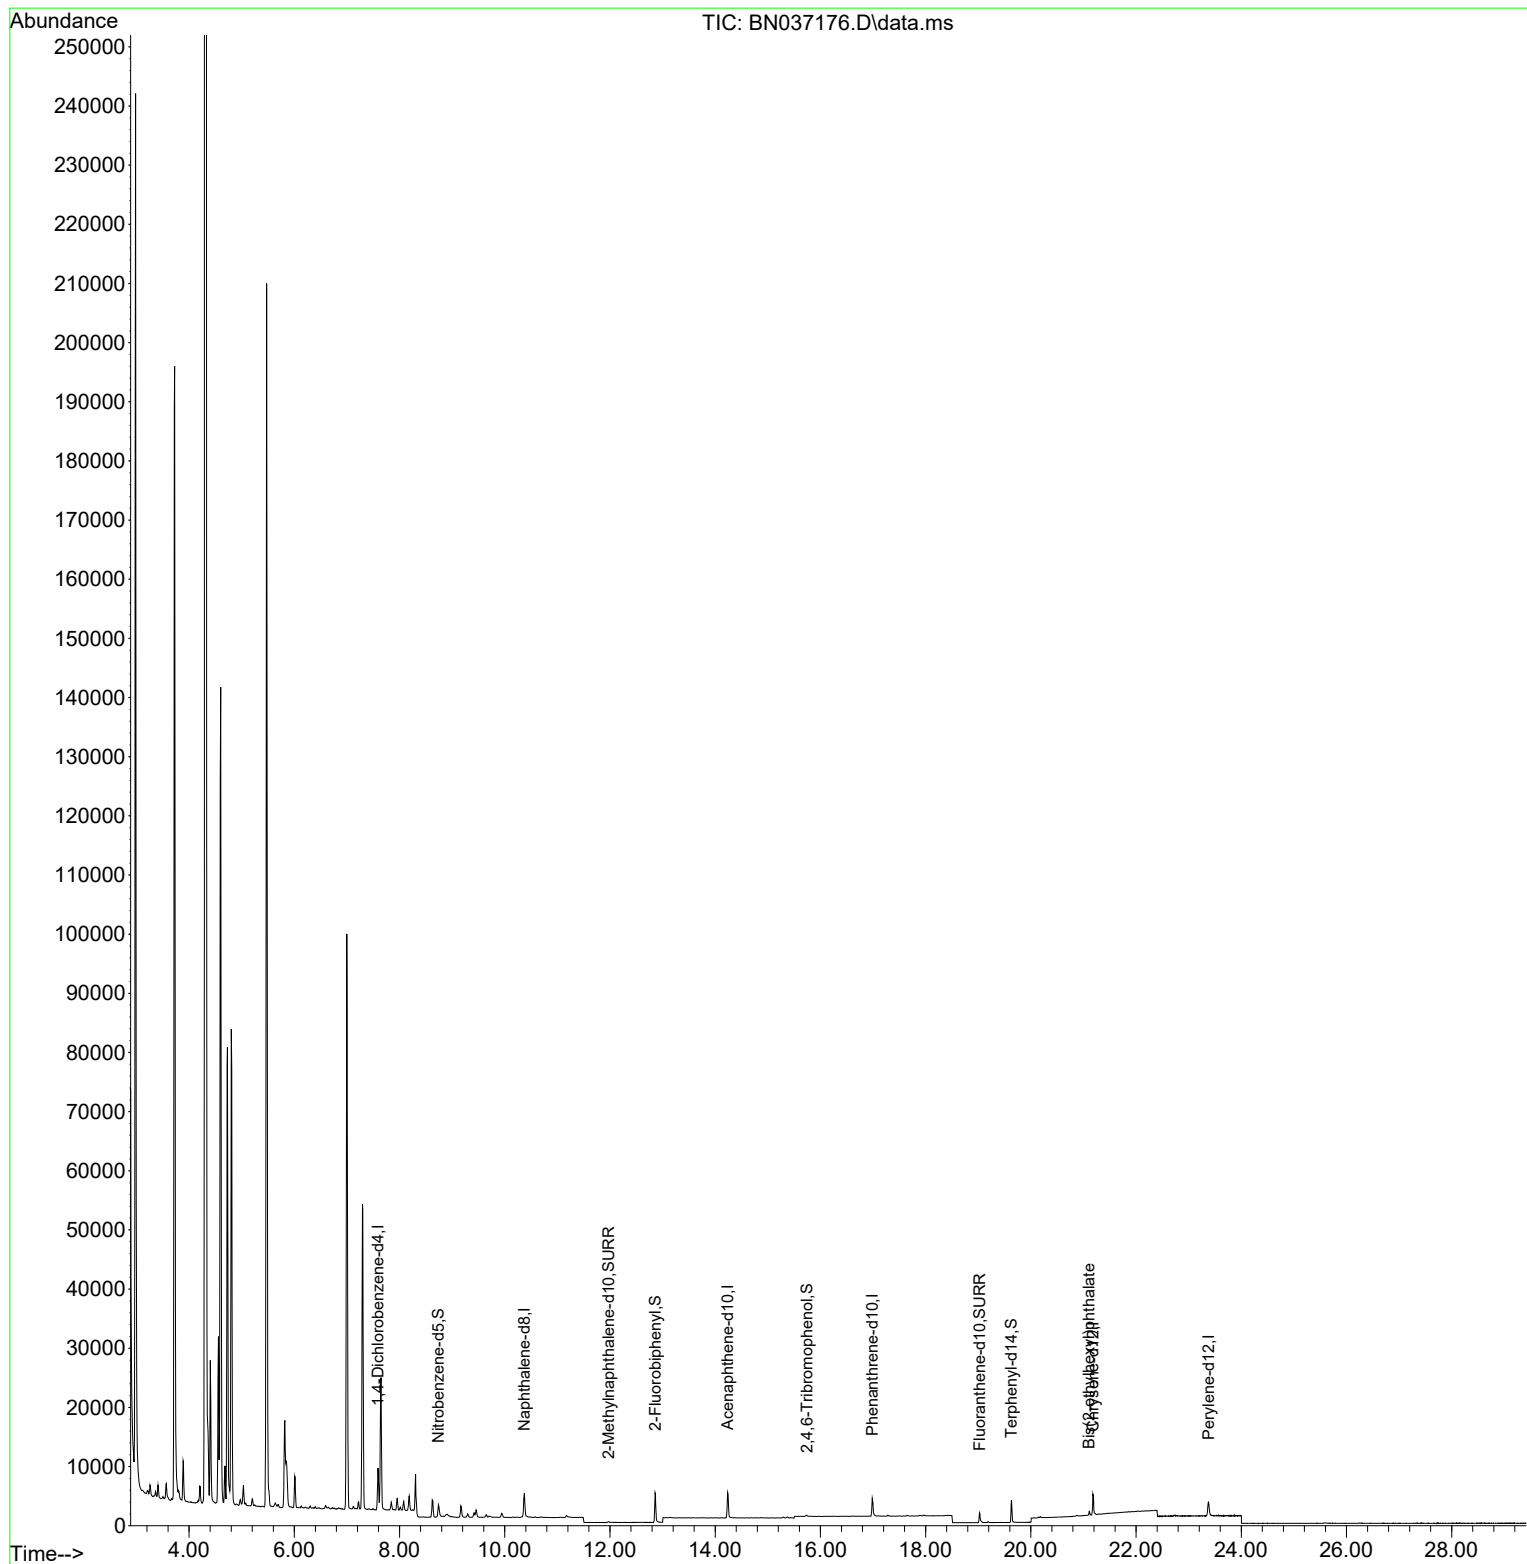






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.589 min Scan# 61
 Delta R.T. -0.001 min
 Lab File: BN037176.D
 Acq: 05 Jun 2025 12:08

Instrument :
 BNA_N
 ClientSampleId :
 VPB182-HYD-20250530

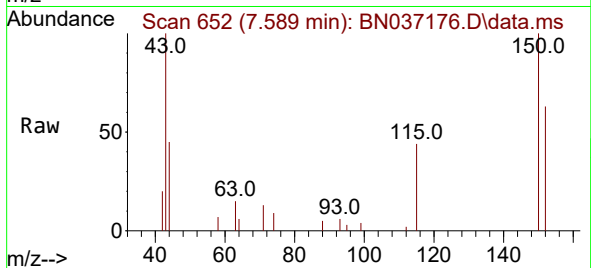

Tgt Ion:152 Resp: 2282

Ion	Ratio	Lower	Upper
152	100		
150	157.0	123.2	184.8
115	70.1	56.6	85.0

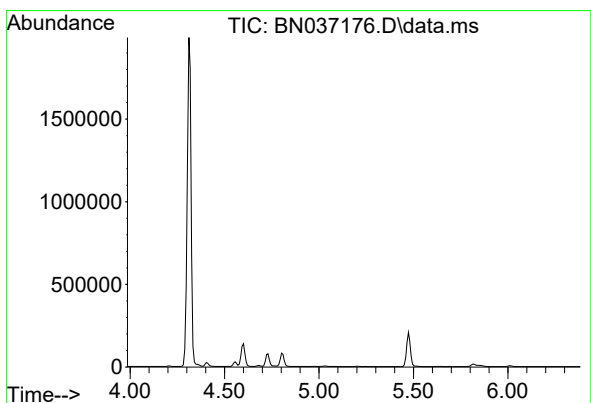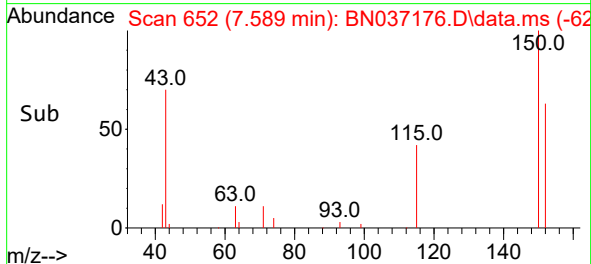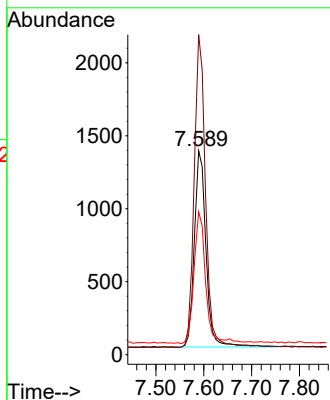



#4
 2-Fluorophenol
 Concen: 0.000 ng
 Expected RT: 5.18 min

Lab File: BN037176.D
 Acq: 05 Jun 2025 12:08

Tgt Ion: 112

Sig	Exp Ratio
112	100
64	70.4
63	45.3


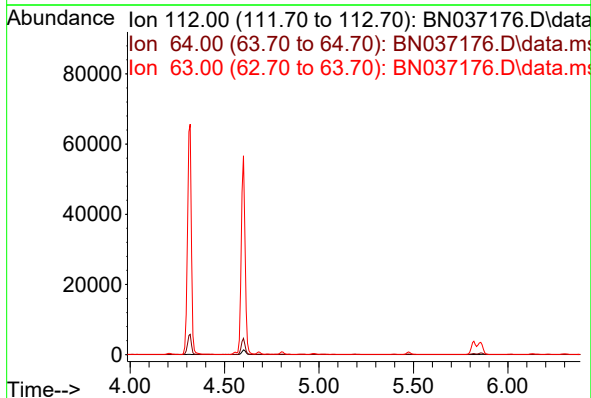


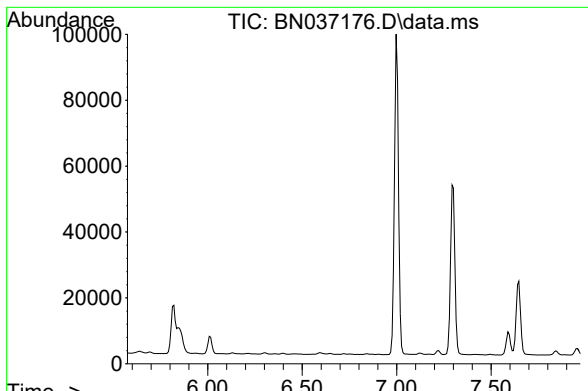

#5
 Phenol-d6
 Concen: 0.000 ng
 Expected RT: 6.77 min
 Lab File: BN037176.D
 Acq: 05 Jun 2025 12:08




Instrument :
 BNA_N
 ClientSampleId :
 VPB182-HYD-20250530


Tgt Ion: 99
 Sig Exp Ratio
 99 100
 42 39.1
 71 47.7

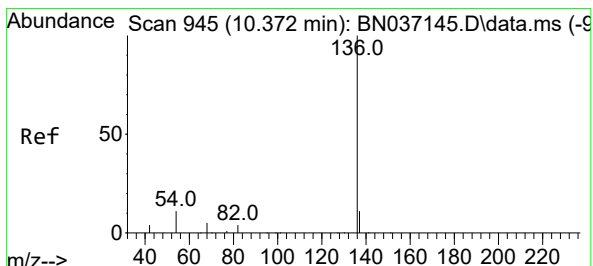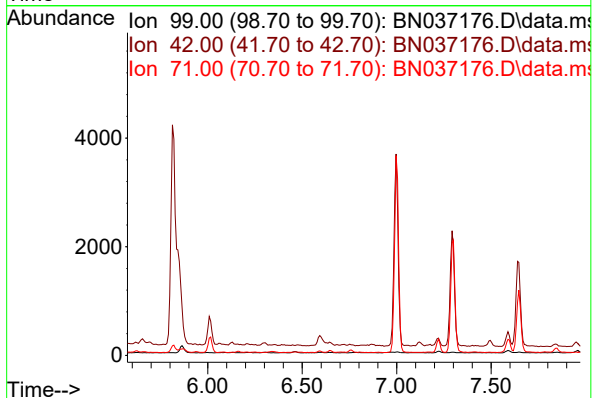

#7
 Naphthalene-d8
 Concen: 0.400 ng
 RT: 10.372 min Scan# 945
 Delta R.T. -0.000 min
 Lab File: BN037176.D
 Acq: 05 Jun 2025 12:08

Tgt Ion: 136 Resp: 5466
 Ion Ratio Lower Upper
 136 100
 137 12.3 9.7 14.5
 54 11.6 9.7 14.5
 68 6.7 5.4 8.2


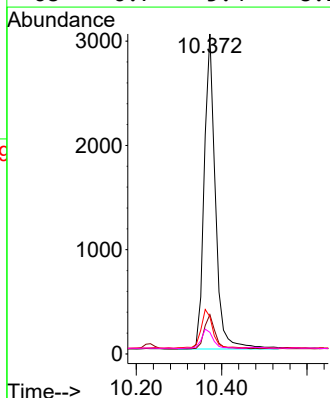
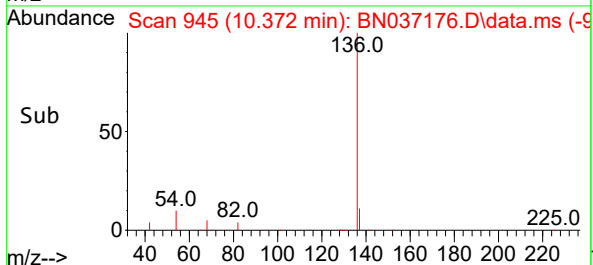
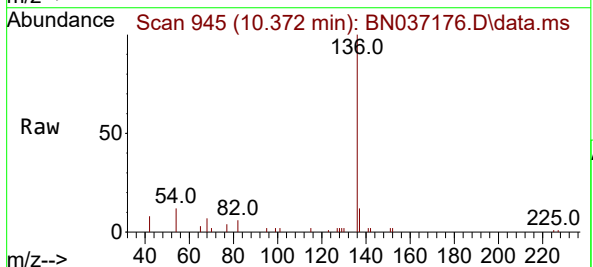


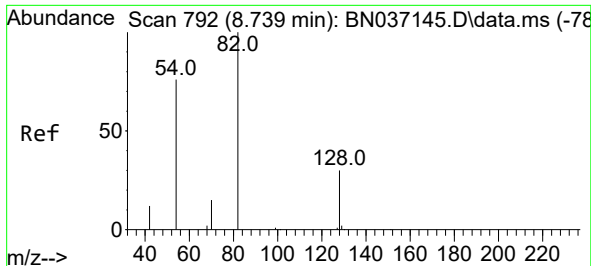

#8
Nitrobenzene-d5
Concen: 0.336 ng
RT: 8.739 min Scan# 792
Delta R.T. -0.000 min
Lab File: BN037176.D
Acq: 05 Jun 2025 12:08




Instrument :
BNA_N
ClientSampleId :
VPB182-HYD-20250530


Tgt Ion: 82 Resp: 1940
Ion Ratio Lower Upper
82 100
128 34.5 26.9 40.3
54 75.8 61.4 92.2

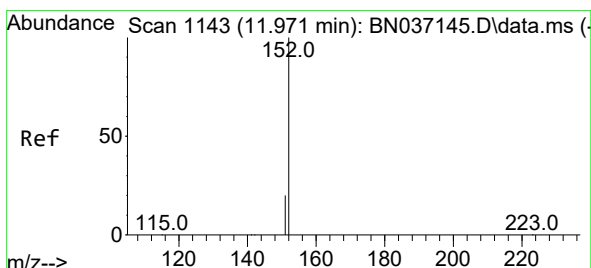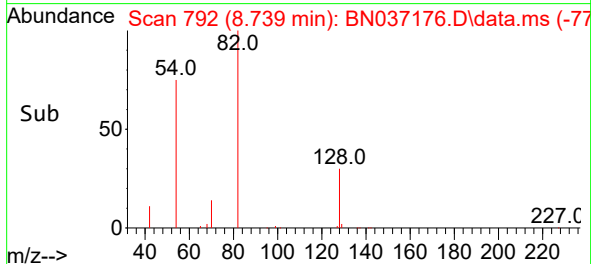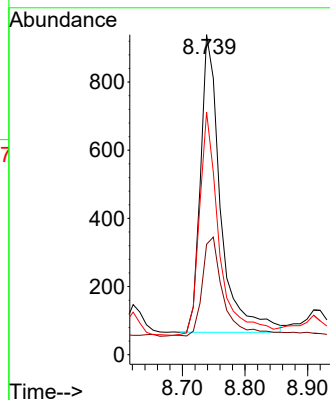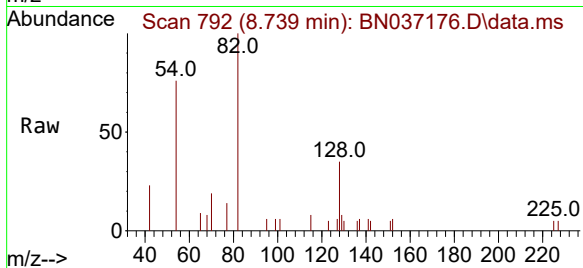

#11
2-Methylnaphthalene-d10
Concen: 0.028 ng
RT: 11.976 min Scan# 1144
Delta R.T. 0.005 min
Lab File: BN037176.D
Acq: 05 Jun 2025 12:08

Tgt Ion: 152 Resp: 211
Ion Ratio Lower Upper
152 100
151 24.2 17.1 25.7


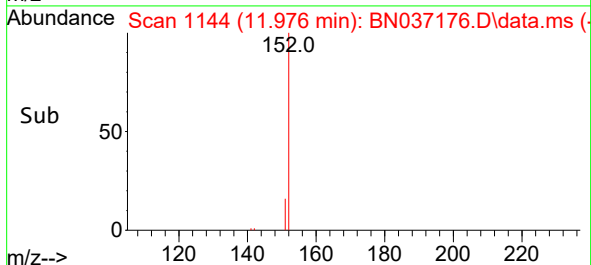
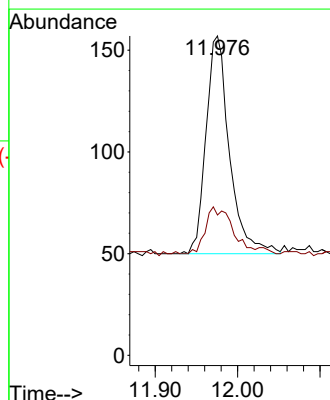
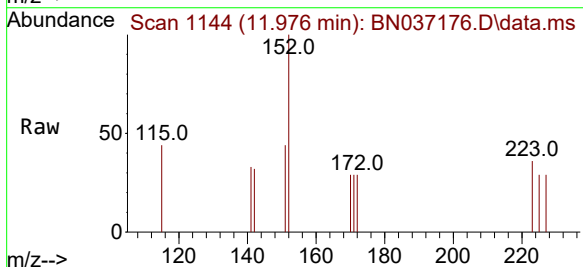


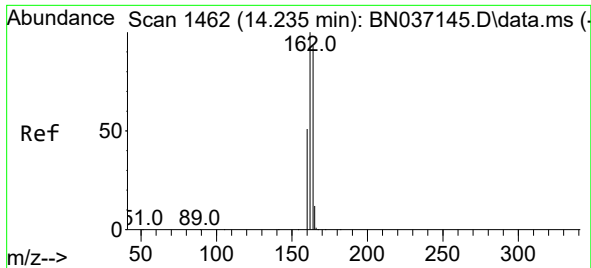

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.234 min Scan# 1462
Delta R.T. -0.000 min
Lab File: BN037176.D
Acq: 05 Jun 2025 12:08




Instrument :
BNA_N
ClientSampleId :
VPB182-HYD-20250530


Tgt Ion:164 Resp: 2730
Ion Ratio Lower Upper
164 100
162 104.7 85.5 128.3
160 55.1 44.6 67.0

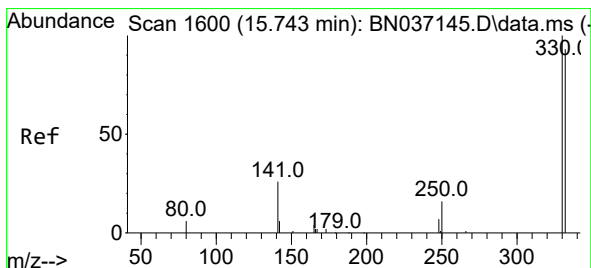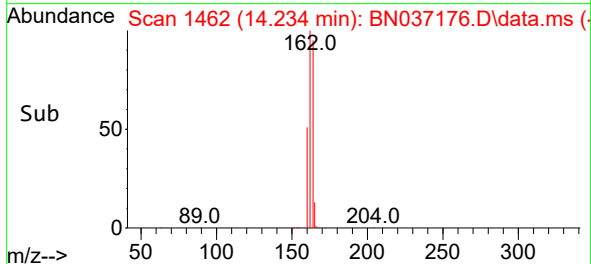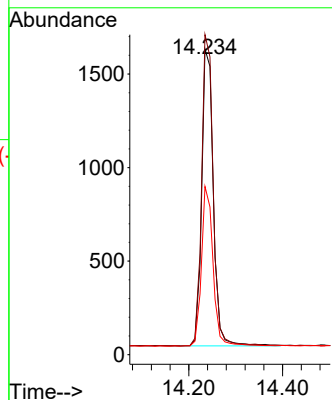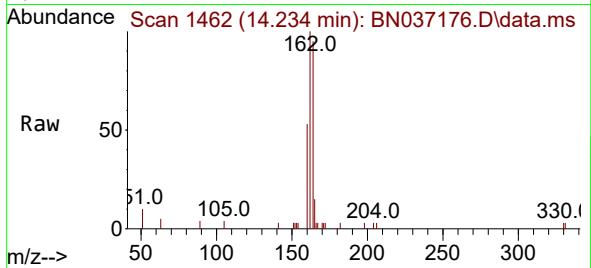

#14
2,4,6-Tribromophenol
Concen: 0.121 ng
RT: 15.743 min Scan# 1600
Delta R.T. -0.000 min
Lab File: BN037176.D
Acq: 05 Jun 2025 12:08

Tgt Ion:330 Resp: 133
Ion Ratio Lower Upper
330 100
332 136.1 77.1 115.7#
141 49.6 46.4 69.6

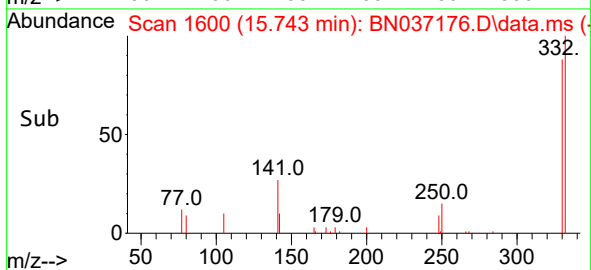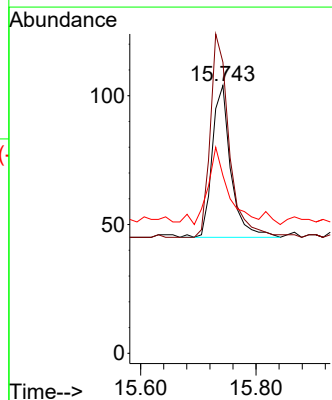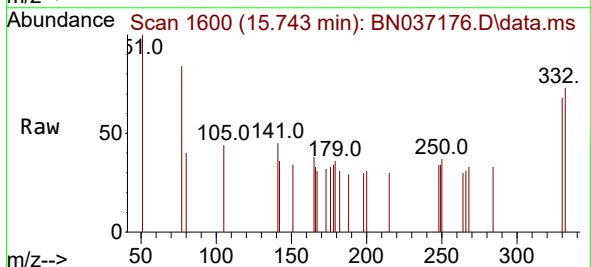

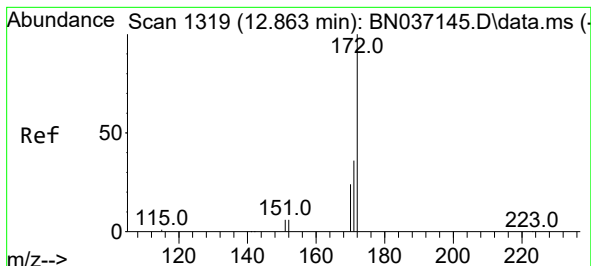

#15

2-Fluorobiphenyl

Concen: 0.416 ng

RT: 12.858 min Scan# 11

Delta R.T. -0.005 min

Lab File: BN037176.D

Acq: 05 Jun 2025 12:08

Instrument :

BNA_N

ClientSampleId :

VPB182-HYD-20250530





Tgt Ion:172 Resp: 4844

Ion Ratio Lower Upper

172 100

171 37.2 29.6 44.4

170 25.7 20.3 30.5

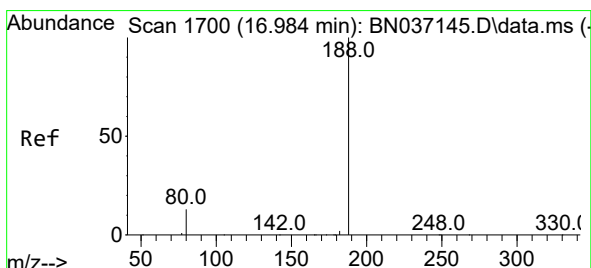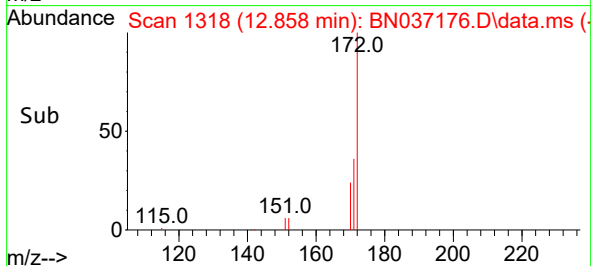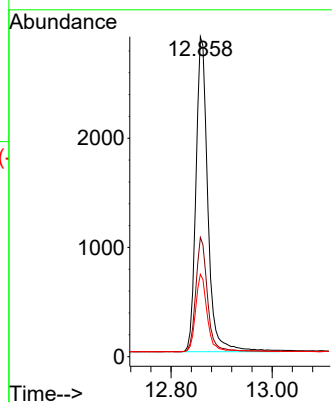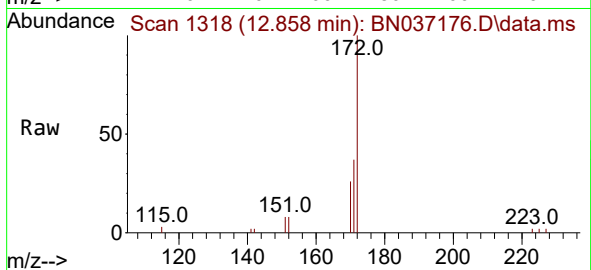

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.984 min Scan# 1700

Delta R.T. -0.000 min

Lab File: BN037176.D

Acq: 05 Jun 2025 12:08




Tgt Ion:188 Resp: 4699


Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 15.7 11.3 16.9


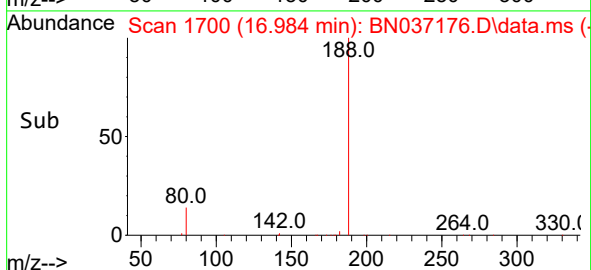
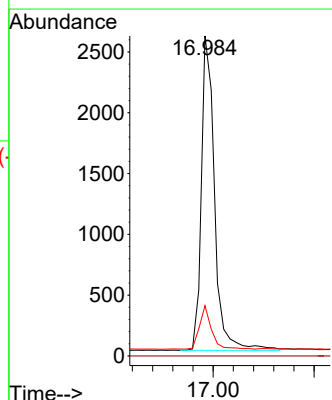
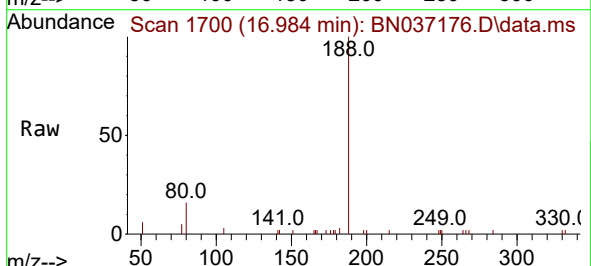


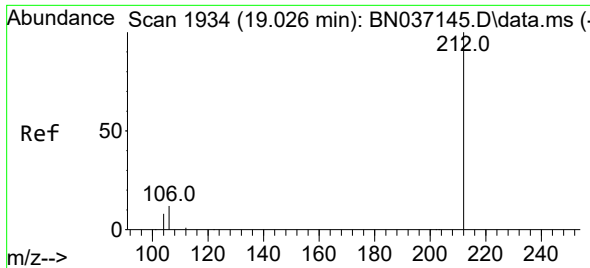

#27
Fluoranthene-d10
Concen: 0.166 ng
RT: 19.026 min Scan# 1934
Delta R.T. -0.000 min
Lab File: BN037176.D
Acq: 05 Jun 2025 12:08




Instrument :
BNA_N
ClientSampleId :
VPB182-HYD-20250530


Tgt Ion:212 Resp: 1985
Ion Ratio Lower Upper
212 100
106 13.8 10.6 15.8
104 8.3 6.6 9.8

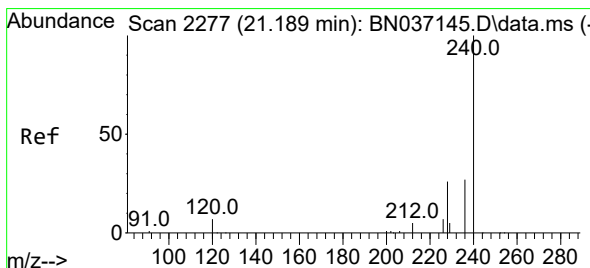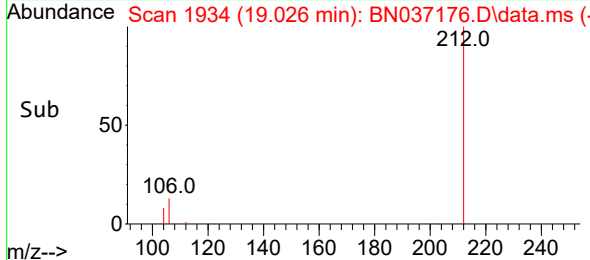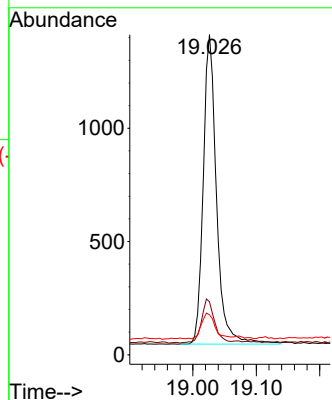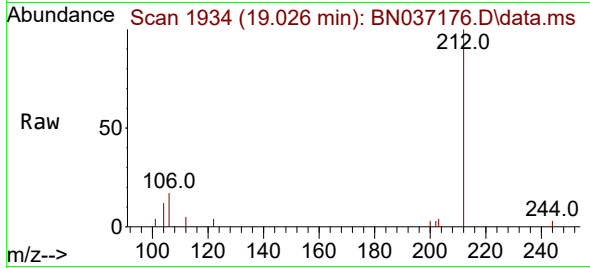

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.180 min Scan# 2276
Delta R.T. -0.009 min
Lab File: BN037176.D
Acq: 05 Jun 2025 12:08

Tgt Ion:240 Resp: 3527
Ion Ratio Lower Upper
240 100
120 17.5 9.0 13.4#
236 28.6 23.0 34.4


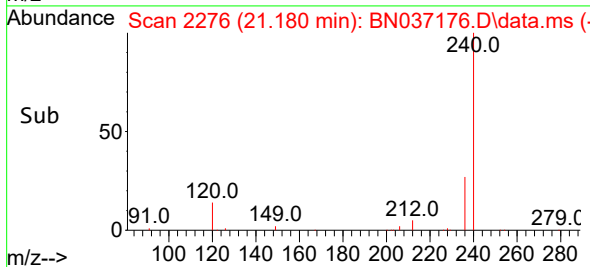
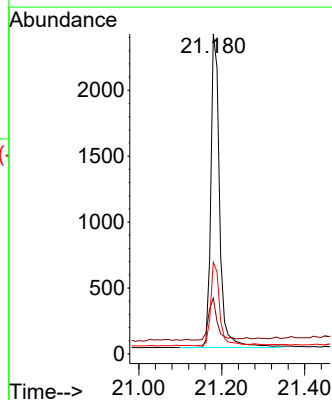
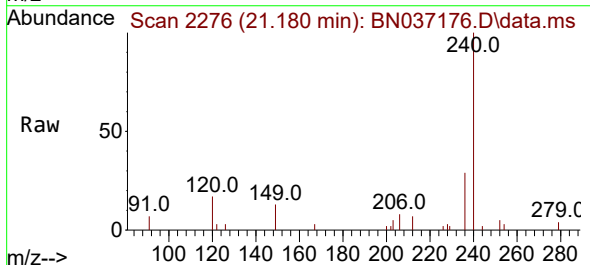


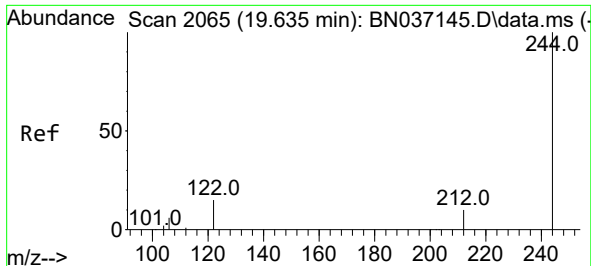

#31
 Terphenyl-d14
 Concen: 0.449 ng
 RT: 19.630 min Scan# 2065
 Delta R.T. -0.005 min
 Lab File: BN037176.D
 Acq: 05 Jun 2025 12:08




Instrument :
 BNA_N
 ClientSampleId :
 VPB182-HYD-20250530


Tgt Ion:244 Resp: 3730
 Ion Ratio Lower Upper
 244 100
 212 12.2 10.0 15.0
 122 17.5 13.2 19.8

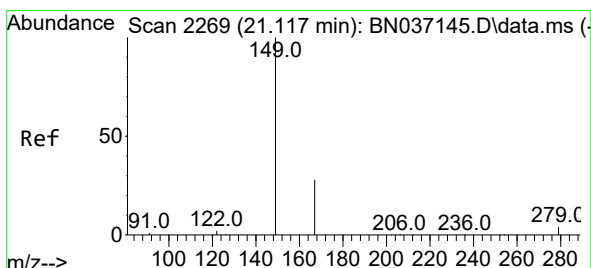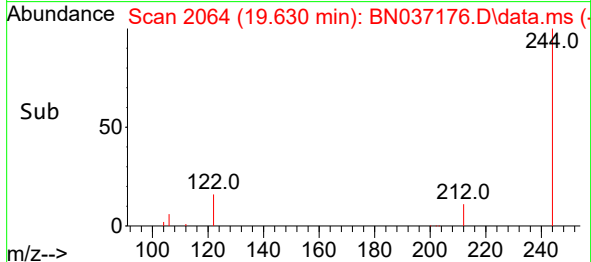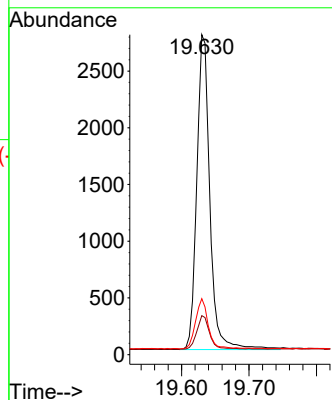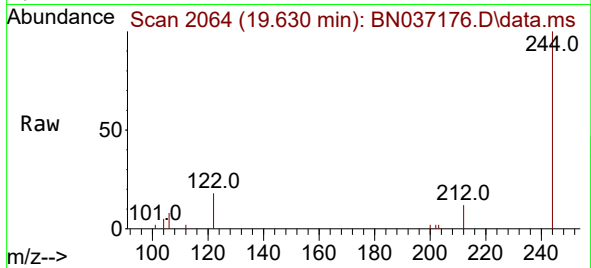

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.083 ng
 RT: 21.108 min Scan# 2268
 Delta R.T. -0.009 min
 Lab File: BN037176.D
 Acq: 05 Jun 2025 12:08


Tgt Ion:149 Resp: 672
 Ion Ratio Lower Upper
 149 100
 167 25.9 21.0 31.4
 279 2.7 2.9 4.3#

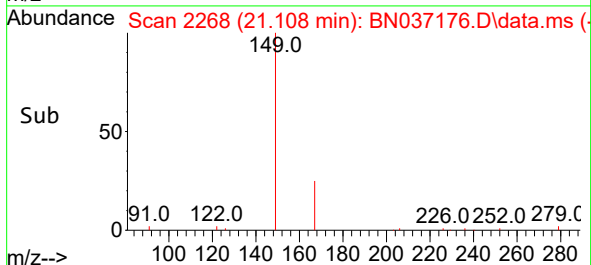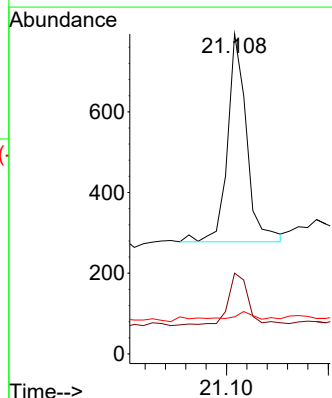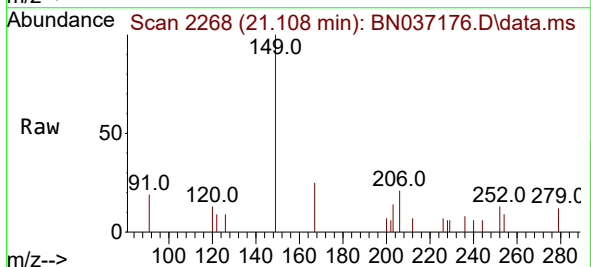

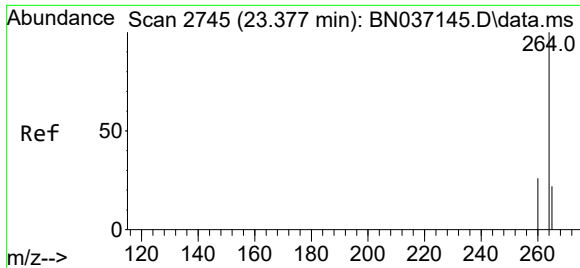

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.374 min Scan# 21
Delta R.T. -0.003 min
Lab File: BN037176.D
Acq: 05 Jun 2025 12:08

Instrument :
BNA_N
ClientSampleId :
VPB182-HYD-20250530

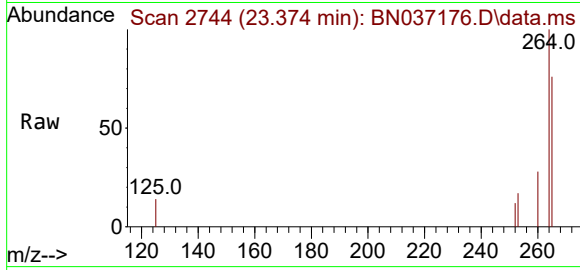

Tgt Ion: 264 Resp: 3289

Ion	Ratio	Lower	Upper
264	100		
260	28.4	22.1	33.1
265	75.6	55.8	83.8

